

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052421\
 Data File : PL066846.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2021 21:06
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 25 05:57:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052421.M
 Quant Title : GC Extractables
 QLast Update : Tue May 25 05:57:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.481	5.532	29152735	41867776	50.000	50.000
28)	SA Decachlor...	10.224	11.431	36041156	41363713	50.000	50.000
Target Compounds							
23)	Chlordane-1	5.802	6.914	10368761	14876955	500.000	500.000
24)	Chlordane-2	6.487	7.505	14087229	18484134	500.000	500.000
25)	Chlordane-3	7.186	8.262	39687987	63767979	500.000	500.000
26)	Chlordane-4	7.253	8.344	42968611	76947163	500.000	500.000
27)	Chlordane-5	8.193	9.229	14080245	13906422	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052421\
Data File : PL066846.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2021 21:06
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 25 05:57:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052421.M
Quant Title : GC Extractables
QLast Update : Tue May 25 05:57:00 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

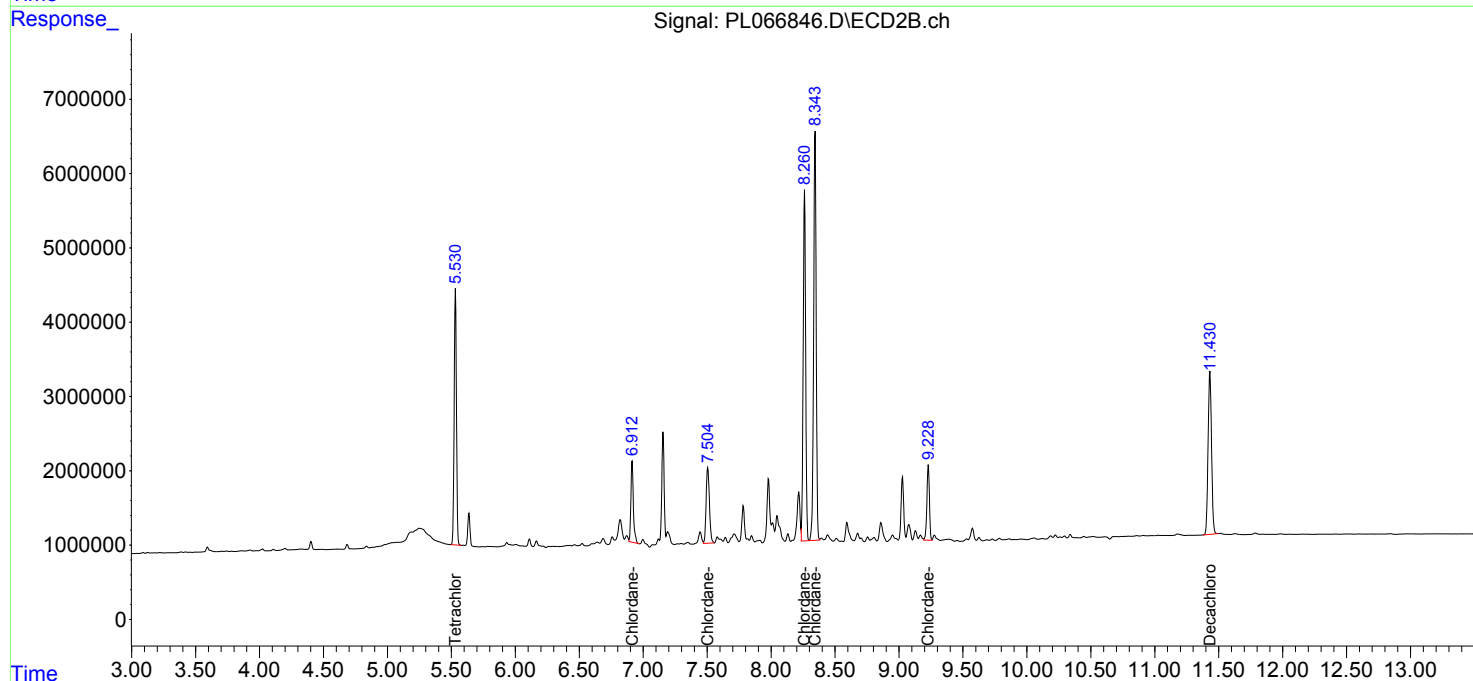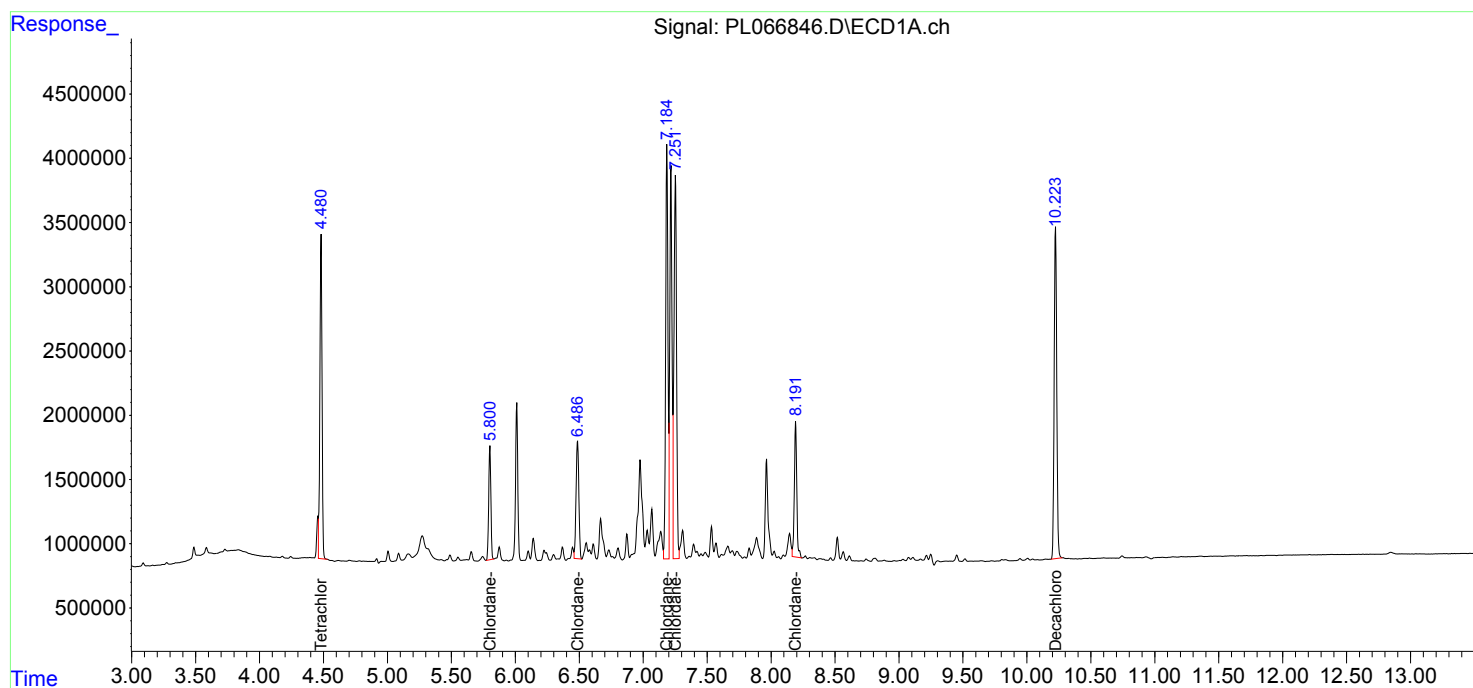


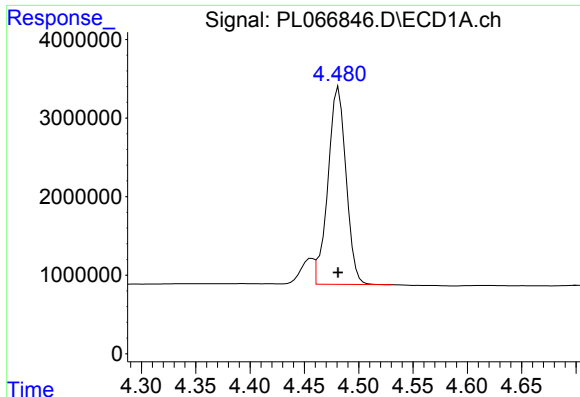

#1 Tetrachloro-m-xylene


R.T.: 4.481 min
Delta R.T.: 0.000 min
Response: 29152735
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

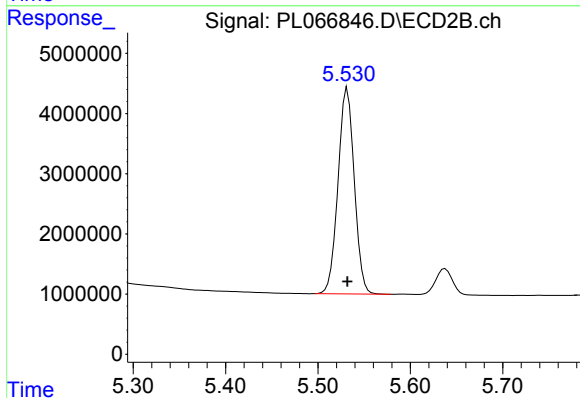


#1 Tetrachloro-m-xylene

R.T.: 5.532 min
Delta R.T.: 0.000 min
Response: 41867776
Conc: 50.00 ng/ml

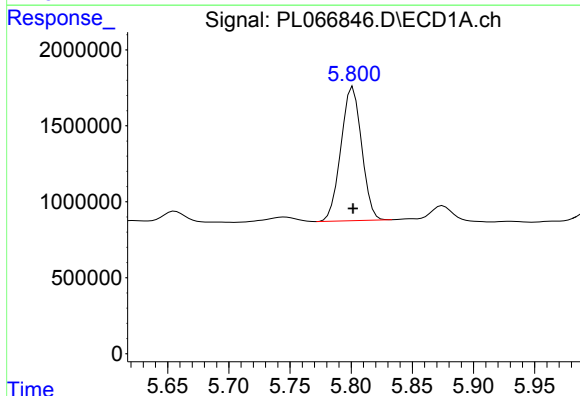


#23 Chlordane-1

R.T.: 5.802 min
Delta R.T.: 0.000 min
Response: 10368761
Conc: 500.00 ng/ml

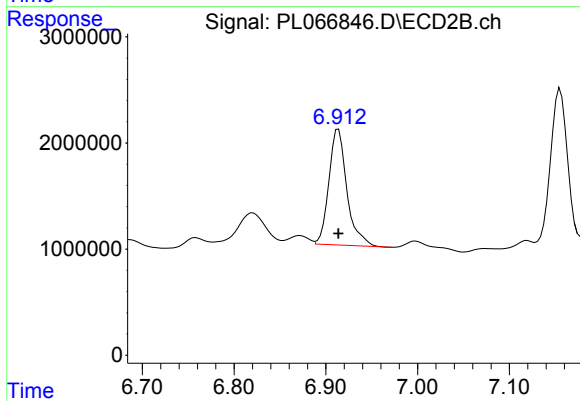

#23 Chlordane-1


R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 14876955
Conc: 500.00 ng/ml

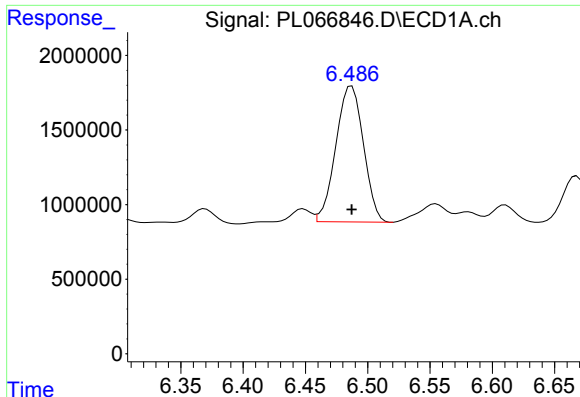

#24 Chlordane-2


R.T.: 6.487 min
Delta R.T.: 0.000 min
Response: 14087229
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

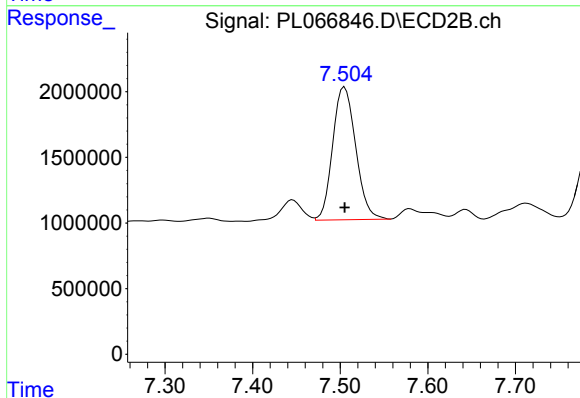


#24 Chlordane-2

R.T.: 7.505 min
Delta R.T.: 0.000 min
Response: 18484134
Conc: 500.00 ng/ml

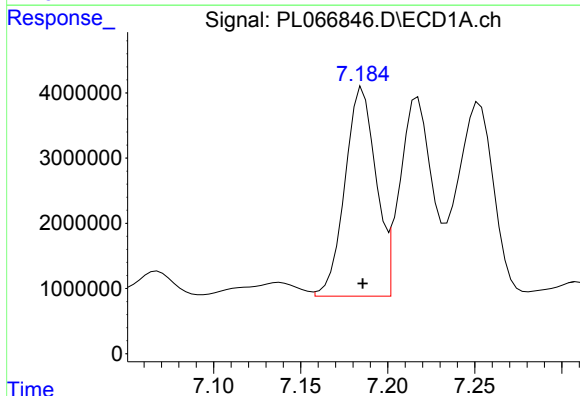


#25 Chlordane-3

R.T.: 7.186 min
Delta R.T.: 0.000 min
Response: 39687987
Conc: 500.00 ng/ml

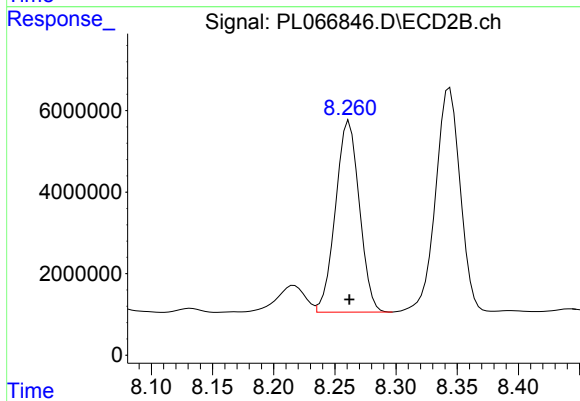

#25 Chlordane-3


R.T.: 8.262 min
Delta R.T.: 0.000 min
Response: 63767979
Conc: 500.00 ng/ml

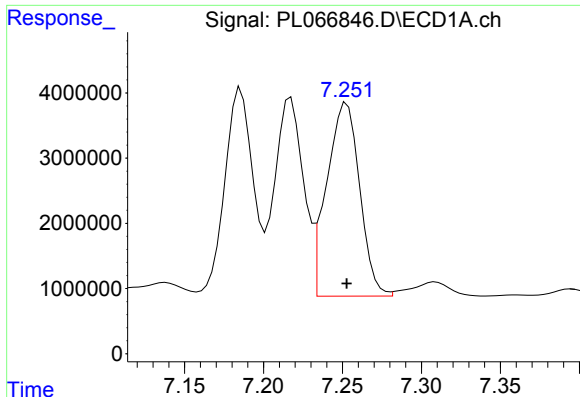

#26 Chlordane-4


R.T.: 7.253 min
Delta R.T.: 0.000 min
Response: 42968611
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

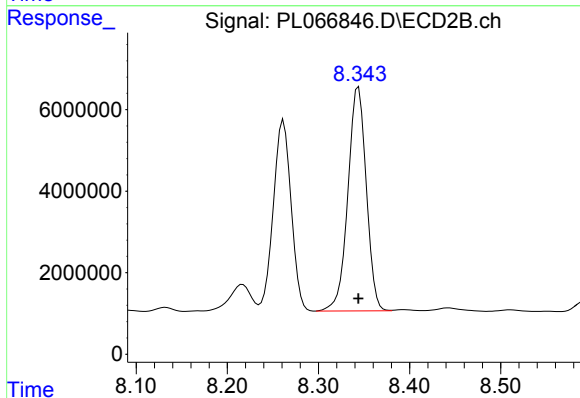


#26 Chlordane-4

R.T.: 8.344 min
Delta R.T.: 0.000 min
Response: 76947163
Conc: 500.00 ng/ml

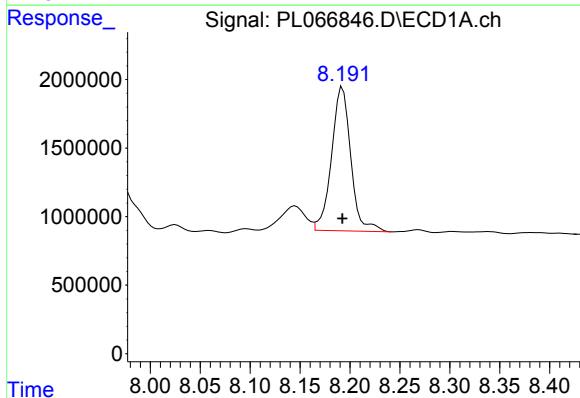


#27 Chlordane-5

R.T.: 8.193 min
Delta R.T.: 0.000 min
Response: 14080245
Conc: 500.00 ng/ml

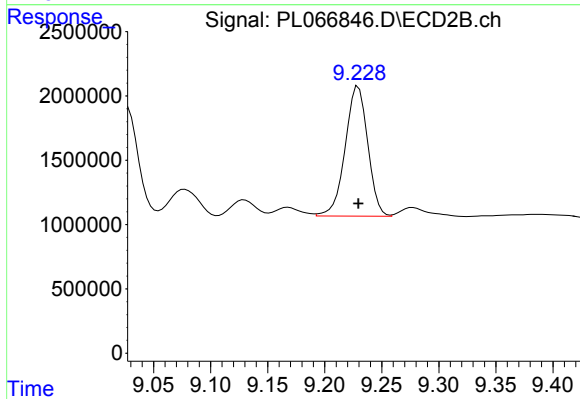

#27 Chlordane-5


R.T.: 9.229 min
Delta R.T.: 0.000 min
Response: 13906422
Conc: 500.00 ng/ml

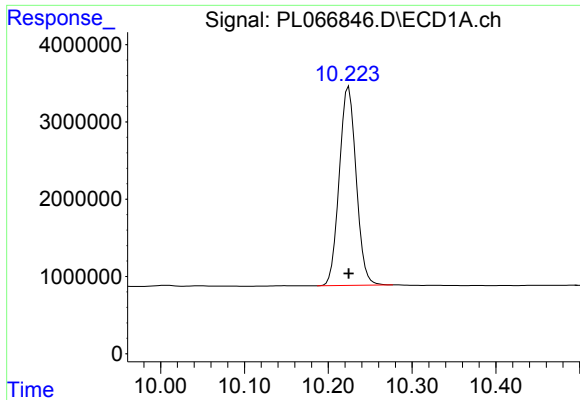

#28 Decachlorobiphenyl

R.T.: 10.224 min
Delta R.T.: 0.000 min
Response: 36041156
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

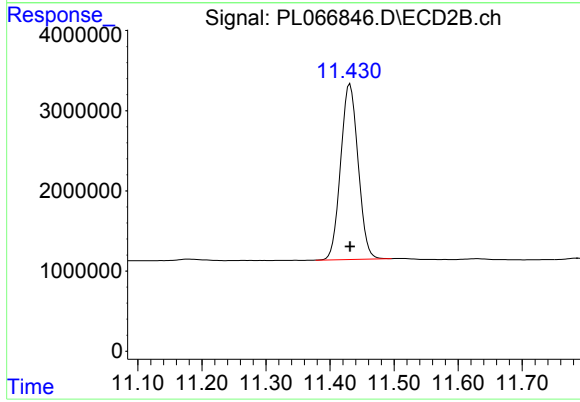

#28 Decachlorobiphenyl

R.T.: 11.431 min
Delta R.T.: 0.000 min
Response: 41363713
Conc: 50.00 ng/ml