

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052422\
 Data File : PL074972.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2022 09:13
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 25 02:12:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.645	4.648	11073700	28993552	21.810	21.124
28)	SA Decachlor...	11.640	10.396	11145403	25488070	24.957	24.832
Target Compounds							
4)	MA Heptachlor	0.000	6.160f	0	104766	N.D.	0.069 #
6)	B beta-BHC	0.000	6.160	0	104766	N.D.	0.132 #
8)	B Heptachlo...	8.126	0.000	1035270	0	1.820	N.D. #
10)	B gamma-Chl...	8.380f	0.000	379849	0	0.734	N.D. #
13)	MA Dieldrin	0.000	7.780	0	1055036	N.D.	0.828 #
14)	MA Endrin	0.000	8.078	0	701370	N.D.	0.664 #
21)	B Endrin ke...	10.187	0.000	401796	0	0.783	N.D. #
25)	Chlordane-3	8.380f	0.000	379849	0	5.549	N.D. #
27)	Chlordane-5	0.000	8.164f	0	474656	N.D.	12.838 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052422\
Data File : PL074972.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2022 09:13
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 25 02:12:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

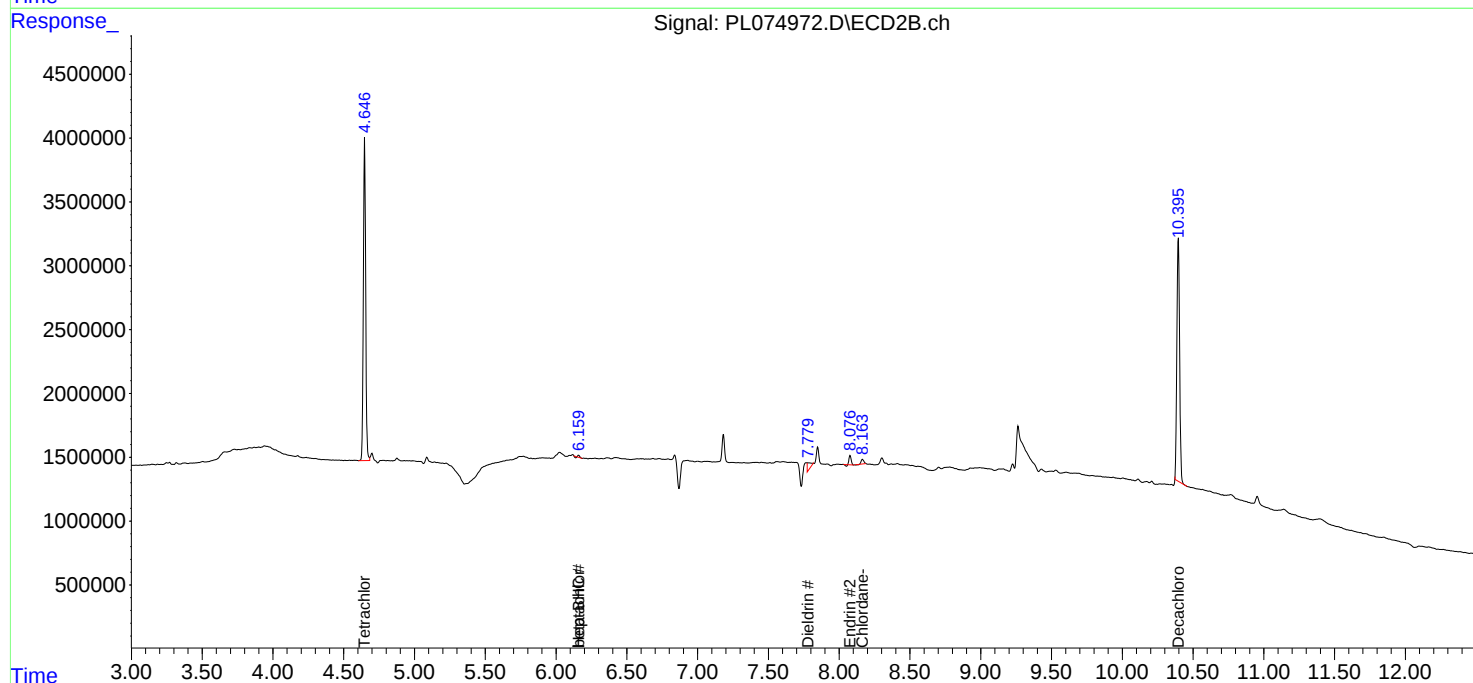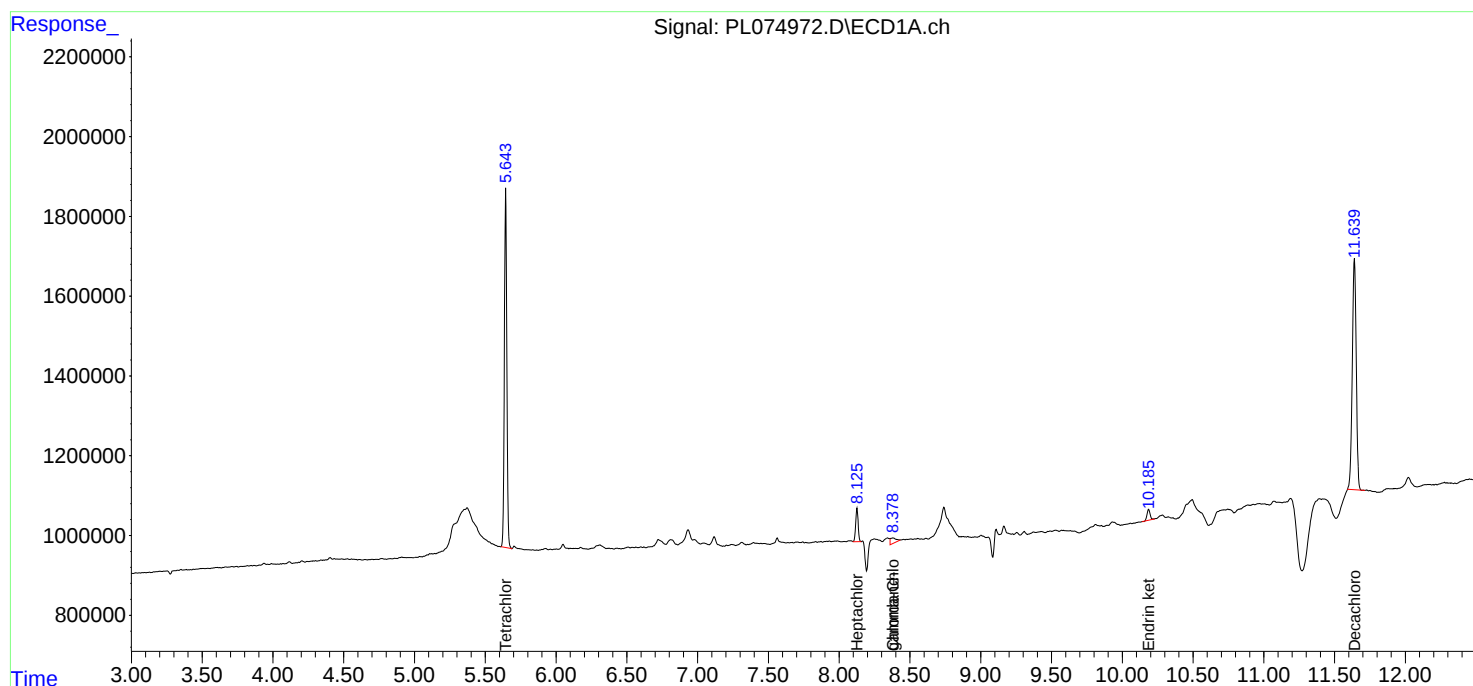


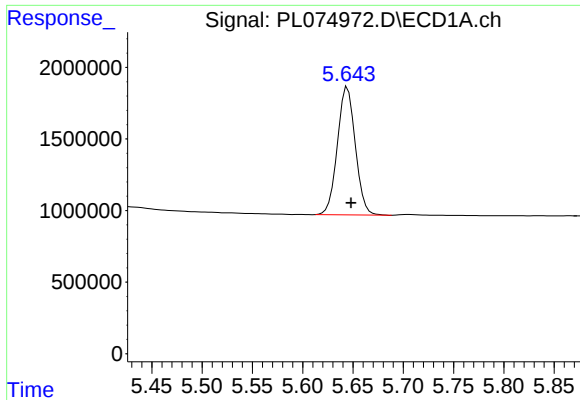

#1 Tetrachloro-m-xylene


R.T.: 5.645 min
Delta R.T.: -0.003 min
Response: 11073700
Conc: 21.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

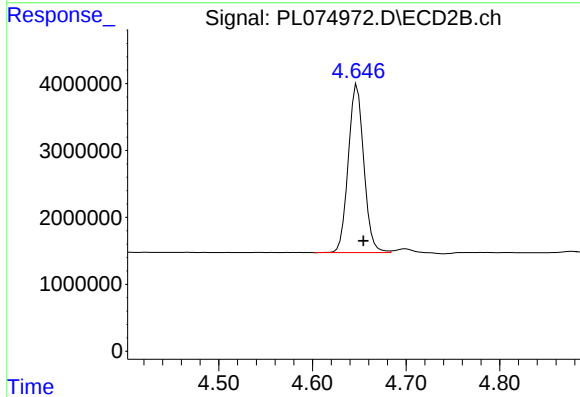


#1 Tetrachloro-m-xylene

R.T.: 4.648 min
Delta R.T.: -0.007 min
Response: 28993552
Conc: 21.12 ng/ml

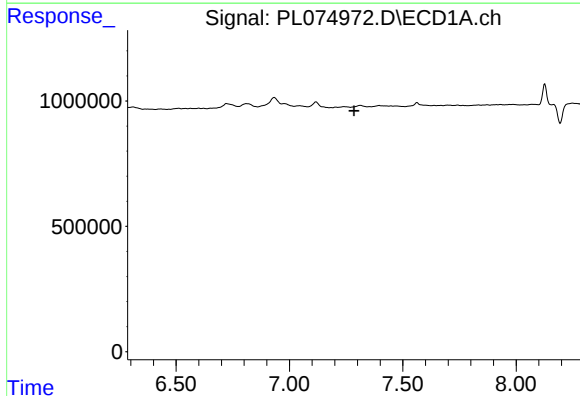


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.286 min
Response: 0
Conc: N.D.

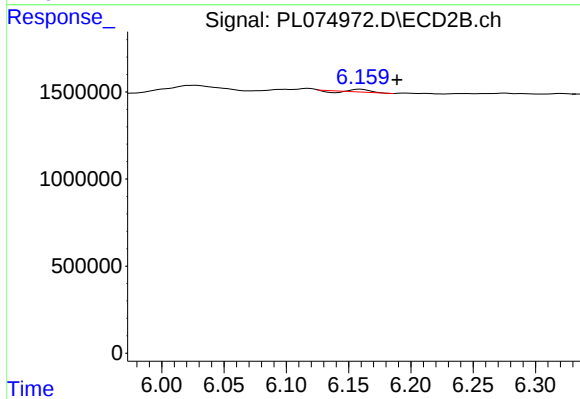

#4 Heptachlor


R.T.: 6.160 min
Delta R.T.: -0.029 min
Response: 104766
Conc: 0.07 ng/ml

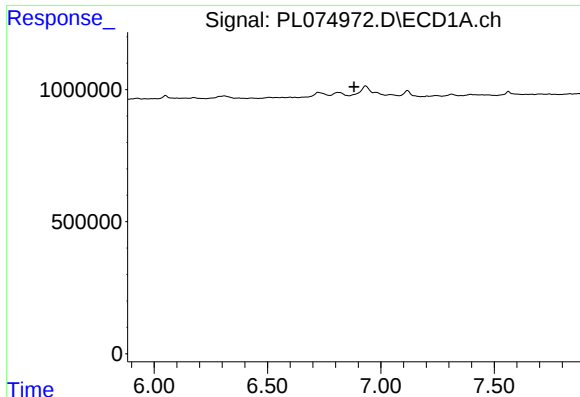

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.882 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

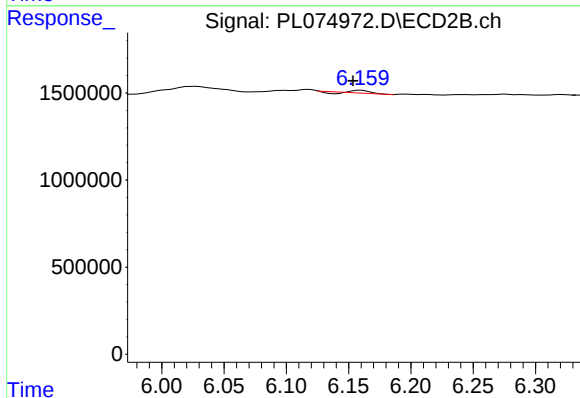


#6 beta-BHC

R.T.: 6.160 min
Delta R.T.: 0.006 min
Response: 104766
Conc: 0.13 ng/ml

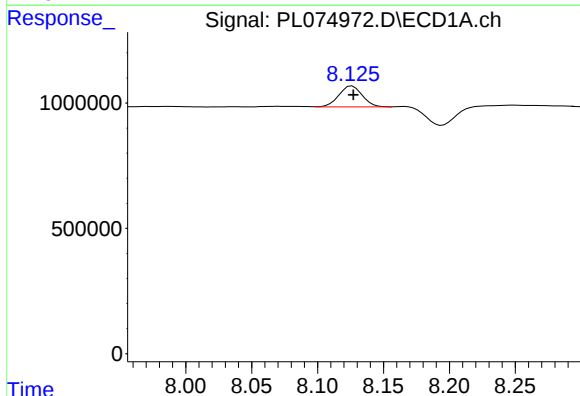


#8 Heptachlor epoxide

R.T.: 8.126 min
Delta R.T.: -0.001 min
Response: 1035270
Conc: 1.82 ng/ml

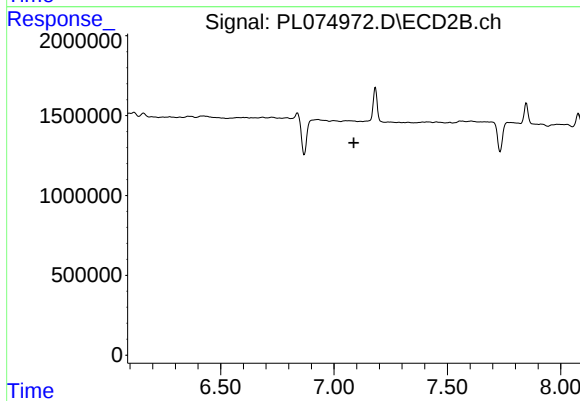

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 7.087 min
Response: 0
Conc: N.D.

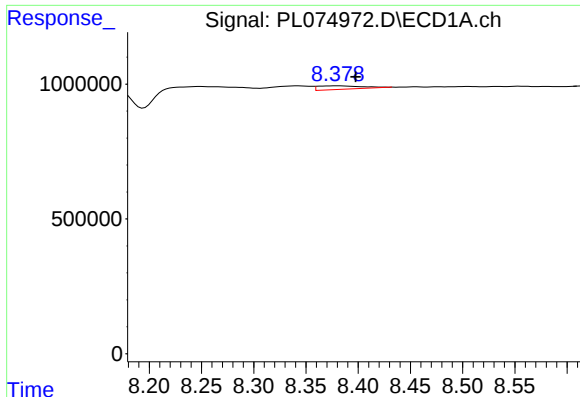

#10 gamma-Chlordane


R.T.: 8.380 min
Delta R.T.: -0.018 min
Response: 379849
Conc: 0.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

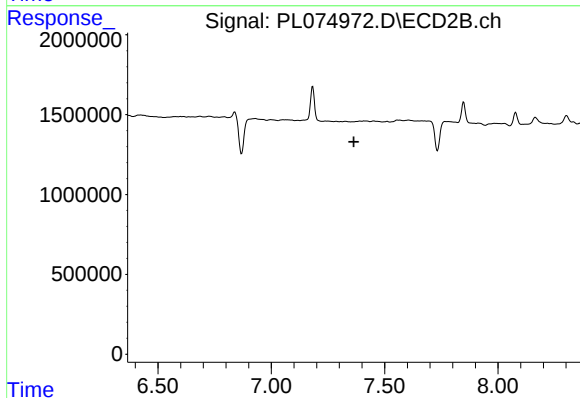


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.363 min
Response: 0
Conc: N.D.

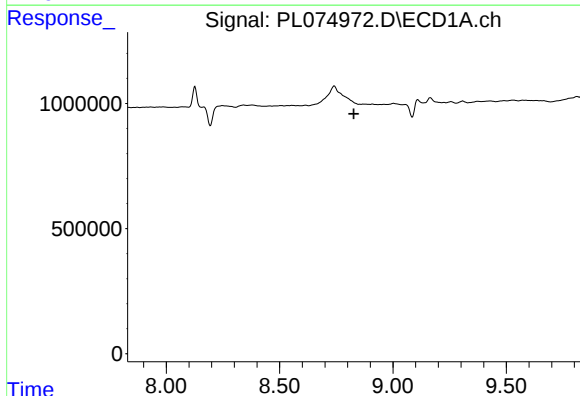


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.827 min
Response: 0
Conc: N.D.

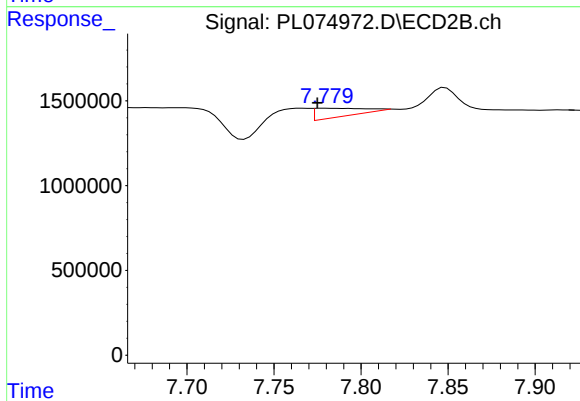

#13 Dieldrin


R.T.: 7.780 min
Delta R.T.: 0.005 min
Response: 1055036
Conc: 0.83 ng/ml

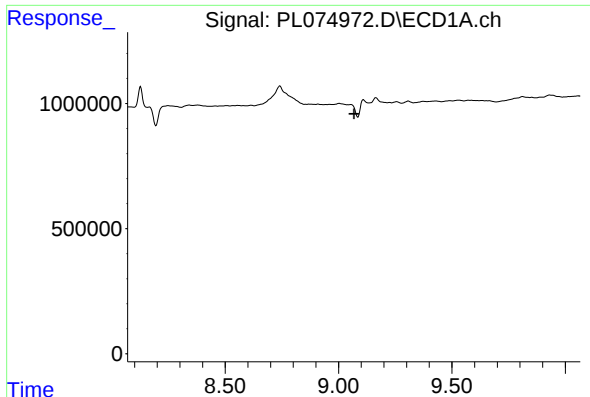

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.068 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

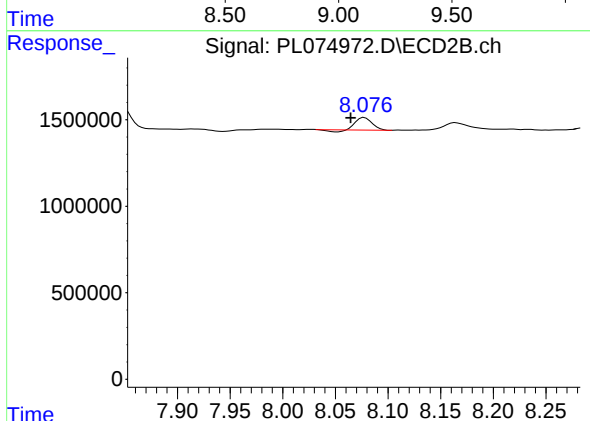


#14 Endrin

R.T.: 8.078 min
Delta R.T.: 0.013 min
Response: 701370
Conc: 0.66 ng/ml

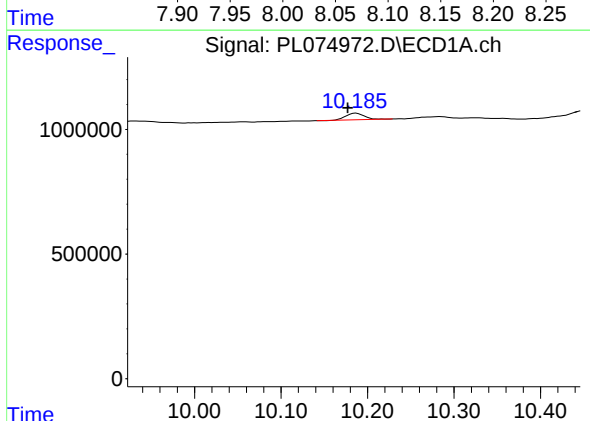


#21 Endrin ketone

R.T.: 10.187 min
Delta R.T.: 0.009 min
Response: 401796
Conc: 0.78 ng/ml

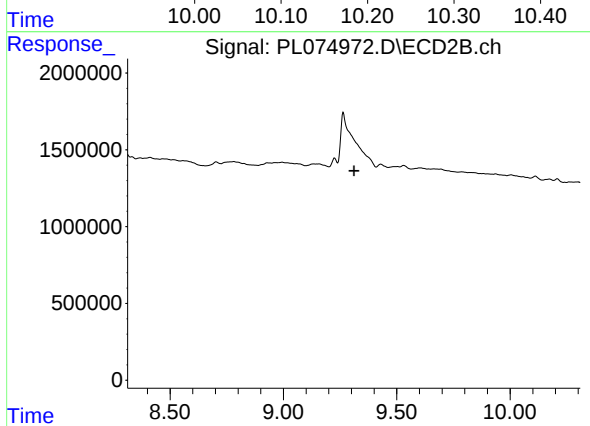

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.311 min
Response: 0
Conc: N.D.

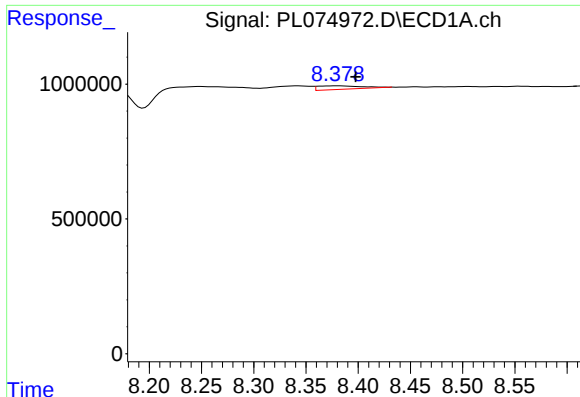

#25 Chlordane-3


R.T.: 8.380 min
Delta R.T.: -0.018 min
Response: 379849
Conc: 5.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

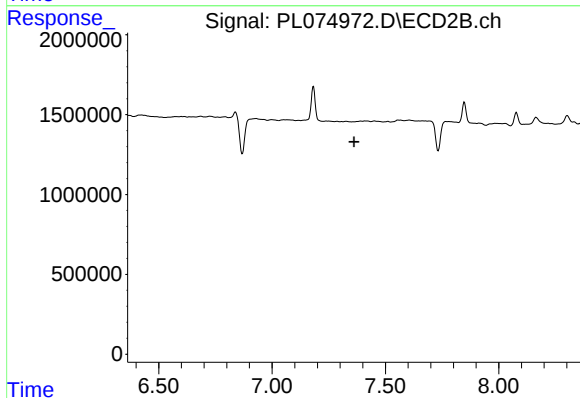


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.362 min
Response: 0
Conc: N.D.

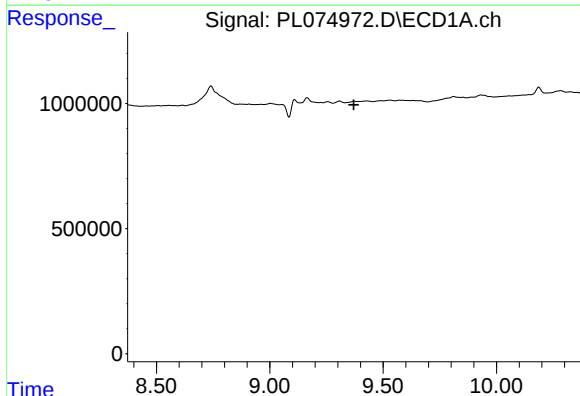


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.371 min
Response: 0
Conc: N.D.

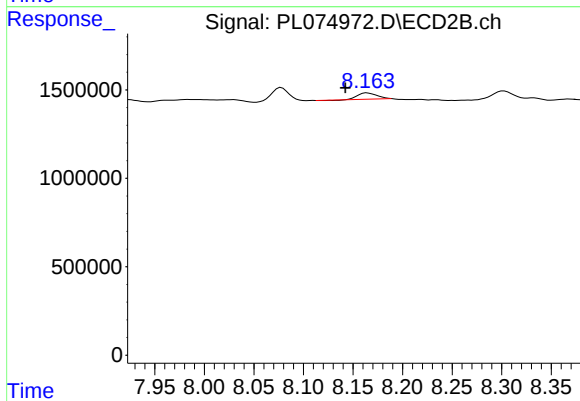

#27 Chlordane-5


R.T.: 8.164 min
Delta R.T.: 0.022 min
Response: 474656
Conc: 12.84 ng/ml

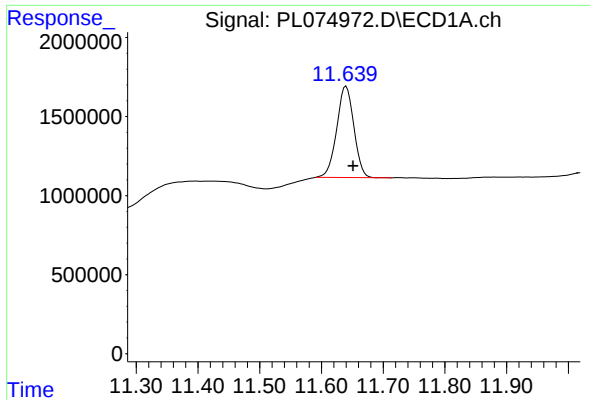

#28 Decachlorobiphenyl

R.T.: 11.640 min
Delta R.T.: -0.011 min
Response: 11145403
Conc: 24.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

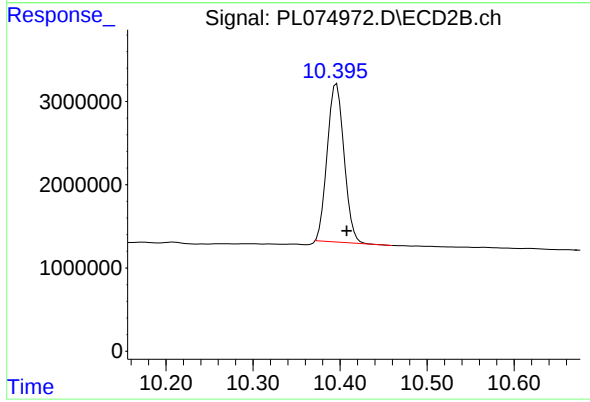

#28 Decachlorobiphenyl

R.T.: 10.396 min
Delta R.T.: -0.012 min
Response: 25488070
Conc: 24.83 ng/ml