

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052422\
 Data File : PL074988.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2022 17:53
 Operator : AR\AJ
 Sample : N2896-20
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 25 02:18:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.643	4.647	2807139	8074961	5.529	5.883
28)	SA Decachlor...	11.637	10.396	6190581	15277095	13.862	14.884
Target Compounds							
8)	B Heptachlo...	8.125	0.000	6963	0	0.012	N.D. #
10)	B gamma-Chl...	0.000	7.392f	0	210852	N.D.	0.152 #
13)	MA Dieldrin	8.812f	7.797f	223692	435006	0.426	0.341
14)	MA Endrin	0.000	8.071	0	837867	N.D.	0.793 #
16)	A 4,4'-DDD	9.202	0.000	1179238	0	2.608	N.D. #
17)	MA 4,4'-DDT	0.000	8.472f	0	1397602	N.D.	1.397 #
19)	B Endosulfa...	0.000	8.782	0	1627370	N.D.	1.495 #
21)	B Endrin ke...	0.000	9.334f	0	1639557	N.D.	1.471 #
22)	Mirex	10.642	0.000	312505	0	0.774	N.D. #
27)	Chlordane-5	0.000	8.134	0	3014909	N.D.	81.542 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052422\
Data File : PL074988.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2022 17:53
Operator : AR\AJ
Sample : N2896-20
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 25 02:18:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

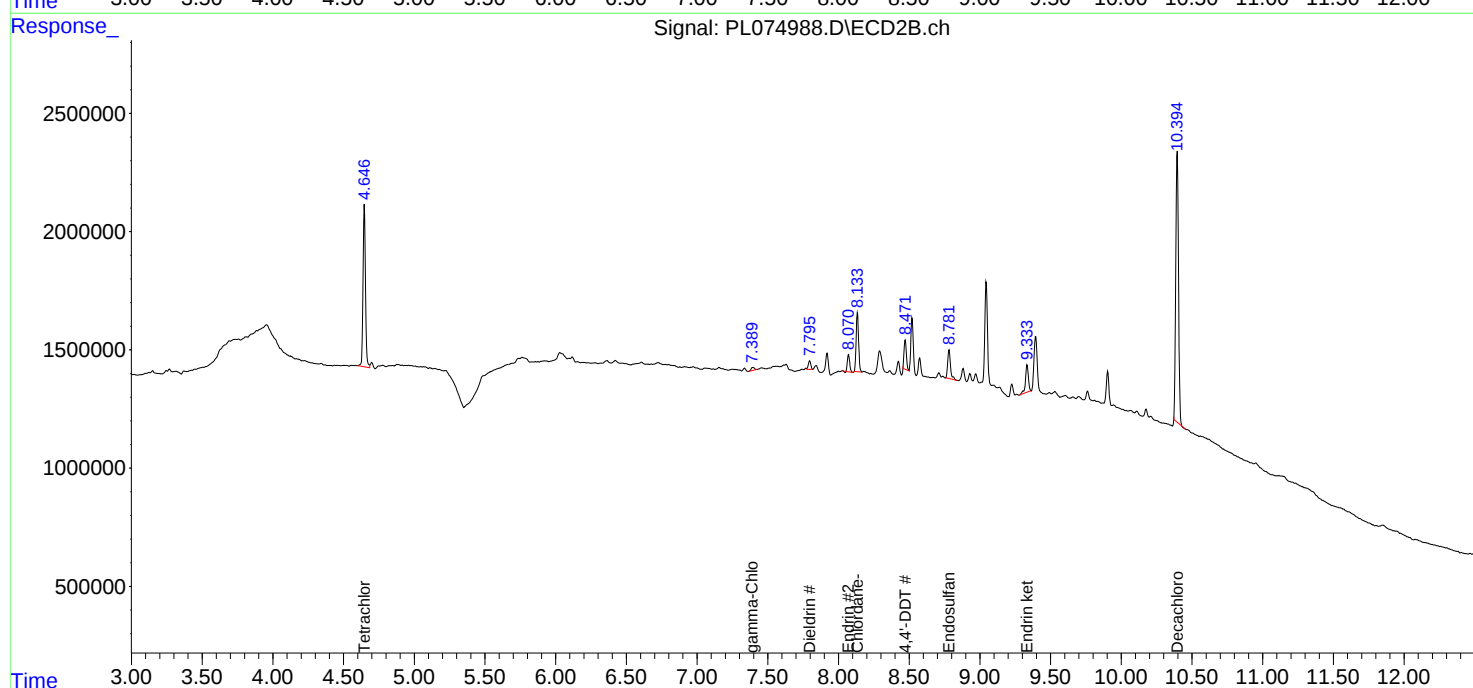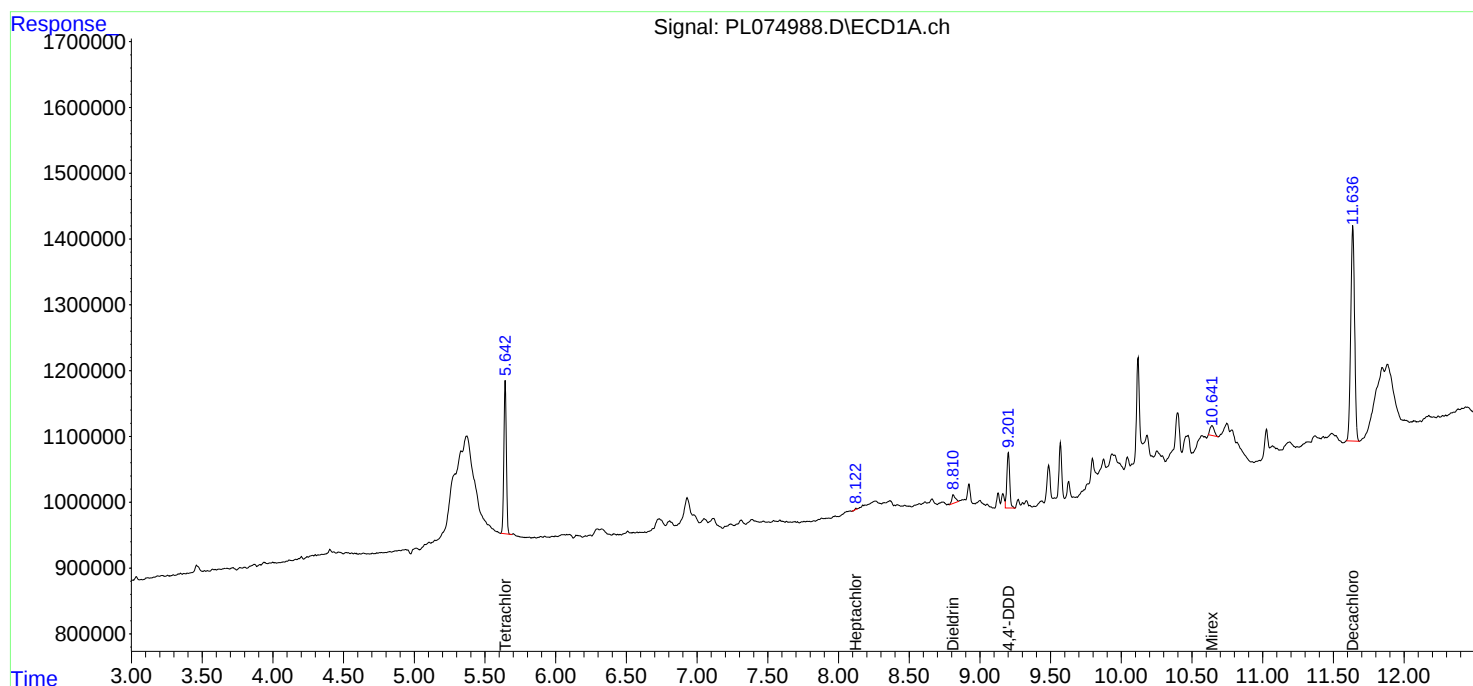


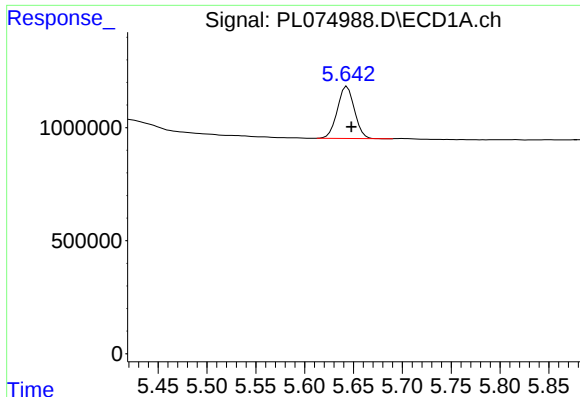

#1 Tetrachloro-m-xylene


R.T.: 5.643 min
Delta R.T.: -0.005 min
Response: 2807139
Conc: 5.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

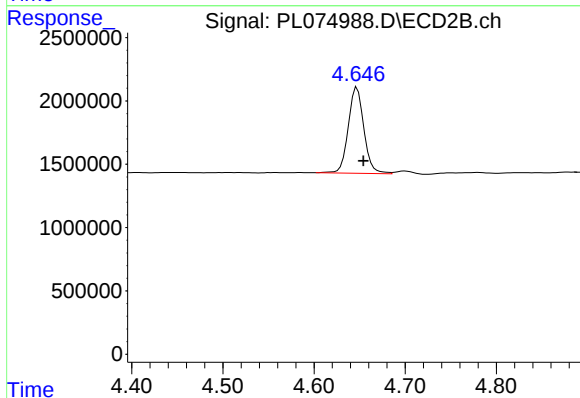


#1 Tetrachloro-m-xylene

R.T.: 4.647 min
Delta R.T.: -0.007 min
Response: 8074961
Conc: 5.88 ng/ml

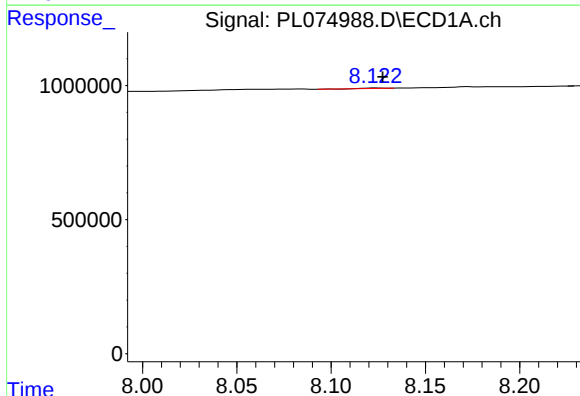


#8 Heptachlor epoxide

R.T.: 8.125 min
Delta R.T.: -0.003 min
Response: 6963
Conc: 0.01 ng/ml

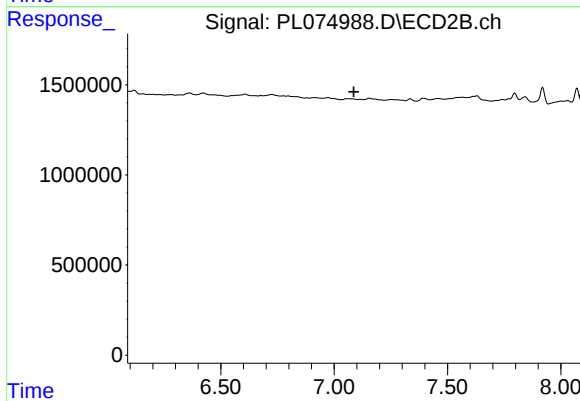

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 7.087 min
Response: 0
Conc: N.D.

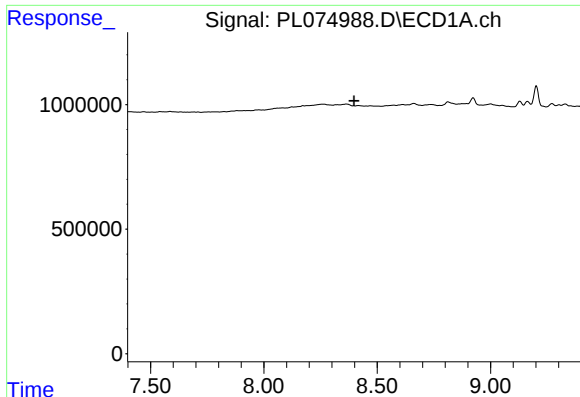

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

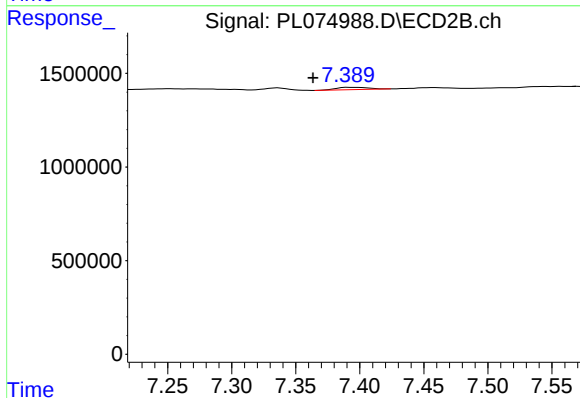


#10 gamma-Chlordane

R.T.: 7.392 min
Delta R.T.: 0.028 min
Response: 210852
Conc: 0.15 ng/ml

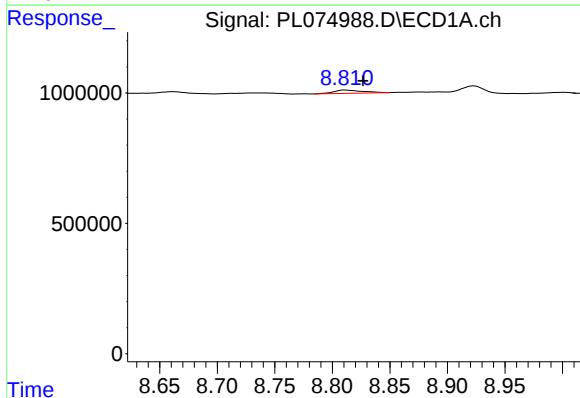


#13 Dieldrin

R.T.: 8.812 min
Delta R.T.: -0.015 min
Response: 223692
Conc: 0.43 ng/ml

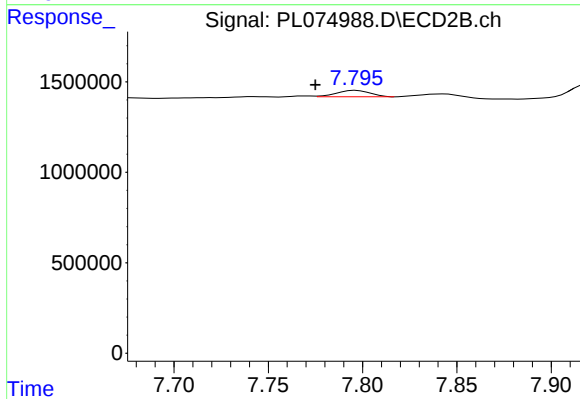

#13 Dieldrin


R.T.: 7.797 min
Delta R.T.: 0.022 min
Response: 435006
Conc: 0.34 ng/ml

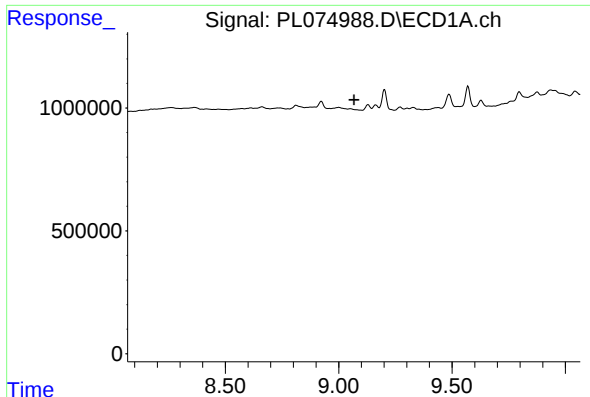

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.068 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

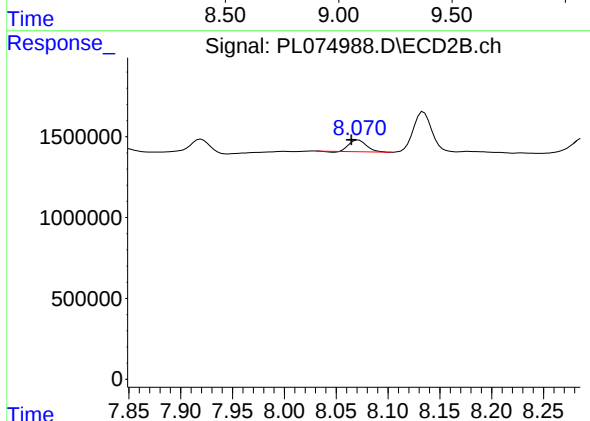


#14 Endrin

R.T.: 8.071 min
Delta R.T.: 0.007 min
Response: 837867
Conc: 0.79 ng/ml

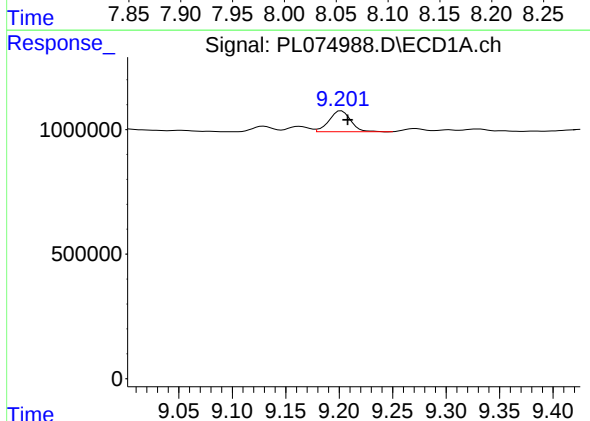


#16 4,4'-DDD

R.T.: 9.202 min
Delta R.T.: -0.006 min
Response: 1179238
Conc: 2.61 ng/ml

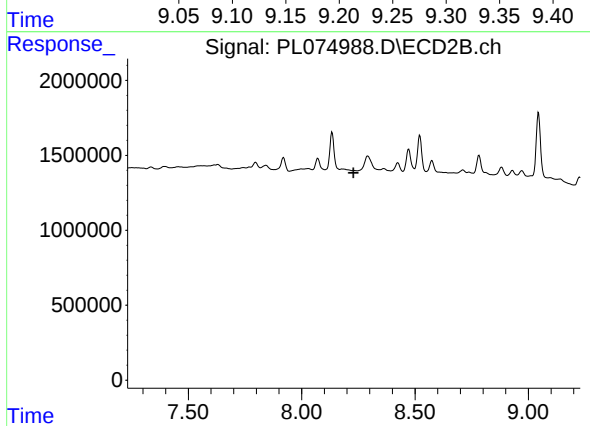

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.229 min
Response: 0
Conc: N.D.

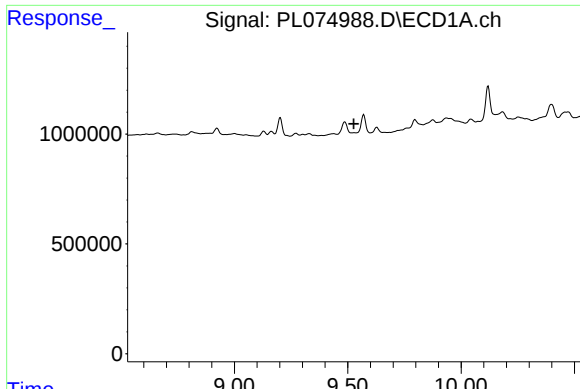

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 9.527 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

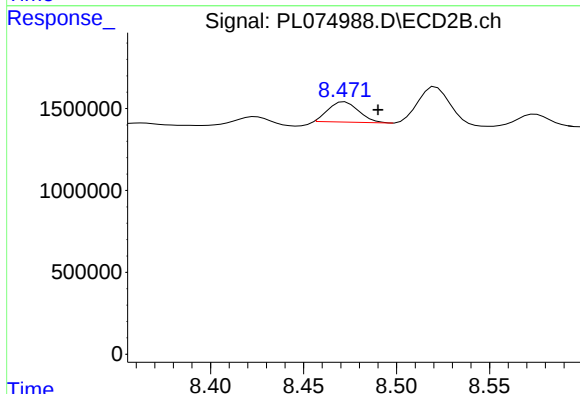


#17 4,4'-DDT

R.T.: 8.472 min
Delta R.T.: -0.018 min
Response: 1397602
Conc: 1.40 ng/ml

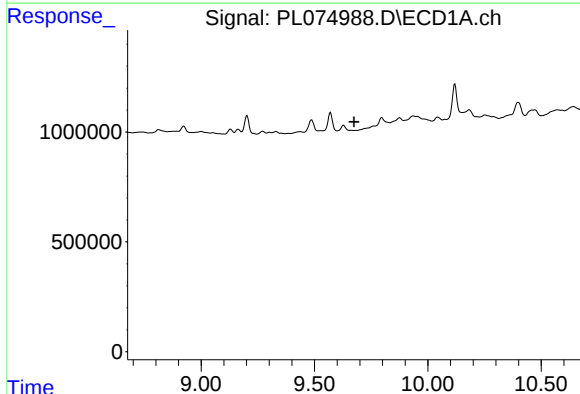


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 9.675 min
Response: 0
Conc: N.D.

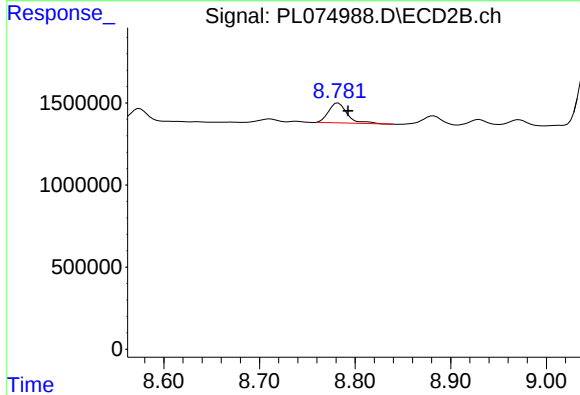

#19 Endosulfan Sulfate


R.T.: 8.782 min
Delta R.T.: -0.010 min
Response: 1627370
Conc: 1.49 ng/ml

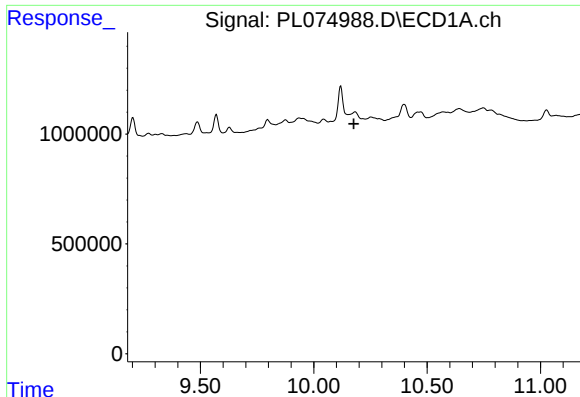

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 10.177 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

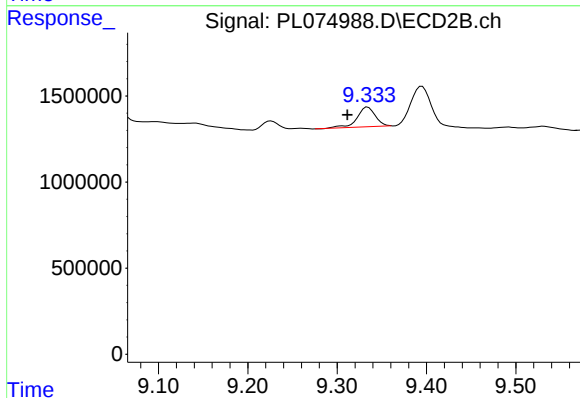


#21 Endrin ketone

R.T.: 9.334 min
Delta R.T.: 0.023 min
Response: 1639557
Conc: 1.47 ng/ml

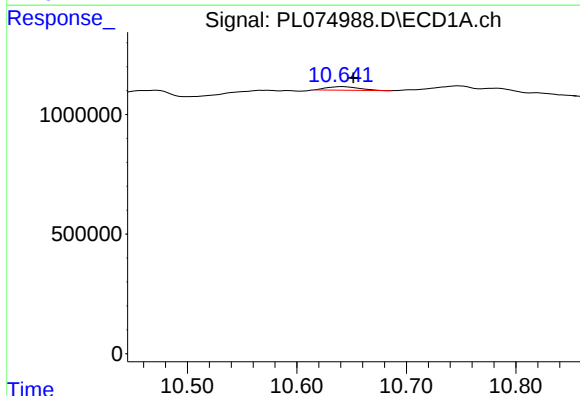


#22 Mirex

R.T.: 10.642 min
Delta R.T.: -0.010 min
Response: 312505
Conc: 0.77 ng/ml

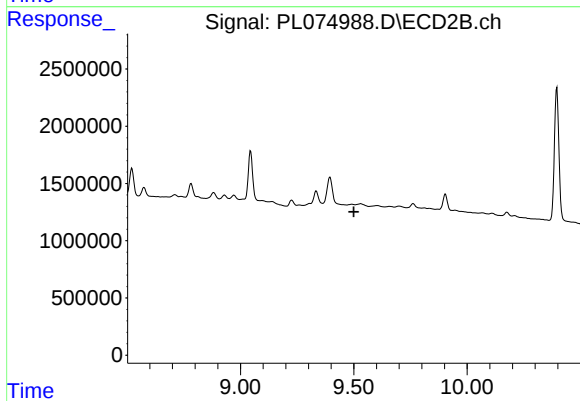

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 9.501 min
Response: 0
Conc: N.D.

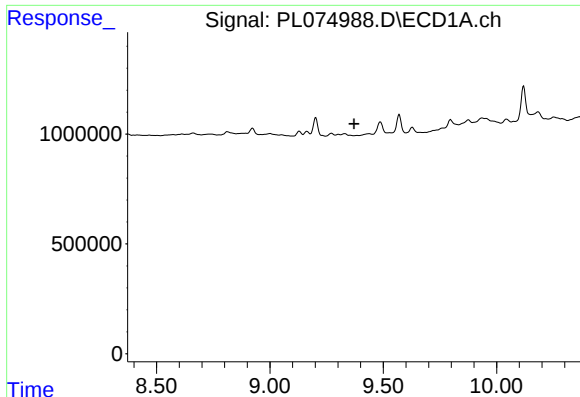

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 9.371 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

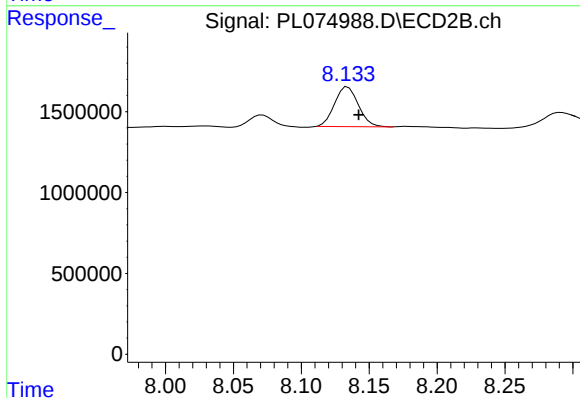


#27 Chlordane-5

R.T.: 8.134 min
Delta R.T.: -0.008 min
Response: 3014909
Conc: 81.54 ng/ml

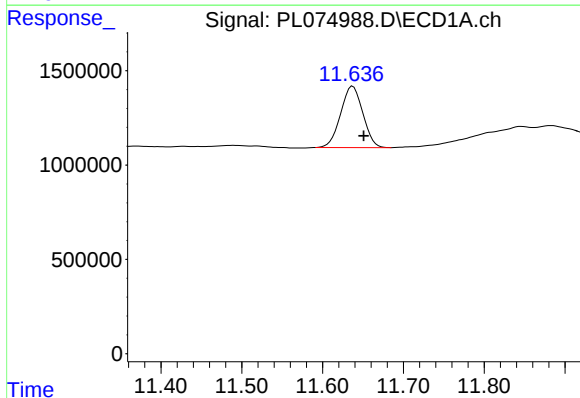

#28 Decachlorobiphenyl

R.T.: 11.637 min
Delta R.T.: -0.014 min
Response: 6190581
Conc: 13.86 ng/ml

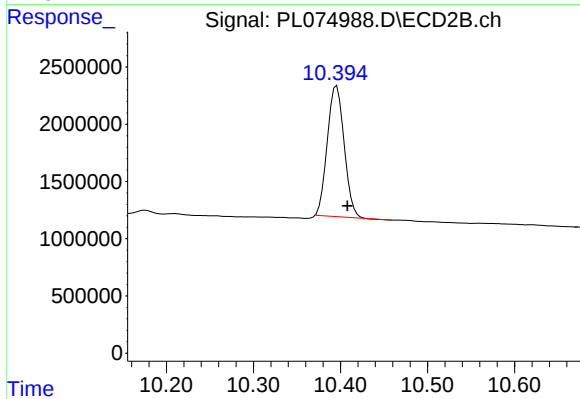

#28 Decachlorobiphenyl

R.T.: 10.396 min
Delta R.T.: -0.012 min
Response: 15277095
Conc: 14.88 ng/ml