

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052423\
 Data File : PL082965.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2023 13:22
 Operator : AR\AJ
 Sample : 02830-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SEMI-ANNUAL-CONDENSATE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/26/2023
 Supervised By :Ankita Jodhani 05/26/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 21:21:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
 Quant Title : GC Extractables
 QLast Update : Sat May 20 04:58:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.316	2.635	123.7E6	43096892	42.092	16.601m#
28)	SA Decachlor...	8.744	7.748	21030727	51298293	10.027m	20.630 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052423\
Data File : PL082965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2023 13:22
Operator : AR\AJ
Sample : 02830-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SEMI-ANNUAL-CONDENSATE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/26/2023
Supervised By : Ankita Jodhani 05/26/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 21:21:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
Quant Title : GC Extractables
QLast Update : Sat May 20 04:58:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

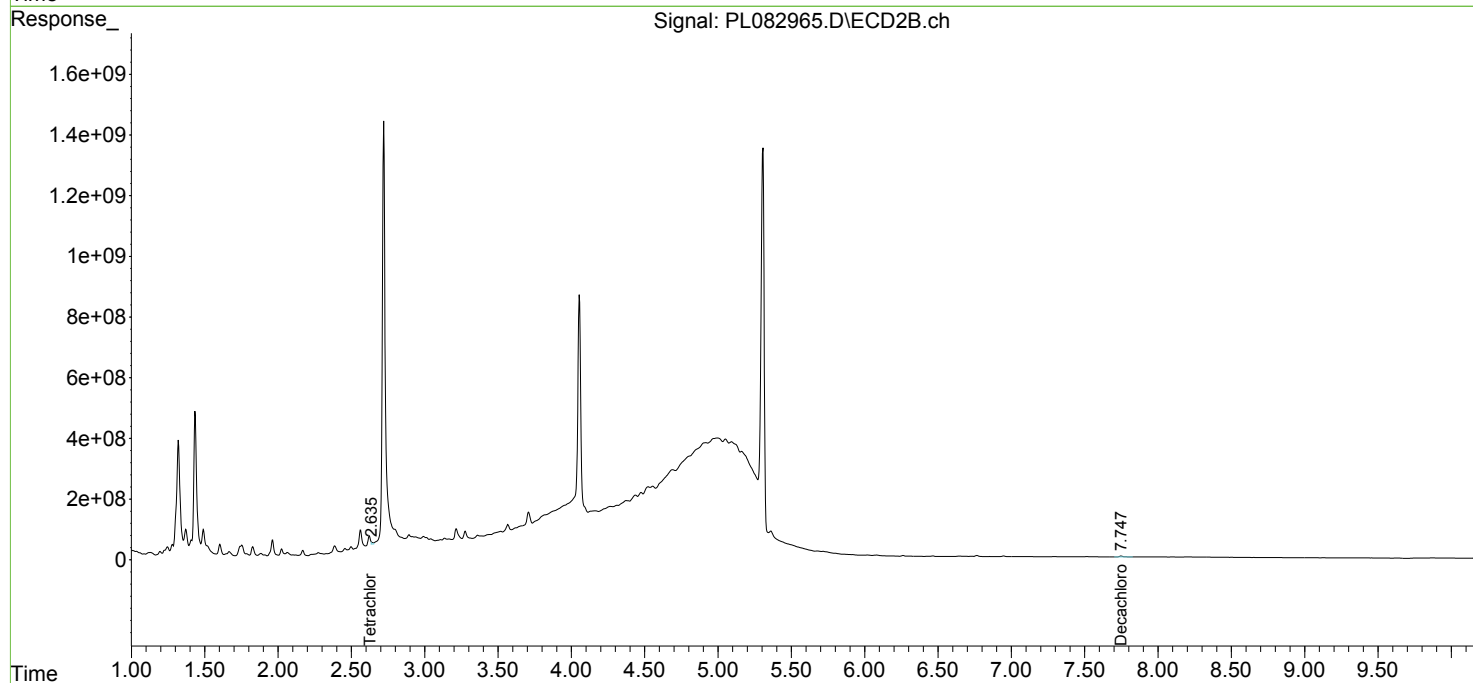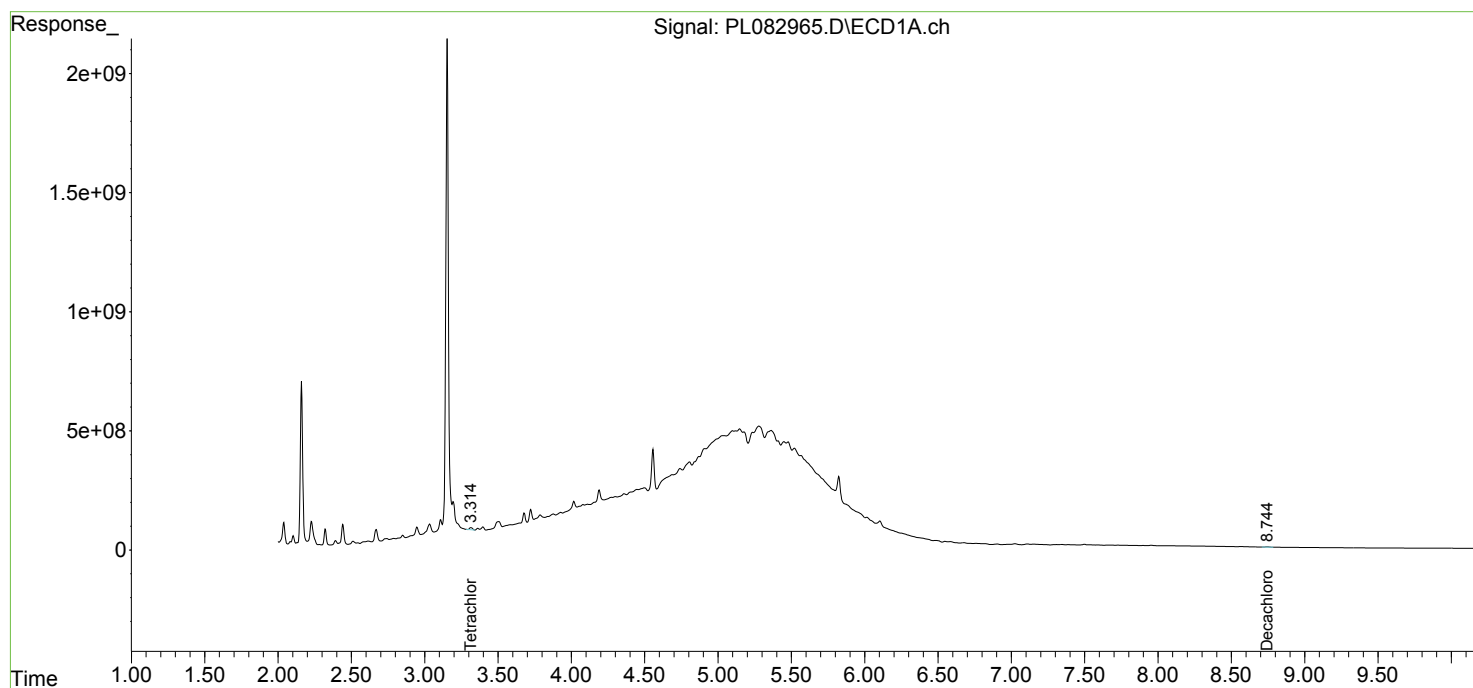

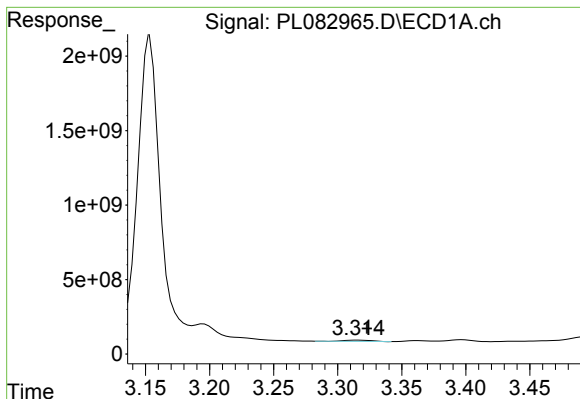


#1 Tetrachloro-m-xylene

R.T.: 3.316 min
Delta R.T.: -0.007 min
Response: 123709489
Conc: 42.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
SEMI-ANNUAL-CONDENSATE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/26/2023
Supervised By :Ankita Jodhani 05/26/2023

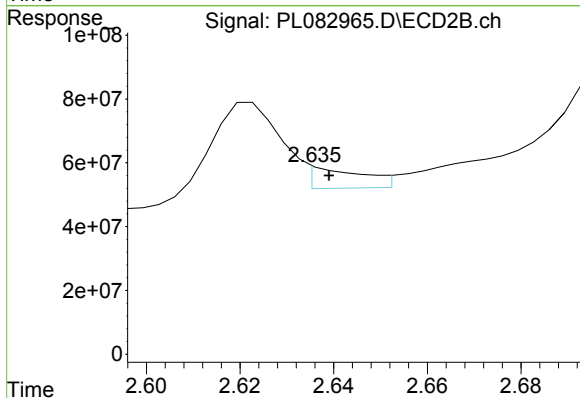


#1 Tetrachloro-m-xylene

R.T.: 2.635 min
Delta R.T.: -0.004 min
Response: 43096892
Conc: 16.60 ng/ml m

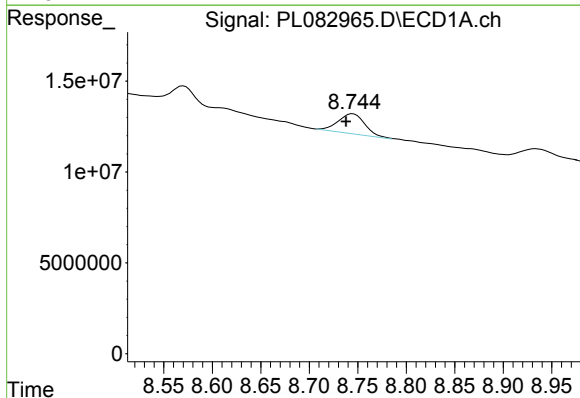

#28 Decachlorobiphenyl

R.T.: 8.744 min
Delta R.T.: 0.006 min
Response: 21030727
Conc: 10.03 ng/ml m

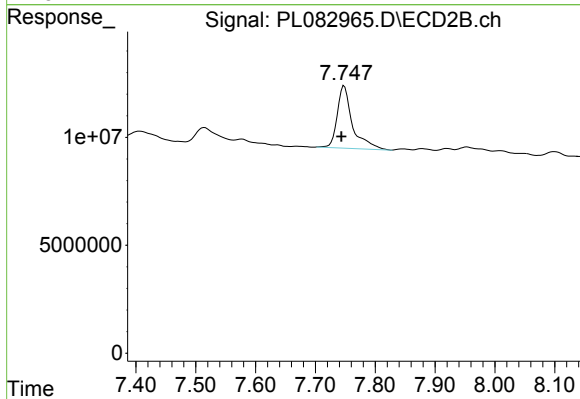

#28 Decachlorobiphenyl

R.T.: 7.748 min
Delta R.T.: 0.005 min
Response: 51298293
Conc: 20.63 ng/ml