

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052424\
 Data File : PL089714.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2024 12:10
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 14:29:42 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052424.M
 Quant Title : GC Extractables
 QLast Update : Fri May 24 14:27:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	2.793	165.7E6	158.4E6	97.884	101.192
28)	SA Decachlor...	9.060	7.941	120.2E6	129.4E6	96.793	99.047
Target Compounds							
23)	Chlordane-1	4.711	3.796	98288681	64313561	971.565	1009.995
24)	Chlordane-2	5.239	4.373	103.7E6	73499606	958.871	985.638
25)	Chlordane-3	5.949	5.004	366.9E6	230.1E6	991.138	1027.734
26)	Chlordane-4	6.031	5.068	446.3E6	211.9E6	988.936	1011.326
27)	Chlordane-5	6.879	5.733	87097759	63984824	970.097	1001.416



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052424\
Data File : PL089714.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2024 12:10
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 14:29:42 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052424.M
Quant Title : GC Extractables
QLast Update : Fri May 24 14:27:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

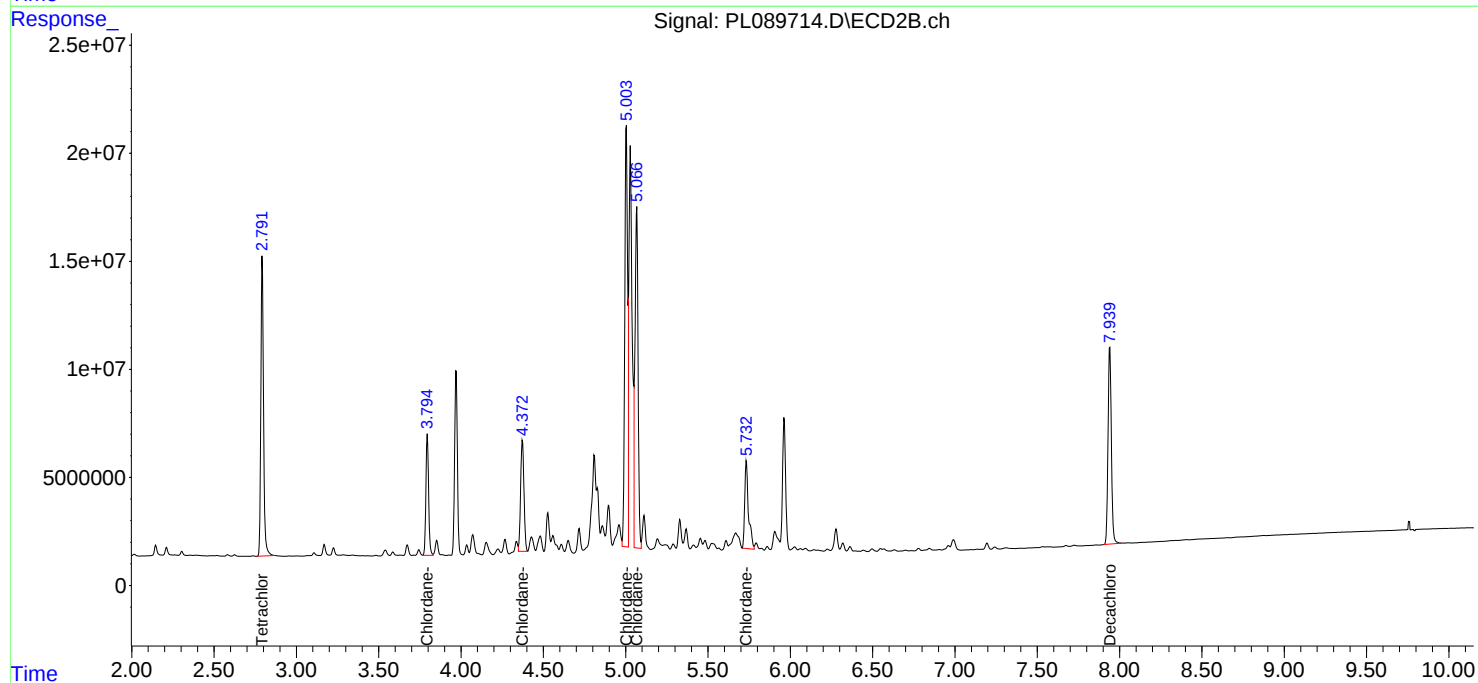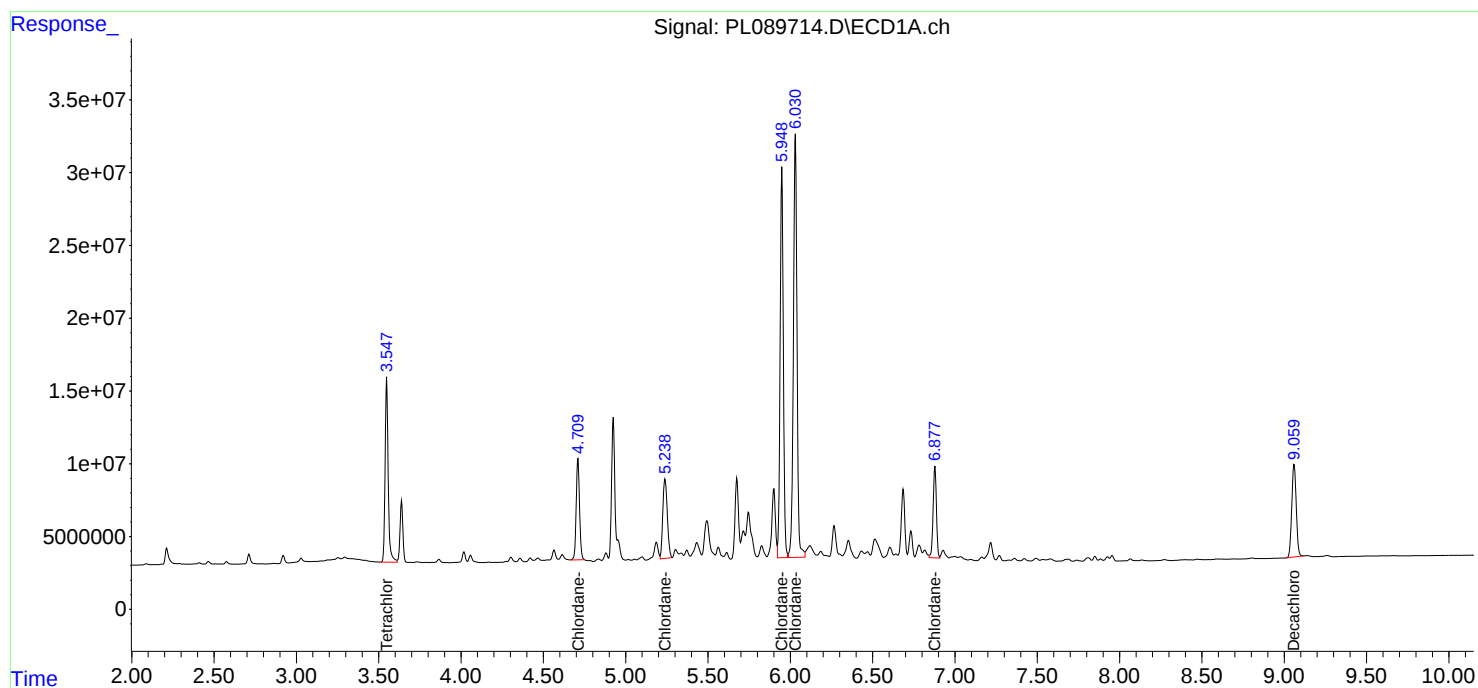


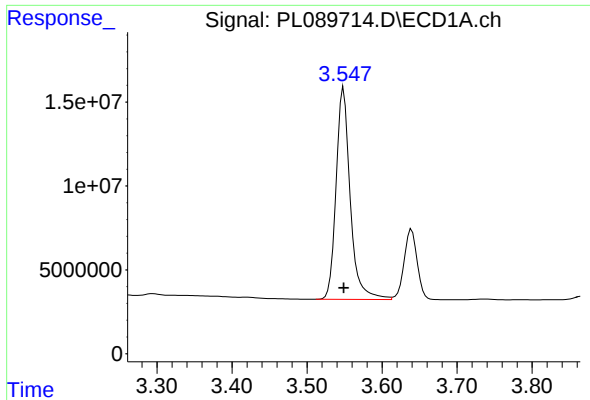

#1 Tetrachloro-m-xylene


R.T.: 3.549 min
Delta R.T.: 0.000 min
Response: 165740832
Conc: 97.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

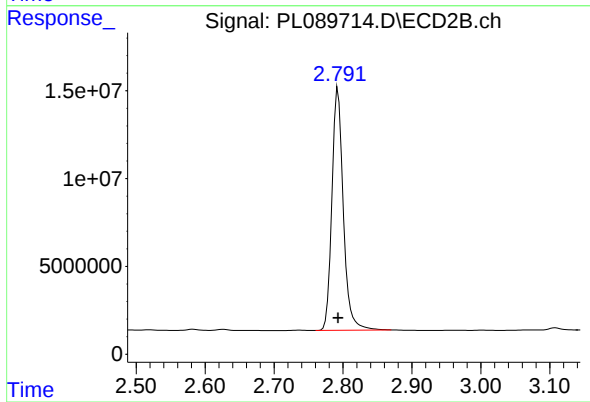


#1 Tetrachloro-m-xylene

R.T.: 2.793 min
Delta R.T.: 0.000 min
Response: 158435443
Conc: 101.19 ng/ml

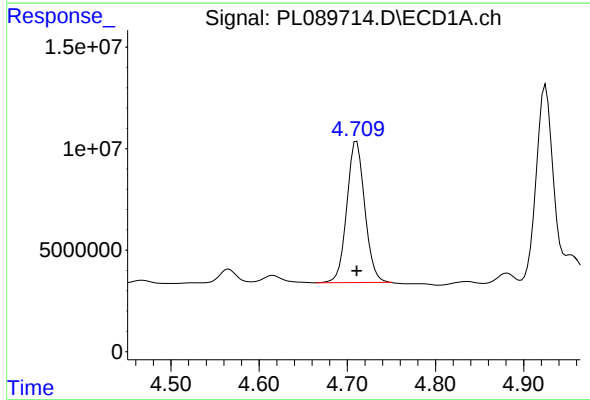


#23 Chlordane-1

R.T.: 4.711 min
Delta R.T.: 0.000 min
Response: 98288681
Conc: 971.56 ng/ml

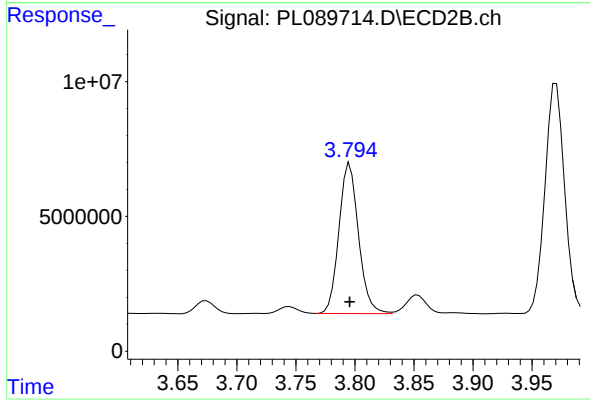

#23 Chlordane-1


R.T.: 3.796 min
Delta R.T.: 0.000 min
Response: 64313561
Conc: 1010.00 ng/ml

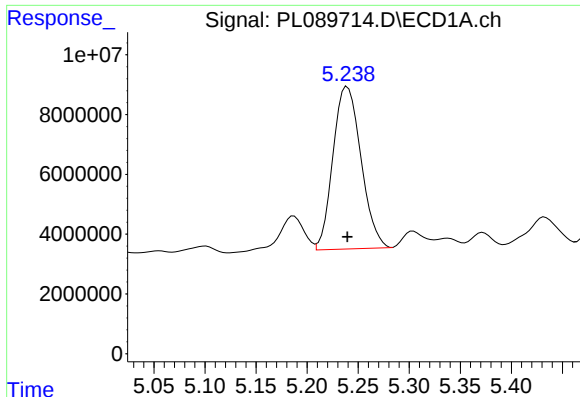

#24 Chlordane-2


R.T.: 5.239 min
Delta R.T.: 0.000 min
Response: 103733192
Conc: 958.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

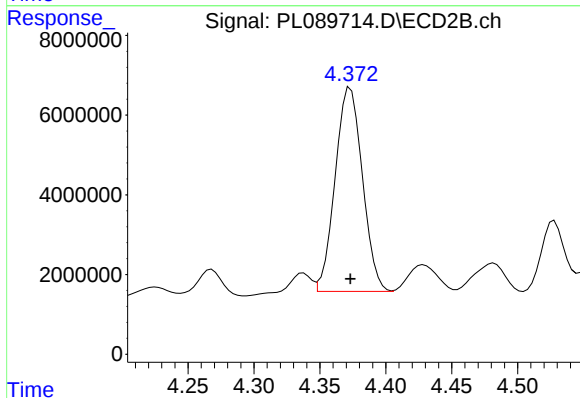


#24 Chlordane-2

R.T.: 4.373 min
Delta R.T.: 0.000 min
Response: 73499606
Conc: 985.64 ng/ml

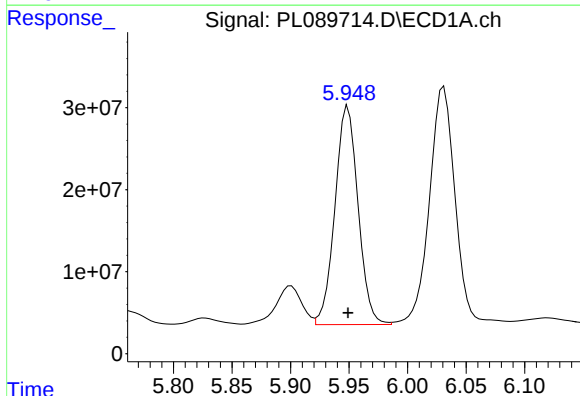


#25 Chlordane-3

R.T.: 5.949 min
Delta R.T.: 0.000 min
Response: 366856909
Conc: 991.14 ng/ml

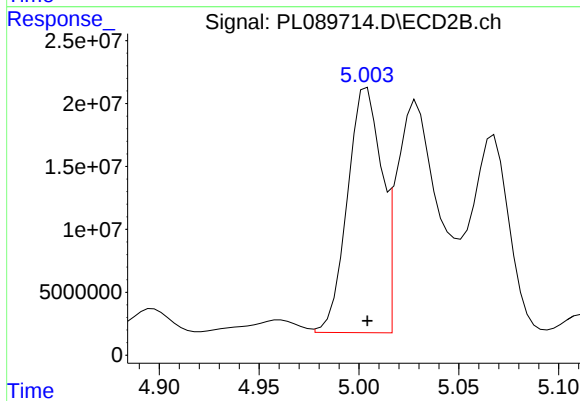

#25 Chlordane-3


R.T.: 5.004 min
Delta R.T.: 0.000 min
Response: 230125799
Conc: 1027.73 ng/ml

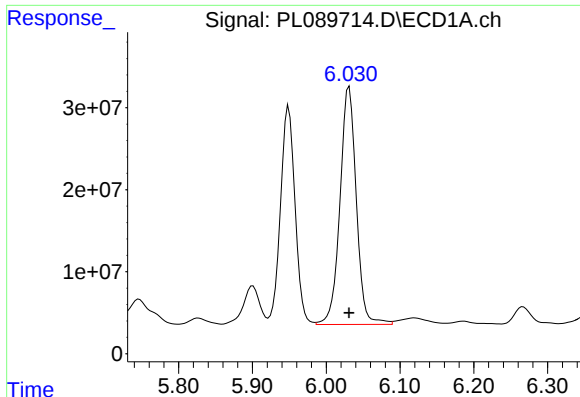

#26 Chlordane-4


R.T.: 6.031 min
Delta R.T.: 0.000 min
Response: 446287834
Conc: 988.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

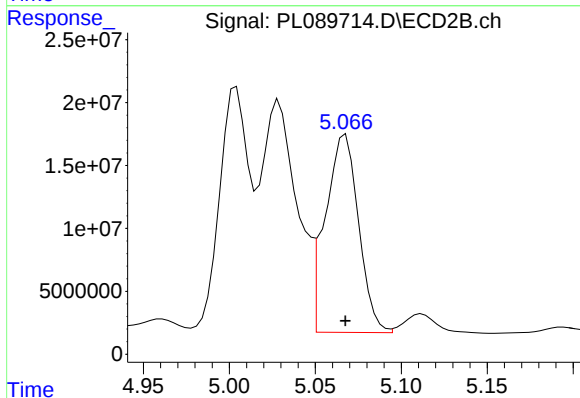


#26 Chlordane-4

R.T.: 5.068 min
Delta R.T.: 0.000 min
Response: 211949419
Conc: 1011.33 ng/ml

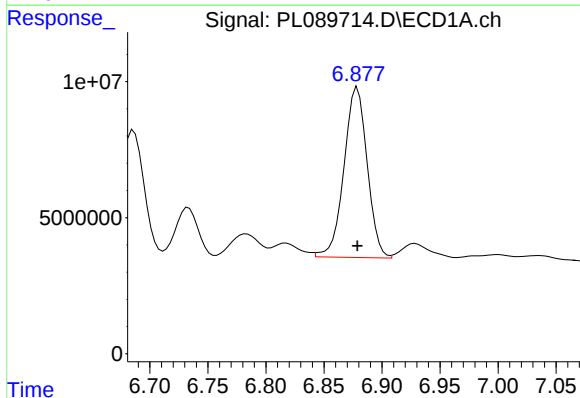


#27 Chlordane-5

R.T.: 6.879 min
Delta R.T.: 0.000 min
Response: 87097759
Conc: 970.10 ng/ml

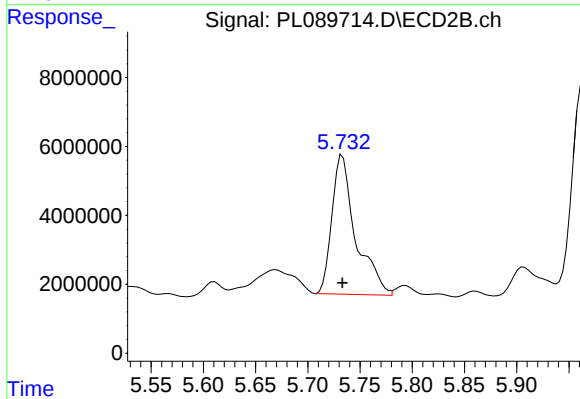

#27 Chlordane-5

R.T.: 5.733 min
Delta R.T.: 0.000 min
Response: 63984824
Conc: 1001.42 ng/ml

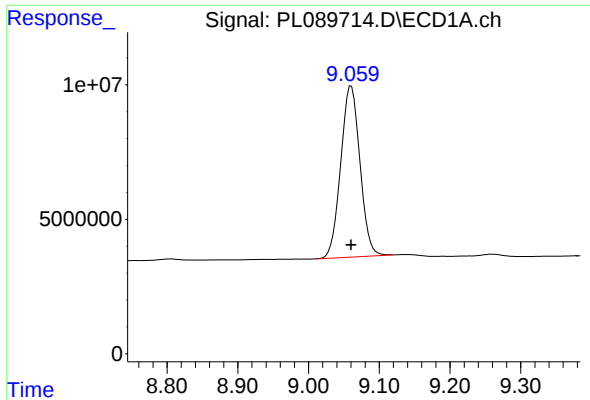

#28 Decachlorobiphenyl


R.T.: 9.060 min

Delta R.T.: 0.000 min

Response: 120195225

Conc: 96.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

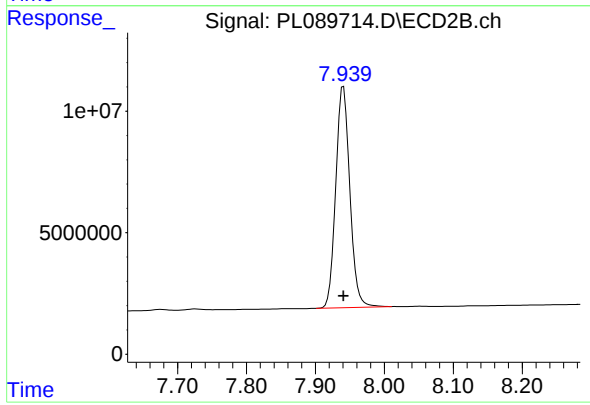

#28 Decachlorobiphenyl

R.T.: 7.941 min

Delta R.T.: 0.000 min

Response: 129355600

Conc: 99.05 ng/ml