

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052424\
 Data File : PL089715.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2024 12:23
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 14:31:40 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052424.M
 Quant Title : GC Extractables
 QLast Update : Fri May 24 14:27:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	2.793	123.8E6	115.9E6	73.746	74.345
28)	SA Decachlor...	9.061	7.941	90318803	96117553	73.473	74.059
Target Compounds							
23)	Chlordane-1	4.711	3.795	74280874	47316744	739.427	745.368
24)	Chlordane-2	5.239	4.373	79390322	55267966	739.159	744.076
25)	Chlordane-3	5.949	5.004	271.6E6	166.5E6	739.115	745.763
26)	Chlordane-4	6.031	5.067	330.7E6	154.7E6	738.411	742.094
27)	Chlordane-5	6.879	5.733	65557837	47251237	736.673	742.982



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052424\
Data File : PL089715.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2024 12:23
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 14:31:40 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052424.M
Quant Title : GC Extractables
QLast Update : Fri May 24 14:27:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

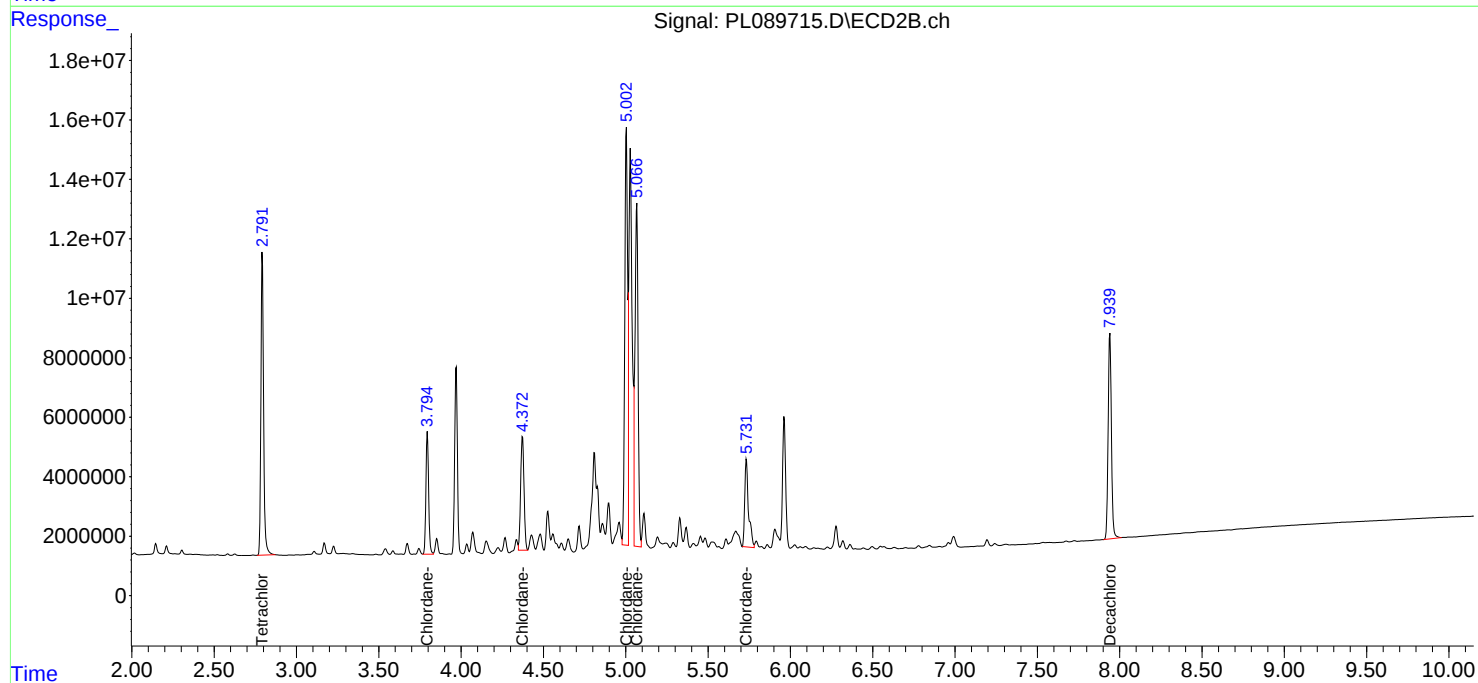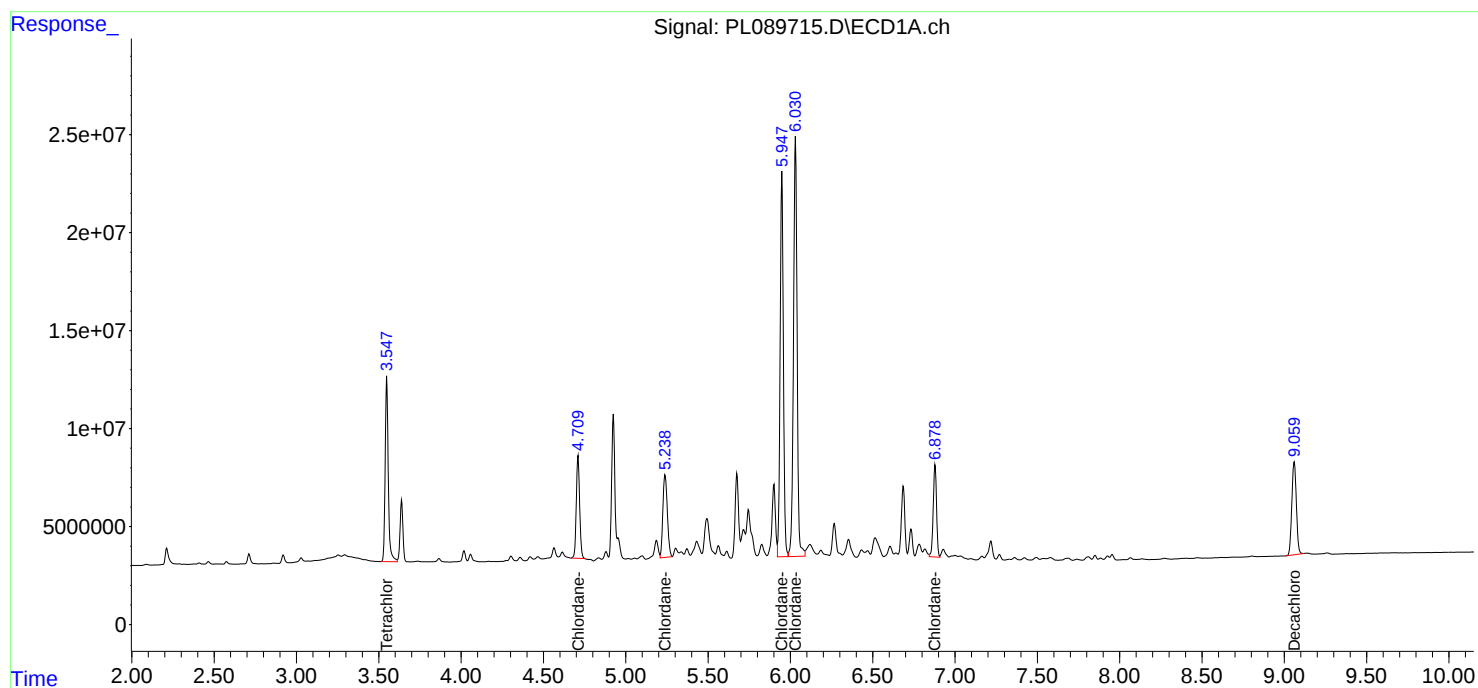


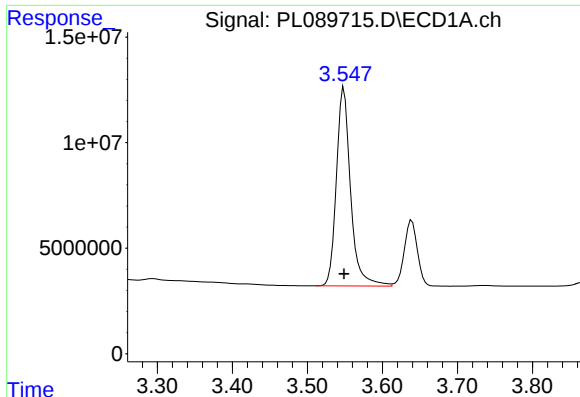

#1 Tetrachloro-m-xylene


R.T.: 3.549 min
Delta R.T.: 0.000 min
Response: 123835834
Conc: 73.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

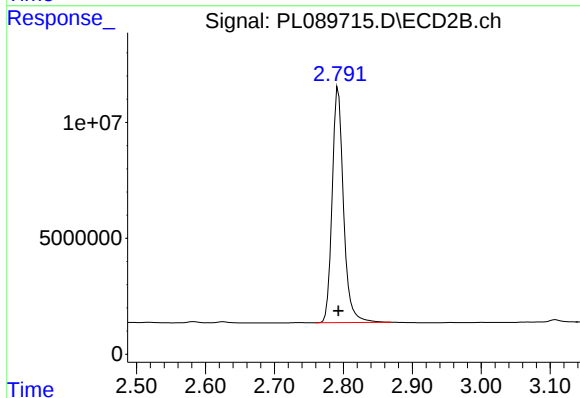


#1 Tetrachloro-m-xylene

R.T.: 2.793 min
Delta R.T.: 0.000 min
Response: 115896675
Conc: 74.35 ng/ml

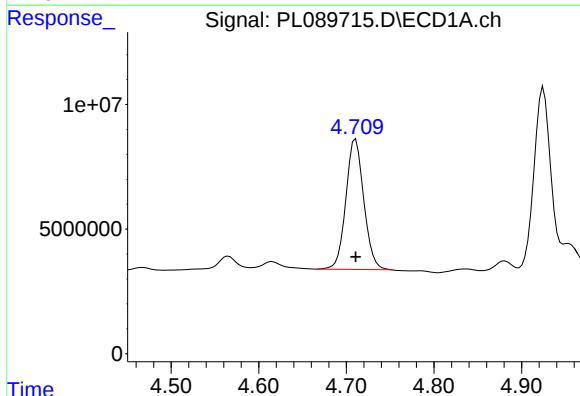


#23 Chlordane-1

R.T.: 4.711 min
Delta R.T.: 0.000 min
Response: 74280874
Conc: 739.43 ng/ml

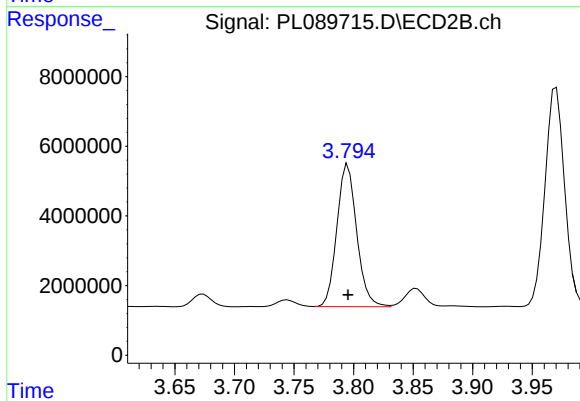

#23 Chlordane-1


R.T.: 3.795 min
Delta R.T.: 0.000 min
Response: 47316744
Conc: 745.37 ng/ml

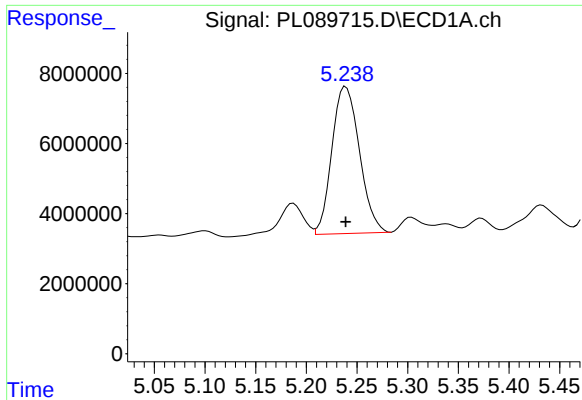

#24 Chlordane-2


R.T.: 5.239 min
Delta R.T.: 0.000 min
Response: 79390322
Conc: 739.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

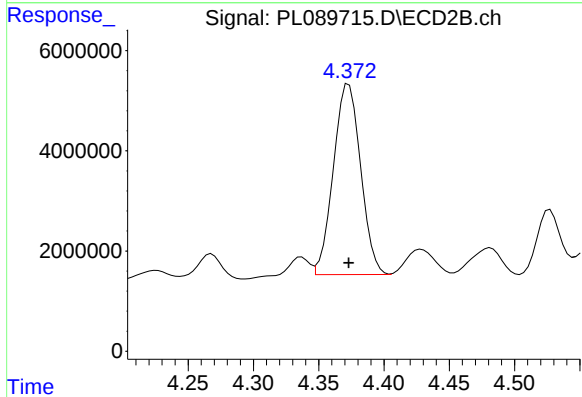


#24 Chlordane-2

R.T.: 4.373 min
Delta R.T.: 0.000 min
Response: 55267966
Conc: 744.08 ng/ml

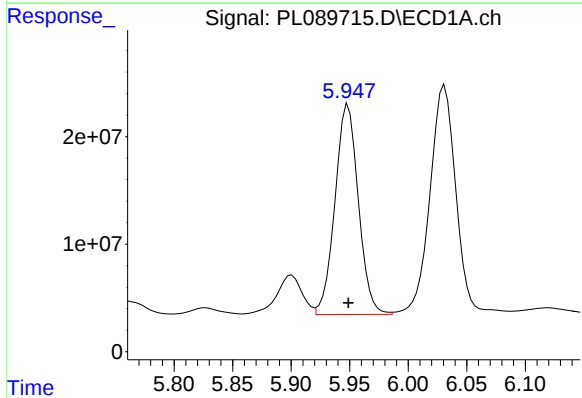


#25 Chlordane-3

R.T.: 5.949 min
Delta R.T.: 0.000 min
Response: 271602893
Conc: 739.11 ng/ml

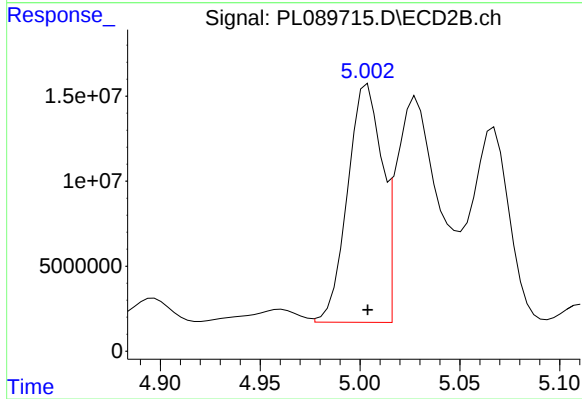

#25 Chlordane-3


R.T.: 5.004 min
Delta R.T.: 0.000 min
Response: 166517688
Conc: 745.76 ng/ml

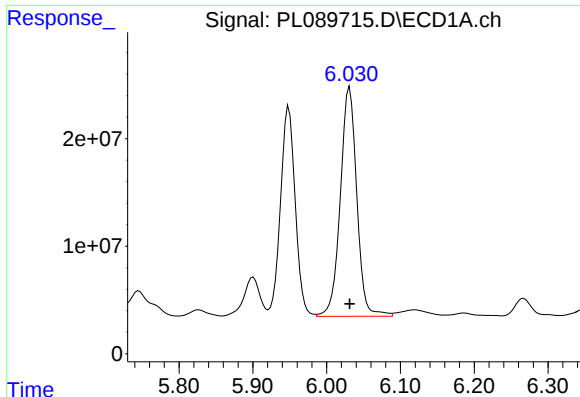

#26 Chlordane-4


R.T.: 6.031 min
Delta R.T.: 0.000 min
Response: 330675711
Conc: 738.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

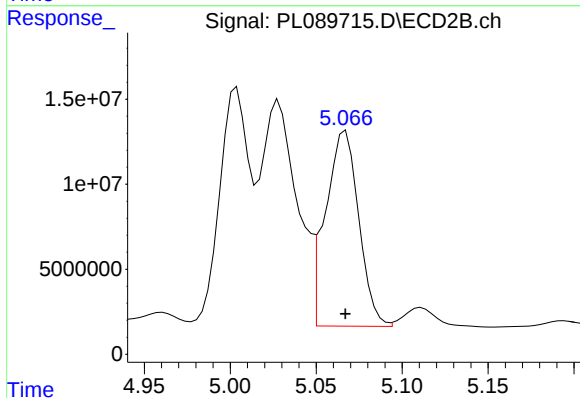


#26 Chlordane-4

R.T.: 5.067 min
Delta R.T.: 0.000 min
Response: 154709300
Conc: 742.09 ng/ml

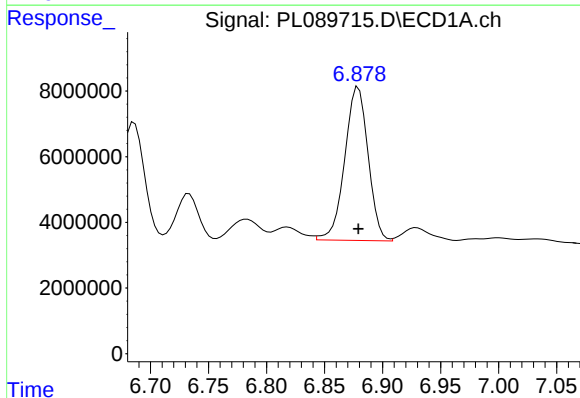


#27 Chlordane-5

R.T.: 6.879 min
Delta R.T.: 0.000 min
Response: 65557837
Conc: 736.67 ng/ml

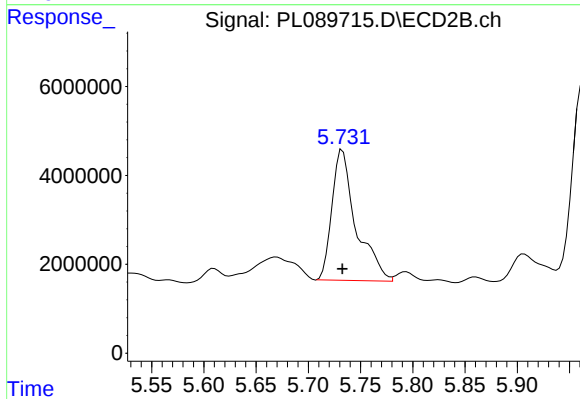

#27 Chlordane-5


R.T.: 5.733 min
Delta R.T.: 0.000 min
Response: 47251237
Conc: 742.98 ng/ml

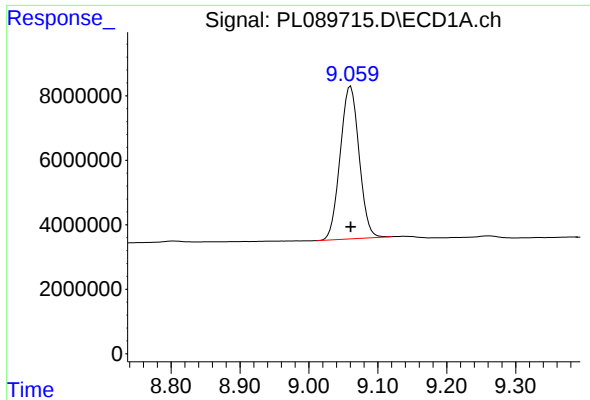

#28 Decachlorobiphenyl

R.T.: 9.061 min
Delta R.T.: 0.000 min
Response: 90318803
Conc: 73.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

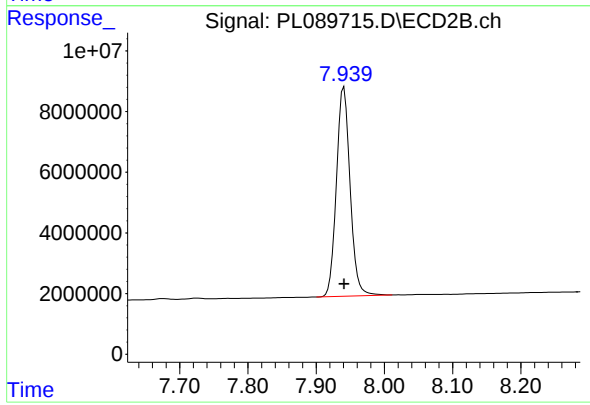

#28 Decachlorobiphenyl

R.T.: 7.941 min
Delta R.T.: 0.000 min
Response: 96117553
Conc: 74.06 ng/ml