

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052424\
 Data File : PL089716.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2024 12:37
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 14:27:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052424.M
 Quant Title : GC Extractables
 QLast Update : Fri May 24 14:27:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.792	86454027	77352010	50.000	50.000
28)	SA Decachlor...	9.061	7.941	64080623	65922451	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.710	3.795	52021012	31520328	500.000	500.000
24)	Chlordane-2	5.239	4.373	56316039	37820788	500.000	500.000
25)	Chlordane-3	5.949	5.004	186.7E6	108.9E6	500.000	500.000
26)	Chlordane-4	6.031	5.067	228.1E6	103.6E6	500.000	500.000
27)	Chlordane-5	6.879	5.733	46233609	31901930	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052424\
Data File : PL089716.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2024 12:37
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 14:27:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052424.M
Quant Title : GC Extractables
QLast Update : Fri May 24 14:27:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

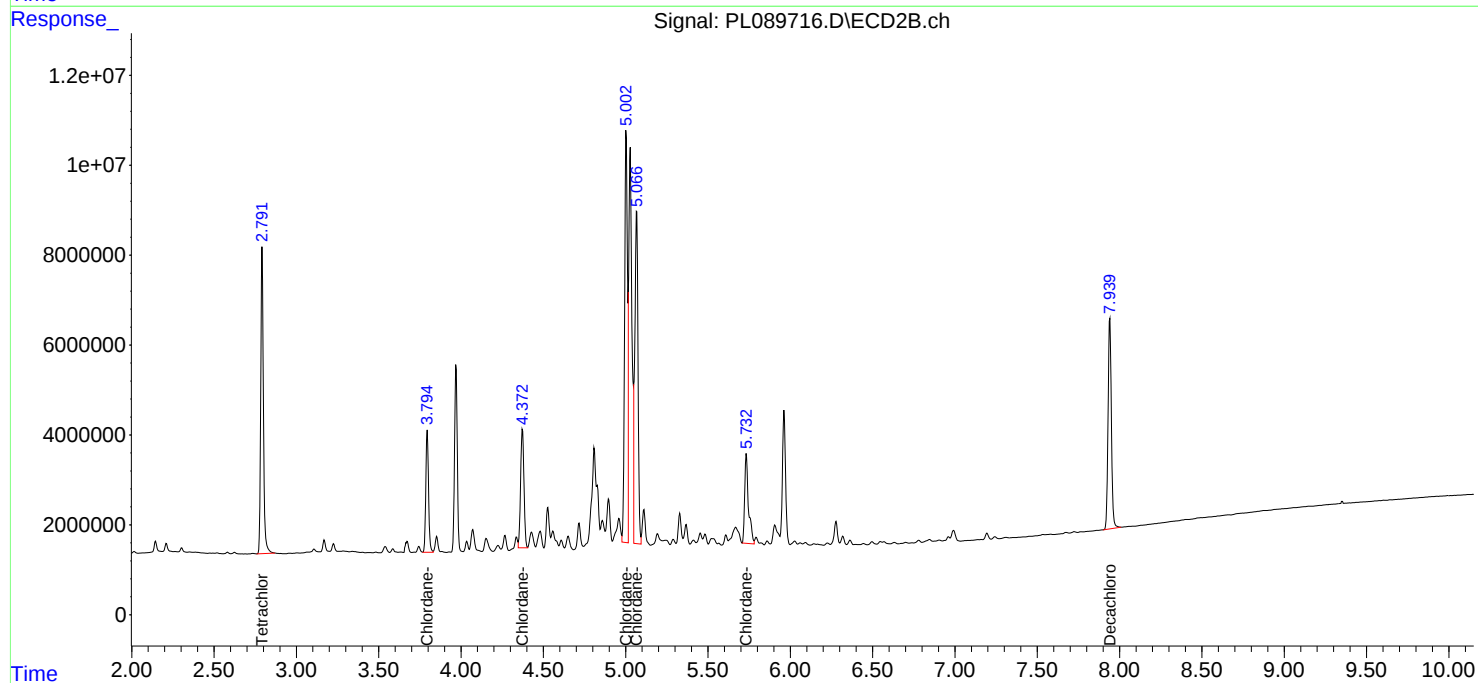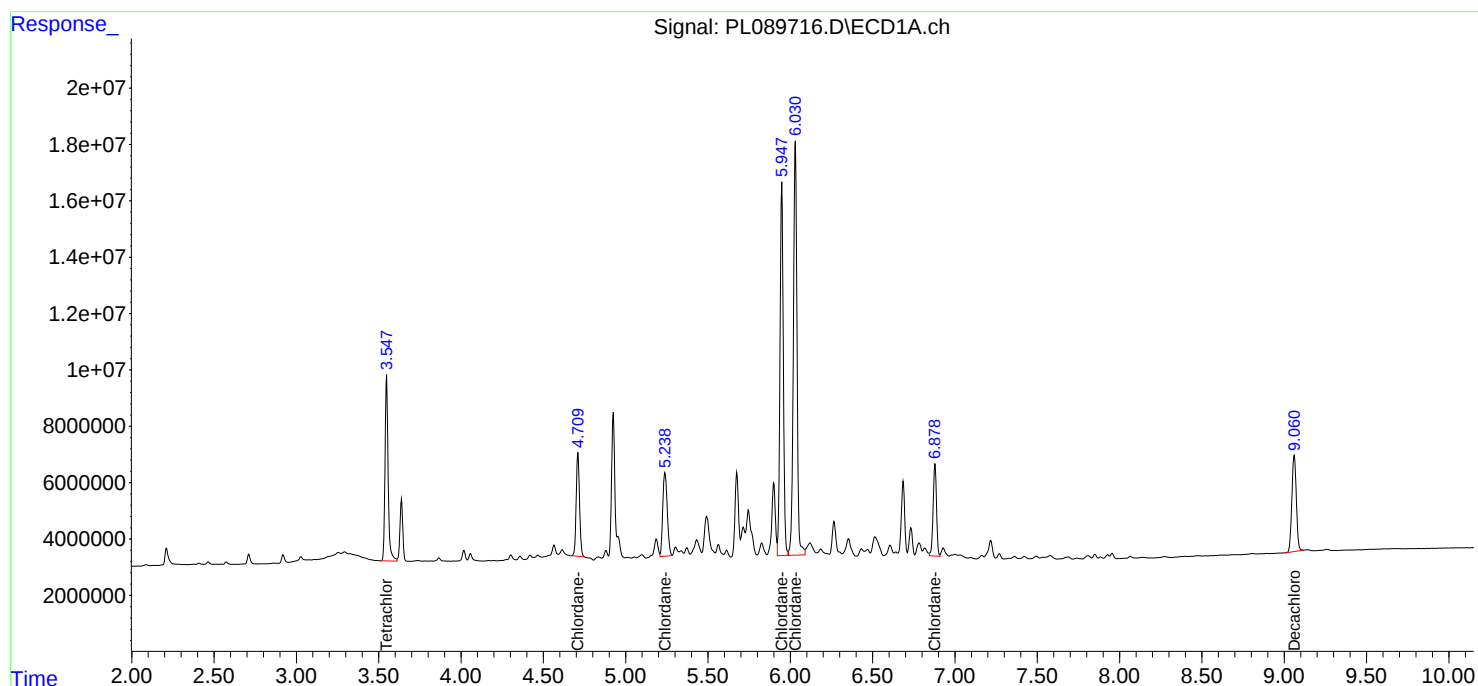


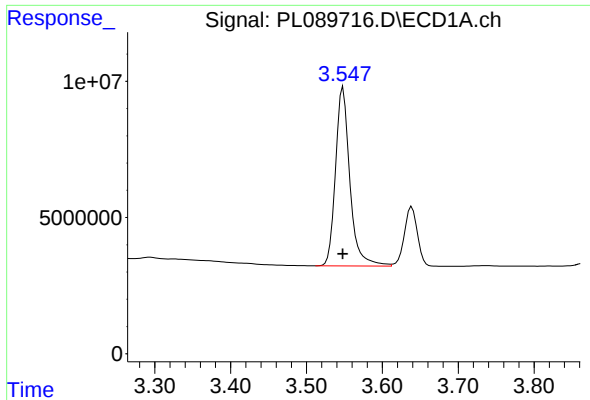

#1 Tetrachloro-m-xylene


R.T.: 3.548 min
Delta R.T.: 0.000 min
Response: 86454027
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

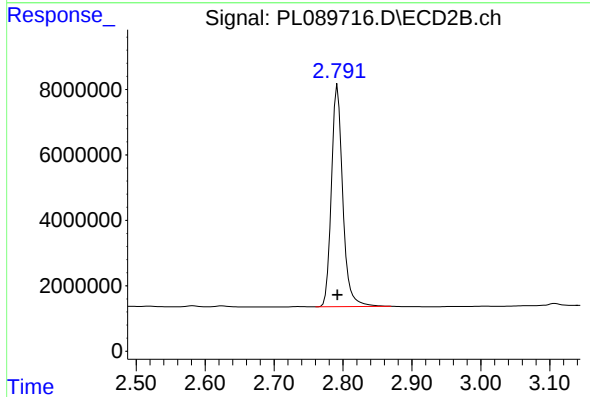


#1 Tetrachloro-m-xylene

R.T.: 2.792 min
Delta R.T.: 0.000 min
Response: 77352010
Conc: 50.00 ng/ml

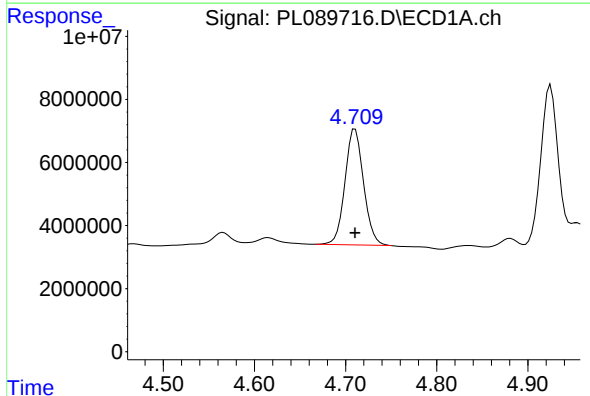


#23 Chlordane-1

R.T.: 4.710 min
Delta R.T.: 0.000 min
Response: 52021012
Conc: 500.00 ng/ml

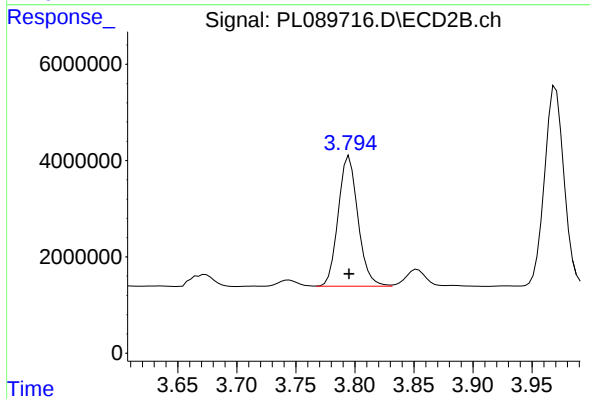

#23 Chlordane-1


R.T.: 3.795 min
Delta R.T.: 0.000 min
Response: 31520328
Conc: 500.00 ng/ml

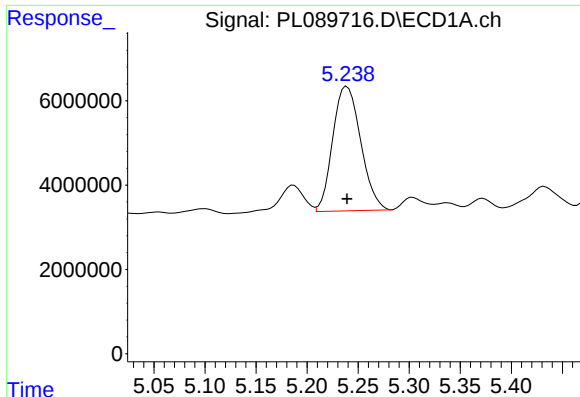

#24 Chlordane-2


R.T.: 5.239 min
Delta R.T.: 0.000 min
Response: 56316039
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

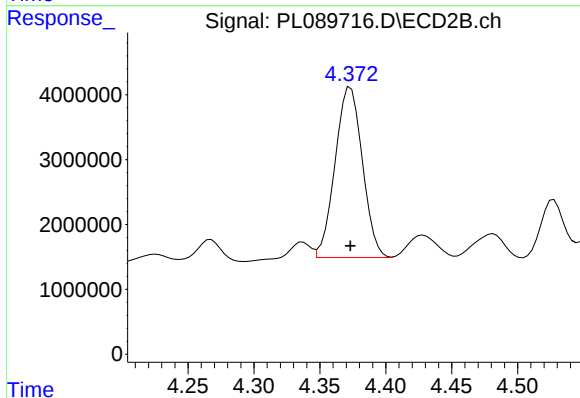


#24 Chlordane-2

R.T.: 4.373 min
Delta R.T.: 0.000 min
Response: 37820788
Conc: 500.00 ng/ml

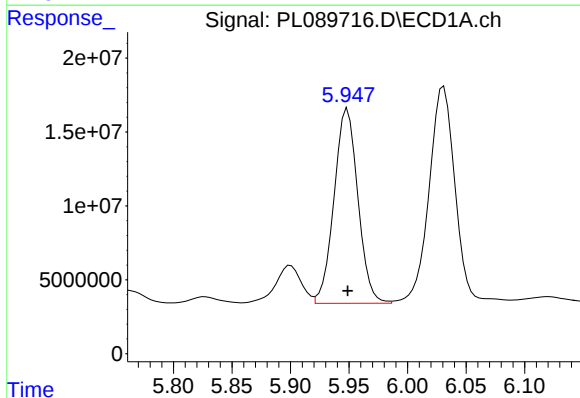


#25 Chlordane-3

R.T.: 5.949 min
Delta R.T.: 0.000 min
Response: 186708670
Conc: 500.00 ng/ml

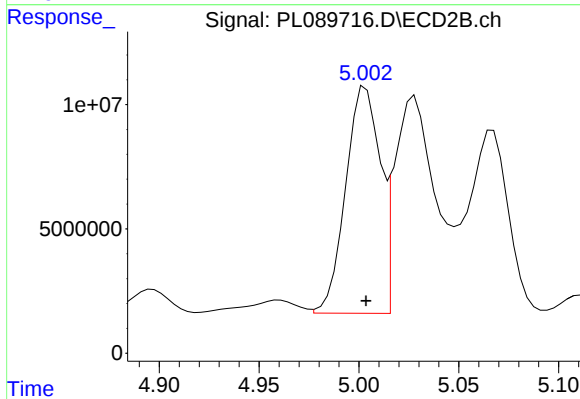

#25 Chlordane-3


R.T.: 5.004 min
Delta R.T.: 0.000 min
Response: 108852777
Conc: 500.00 ng/ml

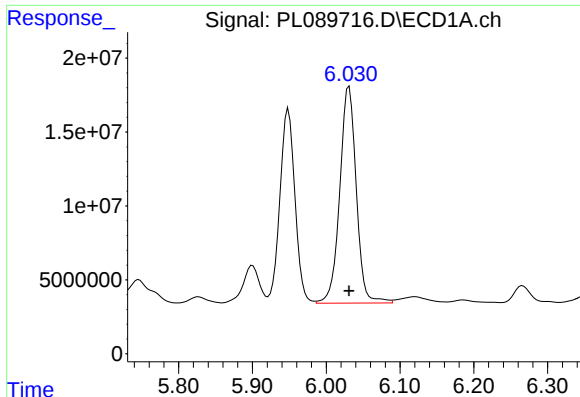

#26 Chlordane-4


R.T.: 6.031 min
Delta R.T.: 0.000 min
Response: 228136988
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

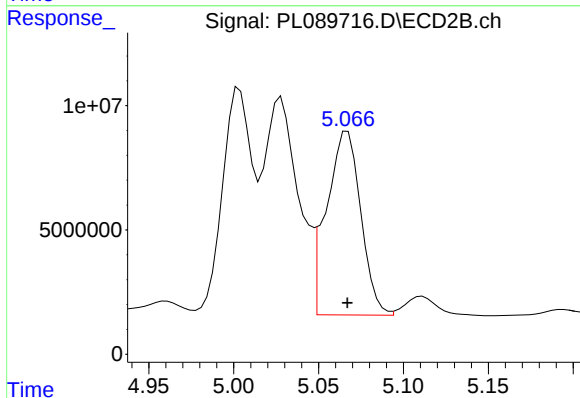


#26 Chlordane-4

R.T.: 5.067 min
Delta R.T.: 0.000 min
Response: 103600981
Conc: 500.00 ng/ml

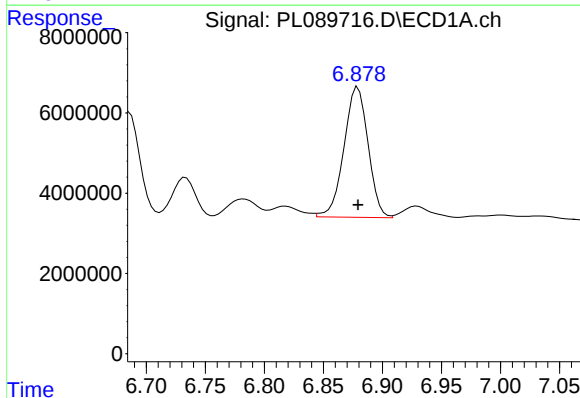


#27 Chlordane-5

R.T.: 6.879 min
Delta R.T.: 0.000 min
Response: 46233609
Conc: 500.00 ng/ml

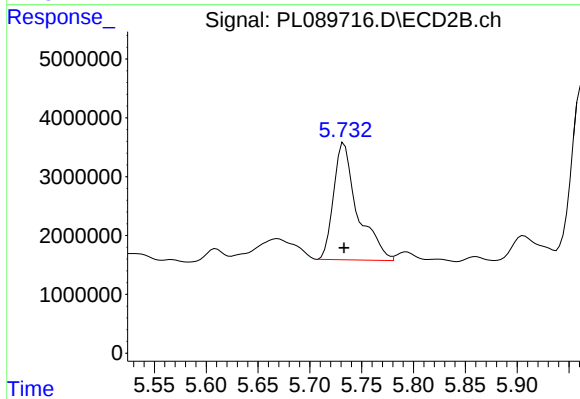

#27 Chlordane-5


R.T.: 5.733 min
Delta R.T.: 0.000 min
Response: 31901930
Conc: 500.00 ng/ml

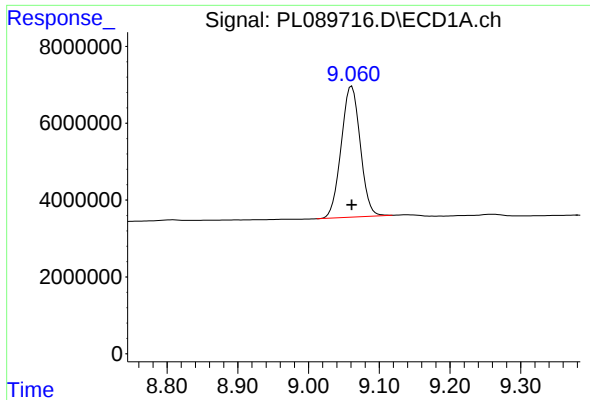

#28 Decachlorobiphenyl

R.T.: 9.061 min
Delta R.T.: 0.000 min
Response: 64080623
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

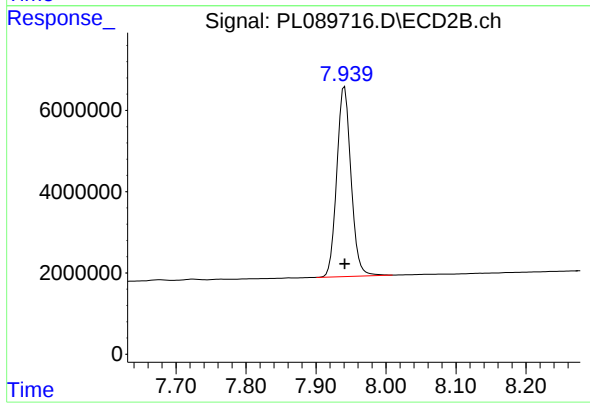

#28 Decachlorobiphenyl

R.T.: 7.941 min
Delta R.T.: 0.000 min
Response: 65922451
Conc: 50.00 ng/ml