

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052424\
 Data File : PL089717.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2024 12:51
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 14:33:37 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052424.M
 Quant Title : GC Extractables
 QLast Update : Fri May 24 14:27:16 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.792	46260217	38566100	26.864	24.804
28)	SA Decachlor...	9.062	7.941	35011373	34455515	27.523	26.143
Target Compounds							
23)	Chlordane-1	4.710	3.795	27660906	16111478	268.542	252.839
24)	Chlordane-2	5.239	4.373	30908490	20012540	277.298	264.295
25)	Chlordane-3	5.948	5.004	98800398	53019973	263.888	240.471
26)	Chlordane-4	6.031	5.067	121.1E6	50538633	265.080	244.270
27)	Chlordane-5	6.879	5.733	25022823	16698401	272.679	259.308



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052424\
Data File : PL089717.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2024 12:51
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 14:33:37 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052424.M
Quant Title : GC Extractables
QLast Update : Fri May 24 14:27:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

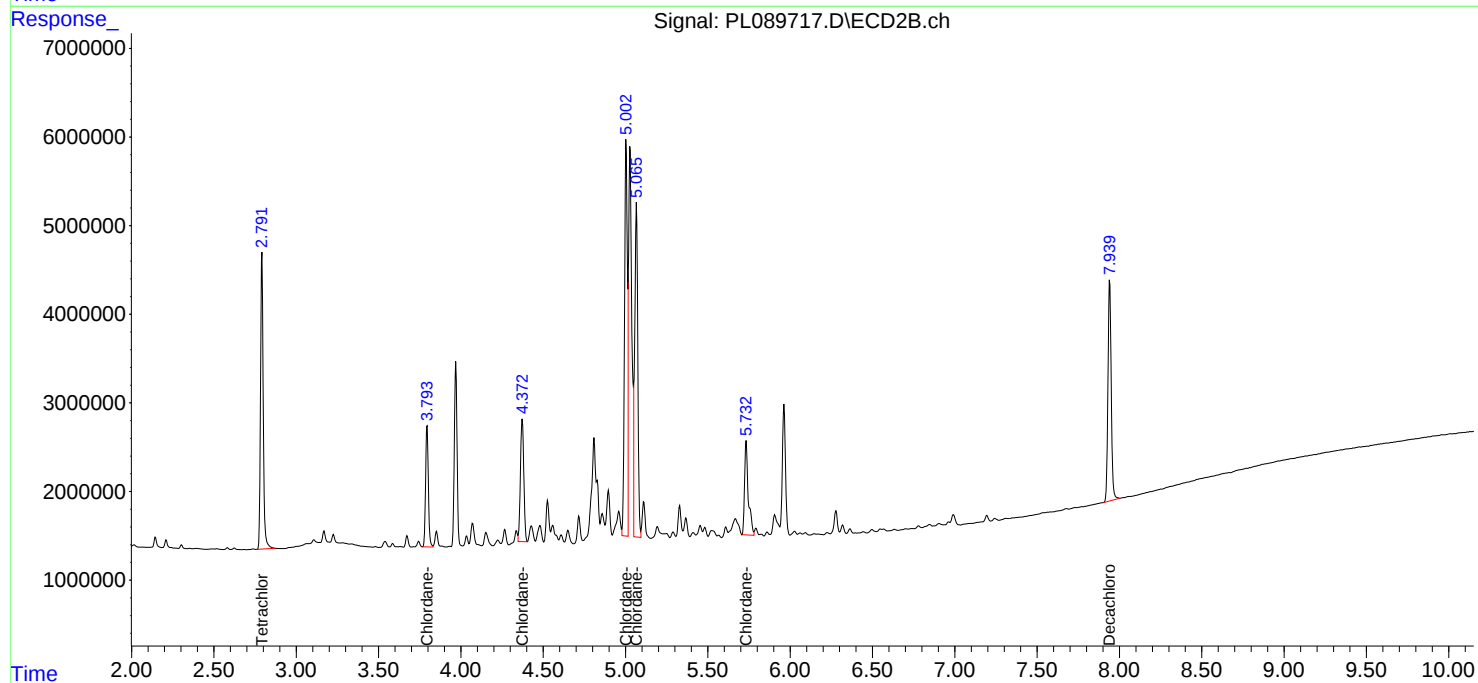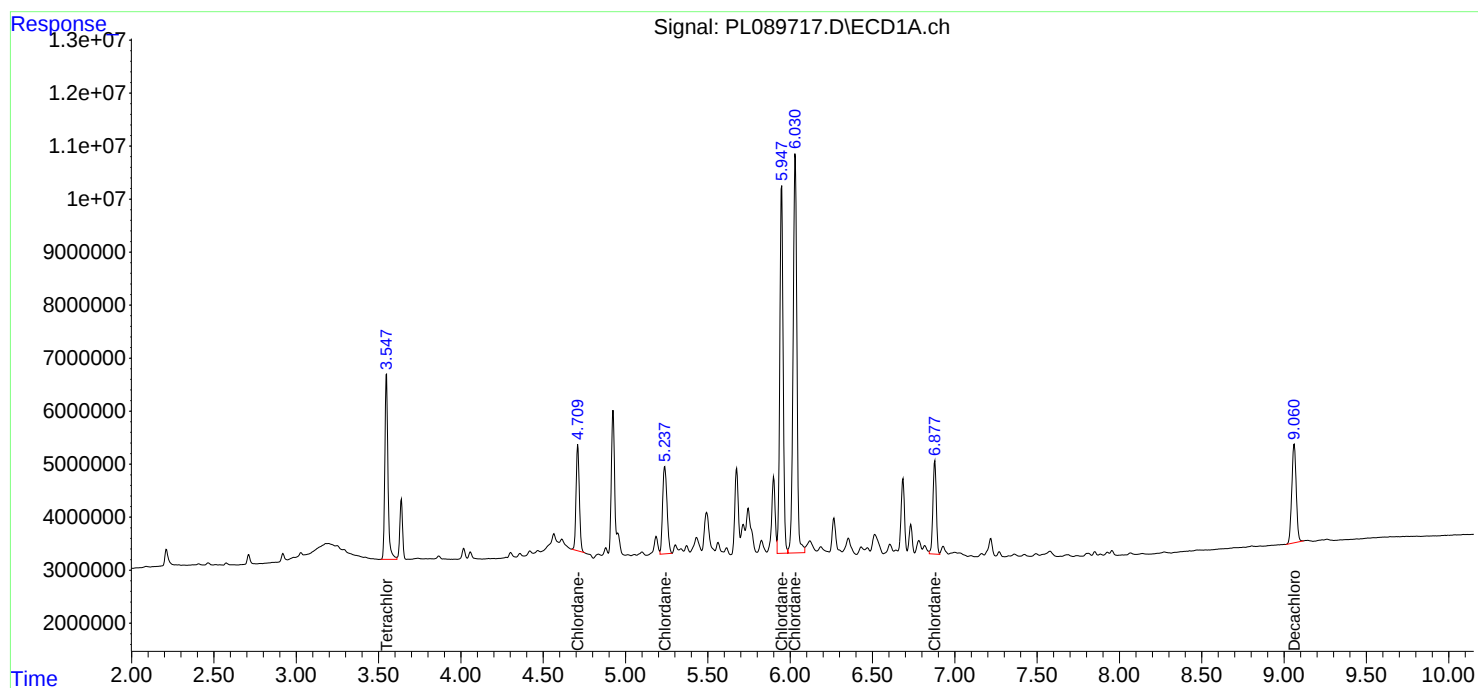


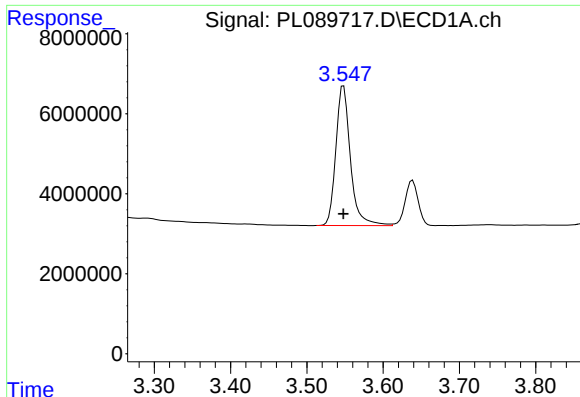

#1 Tetrachloro-m-xylene


R.T.: 3.548 min
Delta R.T.: 0.000 min
Response: 46260217
Conc: 26.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

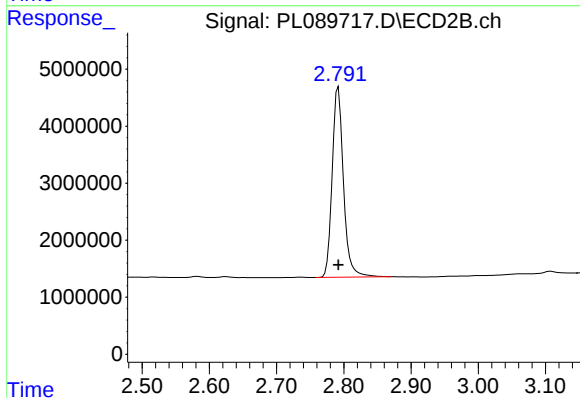


#1 Tetrachloro-m-xylene

R.T.: 2.792 min
Delta R.T.: 0.000 min
Response: 38566100
Conc: 24.80 ng/ml

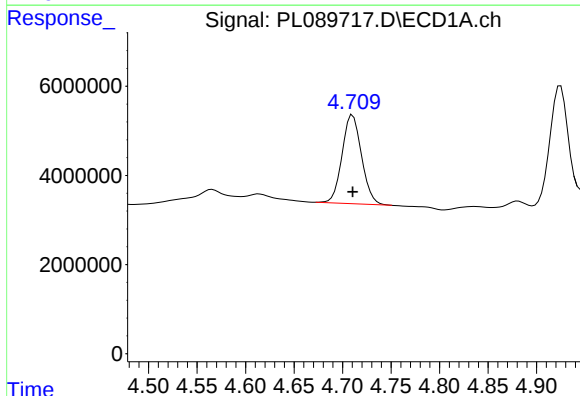


#23 Chlordane-1

R.T.: 4.710 min
Delta R.T.: 0.000 min
Response: 27660906
Conc: 268.54 ng/ml

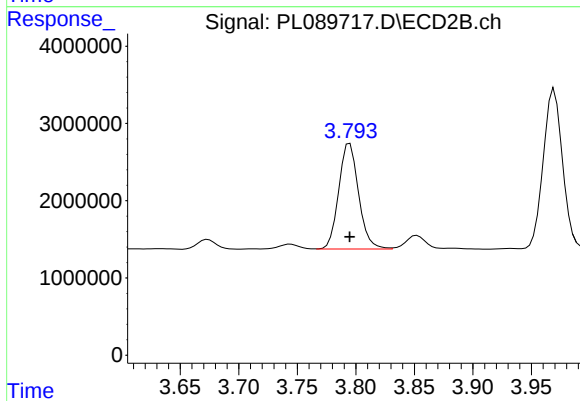

#23 Chlordane-1


R.T.: 3.795 min
Delta R.T.: 0.000 min
Response: 16111478
Conc: 252.84 ng/ml

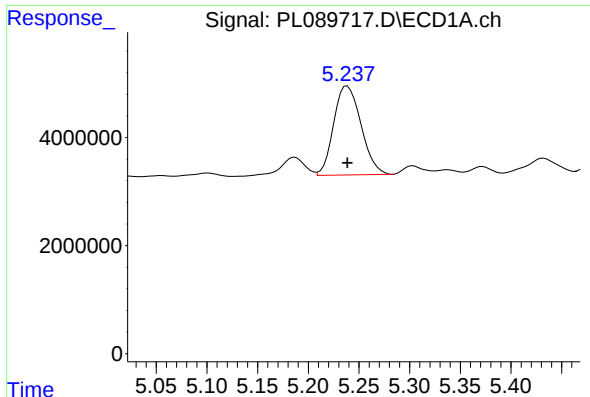

#24 Chlordane-2


R.T.: 5.239 min
Delta R.T.: 0.000 min
Response: 30908490
Conc: 277.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

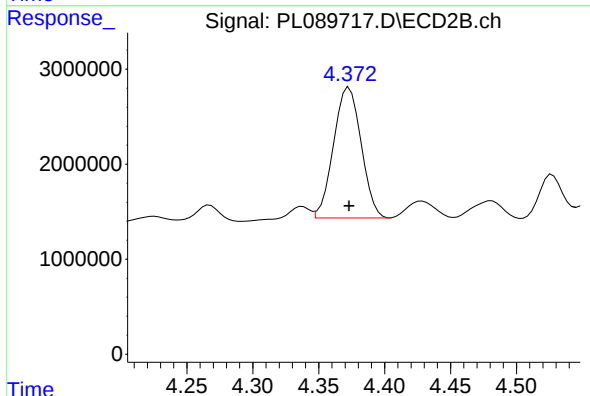


#24 Chlordane-2

R.T.: 4.373 min
Delta R.T.: 0.000 min
Response: 20012540
Conc: 264.29 ng/ml

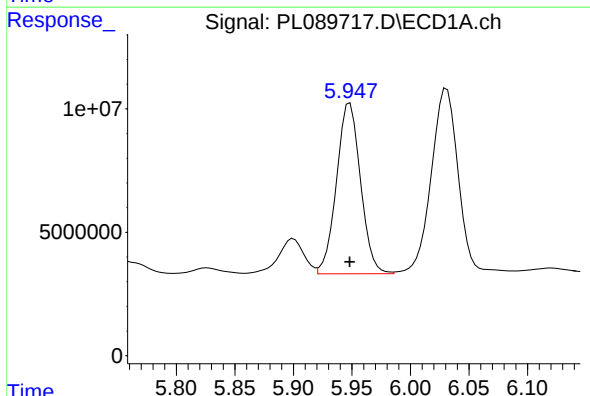


#25 Chlordane-3

R.T.: 5.948 min
Delta R.T.: 0.000 min
Response: 98800398
Conc: 263.89 ng/ml

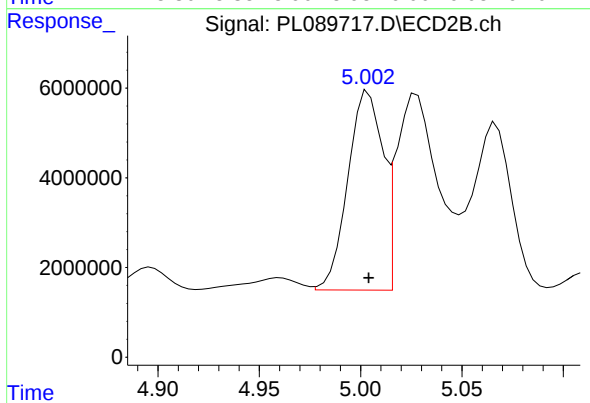

#25 Chlordane-3


R.T.: 5.004 min
Delta R.T.: 0.000 min
Response: 53019973
Conc: 240.47 ng/ml

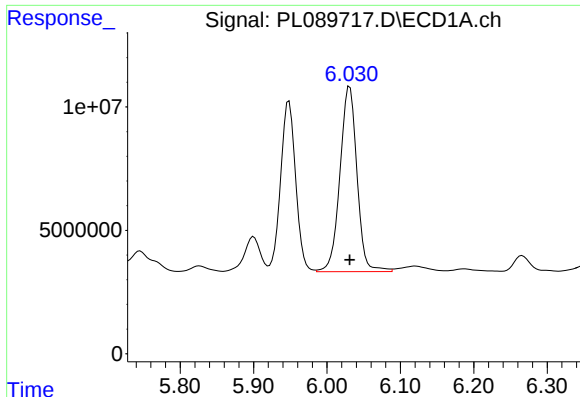

#26 Chlordane-4


R.T.: 6.031 min
Delta R.T.: 0.000 min
Response: 121143865
Conc: 265.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

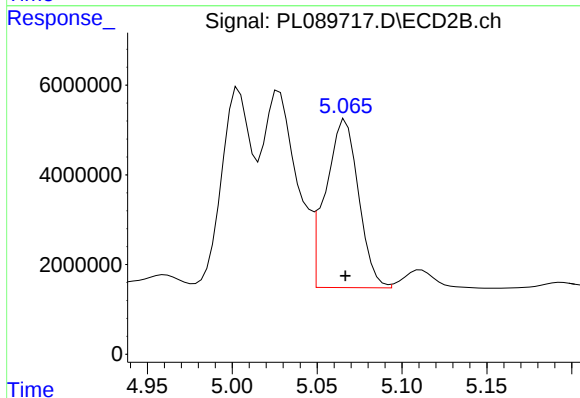


#26 Chlordane-4

R.T.: 5.067 min
Delta R.T.: 0.000 min
Response: 50538633
Conc: 244.27 ng/ml

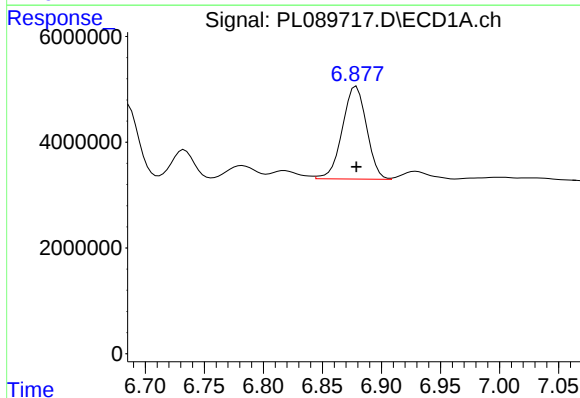


#27 Chlordane-5

R.T.: 6.879 min
Delta R.T.: 0.000 min
Response: 25022823
Conc: 272.68 ng/ml

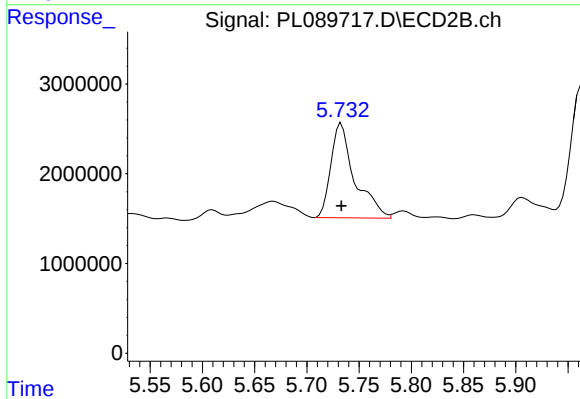

#27 Chlordane-5


R.T.: 5.733 min
Delta R.T.: 0.000 min
Response: 16698401
Conc: 259.31 ng/ml

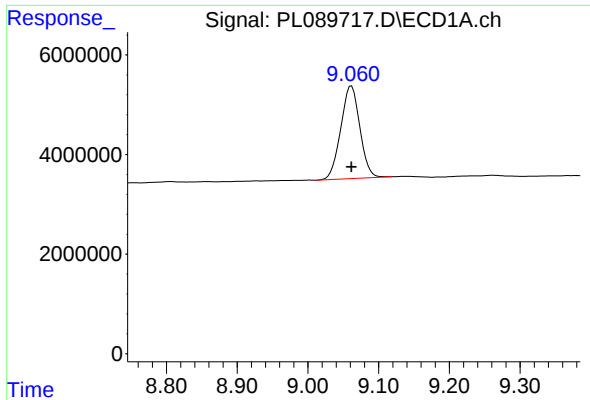

#28 Decachlorobiphenyl

R.T.: 9.062 min
Delta R.T.: 0.000 min
Response: 35011373
Conc: 27.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

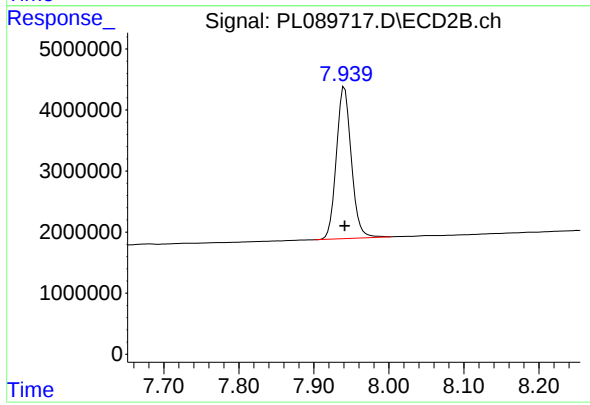

#28 Decachlorobiphenyl

R.T.: 7.941 min
Delta R.T.: 0.000 min
Response: 34455515
Conc: 26.14 ng/ml