

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052424\
 Data File : PL089725.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2024 14:40
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL052424

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 14:54:39 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052424.M
 Quant Title : GC Extractables
 QLast Update : Fri May 24 14:54:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	2.794	82806199	75084613	45.153	47.415
28)	SA Decachlor...	9.063	7.943	61811411	64780904	45.768	47.317
Target Compounds							
23)	Chlordane-1	4.713	3.797	50567730	30882452	466.314	470.893
24)	Chlordane-2	5.242	4.375	54440905	37457495	453.319	469.554
25)	Chlordane-3	5.951	5.006	180.3E6	107.2E6	450.660	481.675
26)	Chlordane-4	6.033	5.069	220.9E6	99272069	451.775	469.510
27)	Chlordane-5	6.881	5.735	44676665	31132134	459.780	458.561



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052424\
Data File : PL089725.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2024 14:40
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL052424

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 14:54:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052424.M
Quant Title : GC Extractables
QLast Update : Fri May 24 14:54:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

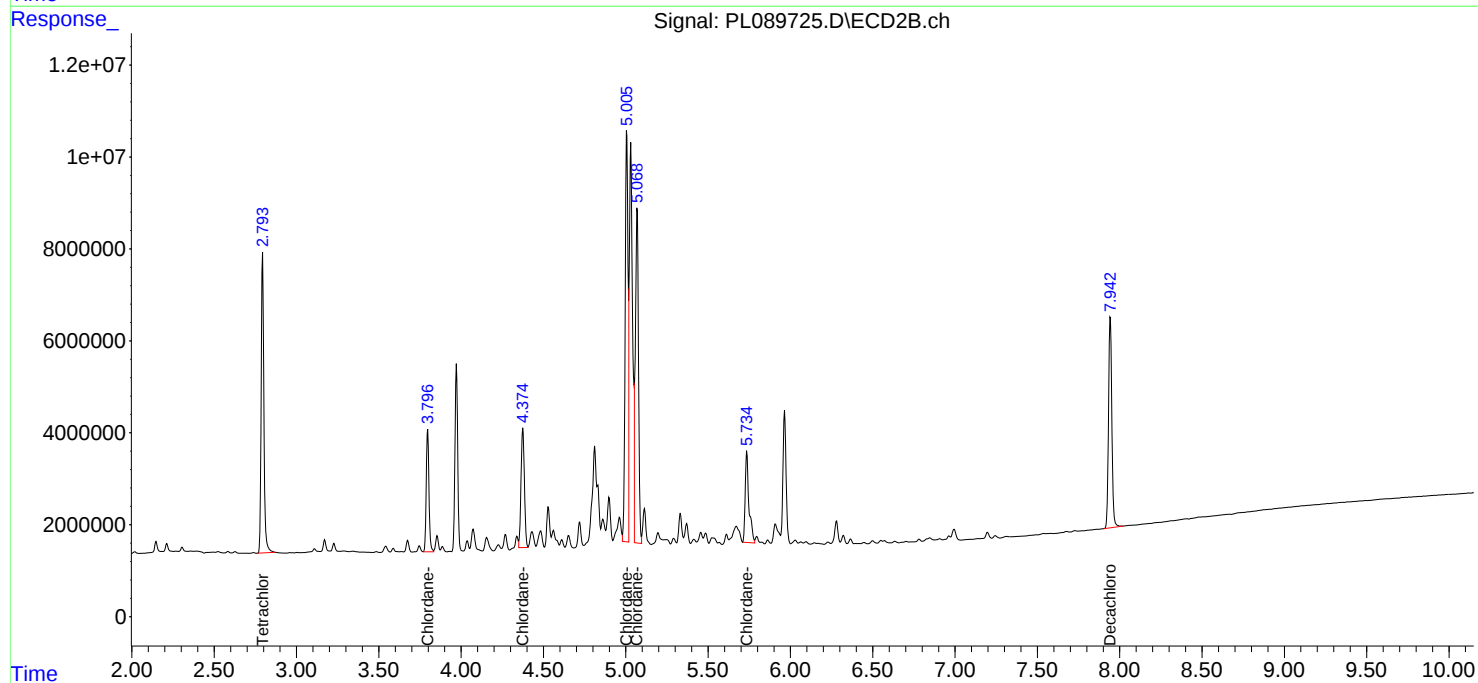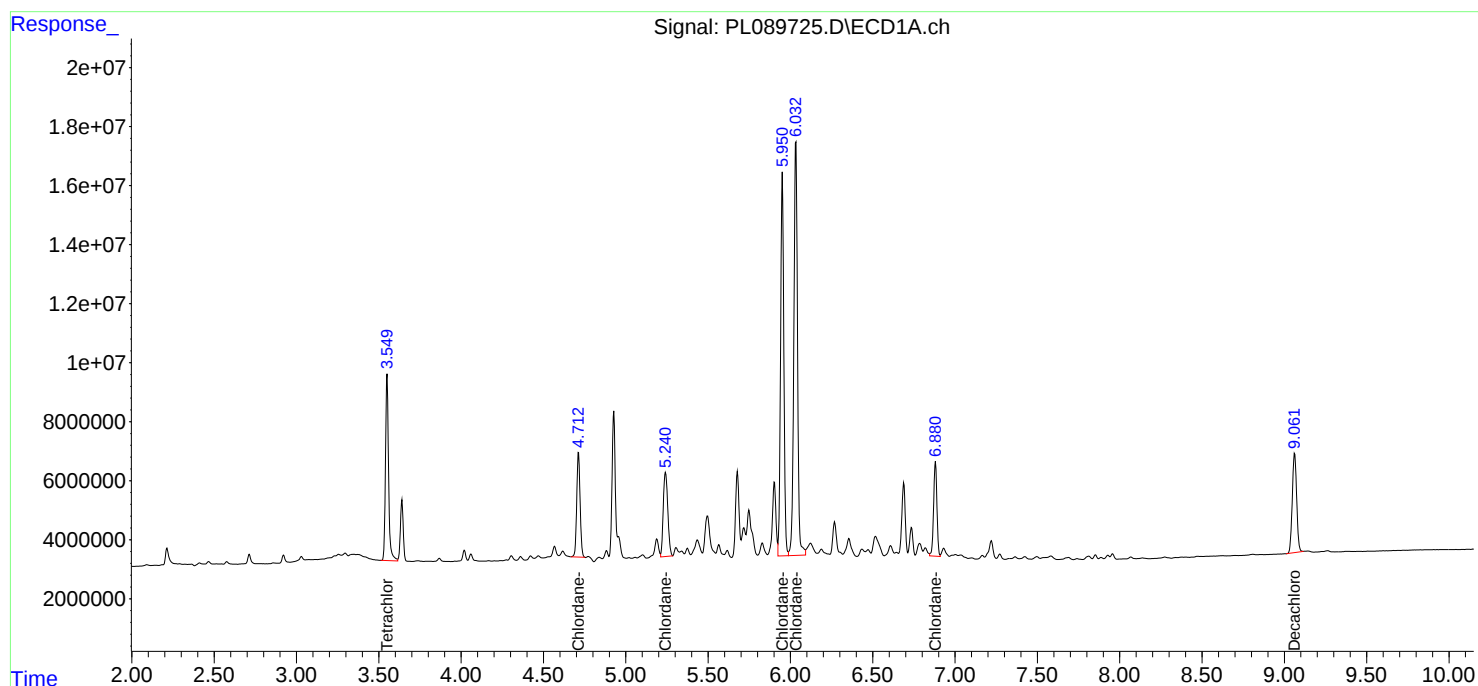


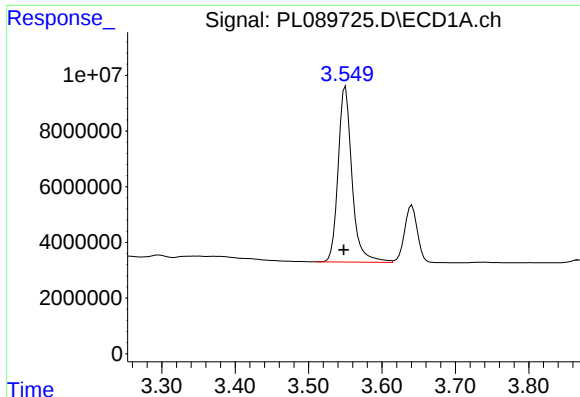

#1 Tetrachloro-m-xylene


R.T.: 3.550 min
Delta R.T.: 0.002 min
Response: 82806199
Conc: 45.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL052424

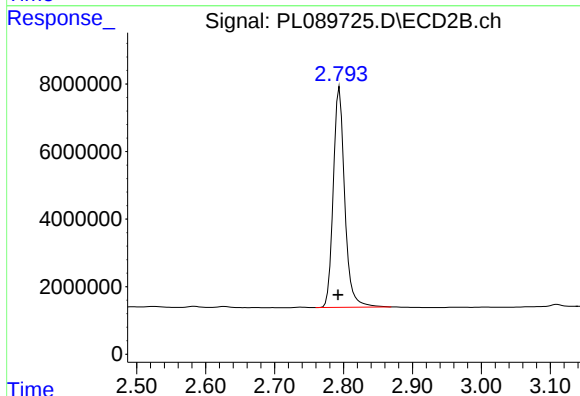


#1 Tetrachloro-m-xylene

R.T.: 2.794 min
Delta R.T.: 0.002 min
Response: 75084613
Conc: 47.42 ng/ml

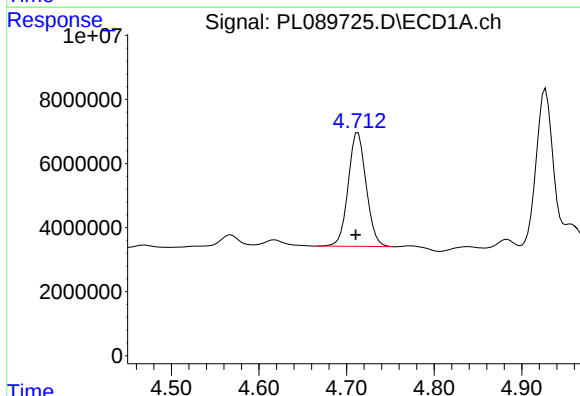


#23 Chlordane-1

R.T.: 4.713 min
Delta R.T.: 0.003 min
Response: 50567730
Conc: 466.31 ng/ml

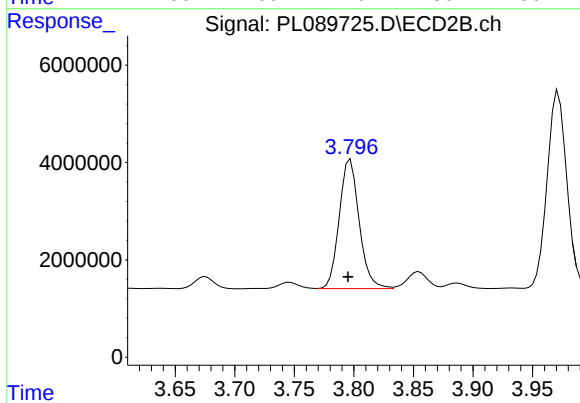

#23 Chlordane-1


R.T.: 3.797 min
Delta R.T.: 0.002 min
Response: 30882452
Conc: 470.89 ng/ml

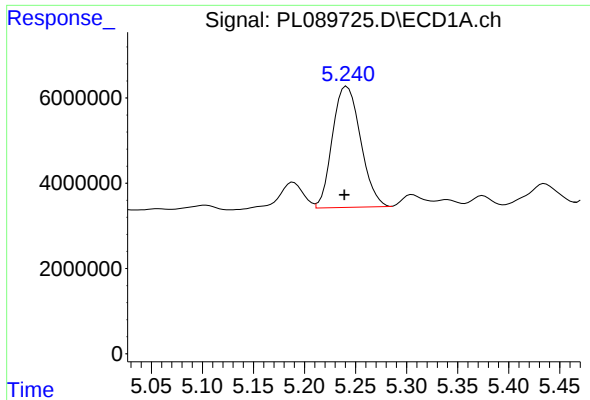

#24 Chlordane-2


R.T.: 5.242 min
Delta R.T.: 0.002 min
Response: 54440905
Conc: 453.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL052424

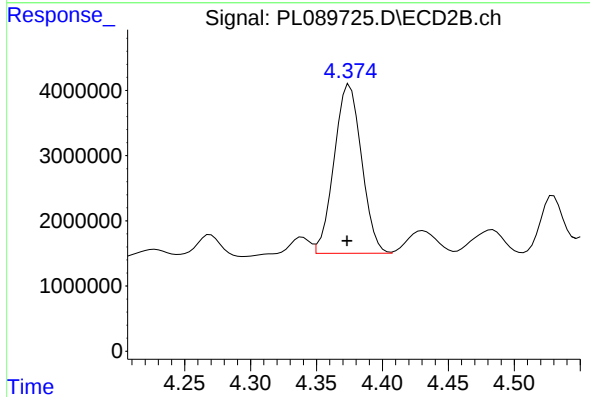


#24 Chlordane-2

R.T.: 4.375 min
Delta R.T.: 0.002 min
Response: 37457495
Conc: 469.55 ng/ml

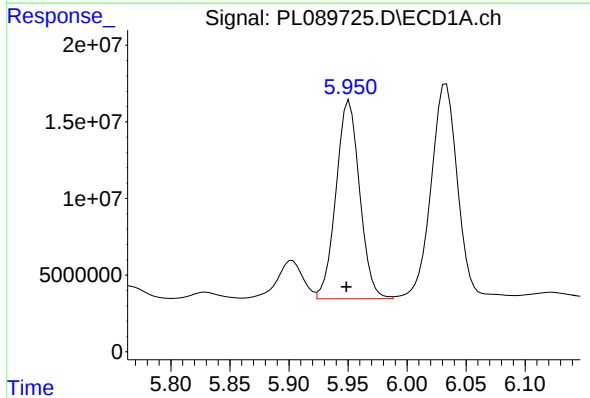


#25 Chlordane-3

R.T.: 5.951 min
Delta R.T.: 0.002 min
Response: 180331123
Conc: 450.66 ng/ml

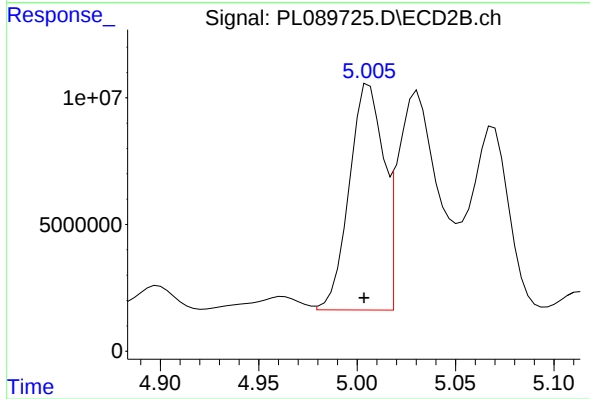

#25 Chlordane-3


R.T.: 5.006 min
Delta R.T.: 0.003 min
Response: 107216480
Conc: 481.68 ng/ml

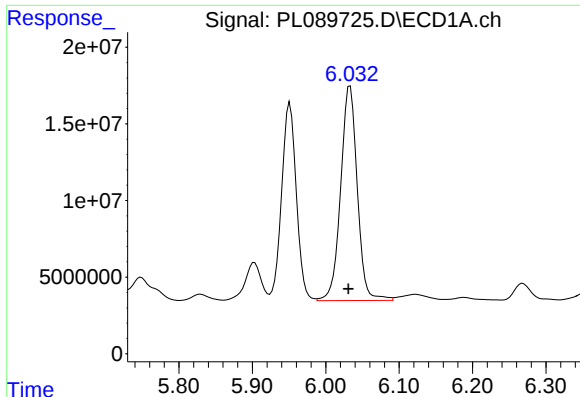

#26 Chlordane-4


R.T.: 6.033 min
Delta R.T.: 0.002 min
Response: 220864405
Conc: 451.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL052424

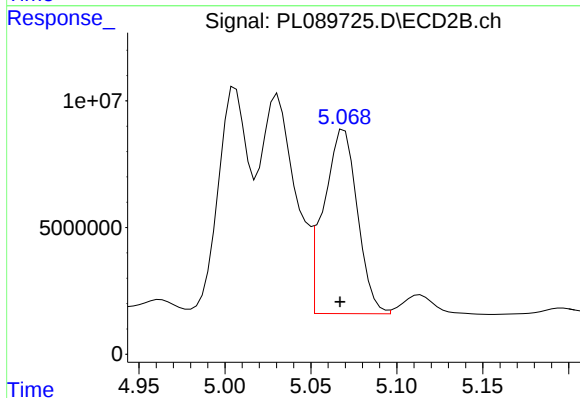


#26 Chlordane-4

R.T.: 5.069 min
Delta R.T.: 0.002 min
Response: 99272069
Conc: 469.51 ng/ml

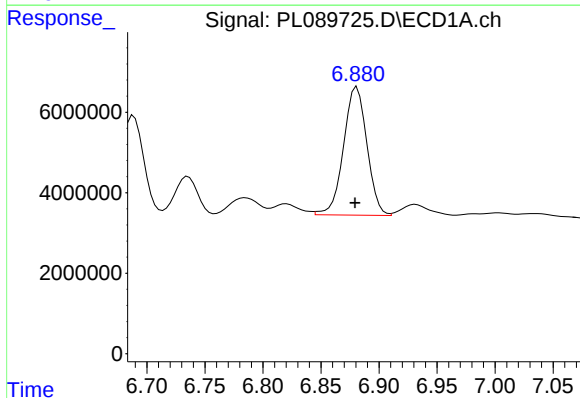


#27 Chlordane-5

R.T.: 6.881 min
Delta R.T.: 0.002 min
Response: 44676665
Conc: 459.78 ng/ml

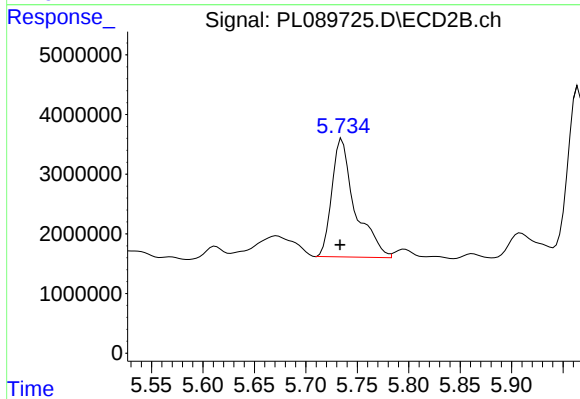

#27 Chlordane-5


R.T.: 5.735 min
Delta R.T.: 0.002 min
Response: 31132134
Conc: 458.56 ng/ml

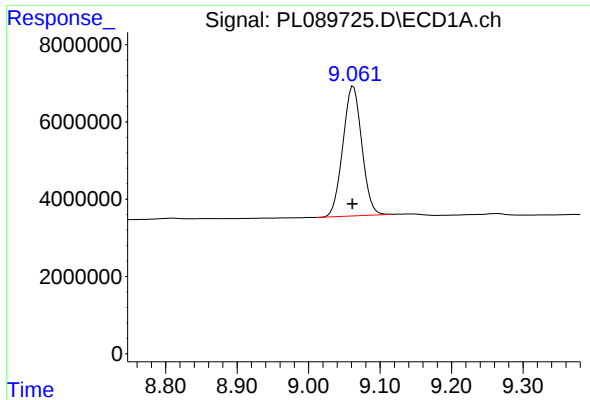

#28 Decachlorobiphenyl

R.T.: 9.063 min
Delta R.T.: 0.001 min
Response: 61811411
Conc: 45.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL052424

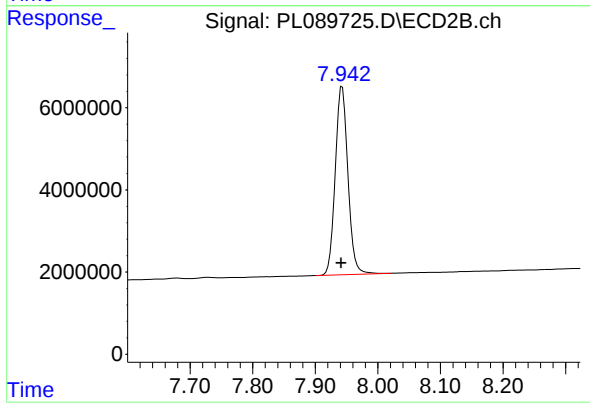

#28 Decachlorobiphenyl

R.T.: 7.943 min
Delta R.T.: 0.002 min
Response: 64780904
Conc: 47.32 ng/ml