

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052519\
 Data File : PL048993.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 May 2019 08:57
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 23:36:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

8) B	Heptachlo...	0.000	5.799	0	37724207	N.D.	12.934	#
9) A	Endosulfan I	5.346f	0.000	5073425	0	0.422	N.D.	#
13) MA	Dieldrin	5.538f	0.000	629325	0	0.048	N.D.	#
14) MA	Endrin	5.832f	0.000	11694028	0	0.961	N.D.	#
15) B	Endosulfa...	6.082	0.000	4604417	0	0.399	N.D.	#
27)	Chlordane-5	6.082	0.000	4604417	0	9.806	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052519\
Data File : PL048993.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 May 2019 08:57
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 23:36:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

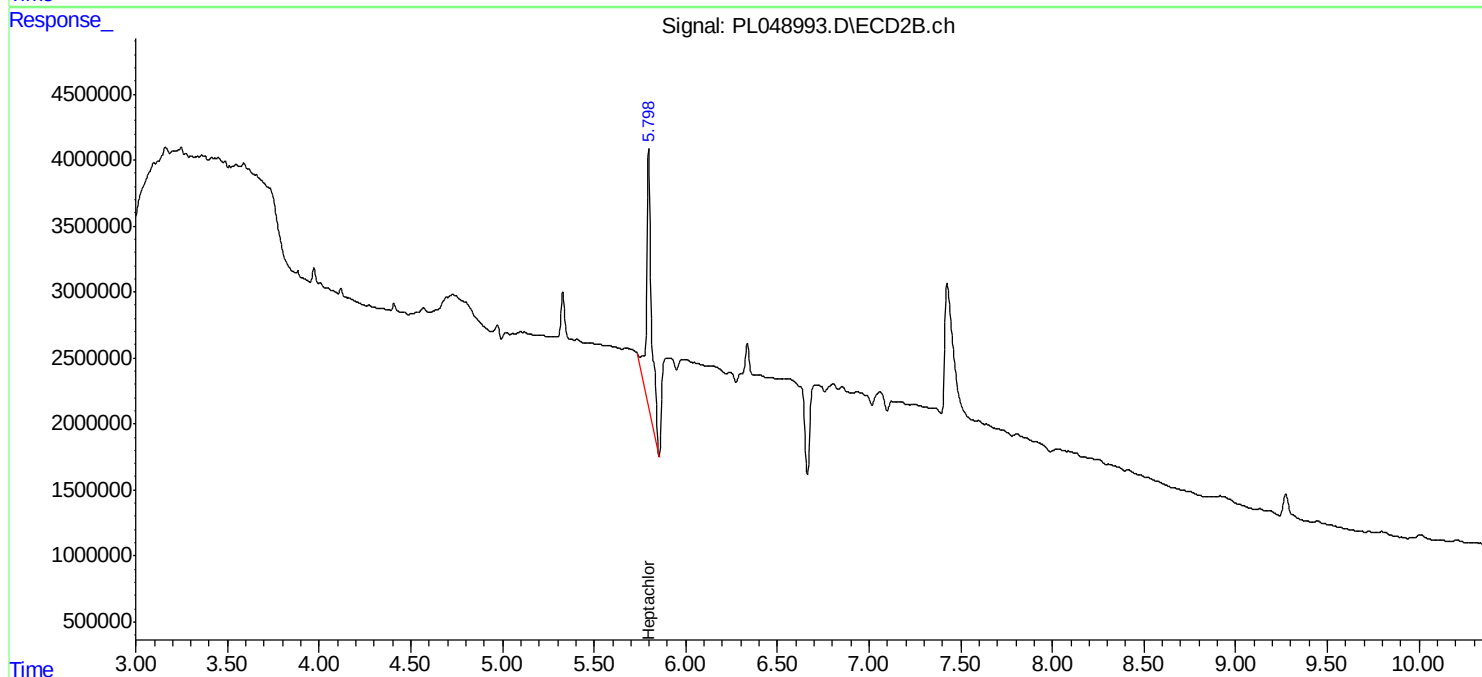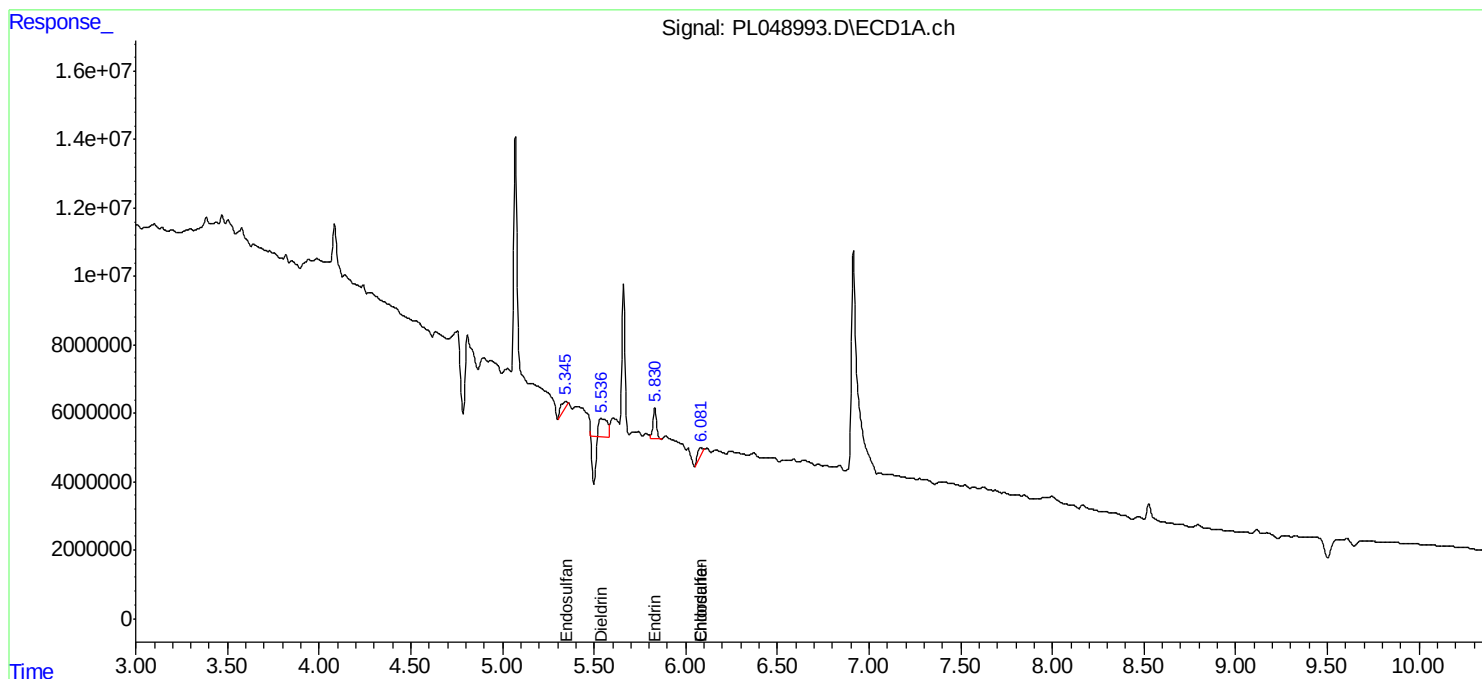


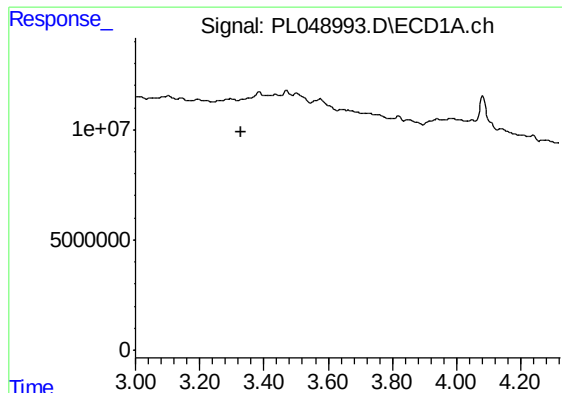

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

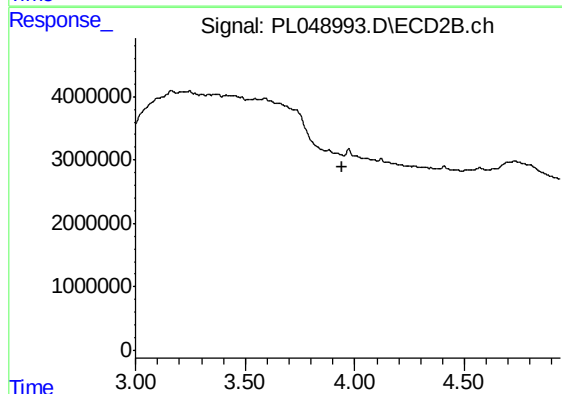


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.940 min
Response: 0
Conc: N.D.

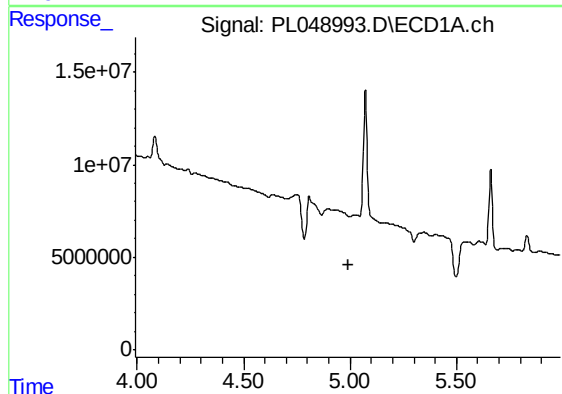


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.992 min
Response: 0
Conc: N.D.

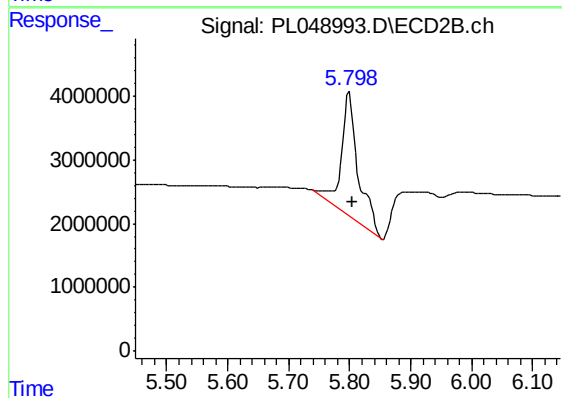

#8 Heptachlor epoxide


R.T.: 5.799 min
Delta R.T.: -0.005 min
Response: 37724207
Conc: 12.93 ng/ml

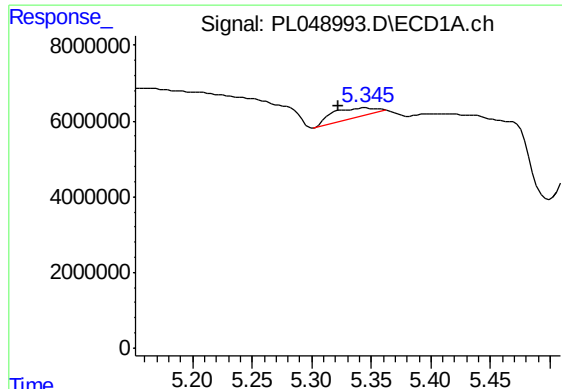

#9 Endosulfan I


R.T.: 5.346 min
Delta R.T.: 0.023 min
Response: 5073425
Conc: 0.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

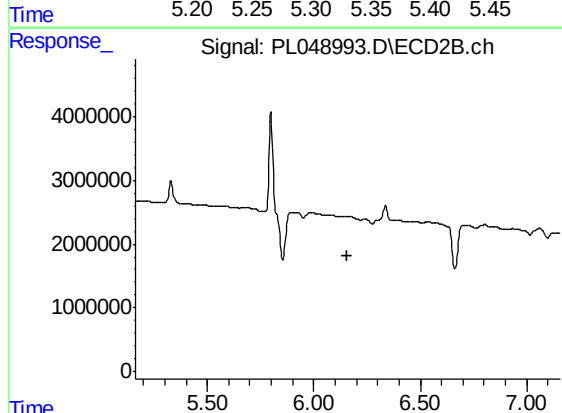


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.159 min
Response: 0
Conc: N.D.

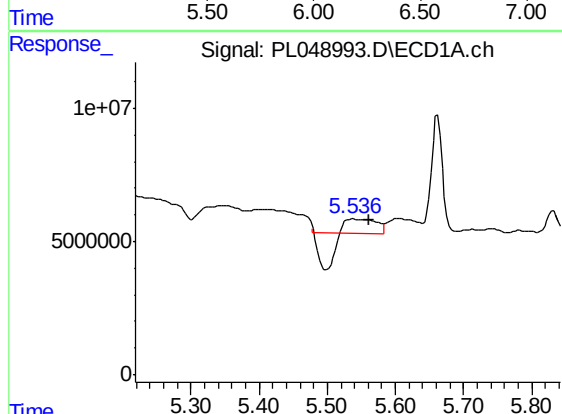


#13 Dieldrin

R.T.: 5.538 min
Delta R.T.: -0.024 min
Response: 629325
Conc: 0.05 ng/ml

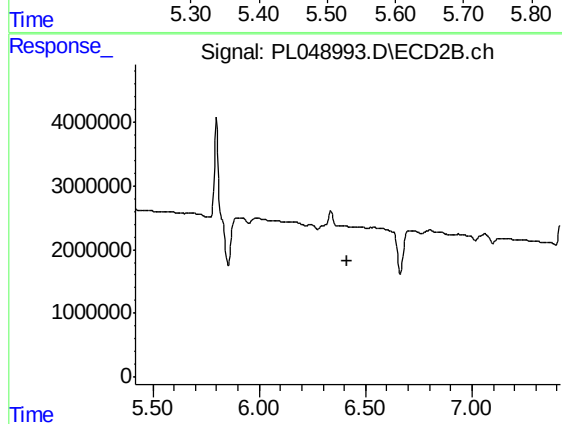

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

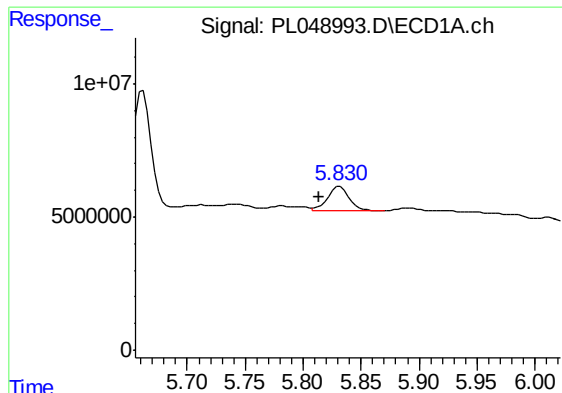

#14 Endrin


R.T.: 5.832 min
Delta R.T.: 0.017 min
Response: 11694028
Conc: 0.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

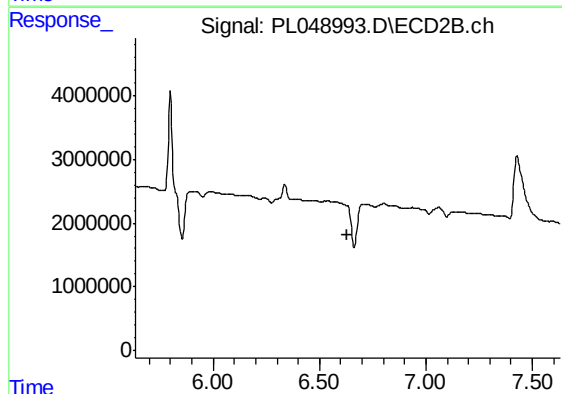


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.632 min
Response: 0
Conc: N.D.

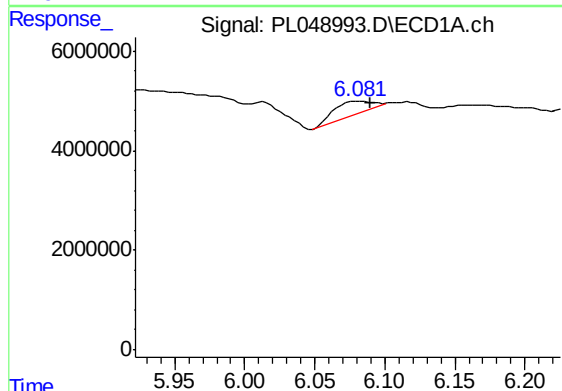


#15 Endosulfan II

R.T.: 6.082 min
Delta R.T.: -0.007 min
Response: 4604417
Conc: 0.40 ng/ml

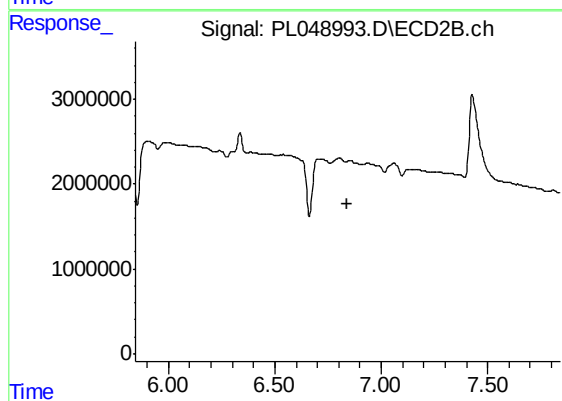

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.843 min
Response: 0
Conc: N.D.

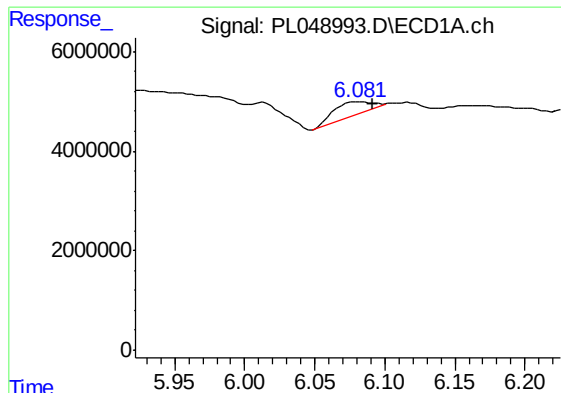

#27 Chlordane-5


R.T.: 6.082 min
Delta R.T.: -0.009 min
Response: 4604417
Conc: 9.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

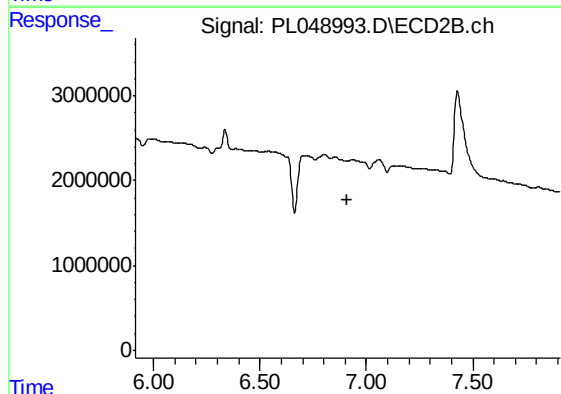


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.913 min
Response: 0
Conc: N.D.

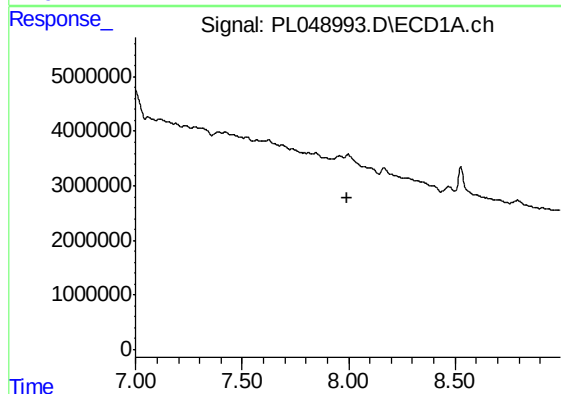

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.996 min
Response: 0
Conc: N.D.

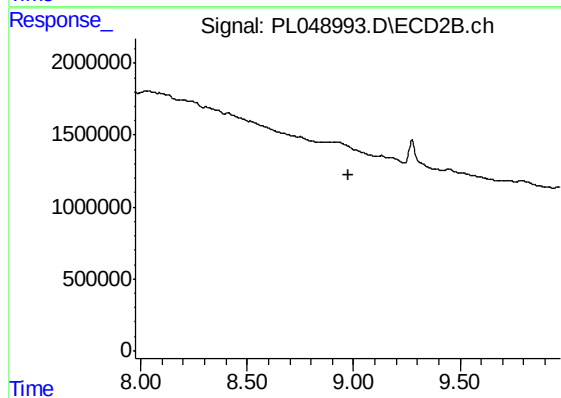

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.975 min
Response: 0
Conc: N.D.