

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052521\
 Data File : PL066857.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 May 2021 08:37
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 25 17:04:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052421.M
 Quant Title : GC Extractables
 QLast Update : Tue May 25 06:06:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
9) A	Endosulfan I	0.000	8.398	0	510633	N.D. 0.617 #
10) B	gamma-Chl...	0.000	8.264	0	3730424	N.D. 3.997 #
11) B	alpha-Chl...	0.000	8.351	0	1069713	N.D. 1.164 #
25)	Chlordane-3	0.000	8.264	0	3730424	N.D. 28.304 #
26)	Chlordane-4	0.000	8.351	0	1069713	N.D. 6.715 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052521\
Data File : PL066857.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 May 2021 08:37
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 25 17:04:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052421.M
Quant Title : GC Extractables
QLast Update : Tue May 25 06:06:45 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

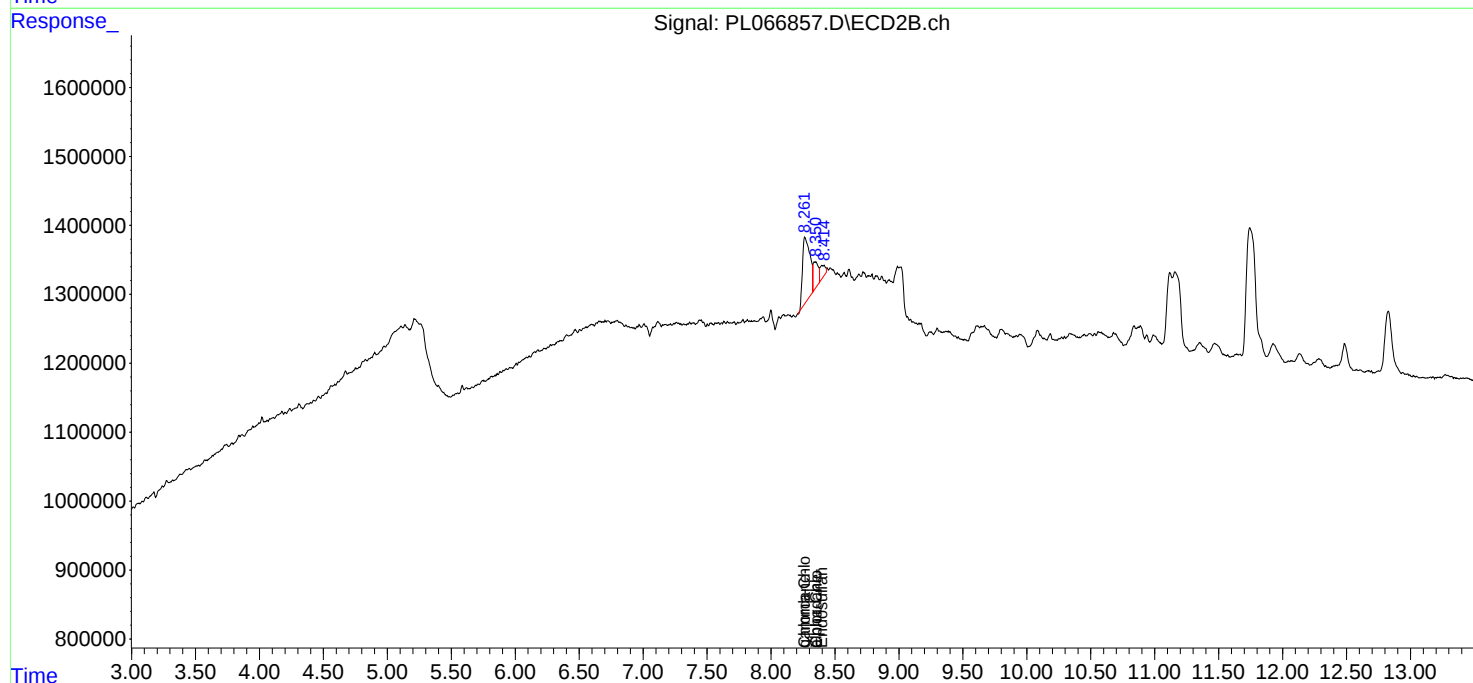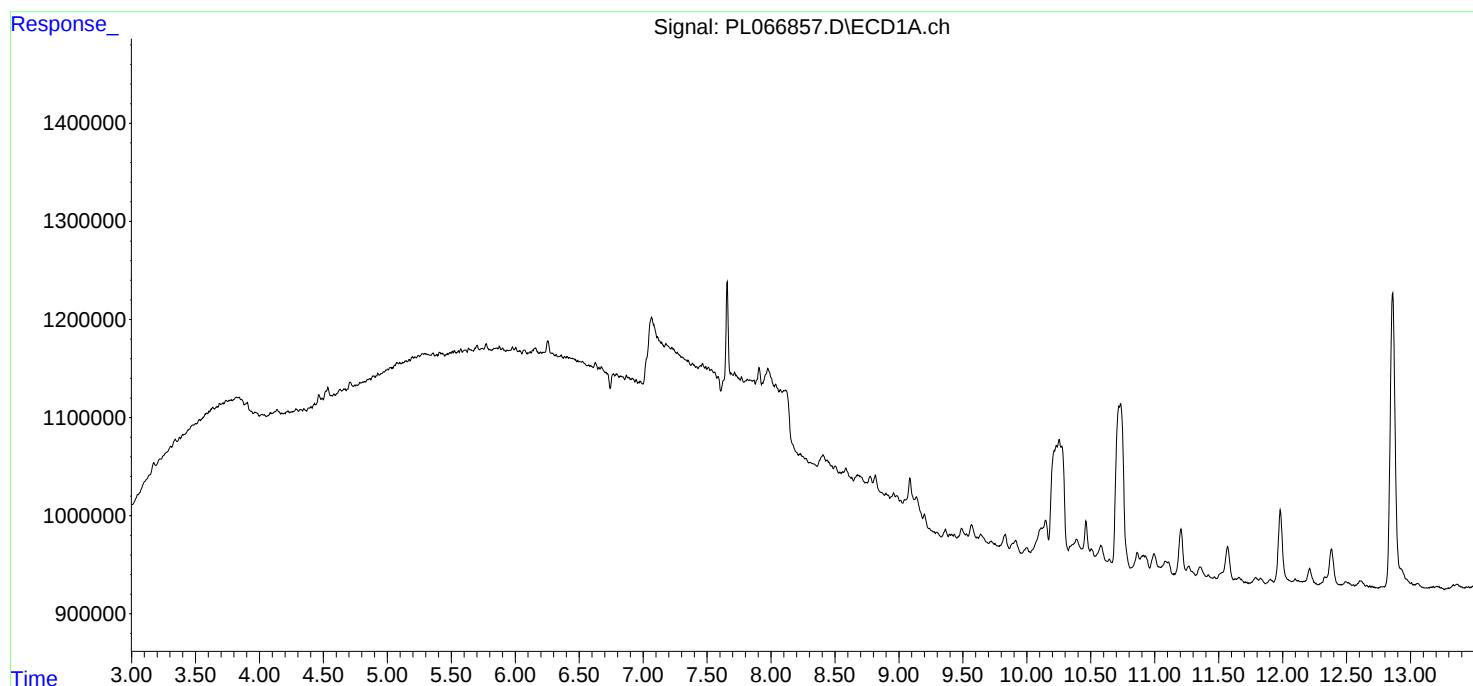


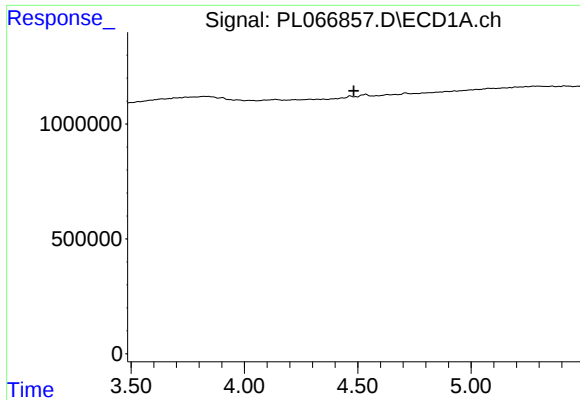

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.482 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

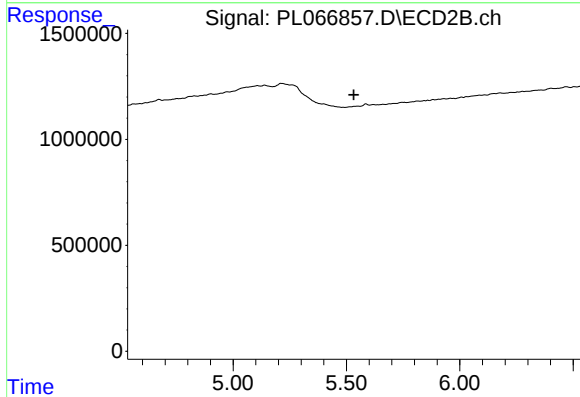


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 5.532 min
Response: 0
Conc: N.D.

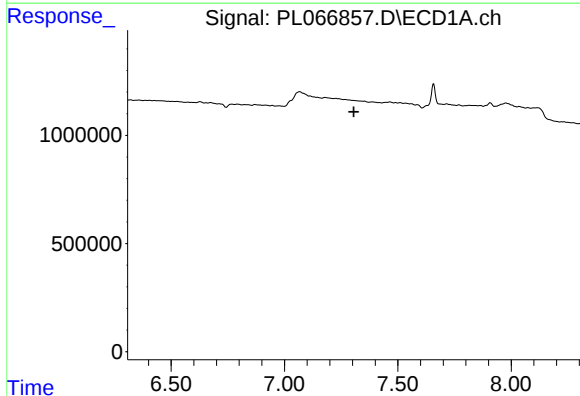


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.306 min
Response: 0
Conc: N.D.

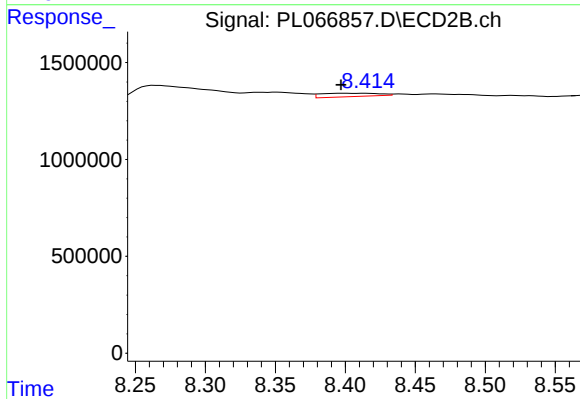

#9 Endosulfan I


R.T.: 8.398 min
Delta R.T.: 0.001 min
Response: 510633
Conc: 0.62 ng/ml

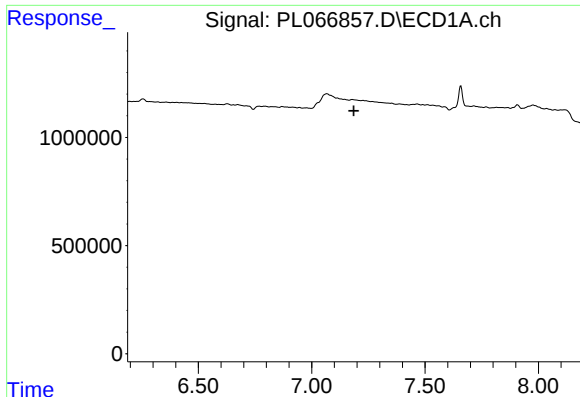

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 7.186 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

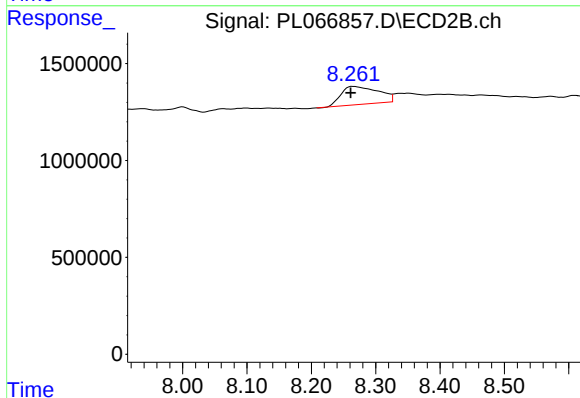


#10 gamma-Chlordane

R.T.: 8.264 min
Delta R.T.: 0.003 min
Response: 3730424
Conc: 4.00 ng/ml

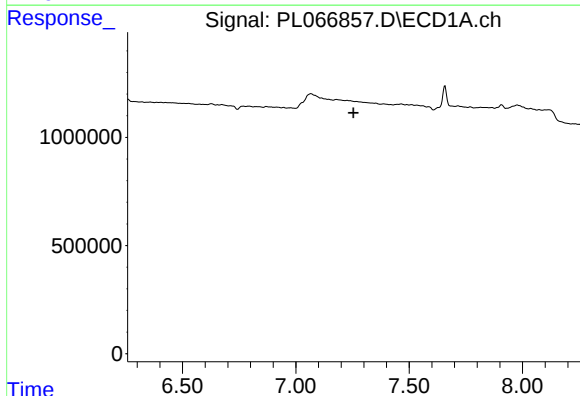


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.255 min
Response: 0
Conc: N.D.

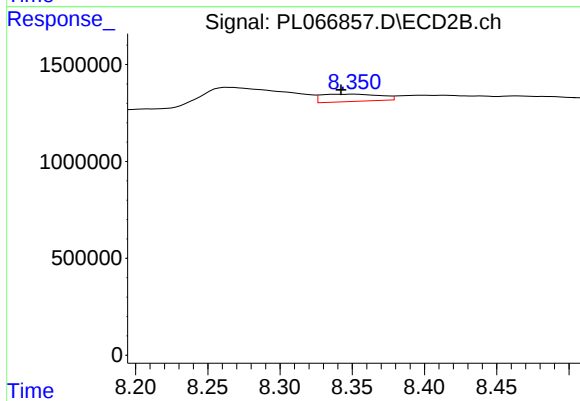

#11 alpha-Chlordane


R.T.: 8.351 min
Delta R.T.: 0.009 min
Response: 1069713
Conc: 1.16 ng/ml

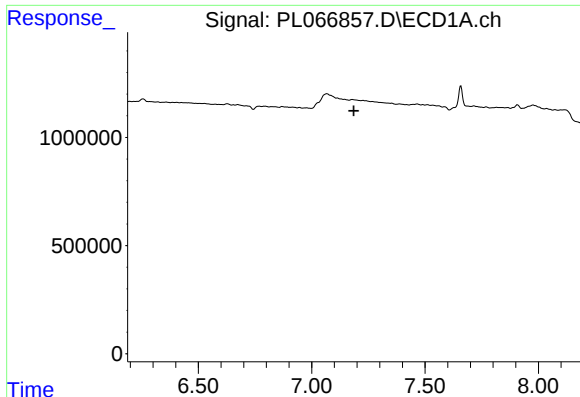

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.186 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

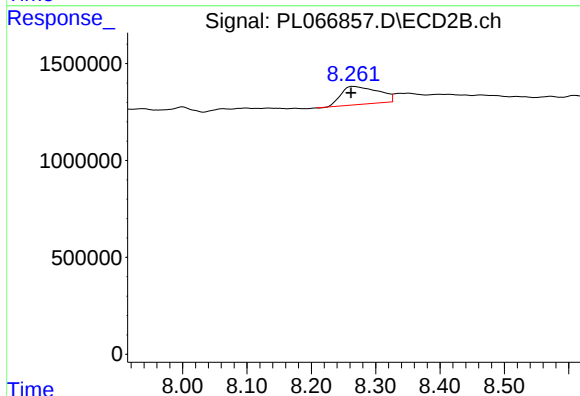


#25 Chlordane-3

R.T.: 8.264 min
Delta R.T.: 0.003 min
Response: 3730424
Conc: 28.30 ng/ml

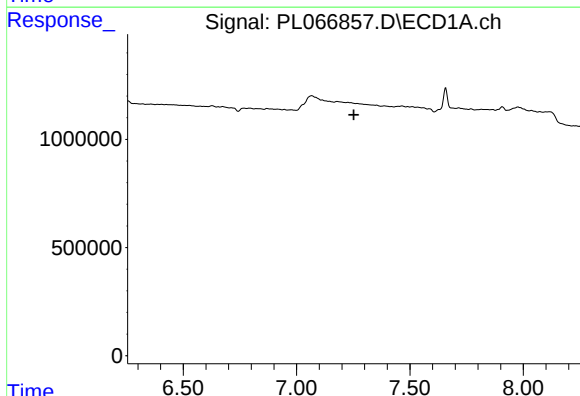


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.253 min
Response: 0
Conc: N.D.

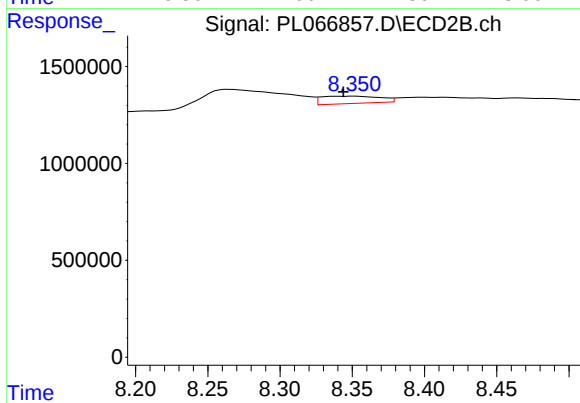

#26 Chlordane-4


R.T.: 8.351 min
Delta R.T.: 0.007 min
Response: 1069713
Conc: 6.72 ng/ml

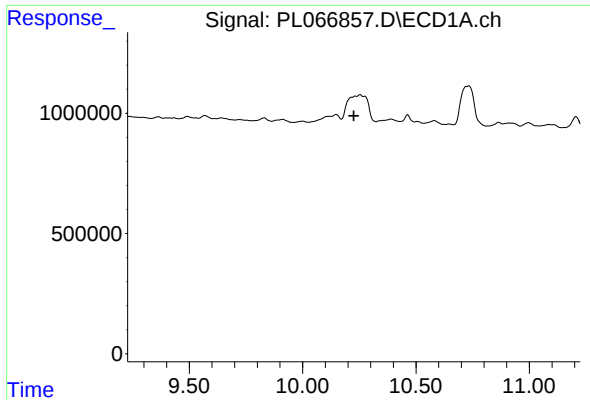

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.225 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

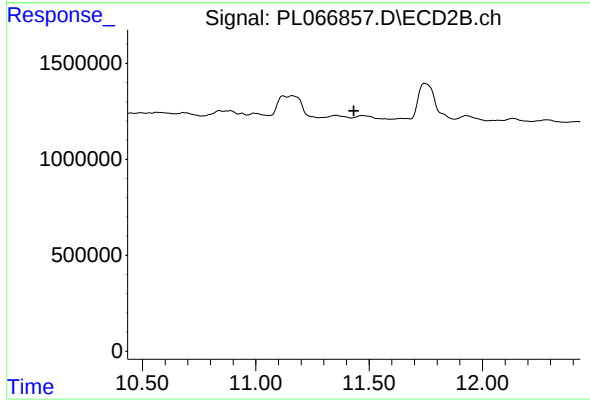

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 11.433 min
Response: 0
Conc: N.D.