

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052521\
 Data File : PL066879.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 May 2021 17:12
 Operator : AR\AJ
 Sample : M2262-07
 Misc : CHLOR LOD 25 PPB
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 25 18:37:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052421.M
 Quant Title : GC Extractables
 QLast Update : Tue May 25 06:06:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.481	5.532	10049991	15190328	17.517	17.685
28)	SA Decachlor...	10.225	11.431	14234684	17295930	19.143	20.071
Target Compounds							
4)	MA Heptachlor	0.000	7.155	0	650551	N.D.	0.693 #
5)	MB Aldrin	0.000	7.503f	0	489688	N.D.	0.501 #
8)	B Heptachlo...	0.000	7.979	0	420651	N.D.	0.466 #
10)	B gamma-Chl...	7.186	8.261	589405	2268811	0.738	2.431 #
11)	B alpha-Chl...	0.000	8.343	0	3215648	N.D.	3.499 #
23)	Chlordane-1	0.000	6.939f	0	1674027	N.D.	55.584 #
24)	Chlordane-2	0.000	7.503	0	489688	N.D.	12.674 #
25)	Chlordane-3	7.186	8.261	589405	2268811	7.314	17.214 #
26)	Chlordane-4	0.000	8.343	0	3215648	N.D.	20.186 #
27)	Chlordane-5	0.000	9.230	0	387803	N.D.	13.731 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052521\
Data File : PL066879.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 May 2021 17:12
Operator : AR\AJ
Sample : M2262-07
Misc : CHLOR LOD 25 PPB
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 25 18:37:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052421.M
Quant Title : GC Extractables
QLast Update : Tue May 25 06:06:45 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

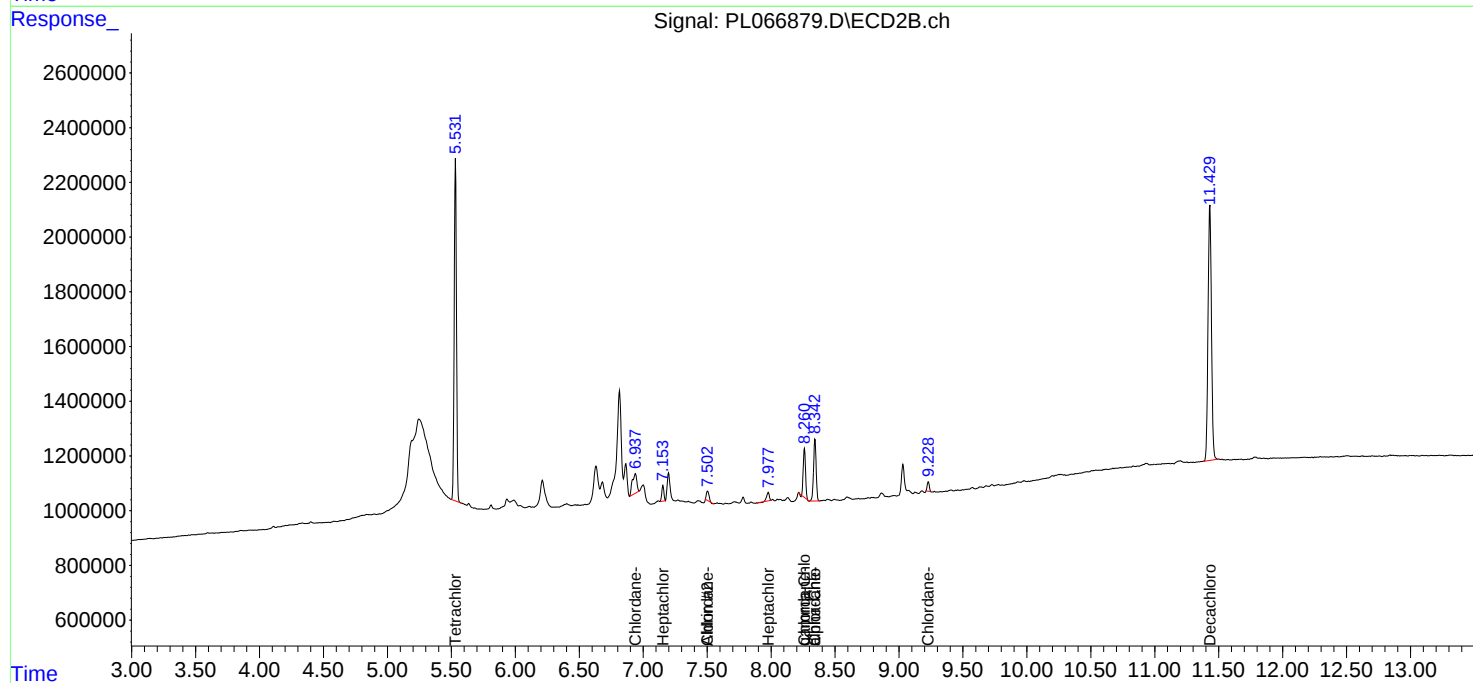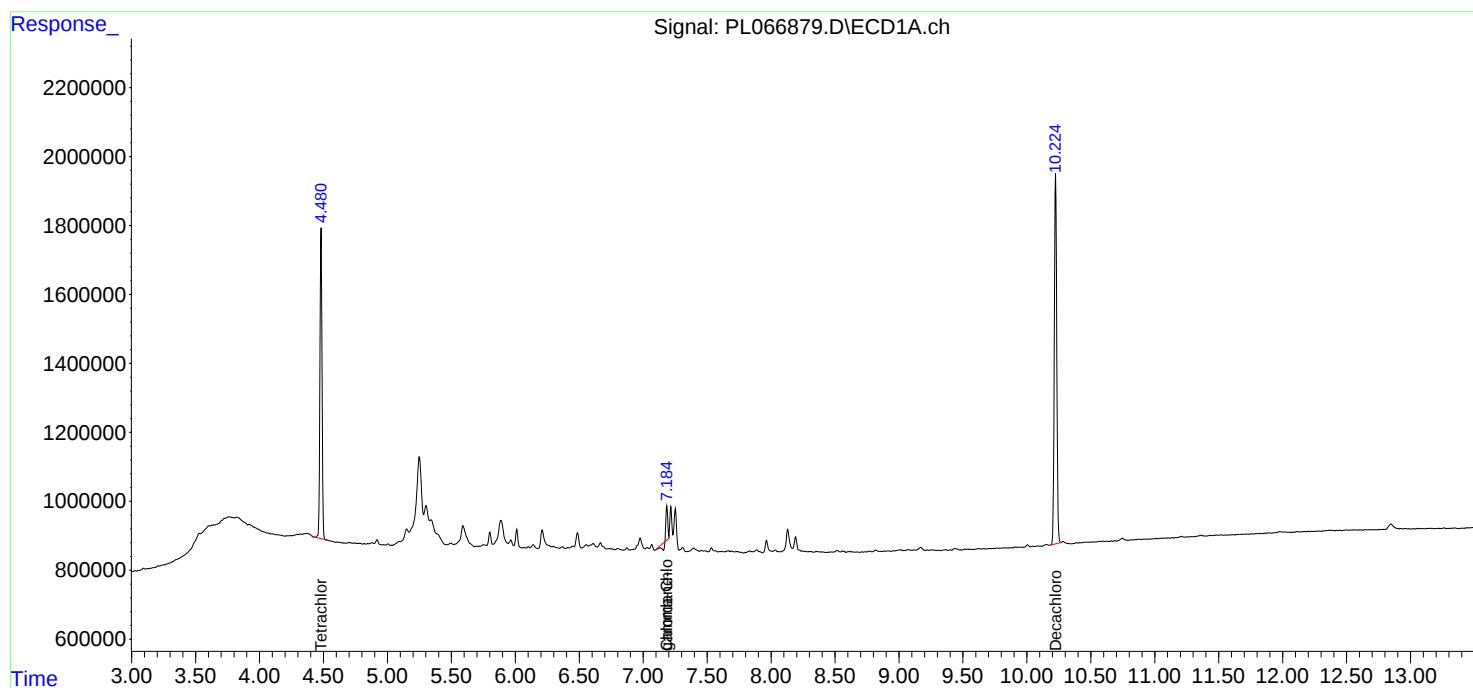


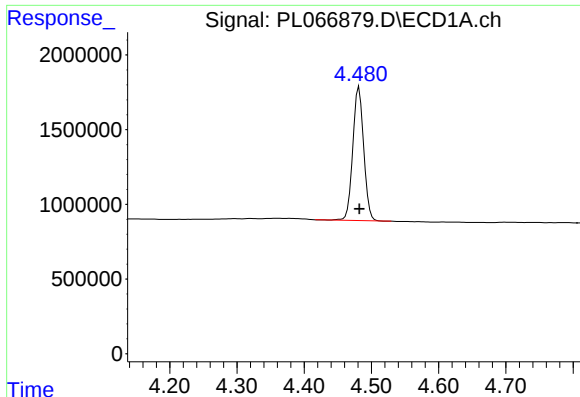

#1 Tetrachloro-m-xylene


R.T.: 4.481 min
Delta R.T.: 0.000 min
Response: 10049991
Conc: 17.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

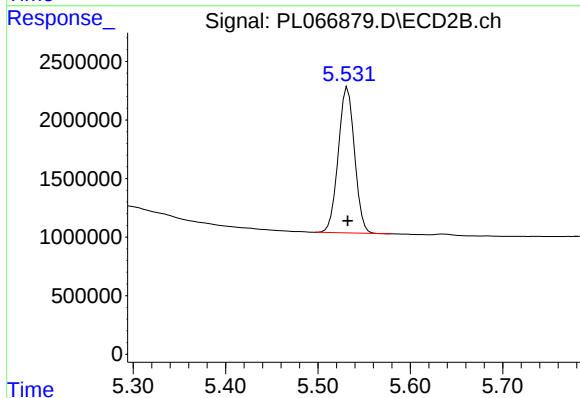


#1 Tetrachloro-m-xylene

R.T.: 5.532 min
Delta R.T.: 0.000 min
Response: 15190328
Conc: 17.69 ng/ml

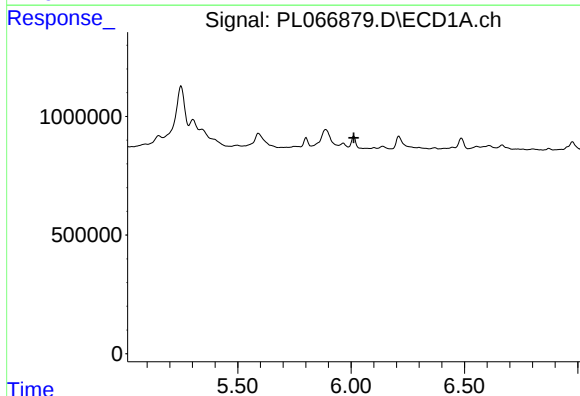


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 6.012 min
Response: 0
Conc: N.D.

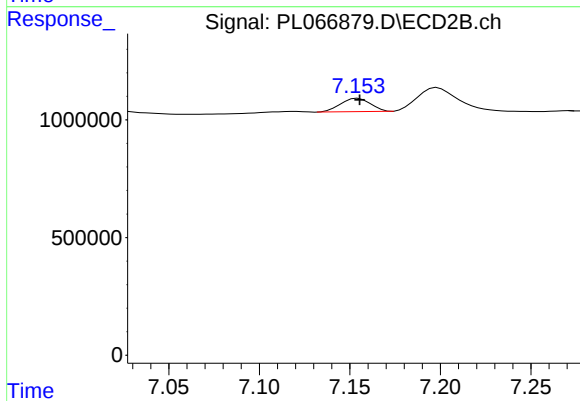

#4 Heptachlor


R.T.: 7.155 min
Delta R.T.: 0.000 min
Response: 650551
Conc: 0.69 ng/ml

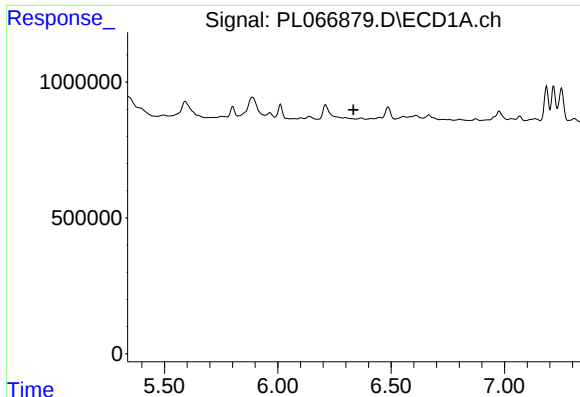

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 6.334 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

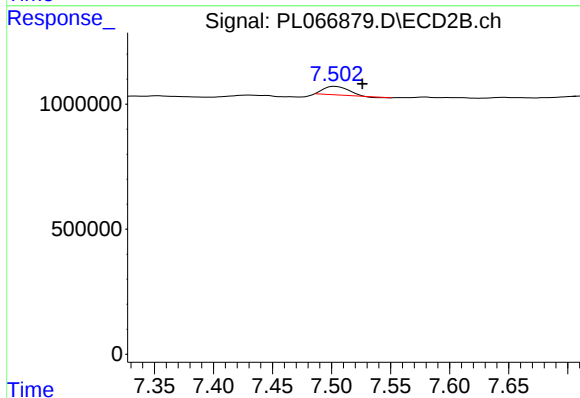


#5 Aldrin

R.T.: 7.503 min
Delta R.T.: -0.023 min
Response: 489688
Conc: 0.50 ng/ml

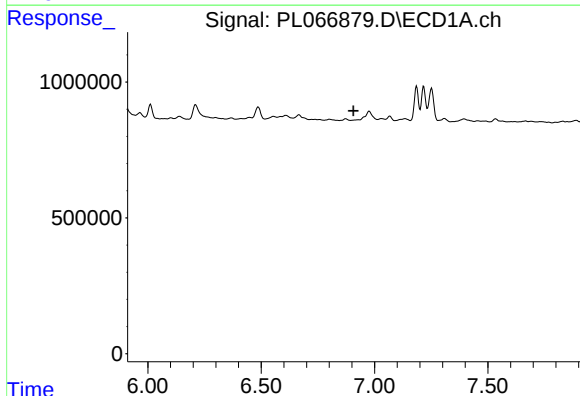


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 6.908 min
Response: 0
Conc: N.D.

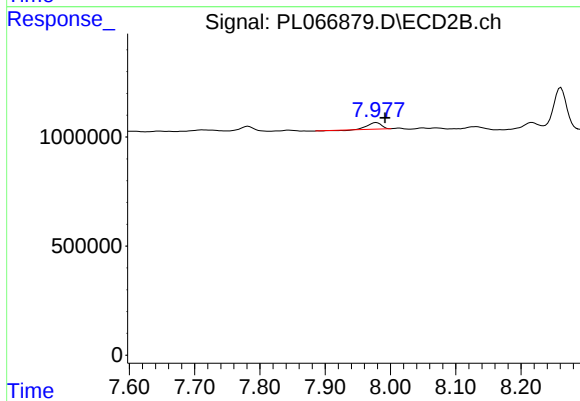

#8 Heptachlor epoxide


R.T.: 7.979 min
Delta R.T.: -0.013 min
Response: 420651
Conc: 0.47 ng/ml

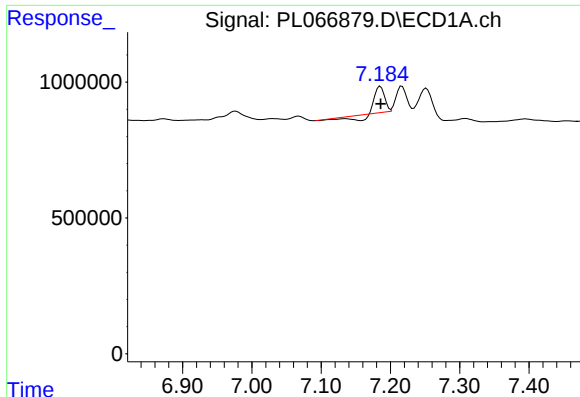

#10 gamma-Chlordane


R.T.: 7.186 min
Delta R.T.: 0.000 min
Response: 589405
Conc: 0.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

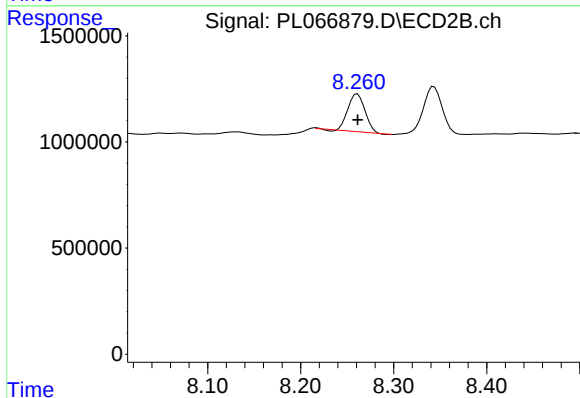


#10 gamma-Chlordane

R.T.: 8.261 min
Delta R.T.: 0.000 min
Response: 2268811
Conc: 2.43 ng/ml

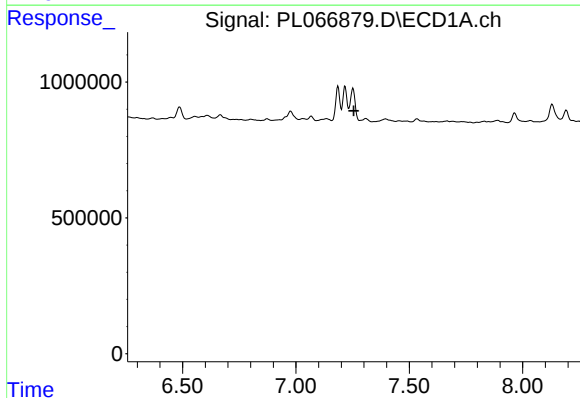


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.255 min
Response: 0
Conc: N.D.

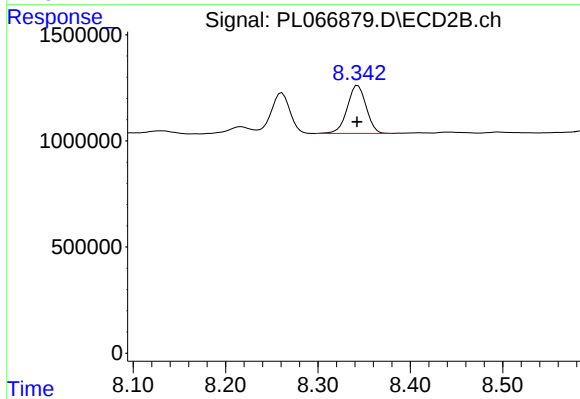

#11 alpha-Chlordane


R.T.: 8.343 min
Delta R.T.: 0.000 min
Response: 3215648
Conc: 3.50 ng/ml

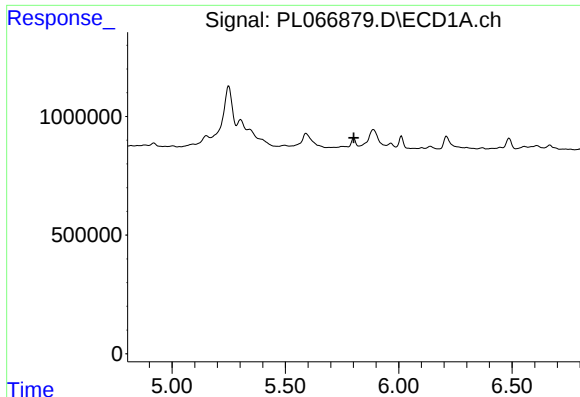

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.802 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

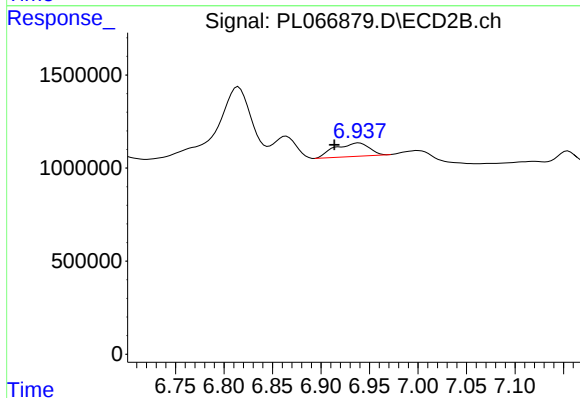


#23 Chlordane-1

R.T.: 6.939 min
Delta R.T.: 0.025 min
Response: 1674027
Conc: 55.58 ng/ml

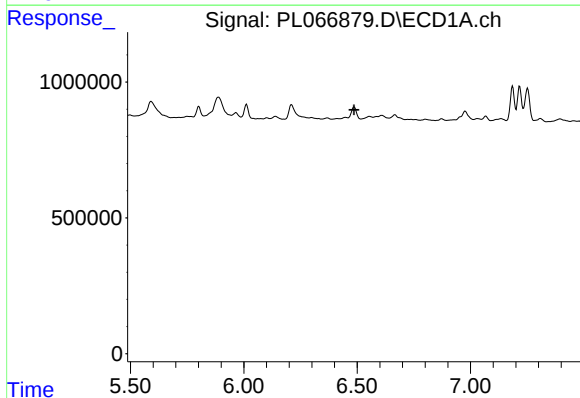


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 6.487 min
Response: 0
Conc: N.D.

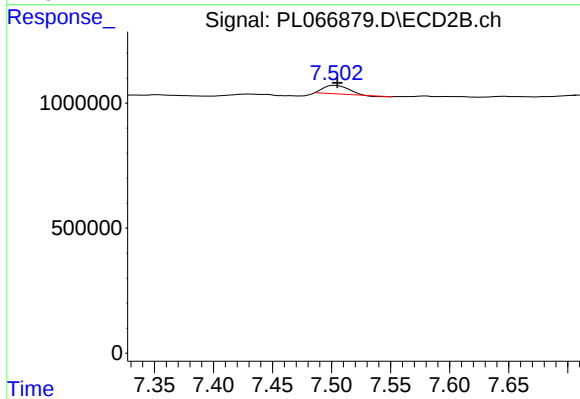

#24 Chlordane-2


R.T.: 7.503 min
Delta R.T.: -0.002 min
Response: 489688
Conc: 12.67 ng/ml

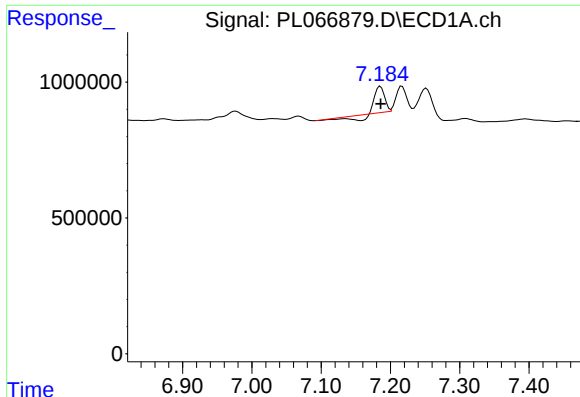

#25 Chlordane-3


R.T.: 7.186 min
Delta R.T.: 0.000 min
Response: 589405
Conc: 7.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

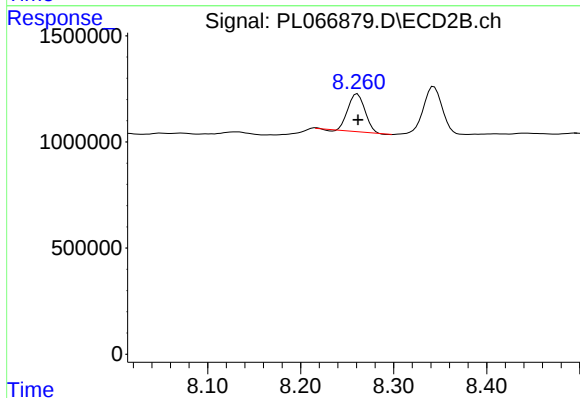


#25 Chlordane-3

R.T.: 8.261 min
Delta R.T.: 0.000 min
Response: 2268811
Conc: 17.21 ng/ml

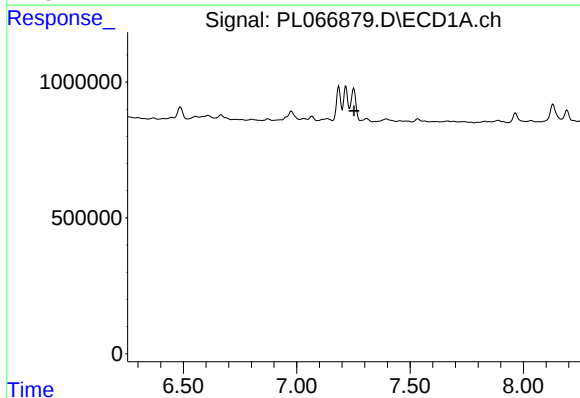


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 7.253 min
Response: 0
Conc: N.D.

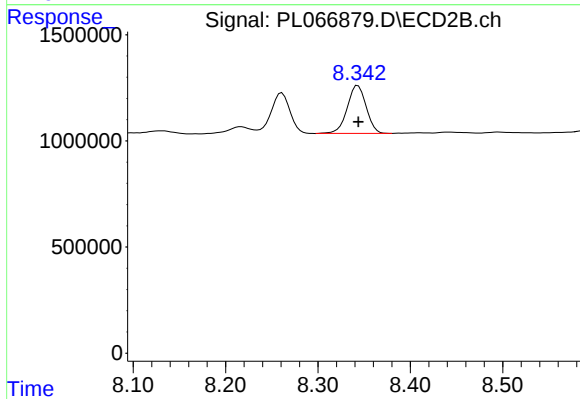

#26 Chlordane-4


R.T.: 8.343 min
Delta R.T.: 0.000 min
Response: 3215648
Conc: 20.19 ng/ml

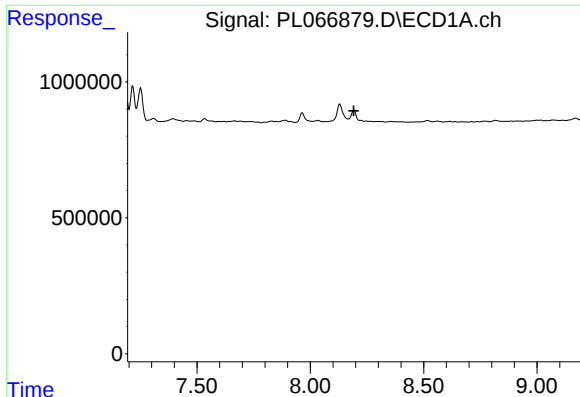

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 8.193 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

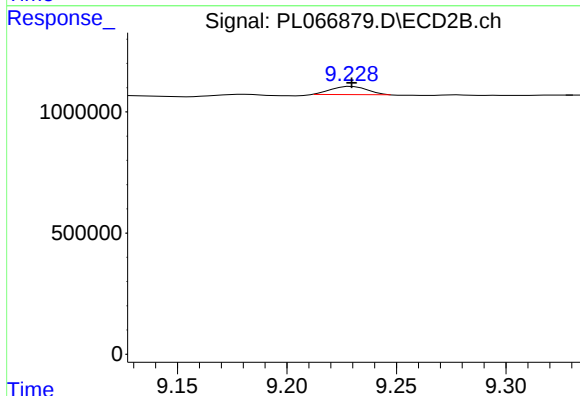


#27 Chlordane-5

R.T.: 9.230 min
Delta R.T.: 0.000 min
Response: 387803
Conc: 13.73 ng/ml

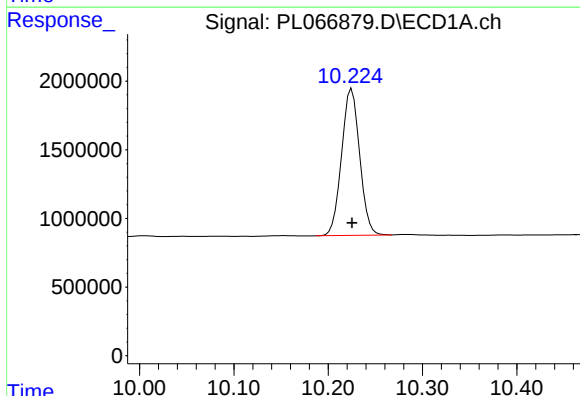

#28 Decachlorobiphenyl

R.T.: 10.225 min
Delta R.T.: 0.000 min
Response: 14234684
Conc: 19.14 ng/ml

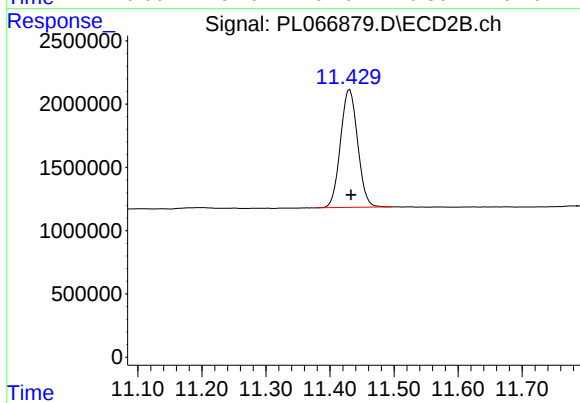

#28 Decachlorobiphenyl

R.T.: 11.431 min
Delta R.T.: -0.002 min
Response: 17295930
Conc: 20.07 ng/ml