

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052522\
 Data File : PL075009.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 May 2022 09:23
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 01:07:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.643	4.646	11922603	31072511	23.482	22.639
28)	SA Decachlor...	11.637	10.394	11267264	25390365	25.230	24.737
Target Compounds							
6)	B beta-BHC	0.000	6.155	0	39979	N.D.	0.050 #
7)	B delta-BHC	0.000	6.416	0	368826	N.D.	0.236 #
8)	B Heptachlo...	8.125	0.000	2725870	0	4.793	N.D. #
10)	B gamma-Chl...	8.385	0.000	602447	0	1.165	N.D. #
13)	MA Dieldrin	0.000	7.764	0	2476114	N.D.	1.944 #
14)	MA Endrin	0.000	8.075	0	1309360	N.D.	1.240 #
21)	B Endrin ke...	10.185	0.000	465304	0	0.907	N.D. #
25)	Chlordane-3	8.385	0.000	602447	0	8.800	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052522\
Data File : PL075009.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 May 2022 09:23
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 01:07:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

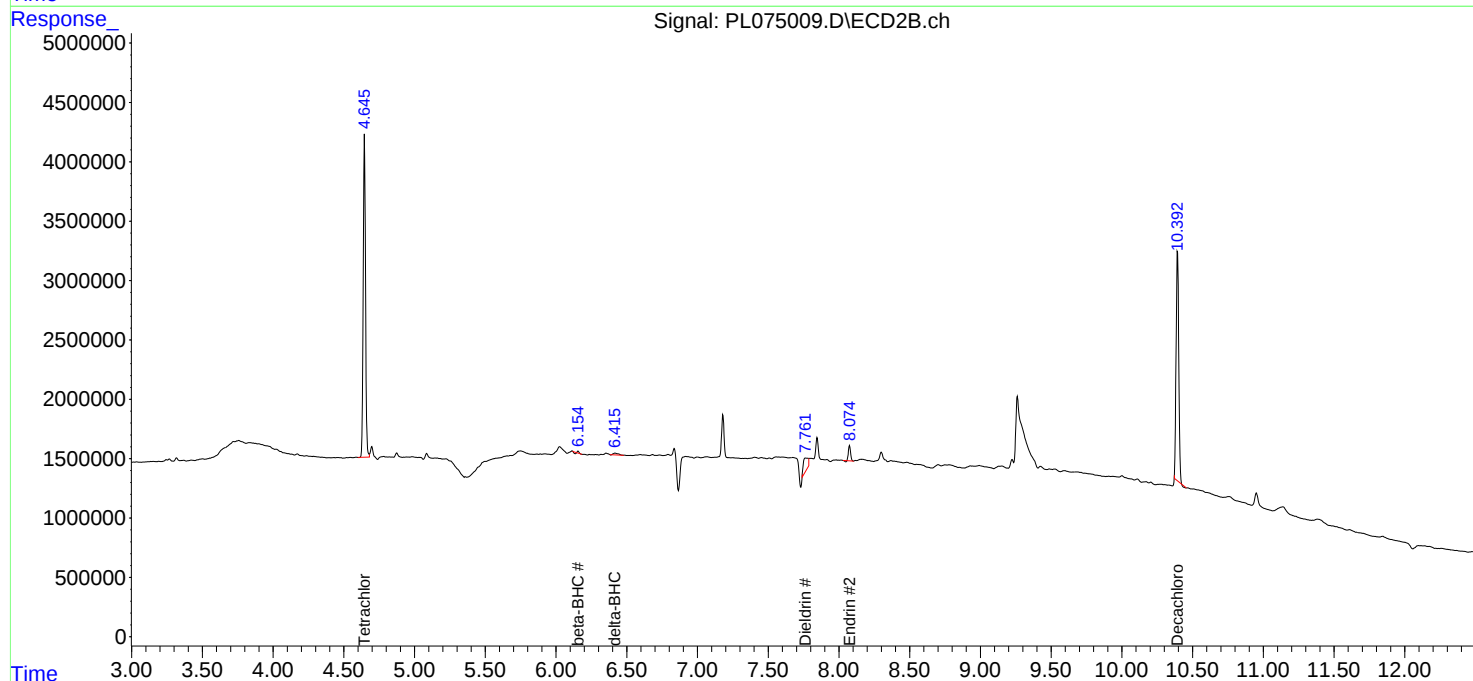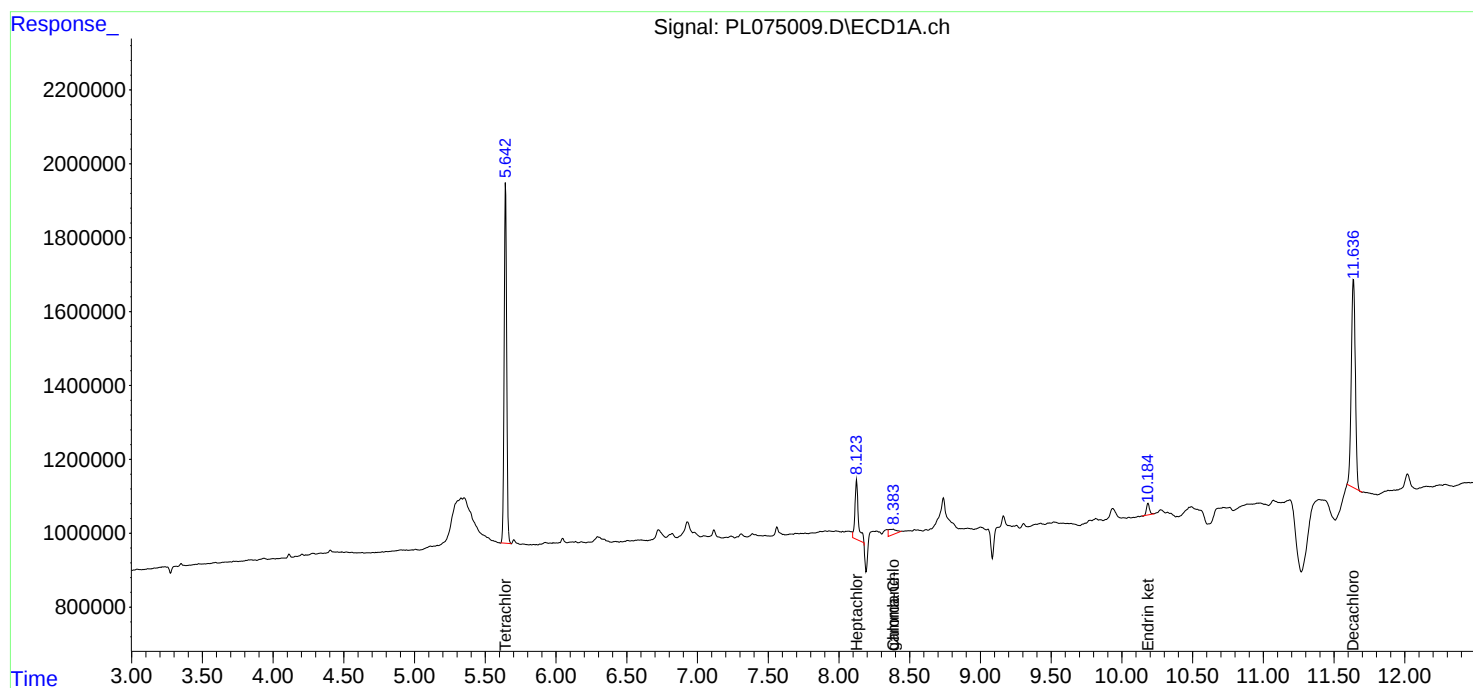


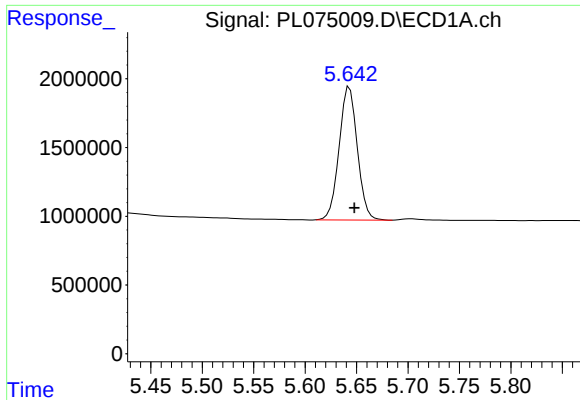

#1 Tetrachloro-m-xylene


R.T.: 5.643 min
Delta R.T.: -0.005 min
Response: 11922603
Conc: 23.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

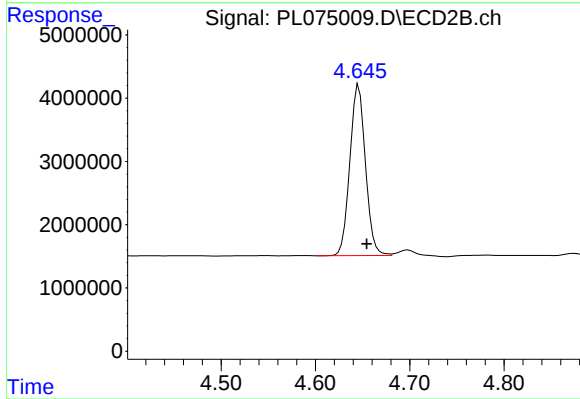


#1 Tetrachloro-m-xylene

R.T.: 4.646 min
Delta R.T.: -0.008 min
Response: 31072511
Conc: 22.64 ng/ml

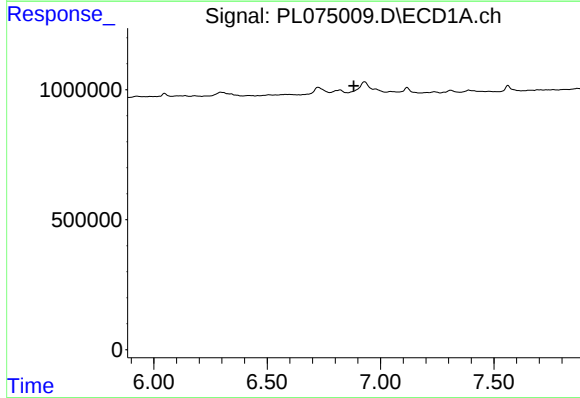


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.882 min
Response: 0
Conc: N.D.

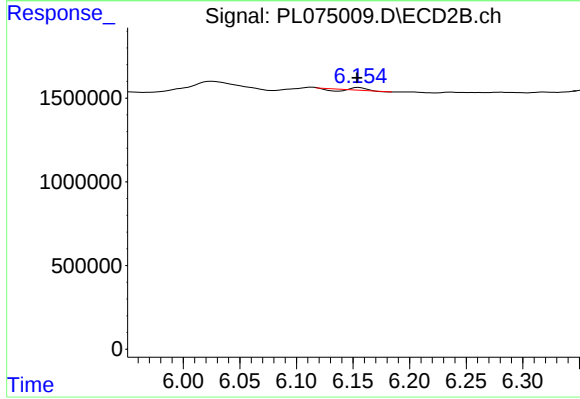

#6 beta-BHC


R.T.: 6.155 min
Delta R.T.: 0.002 min
Response: 39979
Conc: 0.05 ng/ml

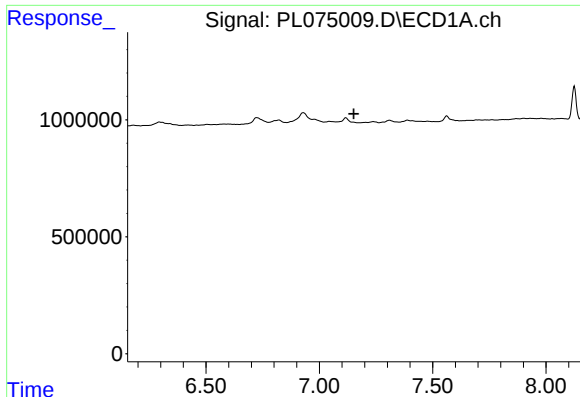

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 7.152 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

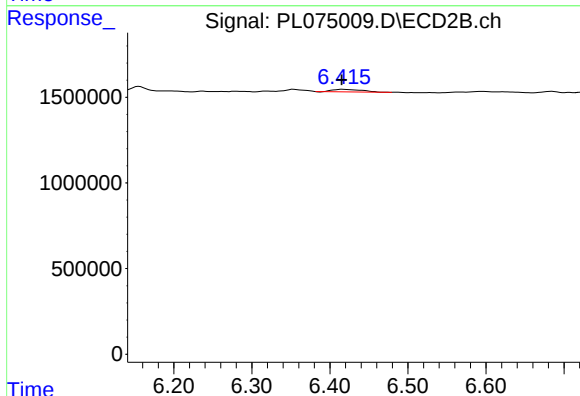


#7 delta-BHC

R.T.: 6.416 min
Delta R.T.: 0.001 min
Response: 368826
Conc: 0.24 ng/ml

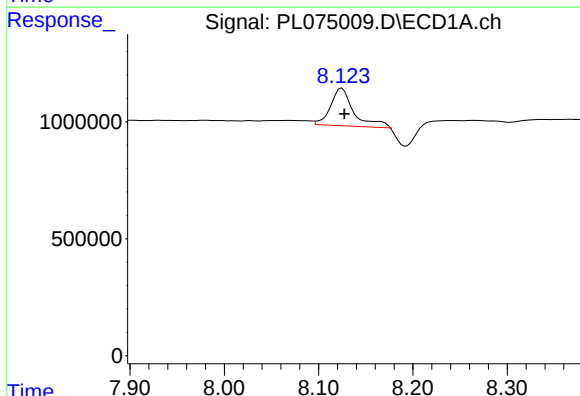


#8 Heptachlor epoxide

R.T.: 8.125 min
Delta R.T.: -0.003 min
Response: 2725870
Conc: 4.79 ng/ml

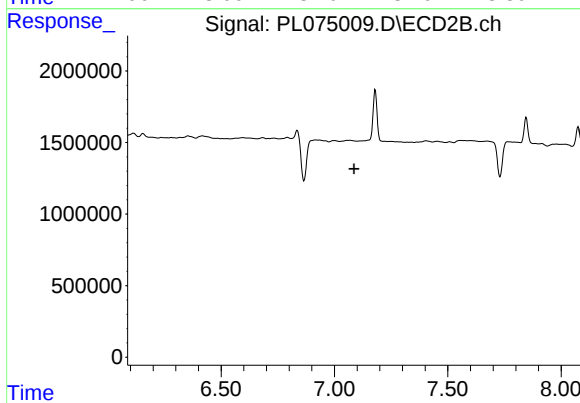

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 7.087 min
Response: 0
Conc: N.D.

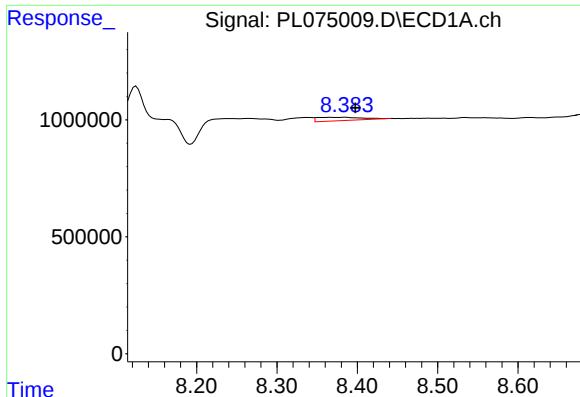

#10 gamma-Chlordane


R.T.: 8.385 min
Delta R.T.: -0.013 min
Response: 602447
Conc: 1.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

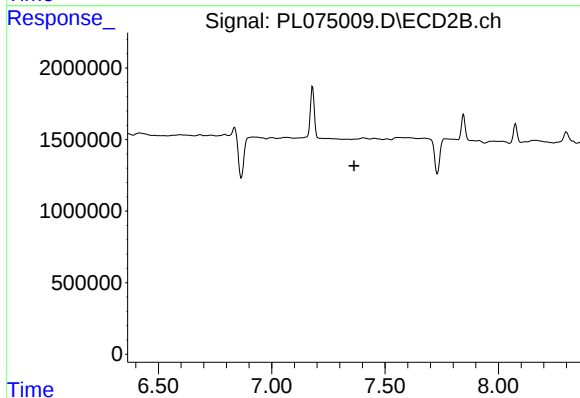


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.363 min
Response: 0
Conc: N.D.

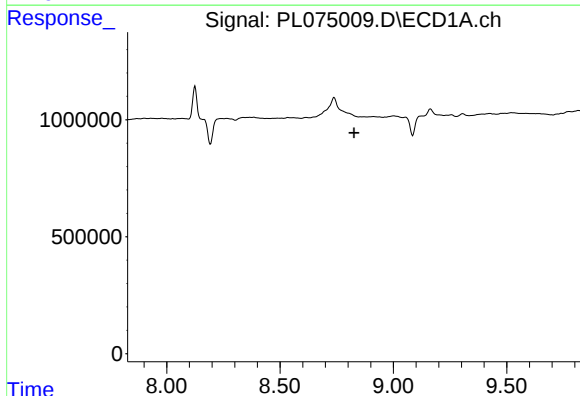


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.827 min
Response: 0
Conc: N.D.

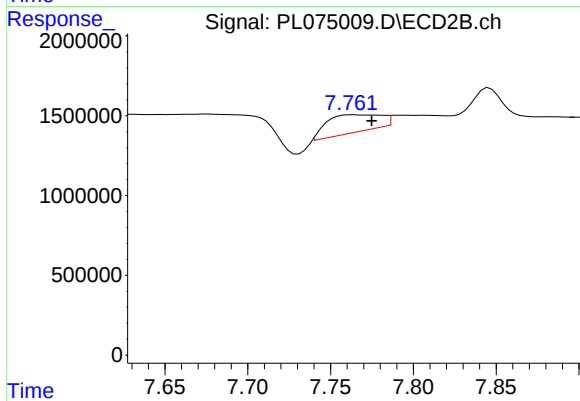

#13 Dieldrin


R.T.: 7.764 min
Delta R.T.: -0.011 min
Response: 2476114
Conc: 1.94 ng/ml

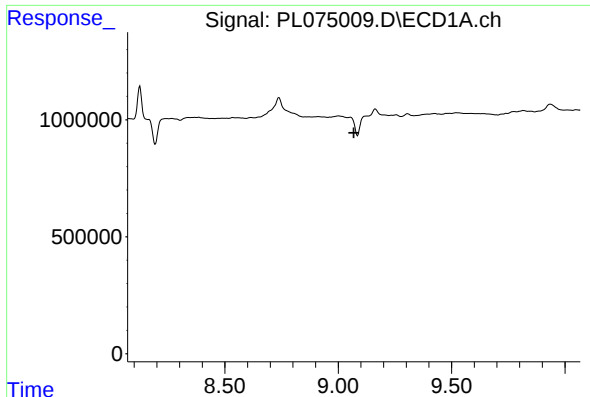

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.068 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

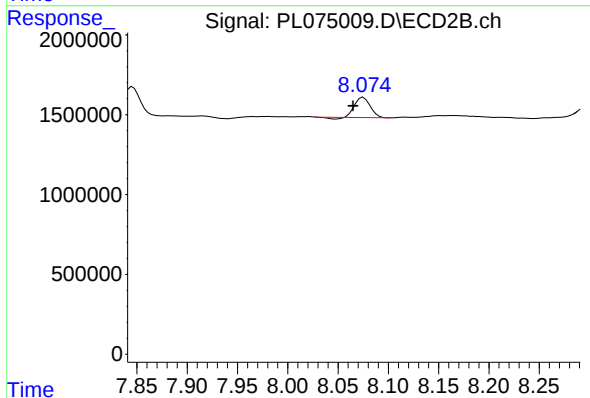


#14 Endrin

R.T.: 8.075 min
Delta R.T.: 0.010 min
Response: 1309360
Conc: 1.24 ng/ml

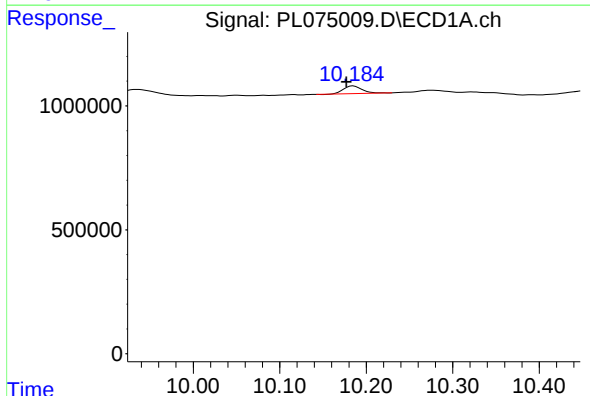


#21 Endrin ketone

R.T.: 10.185 min
Delta R.T.: 0.008 min
Response: 465304
Conc: 0.91 ng/ml

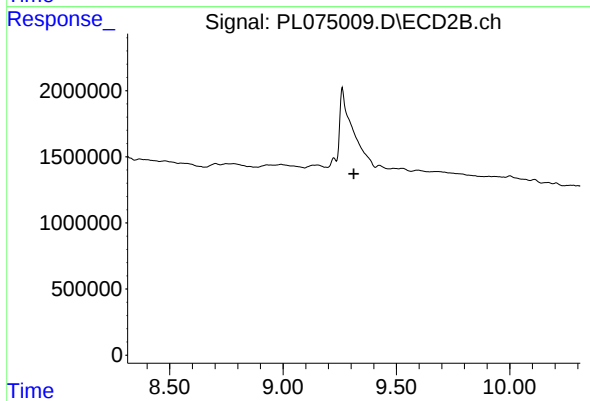

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.311 min
Response: 0
Conc: N.D.

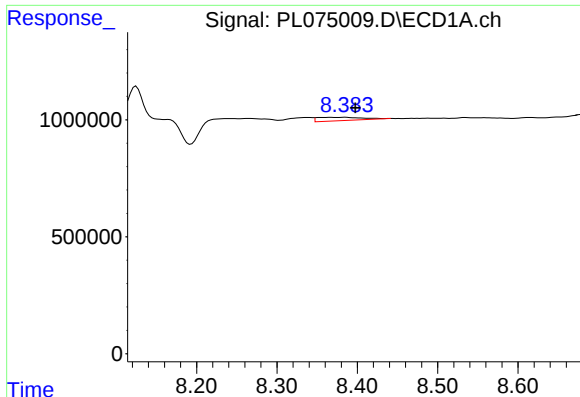

#25 Chlordane-3


R.T.: 8.385 min
Delta R.T.: -0.013 min
Response: 602447
Conc: 8.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

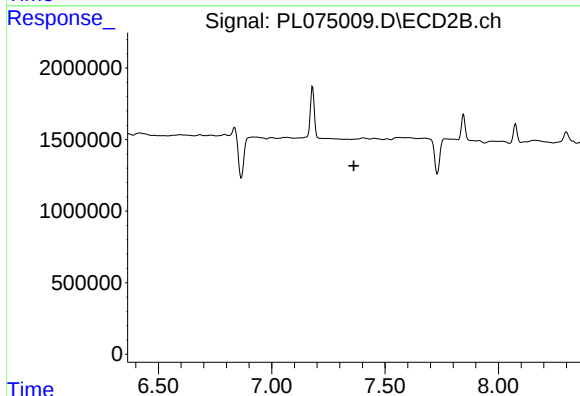


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.362 min
Response: 0
Conc: N.D.

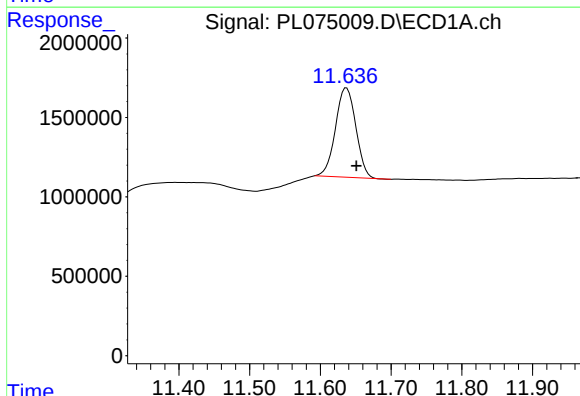

#28 Decachlorobiphenyl

R.T.: 11.637 min
Delta R.T.: -0.014 min
Response: 11267264
Conc: 25.23 ng/ml

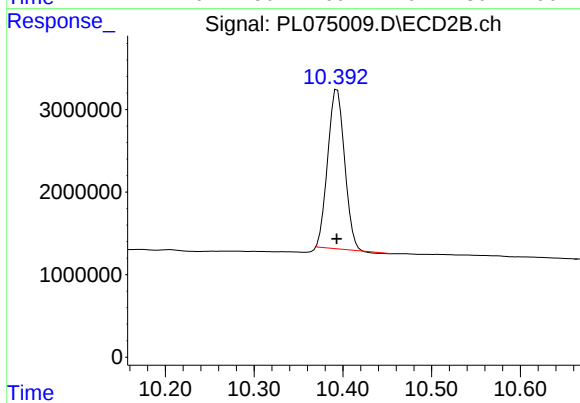

#28 Decachlorobiphenyl

R.T.: 10.394 min
Delta R.T.: 0.000 min
Response: 25390365
Conc: 24.74 ng/ml