

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL052522\  
 Data File : PL075027.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 25 May 2022 17:59  
 Operator : AR\AJ  
 Sample : N2923-08  
 Misc :  
 ALS Vial : 18 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 26 01:11:18 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL051122.M  
 Quant Title : GC Extractables  
 QLast Update : Sat May 14 02:37:15 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

|                             | Compound        | RT#1    | RT#2   | Resp#1  | Resp#2   | ng/ml  | ng/ml     |
|-----------------------------|-----------------|---------|--------|---------|----------|--------|-----------|
| -----                       |                 |         |        |         |          |        |           |
| System Monitoring Compounds |                 |         |        |         |          |        |           |
| 1)                          | SA Tetrachlo... | 5.642   | 4.645  | 7848237 | 20601394 | 15.457 | 15.010    |
| 28)                         | SA Decachlor... | 11.636  | 10.392 | 6056267 | 12646101 | 13.561 | 12.321    |
| Target Compounds            |                 |         |        |         |          |        |           |
| 5)                          | MB Aldrin       | 0.000   | 6.498  | 0       | 770299   | N.D.   | 0.513 #   |
| 13)                         | MA Dieldrin     | 0.000   | 7.794f | 0       | 239518   | N.D.   | 0.188 #   |
| 14)                         | MA Endrin       | 0.000   | 8.067  | 0       | 673828   | N.D.   | 0.638 #   |
| 15)                         | B Endosulfa...  | 9.308   | 0.000  | 464205  | 0        | 1.056  | N.D. #    |
| 16)                         | A 4,4'-DDD      | 9.201   | 0.000  | 2040305 | 0        | 4.513  | N.D. #    |
| 17)                         | MA 4,4'-DDT     | 0.000   | 8.468f | 0       | 3159852  | N.D.   | 3.158 #   |
| 19)                         | B Endosulfa...  | 0.000   | 8.780  | 0       | 1484864  | N.D.   | 1.364 #   |
| 21)                         | B Endrin ke...  | 10.182  | 9.331f | 70794   | 2382988  | 0.138  | 2.137 #   |
| 22)                         | Mirex           | 10.669f | 9.525f | 278070  | 146169   | 0.689  | 0.151 #   |
| 27)                         | Chlordane-5     | 0.000   | 8.131  | 0       | 5193572  | N.D.   | 140.466 # |
| -----                       |                 |         |        |         |          |        |           |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL052522\  
Data File : PL075027.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 25 May 2022 17:59  
Operator : AR\AJ  
Sample : N2923-08  
Misc :  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: May 26 01:11:18 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL051122.M  
Quant Title : GC Extractables  
QLast Update : Sat May 14 02:37:15 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

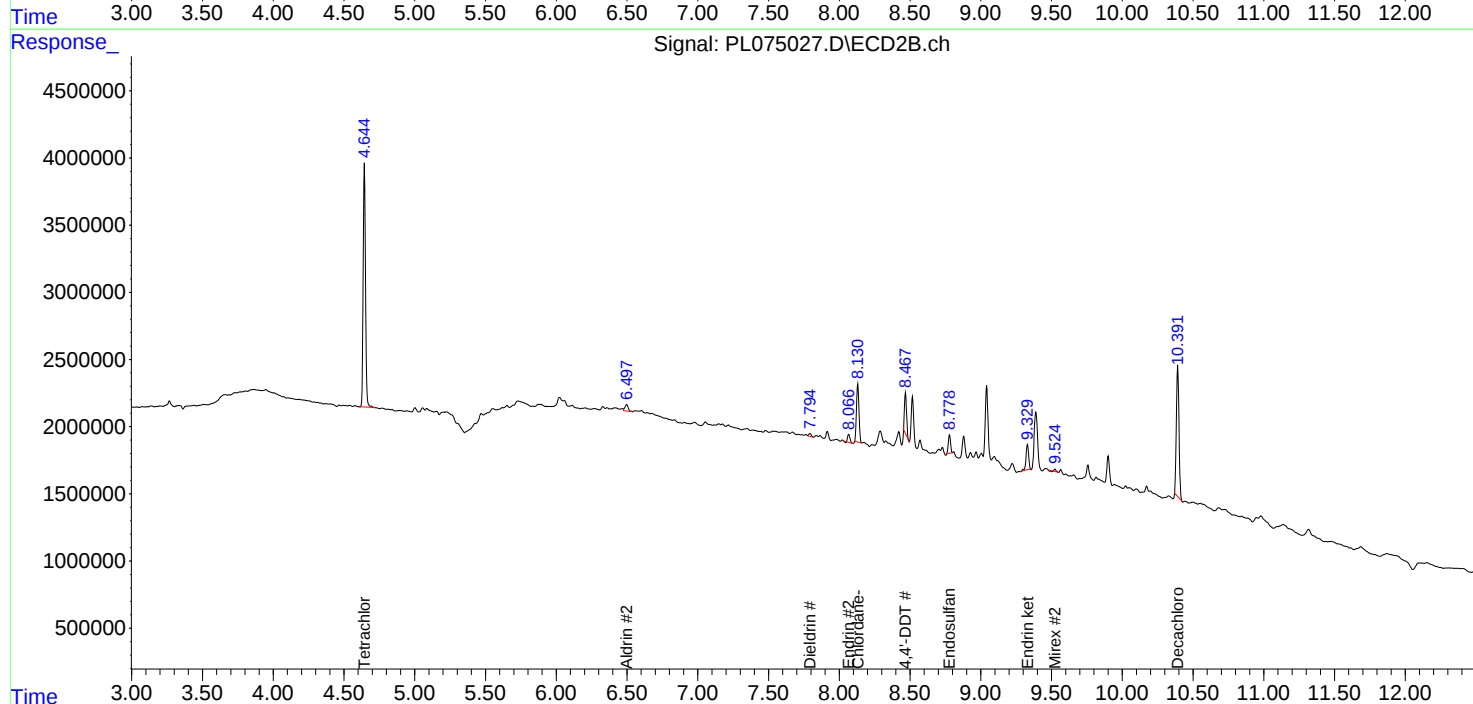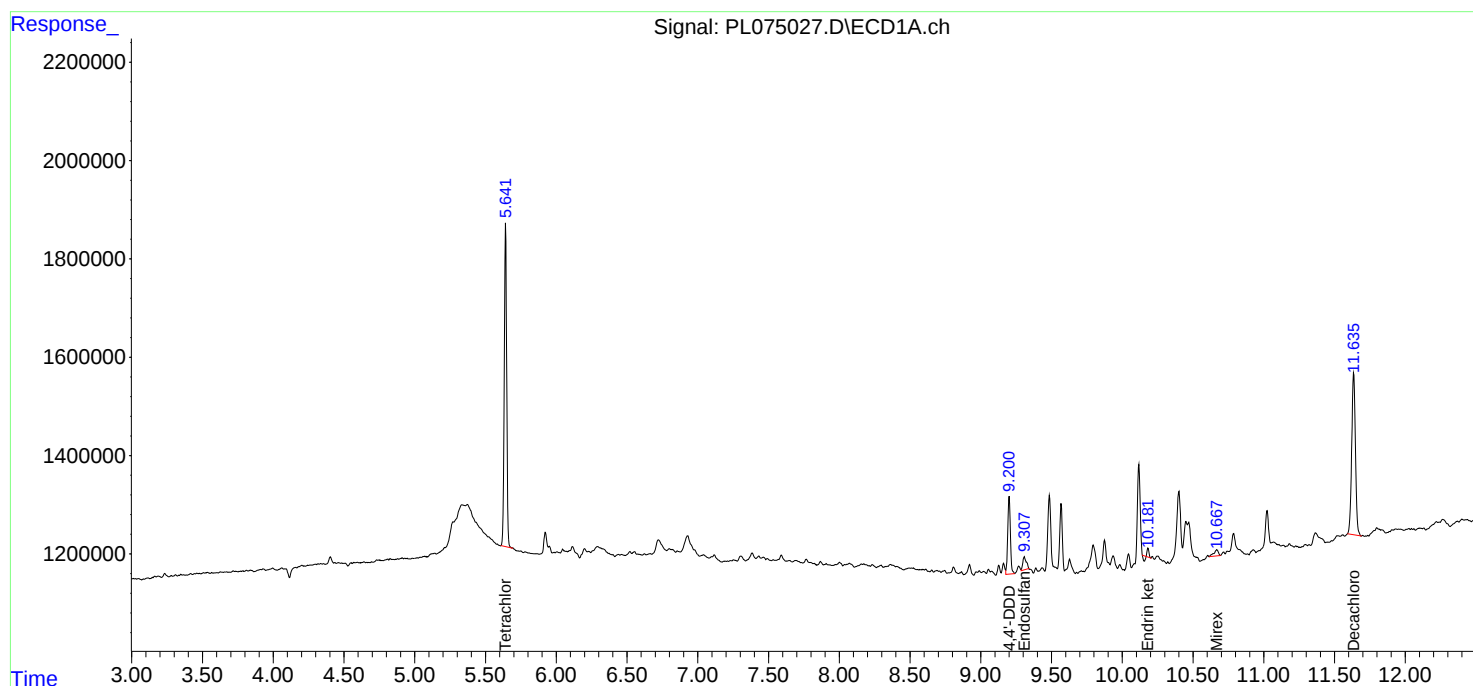


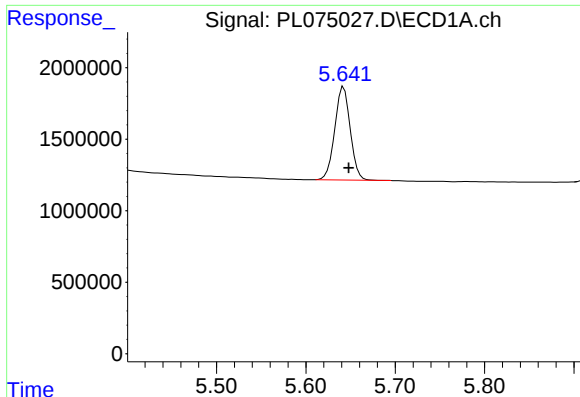

#1 Tetrachloro-m-xylene


R.T.: 5.642 min  
Delta R.T.: -0.006 min  
Response: 7848237  
Conc: 15.46 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

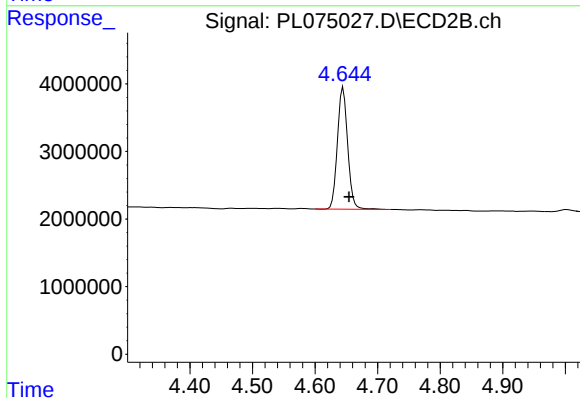


#1 Tetrachloro-m-xylene

R.T.: 4.645 min  
Delta R.T.: -0.009 min  
Response: 20601394  
Conc: 15.01 ng/ml

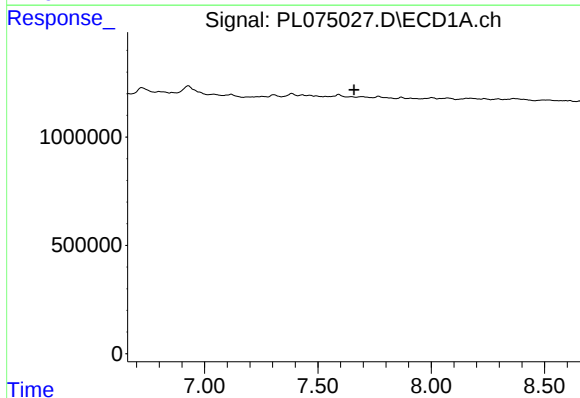


#5 Aldrin

R.T.: 0.000 min  
Exp R.T. : 7.660 min  
Response: 0  
Conc: N.D.

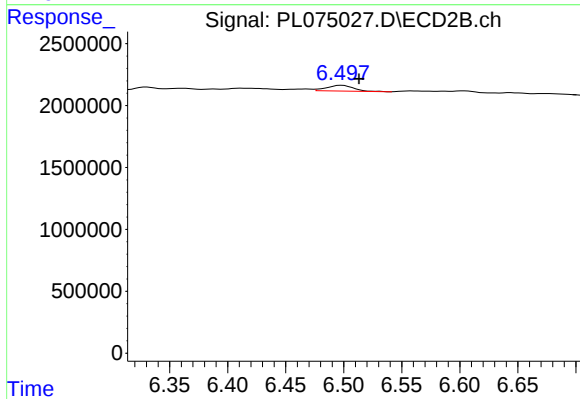

#5 Aldrin


R.T.: 6.498 min  
Delta R.T.: -0.015 min  
Response: 770299  
Conc: 0.51 ng/ml

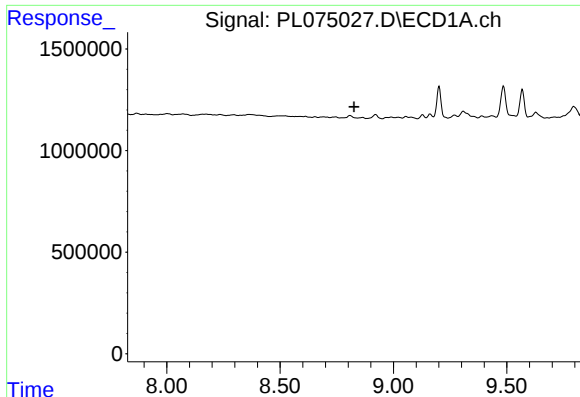

#13 Dieldrin


R.T.: 0.000 min  
Exp R.T. : 8.827 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :

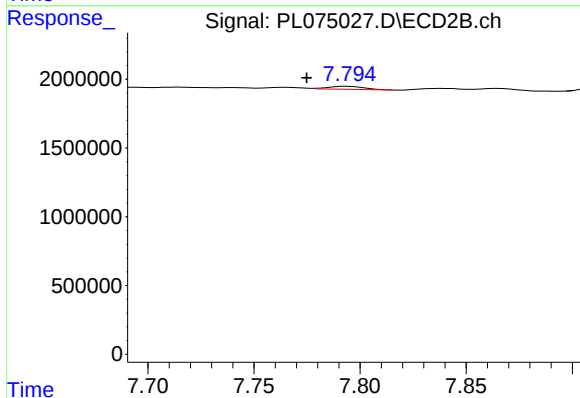


#13 Dieldrin

R.T.: 7.794 min  
Delta R.T.: 0.019 min  
Response: 239518  
Conc: 0.19 ng/ml

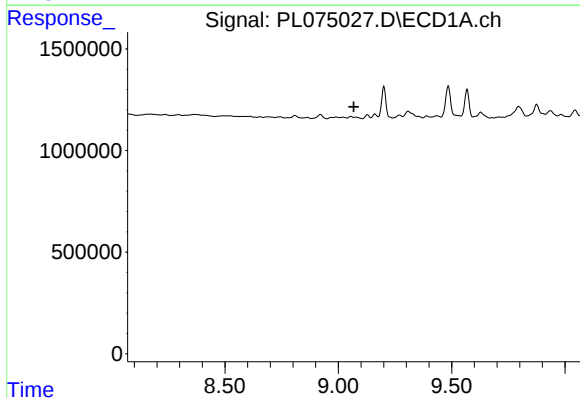


#14 Endrin

R.T.: 0.000 min  
Exp R.T. : 9.068 min  
Response: 0  
Conc: N.D.

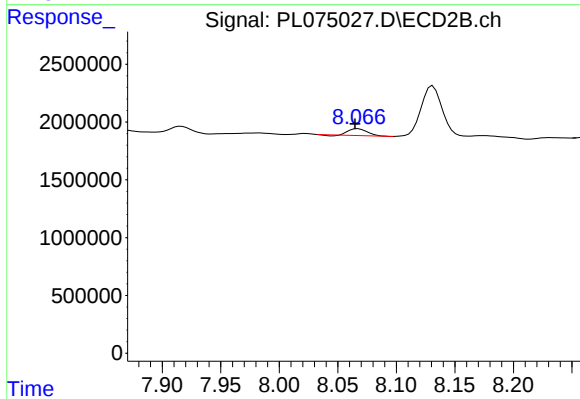

#14 Endrin


R.T.: 8.067 min  
Delta R.T.: 0.002 min  
Response: 673828  
Conc: 0.64 ng/ml

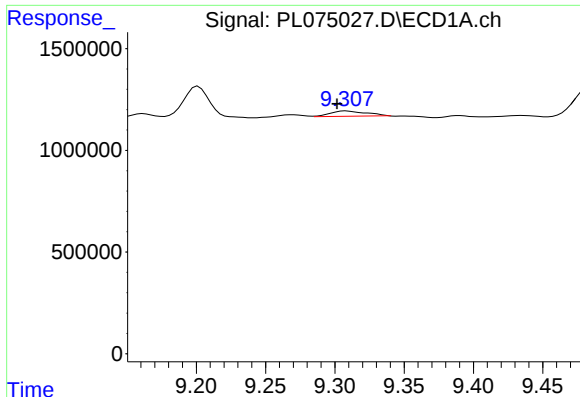

#15 Endosulfan II


R.T.: 9.308 min  
Delta R.T.: 0.007 min  
Response: 464205  
Conc: 1.06 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

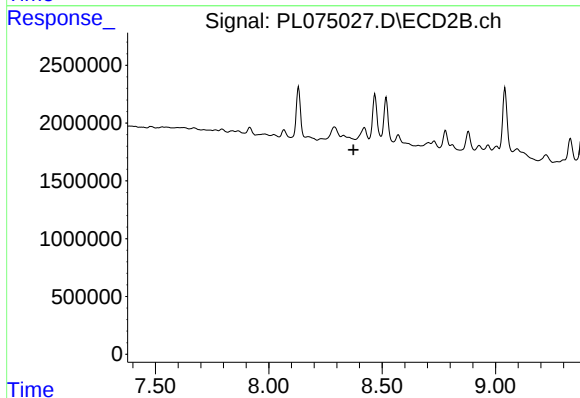


#15 Endosulfan II

R.T.: 0.000 min  
Exp R.T. : 8.374 min  
Response: 0  
Conc: N.D.

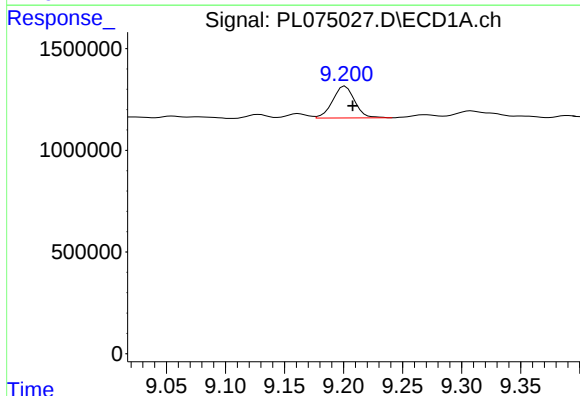


#16 4,4'-DDD

R.T.: 9.201 min  
Delta R.T.: -0.006 min  
Response: 2040305  
Conc: 4.51 ng/ml

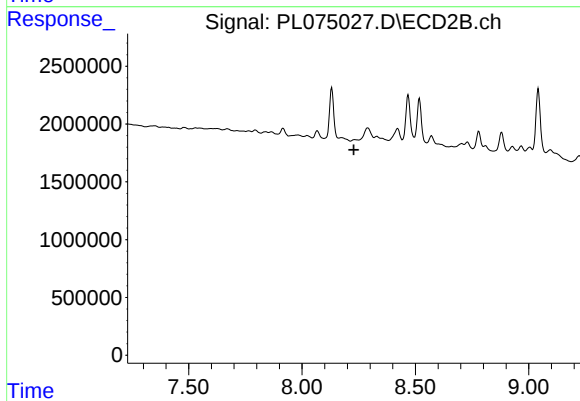

#16 4,4'-DDD


R.T.: 0.000 min  
Exp R.T. : 8.229 min  
Response: 0  
Conc: N.D.

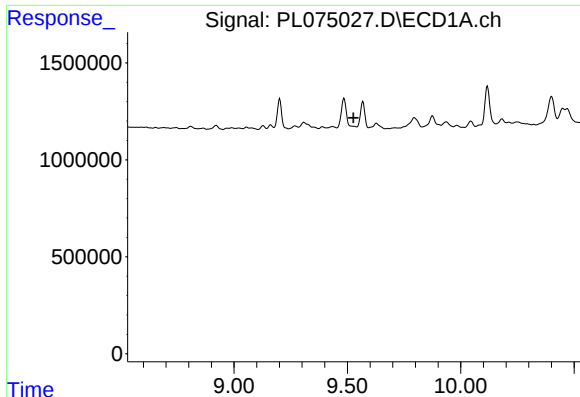

#17 4,4'-DDT


R.T.: 0.000 min  
Exp R.T.: 9.527 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :

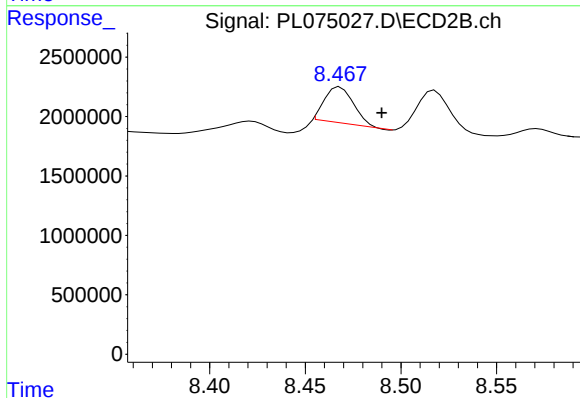


#17 4,4'-DDT

R.T.: 8.468 min  
Delta R.T.: -0.022 min  
Response: 3159852  
Conc: 3.16 ng/ml

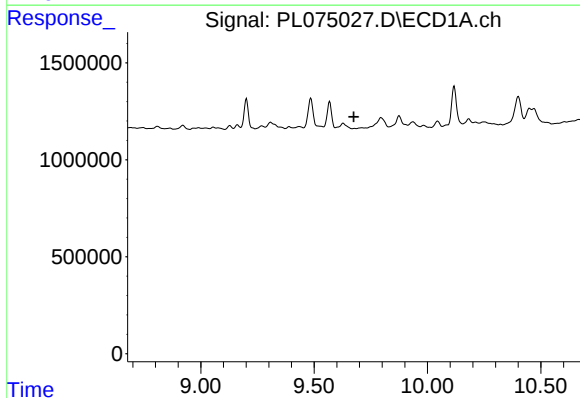


#19 Endosulfan Sulfate

R.T.: 0.000 min  
Exp R.T.: 9.675 min  
Response: 0  
Conc: N.D.

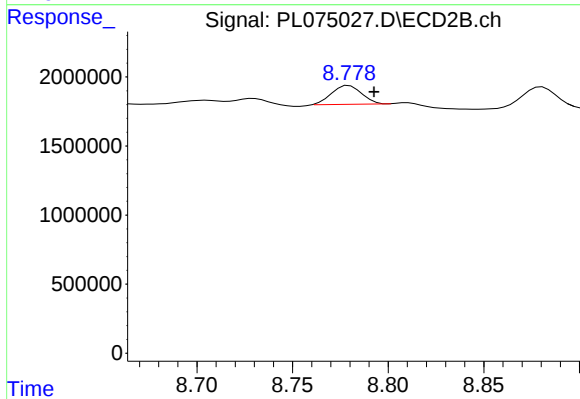

#19 Endosulfan Sulfate


R.T.: 8.780 min  
Delta R.T.: -0.013 min  
Response: 1484864  
Conc: 1.36 ng/ml

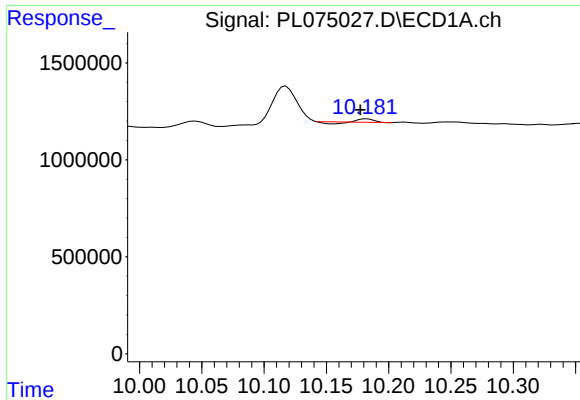

#21 Endrin ketone


R.T.: 10.182 min  
Delta R.T.: 0.005 min  
Response: 70794  
Conc: 0.14 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

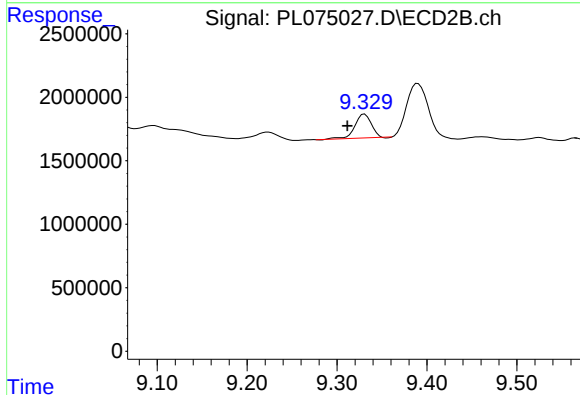


#21 Endrin ketone

R.T.: 9.331 min  
Delta R.T.: 0.019 min  
Response: 2382988  
Conc: 2.14 ng/ml

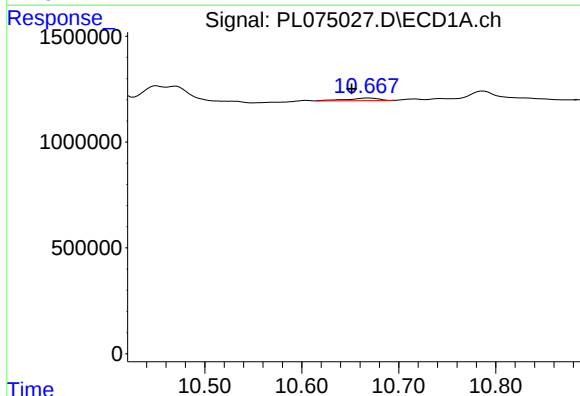


#22 Mirex

R.T.: 10.669 min  
Delta R.T.: 0.017 min  
Response: 278070  
Conc: 0.69 ng/ml

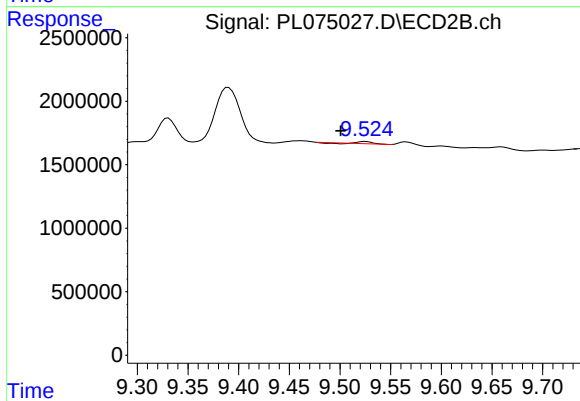

#22 Mirex


R.T.: 9.525 min  
Delta R.T.: 0.025 min  
Response: 146169  
Conc: 0.15 ng/ml

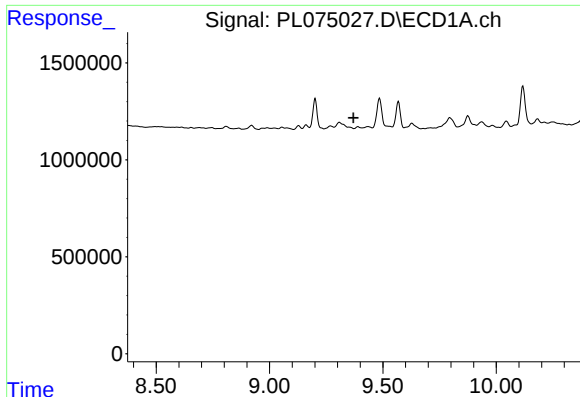

#27 Chlordane-5


R.T.: 0.000 min  
Exp R.T.: 9.371 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :

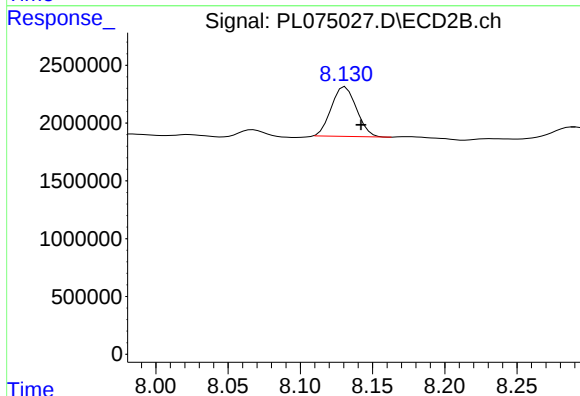


#27 Chlordane-5

R.T.: 8.131 min  
Delta R.T.: -0.011 min  
Response: 5193572  
Conc: 140.47 ng/ml

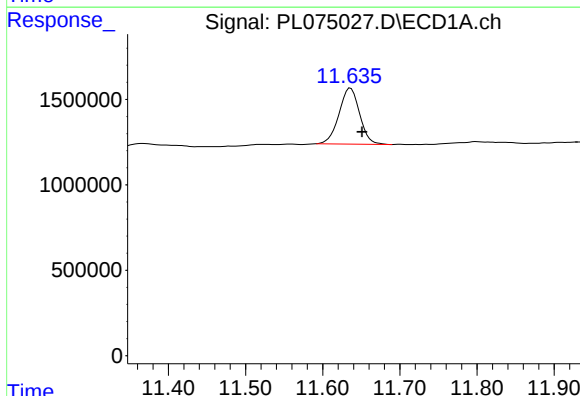

#28 Decachlorobiphenyl

R.T.: 11.636 min  
Delta R.T.: -0.015 min  
Response: 6056267  
Conc: 13.56 ng/ml

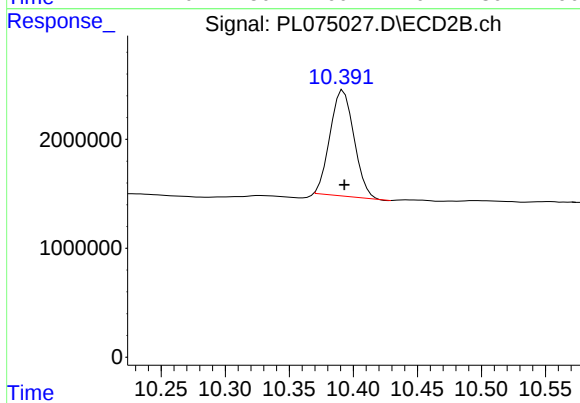

#28 Decachlorobiphenyl

R.T.: 10.392 min  
Delta R.T.: 0.000 min  
Response: 12646101  
Conc: 12.32 ng/ml