

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052522\
 Data File : PL075031.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 May 2022 19:06
 Operator : AR\AJ
 Sample : N2923-20
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 01:12:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.642	4.645	3957722	10508928	7.795	7.657
28)	SA Decachlor...	11.636f	10.392	5926895	11805324	13.272	11.502
Target Compounds							
10)	B gamma-Chl...	0.000	7.386f	0	310742	N.D.	0.224 #
13)	MA Dieldrin	8.810f	7.794f	1426315	2905665	2.714	2.281
14)	MA Endrin	9.053	8.068	291383	4199391	0.706	3.976 #
15)	B Endosulfa...	9.329f	8.359f	893003	1229006	2.031	1.088 #
16)	A 4,4'-DDD	9.201	0.000	11535911	0	25.515	N.D. #
17)	MA 4,4'-DDT	0.000	8.469f	0	16237163	N.D.	16.229 #
19)	B Endosulfa...	0.000	8.780	0	15060609	N.D.	13.836 #
21)	B Endrin ke...	0.000	9.331f	0	15895069	N.D.	14.257 #
22)	Mirex	10.659	0.000	191603	0	0.475	N.D. #
25)	Chlordane-3	0.000	7.386f	0	310742	N.D.	2.394 #
27)	Chlordane-5	0.000	8.132	0	26410381	N.D.	714.300 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052522\
Data File : PL075031.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 May 2022 19:06
Operator : AR\AJ
Sample : N2923-20
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 01:12:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

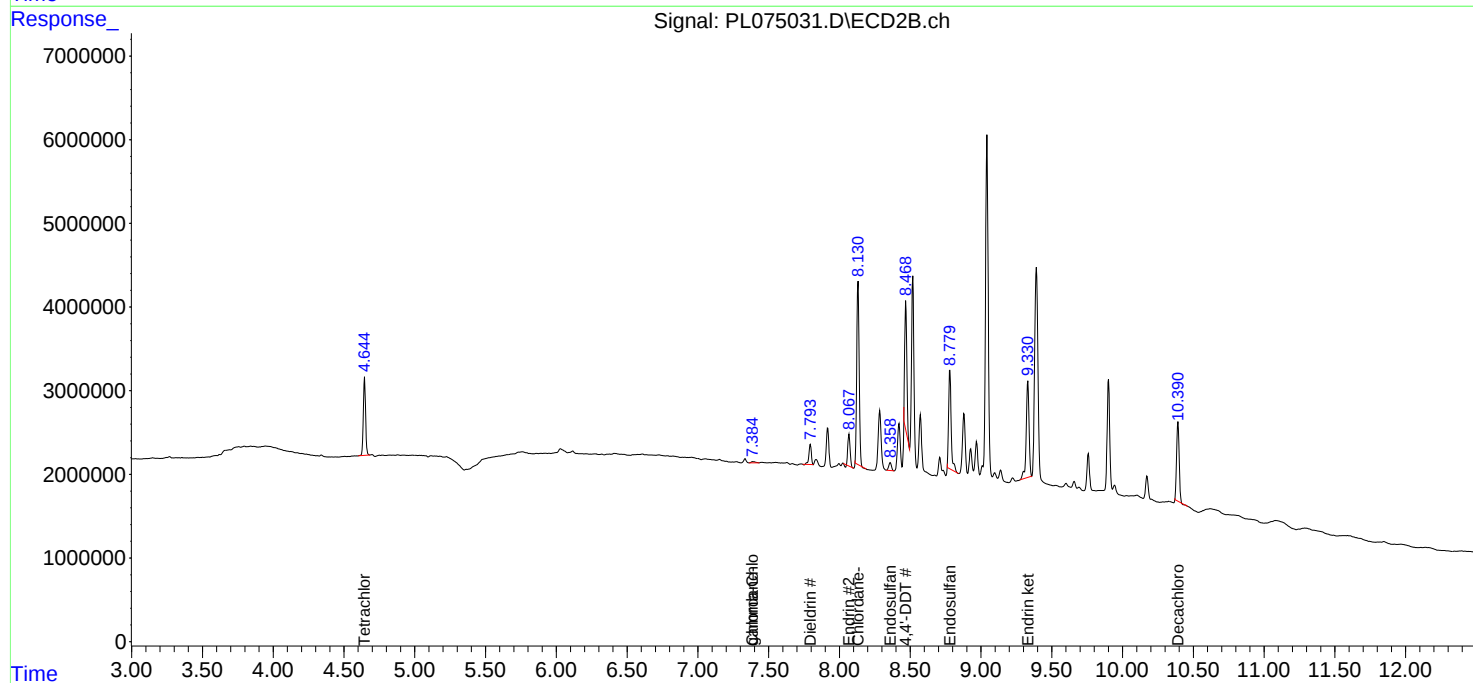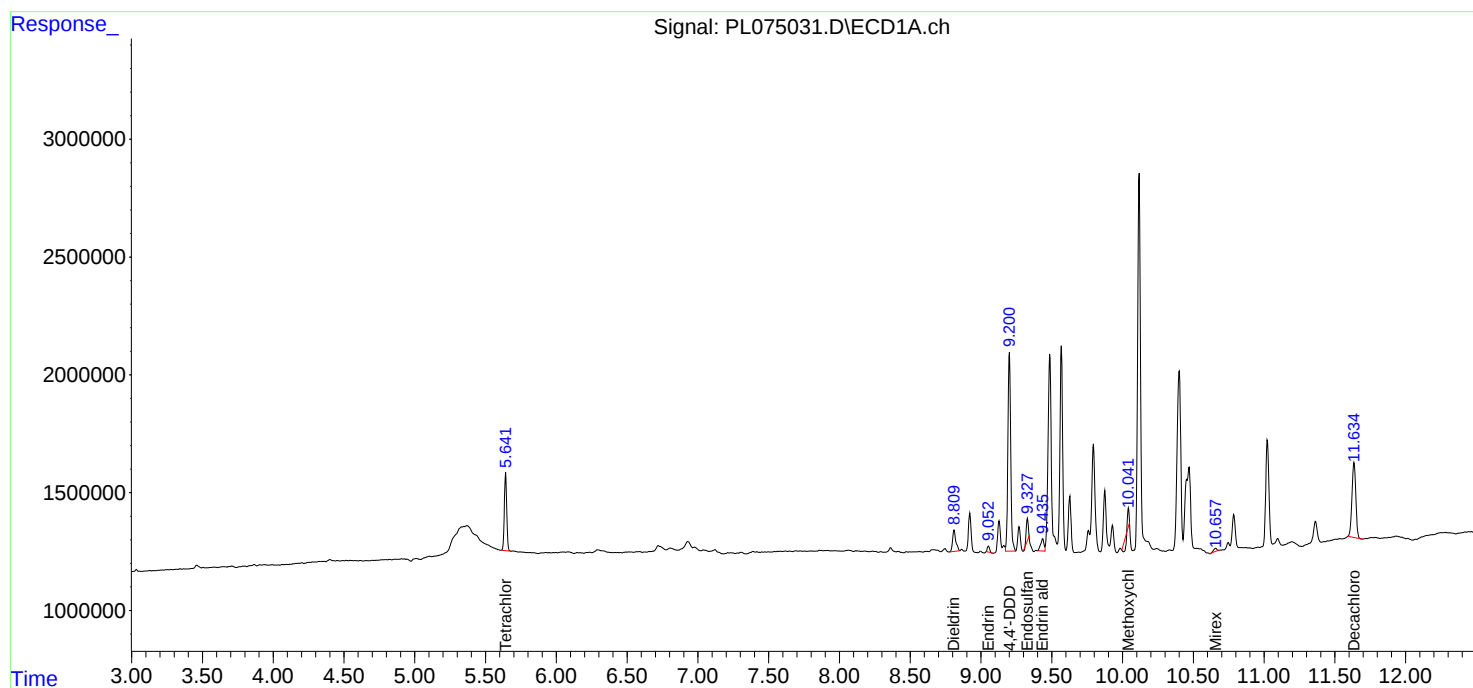


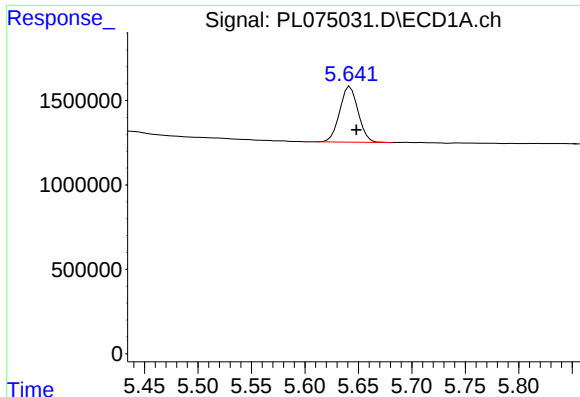

#1 Tetrachloro-m-xylene


R.T.: 5.642 min
Delta R.T.: -0.006 min
Response: 3957722
Conc: 7.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

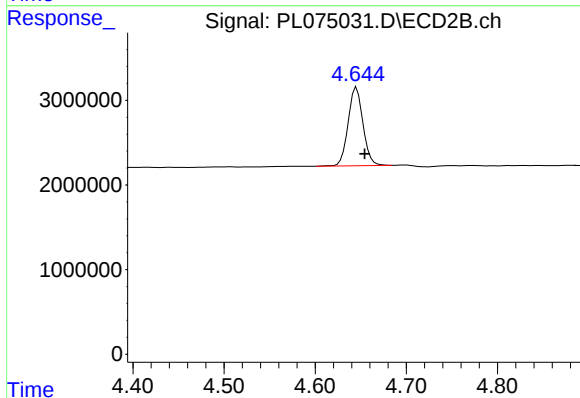


#1 Tetrachloro-m-xylene

R.T.: 4.645 min
Delta R.T.: -0.009 min
Response: 10508928
Conc: 7.66 ng/ml

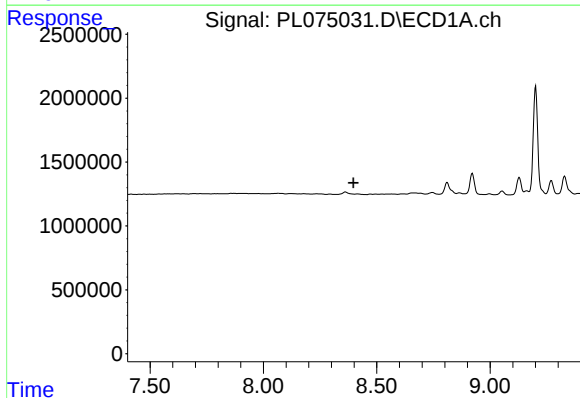


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.398 min
Response: 0
Conc: N.D.

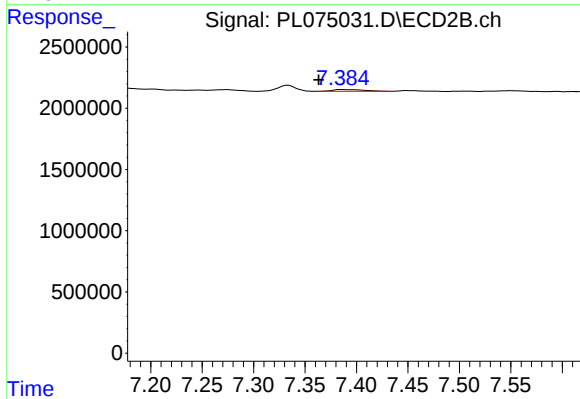

#10 gamma-Chlordane


R.T.: 7.386 min
Delta R.T.: 0.022 min
Response: 310742
Conc: 0.22 ng/ml

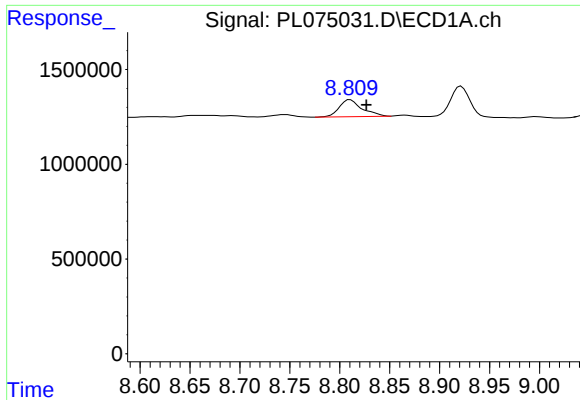

#13 Dieldrin


R.T.: 8.810 min
Delta R.T.: -0.016 min
Response: 1426315
Conc: 2.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

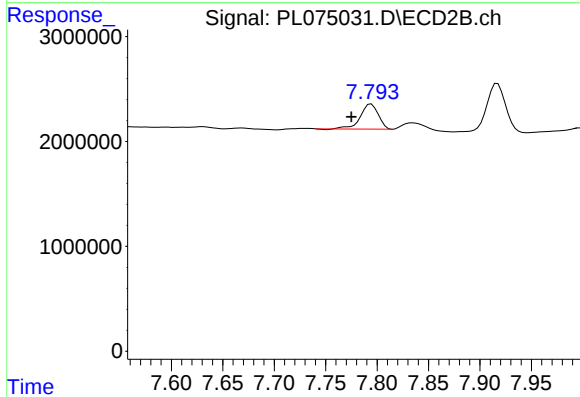


#13 Dieldrin

R.T.: 7.794 min
Delta R.T.: 0.019 min
Response: 2905665
Conc: 2.28 ng/ml

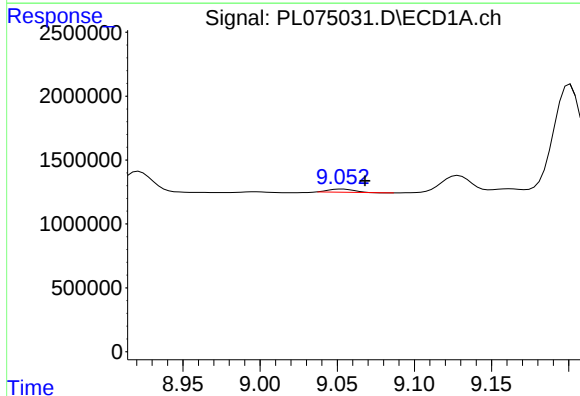


#14 Endrin

R.T.: 9.053 min
Delta R.T.: -0.015 min
Response: 291383
Conc: 0.71 ng/ml

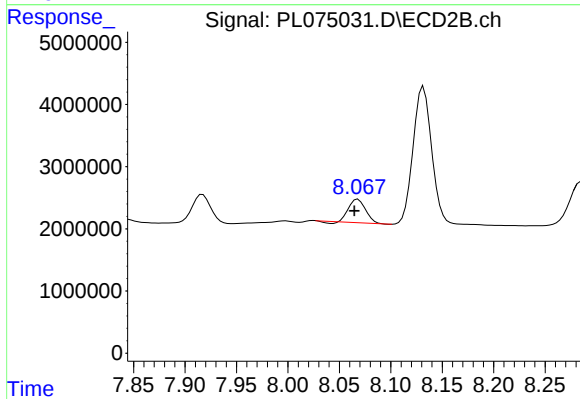

#14 Endrin


R.T.: 8.068 min
Delta R.T.: 0.003 min
Response: 4199391
Conc: 3.98 ng/ml

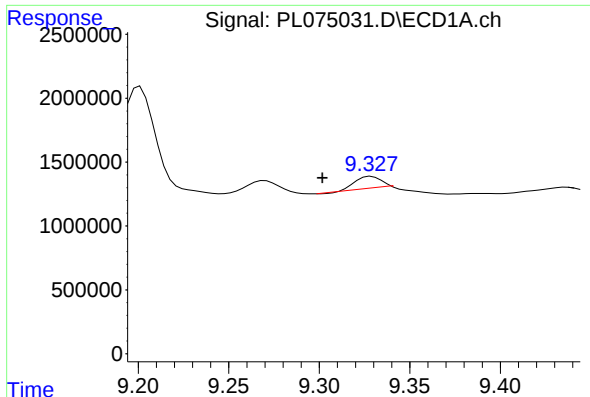

#15 Endosulfan II


R.T.: 9.329 min
Delta R.T.: 0.027 min
Response: 893003
Conc: 2.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

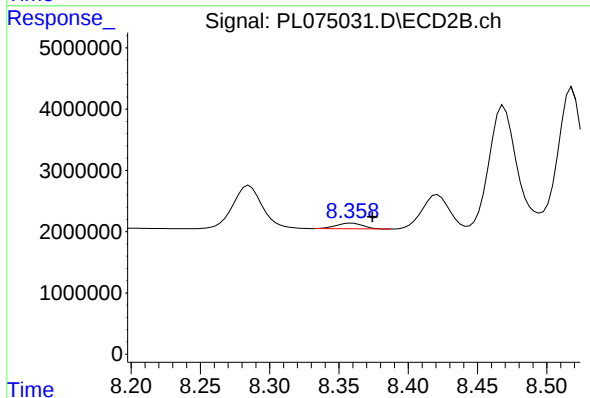


#15 Endosulfan II

R.T.: 8.359 min
Delta R.T.: -0.015 min
Response: 1229006
Conc: 1.09 ng/ml

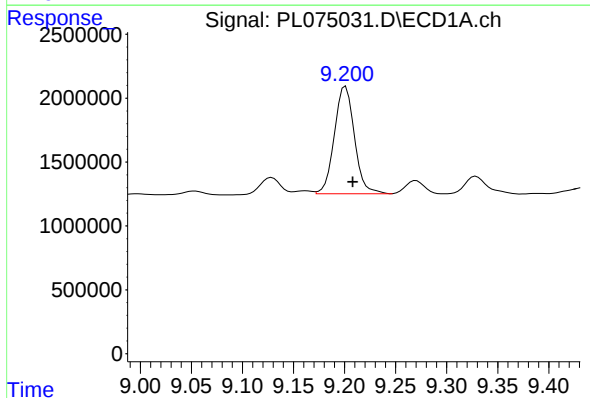


#16 4,4'-DDD

R.T.: 9.201 min
Delta R.T.: -0.007 min
Response: 11535911
Conc: 25.51 ng/ml

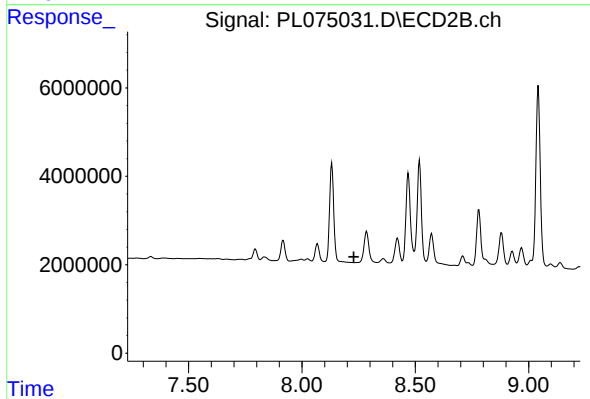

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.229 min
Response: 0
Conc: N.D.

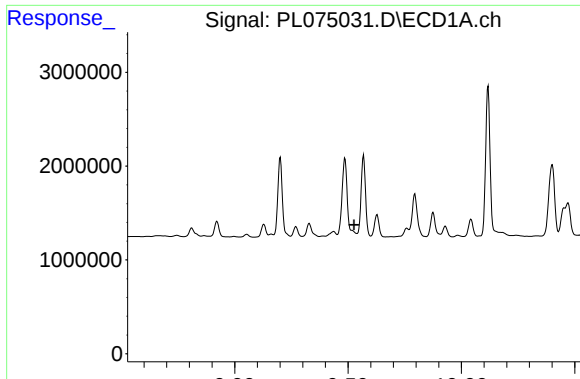

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 9.527 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

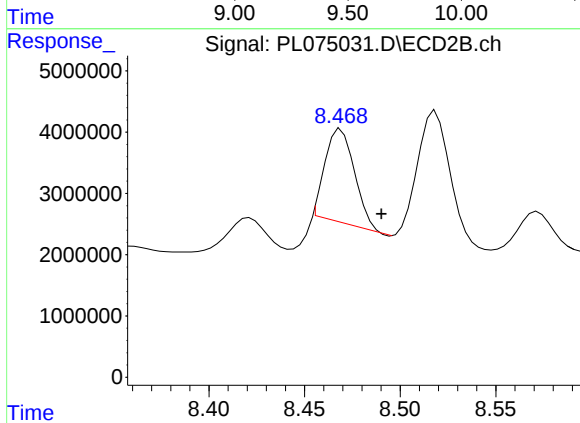


#17 4,4'-DDT

R.T.: 8.469 min
Delta R.T.: -0.021 min
Response: 16237163
Conc: 16.23 ng/ml

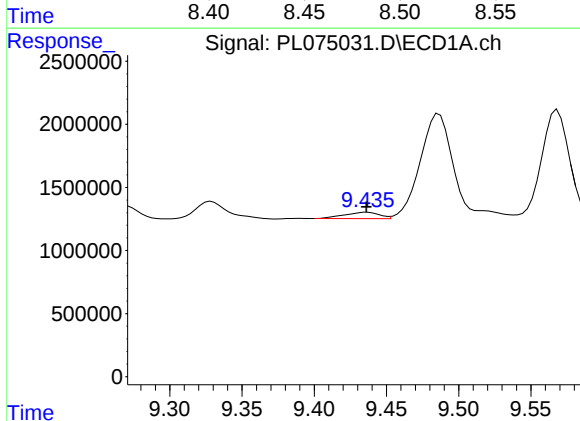


#18 Endrin aldehyde

R.T.: 9.437 min
Delta R.T.: 0.000 min
Response: 861593
Conc: 2.43 ng/ml

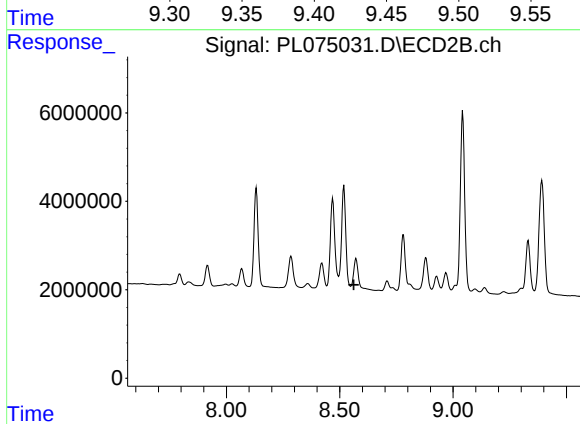

#18 Endrin aldehyde


R.T.: 8.572 min
Delta R.T.: 0.009 min
Response: -5212587
Conc: N.D.

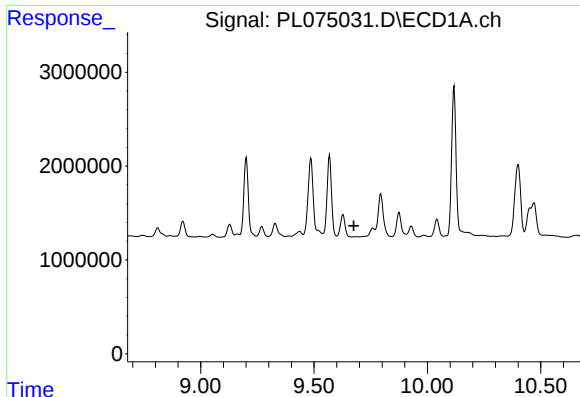

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 9.675 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

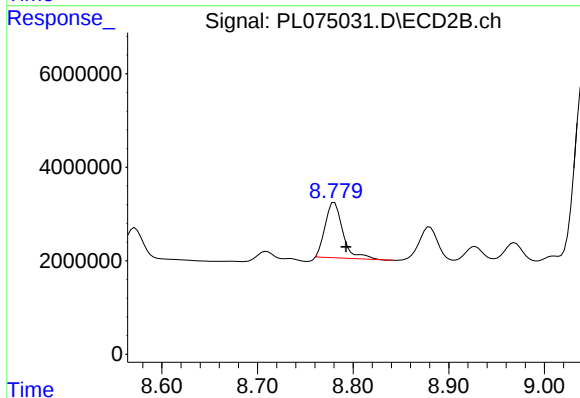


#19 Endosulfan Sulfate

R.T.: 8.780 min
Delta R.T.: -0.012 min
Response: 15060609
Conc: 13.84 ng/ml

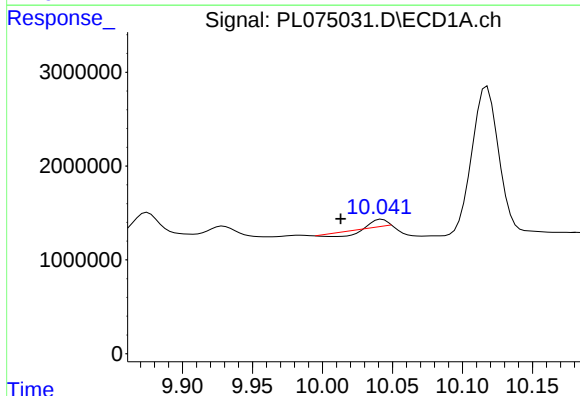


#20 Methoxychlor

R.T.: 10.042 min
Delta R.T.: 0.029 min
Response: 81501
Conc: 0.33 ng/ml

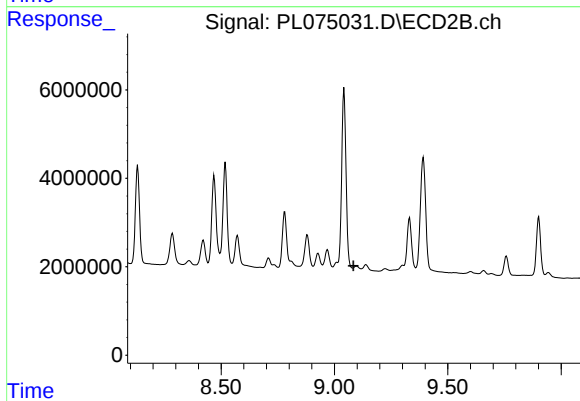

#20 Methoxychlor


R.T.: 9.097 min
Delta R.T.: 0.013 min
Response: -19153340
Conc: N.D.

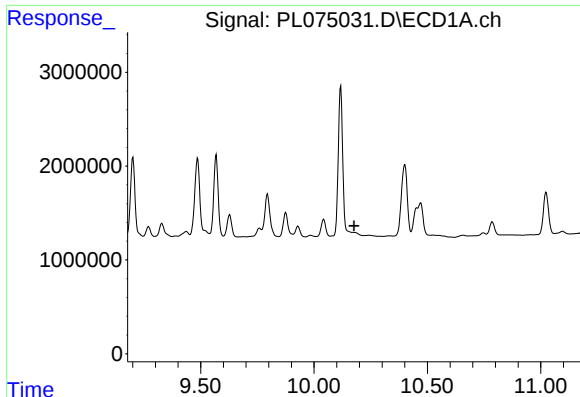

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 10.177 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

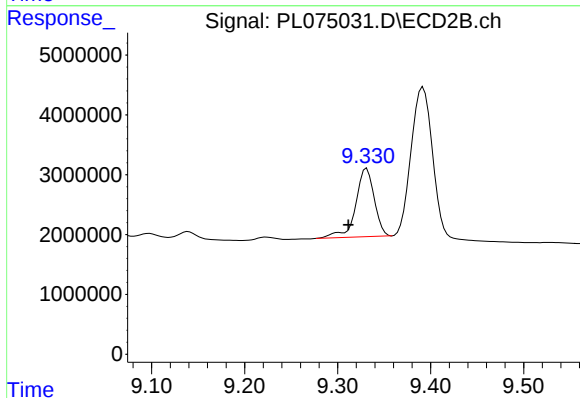


#21 Endrin ketone

R.T.: 9.331 min
Delta R.T.: 0.020 min
Response: 15895069
Conc: 14.26 ng/ml

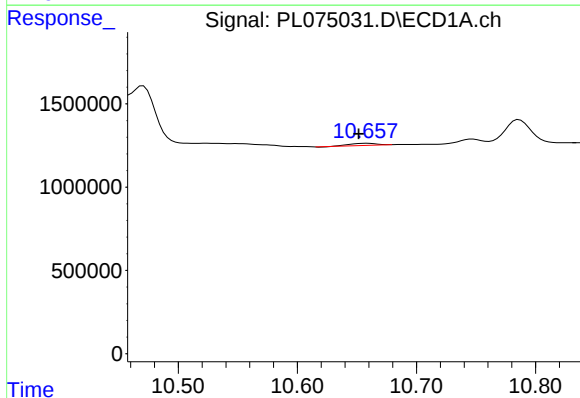


#22 Mirex

R.T.: 10.659 min
Delta R.T.: 0.007 min
Response: 191603
Conc: 0.47 ng/ml

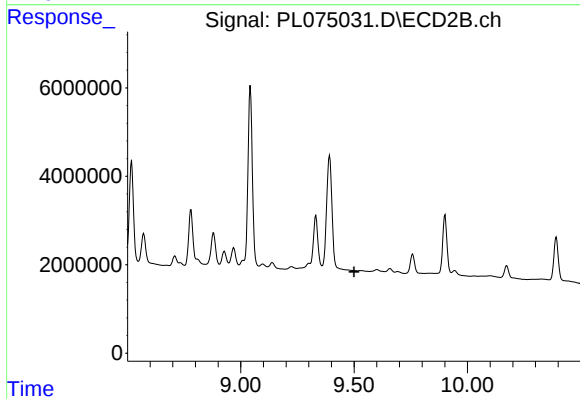

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 9.501 min
Response: 0
Conc: N.D.

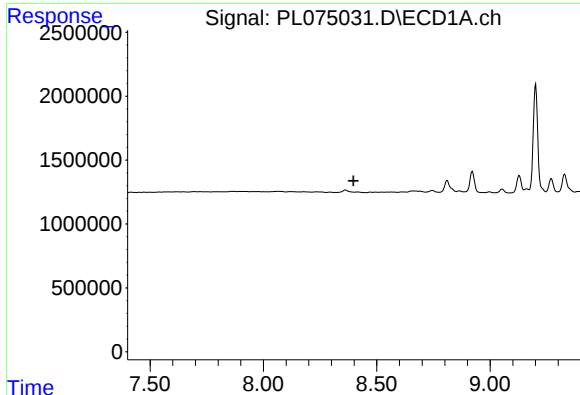

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

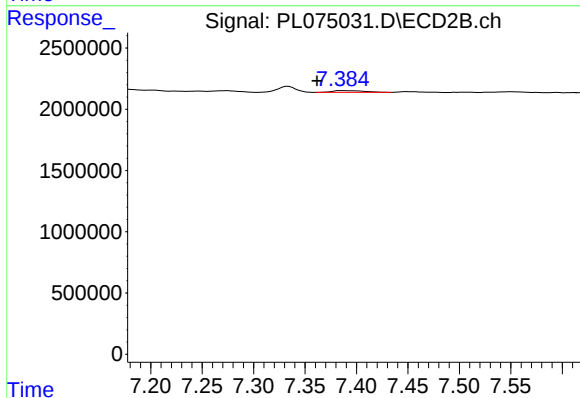


#25 Chlordane-3

R.T.: 7.386 min
Delta R.T.: 0.024 min
Response: 310742
Conc: 2.39 ng/ml

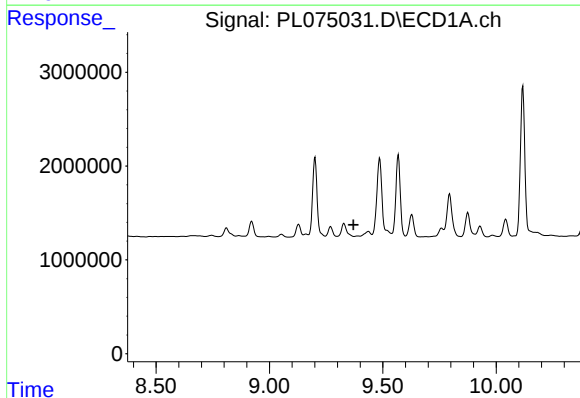


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 9.371 min
Response: 0
Conc: N.D.

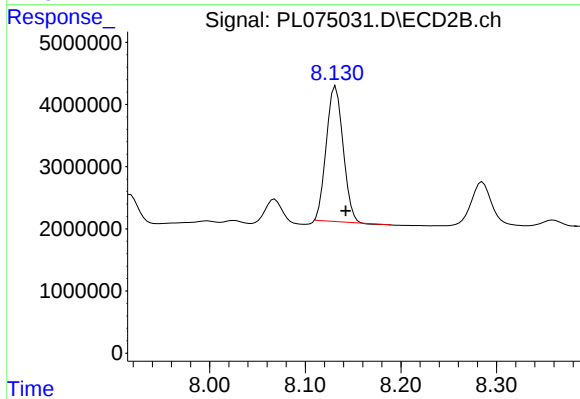

#27 Chlordane-5


R.T.: 8.132 min
Delta R.T.: -0.010 min
Response: 26410381
Conc: 714.30 ng/ml

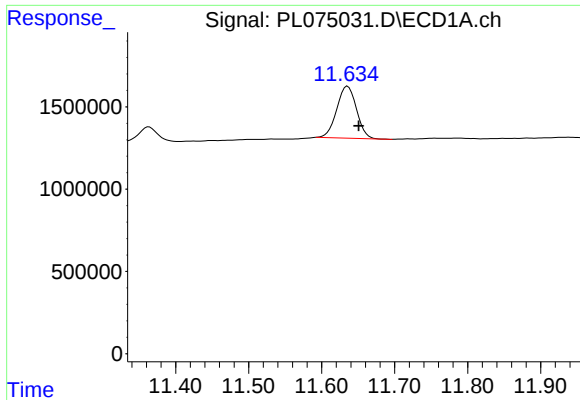

#28 Decachlorobiphenyl

R.T.: 11.636 min
Delta R.T.: -0.015 min
Response: 5926895
Conc: 13.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

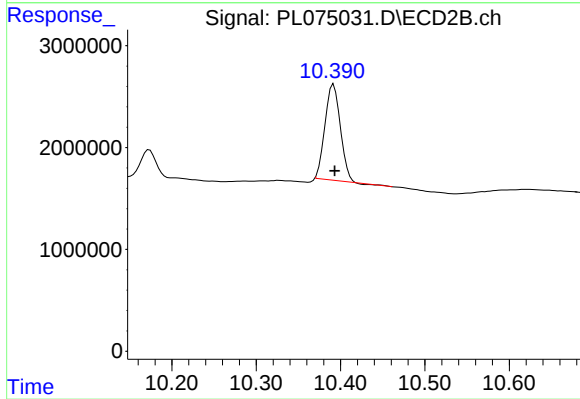

#28 Decachlorobiphenyl

R.T.: 10.392 min
Delta R.T.: -0.001 min
Response: 11805324
Conc: 11.50 ng/ml