

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052522\
 Data File : PL075037.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 May 2022 20:45
 Operator : AR\AJ
 Sample : N2927-04
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 01:14:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.642	4.646	11338056	29649069	22.331	21.602
28)	SA Decachlor...	11.634f	10.393	7911654	16171755	17.716	15.756
Target Compounds							
10)	B gamma-Chl...	0.000	7.335f	0	437550	N.D.	0.316 #
13)	MA Dieldrin	8.810f	7.769	568544	285006	1.082	0.224 #
14)	MA Endrin	0.000	8.069	0	2323503	N.D.	2.200 #
15)	B Endosulfa...	9.330f	8.358f	362517	224678	0.825	0.199 #
16)	A 4,4'-DDD	9.201	0.000	3123819	0	6.909	N.D. #
17)	MA 4,4'-DDT	0.000	8.469f	0	8628699	N.D.	8.624 #
19)	B Endosulfa...	0.000	8.780	0	7474508	N.D.	6.867 #
20)	A Methoxychlor	10.042f	0.000	529650	0	2.163	N.D. #
21)	B Endrin ke...	10.183	9.331f	134600	5741326	0.262	5.150 #
25)	Chlordane-3	0.000	7.335f	0	437550	N.D.	3.371 #
27)	Chlordane-5	0.000	8.132	0	7460784	N.D.	201.786 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052522\
Data File : PL075037.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 May 2022 20:45
Operator : AR\AJ
Sample : N2927-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 01:14:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

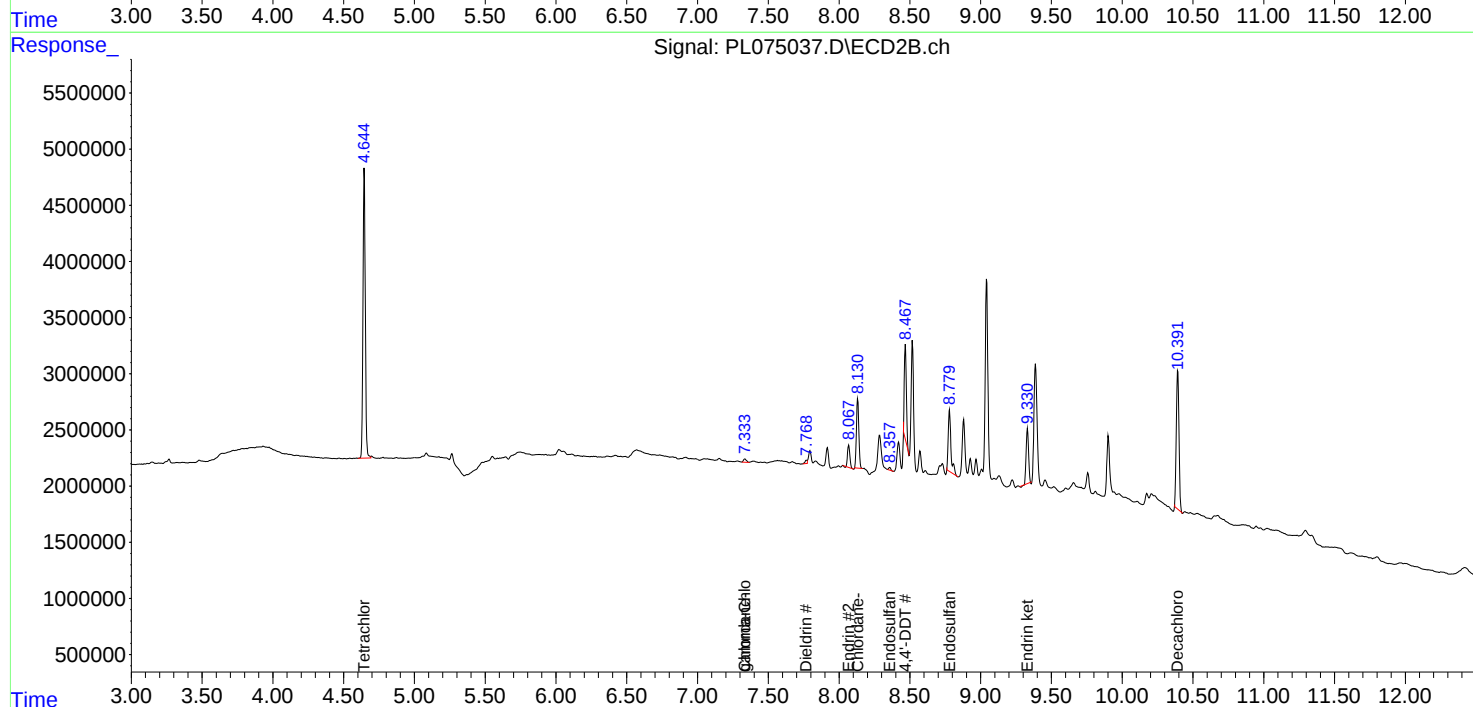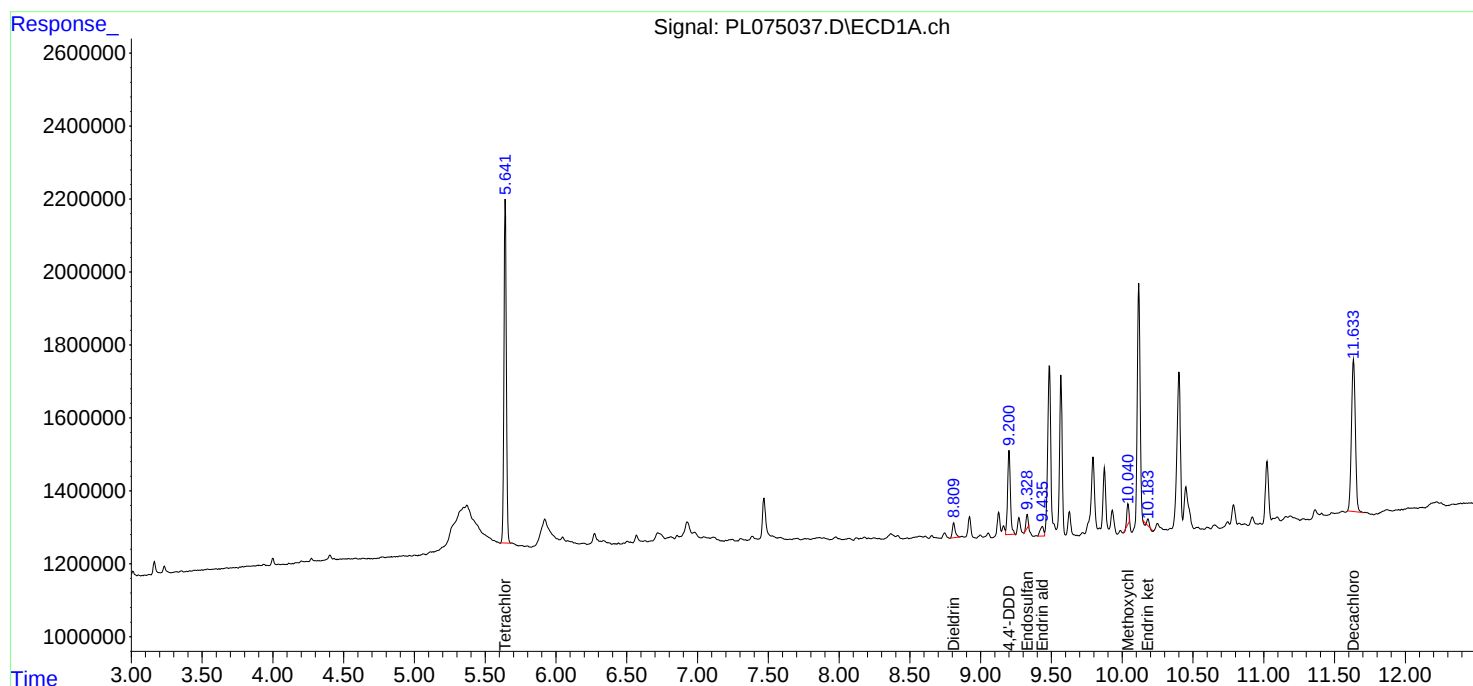


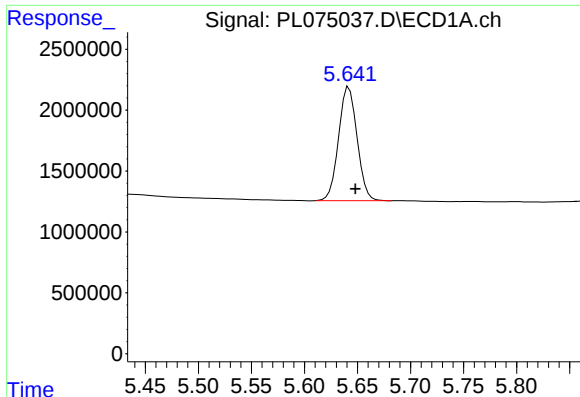

#1 Tetrachloro-m-xylene


R.T.: 5.642 min
Delta R.T.: -0.006 min
Response: 11338056
Conc: 22.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

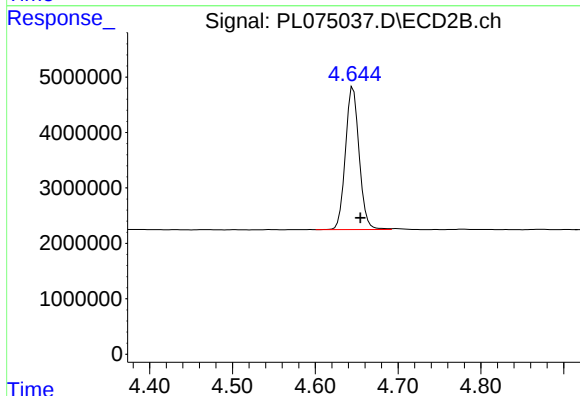


#1 Tetrachloro-m-xylene

R.T.: 4.646 min
Delta R.T.: -0.009 min
Response: 29649069
Conc: 21.60 ng/ml

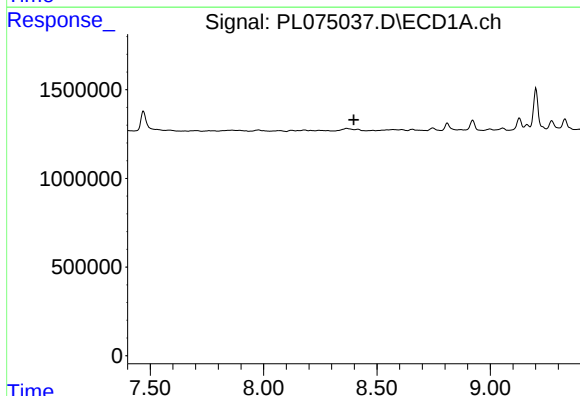


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.398 min
Response: 0
Conc: N.D.

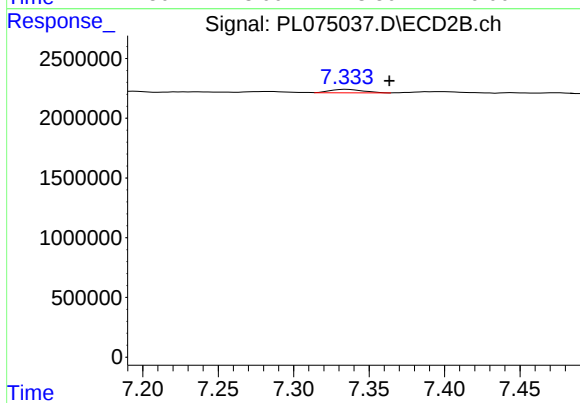

#10 gamma-Chlordane


R.T.: 7.335 min
Delta R.T.: -0.029 min
Response: 437550
Conc: 0.32 ng/ml

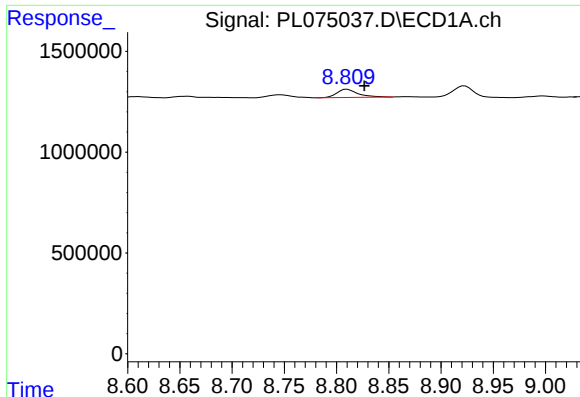

#13 Dieldrin


R.T.: 8.810 min
Delta R.T.: -0.016 min
Response: 568544
Conc: 1.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

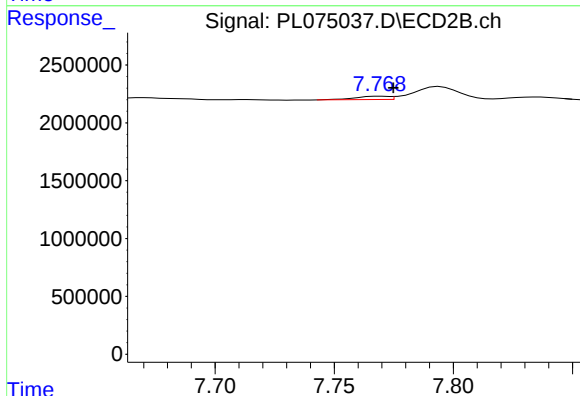


#13 Dieldrin

R.T.: 7.769 min
Delta R.T.: -0.006 min
Response: 285006
Conc: 0.22 ng/ml

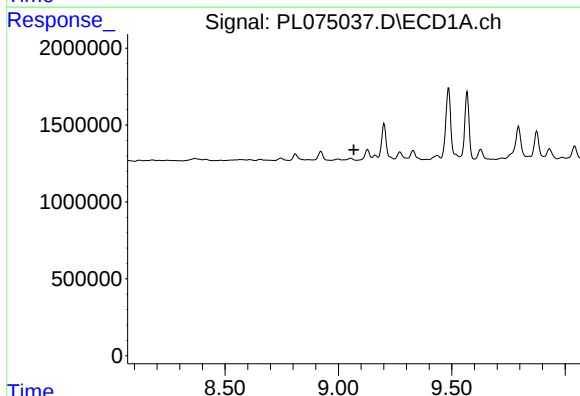


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 9.068 min
Response: 0
Conc: N.D.

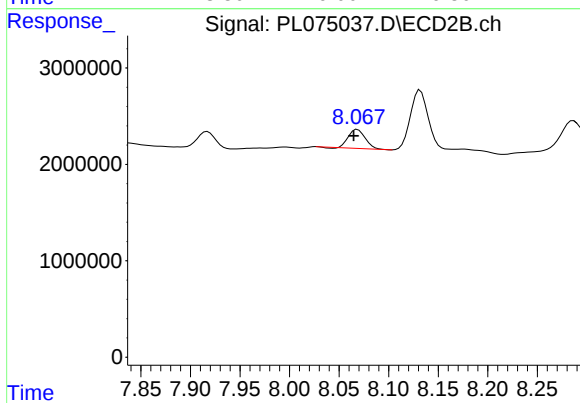

#14 Endrin


R.T.: 8.069 min
Delta R.T.: 0.004 min
Response: 2323503
Conc: 2.20 ng/ml

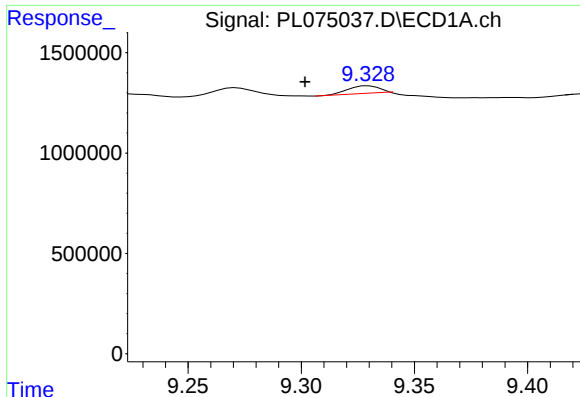

#15 Endosulfan II


R.T.: 9.330 min
Delta R.T.: 0.028 min
Response: 362517
Conc: 0.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

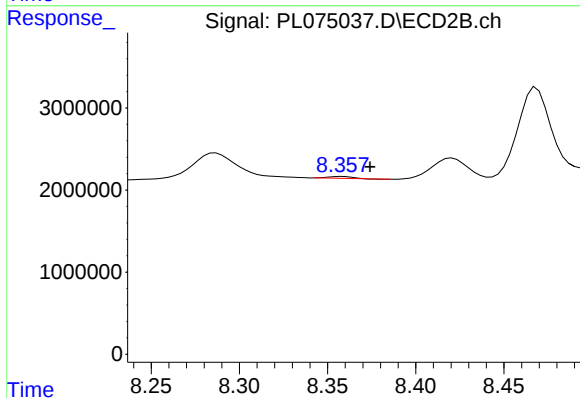


#15 Endosulfan II

R.T.: 8.358 min
Delta R.T.: -0.016 min
Response: 224678
Conc: 0.20 ng/ml

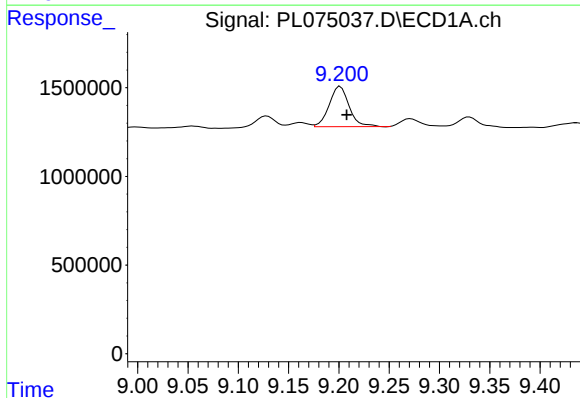


#16 4,4'-DDD

R.T.: 9.201 min
Delta R.T.: -0.006 min
Response: 3123819
Conc: 6.91 ng/ml

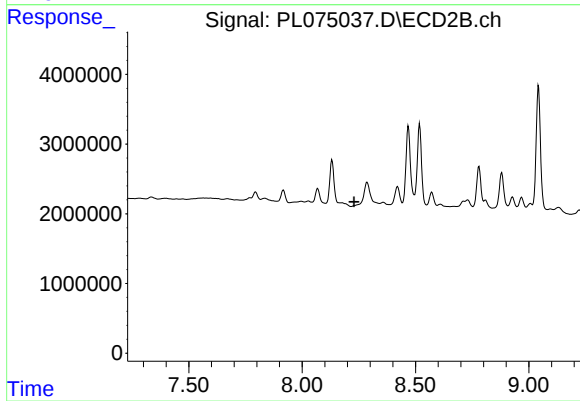

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.229 min
Response: 0
Conc: N.D.

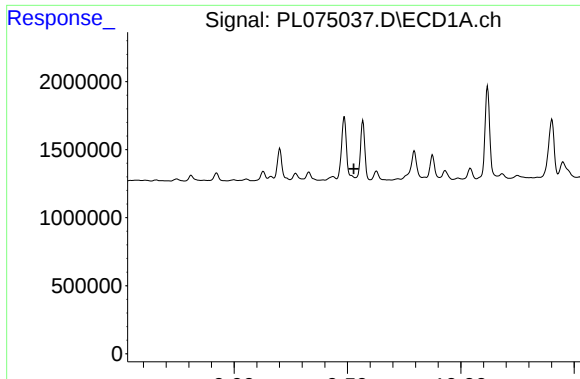

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 9.527 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

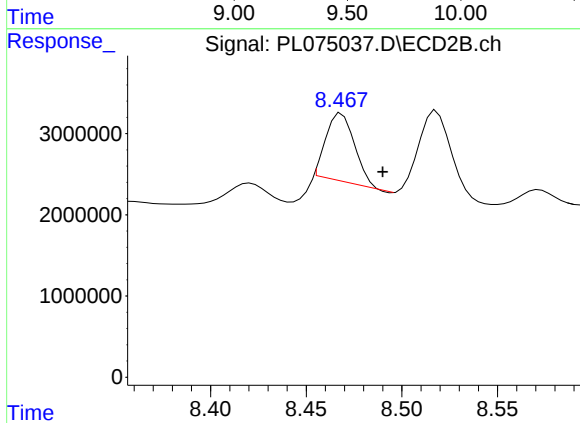


#17 4,4'-DDT

R.T.: 8.469 min
Delta R.T.: -0.021 min
Response: 8628699
Conc: 8.62 ng/ml

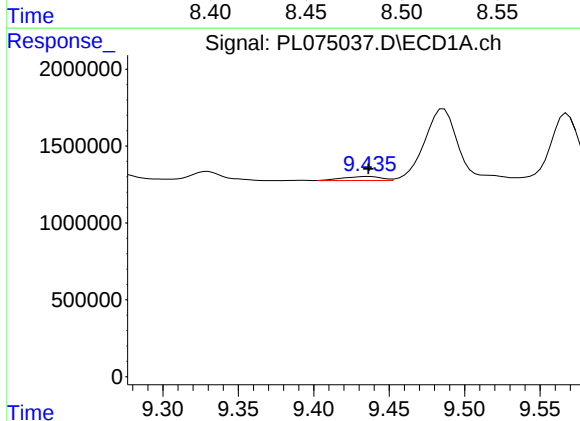


#18 Endrin aldehyde

R.T.: 9.437 min
Delta R.T.: 0.000 min
Response: 464412
Conc: 1.31 ng/ml

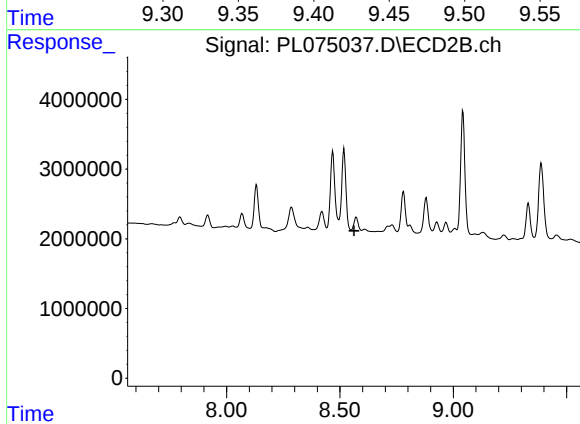

#18 Endrin aldehyde


R.T.: 8.572 min
Delta R.T.: 0.009 min
Response: -1418786
Conc: N.D.

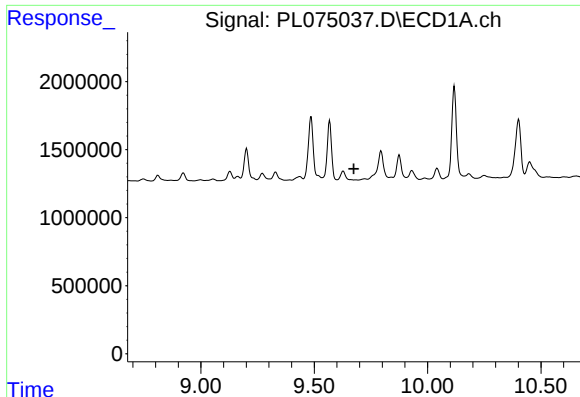

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 9.675 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

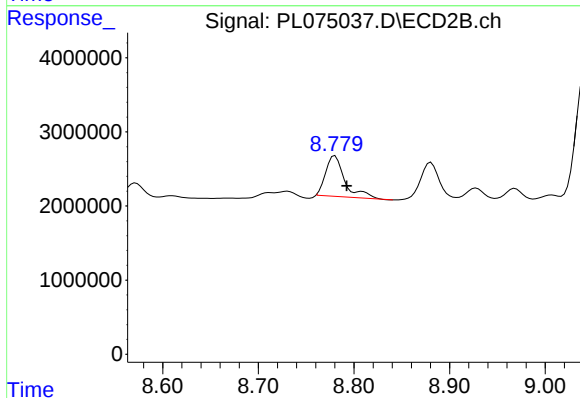


#19 Endosulfan Sulfate

R.T.: 8.780 min
Delta R.T.: -0.012 min
Response: 7474508
Conc: 6.87 ng/ml

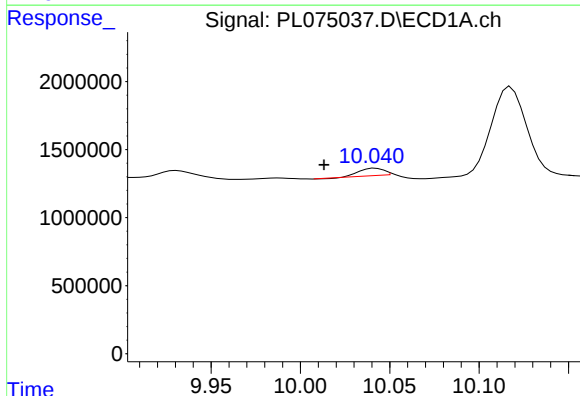


#20 Methoxychlor

R.T.: 10.042 min
Delta R.T.: 0.029 min
Response: 529650
Conc: 2.16 ng/ml

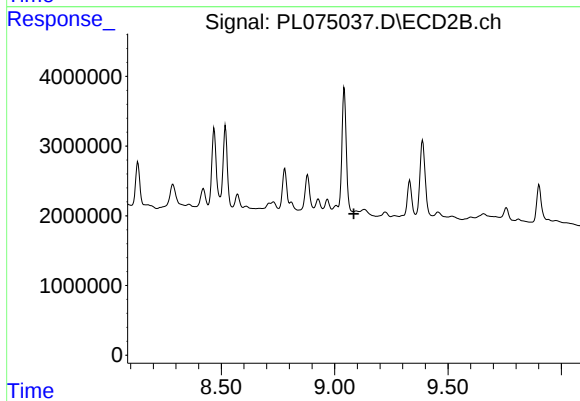

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.084 min
Response: 0
Conc: N.D.

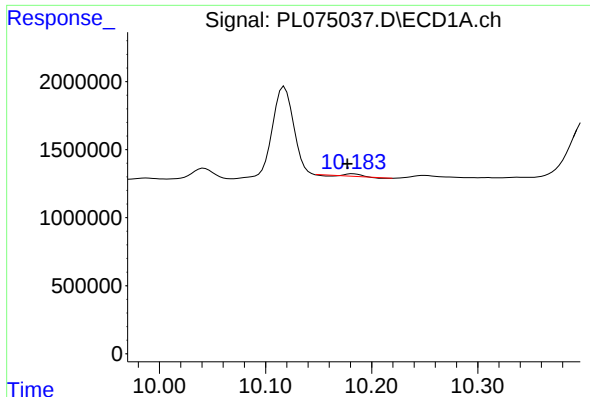

#21 Endrin ketone


R.T.: 10.183 min
Delta R.T.: 0.005 min
Response: 134600
Conc: 0.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

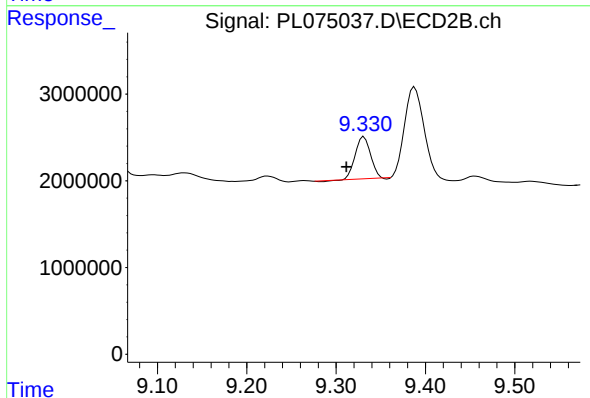


#21 Endrin ketone

R.T.: 9.331 min
Delta R.T.: 0.020 min
Response: 5741326
Conc: 5.15 ng/ml

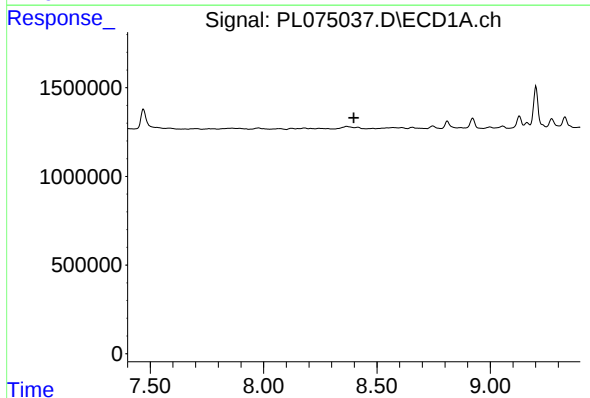


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 8.398 min
Response: 0
Conc: N.D.

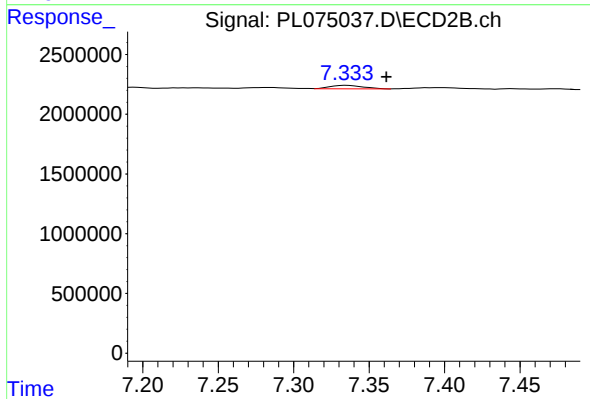

#25 Chlordane-3


R.T.: 7.335 min
Delta R.T.: -0.027 min
Response: 437550
Conc: 3.37 ng/ml

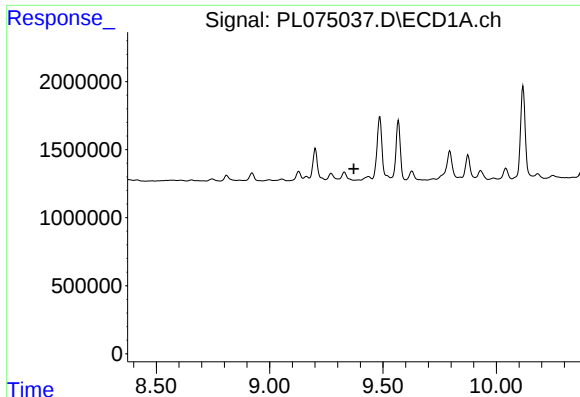

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 9.371 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

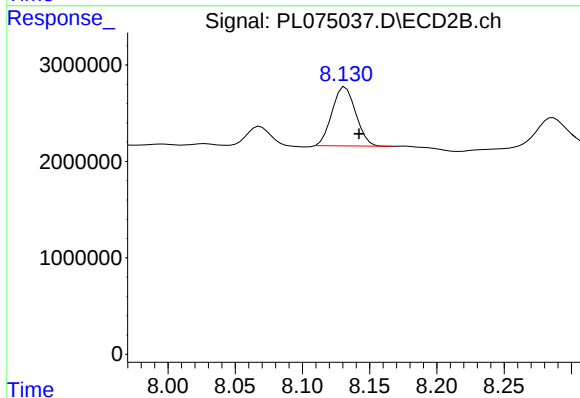


#27 Chlordane-5

R.T.: 8.132 min
Delta R.T.: -0.010 min
Response: 7460784
Conc: 201.79 ng/ml

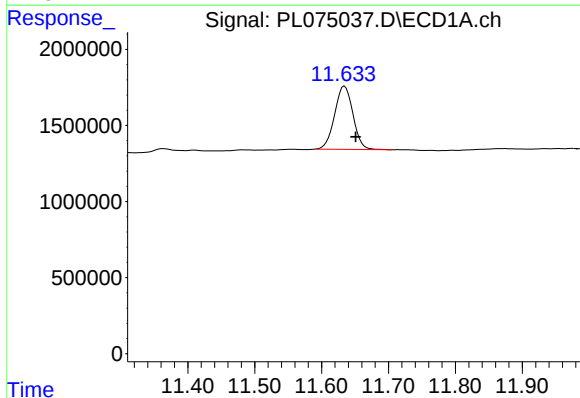

#28 Decachlorobiphenyl

R.T.: 11.634 min
Delta R.T.: -0.017 min
Response: 7911654
Conc: 17.72 ng/ml

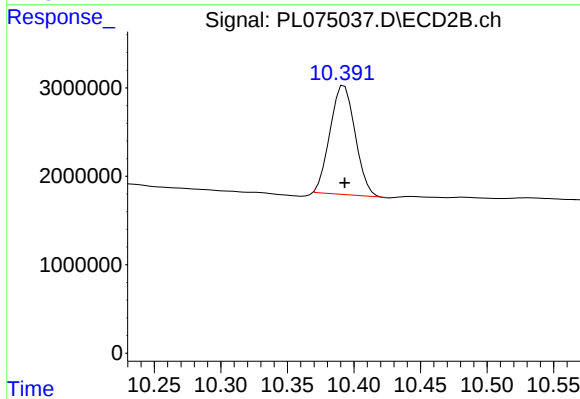

#28 Decachlorobiphenyl

R.T.: 10.393 min
Delta R.T.: 0.000 min
Response: 16171755
Conc: 15.76 ng/ml