

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052522\
 Data File : PL075040.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 May 2022 21:35
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 01:14:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.642	4.645	12243977	31600402	24.115	23.024
28)	SA Decachlor...	11.634f	10.392	10982004	22576320	24.591	21.995
Target Compounds							
6)	B beta-BHC	0.000	6.154	0	144004	N.D.	0.181 #
7)	B delta-BHC	0.000	6.416	0	95331	N.D.	0.061 #
8)	B Heptachlo...	8.123	0.000	4085999	0	7.184	N.D. #
9)	A Endosulfan I	0.000	7.508f	0	102184	N.D.	0.082 #
10)	B gamma-Chl...	8.372f	0.000	367263	0	0.710	N.D. #
11)	B alpha-Chl...	0.000	7.452f	0	473170	N.D.	0.350 #
13)	MA Dieldrin	0.000	7.777	0	3590988	N.D.	2.819 #
14)	MA Endrin	0.000	8.074	0	1067828	N.D.	1.011 #
21)	B Endrin ke...	10.184	0.000	486311	0	0.948	N.D. #
25)	Chlordane-3	8.372f	0.000	367263	0	5.365	N.D. #
26)	Chlordane-4	0.000	7.452f	0	473170	N.D.	3.452 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052522\
Data File : PL075040.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 May 2022 21:35
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 01:14:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

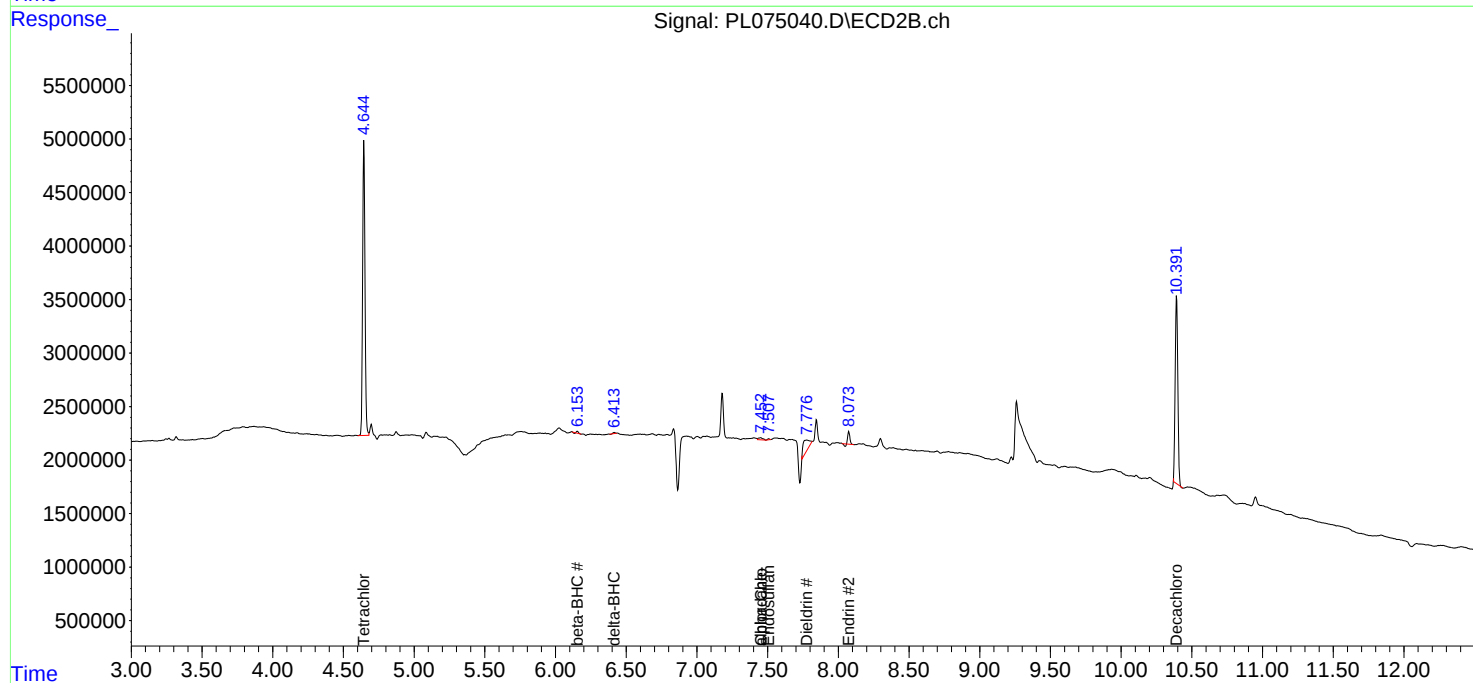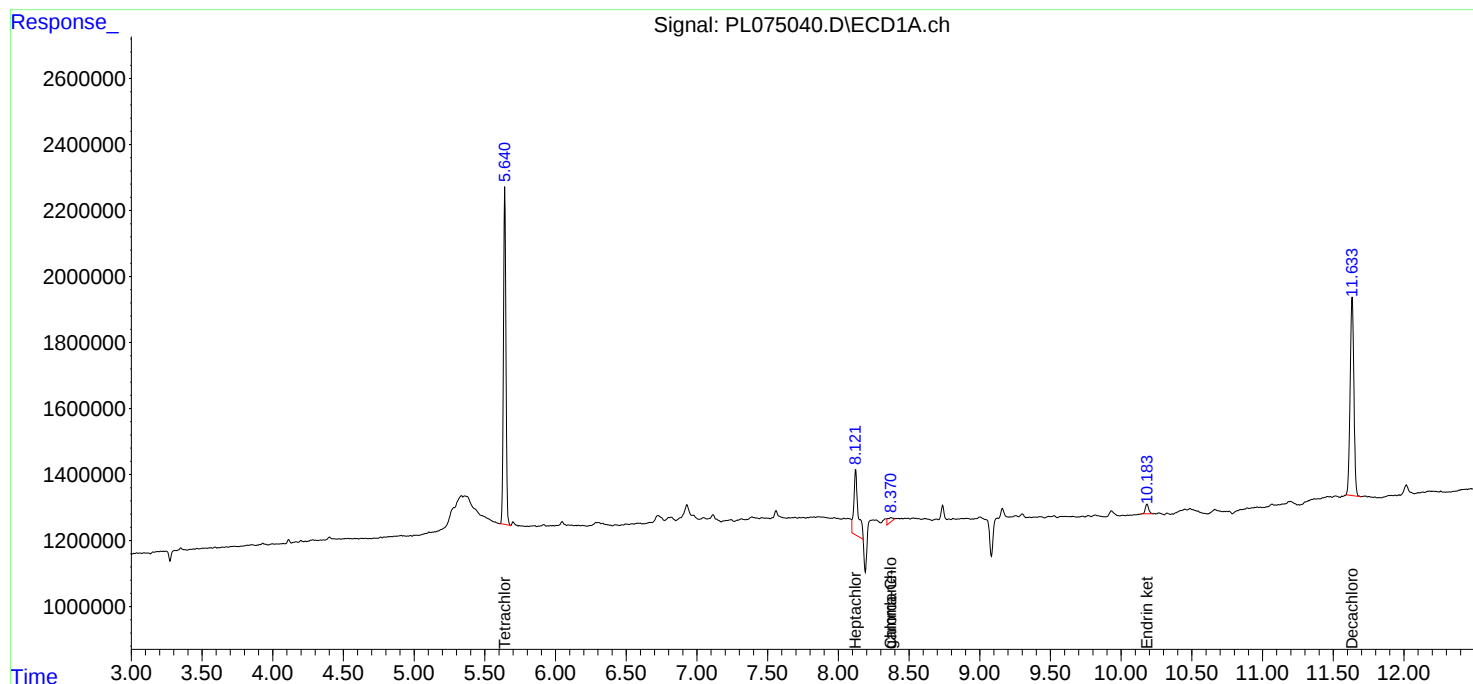


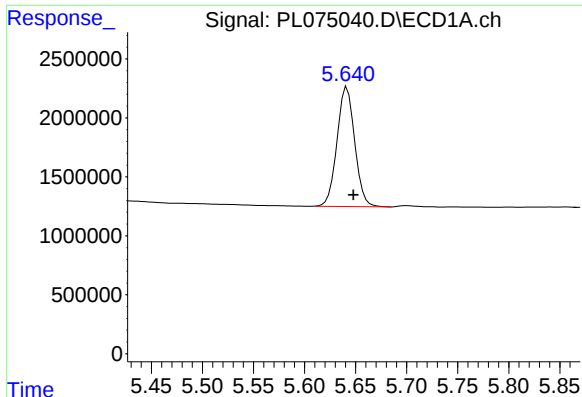

#1 Tetrachloro-m-xylene


R.T.: 5.642 min
Delta R.T.: -0.006 min
Response: 12243977
Conc: 24.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

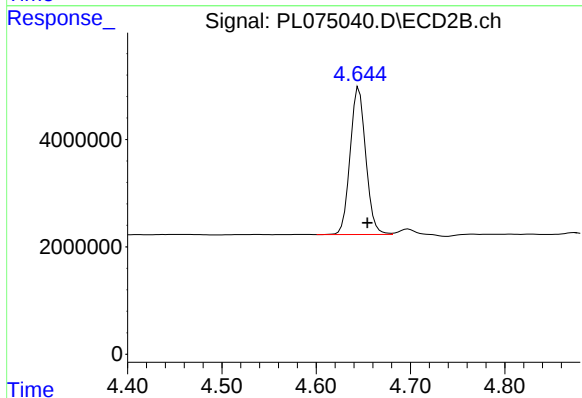


#1 Tetrachloro-m-xylene

R.T.: 4.645 min
Delta R.T.: -0.009 min
Response: 31600402
Conc: 23.02 ng/ml

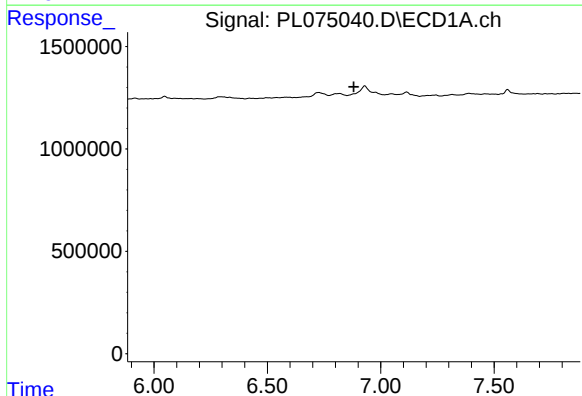


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.882 min
Response: 0
Conc: N.D.

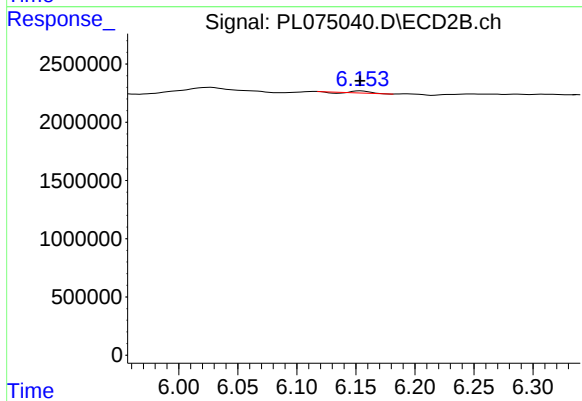

#6 beta-BHC


R.T.: 6.154 min
Delta R.T.: 0.000 min
Response: 144004
Conc: 0.18 ng/ml

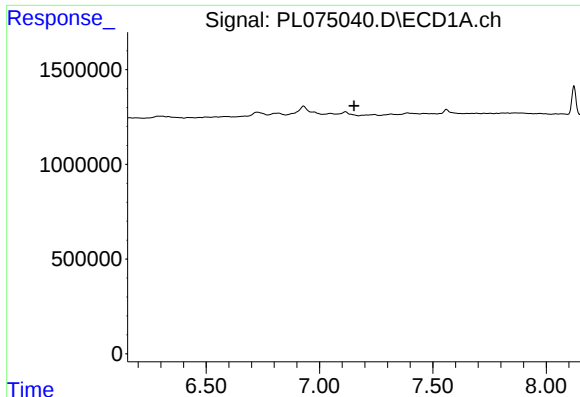

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 7.152 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

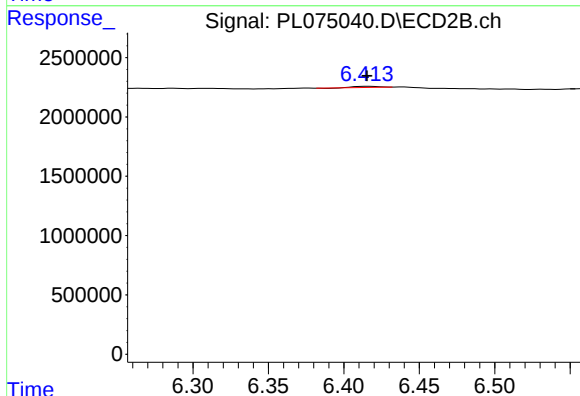


#7 delta-BHC

R.T.: 6.416 min
Delta R.T.: 0.000 min
Response: 95331
Conc: 0.06 ng/ml

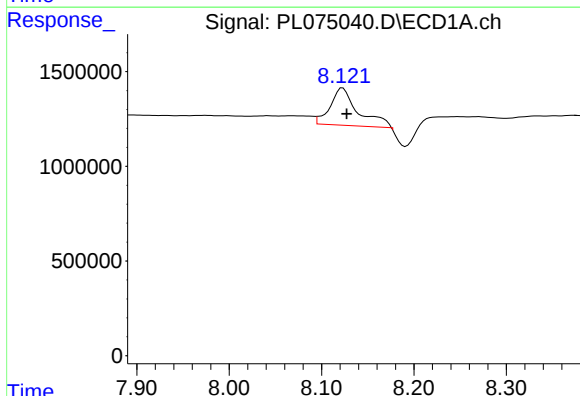


#8 Heptachlor epoxide

R.T.: 8.123 min
Delta R.T.: -0.004 min
Response: 4085999
Conc: 7.18 ng/ml

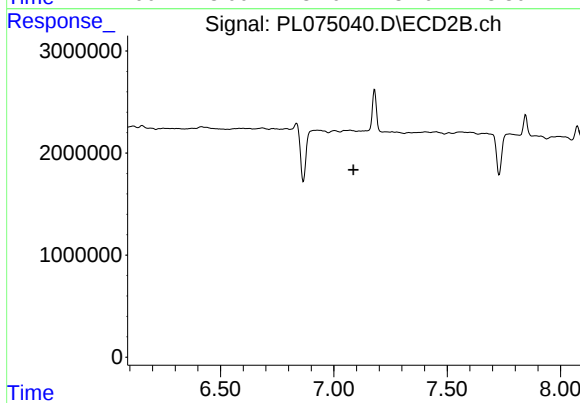

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 7.087 min
Response: 0
Conc: N.D.

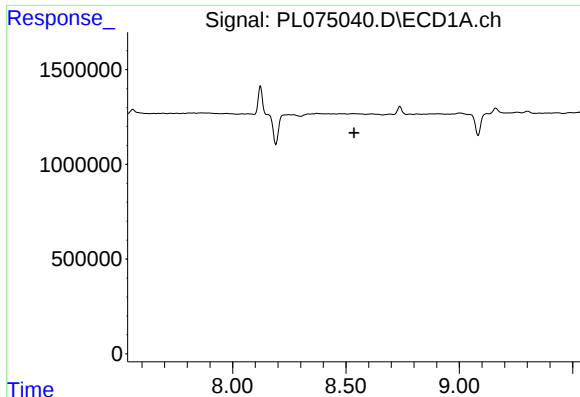

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 8.536 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

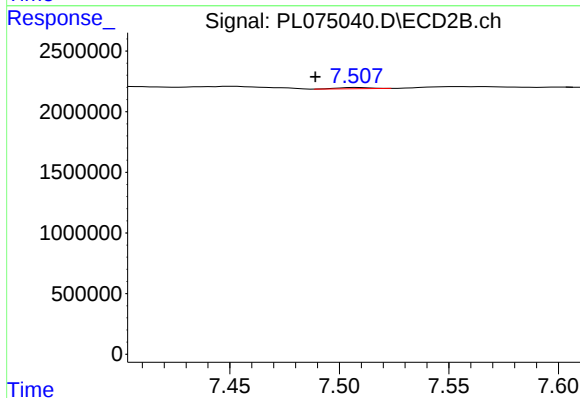


#9 Endosulfan I

R.T.: 7.508 min
Delta R.T.: 0.019 min
Response: 102184
Conc: 0.08 ng/ml

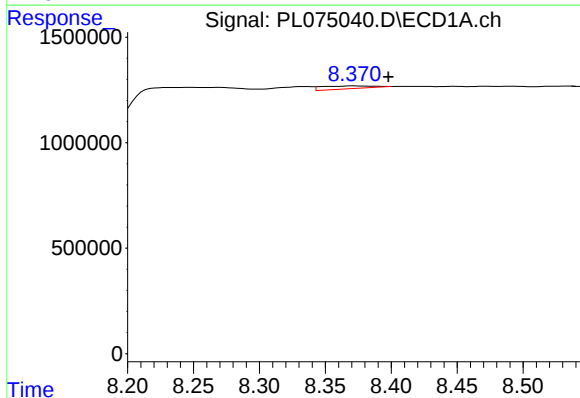


#10 gamma-Chlordane

R.T.: 8.372 min
Delta R.T.: -0.026 min
Response: 367263
Conc: 0.71 ng/ml

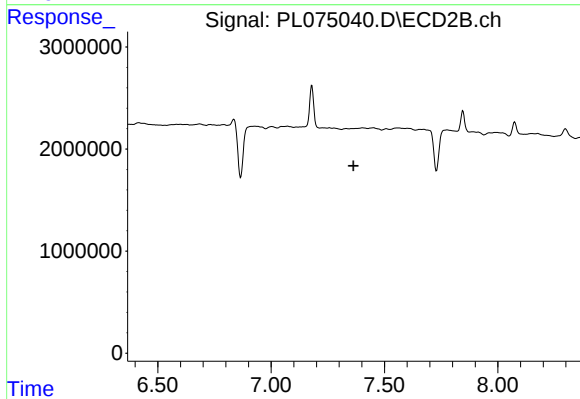

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.363 min
Response: 0
Conc: N.D.

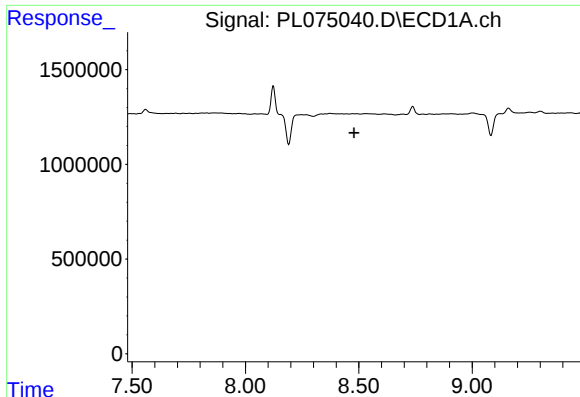

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.480 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

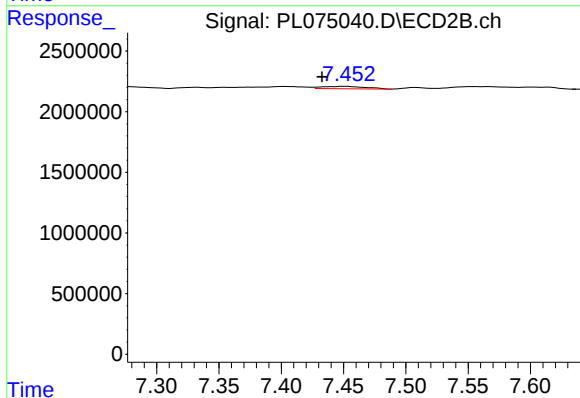


#11 alpha-Chlordane

R.T.: 7.452 min
Delta R.T.: 0.020 min
Response: 473170
Conc: 0.35 ng/ml

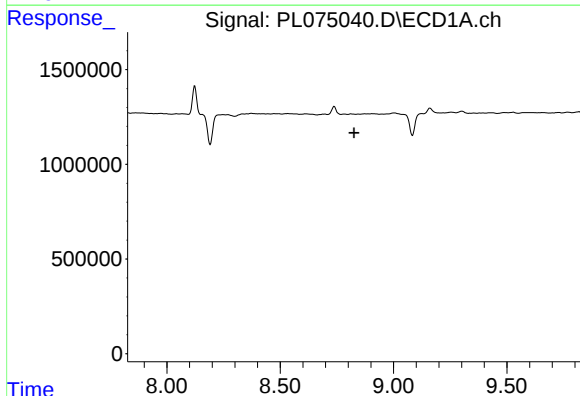


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 8.827 min
Response: 0
Conc: N.D.

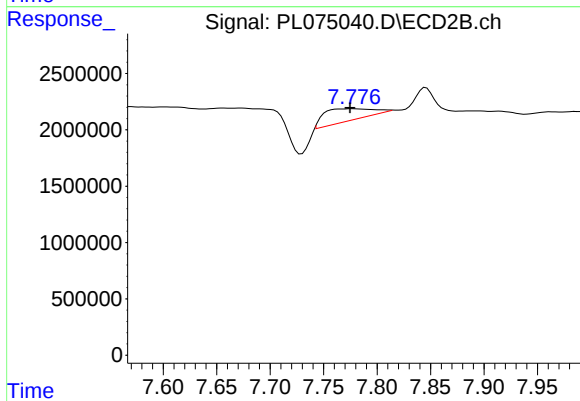

#13 Dieldrin


R.T.: 7.777 min
Delta R.T.: 0.003 min
Response: 3590988
Conc: 2.82 ng/ml

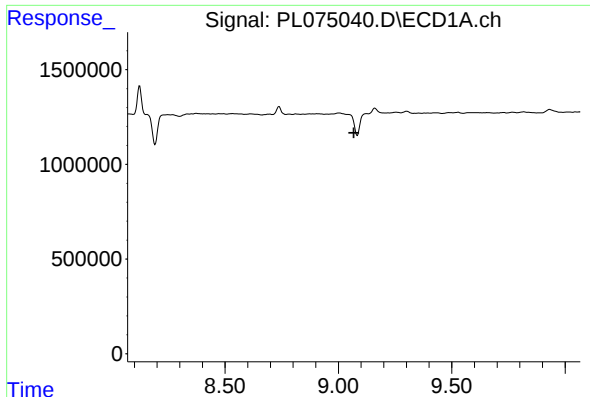

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.068 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

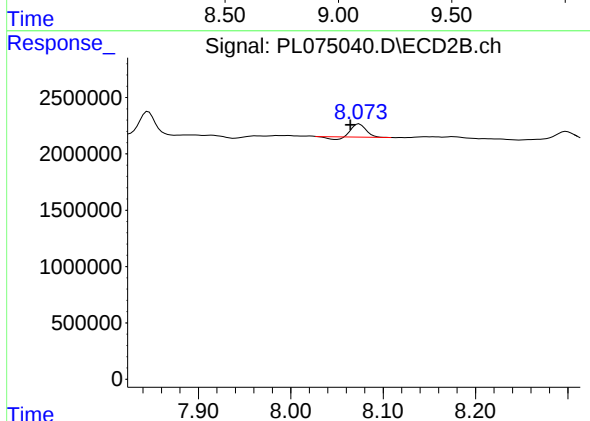


#14 Endrin

R.T.: 8.074 min
Delta R.T.: 0.009 min
Response: 1067828
Conc: 1.01 ng/ml

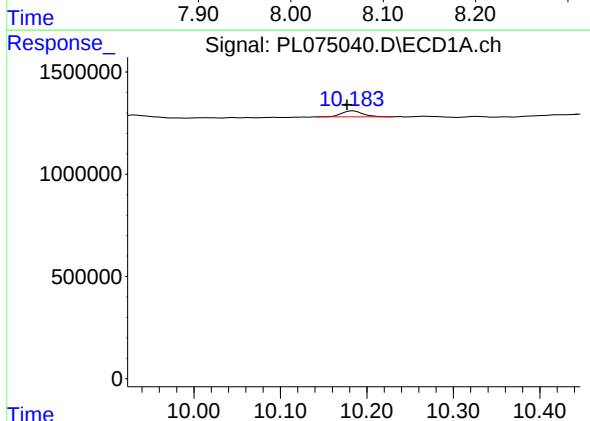


#21 Endrin ketone

R.T.: 10.184 min
Delta R.T.: 0.007 min
Response: 486311
Conc: 0.95 ng/ml

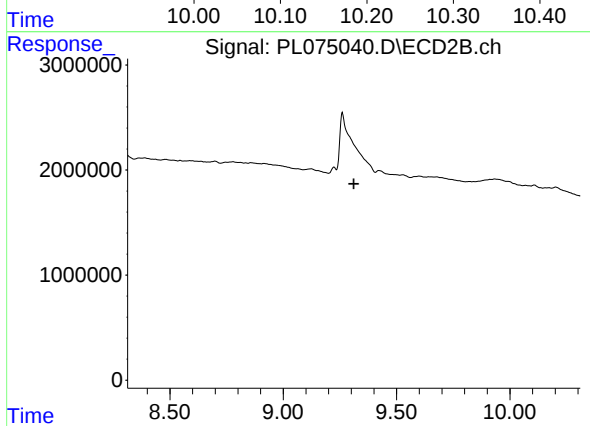

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.311 min
Response: 0
Conc: N.D.

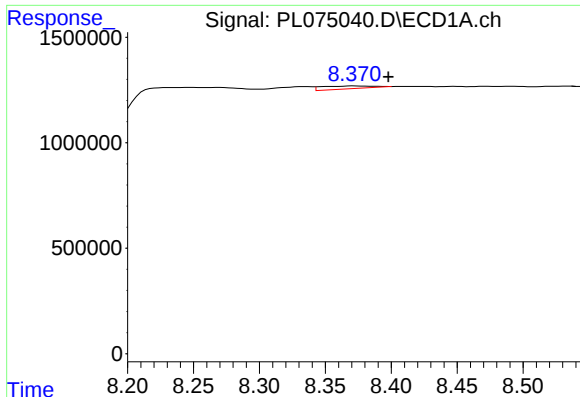

#25 Chlordane-3


R.T.: 8.372 min
Delta R.T.: -0.026 min
Response: 367263
Conc: 5.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

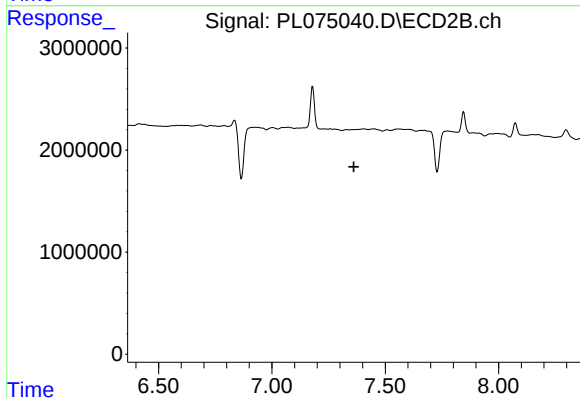


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.362 min
Response: 0
Conc: N.D.

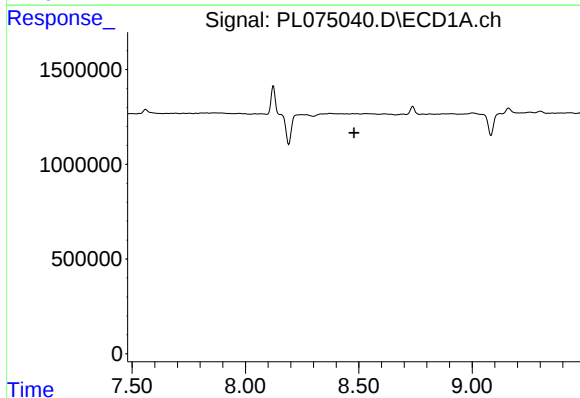


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.479 min
Response: 0
Conc: N.D.

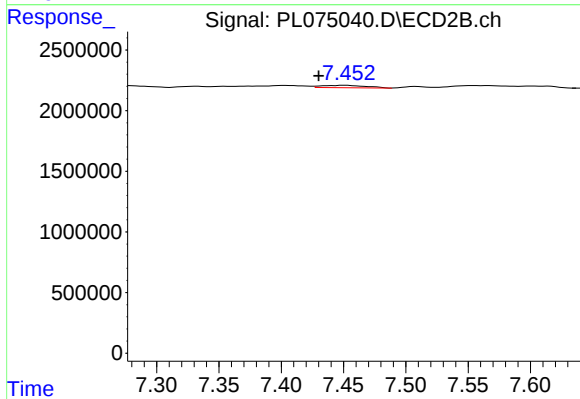

#26 Chlordane-4


R.T.: 7.452 min
Delta R.T.: 0.022 min
Response: 473170
Conc: 3.45 ng/ml

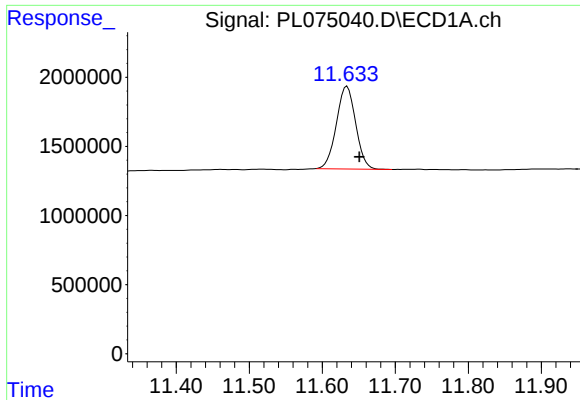

#28 Decachlorobiphenyl

R.T.: 11.634 min
Delta R.T.: -0.017 min
Response: 10982004
Conc: 24.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

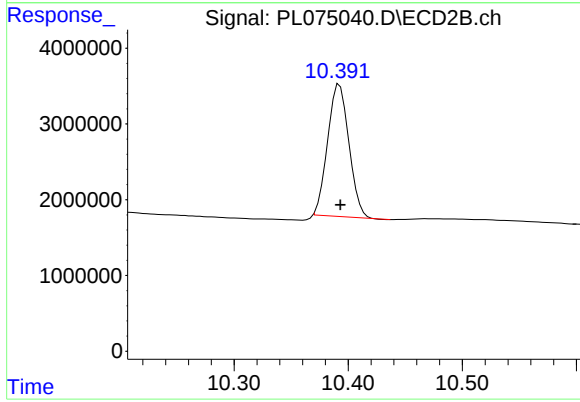

#28 Decachlorobiphenyl

R.T.: 10.392 min
Delta R.T.: 0.000 min
Response: 22576320
Conc: 22.00 ng/ml