

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052522\
 Data File : PL075014.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 May 2022 12:06
 Operator : AR\AJ
 Sample : N2877-12 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 P007-SS017-0006-01

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/26/2022
 Supervised By :Ankita Jodhani 05/26/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 04:19:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.642	4.645	780768	2125624	1.538	1.549
28) SA Decachlor...	11.633	10.393	816496	1949078	1.828m	1.899
Target Compounds						
12) B 4,4'-DDE	8.657	7.632	411890	1047670	0.890	0.890

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052522\
Data File : PL075014.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 May 2022 12:06
Operator : AR\AJ
Sample : N2877-12 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
P007-SS017-0006-01


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/26/2022
Supervised By : Ankita Jodhani 05/26/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 04:19:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

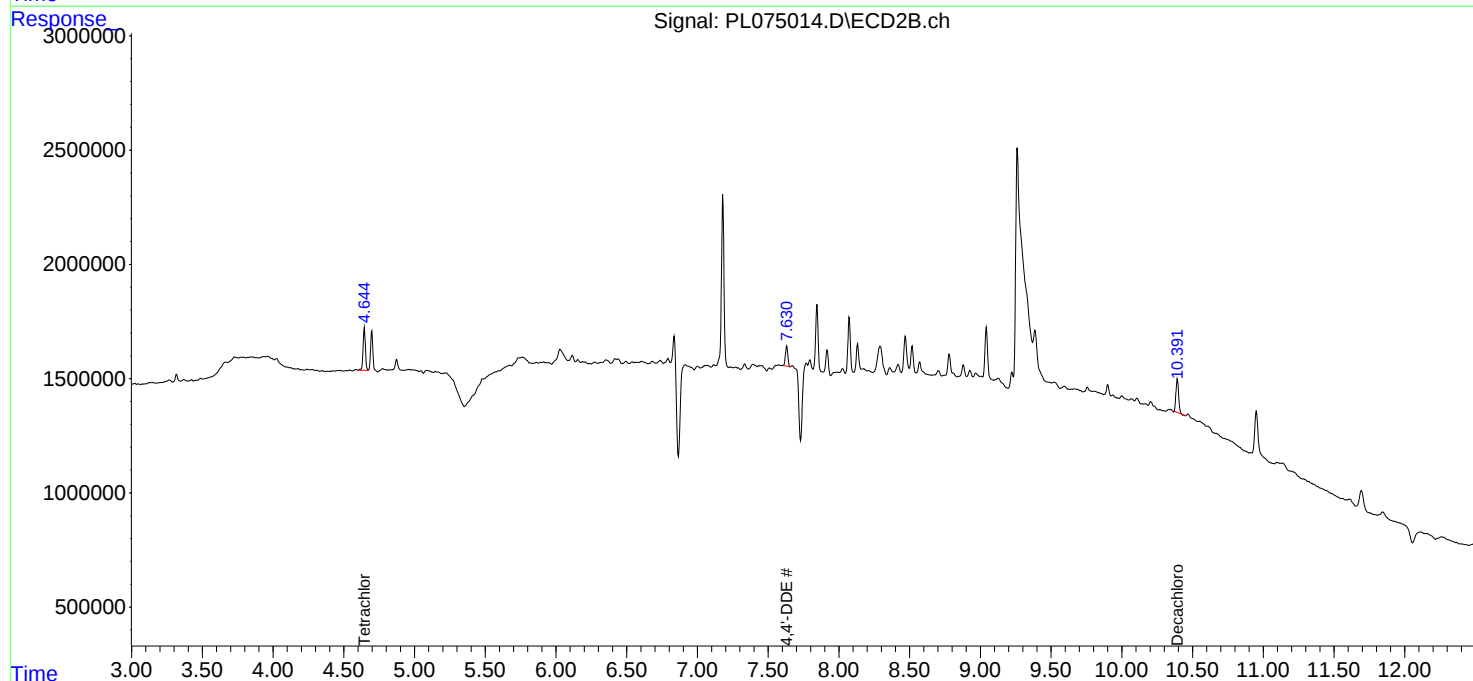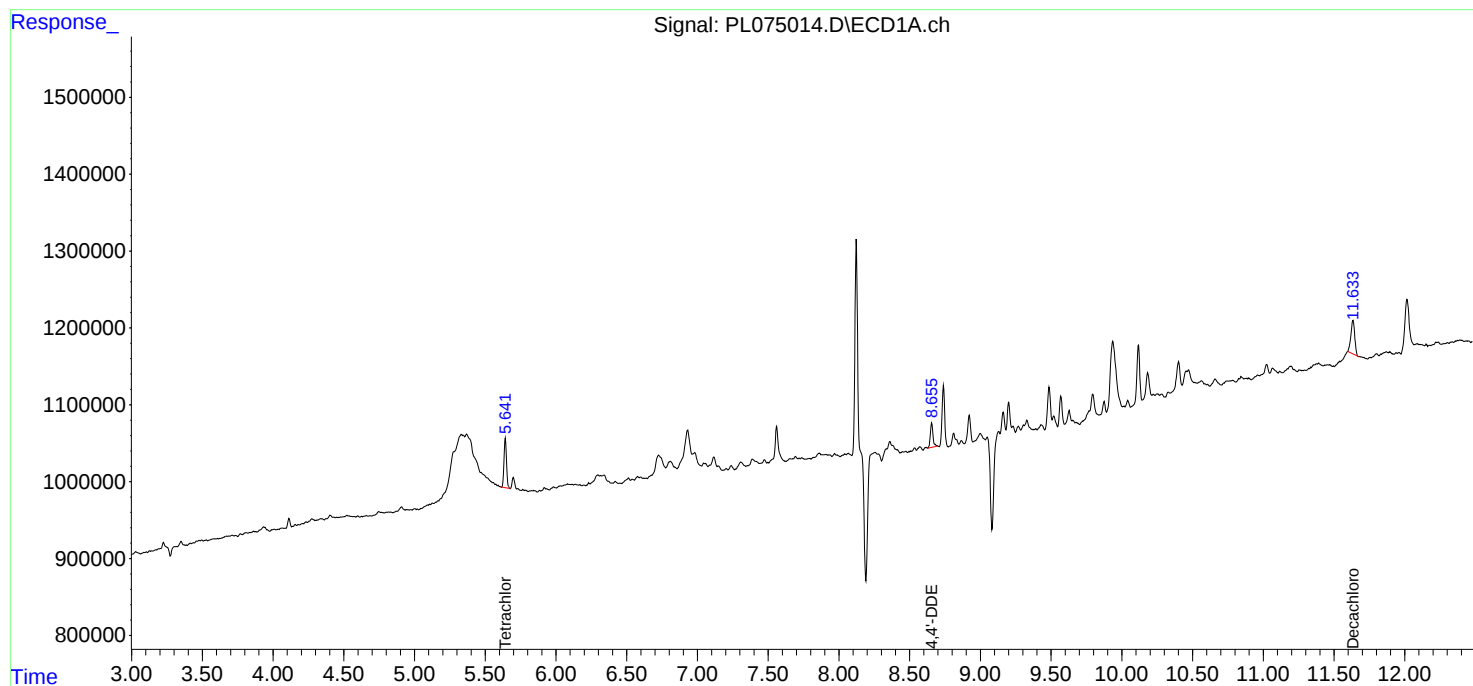

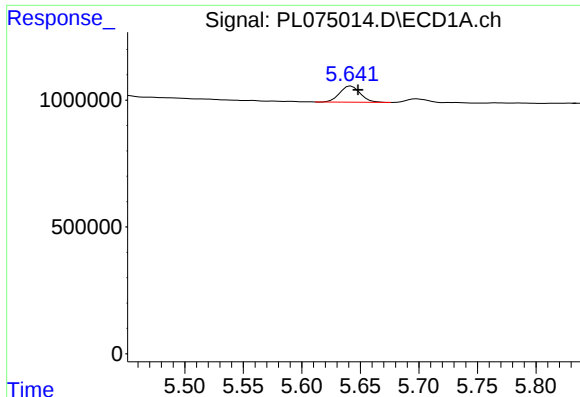


#1 Tetrachloro-m-xylene

R.T.: 5.642 min
Delta R.T.: -0.006 min
Response: 780768
Conc: 1.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
P007-SS017-0006-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/26/2022
Supervised By :Ankita Jodhani 05/26/2022

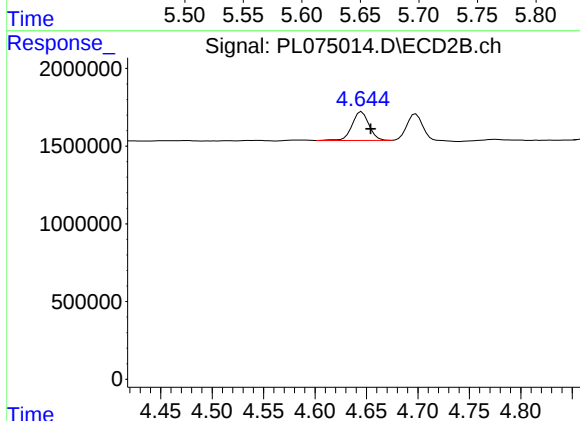


#1 Tetrachloro-m-xylene

R.T.: 4.645 min
Delta R.T.: -0.009 min
Response: 2125624
Conc: 1.55 ng/ml

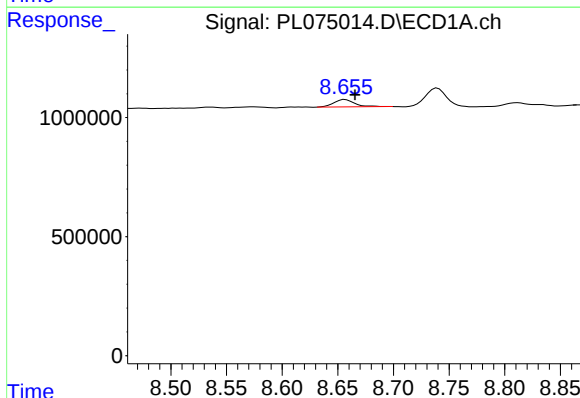


#12 4,4'-DDE

R.T.: 8.657 min
Delta R.T.: -0.009 min
Response: 411890
Conc: 0.89 ng/ml

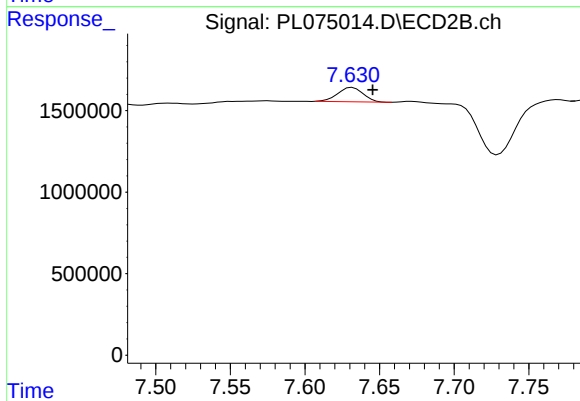

#12 4,4'-DDE

R.T.: 7.632 min
Delta R.T.: -0.013 min
Response: 1047670
Conc: 0.89 ng/ml

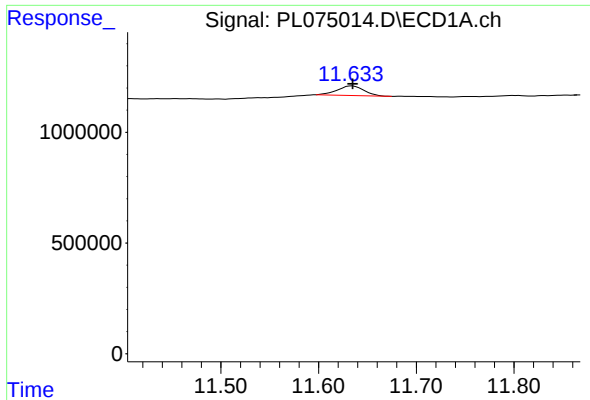


#28 Decachlorobiphenyl

R.T.: 11.633 min
Delta R.T.: -0.002 min
Response: 816496
Conc: 1.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
P007-SS017-0006-01

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/26/2022
Supervised By :Ankita Jodhani 05/26/2022

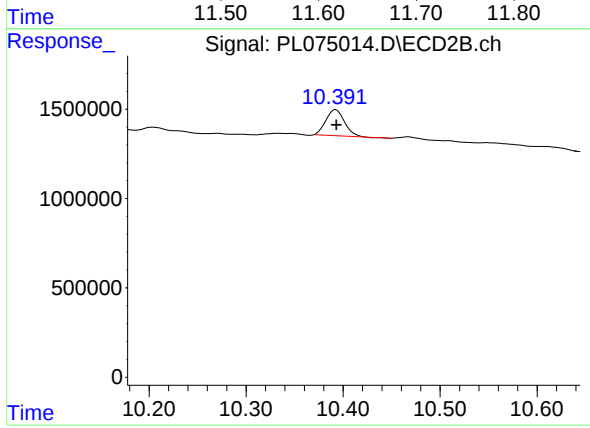

#28 Decachlorobiphenyl

R.T.: 10.393 min
Delta R.T.: 0.000 min
Response: 1949078
Conc: 1.90 ng/ml