

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052522\
 Data File : PL075016.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 May 2022 12:39
 Operator : AR\AJ
 Sample : N2896-21
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 P040-SS001-2430-01

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/26/2022
 Supervised By : Ankita Jodhani 05/26/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 04:16:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.642	4.645	1818647	5368653	3.582	3.912
2) SA Decachlor...	11.634	10.391	3748317	9240673	8.393	9.003m
Target Compounds						
12) B 4,4'-DDE	8.658	7.631	406953	1091070	0.879	0.927

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052522\
Data File : PL075016.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 May 2022 12:39
Operator : AR\AJ
Sample : N2896-21
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
P040-SS001-2430-01


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/26/2022
Supervised By : Ankita Jodhani 05/26/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 04:16:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

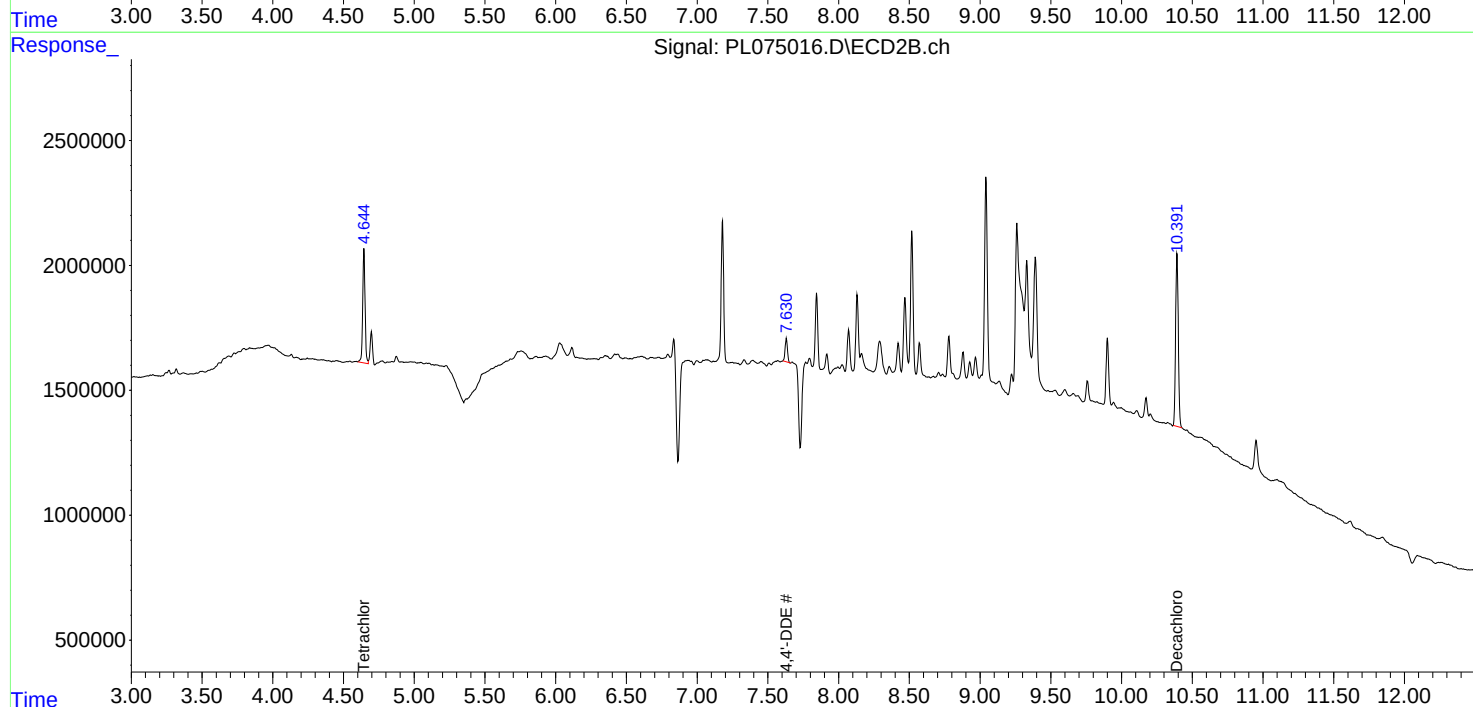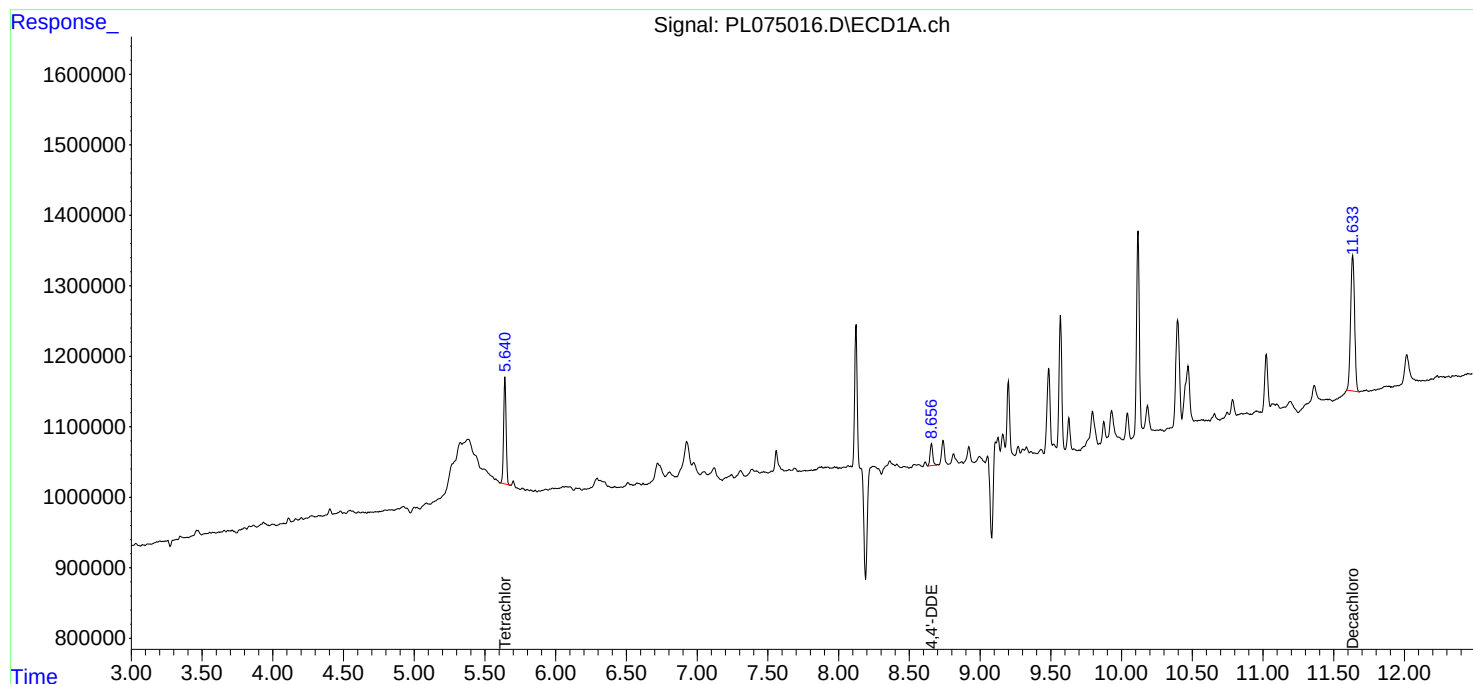

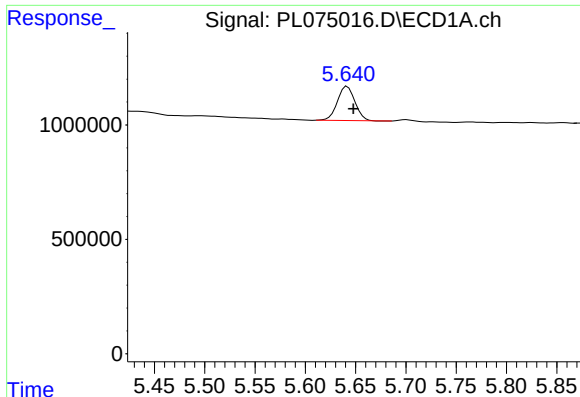


#1 Tetrachloro-m-xylene

R.T.: 5.642 min
Delta R.T.: -0.006 min
Response: 1818647
Conc: 3.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
P040-SS001-2430-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/26/2022
Supervised By :Ankita Jodhani 05/26/2022

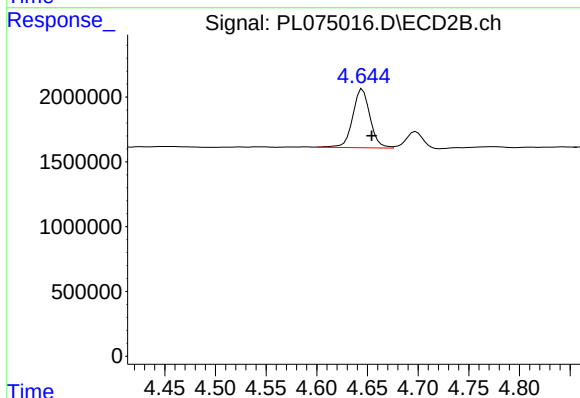


#1 Tetrachloro-m-xylene

R.T.: 4.645 min
Delta R.T.: -0.009 min
Response: 5368653
Conc: 3.91 ng/ml

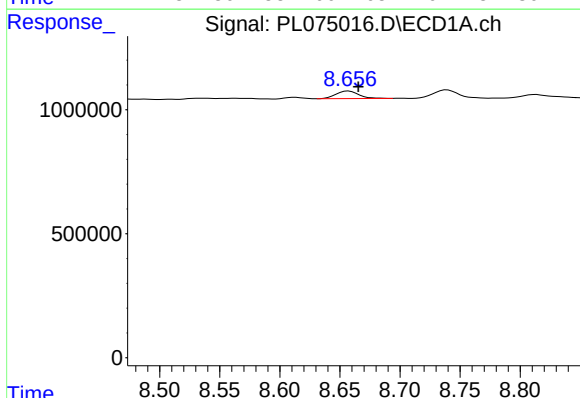


#12 4,4'-DDE

R.T.: 8.658 min
Delta R.T.: -0.008 min
Response: 406953
Conc: 0.88 ng/ml

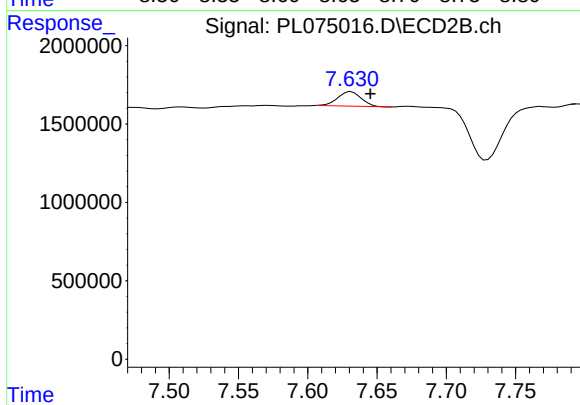

#12 4,4'-DDE

R.T.: 7.631 min
Delta R.T.: -0.014 min
Response: 1091070
Conc: 0.93 ng/ml

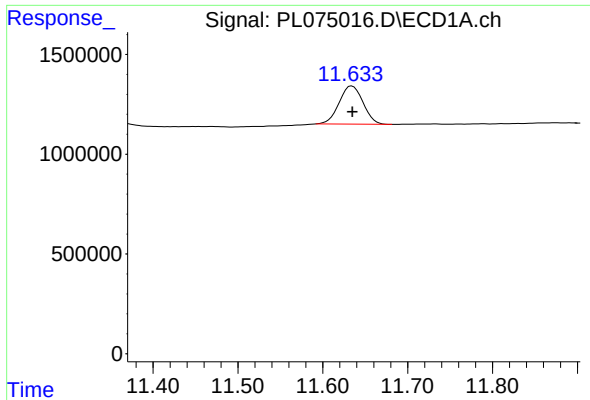


#28 Decachlorobiphenyl

R.T.: 11.634 min
Delta R.T.: 0.000 min
Response: 3748317
Conc: 8.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
P040-SS001-2430-01

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/26/2022
Supervised By :Ankita Jodhani 05/26/2022

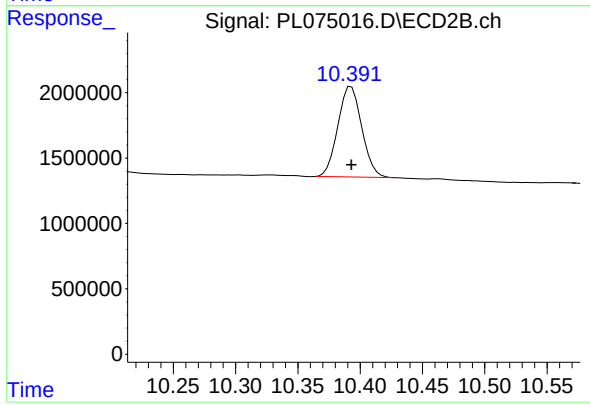

#28 Decachlorobiphenyl

R.T.: 10.391 min
Delta R.T.: -0.002 min
Response: 9240673
Conc: 9.00 ng/ml m