

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052522\
 Data File : PL075020.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 May 2022 13:45
 Operator : AR\AJ
 Sample : N2896-13 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 P039-SS001-0612-01

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/26/2022
 Supervised By : Ankita Jodhani 05/26/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 04:58:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.642	4.643	527907	1306524	1.040	0.952m
28) SA Decachlor...	11.621	10.388	1143304	3422443	2.560m	3.334m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052522\
Data File : PL075020.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 May 2022 13:45
Operator : AR\AJ
Sample : N2896-13 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
P039-SS001-0612-01


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/26/2022
Supervised By : Ankita Jodhani 05/26/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 04:58:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

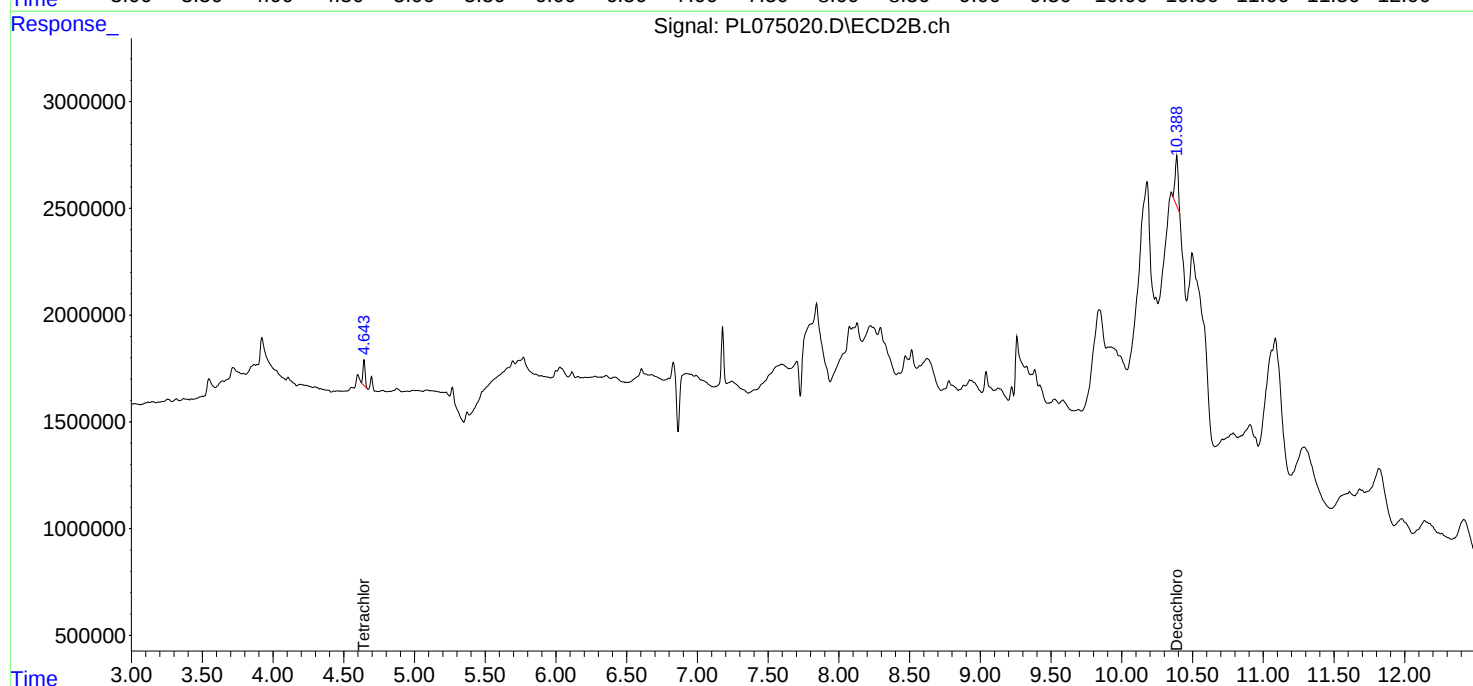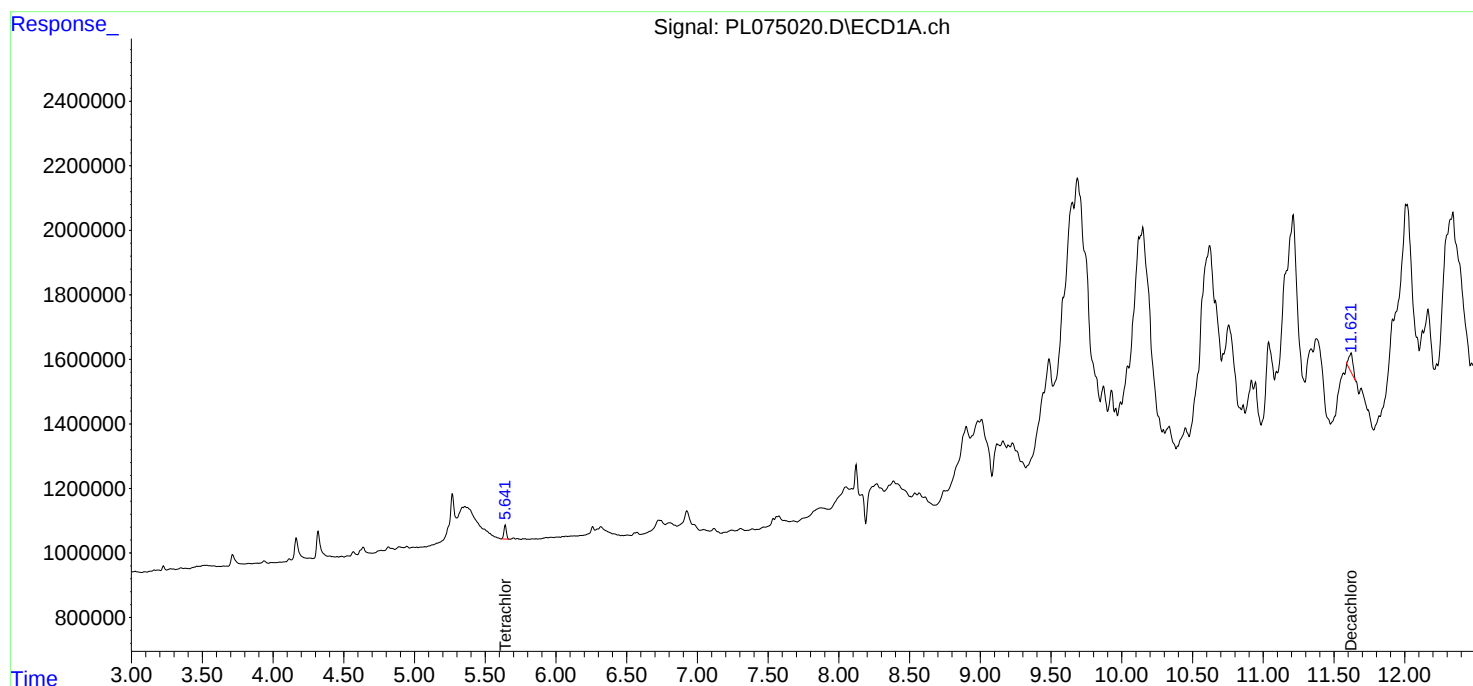

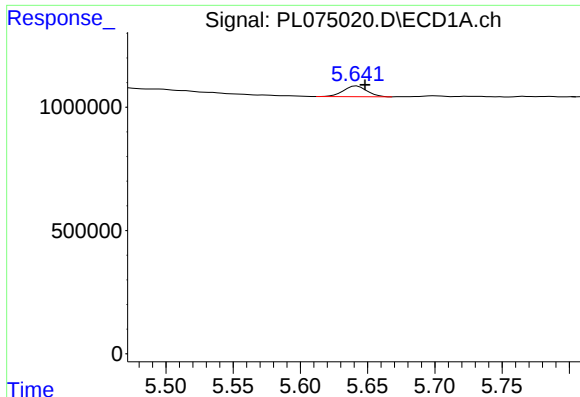


#1 Tetrachloro-m-xylene

R.T.: 5.642 min
Delta R.T.: -0.006 min
Response: 527907
Conc: 1.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
P039-SS001-0612-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/26/2022
Supervised By :Ankita Jodhani 05/26/2022

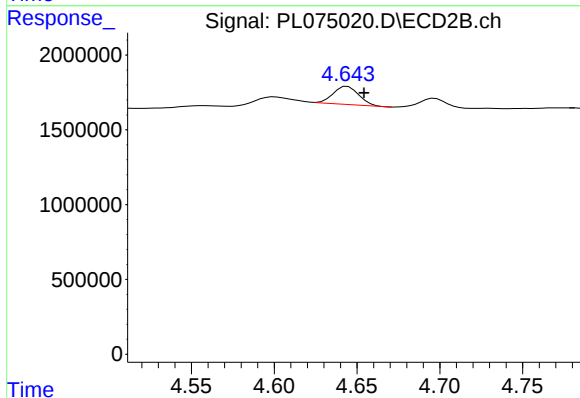


#1 Tetrachloro-m-xylene

R.T.: 4.643 min
Delta R.T.: -0.011 min
Response: 1306524
Conc: 0.95 ng/ml m

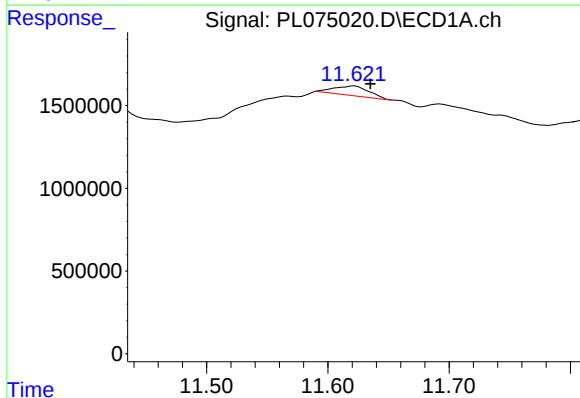

#28 Decachlorobiphenyl

R.T.: 11.621 min
Delta R.T.: -0.014 min
Response: 1143304
Conc: 2.56 ng/ml m

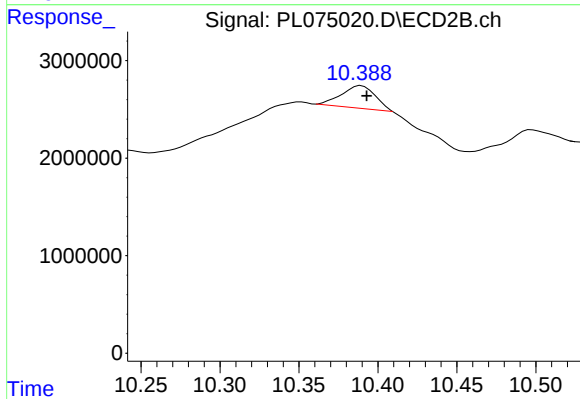

#28 Decachlorobiphenyl

R.T.: 10.388 min
Delta R.T.: -0.005 min
Response: 3422443
Conc: 3.33 ng/ml m