

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052522\
 Data File : PL075046.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2022 02:00
 Operator : AR\AJ
 Sample : N3001-01
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BU-03-052322

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/26/2022
 Supervised By : Ankita Jodhani 05/26/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 06:13:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.642	4.646	2237118	6286759	4.406	4.580
28)	SA Decachlor...	11.636	10.392	5557027	12481998	12.443	12.161m
Target Compounds							
12)	B 4,4'-DDE	8.656	7.631	1003290	2796349	2.167m	2.376m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052522\
Data File : PL075046.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2022 02:00
Operator : AR\AJ
Sample : N3001-01
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BU-03-052322


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/26/2022
Supervised By : Ankita Jodhani 05/26/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 06:13:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

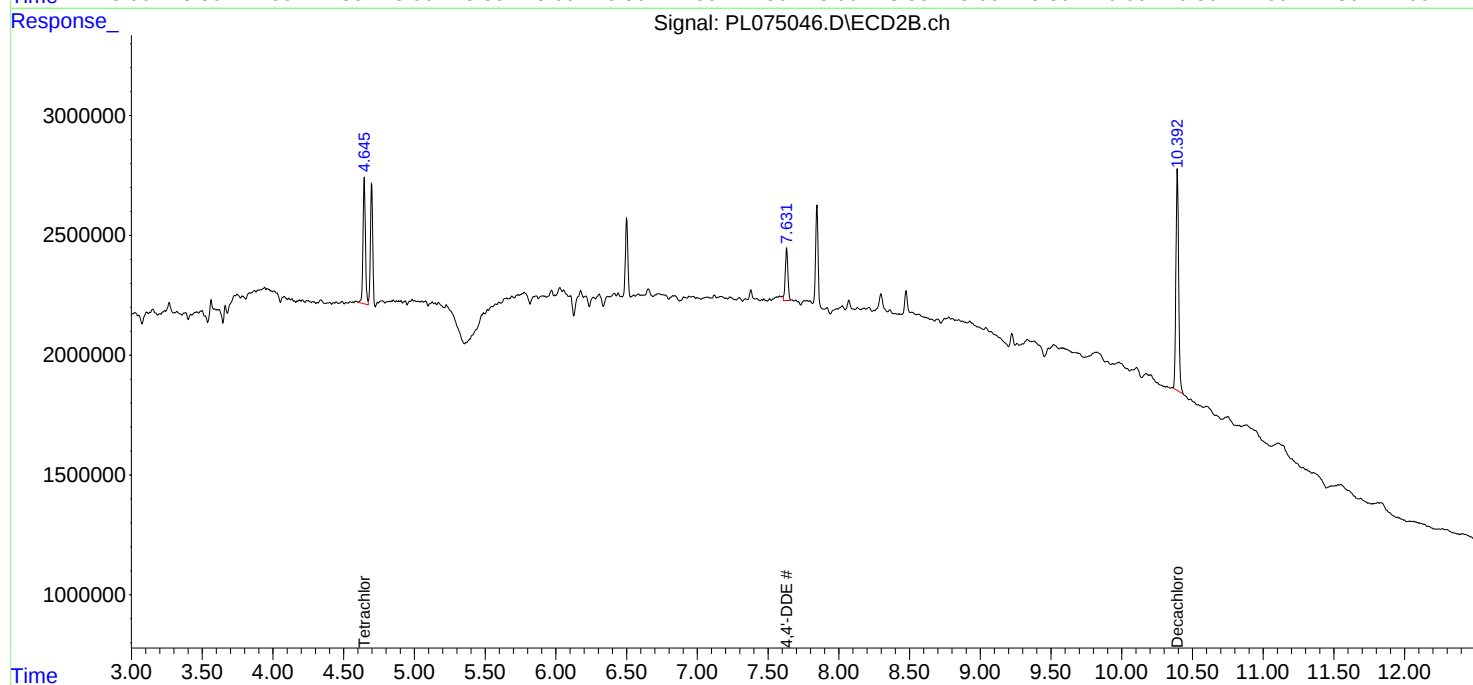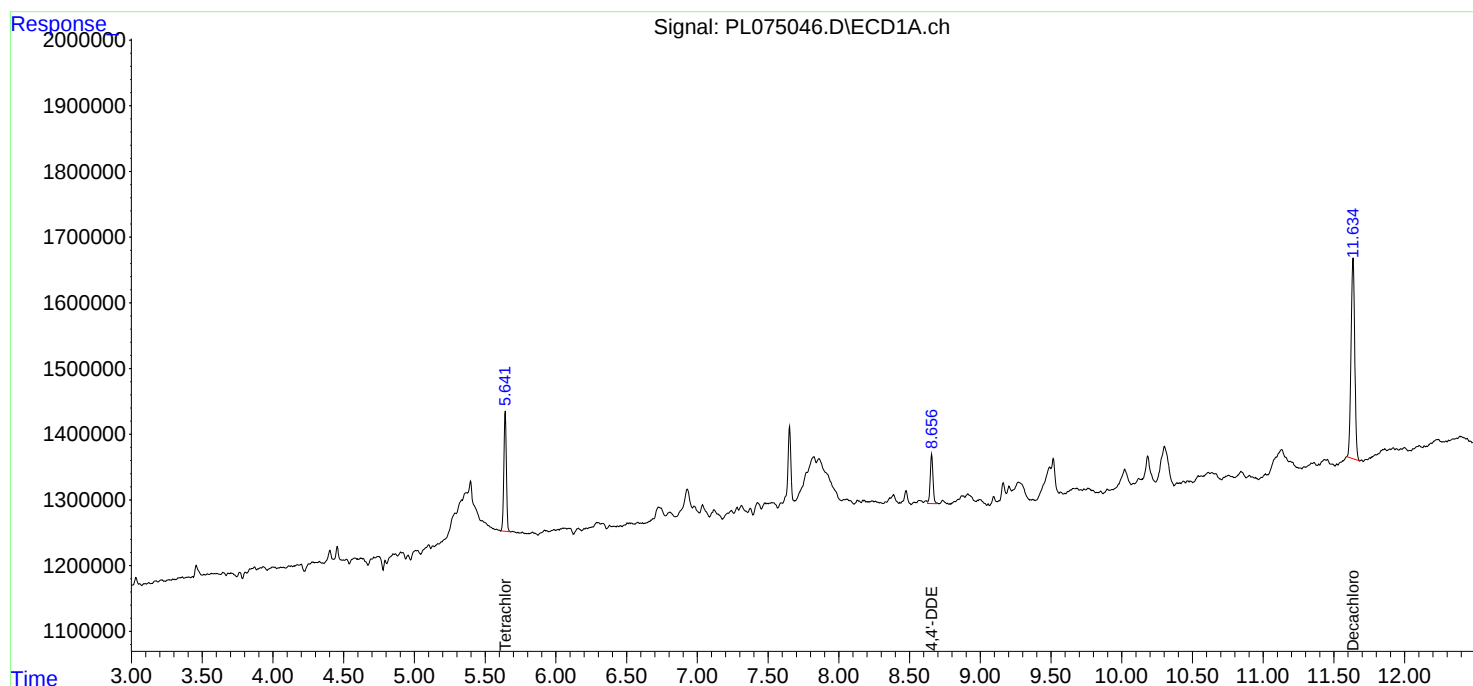

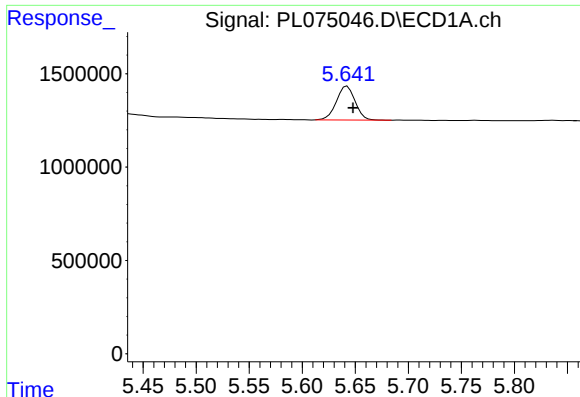


#1 Tetrachloro-m-xylene

R.T.: 5.642 min
Delta R.T.: -0.006 min
Response: 2237118
Conc: 4.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
BU-03-052322


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/26/2022
Supervised By :Ankita Jodhani 05/26/2022

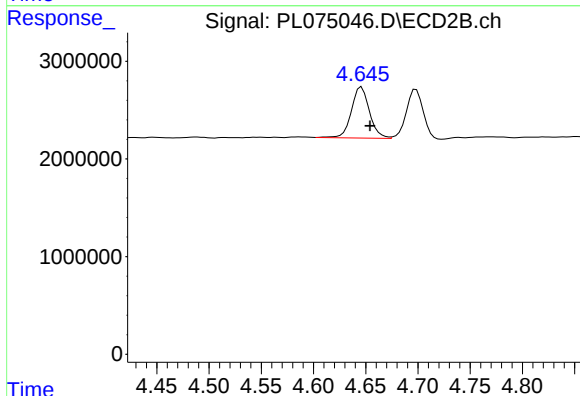


#1 Tetrachloro-m-xylene

R.T.: 4.646 min
Delta R.T.: -0.008 min
Response: 6286759
Conc: 4.58 ng/ml

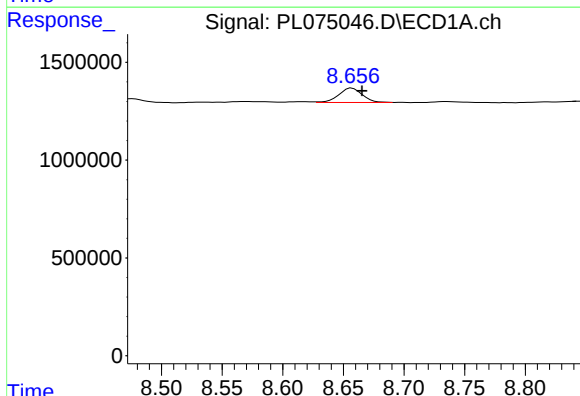


#12 4,4'-DDE

R.T.: 8.656 min
Delta R.T.: -0.010 min
Response: 1003290
Conc: 2.17 ng/ml m

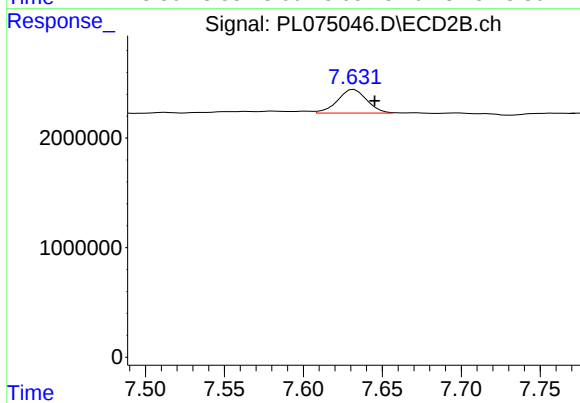

#12 4,4'-DDE

R.T.: 7.631 min
Delta R.T.: -0.014 min
Response: 2796349
Conc: 2.38 ng/ml m

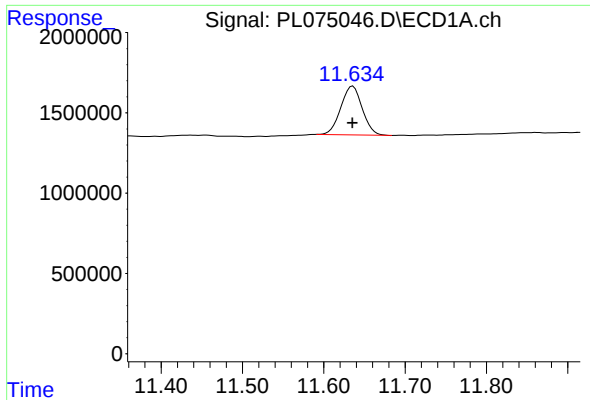


#28 Decachlorobiphenyl

R.T.: 11.636 min
Delta R.T.: 0.000 min
Response: 5557027
Conc: 12.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
BU-03-052322

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/26/2022
Supervised By :Ankita Jodhani 05/26/2022

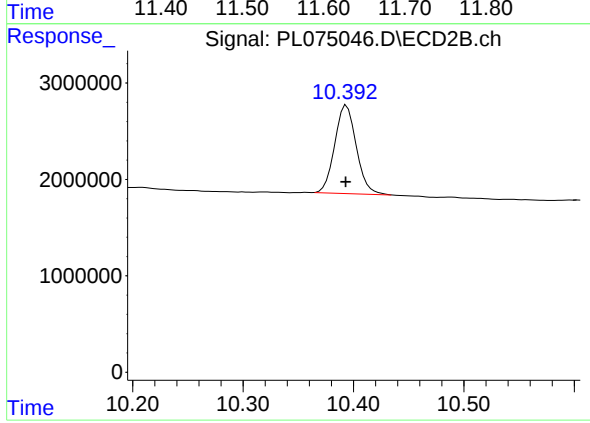

#28 Decachlorobiphenyl

R.T.: 10.392 min
Delta R.T.: 0.000 min
Response: 12481998
Conc: 12.16 ng/ml m