

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052620\
 Data File : PL058882.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2020 15:56
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NM42-COMP-2020-0-6MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 17:02:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
 Quant Title : GC Extractables
 QLast Update : Wed May 20 11:27:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.529	4.097f	41203617	48763659	22.471	18.005
28)	SA Decachlor...	8.311	9.207f	35580244	48440653	21.059	18.375
Target Compounds							
8)	B Heptachlo...	0.000	5.977	0	5258465	N.D.	1.594 #
9)	A Endosulfan I	0.000	6.320	0	585913	N.D.	0.199 #
10)	B gamma-Chl...	0.000	6.191	0	6454674	N.D.	1.949 #
11)	B alpha-Chl...	0.000	6.293f	0	944609	N.D.	0.291 #
15)	B Endosulfa...	0.000	7.032f	0	1458368	N.D.	0.520 #
16)	A 4,4'-DDD	0.000	6.901f	0	616603	N.D.	0.258 #
25)	Chlordane-3	0.000	6.191	0	6454674	N.D.	16.956 #
26)	Chlordane-4	0.000	6.293f	0	944609	N.D.	2.074 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052620\
Data File : PL058882.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2020 15:56
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
NM42-COMP-2020-0-6MS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 17:02:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
Quant Title : GC Extractables
QLast Update : Wed May 20 11:27:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

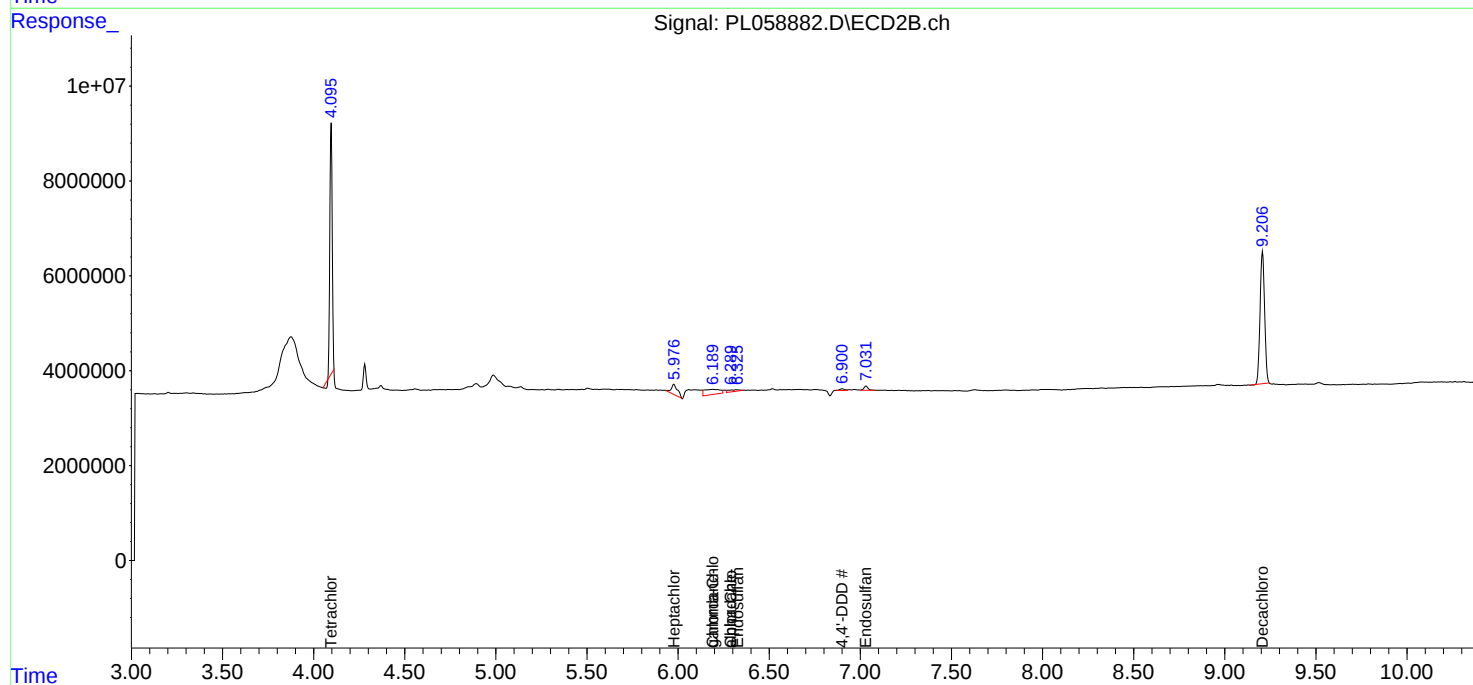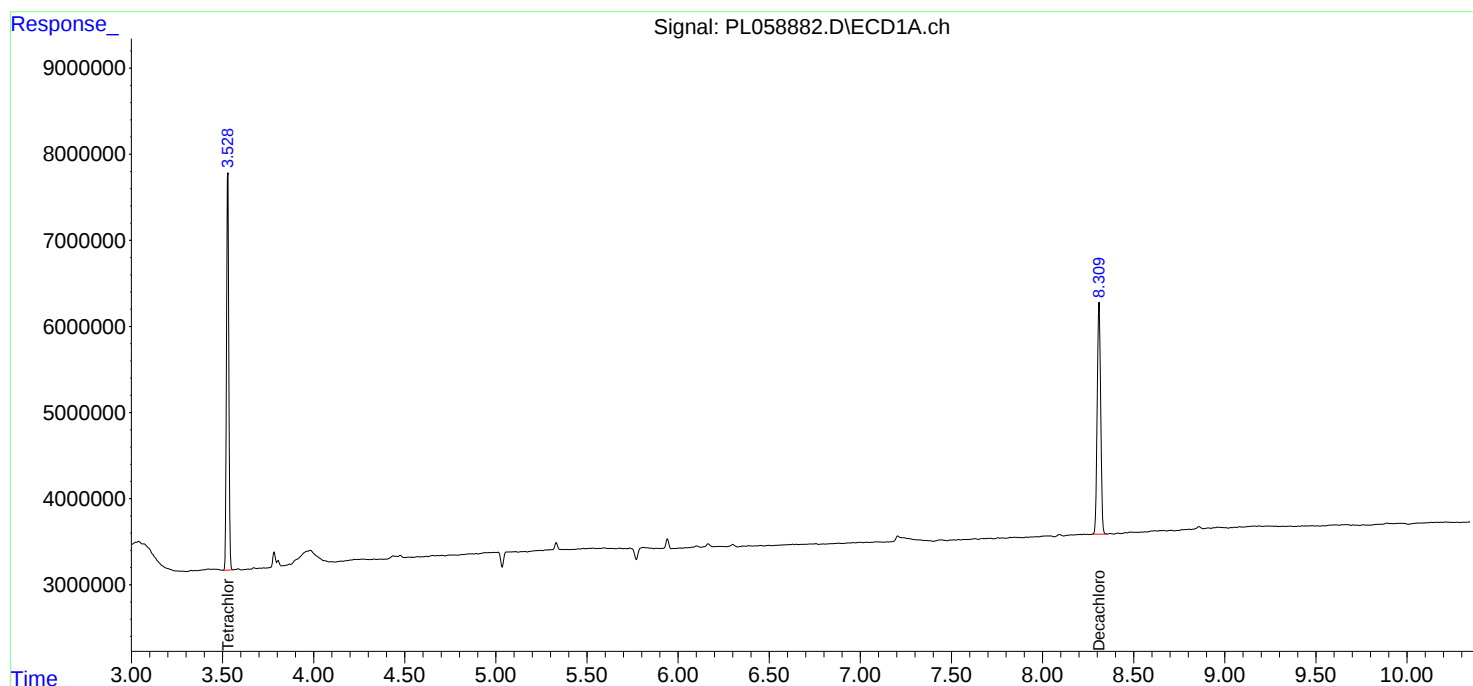


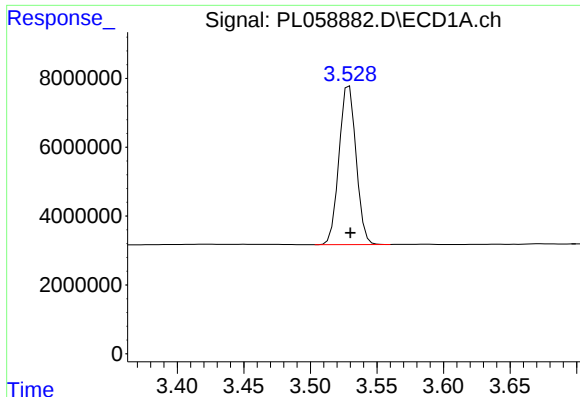

#1 Tetrachloro-m-xylene


R.T.: 3.529 min
Delta R.T.: 0.000 min
Response: 41203617
Conc: 22.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
NM42-COMP-2020-0-6MS

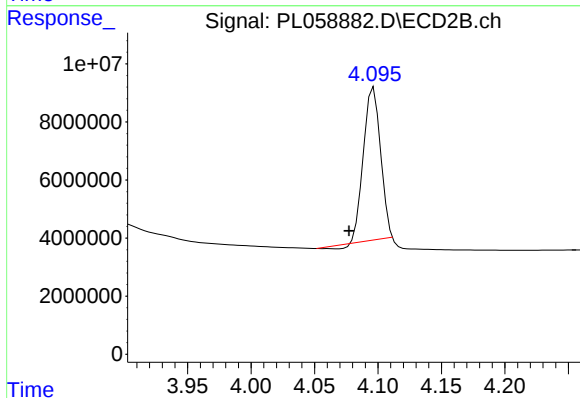


#1 Tetrachloro-m-xylene

R.T.: 4.097 min
Delta R.T.: 0.019 min
Response: 48763659
Conc: 18.00 ng/ml

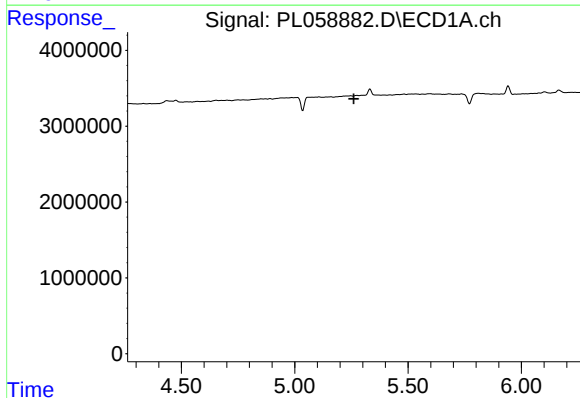


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.261 min
Response: 0
Conc: N.D.

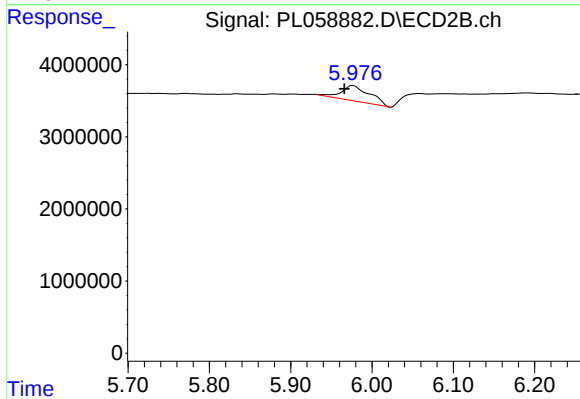

#8 Heptachlor epoxide


R.T.: 5.977 min
Delta R.T.: 0.011 min
Response: 5258465
Conc: 1.59 ng/ml

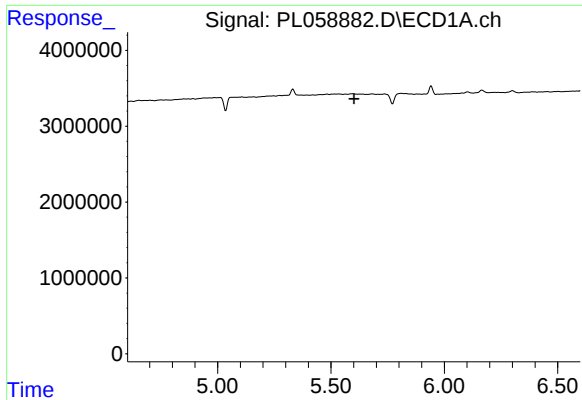

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.603 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
NM42-COMP-2020-0-6MS

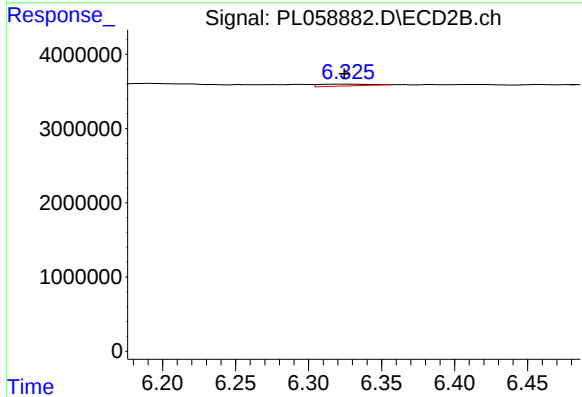


#9 Endosulfan I

R.T.: 6.320 min
Delta R.T.: -0.004 min
Response: 585913
Conc: 0.20 ng/ml

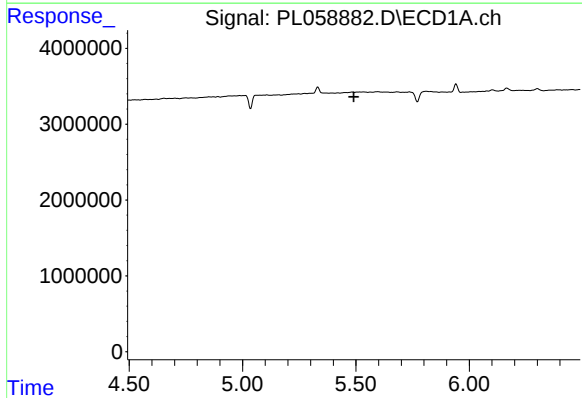


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.490 min
Response: 0
Conc: N.D.

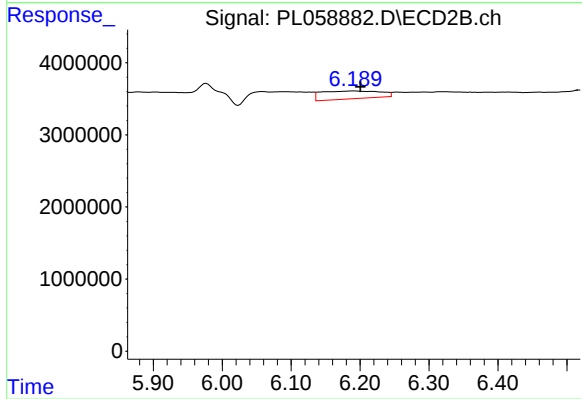

#10 gamma-Chlordane


R.T.: 6.191 min
Delta R.T.: -0.009 min
Response: 6454674
Conc: 1.95 ng/ml

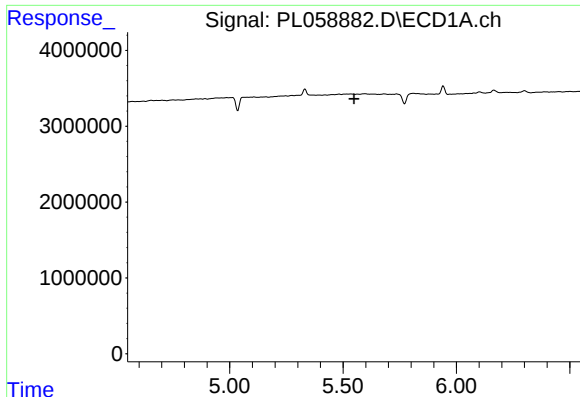

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.549 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
NM42-COMP-2020-0-6MS

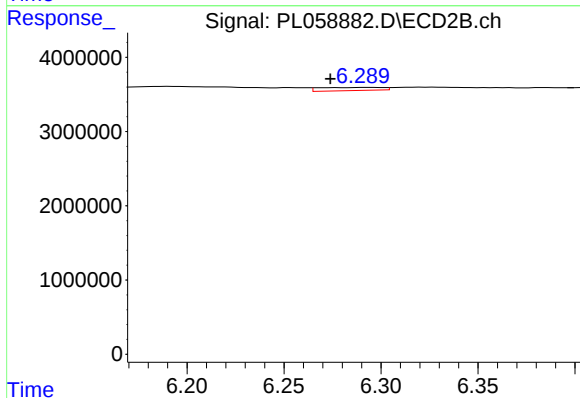


#11 alpha-Chlordane

R.T.: 6.293 min
Delta R.T.: 0.019 min
Response: 944609
Conc: 0.29 ng/ml

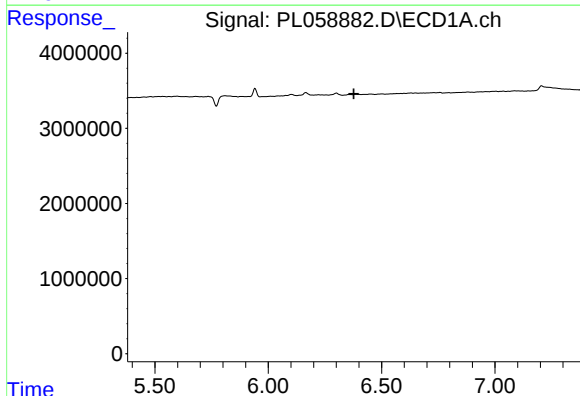


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.377 min
Response: 0
Conc: N.D.

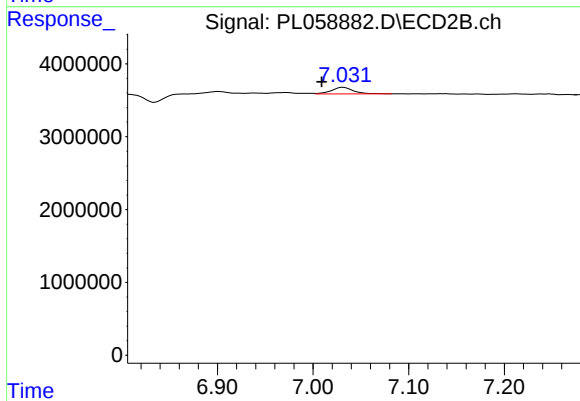

#15 Endosulfan II


R.T.: 7.032 min
Delta R.T.: 0.023 min
Response: 1458368
Conc: 0.52 ng/ml

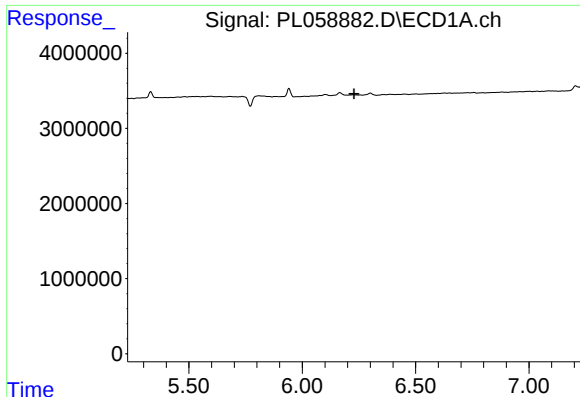

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.229 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
NM42-COMP-2020-0-6MS

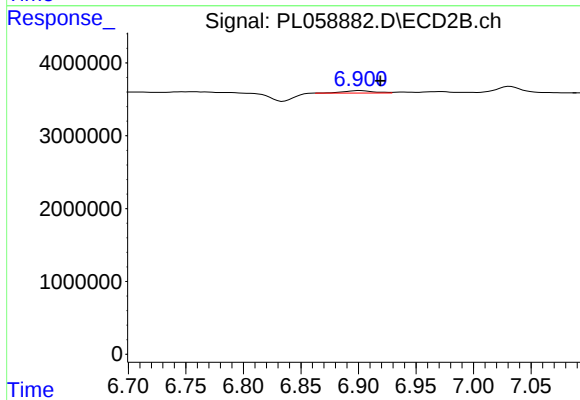


#16 4,4'-DDD

R.T.: 6.901 min
Delta R.T.: -0.018 min
Response: 616603
Conc: 0.26 ng/ml

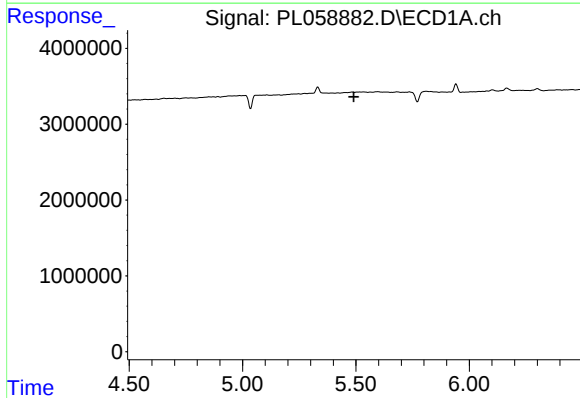


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.491 min
Response: 0
Conc: N.D.

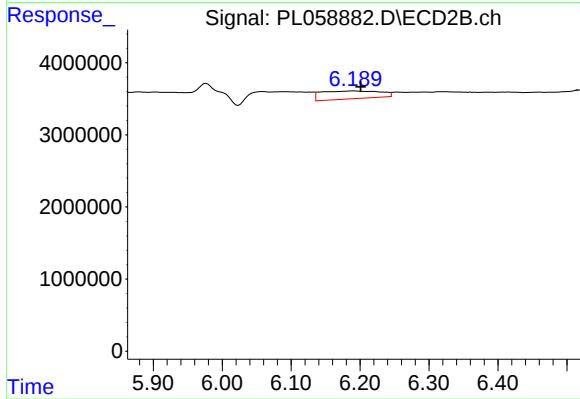

#25 Chlordane-3


R.T.: 6.191 min
Delta R.T.: -0.010 min
Response: 6454674
Conc: 16.96 ng/ml

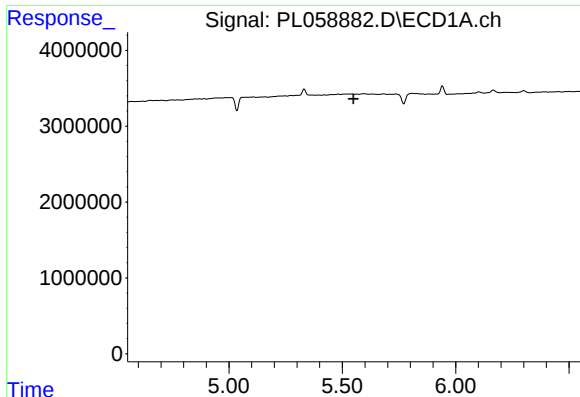

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.549 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
NM42-COMP-2020-0-6MS

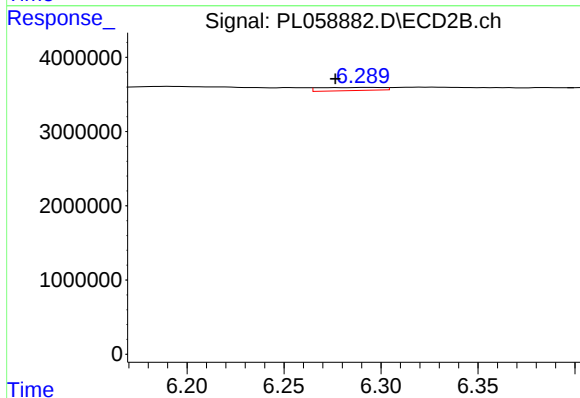


#26 Chlordane-4

R.T.: 6.293 min
Delta R.T.: 0.017 min
Response: 944609
Conc: 2.07 ng/ml

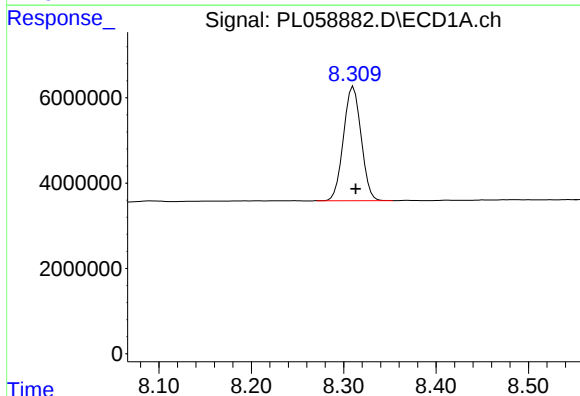

#28 Decachlorobiphenyl

R.T.: 8.311 min
Delta R.T.: -0.002 min
Response: 35580244
Conc: 21.06 ng/ml

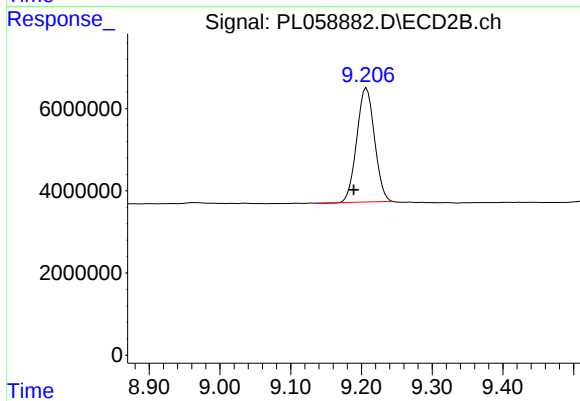

#28 Decachlorobiphenyl

R.T.: 9.207 min
Delta R.T.: 0.018 min
Response: 48440653
Conc: 18.38 ng/ml