

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052620\
 Data File : PL058897.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2020 19:43
 Operator : AJ\MA
 Sample : L2745-10 10X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NM64-COMP-2020-0-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 05:16:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
 Quant Title : GC Extractables
 QLast Update : Wed May 20 11:27:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.530	4.077	1436982	1898870	0.784	0.701
28)	SA Decachlor...	8.310	9.190	1633233	3055800	0.967	1.159
Target Compounds							
2)	A alpha-BHC	3.982	0.000	3627339	0	1.334	N.D. #
4)	MA Heptachlor	0.000	5.274	0	321043	N.D.	0.084 #
7)	B delta-BHC	0.000	5.119f	0	2037076	N.D.	0.559 #
11)	B alpha-Chl...	0.000	6.274	0	891357	N.D.	0.274 #
15)	B Endosulfa...	0.000	7.015	0	1047809	N.D.	0.374 #
19)	B Endosulfa...	0.000	7.346	0	273294	N.D.	0.104 #
20)	A Methoxychlor	0.000	7.701f	0	954530	N.D.	0.684 #
26)	Chlordane-4	0.000	6.274	0	891357	N.D.	1.957 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052620\
Data File : PL058897.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2020 19:43
Operator : AJ\MA
Sample : L2745-10 10X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
NM64-COMP-2020-0-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 05:16:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
Quant Title : GC Extractables
QLast Update : Wed May 20 11:27:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

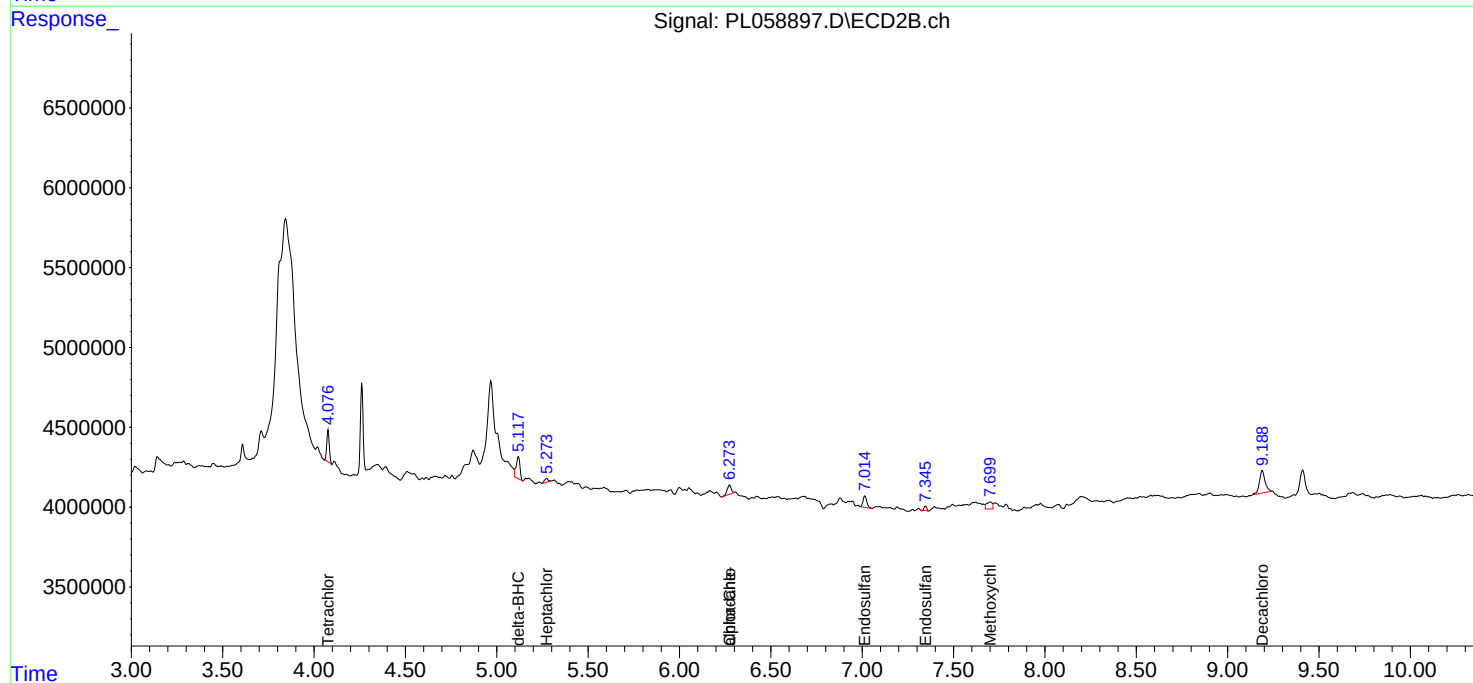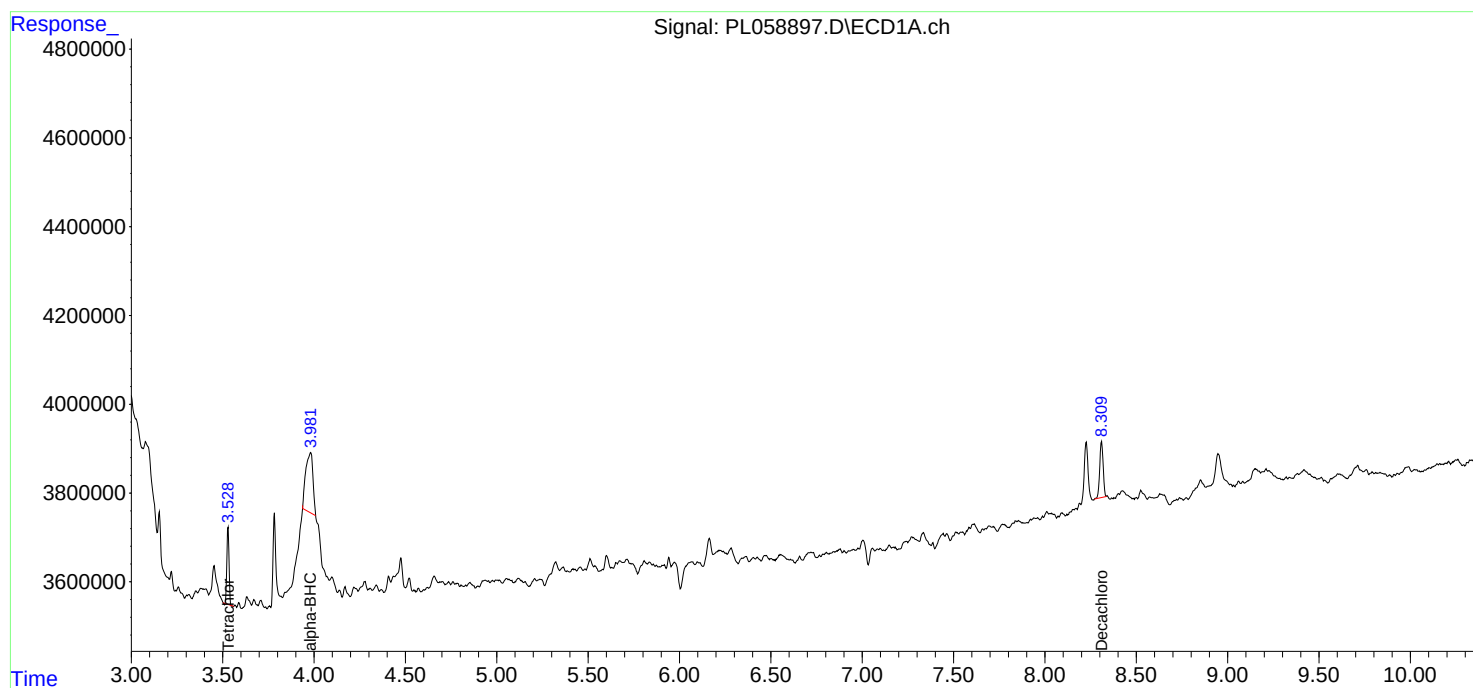


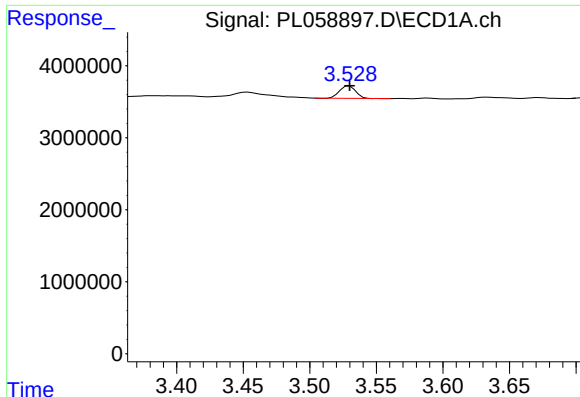

#1 Tetrachloro-m-xylene


R.T.: 3.530 min
Delta R.T.: 0.000 min
Response: 1436982
Conc: 0.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
NM64-COMP-2020-0-6

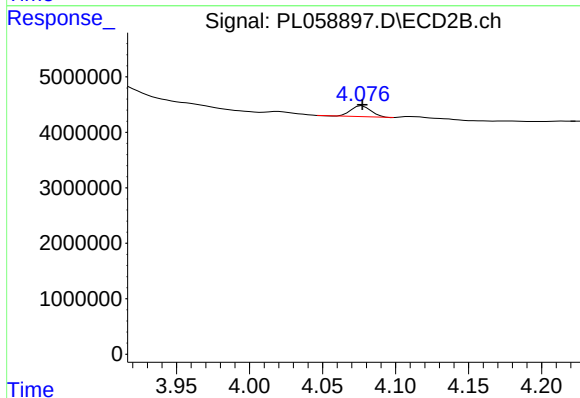


#1 Tetrachloro-m-xylene

R.T.: 4.077 min
Delta R.T.: 0.000 min
Response: 1898870
Conc: 0.70 ng/ml

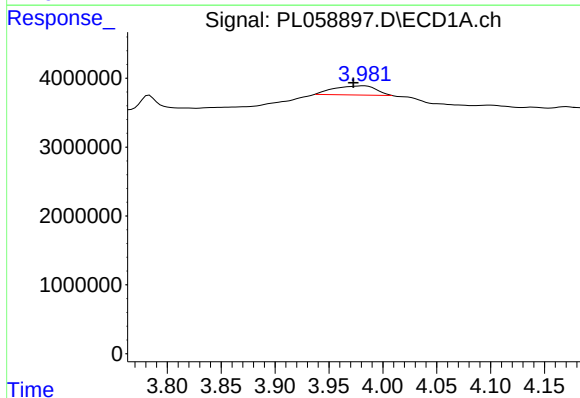


#2 alpha-BHC

R.T.: 3.982 min
Delta R.T.: 0.010 min
Response: 3627339
Conc: 1.33 ng/ml

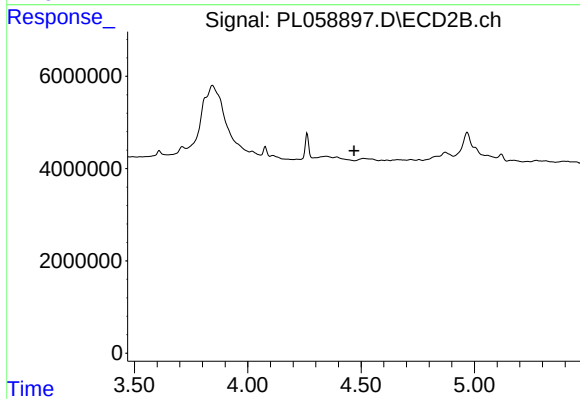

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.469 min
Response: 0
Conc: N.D.

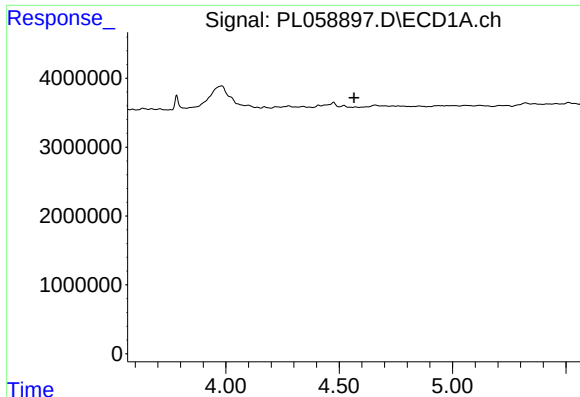

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.566 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
NM64-COMP-2020-0-6

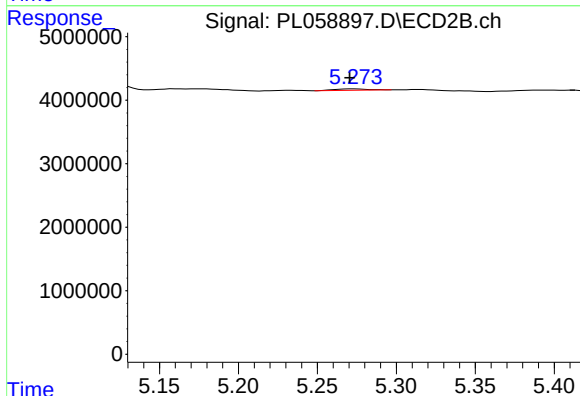


#4 Heptachlor

R.T.: 5.274 min
Delta R.T.: 0.003 min
Response: 321043
Conc: 0.08 ng/ml

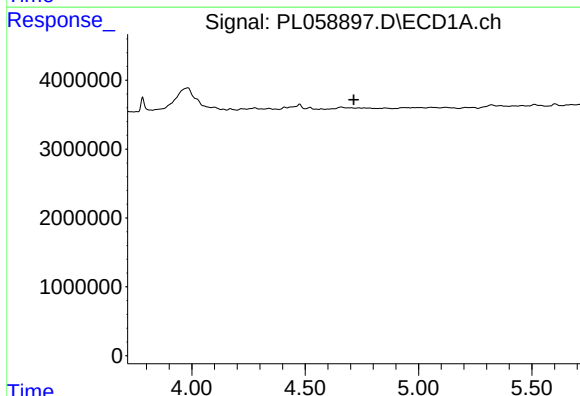


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.715 min
Response: 0
Conc: N.D.

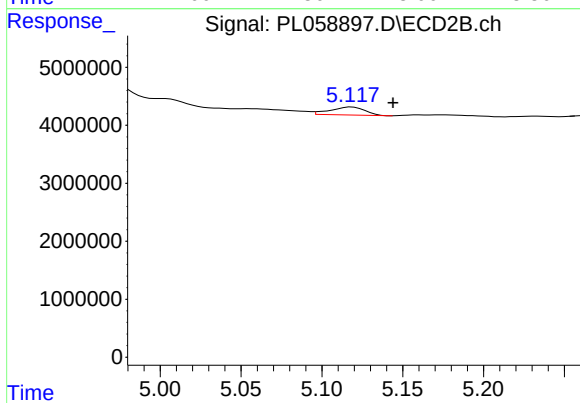

#7 delta-BHC


R.T.: 5.119 min
Delta R.T.: -0.025 min
Response: 2037076
Conc: 0.56 ng/ml

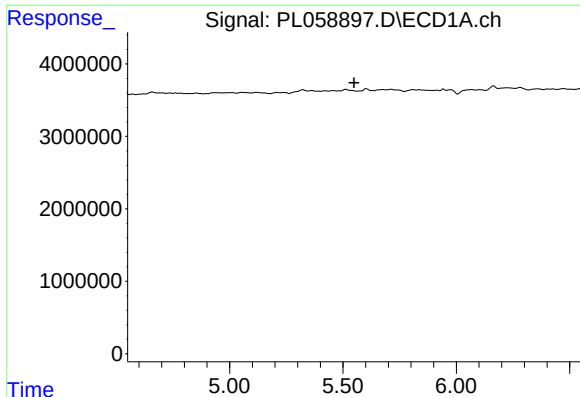

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.549 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
NM64-COMP-2020-0-6

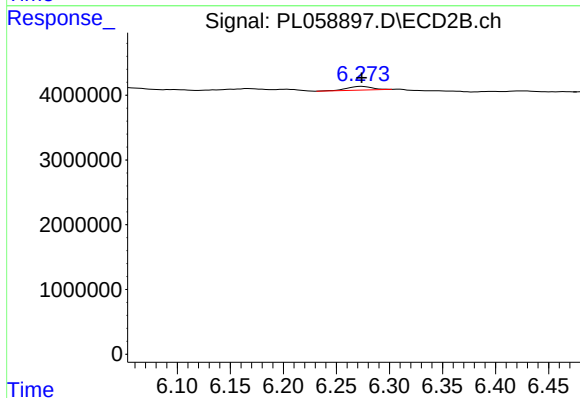


#11 alpha-Chlordane

R.T.: 6.274 min
Delta R.T.: 0.000 min
Response: 891357
Conc: 0.27 ng/ml

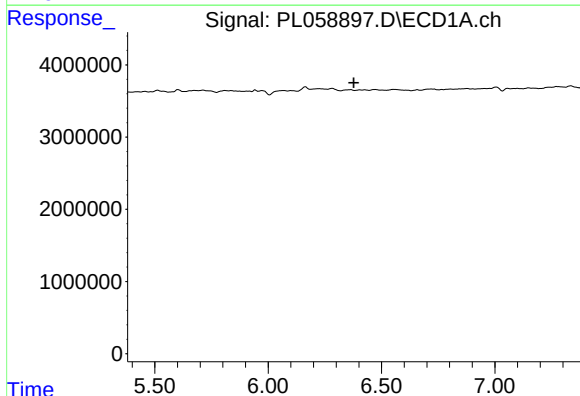


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.377 min
Response: 0
Conc: N.D.

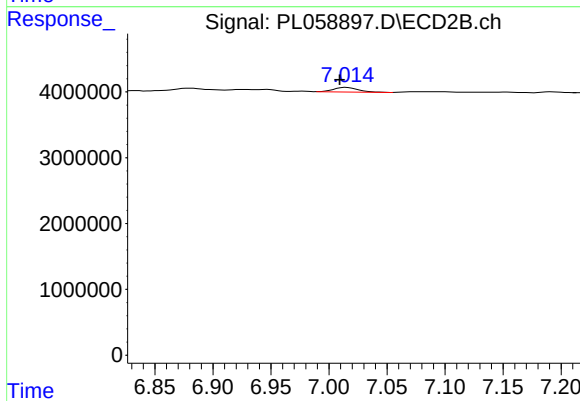

#15 Endosulfan II


R.T.: 7.015 min
Delta R.T.: 0.006 min
Response: 1047809
Conc: 0.37 ng/ml

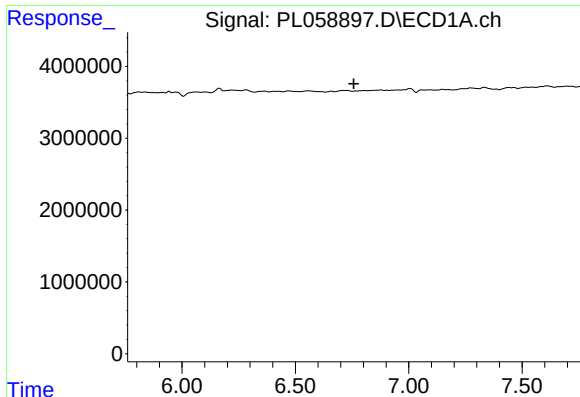

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.758 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
NM64-COMP-2020-0-6

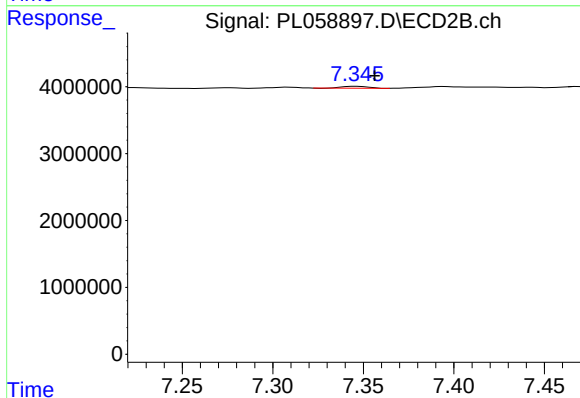


#19 Endosulfan Sulfate

R.T.: 7.346 min
Delta R.T.: -0.010 min
Response: 273294
Conc: 0.10 ng/ml

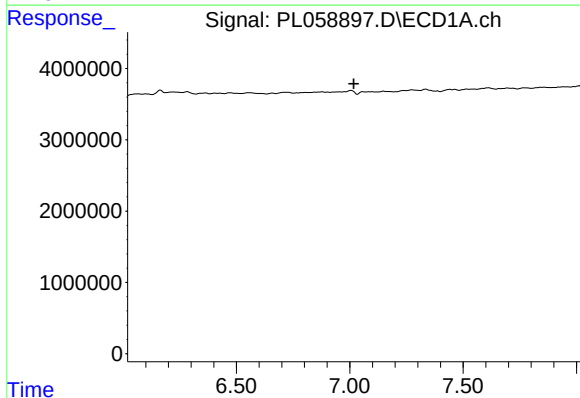


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 7.018 min
Response: 0
Conc: N.D.

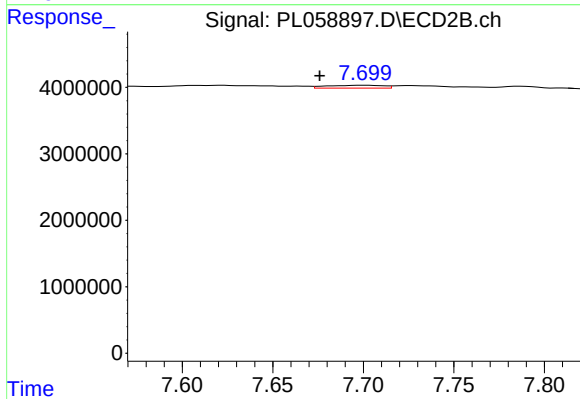

#20 Methoxychlor


R.T.: 7.701 min
Delta R.T.: 0.025 min
Response: 954530
Conc: 0.68 ng/ml

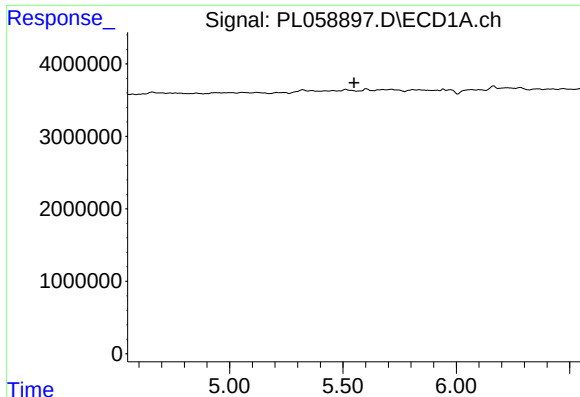

#26 Chlorodane-4


R.T.: 0.000 min
Exp R.T.: 5.549 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
NM64-COMP-2020-0-6

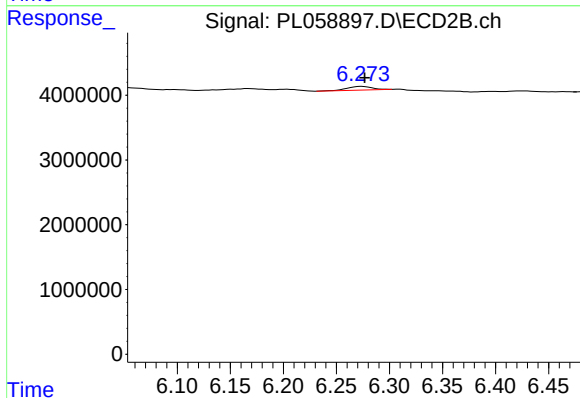


#26 Chlorodane-4

R.T.: 6.274 min
Delta R.T.: -0.002 min
Response: 891357
Conc: 1.96 ng/ml

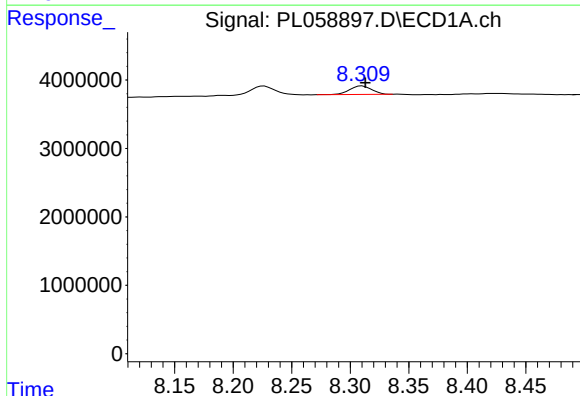

#28 Decachlorobiphenyl

R.T.: 8.310 min
Delta R.T.: -0.003 min
Response: 1633233
Conc: 0.97 ng/ml

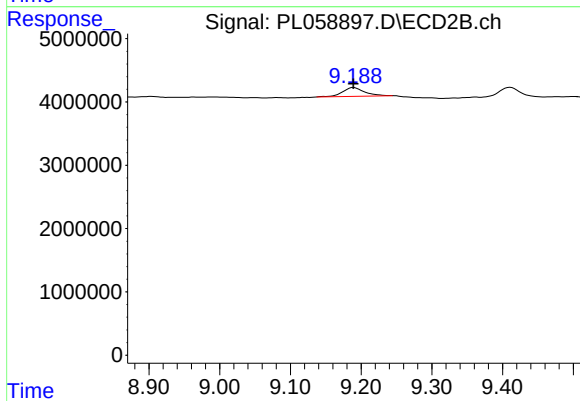

#28 Decachlorobiphenyl

R.T.: 9.190 min
Delta R.T.: 0.000 min
Response: 3055800
Conc: 1.16 ng/ml