

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052620\
 Data File : PL058876.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2020 14:20
 Operator : AJ\MA
 Sample : L2744-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NM54-COMP-2020-0-6

Manual Integrations
 APPROVED

mohammad
 5/28/2020 10:33:30 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 17:00:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
 Quant Title : GC Extractables
 QLast Update : Wed May 20 11:27:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.529	4.076	21432657	29241399	11.689	10.797
28)	SA Decachlor...	8.310	9.188	15036325	19396089	8.900	7.358
Target Compounds							
12)	B 4,4'-DDE	5.710	6.428	897747	3480577	0.547	1.220m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052620\
Data File : PL058876.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2020 14:20
Operator : AJ\MA
Sample : L2744-03
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
NM54-COMP-2020-0-6


Manual Integrations
APPROVED

mohammad
5/28/2020 10:33:30 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 17:00:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
Quant Title : GC Extractables
QLast Update : Wed May 20 11:27:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

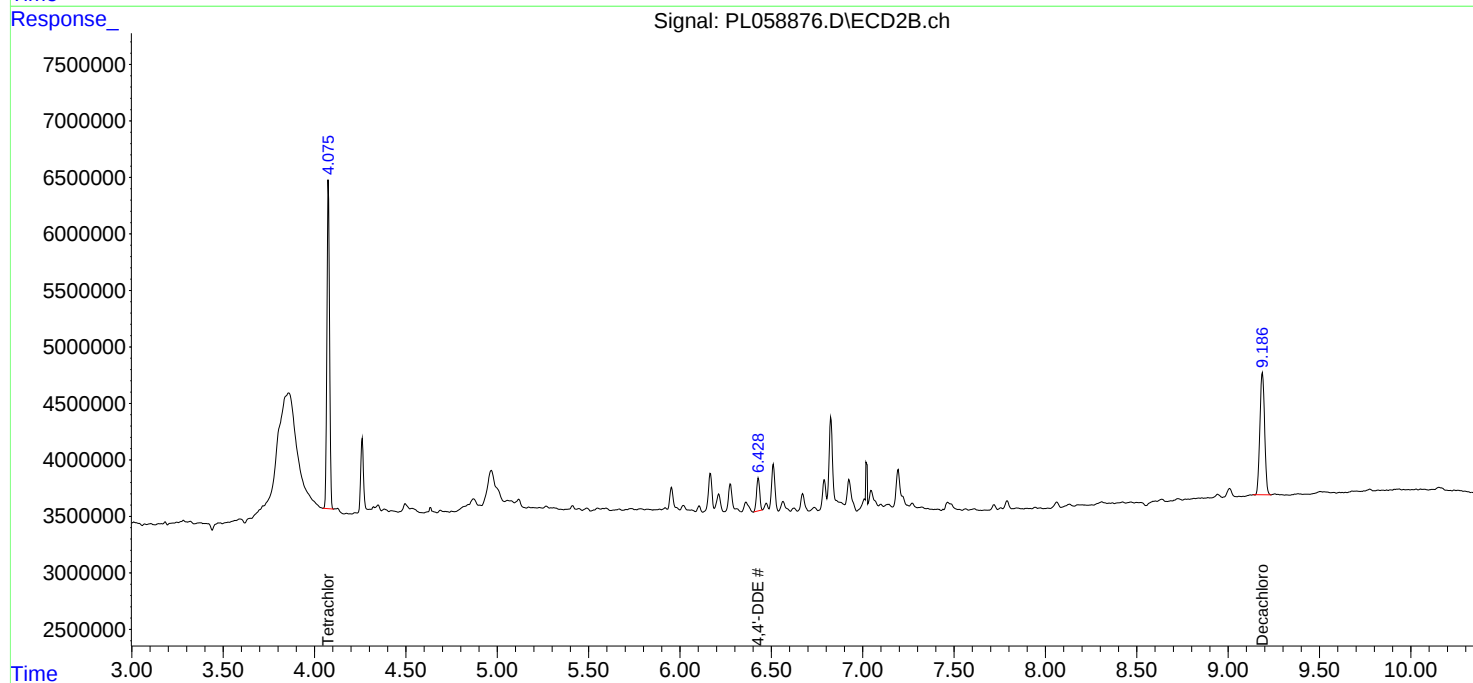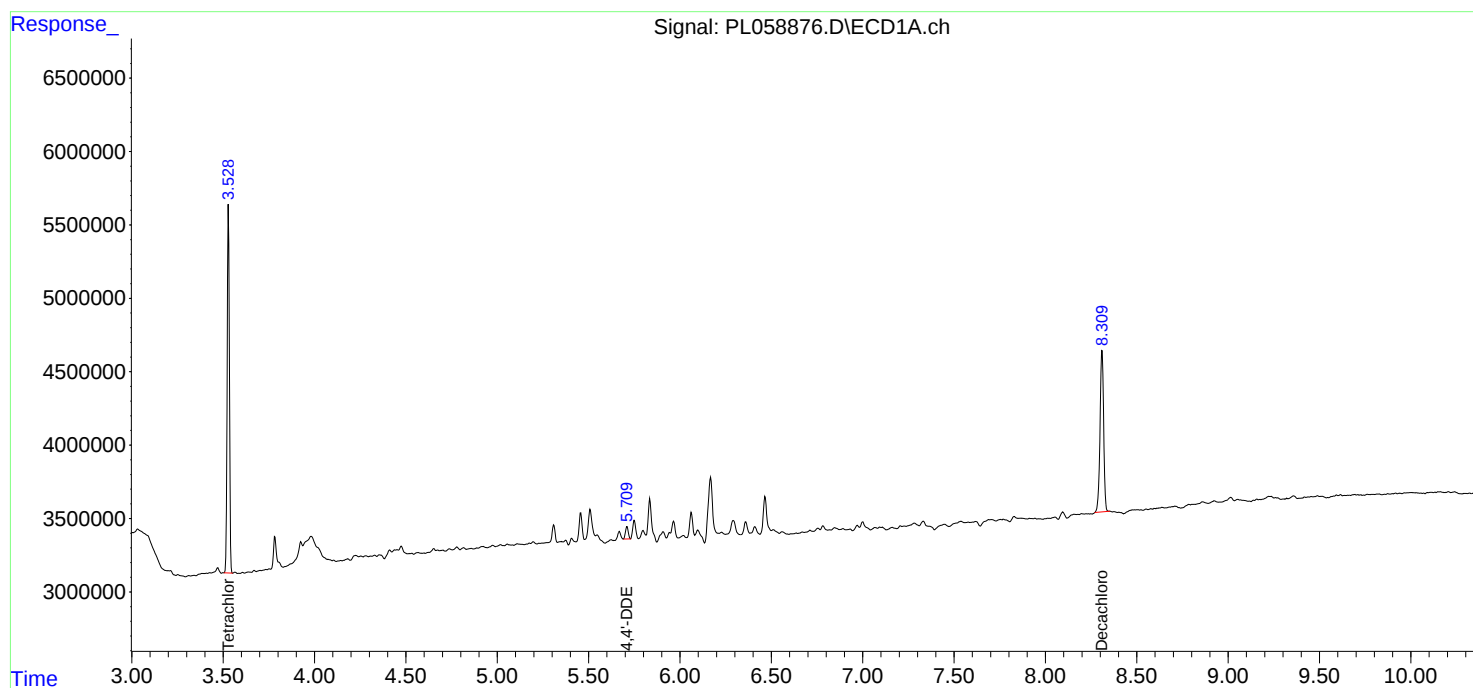

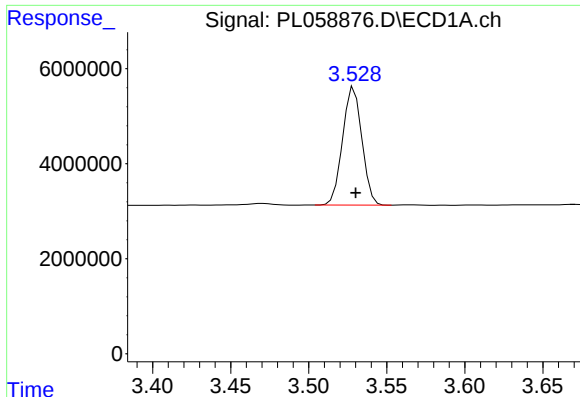


#1 Tetrachloro-m-xylene

R.T.: 3.529 min
Delta R.T.: 0.000 min
Response: 21432657
Conc: 11.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
NM54-COMP-2020-0-6


Manual Integrations
APPROVED

mohammad
5/28/2020 10:33:30 AM

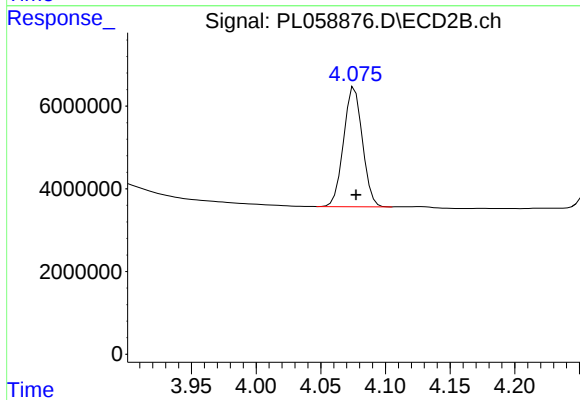


#1 Tetrachloro-m-xylene

R.T.: 4.076 min
Delta R.T.: -0.001 min
Response: 29241399
Conc: 10.80 ng/ml

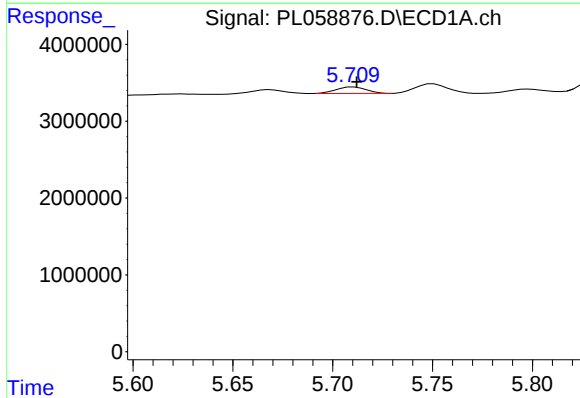


#12 4,4'-DDE

R.T.: 5.710 min
Delta R.T.: -0.002 min
Response: 897747
Conc: 0.55 ng/ml

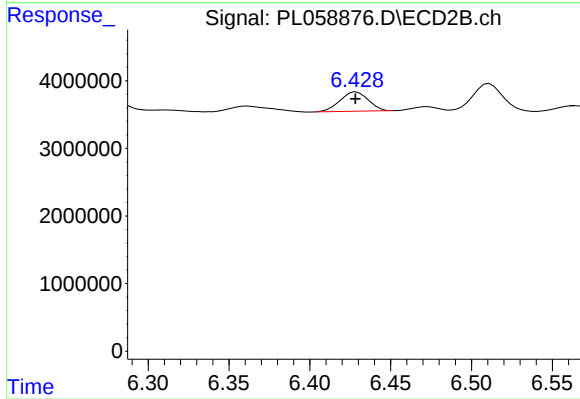

#12 4,4'-DDE

R.T.: 6.428 min
Delta R.T.: 0.000 min
Response: 3480577
Conc: 1.22 ng/ml m

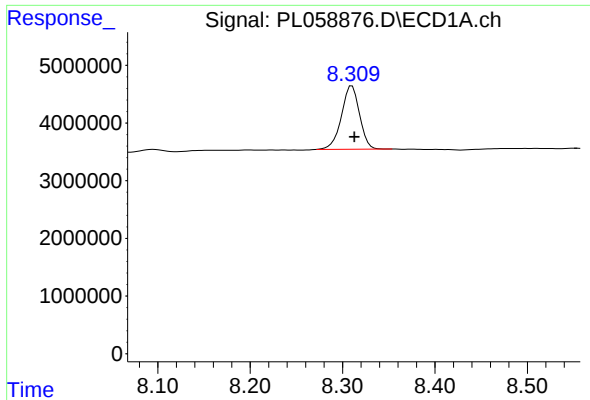


#28 Decachlorobiphenyl

R.T.: 8.310 min
Delta R.T.: -0.003 min
Response: 15036325
Conc: 8.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
NM54-COMP-2020-0-6

Manual Integrations
APPROVED

mohammad
5/28/2020 10:33:30 AM

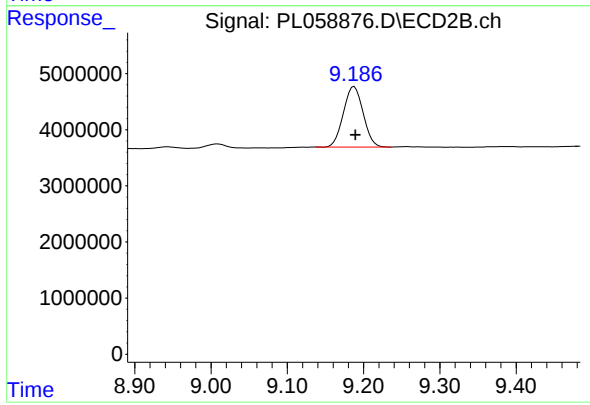

#28 Decachlorobiphenyl

R.T.: 9.188 min
Delta R.T.: -0.002 min
Response: 19396089
Conc: 7.36 ng/ml