

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052620\
 Data File : PL058880.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2020 15:42
 Operator : AJ\MA
 Sample : L2744-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NM52-COMP-2020-0-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 17:01:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
 Quant Title : GC Extractables
 QLast Update : Wed May 20 11:27:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.529	4.076	21542435	29827204	11.748	11.013
28)	SA Decachlor...	8.310	9.188	14806177	19898313	8.763	7.548
Target Compounds							
12)	B 4,4'-DDE	5.711	6.428	1292671	2833888	0.787	0.993 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052620\
Data File : PL058880.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2020 15:42
Operator : AJ\MA
Sample : L2744-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
NM52-COMP-2020-0-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 17:01:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
Quant Title : GC Extractables
QLast Update : Wed May 20 11:27:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

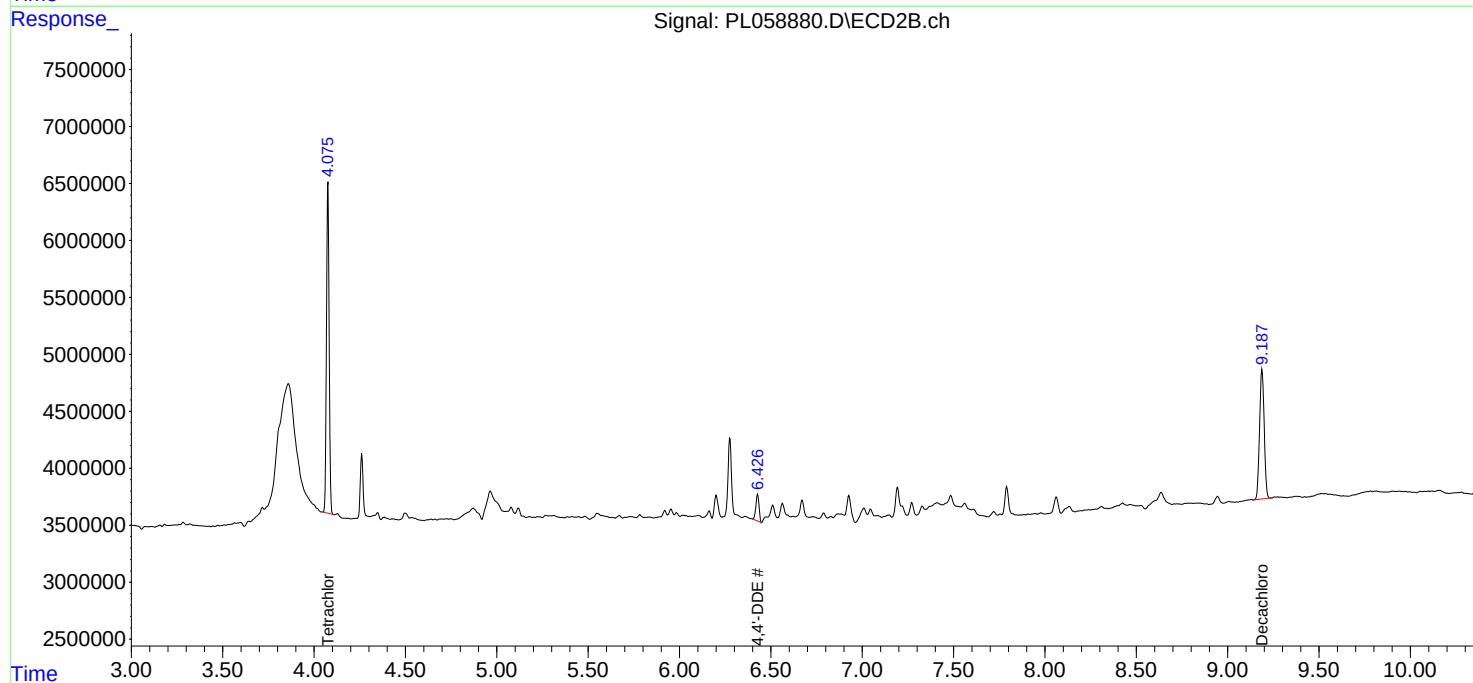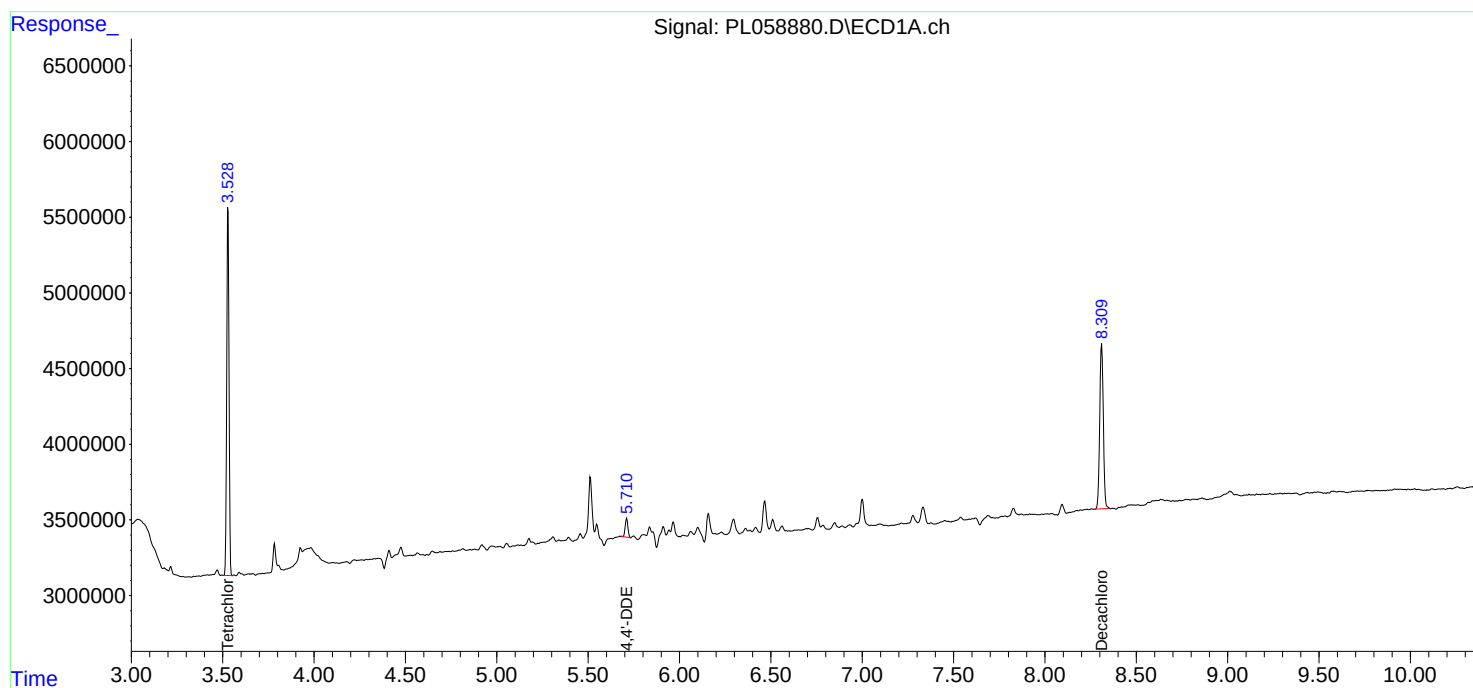


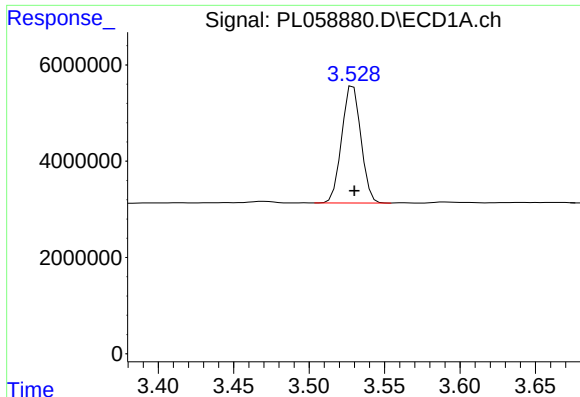

#1 Tetrachloro-m-xylene


R.T.: 3.529 min
Delta R.T.: 0.000 min
Response: 21542435
Conc: 11.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
NM52-COMP-2020-0-6

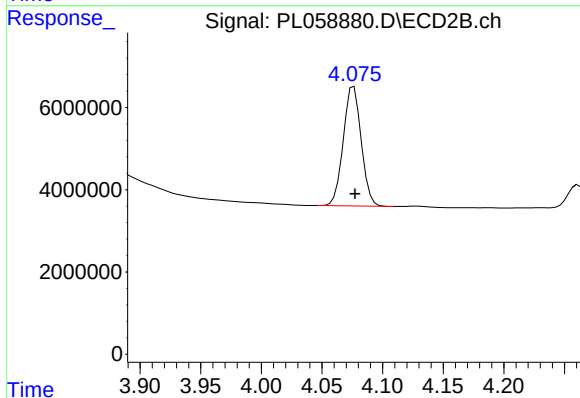


#1 Tetrachloro-m-xylene

R.T.: 4.076 min
Delta R.T.: -0.001 min
Response: 29827204
Conc: 11.01 ng/ml

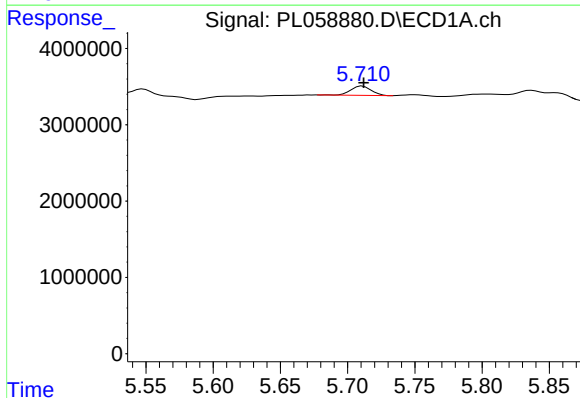


#12 4,4'-DDE

R.T.: 5.711 min
Delta R.T.: -0.001 min
Response: 1292671
Conc: 0.79 ng/ml

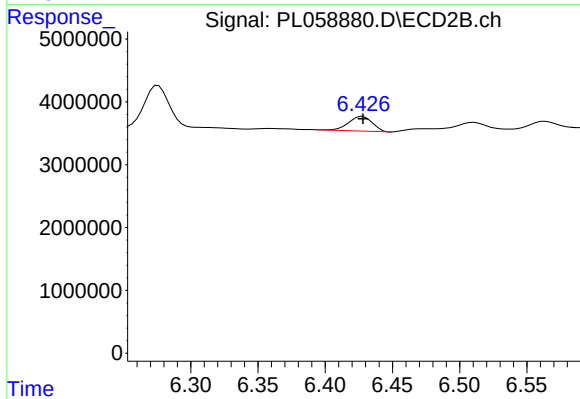

#12 4,4'-DDE


R.T.: 6.428 min
Delta R.T.: 0.000 min
Response: 2833888
Conc: 0.99 ng/ml

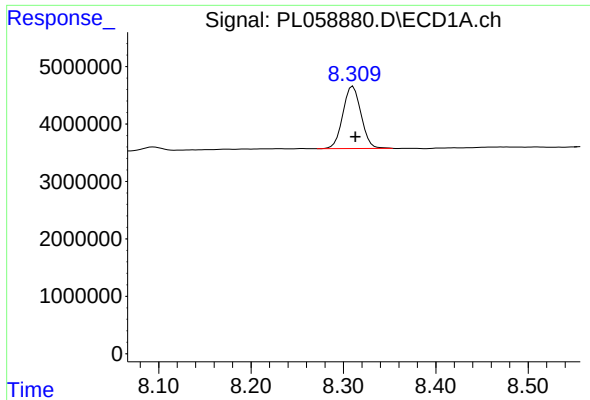

#28 Decachlorobiphenyl

R.T.: 8.310 min
Delta R.T.: -0.003 min
Response: 14806177
Conc: 8.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
NM52-COMP-2020-0-6

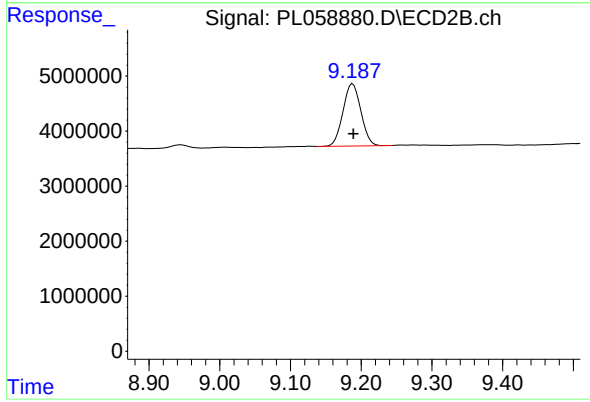

#28 Decachlorobiphenyl

R.T.: 9.188 min
Delta R.T.: -0.001 min
Response: 19898313
Conc: 7.55 ng/ml