

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052621\
 Data File : PL066898.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2021 02:39
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 07:54:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052421.M
 Quant Title : GC Extractables
 QLast Update : Tue May 25 06:06:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.481	5.532	11432931	17078034	19.927	19.883
28)	SA Decachlor...	10.225	11.431	15520785	18585179	20.872	21.568
Target Compounds							
8)	B Heptachlo...	0.000	7.998	0	3978823	N.D.	4.403 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052621\
Data File : PL066898.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2021 02:39
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 07:54:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052421.M
Quant Title : GC Extractables
QLast Update : Tue May 25 06:06:45 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

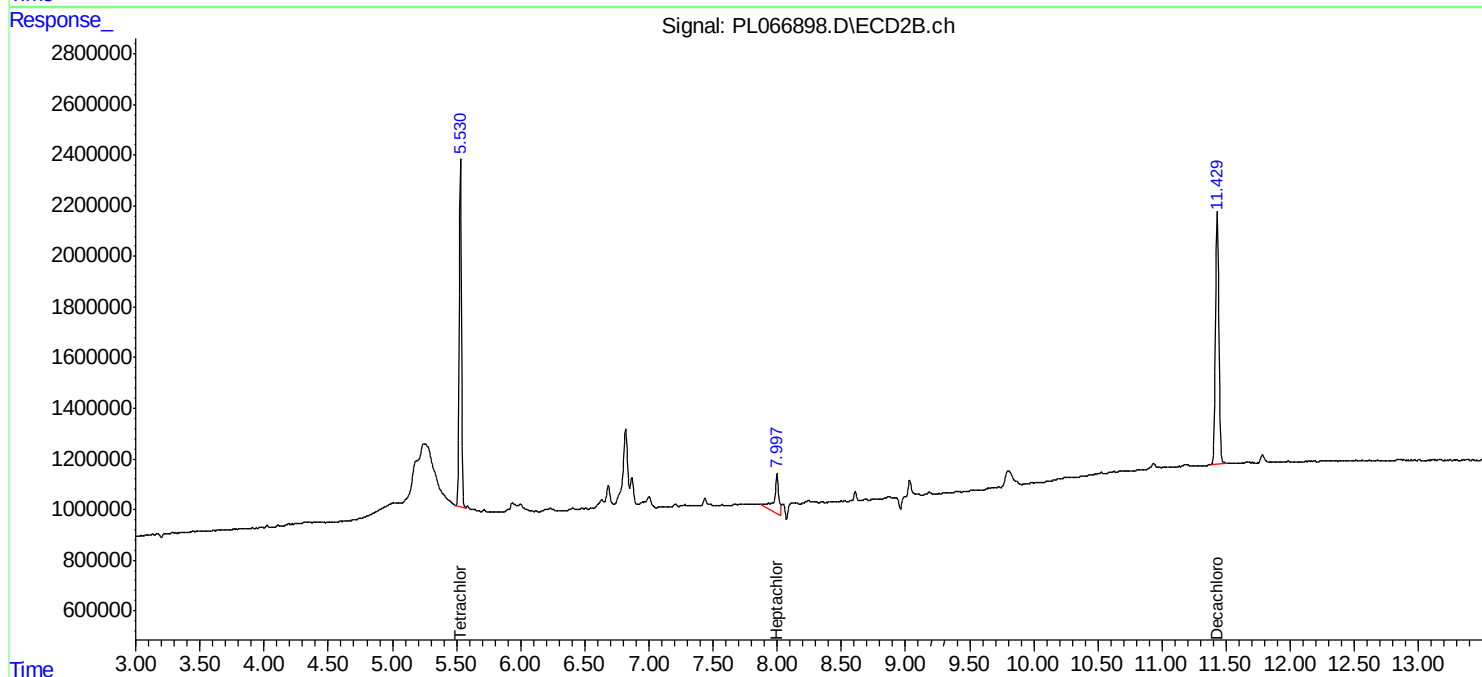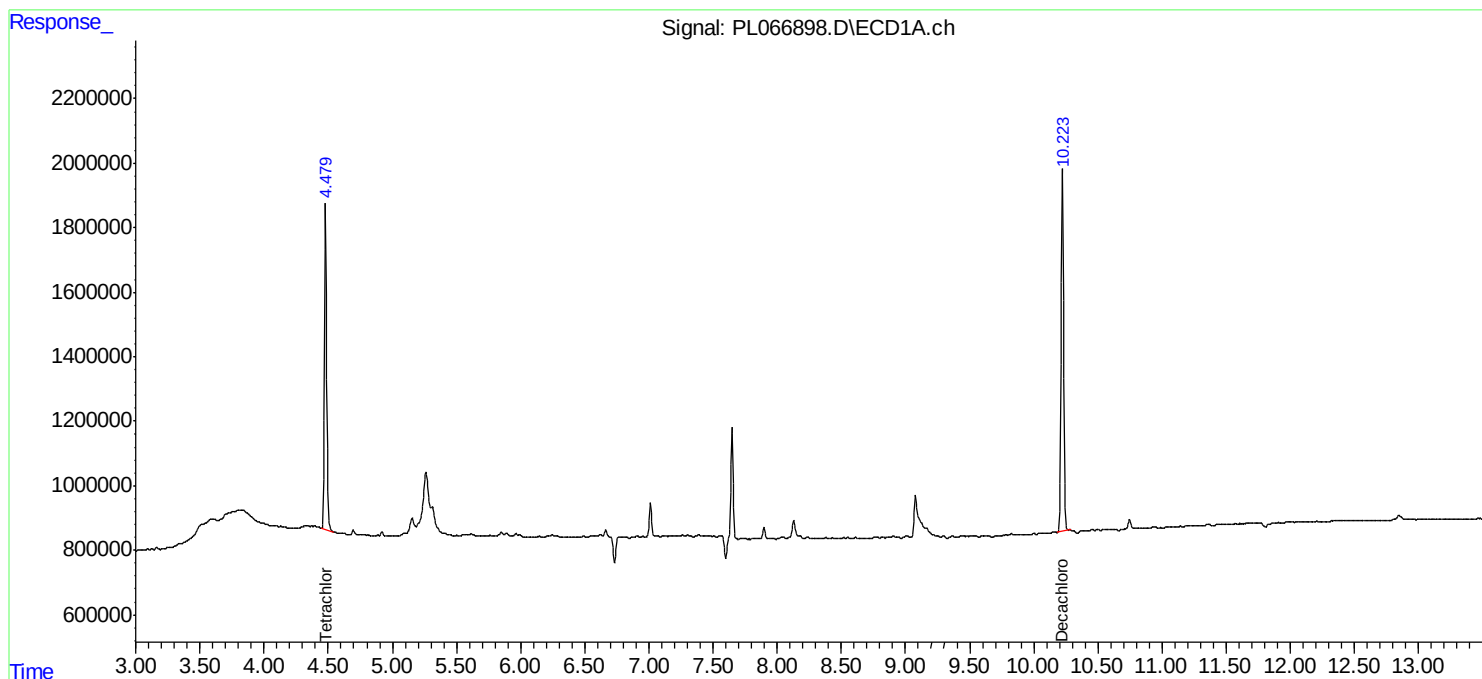


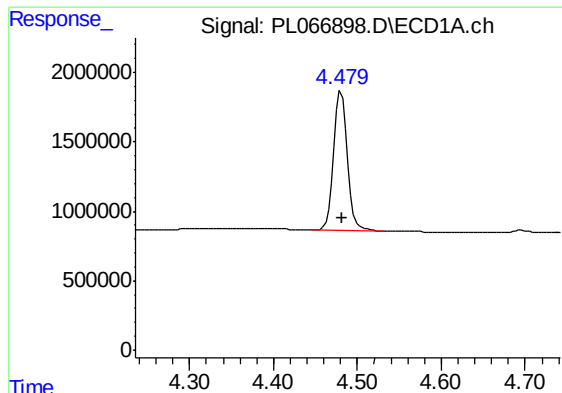

#1 Tetrachloro-m-xylene


R.T.: 4.481 min
Delta R.T.: -0.001 min
Response: 11432931
Conc: 19.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

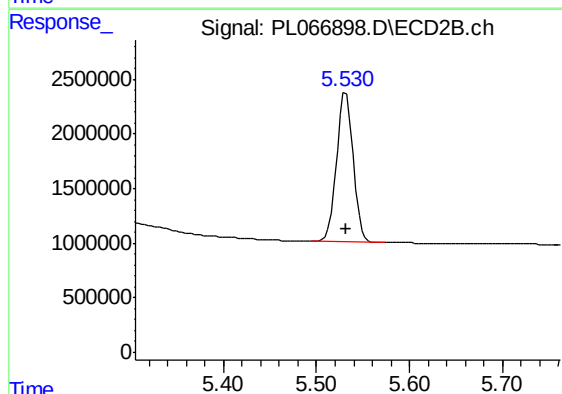


#1 Tetrachloro-m-xylene

R.T.: 5.532 min
Delta R.T.: 0.000 min
Response: 17078034
Conc: 19.88 ng/ml

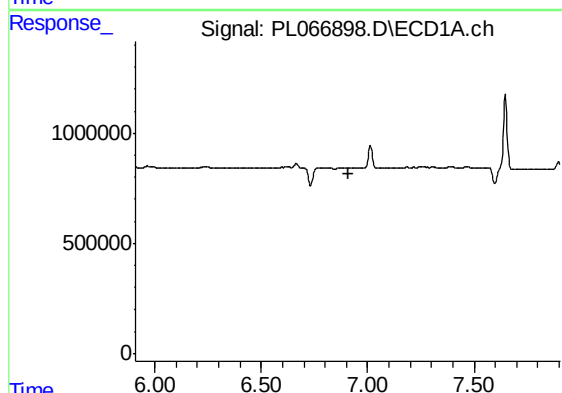


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 6.908 min
Response: 0
Conc: N.D.

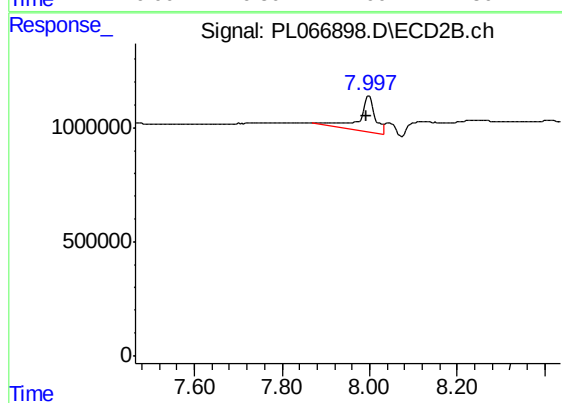

#8 Heptachlor epoxide


R.T.: 7.998 min
Delta R.T.: 0.006 min
Response: 3978823
Conc: 4.40 ng/ml

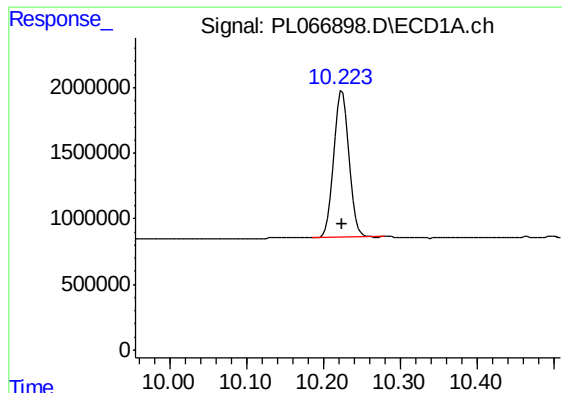

#28 Decachlorobiphenyl

R.T.: 10.225 min
Delta R.T.: 0.000 min
Response: 15520785
Conc: 20.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

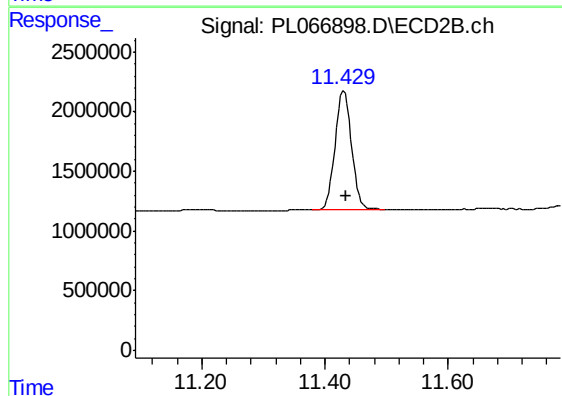

#28 Decachlorobiphenyl

R.T.: 11.431 min
Delta R.T.: -0.002 min
Response: 18585179
Conc: 21.57 ng/ml