

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052623\
 Data File : PL083061.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2023 19:01
 Operator : AR\AJ
 Sample : 02945-06
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB23

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 05/30/2023
 Supervised By :Ankita Jodhani 05/30/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 22:00:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
 Quant Title : GC Extractables
 QLast Update : Sat May 20 04:58:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.315	2.636	28034864	25744688	9.539	9.917
28)	SA Decachlor...	8.729	7.739	21861674	25854810	10.424	10.398
Target Compounds							
12)	B 4,4'-DDE	5.942	5.066	1950447	1608133	0.708	0.662m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052623\
Data File : PL083061.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2023 19:01
Operator : AR\AJ
Sample : 02945-06
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SB23


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/30/2023
Supervised By : Ankita Jodhani 05/30/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 22:00:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051923.M
Quant Title : GC Extractables
QLast Update : Sat May 20 04:58:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

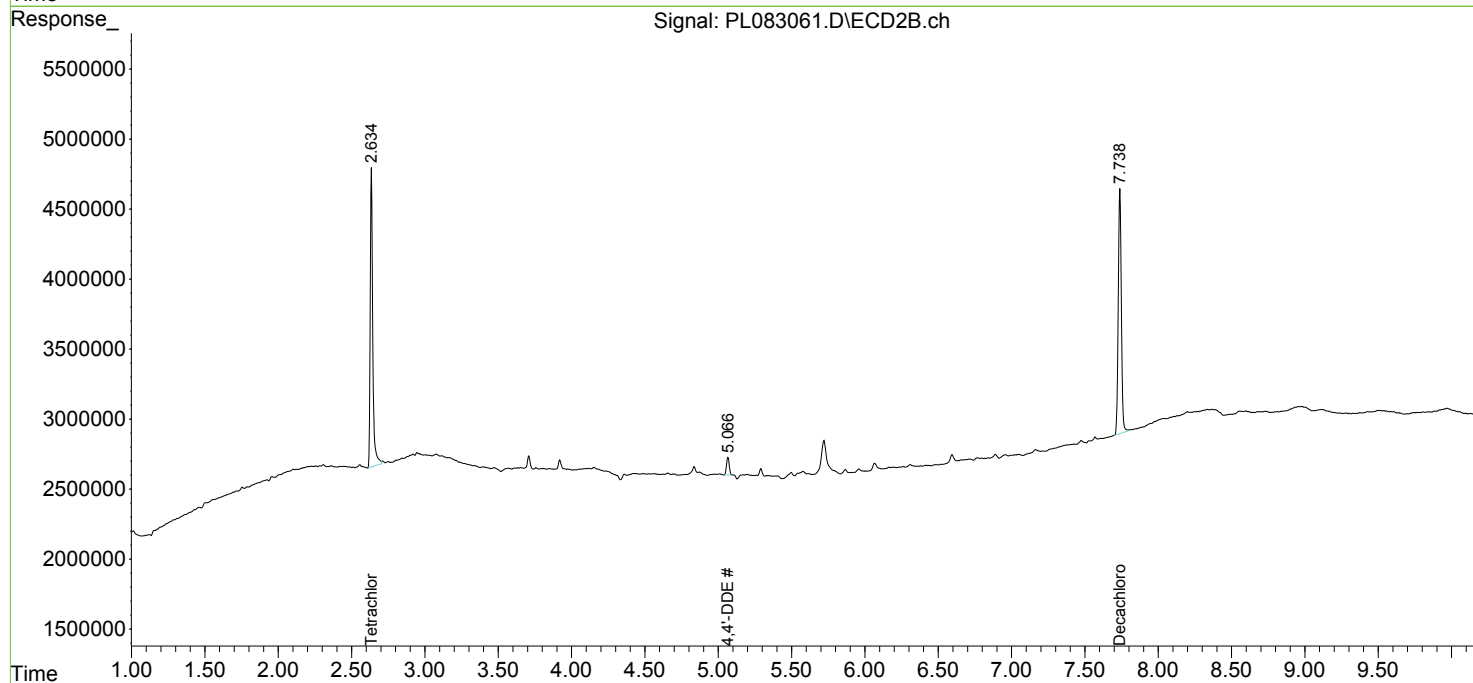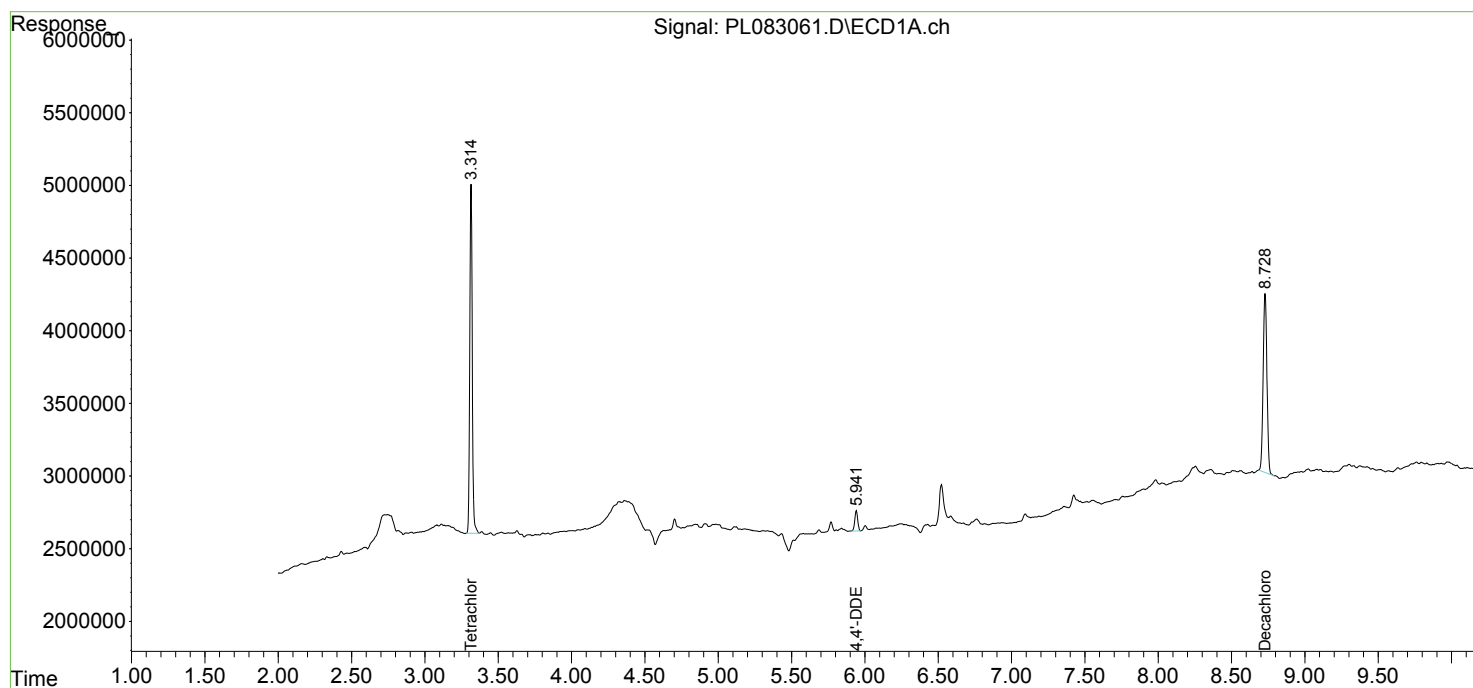

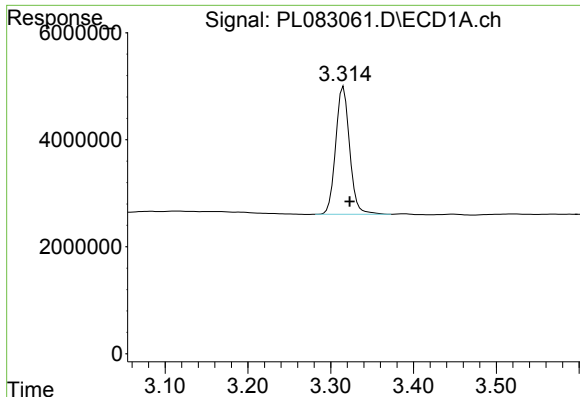


#1 Tetrachloro-m-xylene

R.T.: 3.315 min
Delta R.T.: -0.008 min
Response: 28034864
Conc: 9.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB23


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/30/2023
Supervised By :Ankita Jodhani 05/30/2023

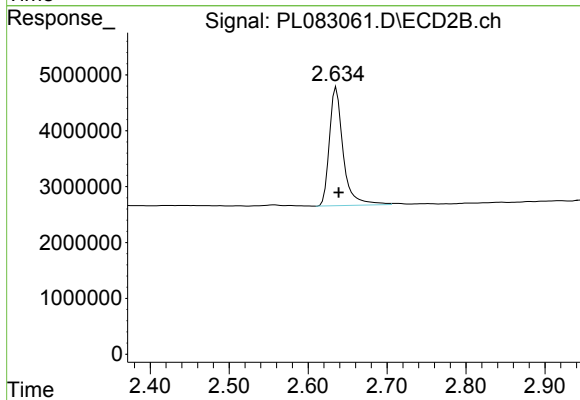


#1 Tetrachloro-m-xylene

R.T.: 2.636 min
Delta R.T.: -0.003 min
Response: 25744688
Conc: 9.92 ng/ml

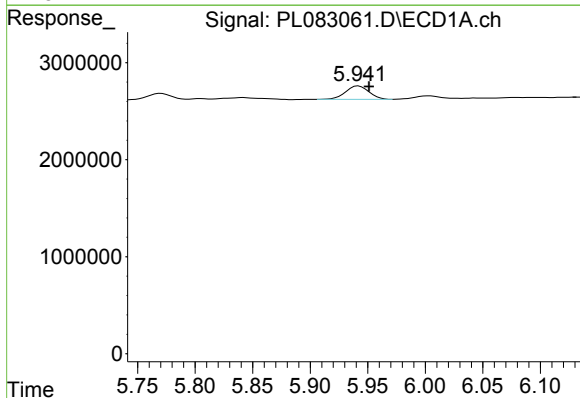


#12 4,4'-DDE

R.T.: 5.942 min
Delta R.T.: -0.009 min
Response: 1950447
Conc: 0.71 ng/ml

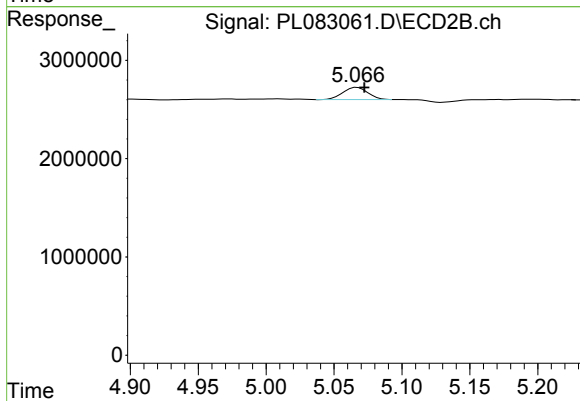

#12 4,4'-DDE

R.T.: 5.066 min
Delta R.T.: -0.007 min
Response: 1608133
Conc: 0.66 ng/ml m

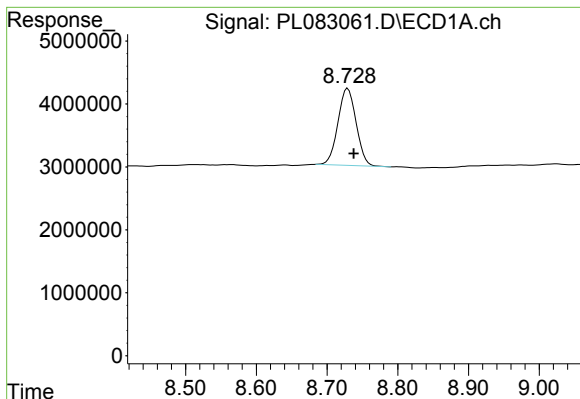


#28 Decachlorobiphenyl

R.T.: 8.729 min
Delta R.T.: -0.009 min
Response: 21861674
Conc: 10.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB23

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/30/2023
Supervised By :Ankita Jodhani 05/30/2023

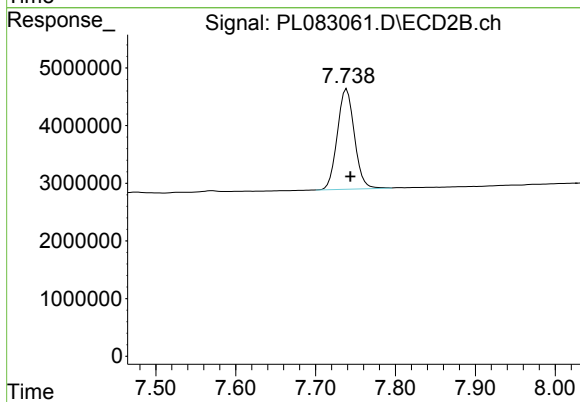

#28 Decachlorobiphenyl

R.T.: 7.739 min
Delta R.T.: -0.004 min
Response: 25854810
Conc: 10.40 ng/ml