

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052720\
 Data File : PL058898.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 May 2020 10:22
 Operator : AJ\MA
 Sample : L2745-15 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NM22-COMP-2020-0-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 12:42:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
 Quant Title : GC Extractables
 QLast Update : Wed May 20 11:27:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.529	4.076	3084334	3658297	1.682	1.351
28)	SA Decachlor...	8.309	9.187	3090104	4259509	1.829	1.616
Target Compounds							
3)	MA gamma-BHC...	0.000	4.753	0	128710	N.D.	0.034 #
4)	MA Heptachlor	0.000	5.269	0	414802	N.D.	0.108 #
7)	B delta-BHC	0.000	5.170f	0	1438105	N.D.	0.394 #
9)	A Endosulfan I	5.601	0.000	1077388	0	0.635	N.D. #
11)	B alpha-Chl...	0.000	6.273	0	3781421	N.D.	1.164 #
12)	B 4,4'-DDE	0.000	6.426	0	417028	N.D.	0.146 #
15)	B Endosulfa...	0.000	7.019	0	775964	N.D.	0.277 #
17)	MA 4,4'-DDT	0.000	7.191f	0	351350	N.D.	0.148 #
19)	B Endosulfa...	0.000	7.345	0	532510	N.D.	0.203 #
20)	A Methoxychlor	0.000	7.694f	0	764661	N.D.	0.548 #
26)	Chlordane-4	0.000	6.273	0	3781421	N.D.	8.304 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052720\
Data File : PL058898.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 May 2020 10:22
Operator : AJ\MA
Sample : L2745-15 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
NM22-COMP-2020-0-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 12:42:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
Quant Title : GC Extractables
QLast Update : Wed May 20 11:27:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

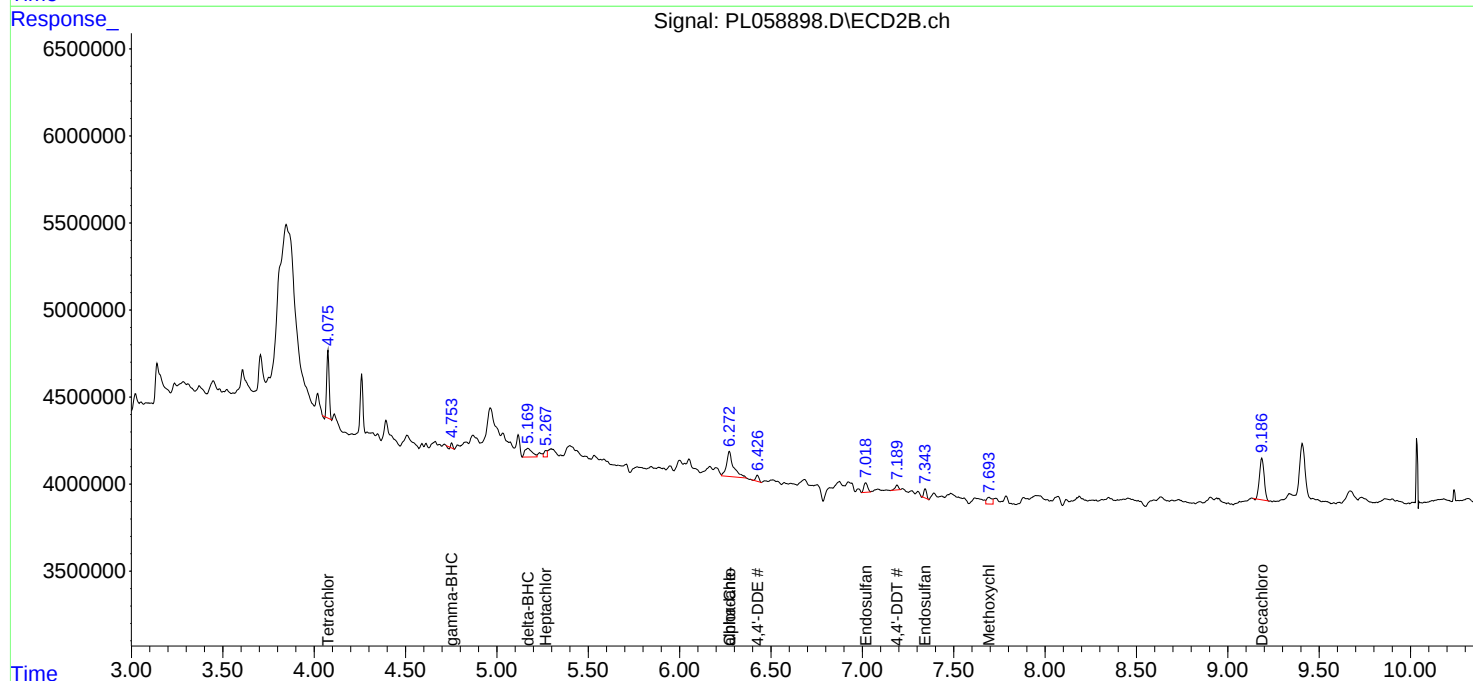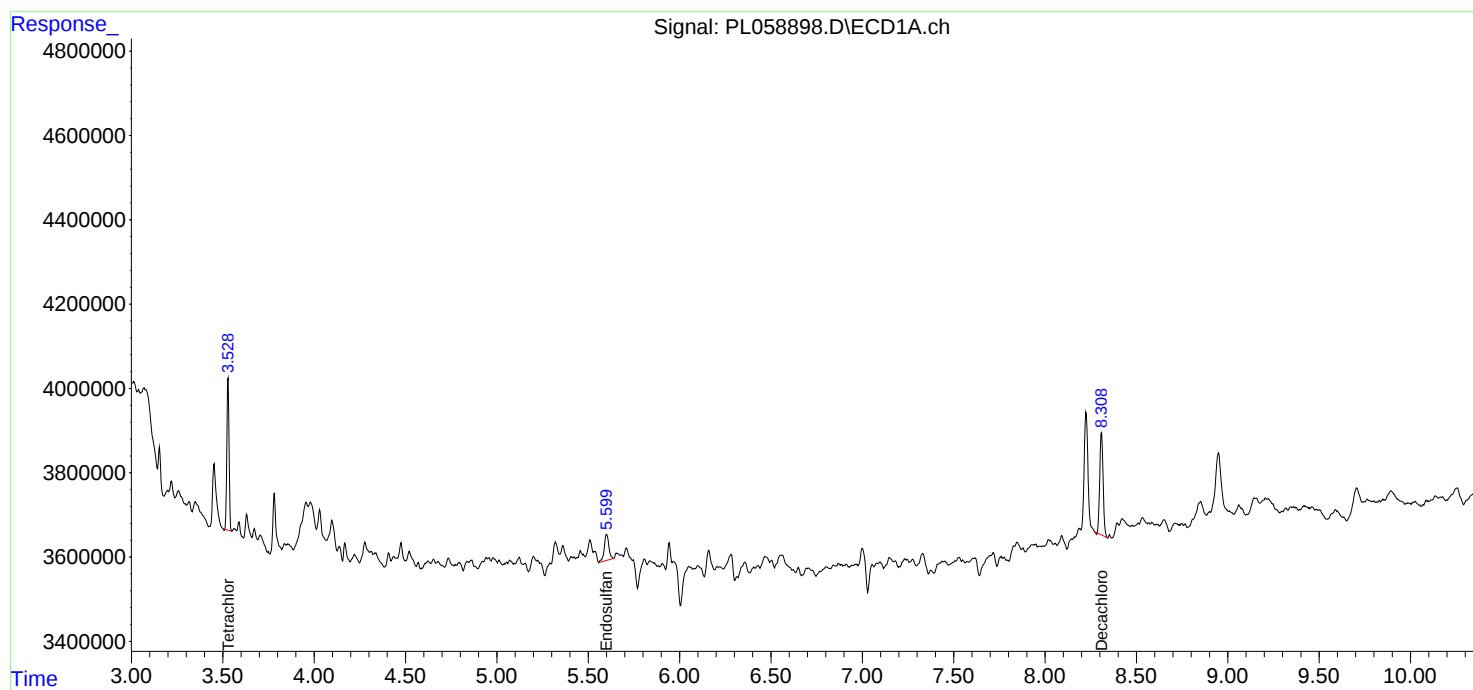


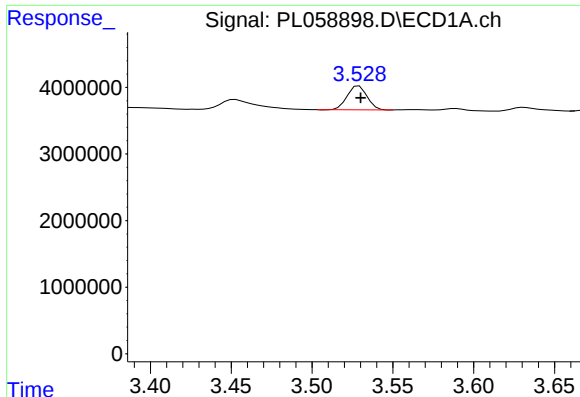

#1 Tetrachloro-m-xylene


R.T.: 3.529 min
Delta R.T.: 0.000 min
Response: 3084334
Conc: 1.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
NM22-COMP-2020-0-6

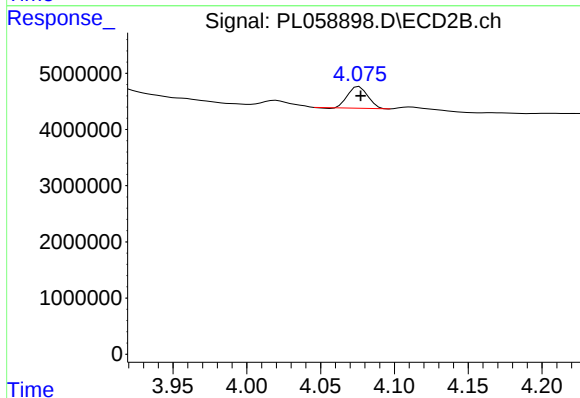


#1 Tetrachloro-m-xylene

R.T.: 4.076 min
Delta R.T.: -0.001 min
Response: 3658297
Conc: 1.35 ng/ml

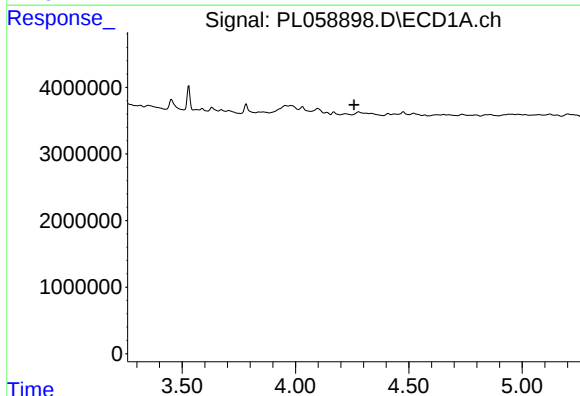


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.258 min
Response: 0
Conc: N.D.

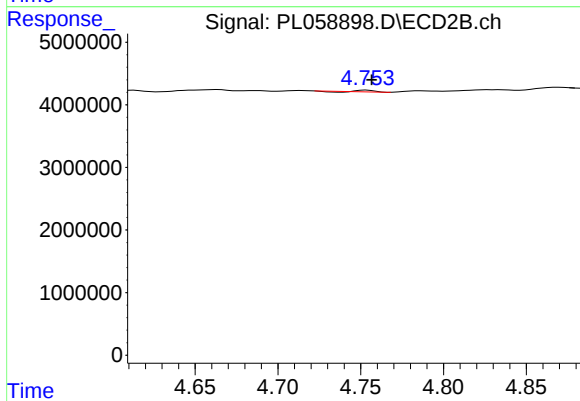

#3 gamma-BHC (Lindane)


R.T.: 4.753 min
Delta R.T.: -0.003 min
Response: 128710
Conc: 0.03 ng/ml

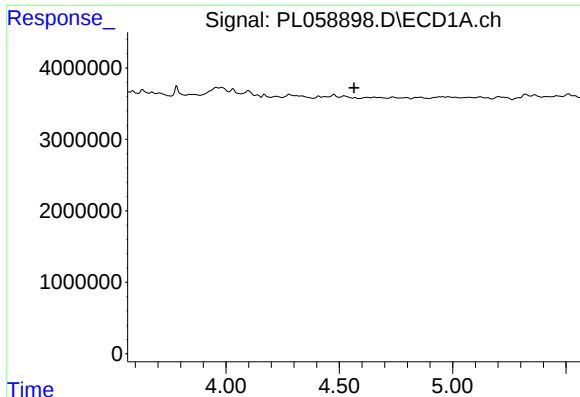

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.566 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
NM22-COMP-2020-0-6

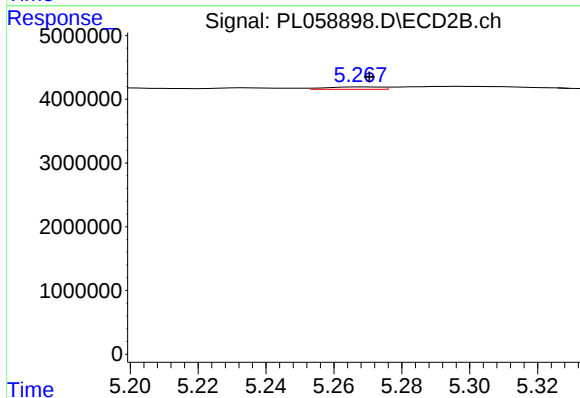


#4 Heptachlor

R.T.: 5.269 min
Delta R.T.: -0.002 min
Response: 414802
Conc: 0.11 ng/ml

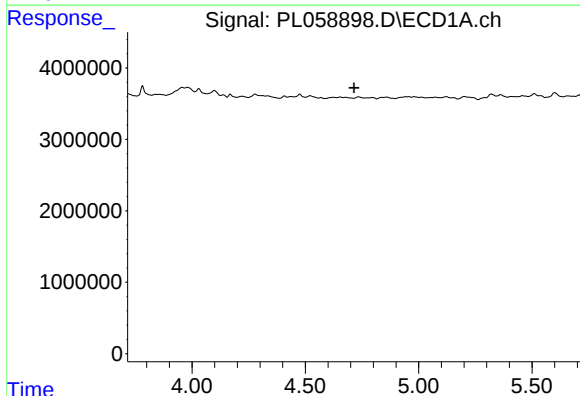


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.715 min
Response: 0
Conc: N.D.

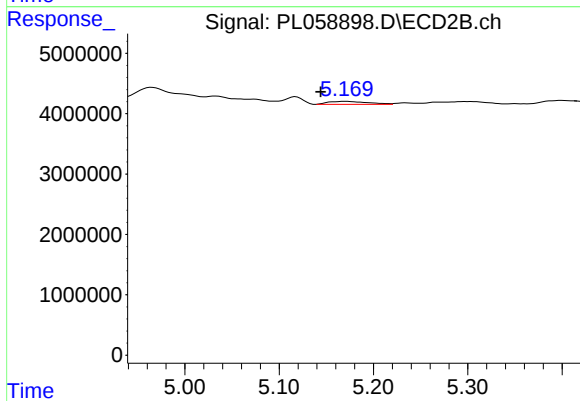

#7 delta-BHC


R.T.: 5.170 min
Delta R.T.: 0.026 min
Response: 1438105
Conc: 0.39 ng/ml

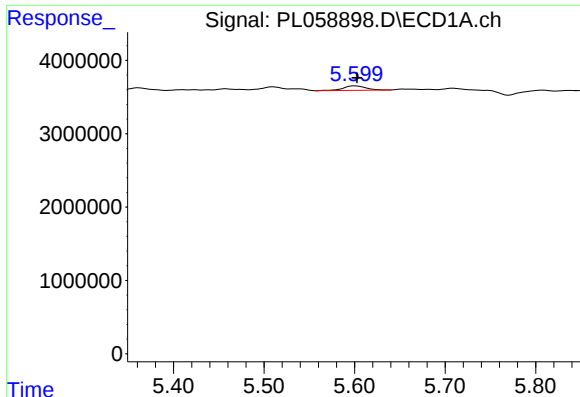

#9 Endosulfan I


R.T.: 5.601 min
Delta R.T.: -0.002 min
Response: 1077388
Conc: 0.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
NM22-COMP-2020-0-6

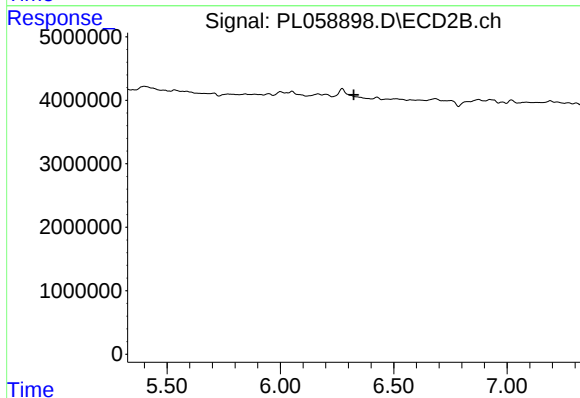


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.325 min
Response: 0
Conc: N.D.

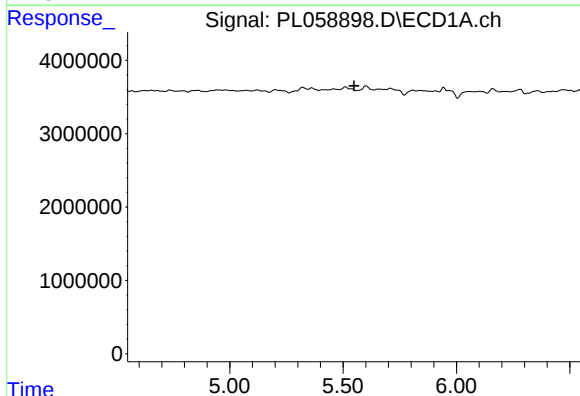


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.549 min
Response: 0
Conc: N.D.

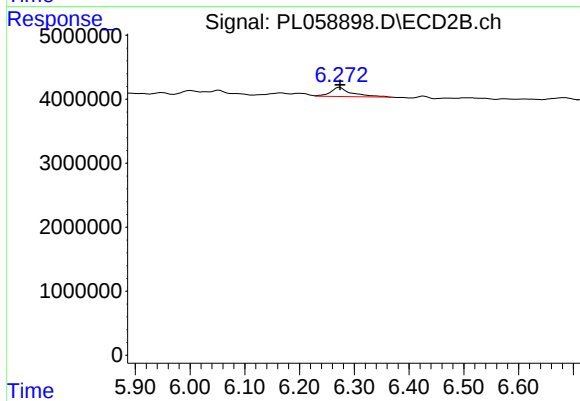

#11 alpha-Chlordane


R.T.: 6.273 min
Delta R.T.: -0.001 min
Response: 3781421
Conc: 1.16 ng/ml

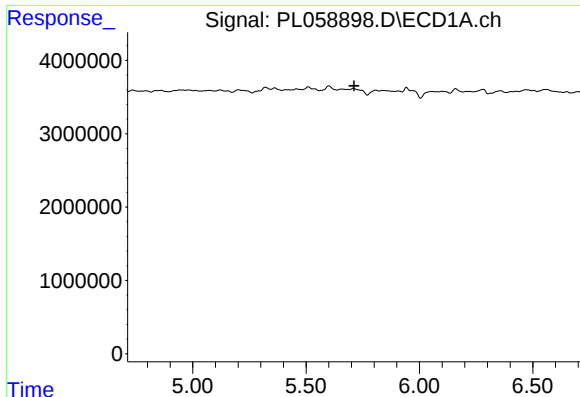

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.712 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
NM22-COMP-2020-0-6

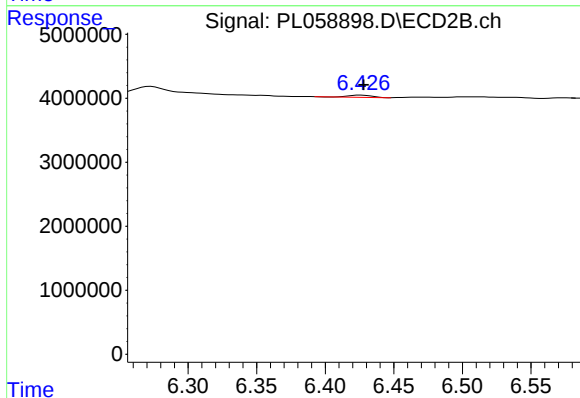


#12 4,4'-DDE

R.T.: 6.426 min
Delta R.T.: -0.002 min
Response: 417028
Conc: 0.15 ng/ml

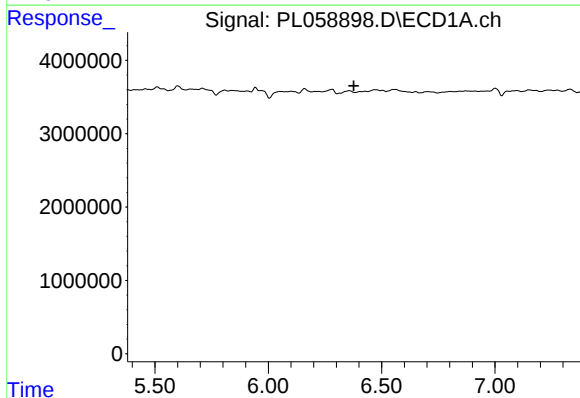


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.377 min
Response: 0
Conc: N.D.

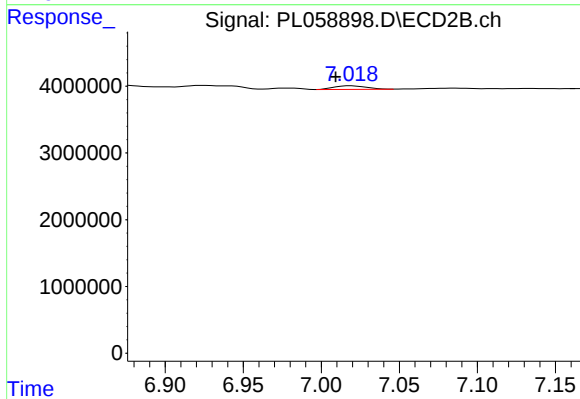

#15 Endosulfan II

R.T.: 7.019 min
Delta R.T.: 0.010 min
Response: 775964
Conc: 0.28 ng/ml

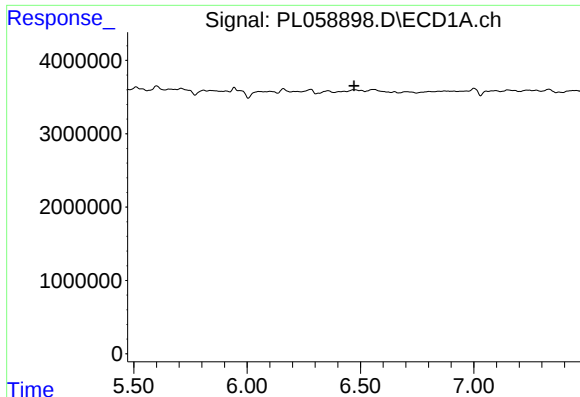

#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.471 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
NM22-COMP-2020-0-6

#17 4,4'-DDT


R.T.: 7.191 min
Delta R.T.: -0.028 min
Response: 351350
Conc: 0.15 ng/ml

#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 6.758 min
Response: 0
Conc: N.D.

#19 Endosulfan Sulfate


R.T.: 7.345 min
Delta R.T.: -0.012 min
Response: 532510
Conc: 0.20 ng/ml

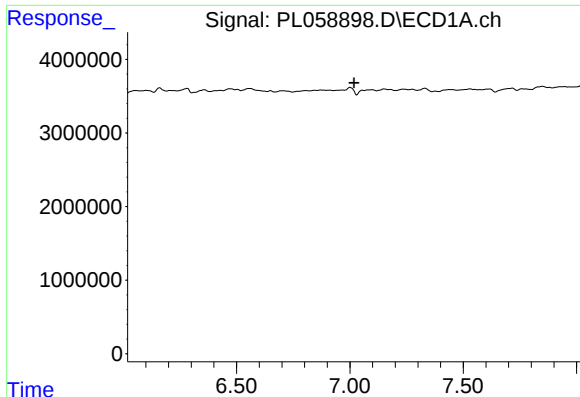

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.018 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
NM22-COMP-2020-0-6

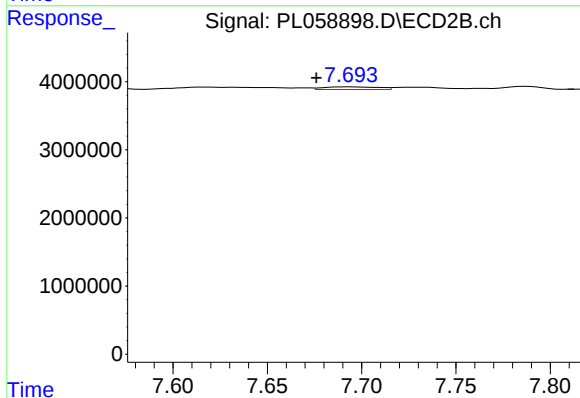


#20 Methoxychlor

R.T.: 7.694 min
Delta R.T.: 0.018 min
Response: 764661
Conc: 0.55 ng/ml

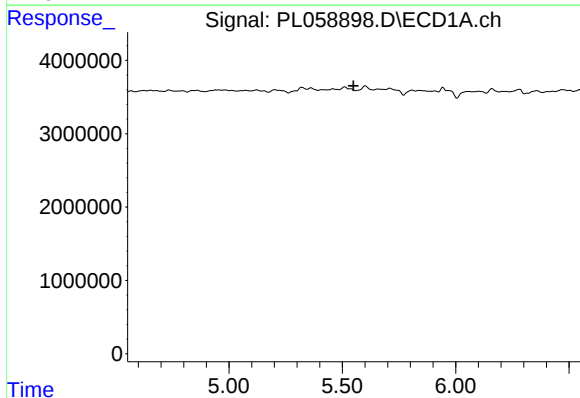


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.549 min
Response: 0
Conc: N.D.

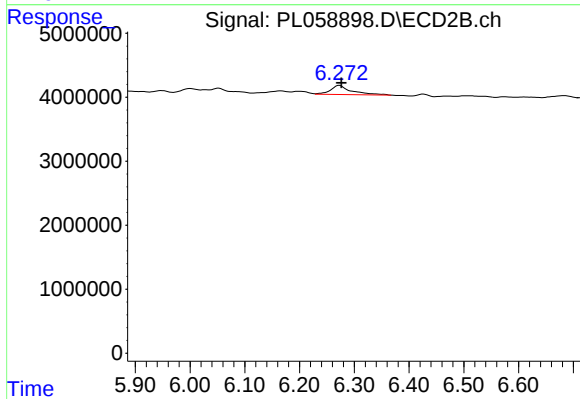

#26 Chlordane-4


R.T.: 6.273 min
Delta R.T.: -0.004 min
Response: 3781421
Conc: 8.30 ng/ml

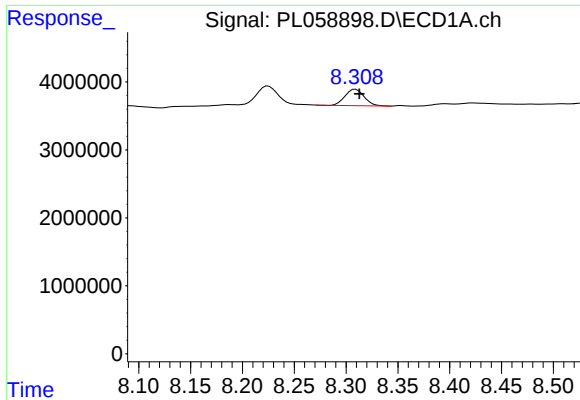

#28 Decachlorobiphenyl

R.T.: 8.309 min
Delta R.T.: -0.004 min
Response: 3090104
Conc: 1.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
NM22-COMP-2020-0-6

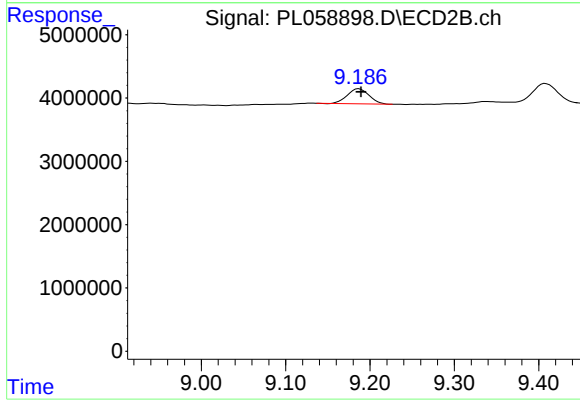

#28 Decachlorobiphenyl

R.T.: 9.187 min
Delta R.T.: -0.002 min
Response: 4259509
Conc: 1.62 ng/ml