

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052720\
 Data File : PL058923.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 May 2020 17:08
 Operator : AJ\MA
 Sample : L2757-01 5X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 C0AP3

Manual Integrations
 APPROVED

mohammad
 5/29/2020 12:32:07 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 28 02:30:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
 Quant Title : GC Extractables
 QLast Update : Wed May 20 11:27:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.522	4.078	16589274	5376548	9.047m	1.985m#
28) SA Decachlor...	8.307	9.184	6315215	6697816	3.738	2.541m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052720\
Data File : PL058923.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 May 2020 17:08
Operator : AJ\MA
Sample : L2757-01 5X
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
C0AP3


Manual Integrations
APPROVED

mohammad
5/29/2020 12:32:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 02:30:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
Quant Title : GC Extractables
QLast Update : Wed May 20 11:27:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

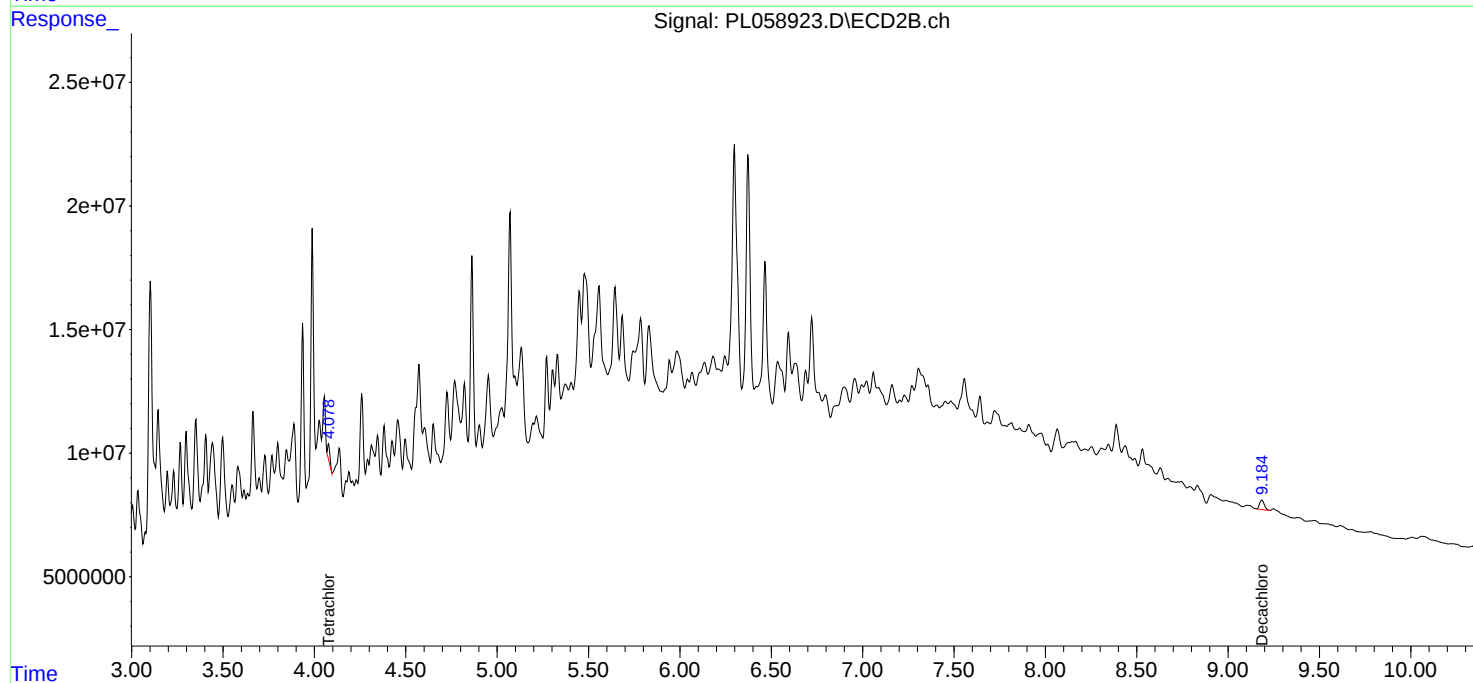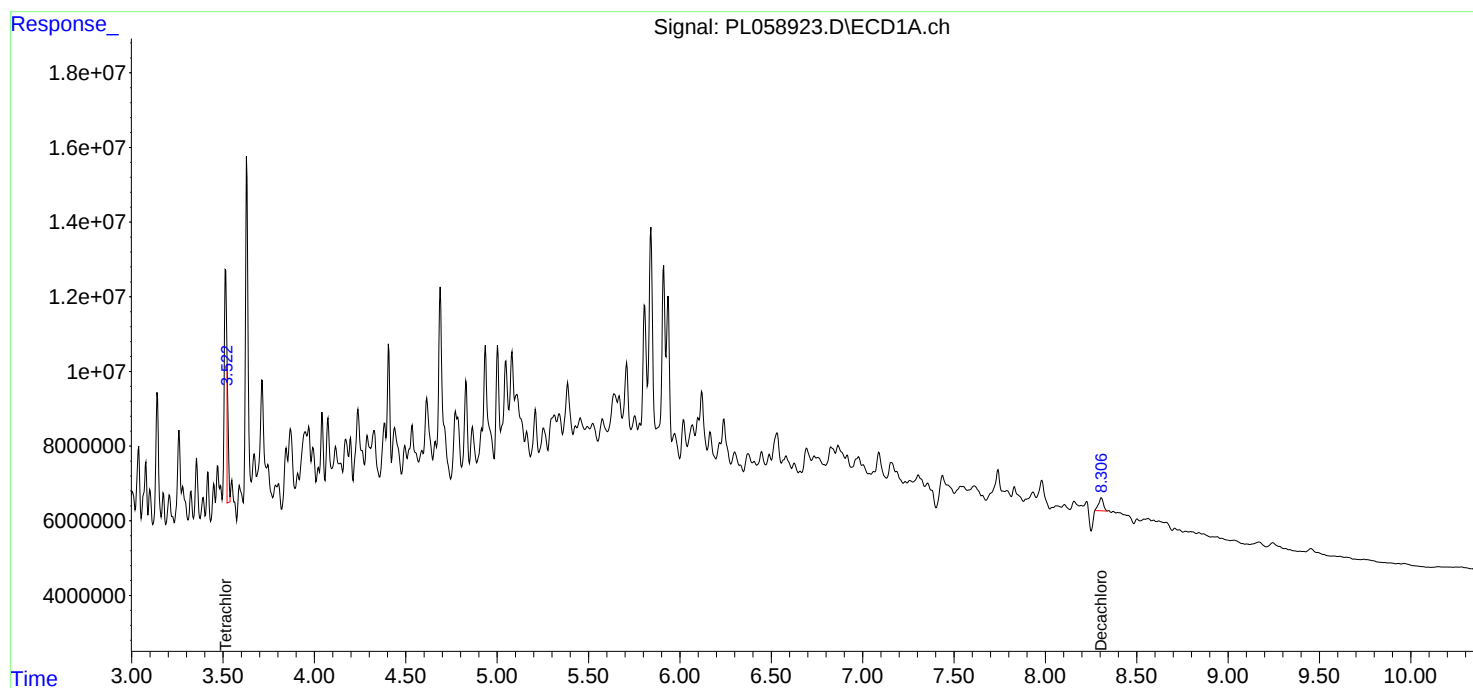

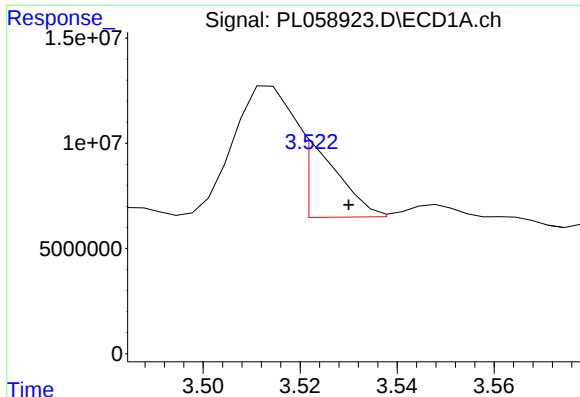


#1 Tetrachloro-m-xylene

R.T.: 3.522 min
Delta R.T.: -0.008 min
Response: 16589274
Conc: 9.05 ng/ml m

Instrument :
ECD_L
ClientSampleId :
C0AP3


Manual Integrations
APPROVED

mohammad
5/29/2020 12:32:07 PM

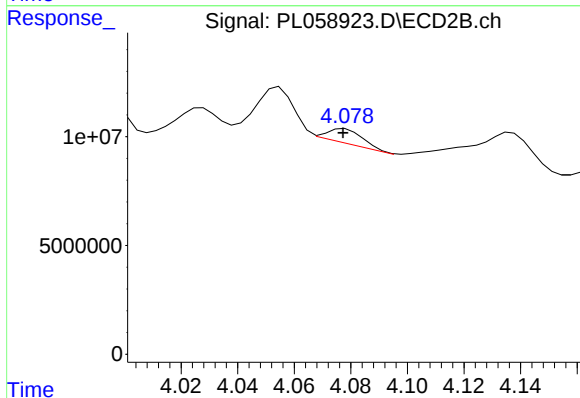


#1 Tetrachloro-m-xylene

R.T.: 4.078 min
Delta R.T.: 0.000 min
Response: 5376548
Conc: 1.99 ng/ml m

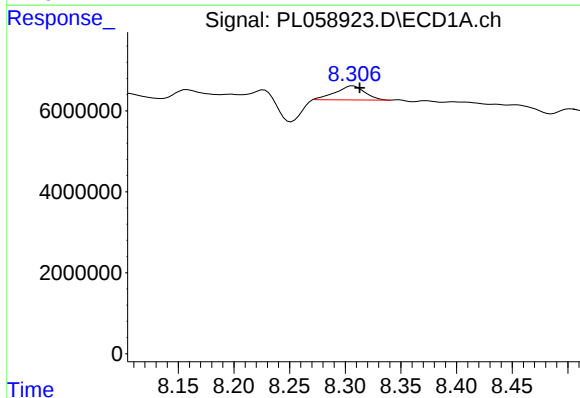

#28 Decachlorobiphenyl

R.T.: 8.307 min
Delta R.T.: -0.006 min
Response: 6315215
Conc: 3.74 ng/ml

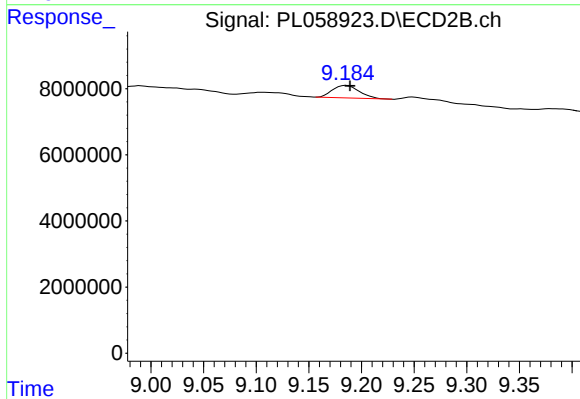

#28 Decachlorobiphenyl

R.T.: 9.184 min
Delta R.T.: -0.005 min
Response: 6697816
Conc: 2.54 ng/ml m