

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052721\
 Data File : PL066910.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2021 20:38
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 02:01:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052721CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 27 02:00:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.481	5.531	2757266	4528979	5.075	5.067
27)	SA Decachlor...	10.226	11.432	7582912	10438454	11.111	11.349
Target Compounds							
2)	A alpha-BHC	5.180	6.111	4844629	5147753	6.093	4.691
3)	MA gamma-BHC...	5.600	6.506	3555899	5079880	4.993	4.765
4)	MA Heptachlor	6.012	7.154	3446118	4961171	5.005	4.962
9)	A Endosulfan I	7.306	8.396	3272450	4200853	5.077	5.053
13)	MA Dieldrin	7.591	8.685	6607881	8649869	9.539	9.860
14)	MA Endrin	7.878	8.924	6177774	7230938	9.808	9.915
16)	A 4,4'-DDD	8.053	9.069	5345108	8073757	9.756	11.087
17)	MA 4,4'-DDT	8.314	9.387	4739068	6327024	8.806	9.510
20)	A Methoxychlor	8.908	9.873	15872174	20281817	52.078	54.184


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052721\
Data File : PL066910.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2021 20:38
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 02:01:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052721CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 27 02:00:36 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

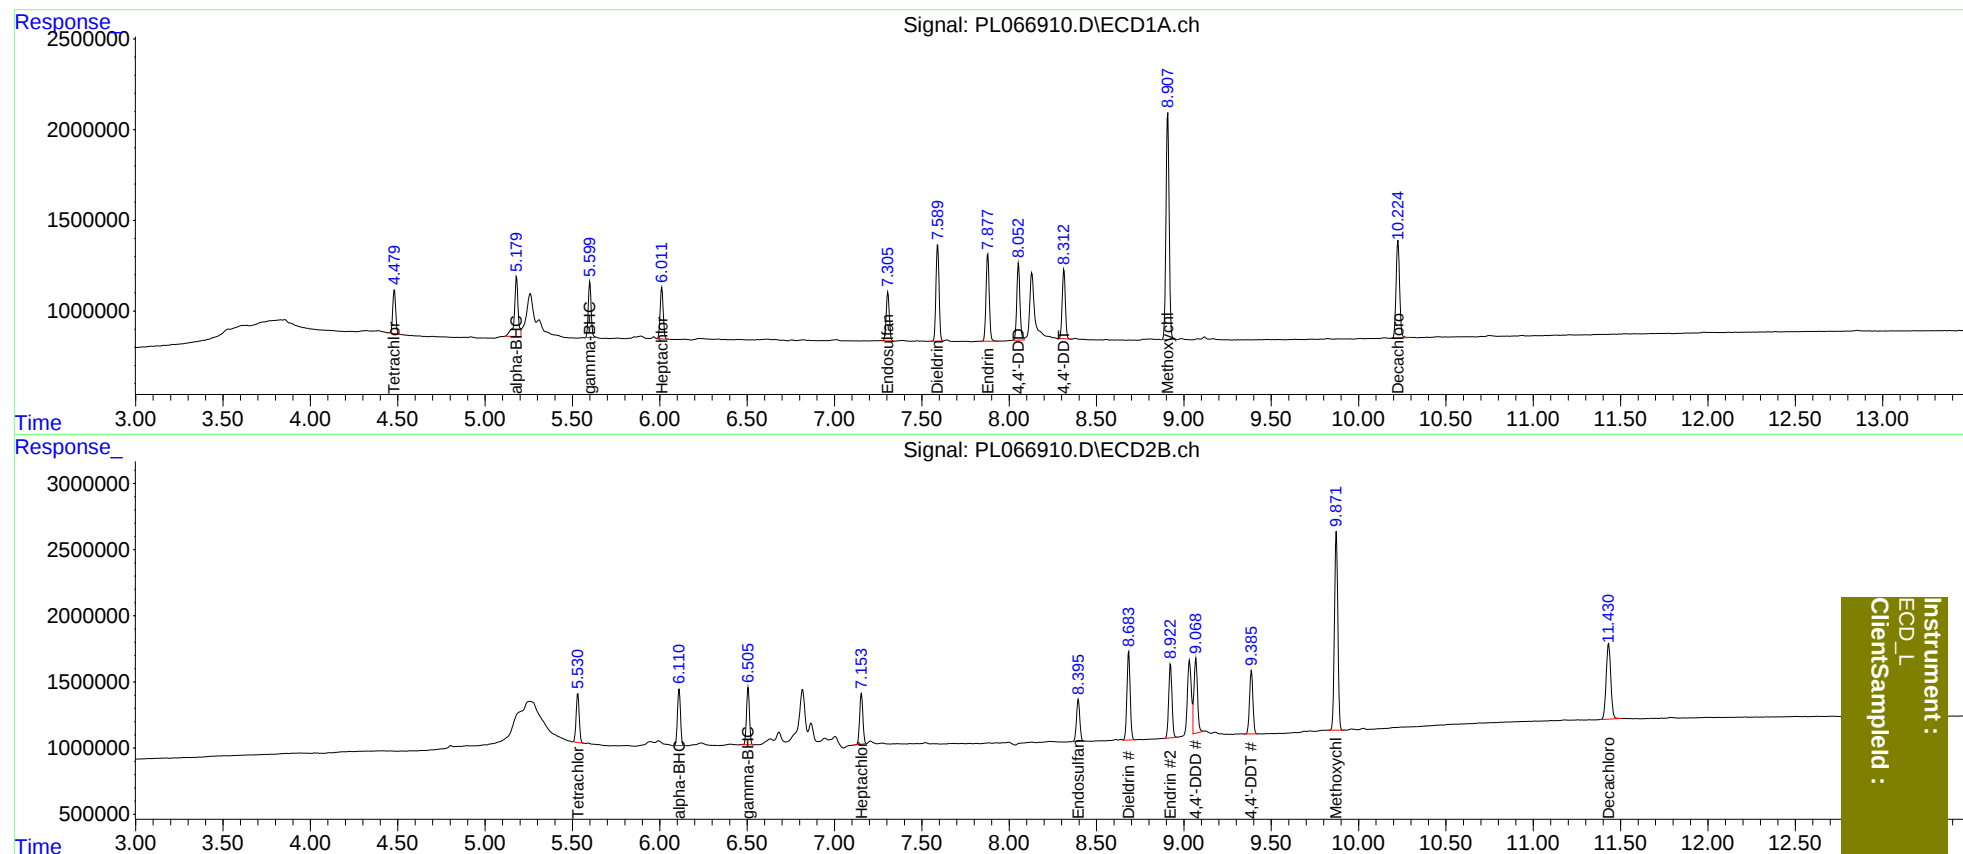


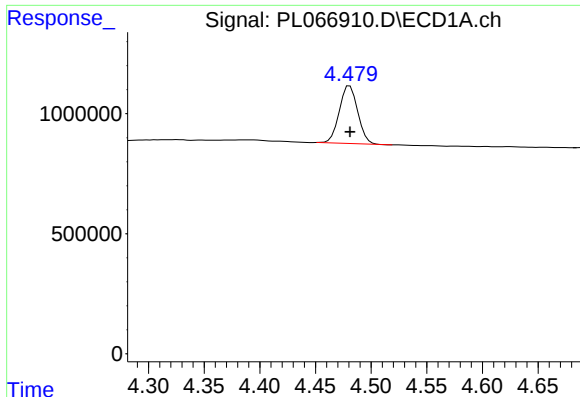

#1 Tetrachloro-m-xylene


R.T.: 4.481 min
Delta R.T.: 0.000 min
Response: 2757266
Conc: 5.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

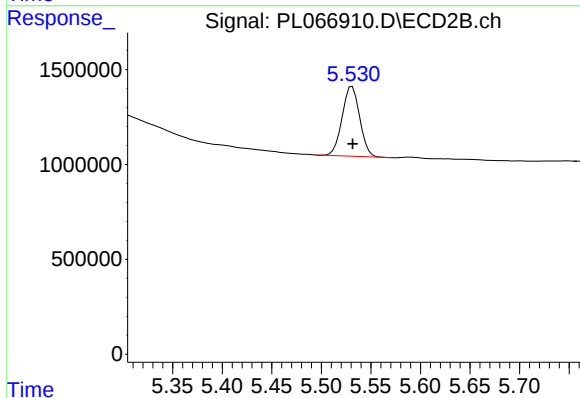


#1 Tetrachloro-m-xylene

R.T.: 5.531 min
Delta R.T.: 0.000 min
Response: 4528979
Conc: 5.07 ng/ml

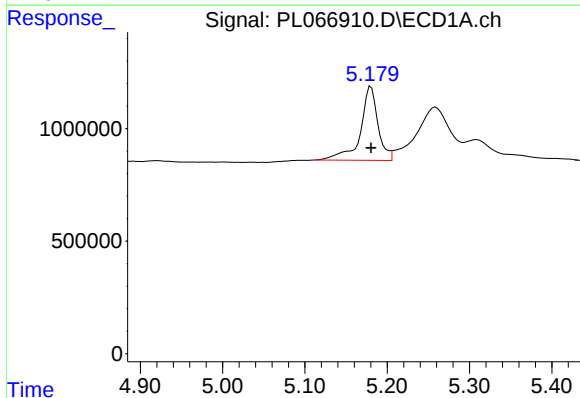


#2 alpha-BHC

R.T.: 5.180 min
Delta R.T.: 0.000 min
Response: 4844629
Conc: 6.09 ng/ml

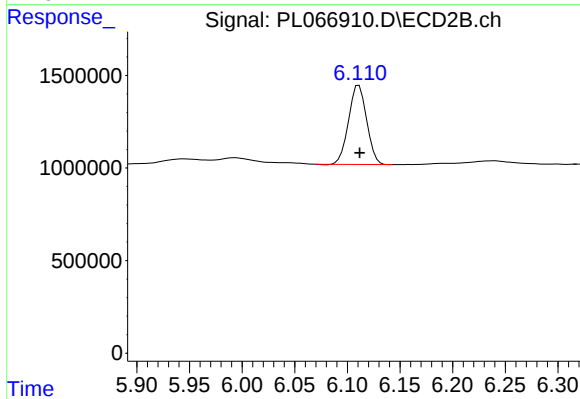

#2 alpha-BHC


R.T.: 6.111 min
Delta R.T.: 0.000 min
Response: 5147753
Conc: 4.69 ng/ml

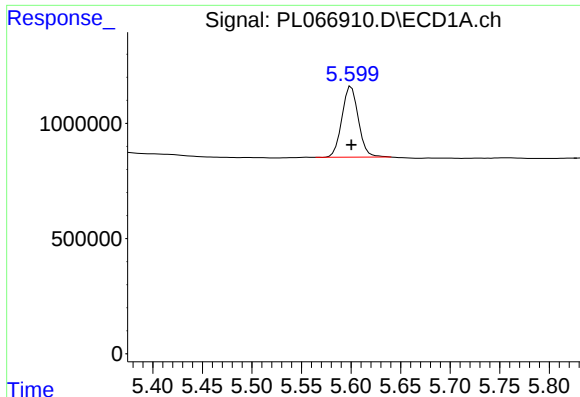

#3 gamma-BHC (Lindane)


R.T.: 5.600 min
Delta R.T.: 0.000 min
Response: 3555899
Conc: 4.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

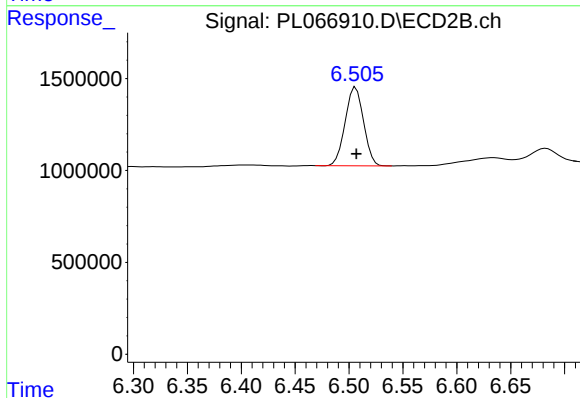


#3 gamma-BHC (Lindane)

R.T.: 6.506 min
Delta R.T.: 0.000 min
Response: 5079880
Conc: 4.77 ng/ml

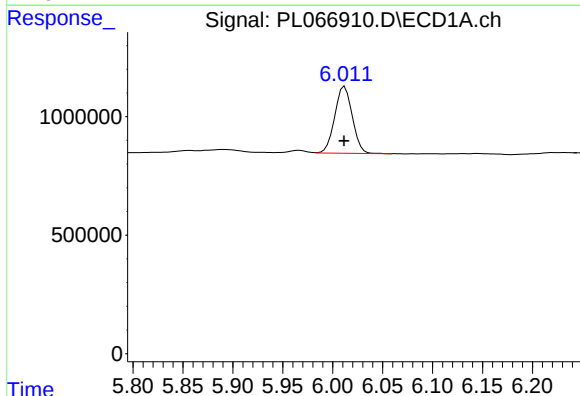


#4 Heptachlor

R.T.: 6.012 min
Delta R.T.: 0.000 min
Response: 3446118
Conc: 5.00 ng/ml

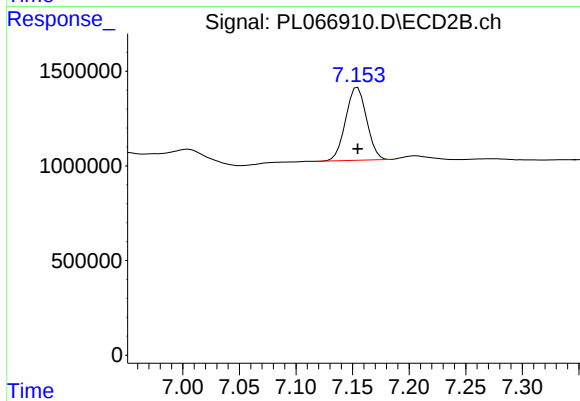

#4 Heptachlor


R.T.: 7.154 min
Delta R.T.: 0.000 min
Response: 4961171
Conc: 4.96 ng/ml

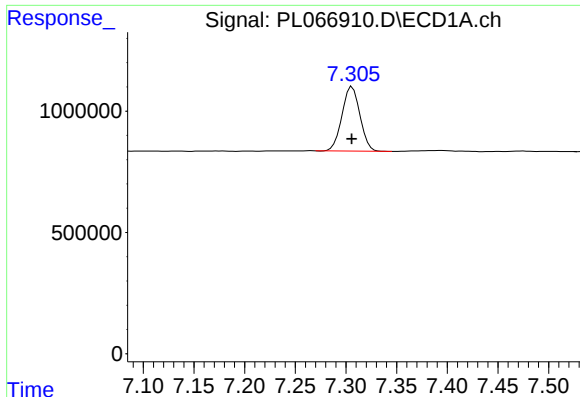

#9 Endosulfan I


R.T.: 7.306 min
Delta R.T.: 0.000 min
Response: 3272450
Conc: 5.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

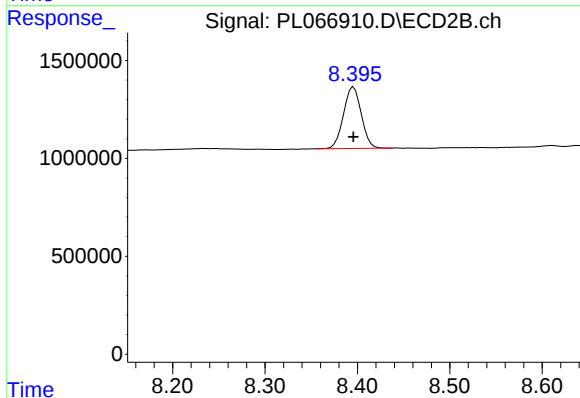


#9 Endosulfan I

R.T.: 8.396 min
Delta R.T.: 0.000 min
Response: 4200853
Conc: 5.05 ng/ml

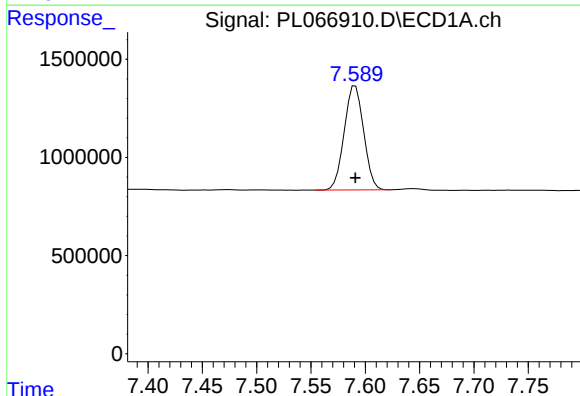


#13 Dieldrin

R.T.: 7.591 min
Delta R.T.: 0.000 min
Response: 6607881
Conc: 9.54 ng/ml

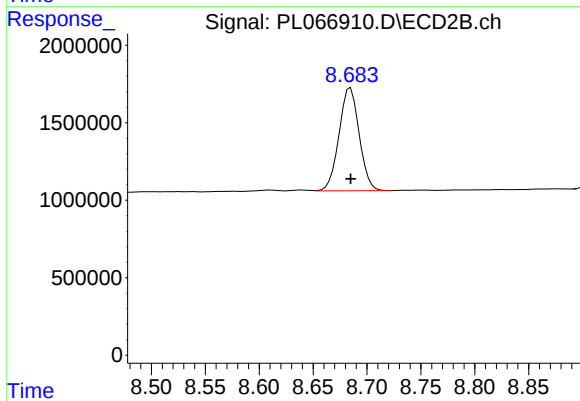

#13 Dieldrin


R.T.: 8.685 min
Delta R.T.: 0.000 min
Response: 8649869
Conc: 9.86 ng/ml

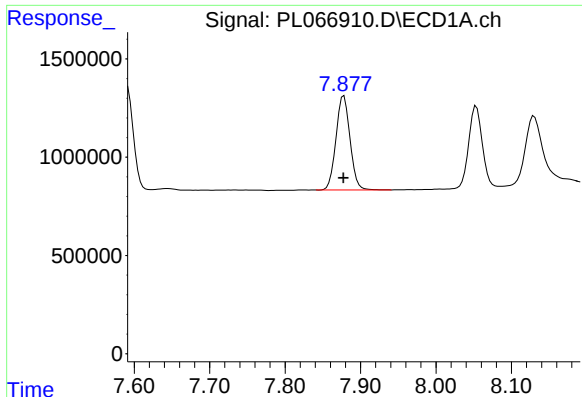

#14 Endrin


R.T.: 7.878 min
Delta R.T.: 0.000 min
Response: 6177774
Conc: 9.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

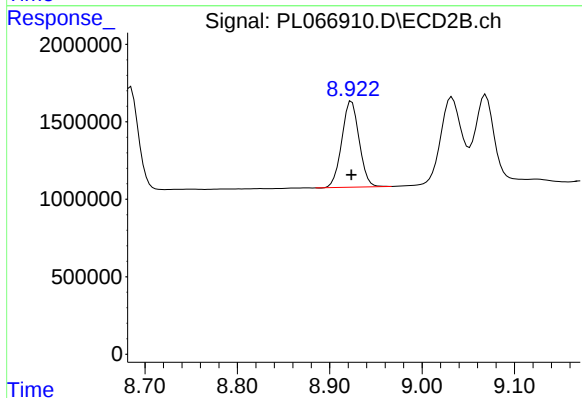


#14 Endrin

R.T.: 8.924 min
Delta R.T.: 0.000 min
Response: 7230938
Conc: 9.91 ng/ml

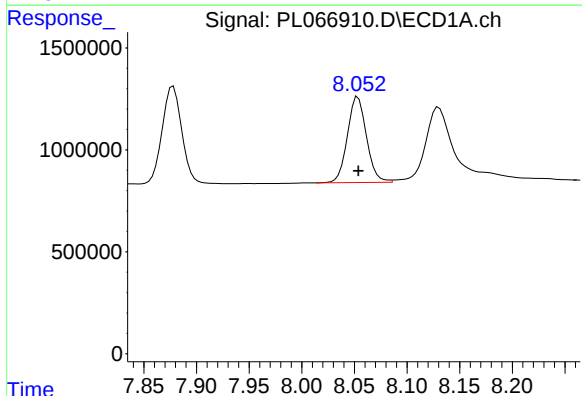


#16 4,4'-DDD

R.T.: 8.053 min
Delta R.T.: 0.000 min
Response: 5345108
Conc: 9.76 ng/ml

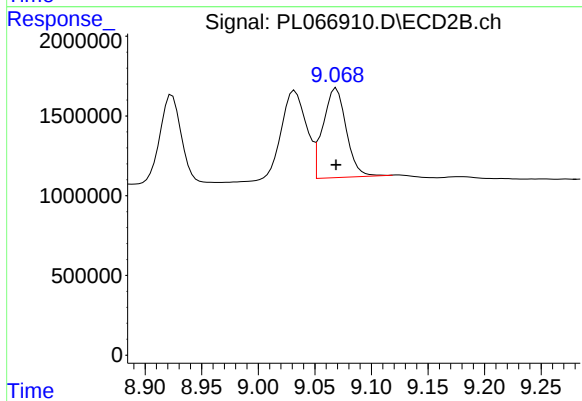

#16 4,4'-DDD


R.T.: 9.069 min
Delta R.T.: 0.000 min
Response: 8073757
Conc: 11.09 ng/ml

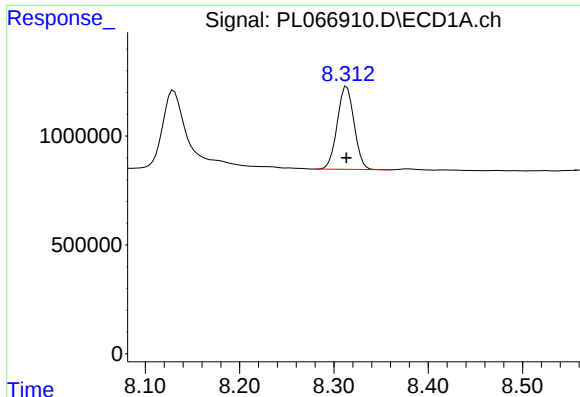

#17 4,4'-DDT


R.T.: 8.314 min
Delta R.T.: 0.000 min
Response: 4739068
Conc: 8.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

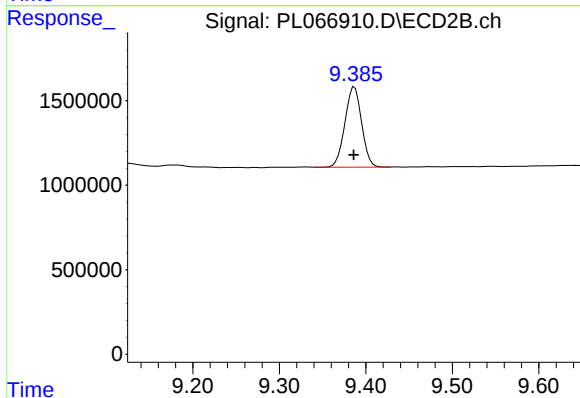


#17 4,4'-DDT

R.T.: 9.387 min
Delta R.T.: 0.000 min
Response: 6327024
Conc: 9.51 ng/ml

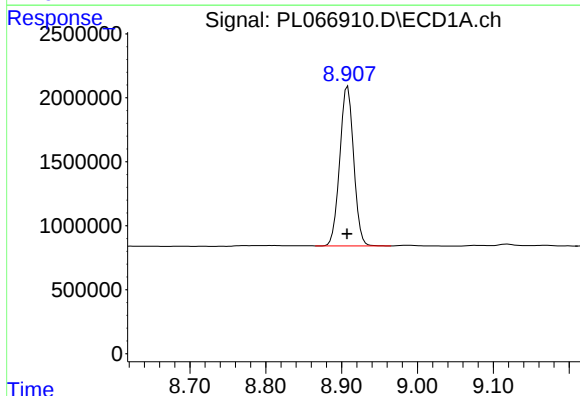


#20 Methoxychlor

R.T.: 8.908 min
Delta R.T.: 0.000 min
Response: 15872174
Conc: 52.08 ng/ml

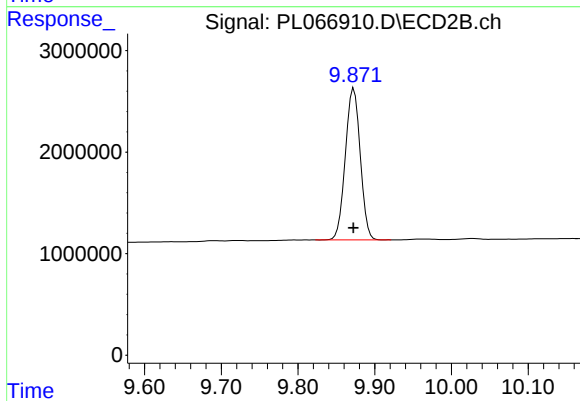

#20 Methoxychlor


R.T.: 9.873 min
Delta R.T.: 0.000 min
Response: 20281817
Conc: 54.18 ng/ml

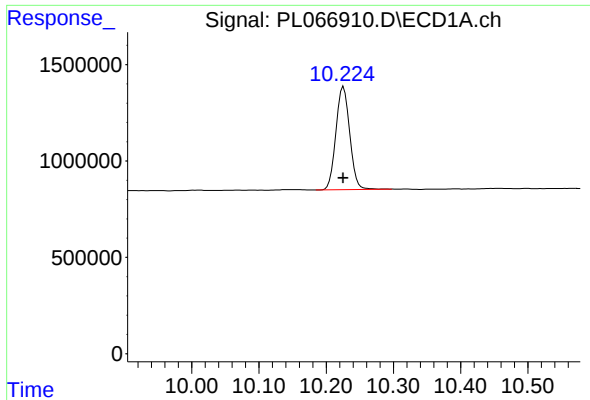

#27 Decachlorobiphenyl

R.T.: 10.226 min
Delta R.T.: 0.000 min
Response: 7582912
Conc: 11.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

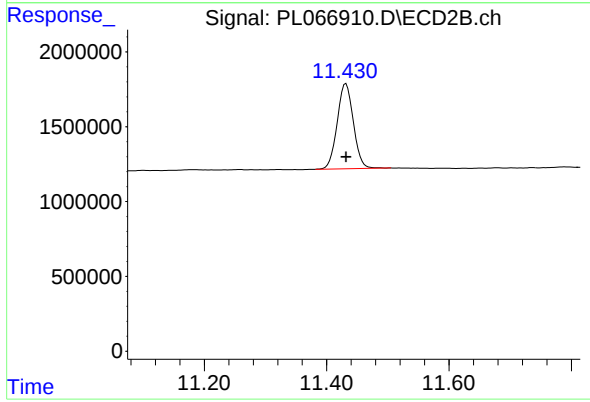

#27 Decachlorobiphenyl

R.T.: 11.432 min
Delta R.T.: 0.000 min
Response: 10438454
Conc: 11.35 ng/ml