

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052721\
 Data File : PL066920.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2021 23:54
 Operator : AR\AJ
 Sample : PIBLK64
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 02:35:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052721CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 27 02:30:58 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.481	5.531	10263182	17294879	19.231	19.559
2)	SA Decachlor...	10.225	11.431	25097569	34889814	37.428	38.216
Target Compounds							
15)	B Endosulfa...	8.130f	0.000	6721922	0	11.194	N.D. #
16)	A 4,4'-DDD	0.000	9.032f	0	8504209	N.D.	11.477

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052721\
Data File : PL066920.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2021 23:54
Operator : AR\AJ
Sample : PIBLK64
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 02:35:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052721CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 27 02:30:58 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

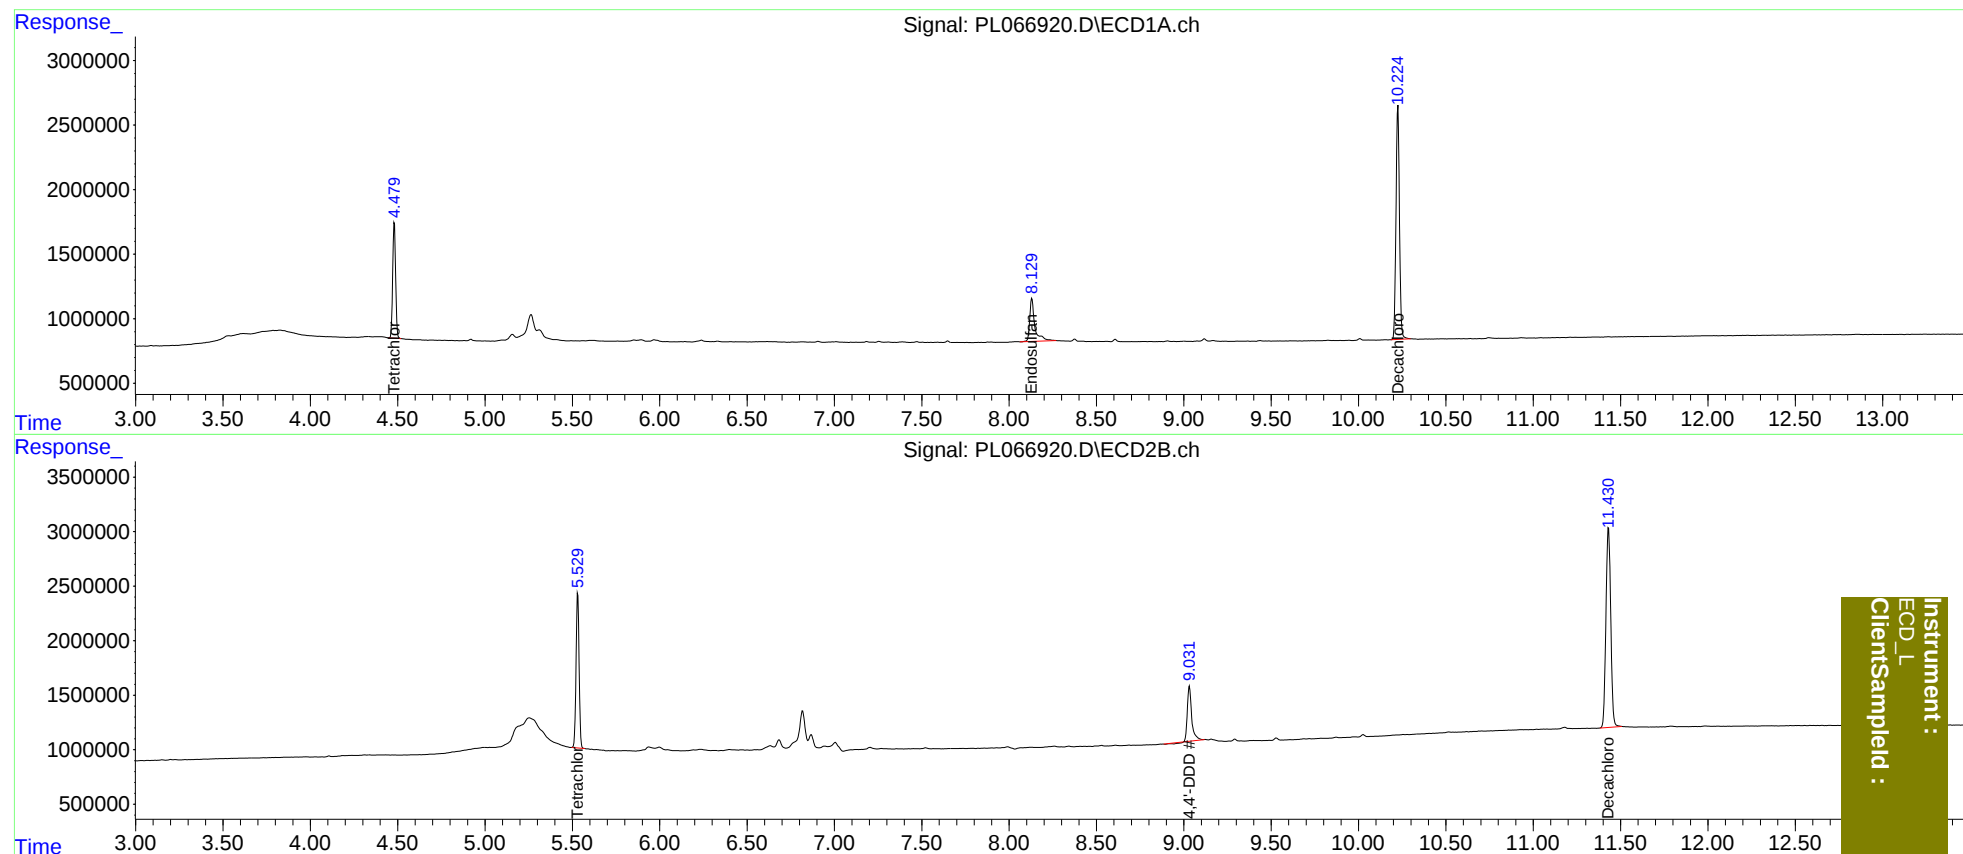


Instrument :
ECD_L
ClientSampled :

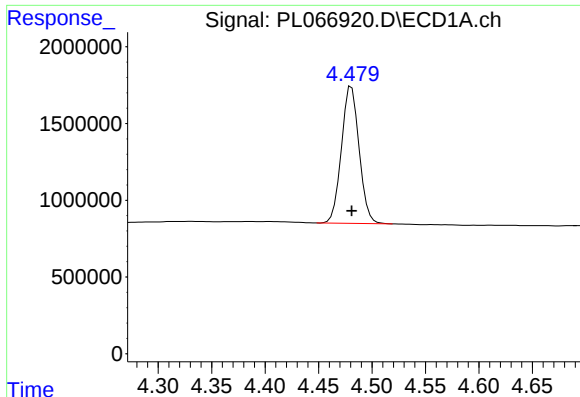

#1 Tetrachloro-m-xylene


R.T.: 4.481 min
Delta R.T.: 0.000 min
Response: 10263182
Conc: 19.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

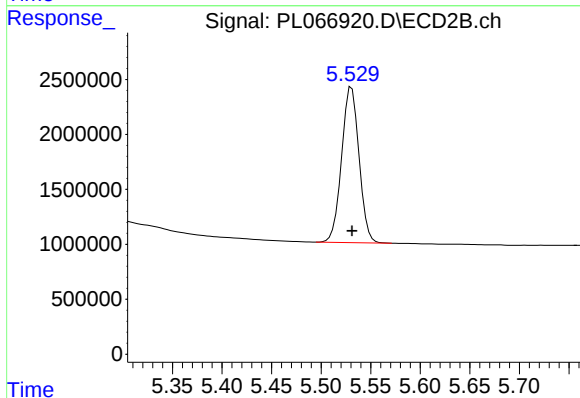


#1 Tetrachloro-m-xylene

R.T.: 5.531 min
Delta R.T.: 0.000 min
Response: 17294879
Conc: 19.56 ng/ml

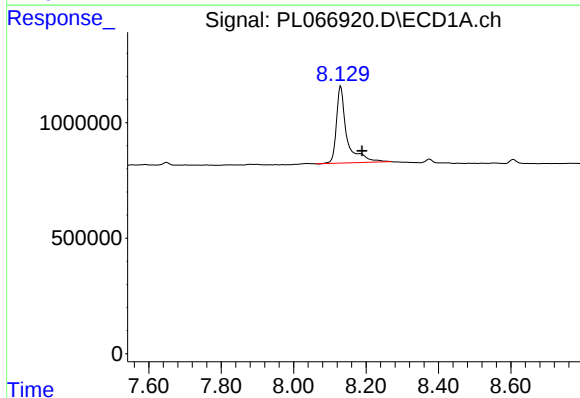


#15 Endosulfan II

R.T.: 8.130 min
Delta R.T.: -0.059 min
Response: 6721922
Conc: 11.19 ng/ml

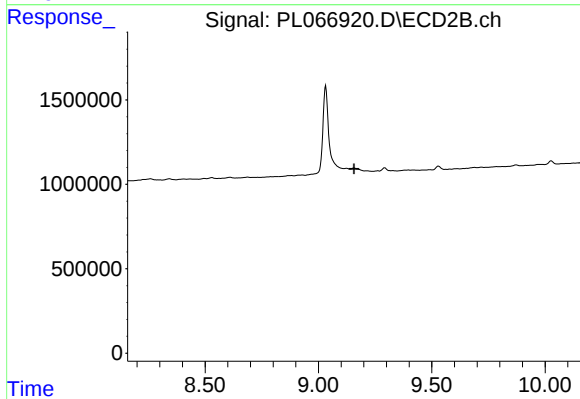

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 9.158 min
Response: 0
Conc: N.D.

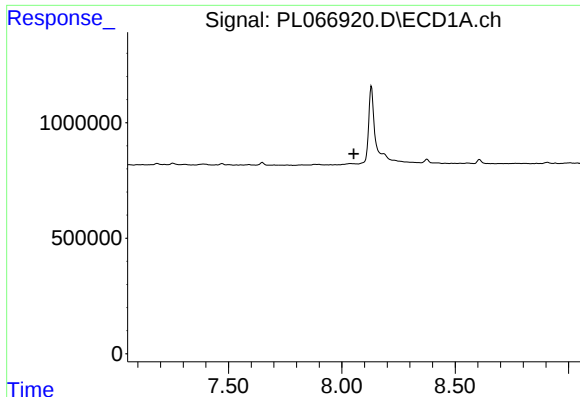

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.053 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

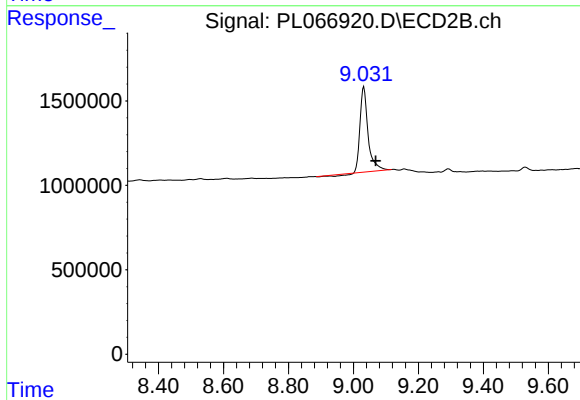


#16 4,4'-DDD

R.T.: 9.032 min
Delta R.T.: -0.037 min
Response: 8504209
Conc: 11.48 ng/ml

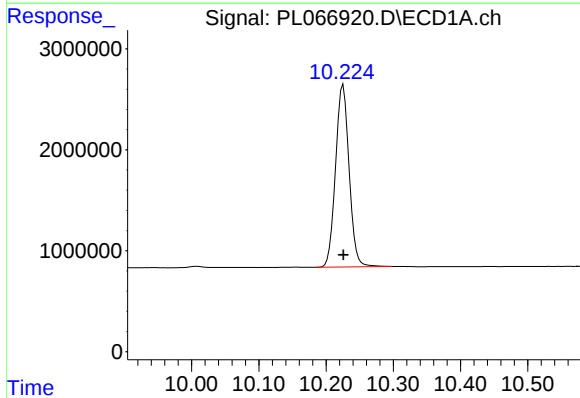

#27 Decachlorobiphenyl

R.T.: 10.225 min
Delta R.T.: 0.000 min
Response: 25097569
Conc: 37.43 ng/ml

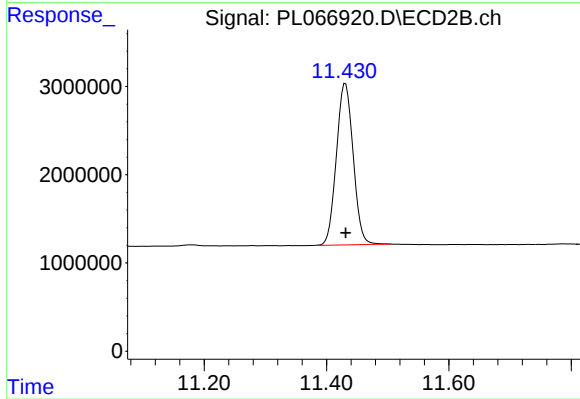

#27 Decachlorobiphenyl

R.T.: 11.431 min
Delta R.T.: 0.000 min
Response: 34889814
Conc: 38.22 ng/ml