

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052722\
 Data File : PL075114.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 May 2022 14:08
 Operator : AR\AJ
 Sample : N2923-20
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 28 02:44:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.643	4.644	4193455	11958879	8.259	8.713
28)	SA Decachlor...	11.640	10.393	6563971	14442012	14.698	14.070
Target Compounds							
7)	B delta-BHC	0.000	6.417	0	303971	N.D.	0.194 #
10)	B gamma-Chl...	0.000	7.390f	0	290186	N.D.	0.209 #
13)	MA Dieldrin	8.813	7.794f	1732097	3459997	3.295	2.716
14)	MA Endrin	9.056	8.068	439183	5212403	1.064	4.935 #
15)	B Endosulfa...	9.273f	8.358f	1404705	1435925	3.195	1.271 #
16)	A 4,4'-DDD	9.203	0.000	12497542	0	27.642	N.D. #
17)	MA 4,4'-DDT	0.000	8.469f	0	16430473	N.D.	16.422 #
19)	B Endosulfa...	0.000	8.780	0	18343293	N.D.	16.851 #
22)	Mirex	10.660	0.000	264998	0	0.657	N.D. #
25)	Chlordane-3	0.000	7.390f	0	290186	N.D.	2.236 #
27)	Chlordane-5	0.000	8.131	0	28626249	N.D.	774.231 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052722\
Data File : PL075114.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 May 2022 14:08
Operator : AR\AJ
Sample : N2923-20
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 02:44:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

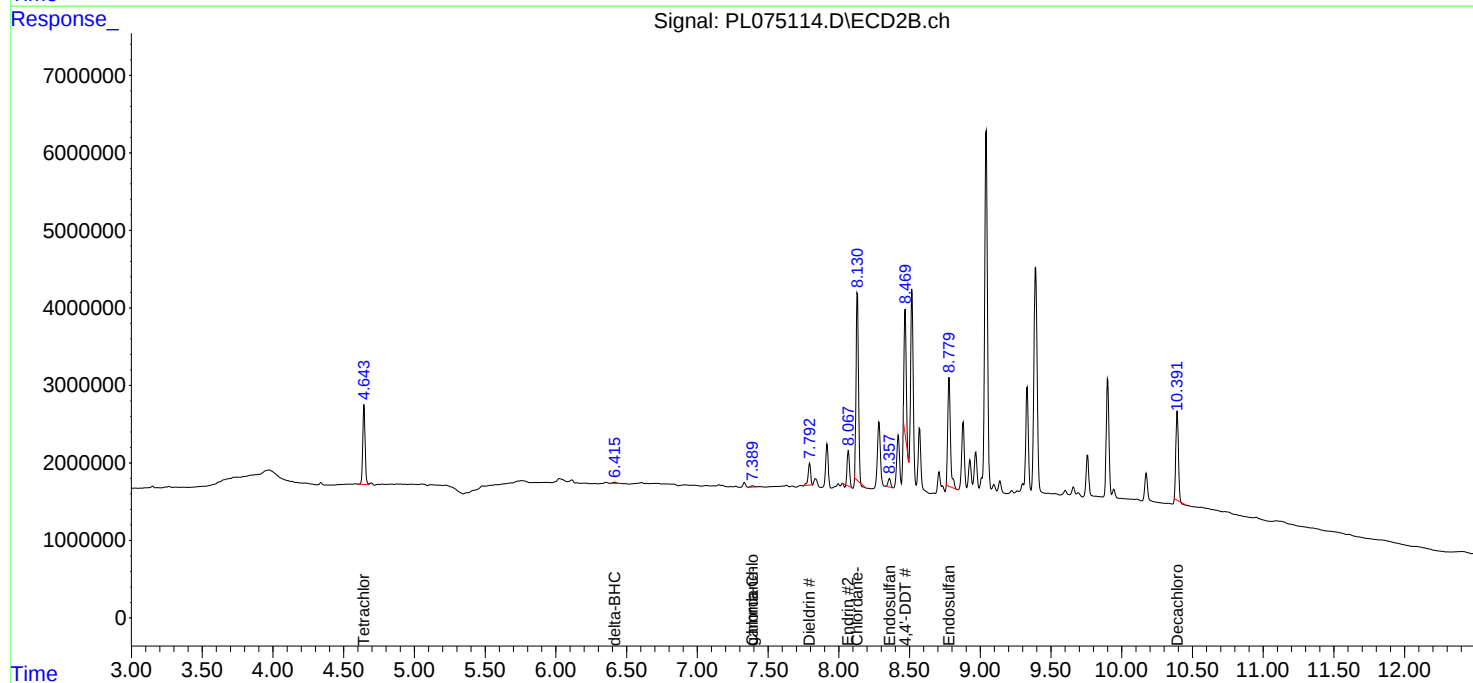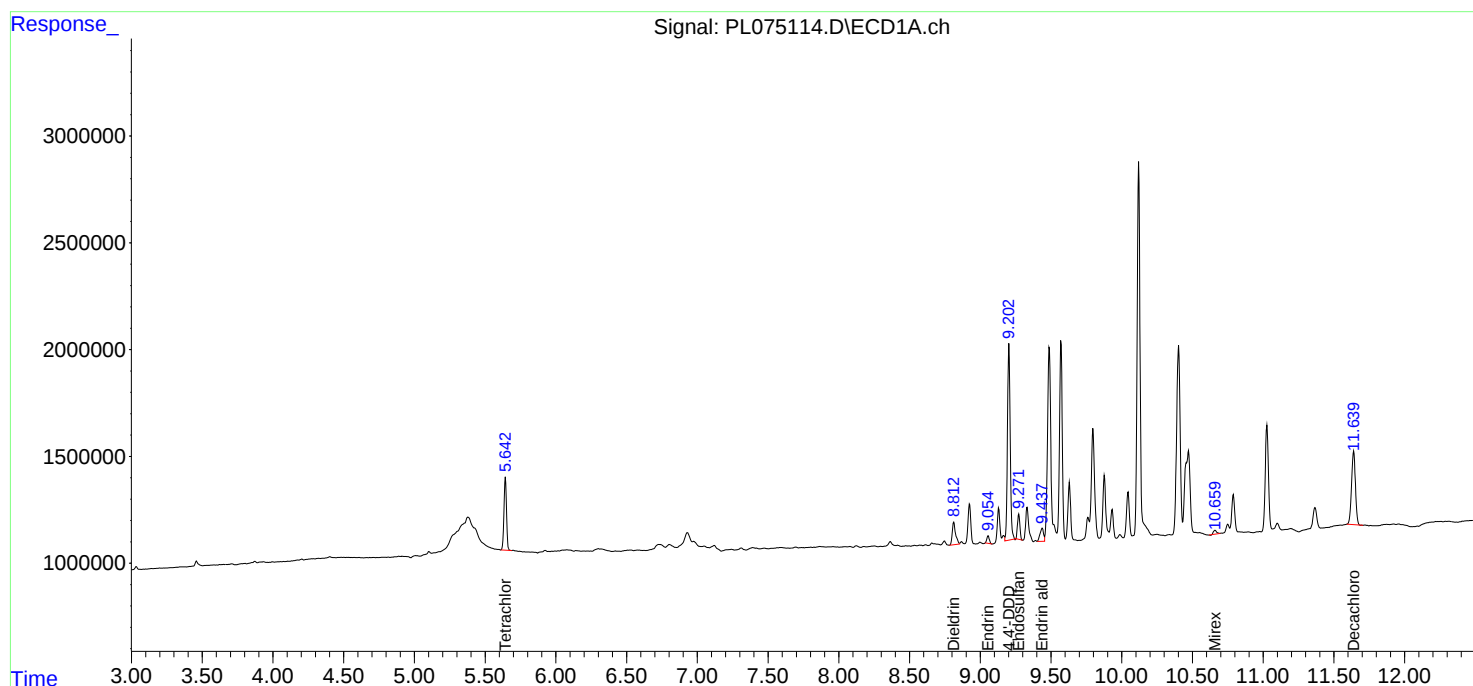


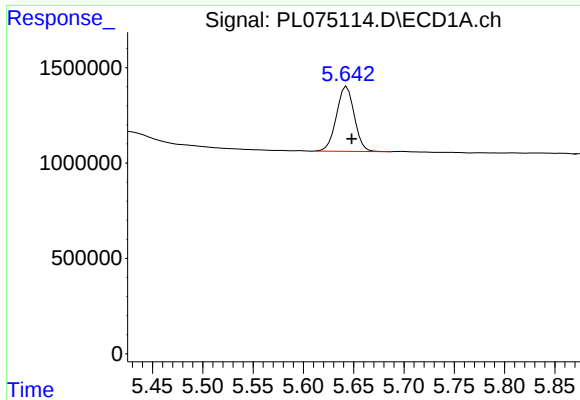

#1 Tetrachloro-m-xylene


R.T.: 5.643 min
Delta R.T.: -0.005 min
Response: 4193455
Conc: 8.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

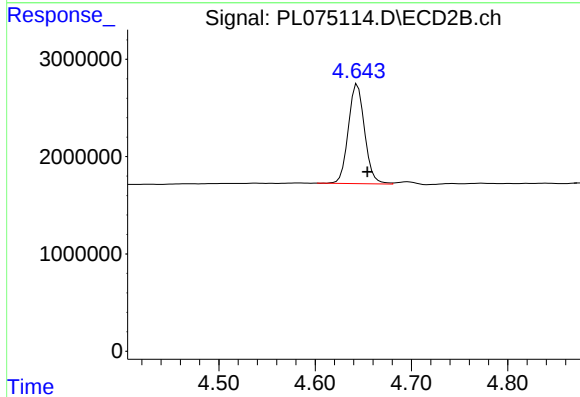


#1 Tetrachloro-m-xylene

R.T.: 4.644 min
Delta R.T.: -0.010 min
Response: 11958879
Conc: 8.71 ng/ml

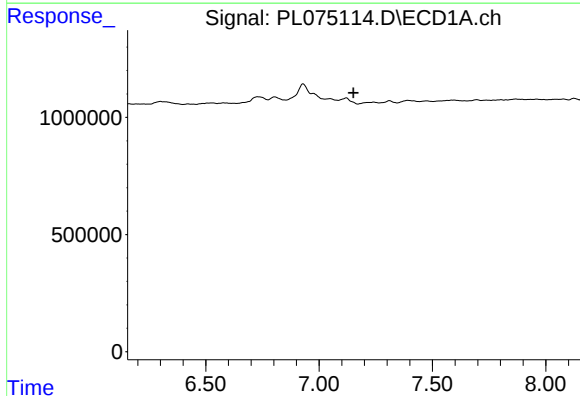


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.152 min
Response: 0
Conc: N.D.

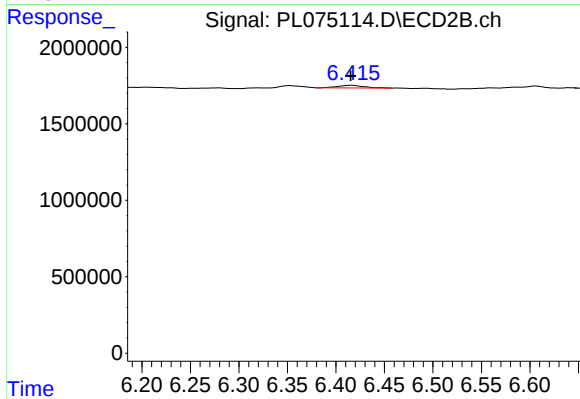

#7 delta-BHC


R.T.: 6.417 min
Delta R.T.: 0.001 min
Response: 303971
Conc: 0.19 ng/ml

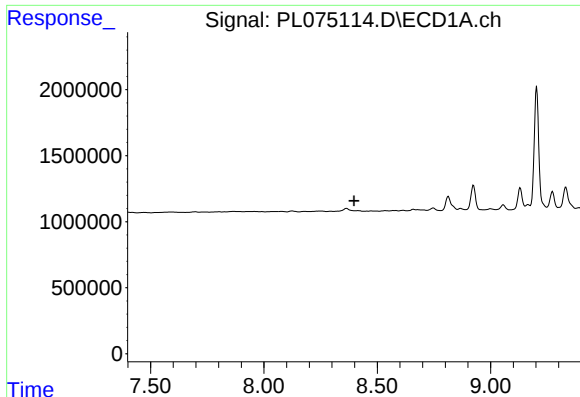

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

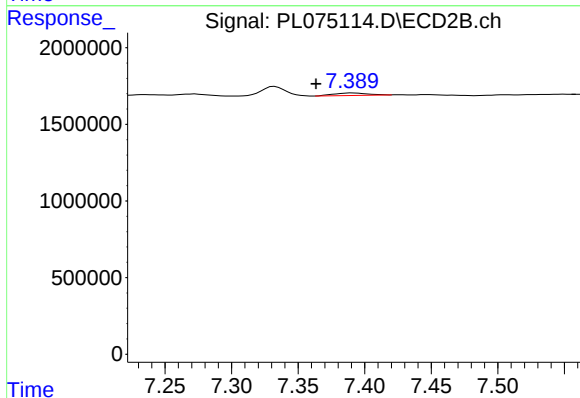


#10 gamma-Chlordane

R.T.: 7.390 min
Delta R.T.: 0.027 min
Response: 290186
Conc: 0.21 ng/ml

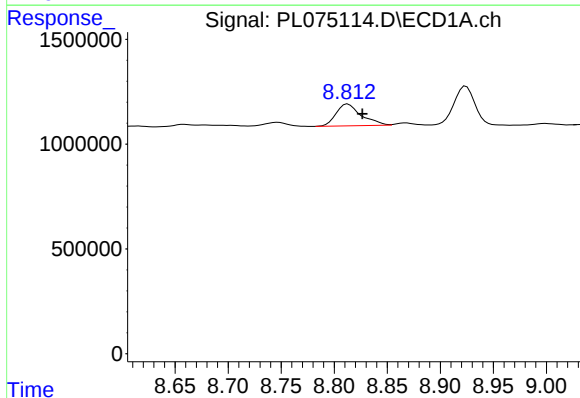


#13 Dieldrin

R.T.: 8.813 min
Delta R.T.: -0.014 min
Response: 1732097
Conc: 3.30 ng/ml

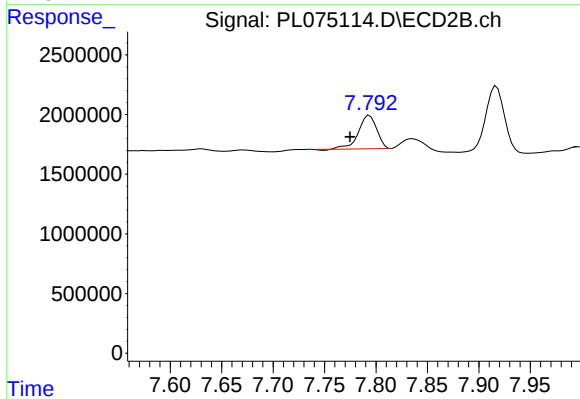

#13 Dieldrin


R.T.: 7.794 min
Delta R.T.: 0.019 min
Response: 3459997
Conc: 2.72 ng/ml

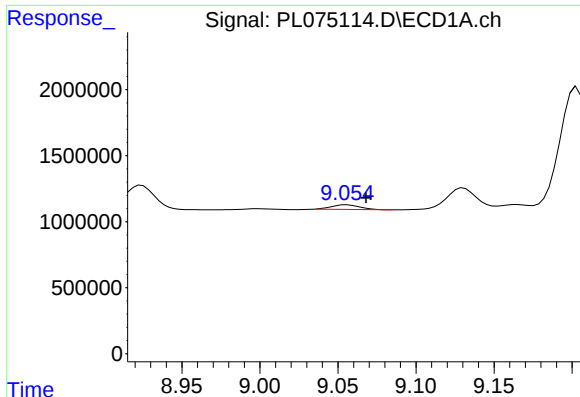

#14 Endrin


R.T.: 9.056 min
Delta R.T.: -0.012 min
Response: 439183
Conc: 1.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

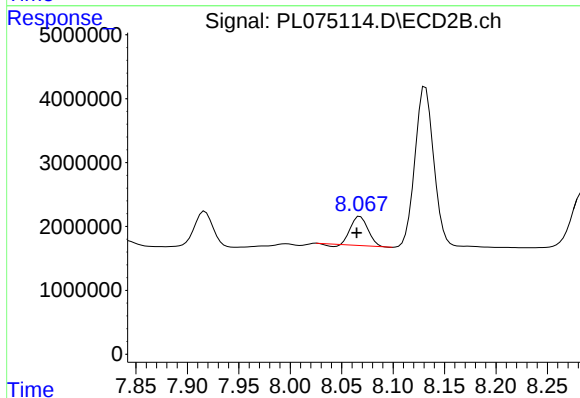


#14 Endrin

R.T.: 8.068 min
Delta R.T.: 0.003 min
Response: 5212403
Conc: 4.93 ng/ml

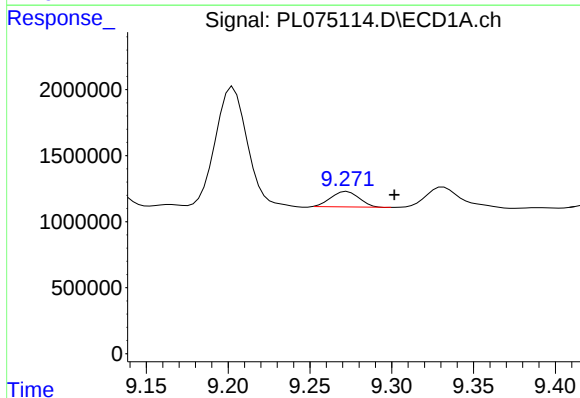


#15 Endosulfan II

R.T.: 9.273 min
Delta R.T.: -0.029 min
Response: 1404705
Conc: 3.20 ng/ml

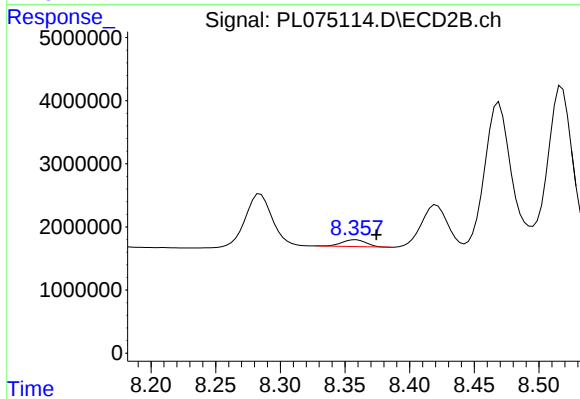

#15 Endosulfan II


R.T.: 8.358 min
Delta R.T.: -0.016 min
Response: 1435925
Conc: 1.27 ng/ml

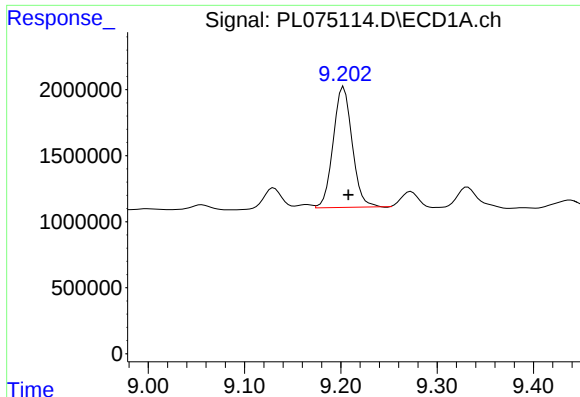

#16 4,4'-DDD


R.T.: 9.203 min
Delta R.T.: -0.005 min
Response: 12497542
Conc: 27.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

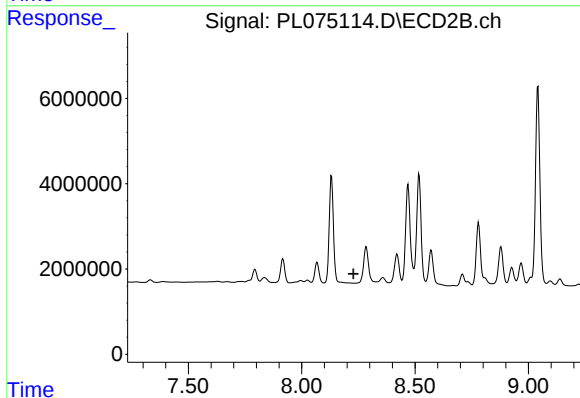


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.229 min
Response: 0
Conc: N.D.

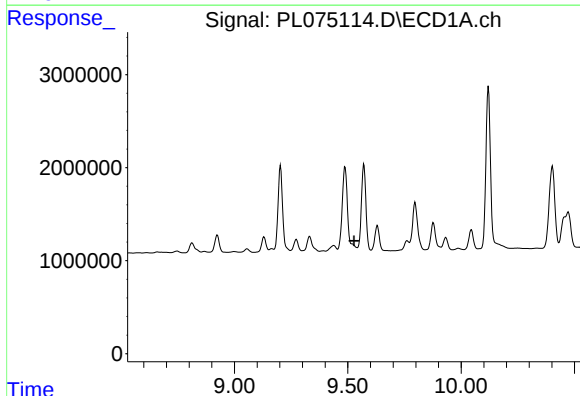


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.527 min
Response: 0
Conc: N.D.

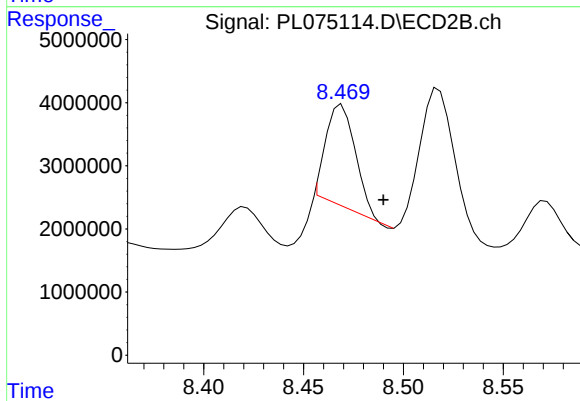

#17 4,4'-DDT


R.T.: 8.469 min
Delta R.T.: -0.021 min
Response: 16430473
Conc: 16.42 ng/ml

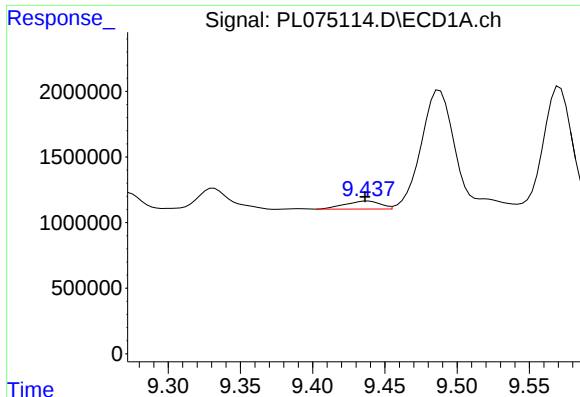

#18 Endrin aldehyde


R.T.: 9.438 min
Delta R.T.: 0.002 min
Response: 1049945
Conc: 2.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

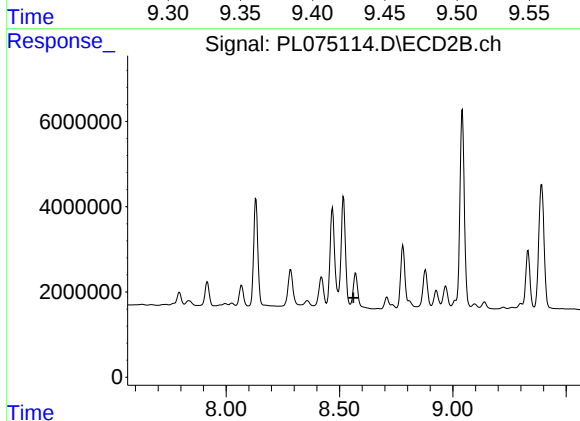


#18 Endrin aldehyde

R.T.: 8.571 min
Delta R.T.: 0.009 min
Response: -7842110
Conc: N.D.

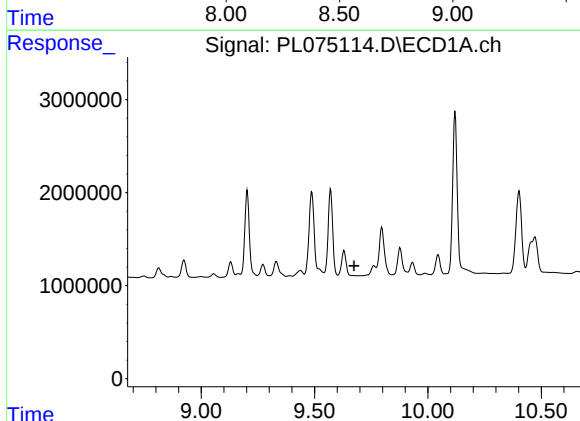


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 9.675 min
Response: 0
Conc: N.D.

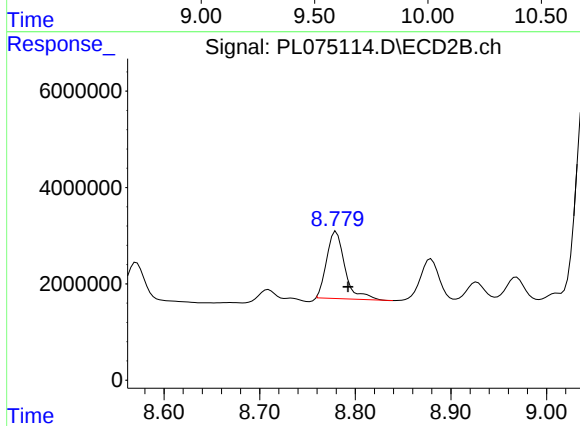

#19 Endosulfan Sulfate


R.T.: 8.780 min
Delta R.T.: -0.013 min
Response: 18343293
Conc: 16.85 ng/ml

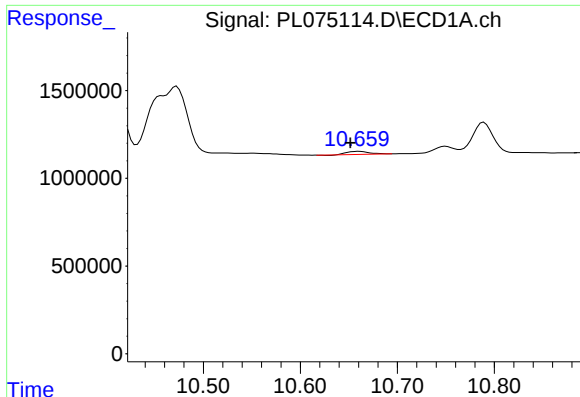

#22 Mirex


R.T.: 10.660 min
Delta R.T.: 0.009 min
Response: 264998
Conc: 0.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

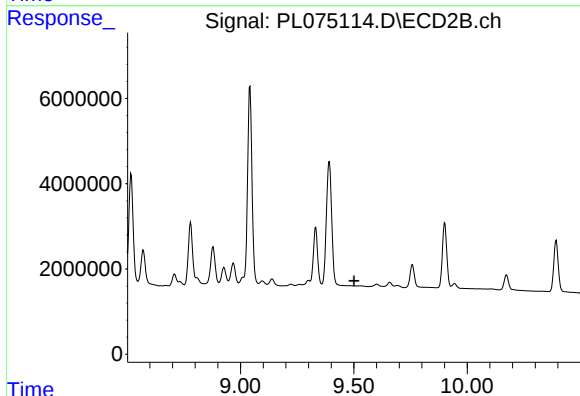


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 9.501 min
Response: 0
Conc: N.D.

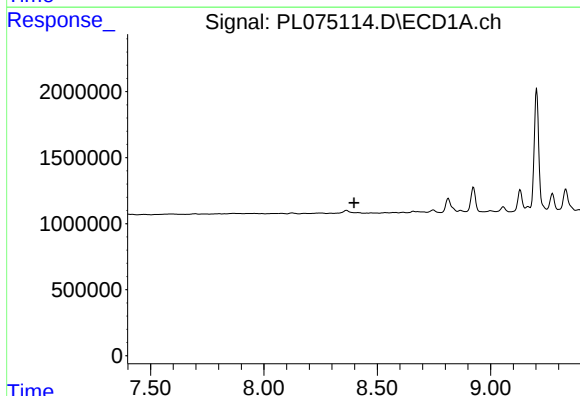


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 8.398 min
Response: 0
Conc: N.D.

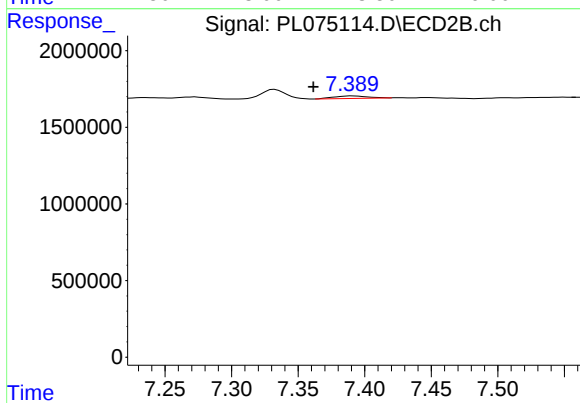

#25 Chlordane-3


R.T.: 7.390 min
Delta R.T.: 0.029 min
Response: 290186
Conc: 2.24 ng/ml

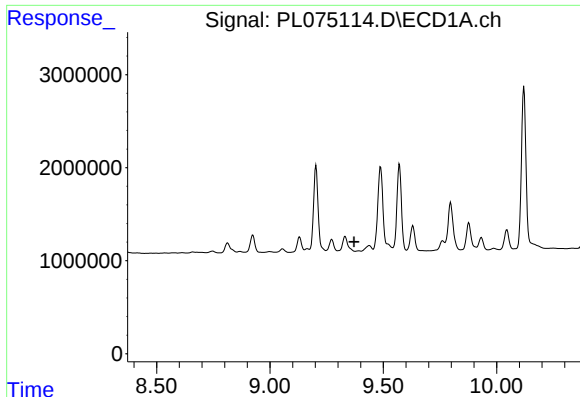

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 9.371 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

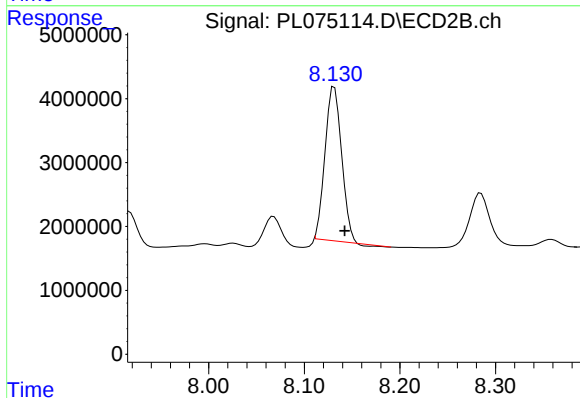


#27 Chlordane-5

R.T.: 8.131 min
Delta R.T.: -0.011 min
Response: 28626249
Conc: 774.23 ng/ml

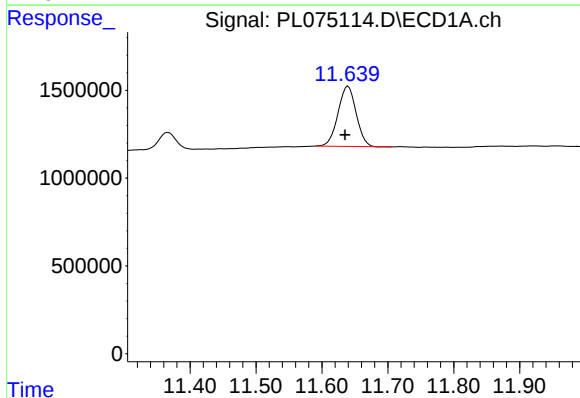

#28 Decachlorobiphenyl

R.T.: 11.640 min
Delta R.T.: 0.005 min
Response: 6563971
Conc: 14.70 ng/ml

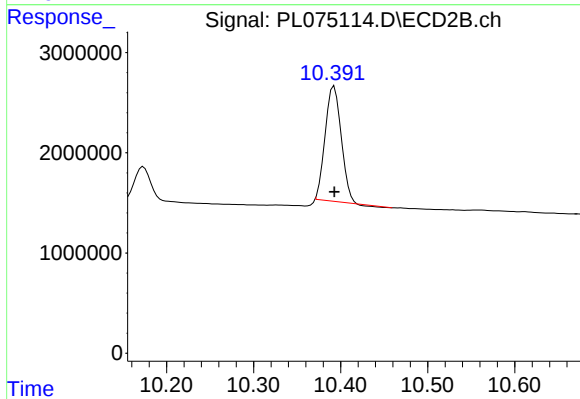

#28 Decachlorobiphenyl

R.T.: 10.393 min
Delta R.T.: 0.000 min
Response: 14442012
Conc: 14.07 ng/ml