

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052722\
 Data File : PL075115.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 May 2022 14:25
 Operator : AR\AJ
 Sample : N2924-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 28 02:44:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.643	4.644	4028817	11457245	7.935	8.348
28)	SA Decachlor...	11.638	10.392	5834639	12288624	13.065	11.972
Target Compounds							
4)	MA Heptachlor	7.312f	0.000	198086	0	0.307	N.D. #
7)	B delta-BHC	0.000	6.418	0	232942	N.D.	0.149 #
13)	MA Dieldrin	8.812	7.769	505565	97277	0.962	0.076 #
14)	MA Endrin	9.056	8.068	399696	2715336	0.969	2.571 #
15)	B Endosulfa...	9.332f	8.355f	304417	825507	0.692	0.731
16)	A 4,4'-DDD	9.203	0.000	6254714	0	13.834	N.D. #
17)	MA 4,4'-DDT	0.000	8.468f	0	9172904	N.D.	9.168 #
19)	B Endosulfa...	0.000	8.779	0	9013500	N.D.	8.280 #
25)	Chlordane-3	0.000	7.333f	0	395374	N.D.	3.046 #
27)	Chlordane-5	0.000	8.132	0	14312318	N.D.	387.094 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052722\
Data File : PL075115.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 May 2022 14:25
Operator : AR\AJ
Sample : N2924-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 02:44:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

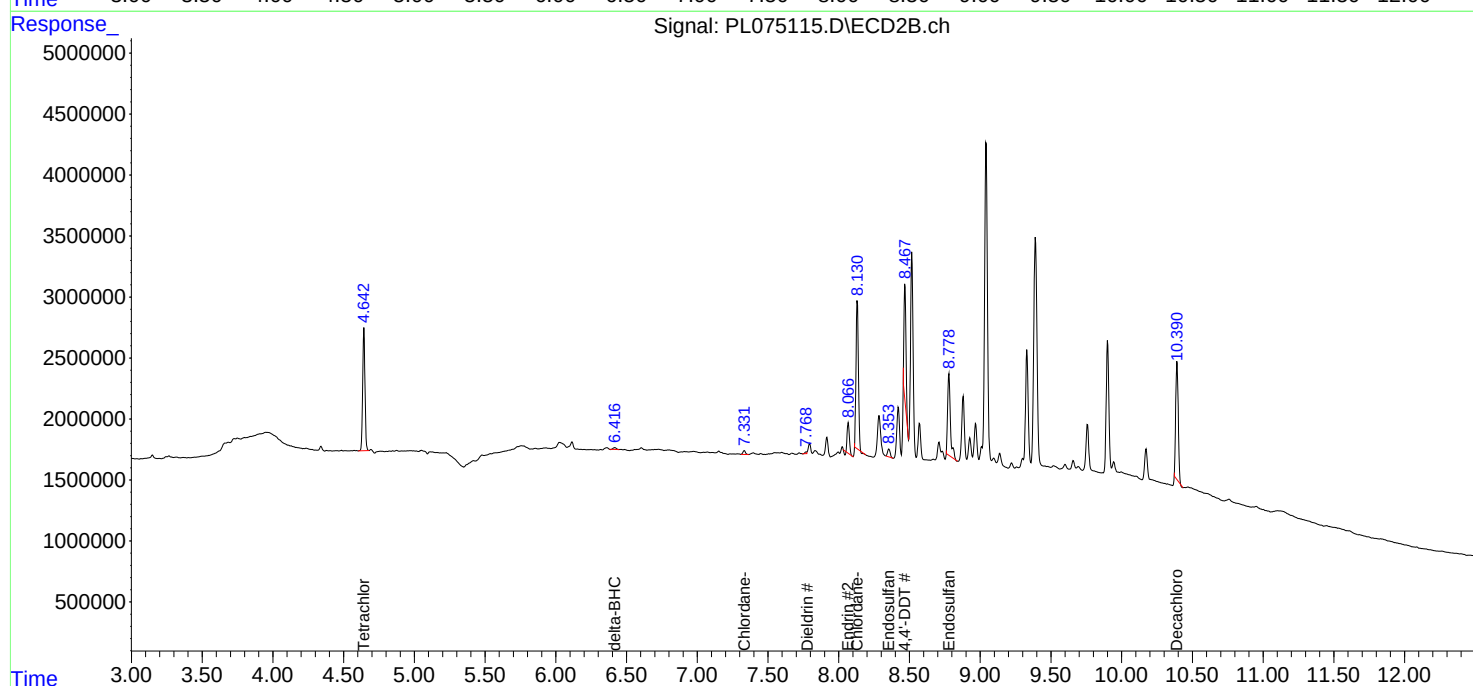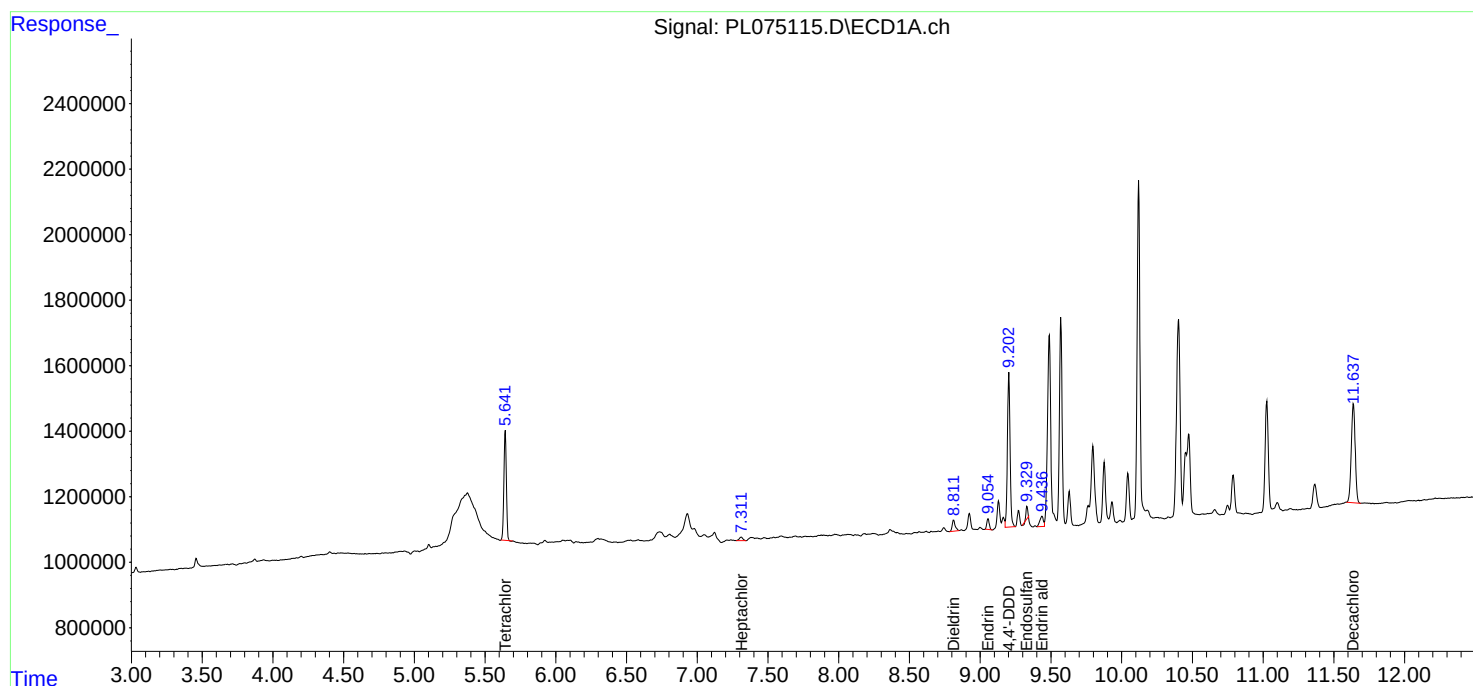


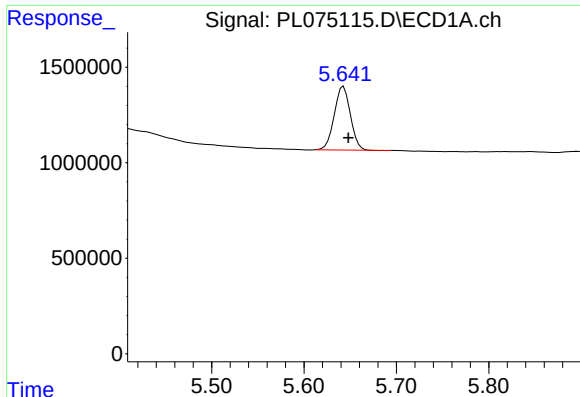

#1 Tetrachloro-m-xylene


R.T.: 5.643 min
Delta R.T.: -0.005 min
Response: 4028817
Conc: 7.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

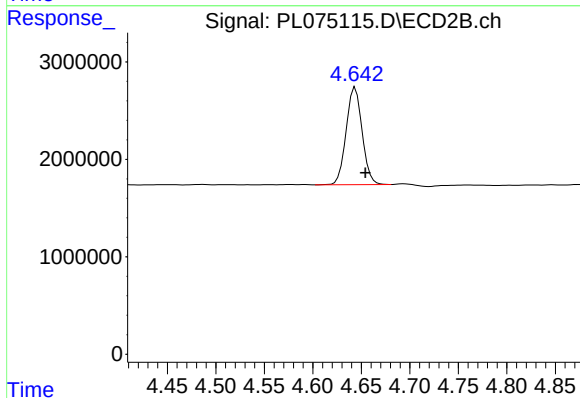


#1 Tetrachloro-m-xylene

R.T.: 4.644 min
Delta R.T.: -0.011 min
Response: 11457245
Conc: 8.35 ng/ml

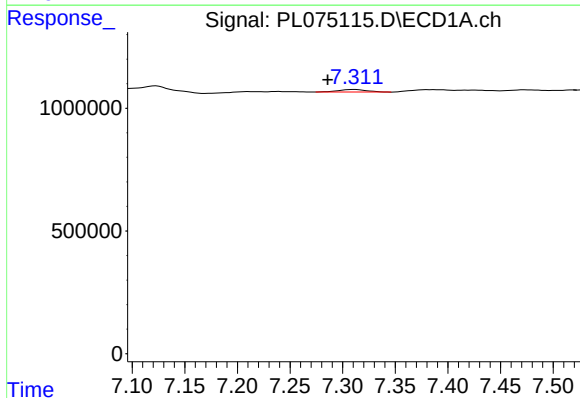


#4 Heptachlor

R.T.: 7.312 min
Delta R.T.: 0.026 min
Response: 198086
Conc: 0.31 ng/ml

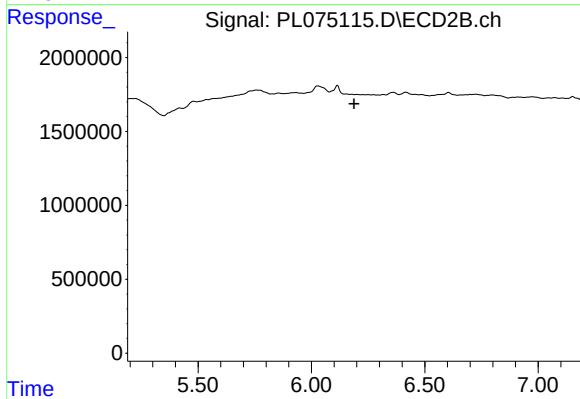

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 6.189 min
Response: 0
Conc: N.D.

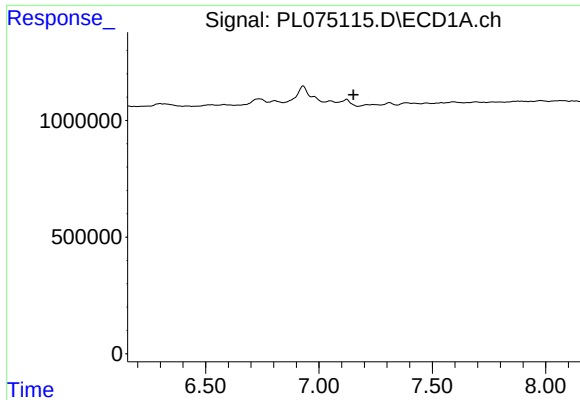

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 7.152 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

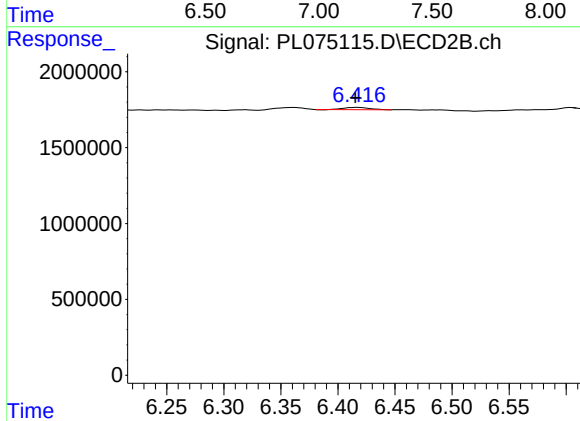


#7 delta-BHC

R.T.: 6.418 min
Delta R.T.: 0.002 min
Response: 232942
Conc: 0.15 ng/ml

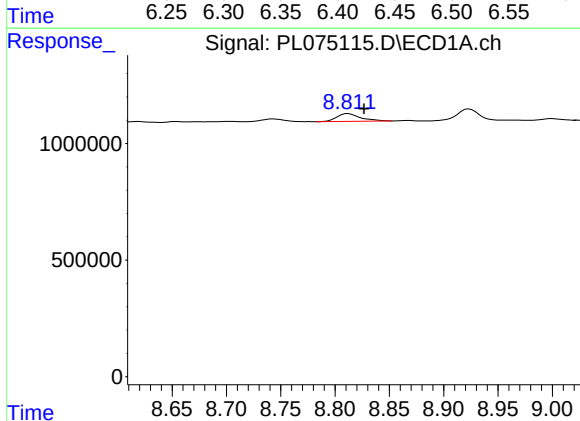


#13 Dieldrin

R.T.: 8.812 min
Delta R.T.: -0.014 min
Response: 505565
Conc: 0.96 ng/ml

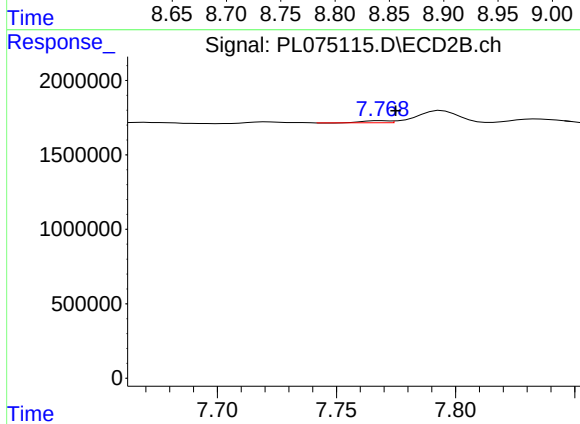

#13 Dieldrin


R.T.: 7.769 min
Delta R.T.: -0.005 min
Response: 97277
Conc: 0.08 ng/ml

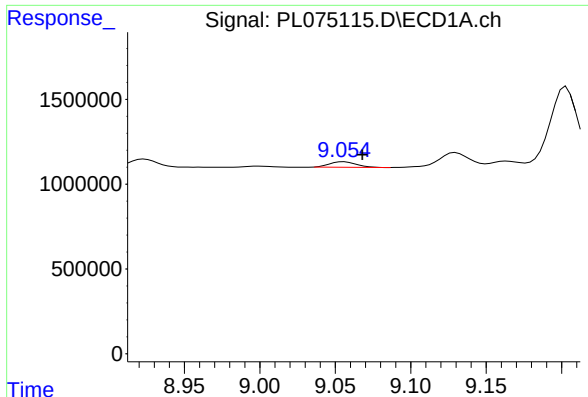

#14 Endrin


R.T.: 9.056 min
Delta R.T.: -0.012 min
Response: 399696
Conc: 0.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

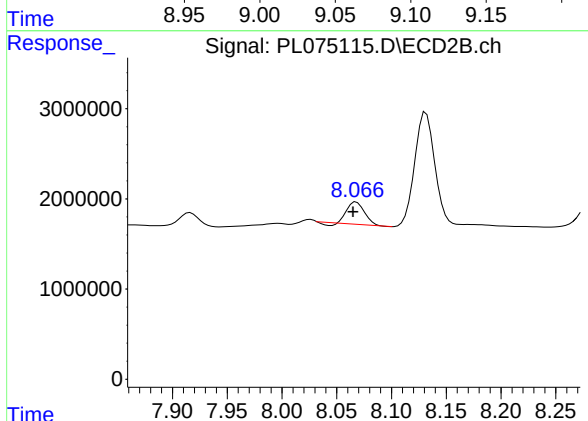


#14 Endrin

R.T.: 8.068 min
Delta R.T.: 0.003 min
Response: 2715336
Conc: 2.57 ng/ml

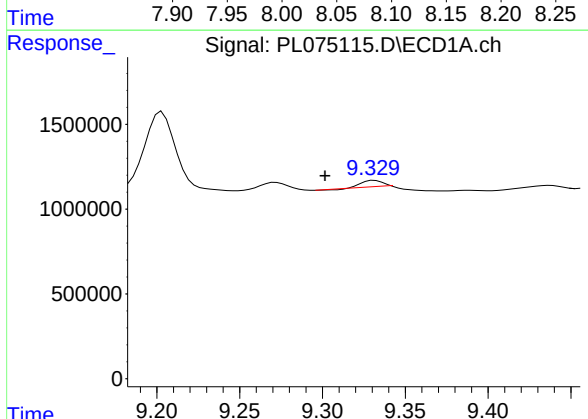


#15 Endosulfan II

R.T.: 9.332 min
Delta R.T.: 0.030 min
Response: 304417
Conc: 0.69 ng/ml

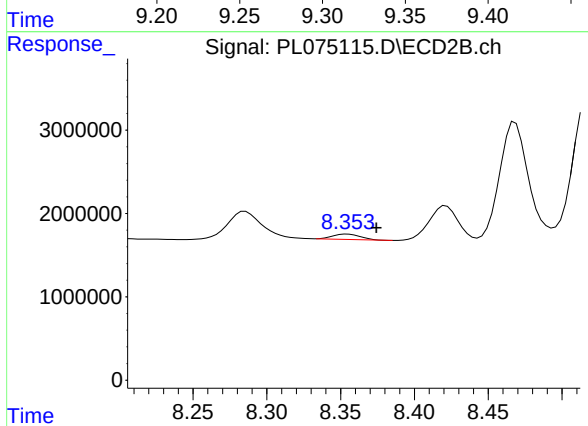

#15 Endosulfan II


R.T.: 8.355 min
Delta R.T.: -0.020 min
Response: 825507
Conc: 0.73 ng/ml

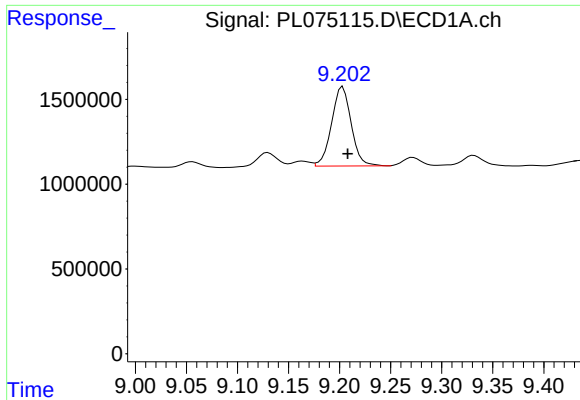

#16 4,4'-DDD


R.T.: 9.203 min
Delta R.T.: -0.005 min
Response: 6254714
Conc: 13.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

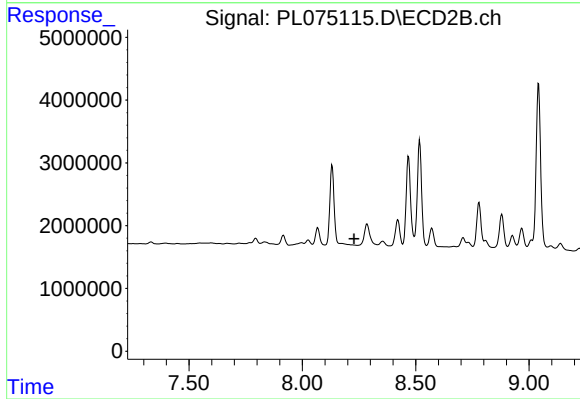


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.229 min
Response: 0
Conc: N.D.

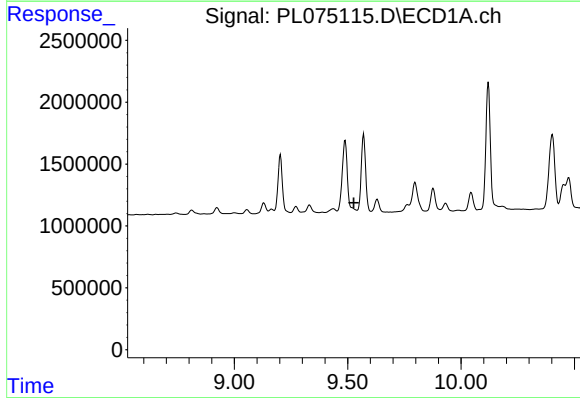


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.527 min
Response: 0
Conc: N.D.

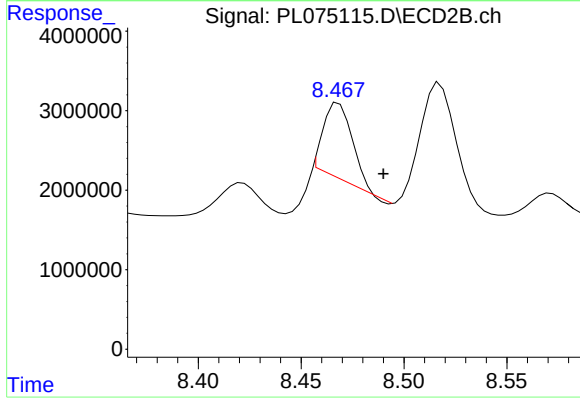

#17 4,4'-DDT


R.T.: 8.468 min
Delta R.T.: -0.022 min
Response: 9172904
Conc: 9.17 ng/ml

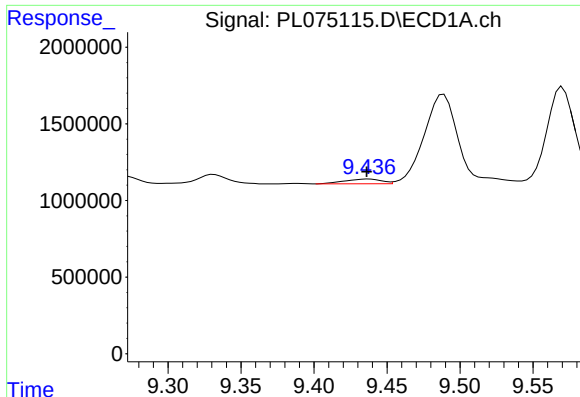

#18 Endrin aldehyde


R.T.: 9.437 min
Delta R.T.: 0.001 min
Response: 540223
Conc: 1.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

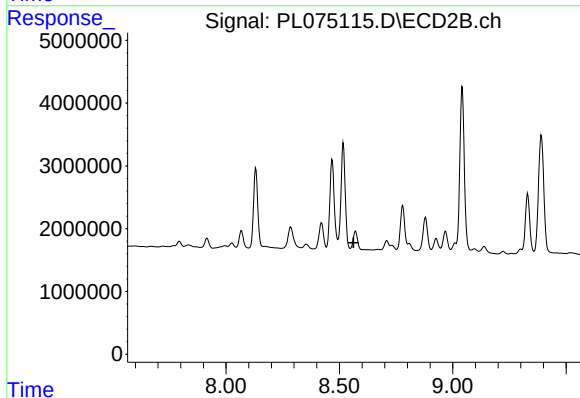


#18 Endrin aldehyde

R.T.: 8.571 min
Delta R.T.: 0.009 min
Response: -6801834
Conc: N.D.

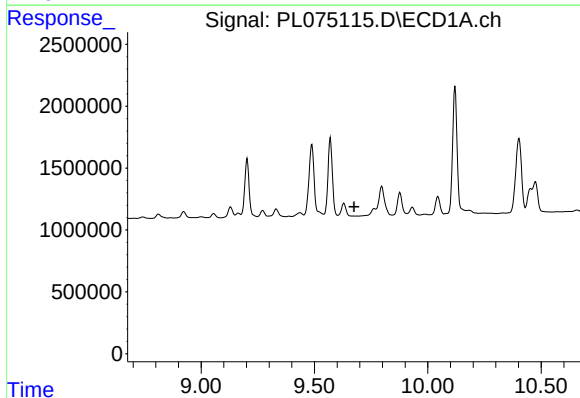


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 9.675 min
Response: 0
Conc: N.D.

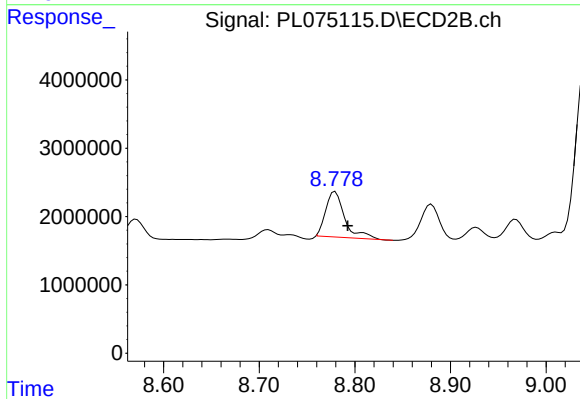

#19 Endosulfan Sulfate


R.T.: 8.779 min
Delta R.T.: -0.013 min
Response: 9013500
Conc: 8.28 ng/ml

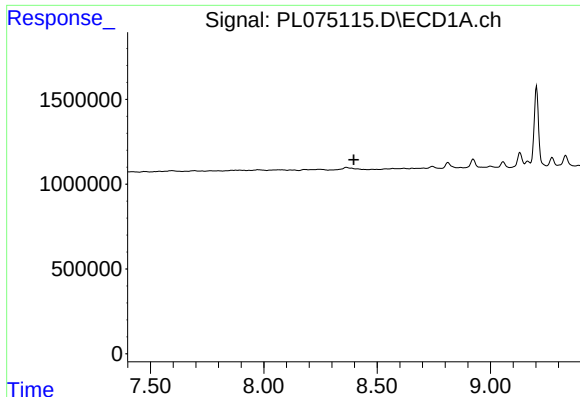

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

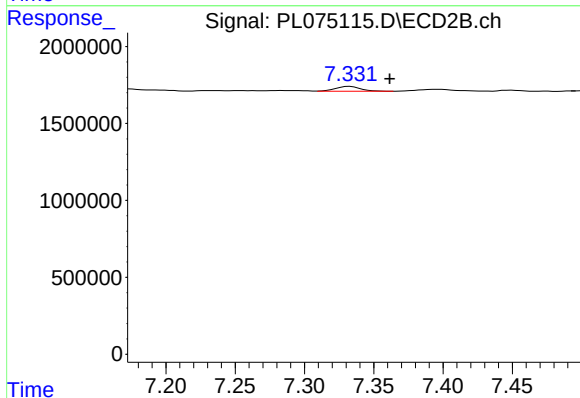


#25 Chlordane-3

R.T.: 7.333 min
Delta R.T.: -0.029 min
Response: 395374
Conc: 3.05 ng/ml

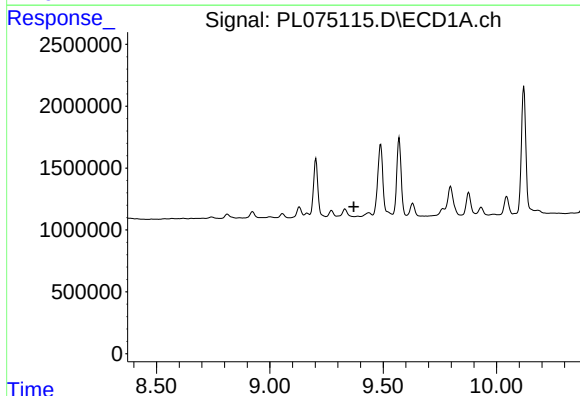


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 9.371 min
Response: 0
Conc: N.D.

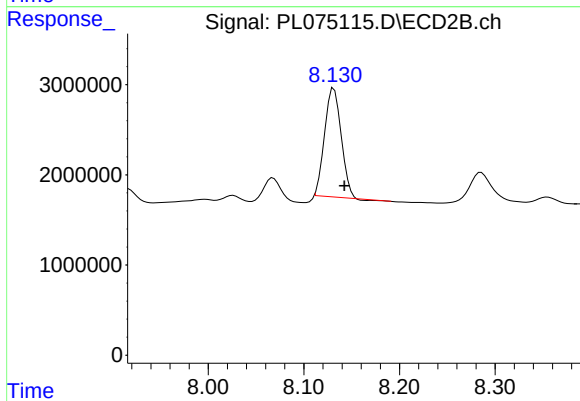

#27 Chlordane-5


R.T.: 8.132 min
Delta R.T.: -0.011 min
Response: 14312318
Conc: 387.09 ng/ml

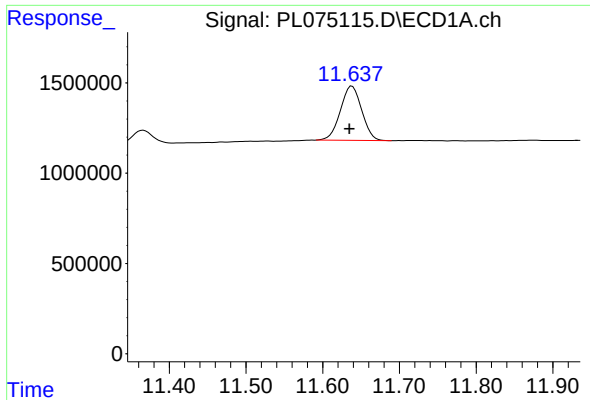

#28 Decachlorobiphenyl

R.T.: 11.638 min
Delta R.T.: 0.003 min
Response: 5834639
Conc: 13.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

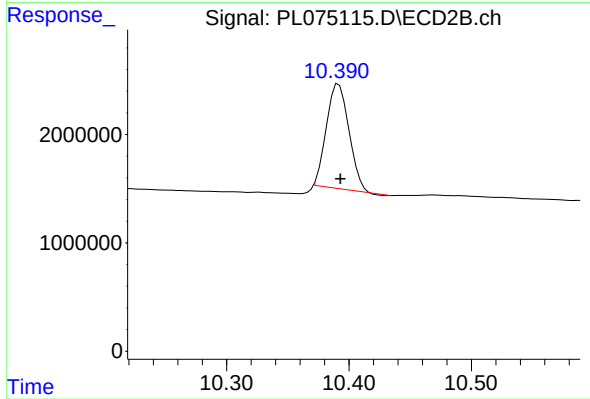

#28 Decachlorobiphenyl

R.T.: 10.392 min
Delta R.T.: -0.001 min
Response: 12288624
Conc: 11.97 ng/ml