

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052722\
 Data File : PL075123.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 May 2022 16:37
 Operator : AR\AJ
 Sample : N2927-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 28 02:46:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.643	4.644	10887366	30864239	21.443	22.487
28)	SA Decachlor...	11.640	10.392	7292696	15917985	16.330	15.508
Target Compounds							
2)	A alpha-BHC	0.000	5.380f	0	23082	N.D.	0.014 #
4)	MA Heptachlor	7.310f	0.000	261686	0	0.405	N.D. #
10)	B gamma-Chl...	0.000	7.334f	0	456962	N.D.	0.330 #
13)	MA Dieldrin	8.813	7.769	646698	266860	1.230	0.209 #
14)	MA Endrin	0.000	8.068	0	2376358	N.D.	2.250 #
15)	B Endosulfa...	9.274f	8.354f	542837	312461	1.235	0.277 #
16)	A 4,4'-DDD	9.204	0.000	2893637	0	6.400	N.D. #
17)	MA 4,4'-DDT	9.523	8.468f	274087	7316478	0.596	7.313 #
19)	B Endosulfa...	0.000	8.780	0	6312334	N.D.	5.799 #
25)	Chlordane-3	0.000	7.334f	0	456962	N.D.	3.521 #
27)	Chlordane-5	0.000	8.131	0	7853724	N.D.	212.413 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052722\
Data File : PL075123.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 May 2022 16:37
Operator : AR\AJ
Sample : N2927-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 02:46:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

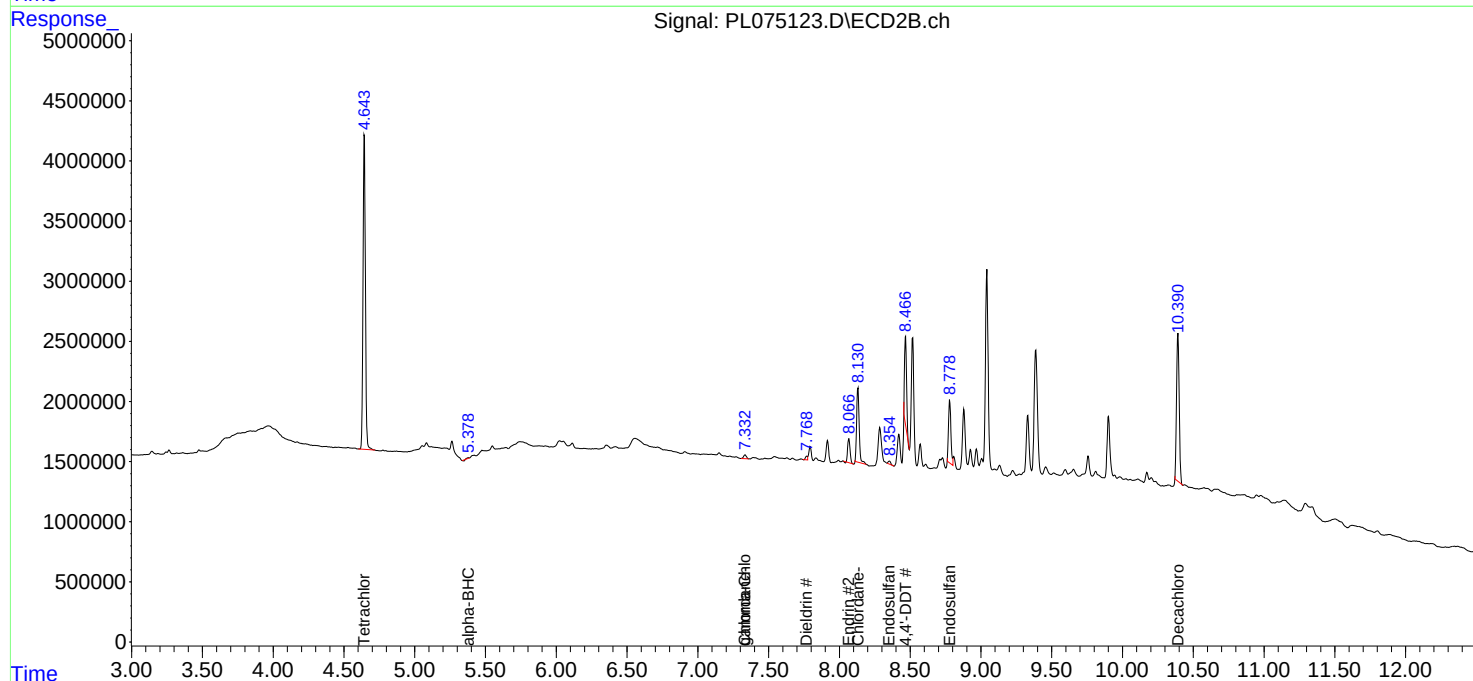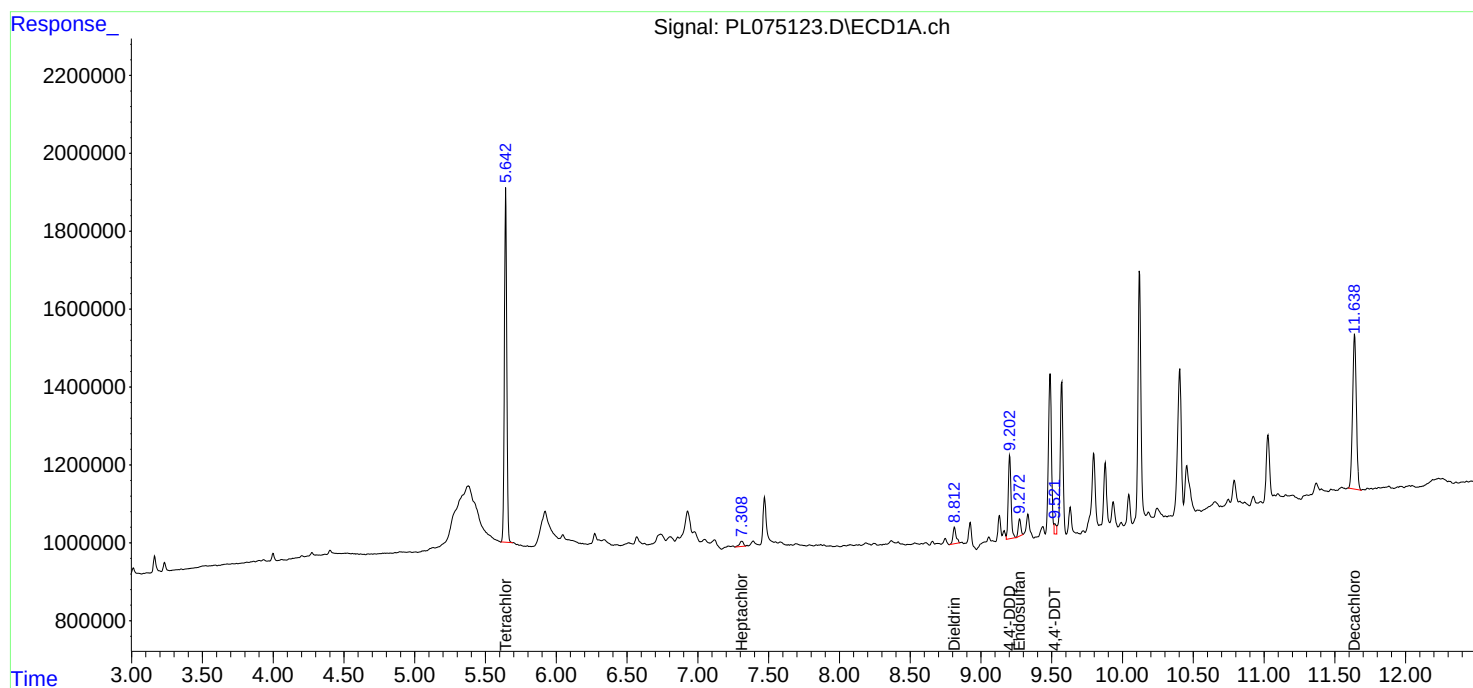


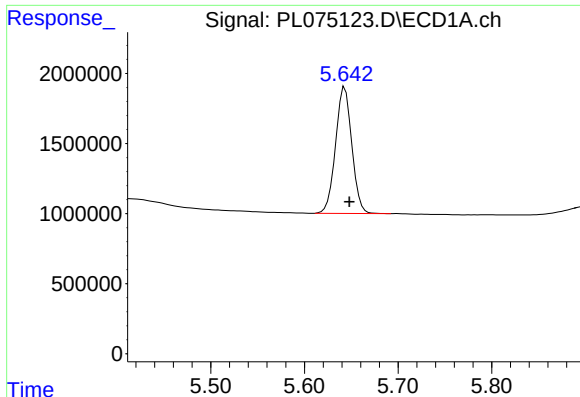

#1 Tetrachloro-m-xylene


R.T.: 5.643 min
Delta R.T.: -0.005 min
Response: 10887366
Conc: 21.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

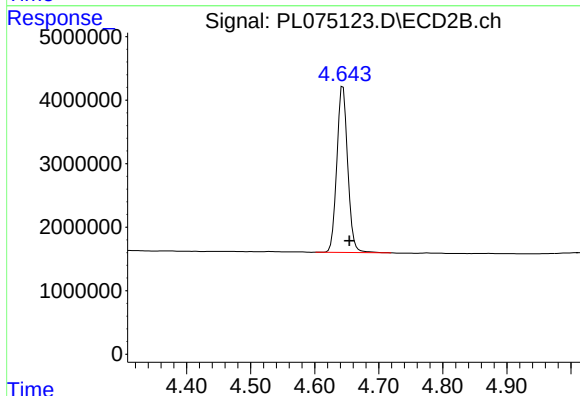


#1 Tetrachloro-m-xylene

R.T.: 4.644 min
Delta R.T.: -0.010 min
Response: 30864239
Conc: 22.49 ng/ml

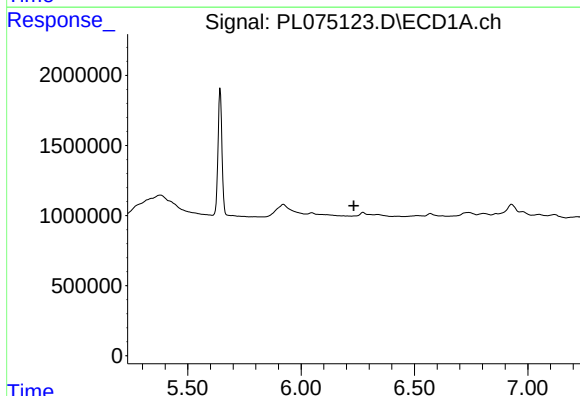


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 6.232 min
Response: 0
Conc: N.D.

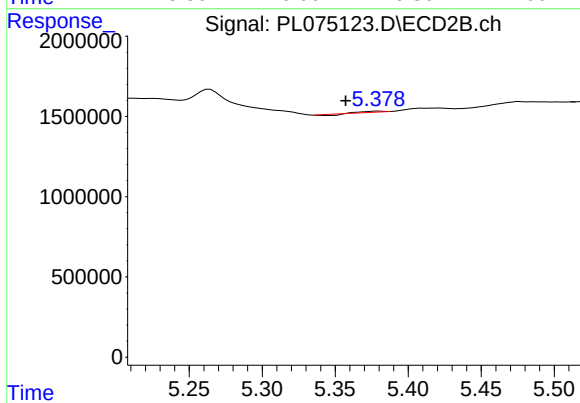

#2 alpha-BHC


R.T.: 5.380 min
Delta R.T.: 0.023 min
Response: 23082
Conc: 0.01 ng/ml

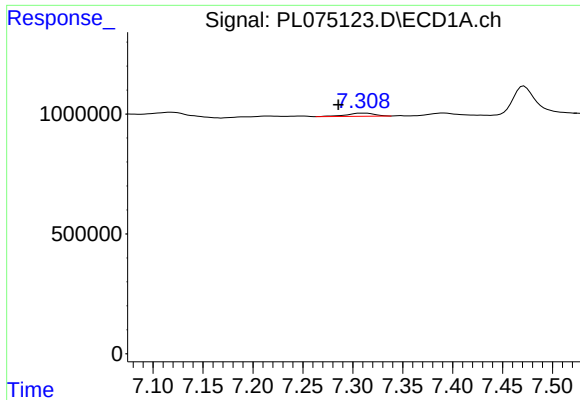

#4 Heptachlor


R.T.: 7.310 min
Delta R.T.: 0.025 min
Response: 261686
Conc: 0.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

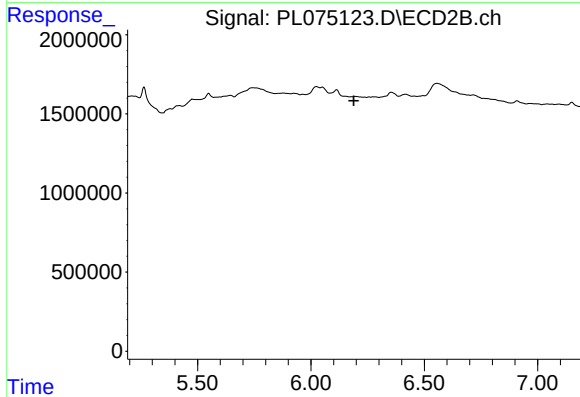


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 6.189 min
Response: 0
Conc: N.D.

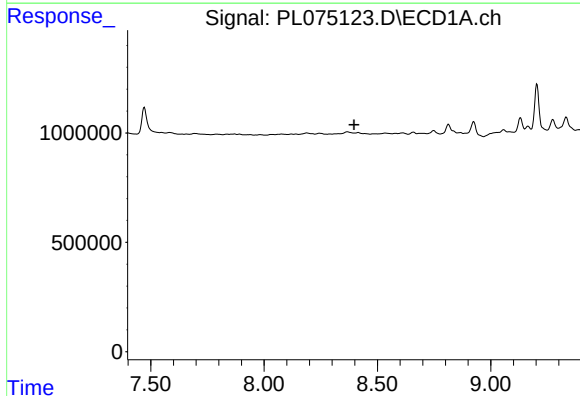


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.398 min
Response: 0
Conc: N.D.

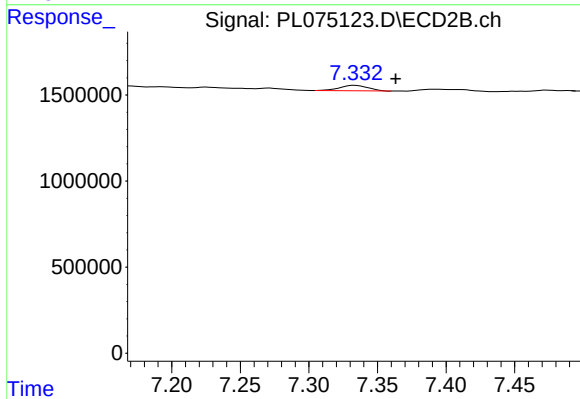

#10 gamma-Chlordane


R.T.: 7.334 min
Delta R.T.: -0.030 min
Response: 456962
Conc: 0.33 ng/ml

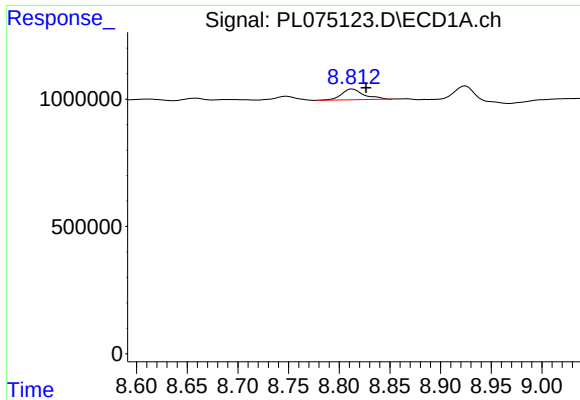

#13 Dieldrin


R.T.: 8.813 min
Delta R.T.: -0.013 min
Response: 646698
Conc: 1.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

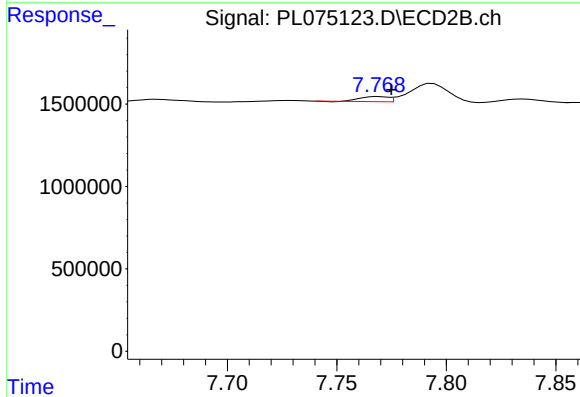


#13 Dieldrin

R.T.: 7.769 min
Delta R.T.: -0.006 min
Response: 266860
Conc: 0.21 ng/ml

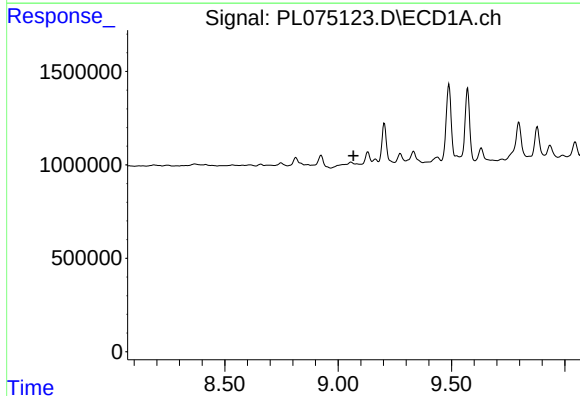


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 9.068 min
Response: 0
Conc: N.D.

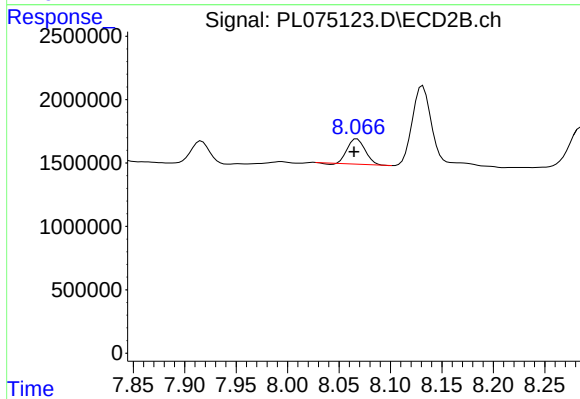

#14 Endrin


R.T.: 8.068 min
Delta R.T.: 0.003 min
Response: 2376358
Conc: 2.25 ng/ml

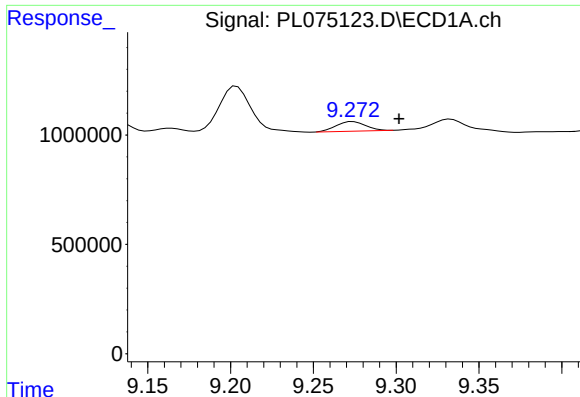

#15 Endosulfan II


R.T.: 9.274 min
Delta R.T.: -0.028 min
Response: 542837
Conc: 1.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

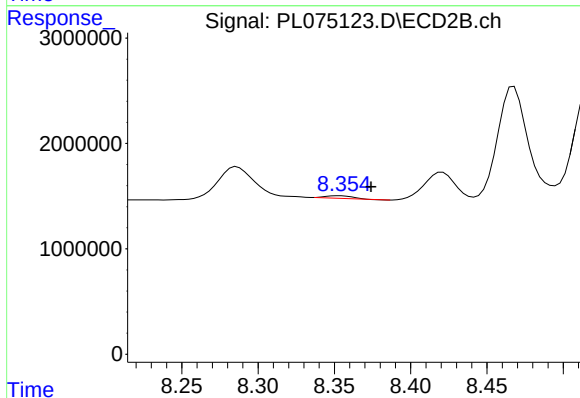


#15 Endosulfan II

R.T.: 8.354 min
Delta R.T.: -0.020 min
Response: 312461
Conc: 0.28 ng/ml

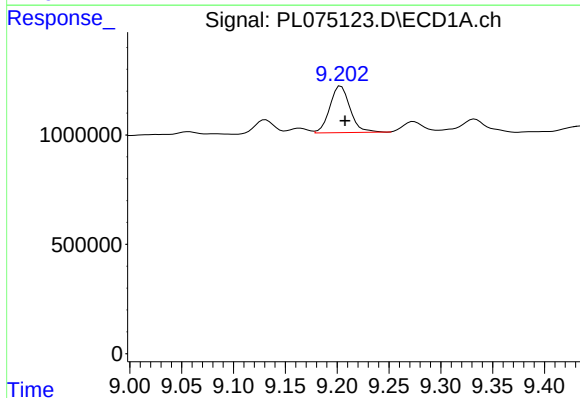


#16 4,4'-DDD

R.T.: 9.204 min
Delta R.T.: -0.004 min
Response: 2893637
Conc: 6.40 ng/ml

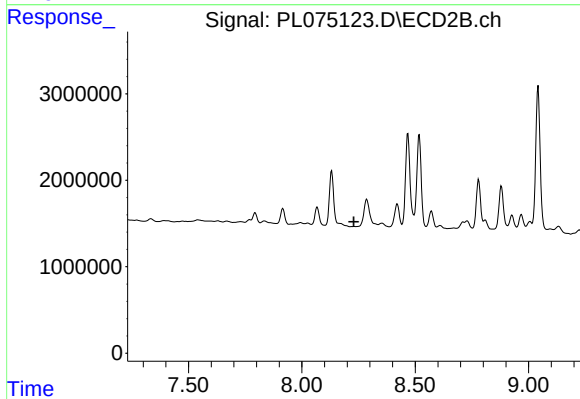

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.229 min
Response: 0
Conc: N.D.

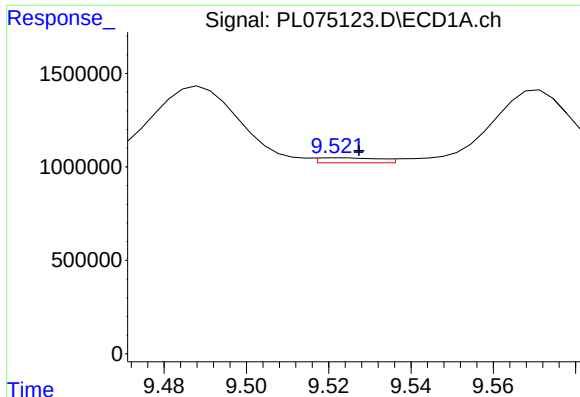

#17 4,4'-DDT


R.T.: 9.523 min
Delta R.T.: -0.005 min
Response: 274087
Conc: 0.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

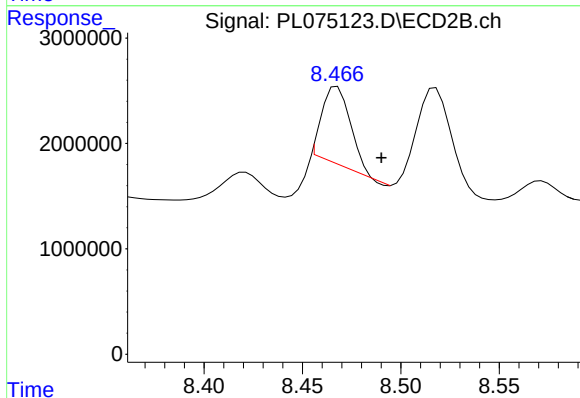


#17 4,4'-DDT

R.T.: 8.468 min
Delta R.T.: -0.022 min
Response: 7316478
Conc: 7.31 ng/ml

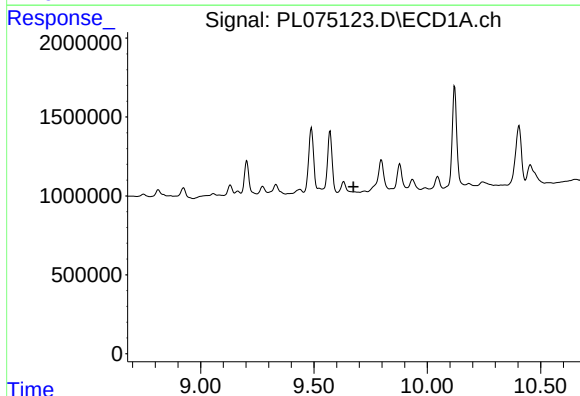


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 9.675 min
Response: 0
Conc: N.D.

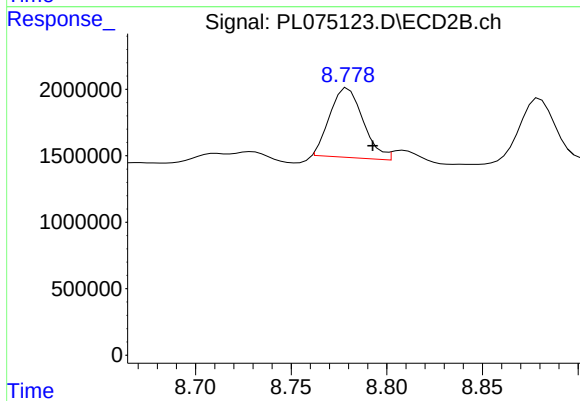

#19 Endosulfan Sulfate


R.T.: 8.780 min
Delta R.T.: -0.013 min
Response: 6312334
Conc: 5.80 ng/ml

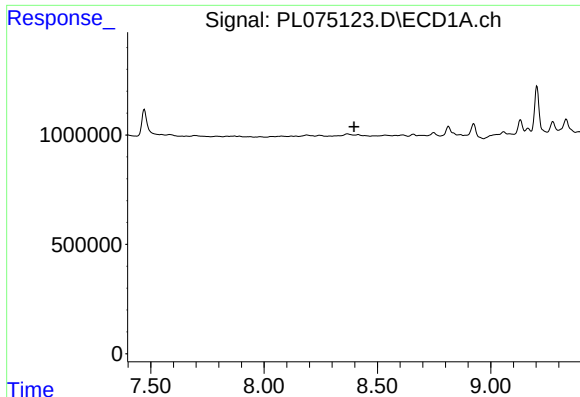

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

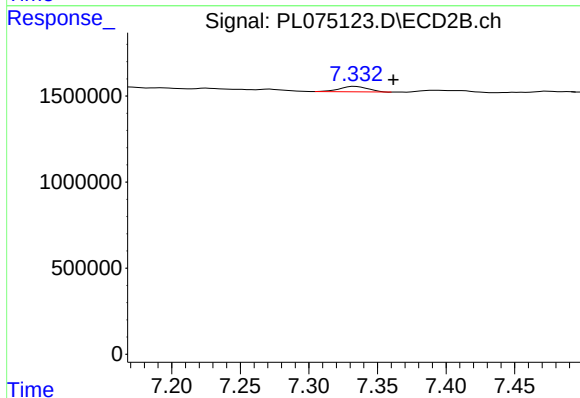


#25 Chlordane-3

R.T.: 7.334 min
Delta R.T.: -0.028 min
Response: 456962
Conc: 3.52 ng/ml

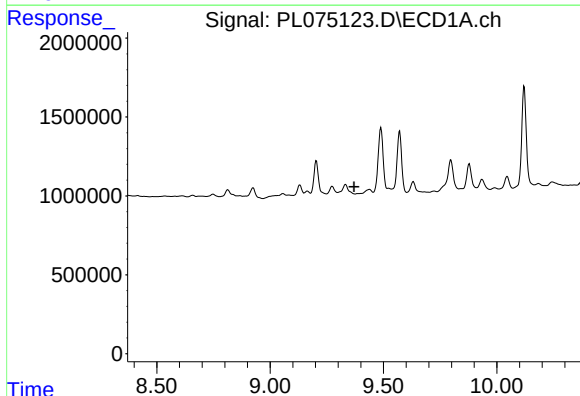


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 9.371 min
Response: 0
Conc: N.D.

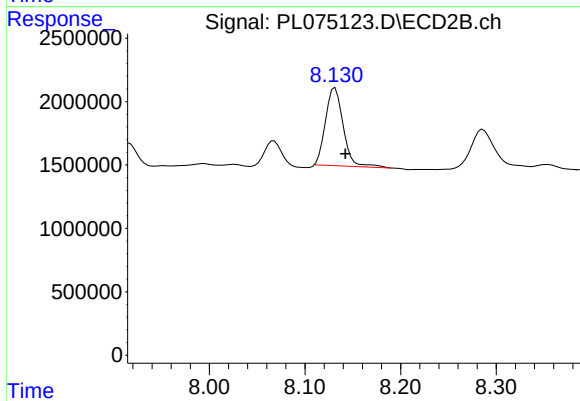

#27 Chlordane-5


R.T.: 8.131 min
Delta R.T.: -0.011 min
Response: 7853724
Conc: 212.41 ng/ml

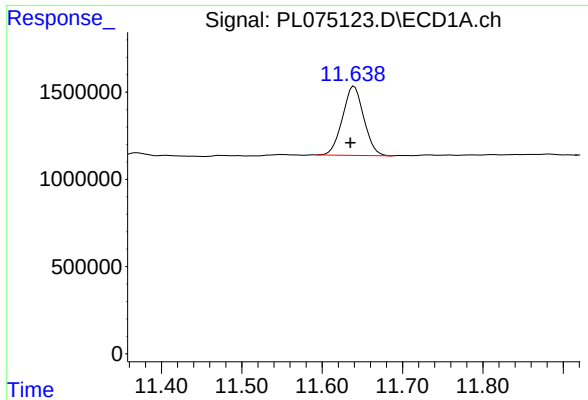

#28 Decachlorobiphenyl

R.T.: 11.640 min
Delta R.T.: 0.005 min
Response: 7292696
Conc: 16.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

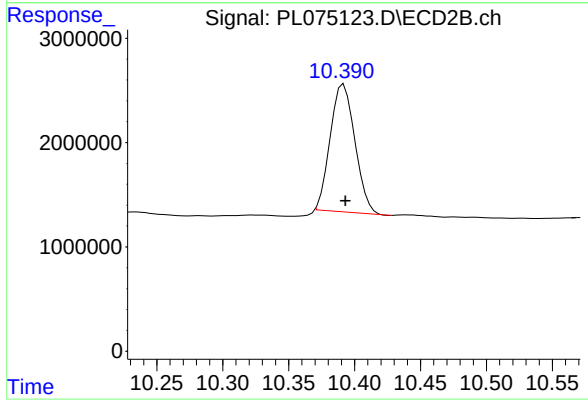

#28 Decachlorobiphenyl

R.T.: 10.392 min
Delta R.T.: -0.001 min
Response: 15917985
Conc: 15.51 ng/ml