

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052722\
 Data File : PL075127.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 May 2022 17:44
 Operator : AR\AJ
 Sample : PB145122BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 28 02:47:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.644	4.645	11216039	31425148	22.090	22.896
28)	SA Decachlor...	11.641	10.393	10459113	22261969	23.420	21.689
Target Compounds							
4)	MA Heptachlor	7.311f	0.000	229770	0	0.356	N.D. #
8)	B Heptachlo...	8.126	0.000	724257	0	1.273	N.D. #
10)	B gamma-Chl...	8.378f	0.000	460011	0	0.889	N.D. #
13)	MA Dieldrin	0.000	7.763	0	855695	N.D.	0.672 #
14)	MA Endrin	0.000	8.073	0	1713139	N.D.	1.622 #
21)	B Endrin ke...	10.187	0.000	371851	0	0.725	N.D. #
22)	Mirex	10.671f	0.000	191366	0	0.474	N.D. #
25)	Chlordane-3	8.378f	0.000	460011	0	6.719	N.D. #
26)	Chlordane-4	0.000	7.403f	0	230362	N.D.	1.680 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052722\
Data File : PL075127.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 May 2022 17:44
Operator : AR\AJ
Sample : PB145122BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 02:47:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

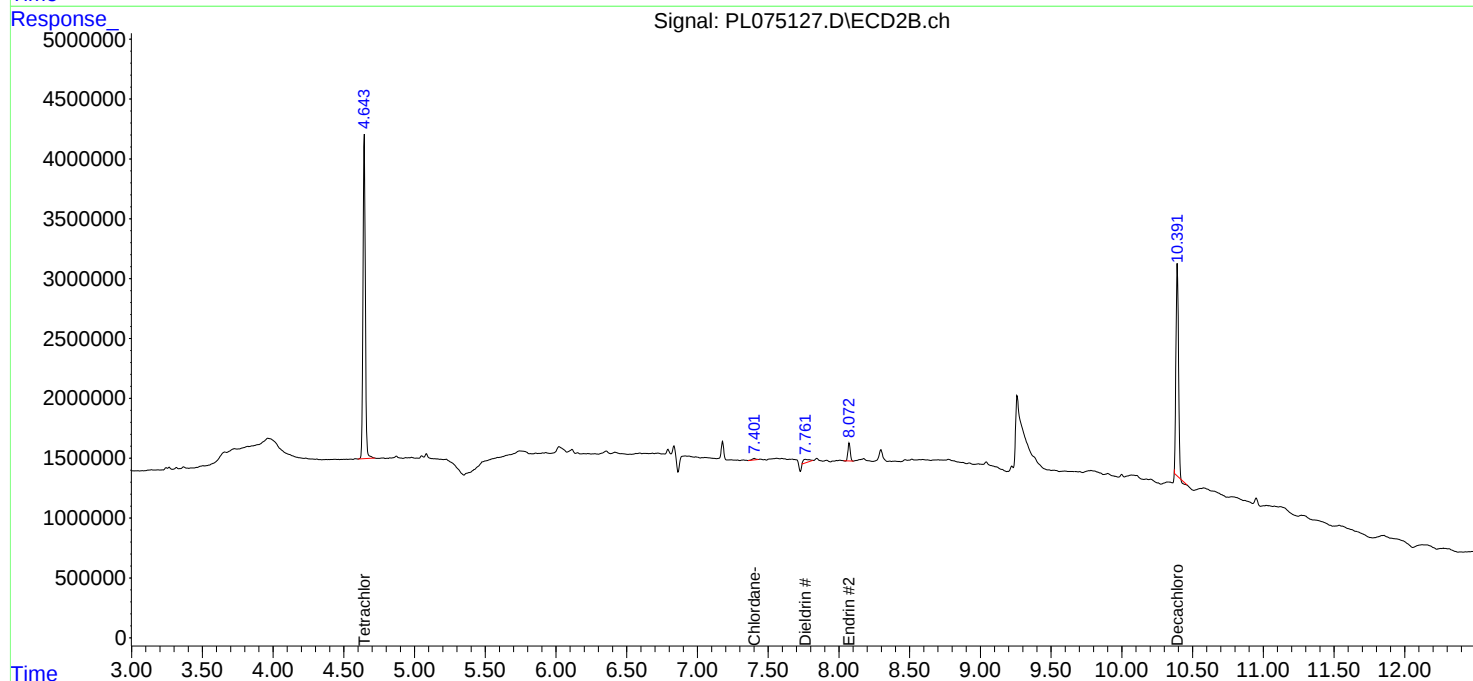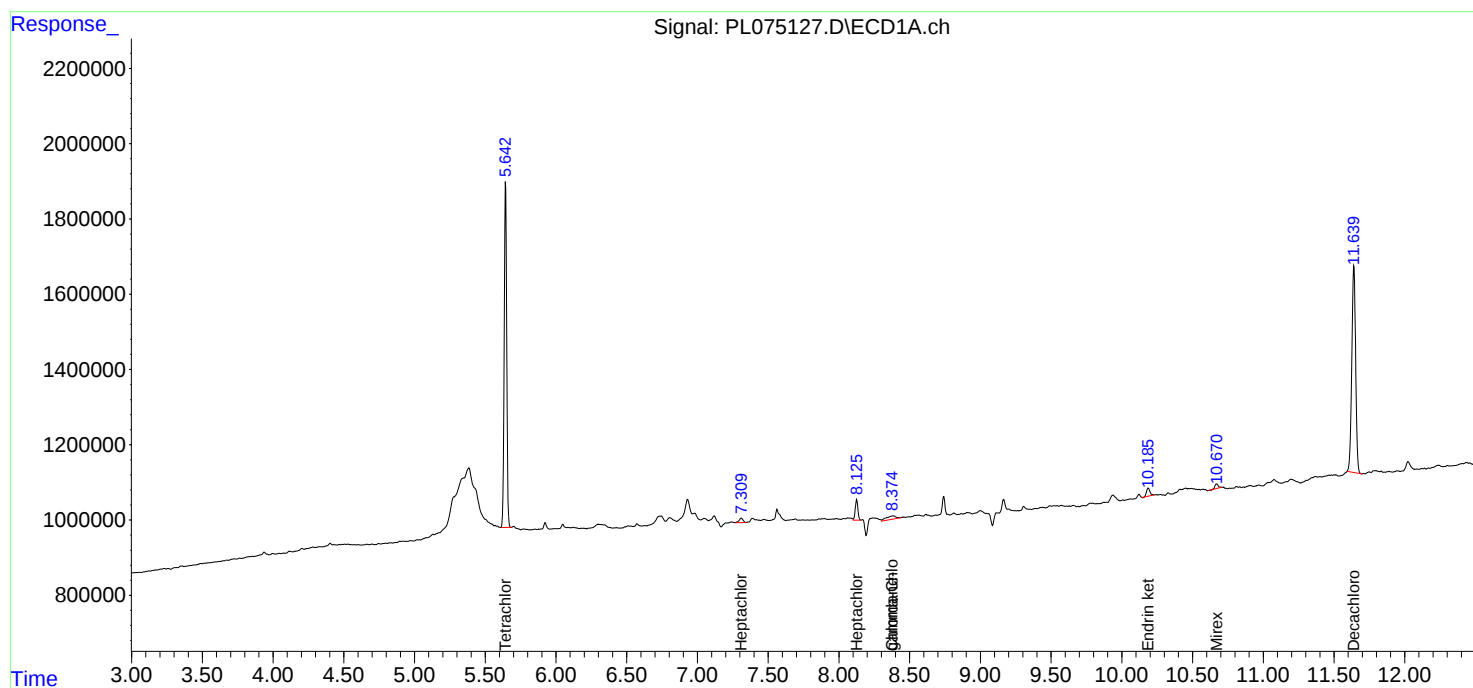


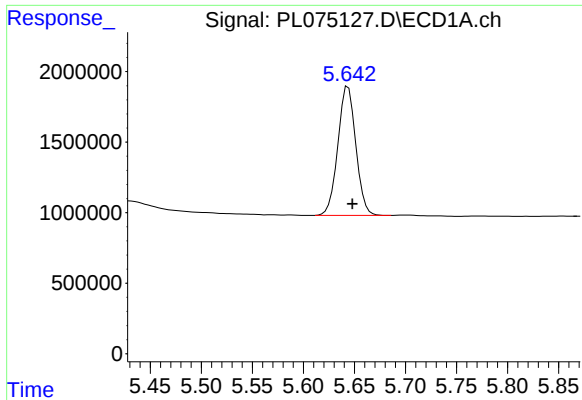

#1 Tetrachloro-m-xylene


R.T.: 5.644 min
Delta R.T.: -0.004 min
Response: 11216039
Conc: 22.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

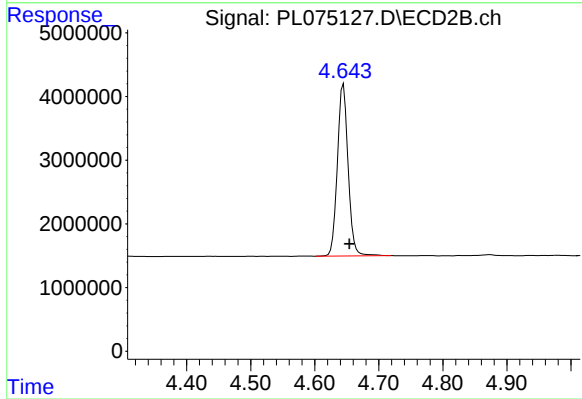


#1 Tetrachloro-m-xylene

R.T.: 4.645 min
Delta R.T.: -0.010 min
Response: 31425148
Conc: 22.90 ng/ml

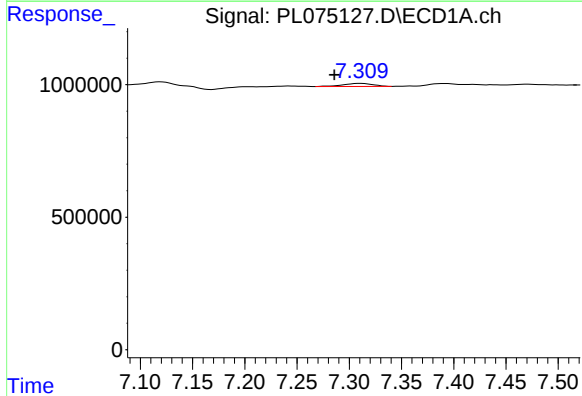


#4 Heptachlor

R.T.: 7.311 min
Delta R.T.: 0.025 min
Response: 229770
Conc: 0.36 ng/ml

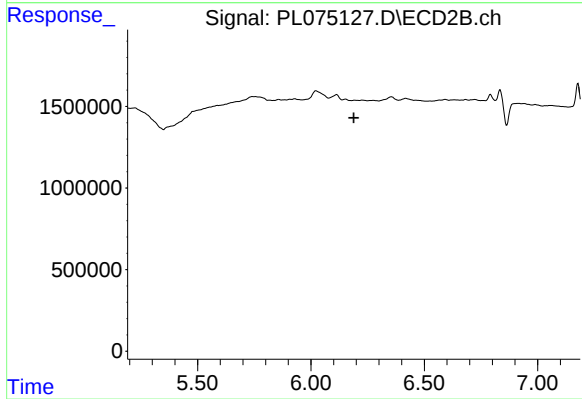

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 6.189 min
Response: 0
Conc: N.D.

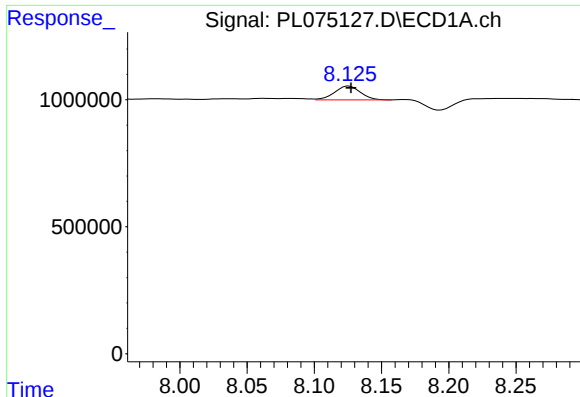

#8 Heptachlor epoxide


R.T.: 8.126 min
Delta R.T.: -0.001 min
Response: 724257
Conc: 1.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

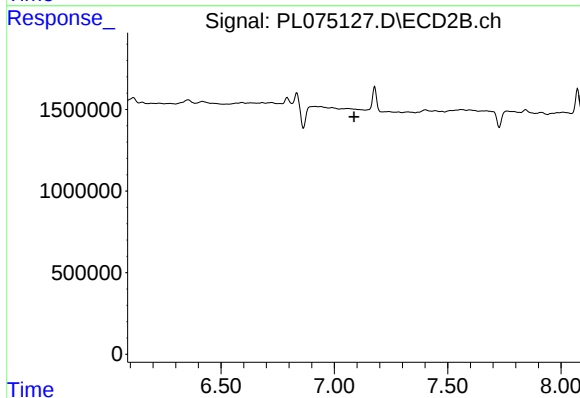


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.087 min
Response: 0
Conc: N.D.

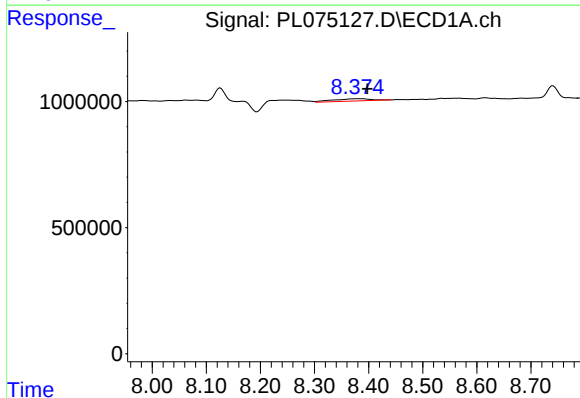


#10 gamma-Chlordane

R.T.: 8.378 min
Delta R.T.: -0.020 min
Response: 460011
Conc: 0.89 ng/ml

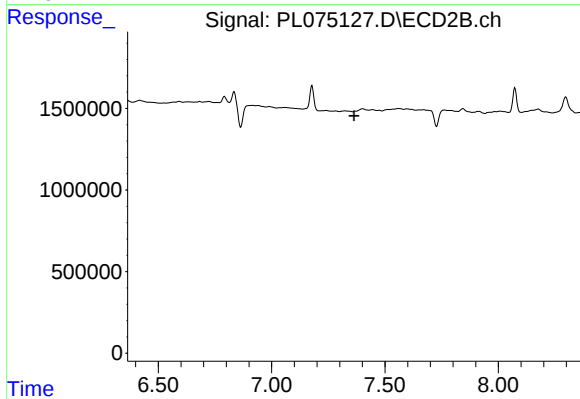

#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.363 min
Response: 0
Conc: N.D.

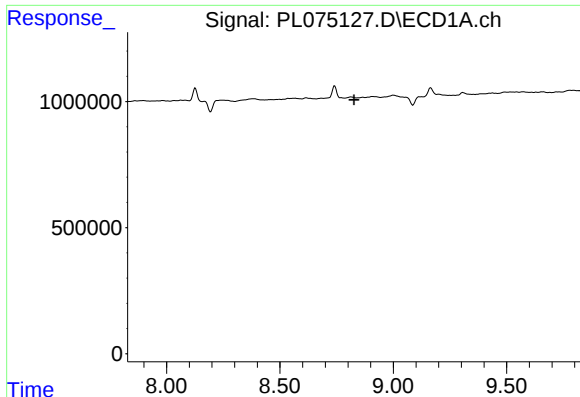

#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 8.827 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

#13 Dieldrin


R.T.: 7.763 min
Delta R.T.: -0.012 min
Response: 855695
Conc: 0.67 ng/ml

#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.068 min
Response: 0
Conc: N.D.

#14 Endrin


R.T.: 8.073 min
Delta R.T.: 0.008 min
Response: 1713139
Conc: 1.62 ng/ml

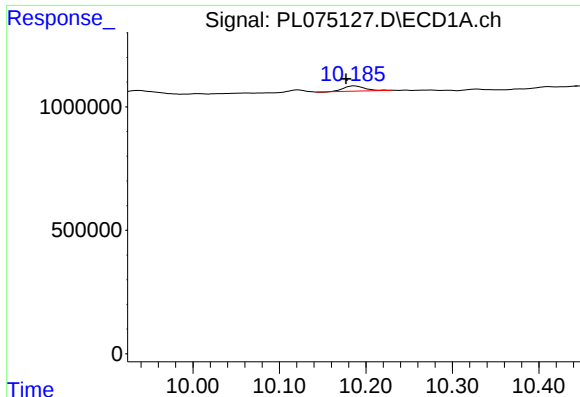

#21 Endrin ketone


R.T.: 10.187 min
Delta R.T.: 0.010 min
Response: 371851
Conc: 0.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

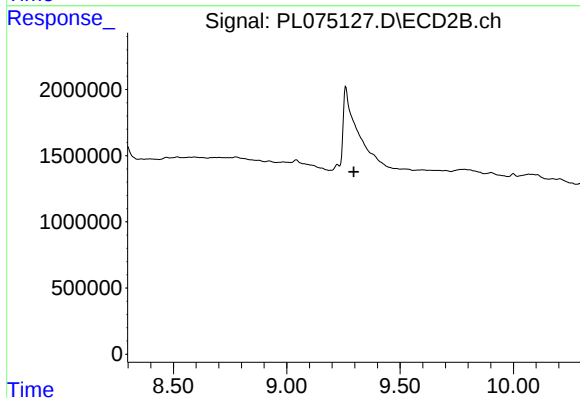


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.296 min
Response: 0
Conc: N.D.

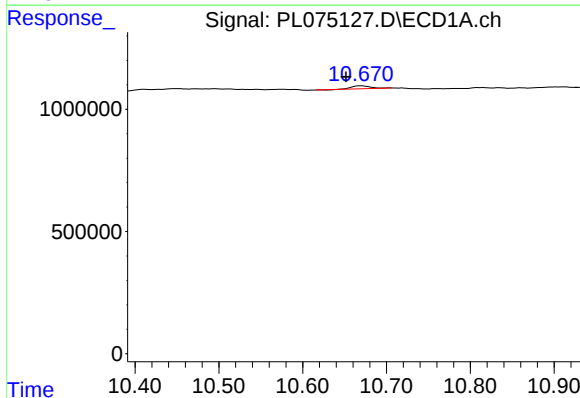


#22 Mirex

R.T.: 10.671 min
Delta R.T.: 0.019 min
Response: 191366
Conc: 0.47 ng/ml

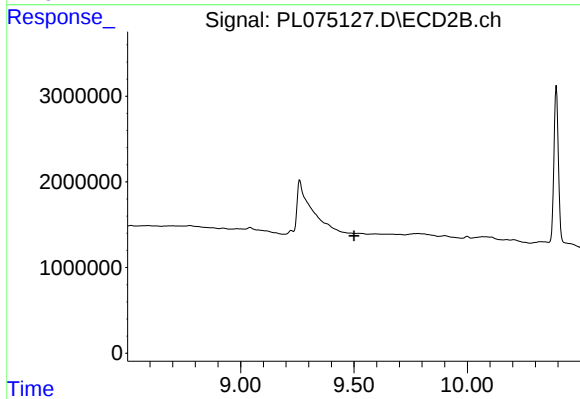

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 9.501 min
Response: 0
Conc: N.D.

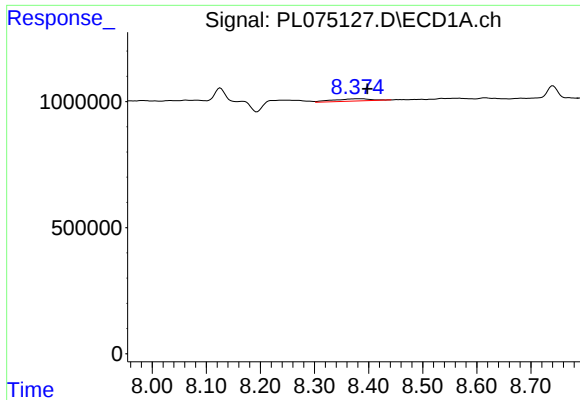

#25 Chlordane-3


R.T.: 8.378 min
Delta R.T.: -0.020 min
Response: 460011
Conc: 6.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

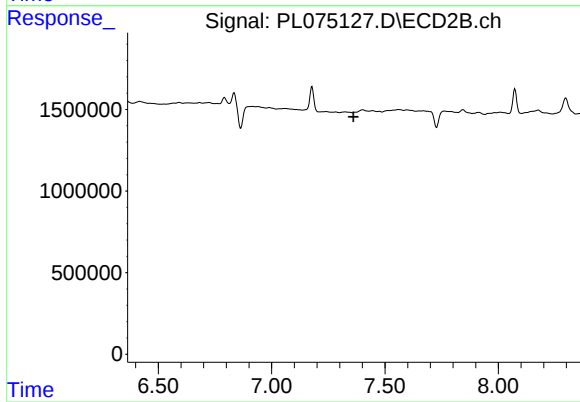


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.362 min
Response: 0
Conc: N.D.

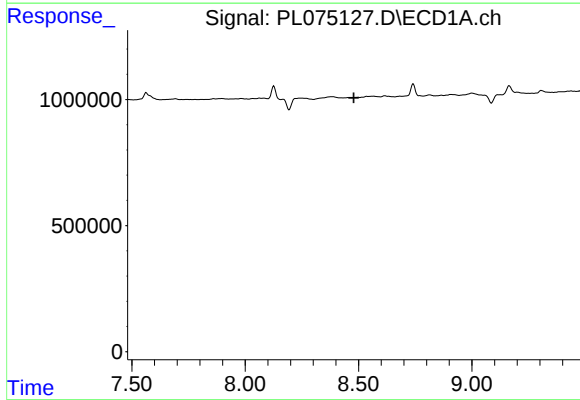


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.479 min
Response: 0
Conc: N.D.

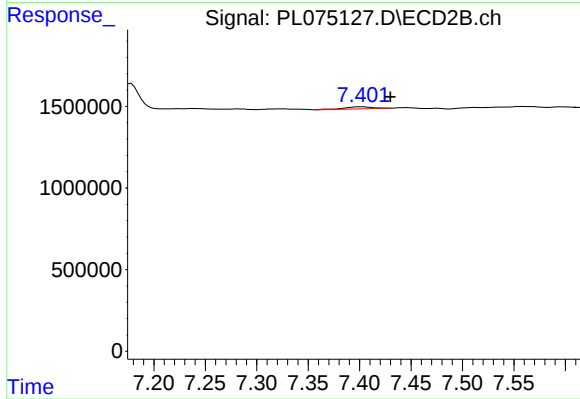

#26 Chlordane-4


R.T.: 7.403 min
Delta R.T.: -0.027 min
Response: 230362
Conc: 1.68 ng/ml

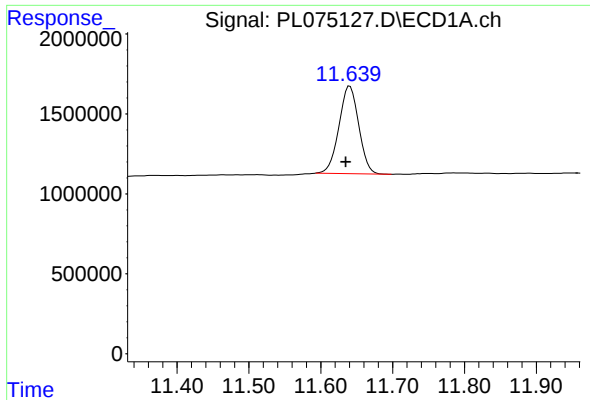

#28 Decachlorobiphenyl

R.T.: 11.641 min
Delta R.T.: 0.006 min
Response: 10459113
Conc: 23.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

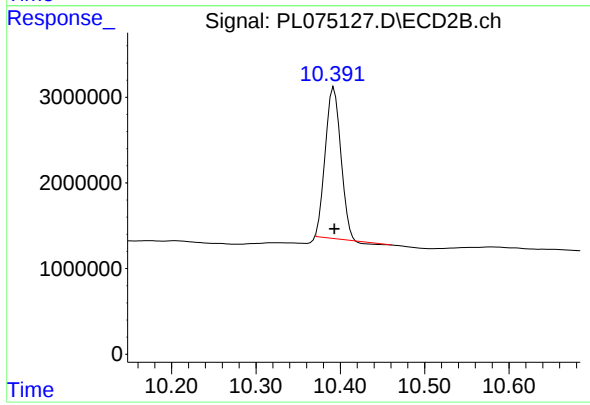

#28 Decachlorobiphenyl

R.T.: 10.393 min
Delta R.T.: 0.000 min
Response: 22261969
Conc: 21.69 ng/ml