

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052722\
 Data File : PL075160.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2022 05:23
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 28 08:58:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
 Quant Title : GC Extractables
 QLast Update : Sat May 14 02:37:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.644	4.645	13081954	35727073	25.765	26.030
28)	SA Decachlor...	11.643	10.394	11358001	25240098	25.433	24.591
Target Compounds							
7)	B delta-BHC	0.000	6.409	0	352635	N.D.	0.226 #
8)	B Heptachlo...	8.127	0.000	362461	0	0.637	N.D. #
10)	B gamma-Chl...	8.380f	0.000	304831	0	0.589	N.D. #
13)	MA Dieldrin	0.000	7.767	0	560633	N.D.	0.440 #
14)	MA Endrin	0.000	8.075	0	661220	N.D.	0.626 #
16)	A 4,4'-DDD	9.207	0.000	103759	0	0.229	N.D. #
17)	MA 4,4'-DDT	0.000	8.469f	0	174981	N.D.	0.175 #
19)	B Endosulfa...	0.000	8.780	0	232214	N.D.	0.213 #
21)	B Endrin ke...	10.188	0.000	232080	0	0.453	N.D. #
25)	Chlordane-3	8.380f	0.000	304831	0	4.453	N.D. #
27)	Chlordane-5	0.000	8.132	0	182515	N.D.	4.936 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052722\
Data File : PL075160.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2022 05:23
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 08:58:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051122.M
Quant Title : GC Extractables
QLast Update : Sat May 14 02:37:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

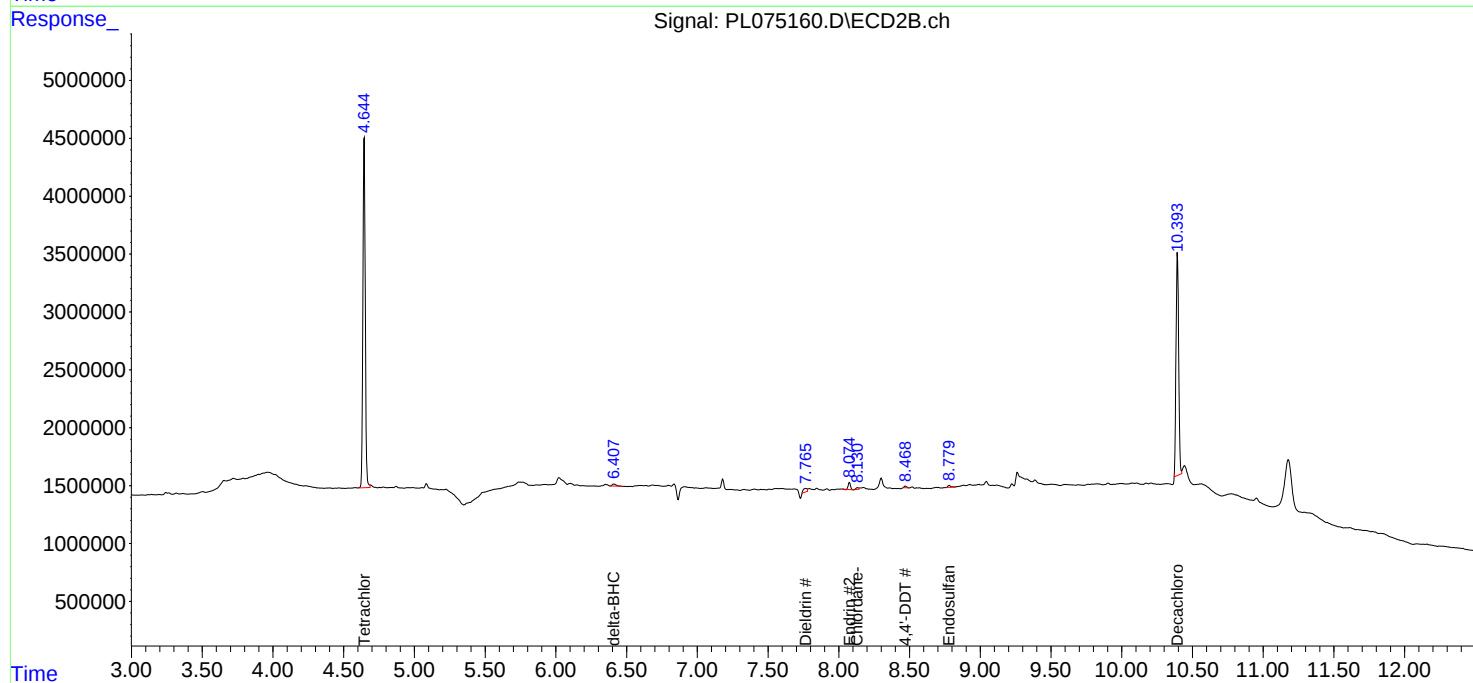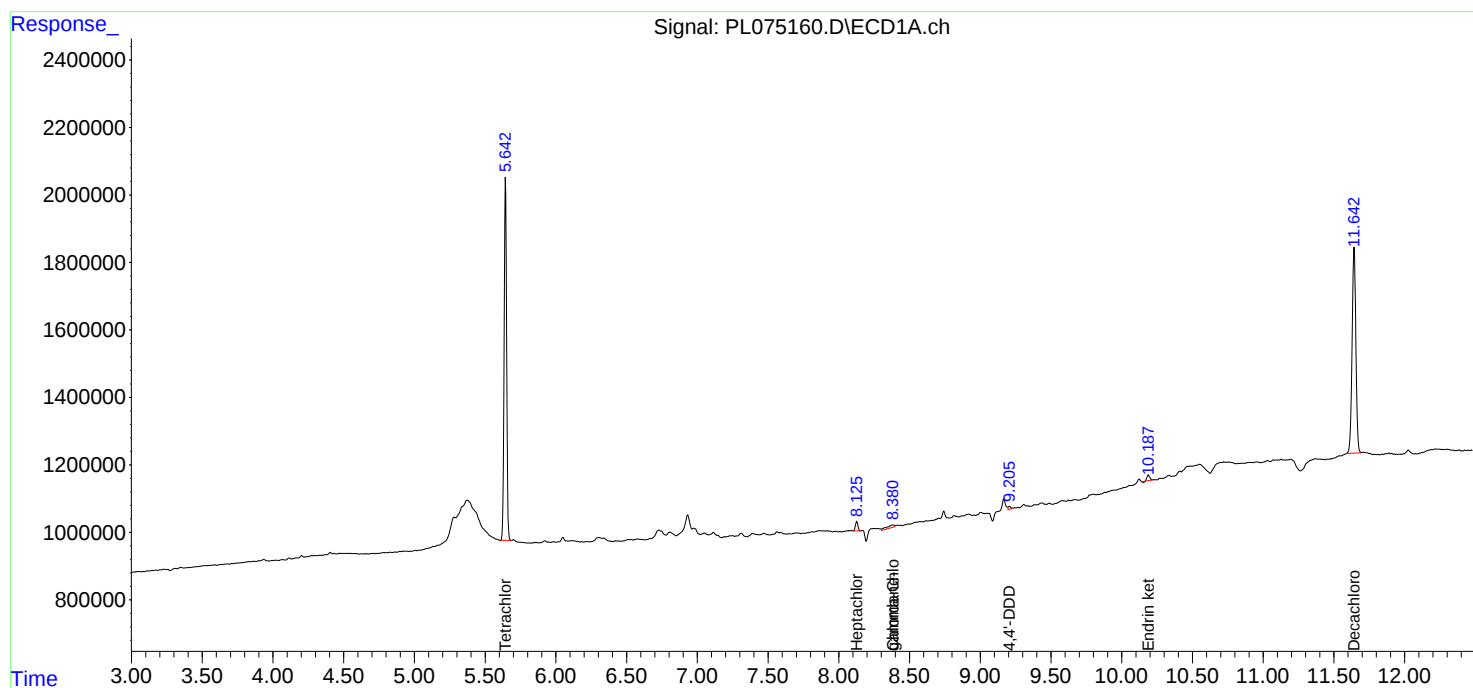


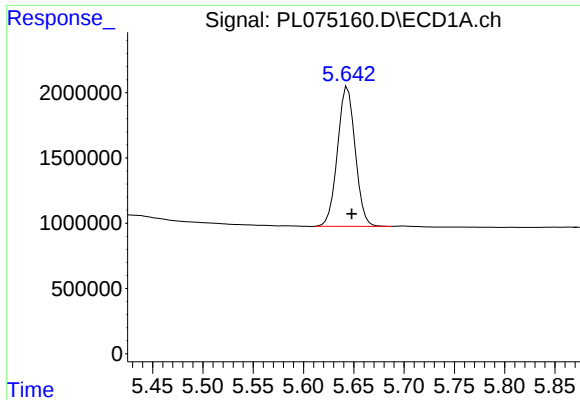

#1 Tetrachloro-m-xylene


R.T.: 5.644 min
Delta R.T.: -0.004 min
Response: 13081954
Conc: 25.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

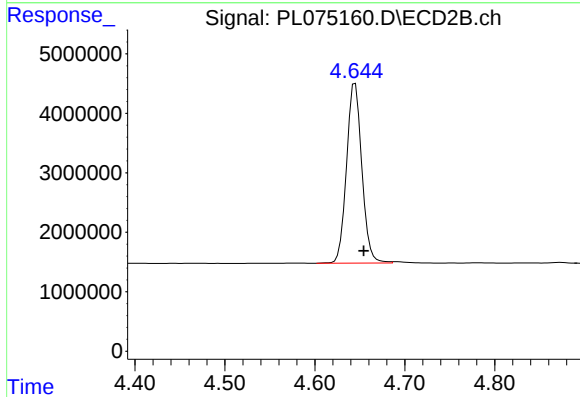


#1 Tetrachloro-m-xylene

R.T.: 4.645 min
Delta R.T.: -0.009 min
Response: 35727073
Conc: 26.03 ng/ml

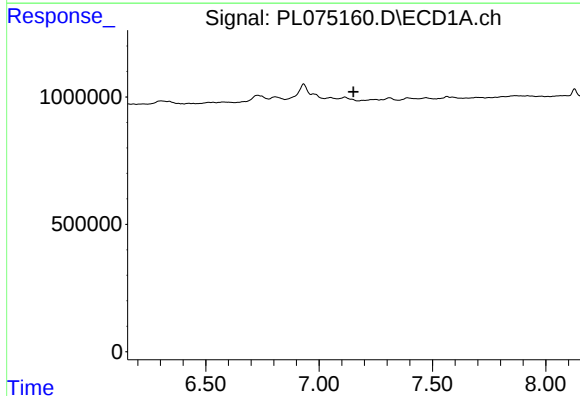


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.152 min
Response: 0
Conc: N.D.

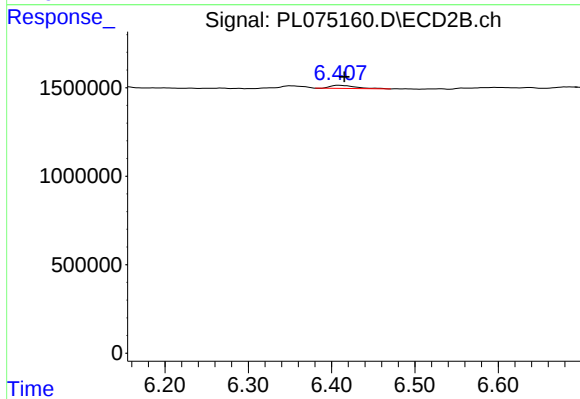

#7 delta-BHC


R.T.: 6.409 min
Delta R.T.: -0.006 min
Response: 352635
Conc: 0.23 ng/ml

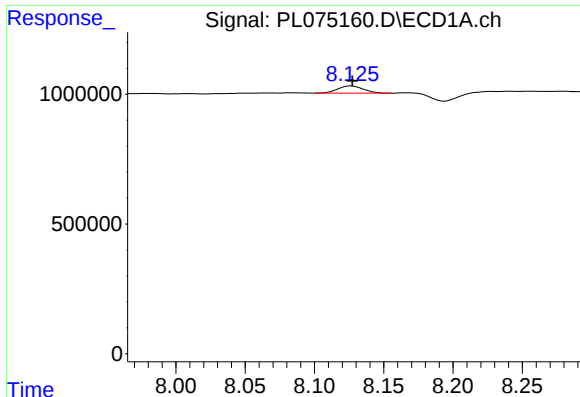

#8 Heptachlor epoxide

R.T.: 8.127 min
Delta R.T.: 0.000 min
Response: 362461
Conc: 0.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

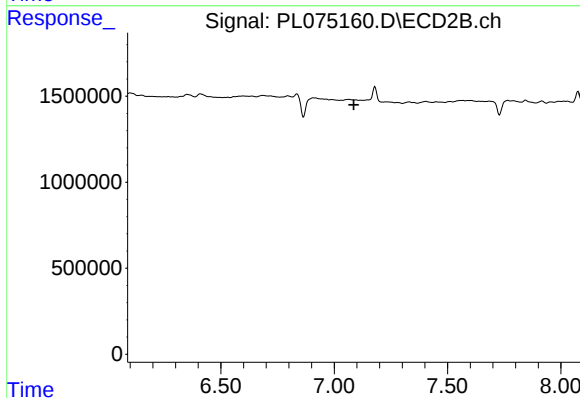

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 7.087 min
Response: 0
Conc: N.D.

#10 gamma-Chlordane

R.T.: 8.380 min
Delta R.T.: -0.018 min
Response: 304831
Conc: 0.59 ng/ml

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 7.363 min
Response: 0
Conc: N.D.

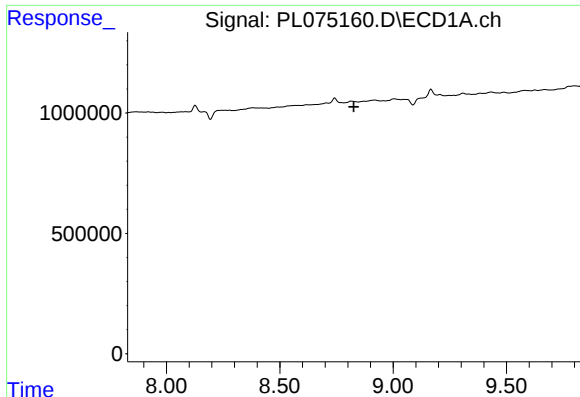

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.827 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

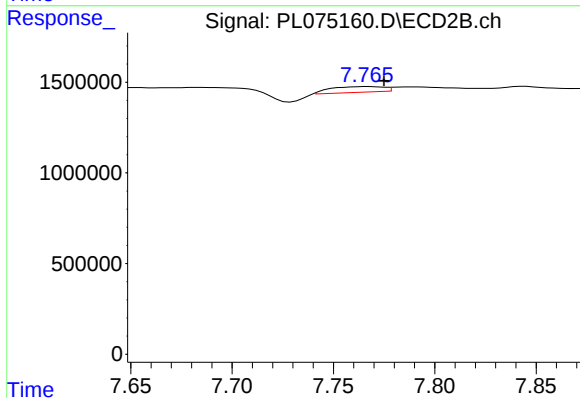


#13 Dieldrin

R.T.: 7.767 min
Delta R.T.: -0.008 min
Response: 560633
Conc: 0.44 ng/ml

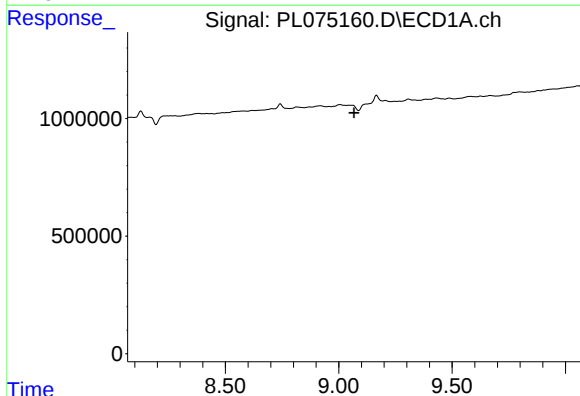


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.068 min
Response: 0
Conc: N.D.

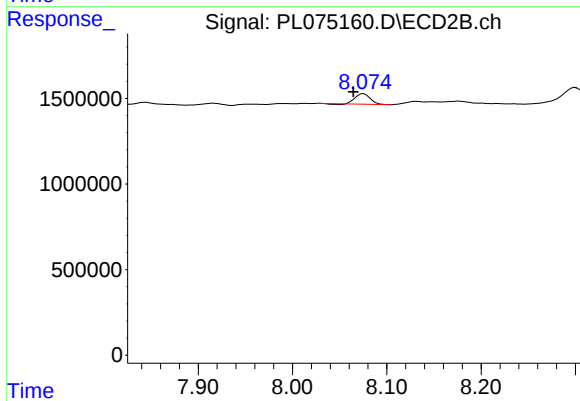

#14 Endrin


R.T.: 8.075 min
Delta R.T.: 0.011 min
Response: 661220
Conc: 0.63 ng/ml

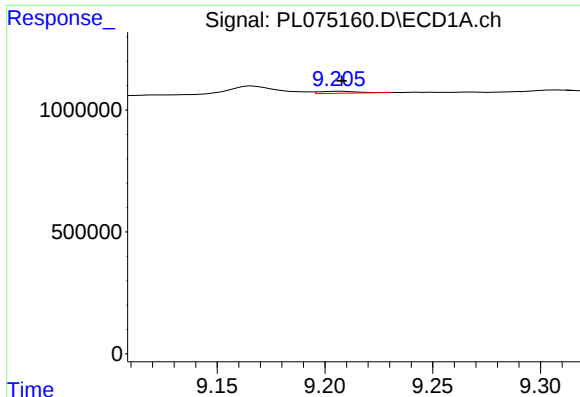

#16 4,4'-DDD


R.T.: 9.207 min
Delta R.T.: 0.000 min
Response: 103759
Conc: 0.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

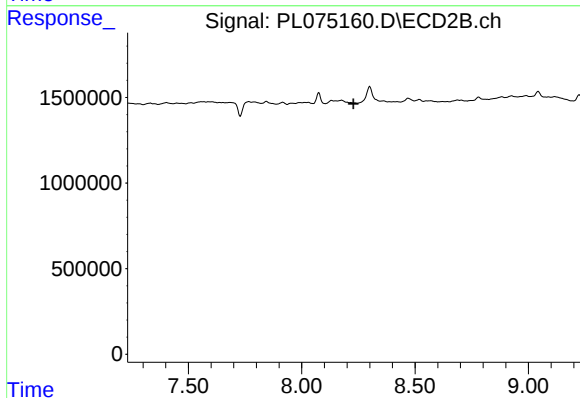


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.229 min
Response: 0
Conc: N.D.

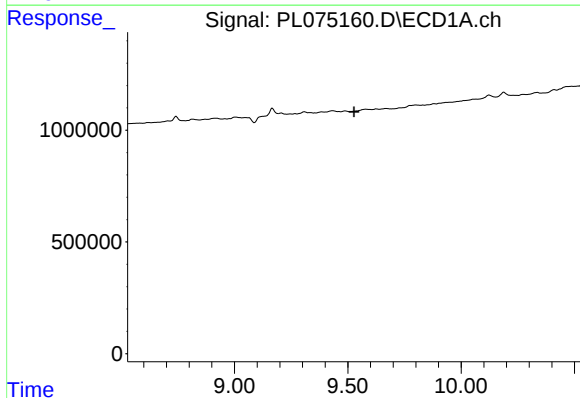


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.527 min
Response: 0
Conc: N.D.

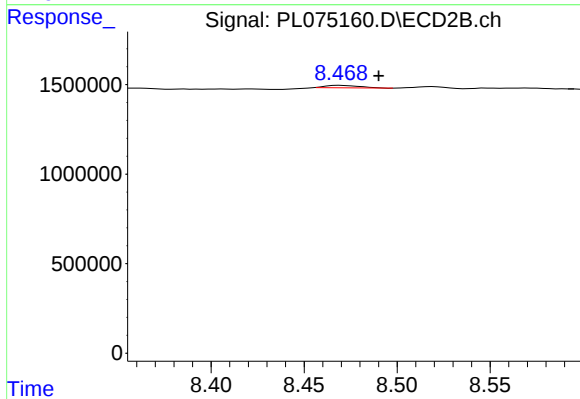

#17 4,4'-DDT


R.T.: 8.469 min
Delta R.T.: -0.021 min
Response: 174981
Conc: 0.17 ng/ml

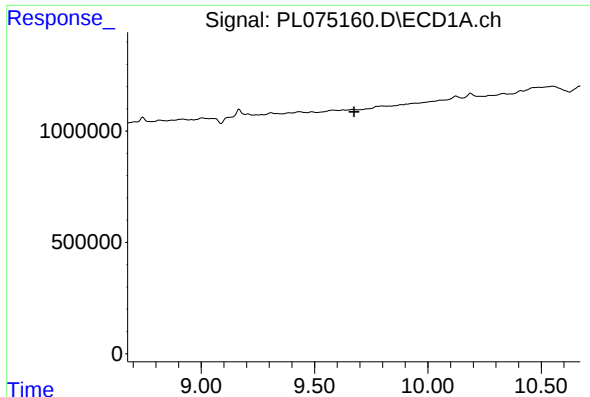

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 9.675 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

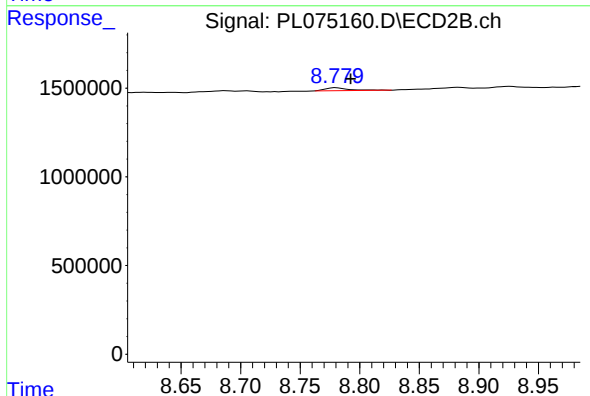


#19 Endosulfan Sulfate

R.T.: 8.780 min
Delta R.T.: -0.012 min
Response: 232214
Conc: 0.21 ng/ml

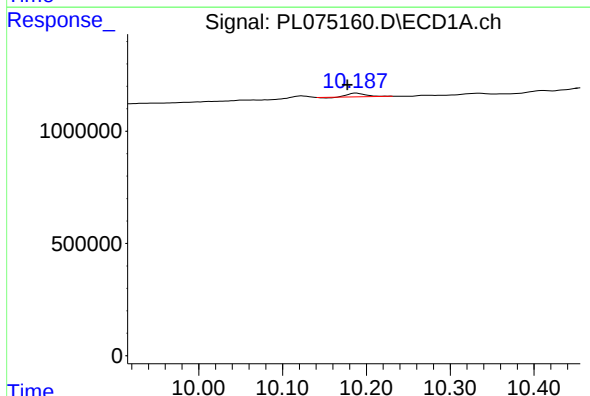


#21 Endrin ketone

R.T.: 10.188 min
Delta R.T.: 0.011 min
Response: 232080
Conc: 0.45 ng/ml

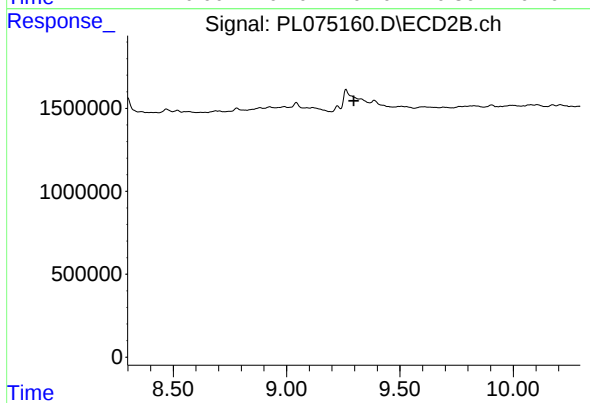

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.296 min
Response: 0
Conc: N.D.

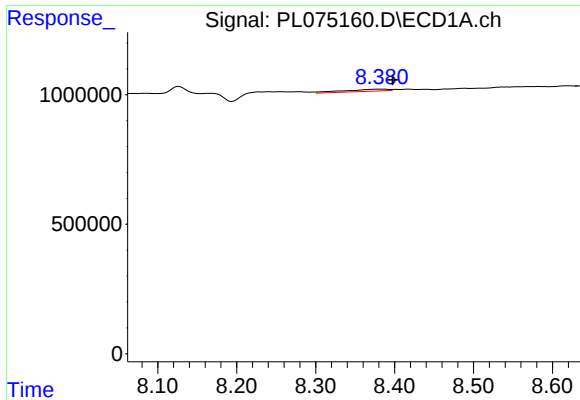

#25 Chlordane-3


R.T.: 8.380 min
Delta R.T.: -0.018 min
Response: 304831
Conc: 4.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

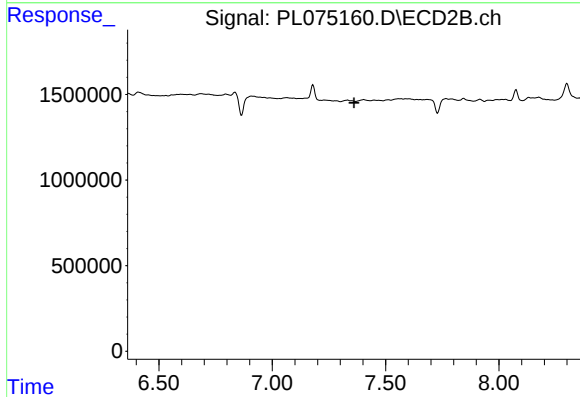


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.362 min
Response: 0
Conc: N.D.

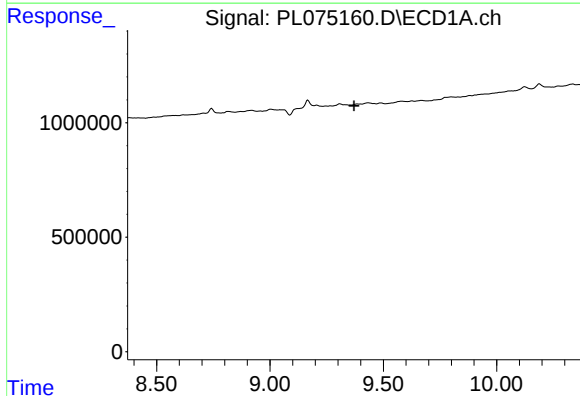


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.371 min
Response: 0
Conc: N.D.

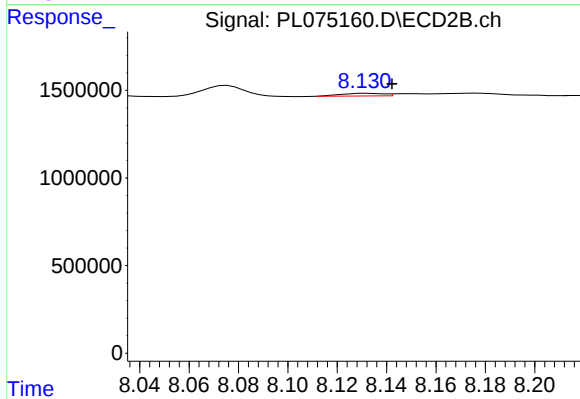

#27 Chlordane-5


R.T.: 8.132 min
Delta R.T.: -0.010 min
Response: 182515
Conc: 4.94 ng/ml

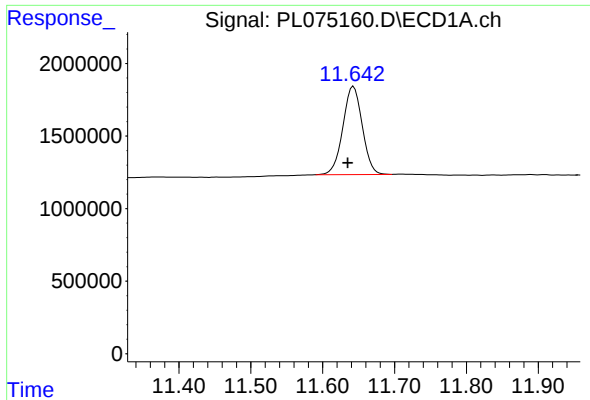

#28 Decachlorobiphenyl

R.T.: 11.643 min
Delta R.T.: 0.008 min
Response: 11358001
Conc: 25.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

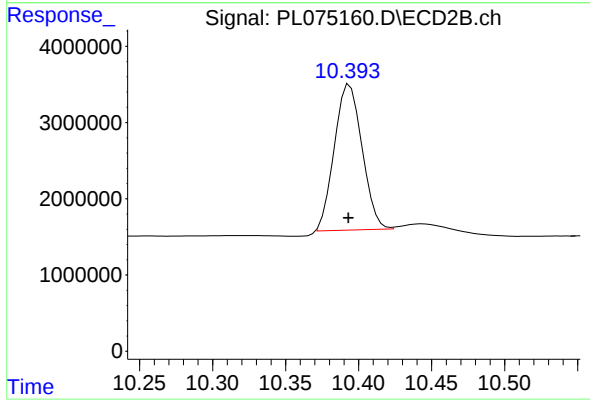

#28 Decachlorobiphenyl

R.T.: 10.394 min
Delta R.T.: 0.000 min
Response: 25240098
Conc: 24.59 ng/ml