

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052819\
 Data File : PL049033.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2019 16:04
 Operator : SM\AJ
 Sample : K3051-04DL 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SP-1-BDL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 29 01:40:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
 Quant Title : GC Extractables
 QLast Update : Thu May 02 09:36:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.330	3.938	19316685	5069726	1.994	2.035
28)	SA Decachlor...	8.001	8.980	24065665	6988665	2.394	2.633
Target Compounds							
10)	B gamma-Chl...	5.223	0.000	9407342	0	0.705	N.D. #
12)	B 4,4'-DDE	5.443	6.270	340.2E6	84540870	26.816	30.621
13)	MA Dieldrin	5.591f	0.000	8985220	0	0.690	N.D. #
14)	MA Endrin	5.825	0.000	88895706	0	7.302	N.D. #
16)	A 4,4'-DDD	5.954	6.760	27094344	9106567	2.783	4.058 #
17)	MA 4,4'-DDT	6.189	7.058	327.7E6	89326162	32.622	38.066
25)	Chlordane-3	5.223	0.000	9407342	0	5.975	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052819\
Data File : PL049033.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2019 16:04
Operator : SM\AJ
Sample : K3051-04DL 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
SP-1-BDL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 29 01:40:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL050119.M
Quant Title : GC Extractables
QLast Update : Thu May 02 09:36:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

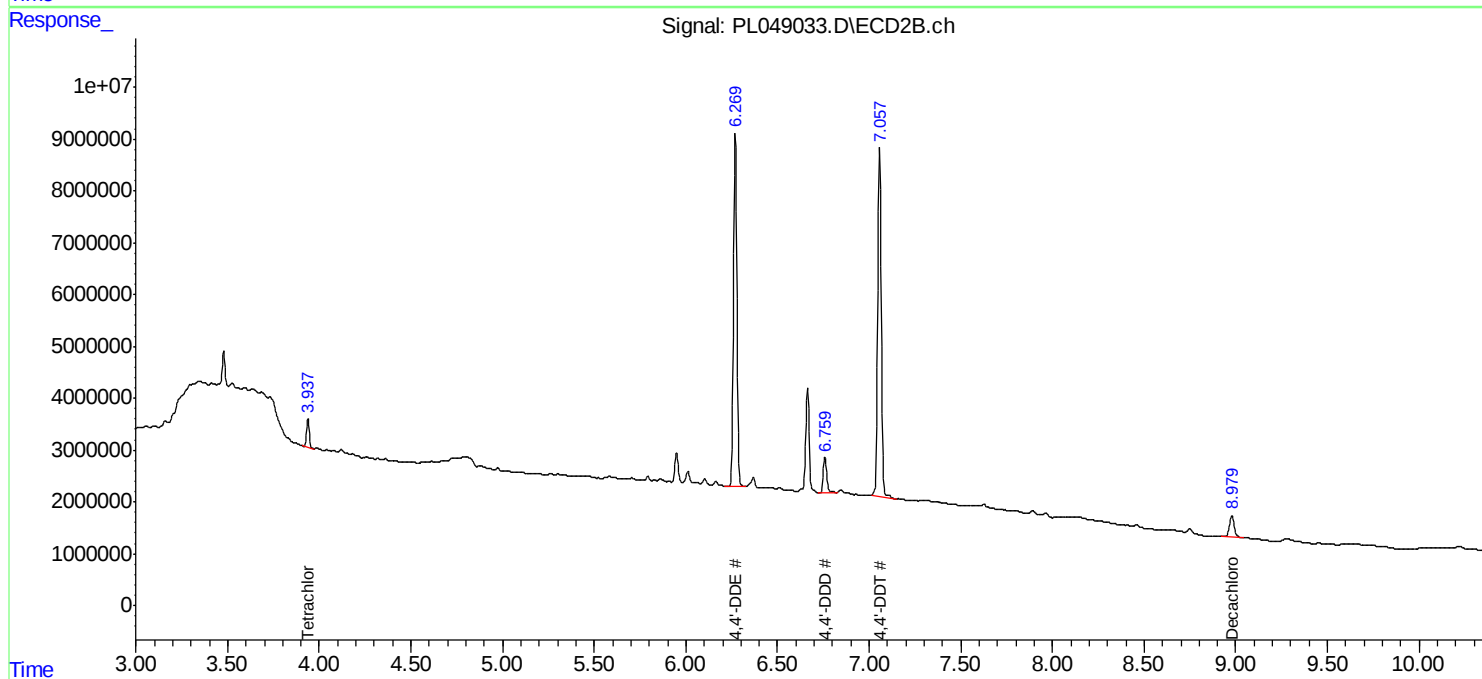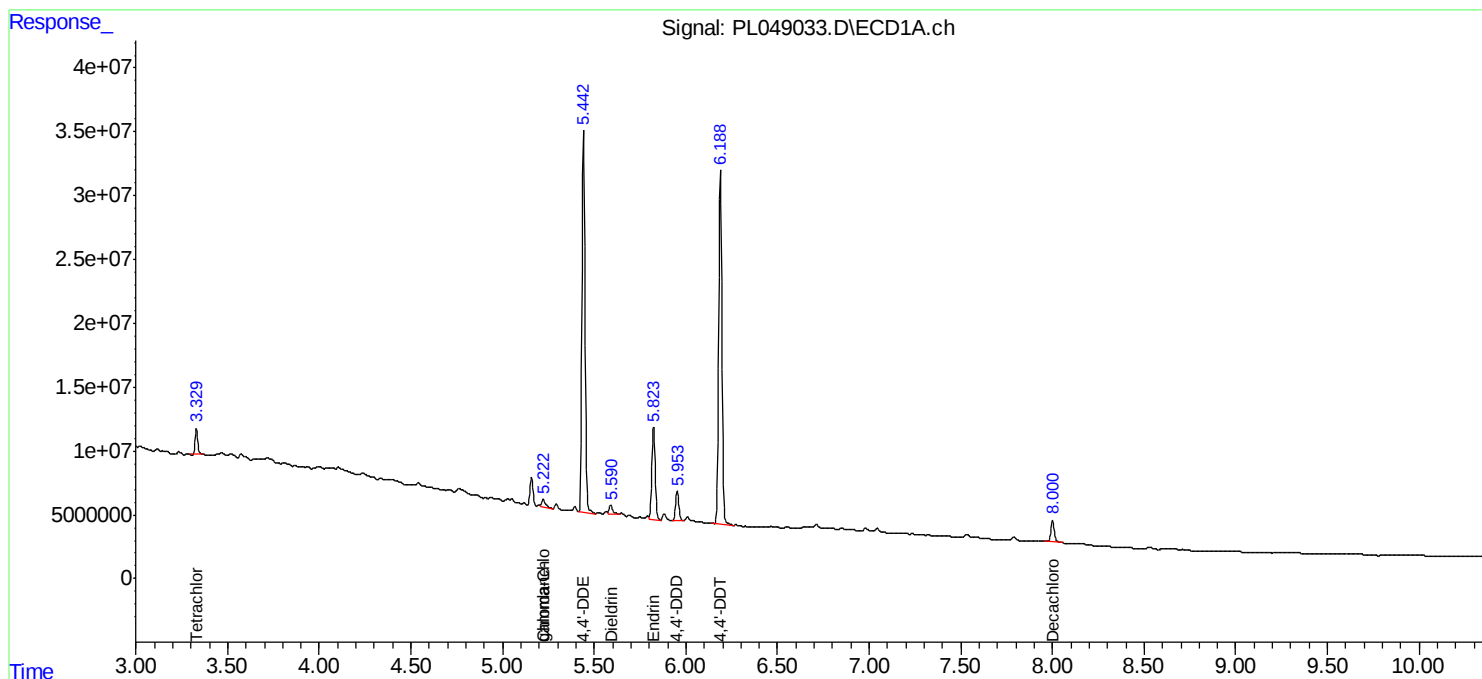


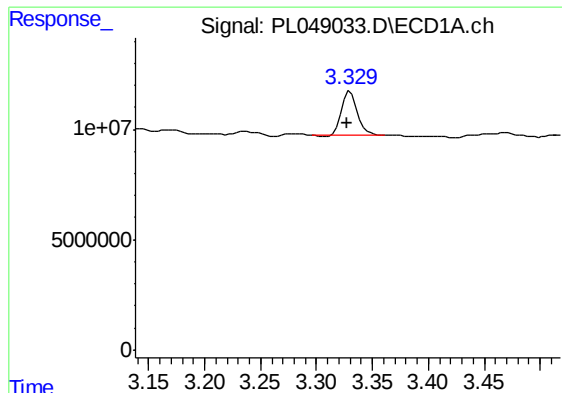

#1 Tetrachloro-m-xylene


R.T.: 3.330 min
Delta R.T.: 0.002 min
Response: 19316685
Conc: 1.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-1-BDL

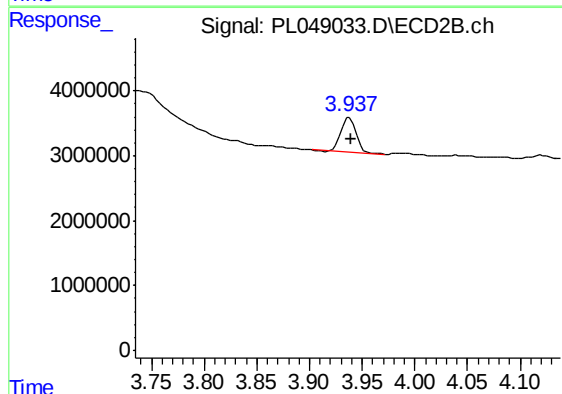


#1 Tetrachloro-m-xylene

R.T.: 3.938 min
Delta R.T.: -0.001 min
Response: 5069726
Conc: 2.04 ng/ml

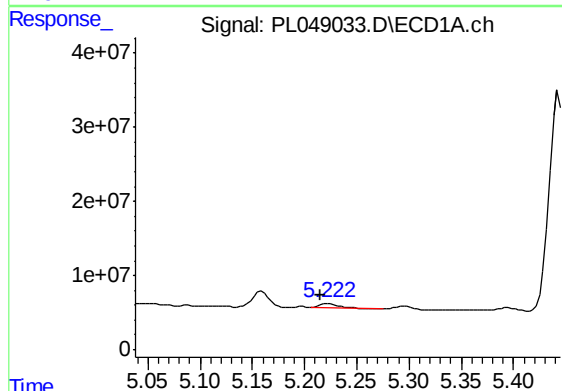


#10 gamma-Chlordane

R.T.: 5.223 min
Delta R.T.: 0.008 min
Response: 9407342
Conc: 0.70 ng/ml

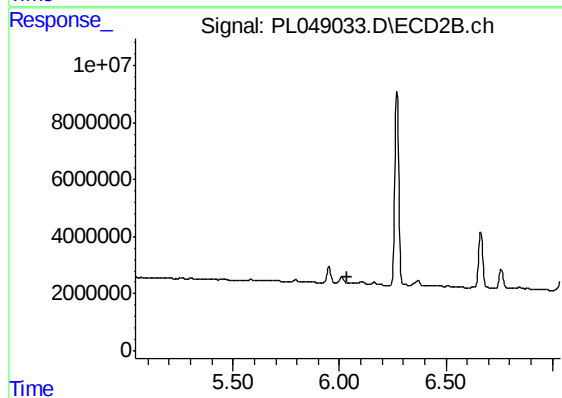

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.038 min
Response: 0
Conc: N.D.

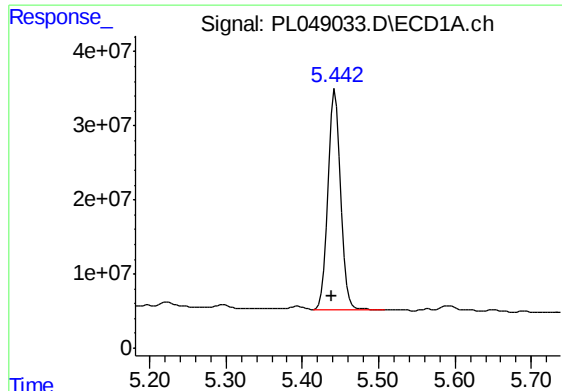

#12 4,4'-DDE


R.T.: 5.443 min
Delta R.T.: 0.004 min
Response: 340169192
Conc: 26.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-1-BDL

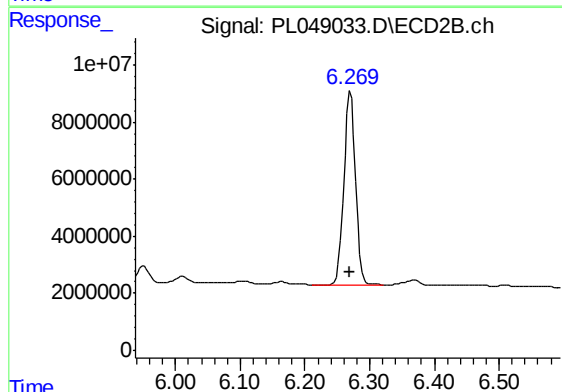


#12 4,4'-DDE

R.T.: 6.270 min
Delta R.T.: 0.000 min
Response: 84540870
Conc: 30.62 ng/ml

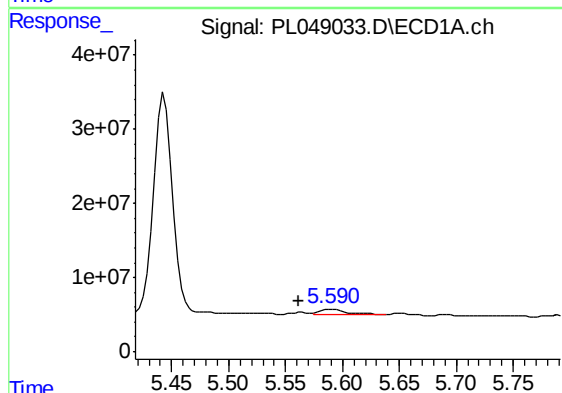


#13 Dieldrin

R.T.: 5.591 min
Delta R.T.: 0.029 min
Response: 8985220
Conc: 0.69 ng/ml

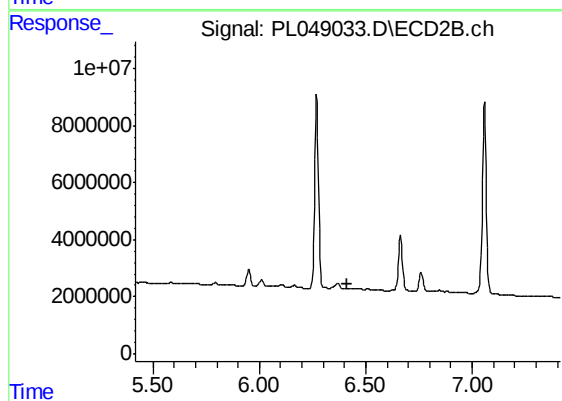

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

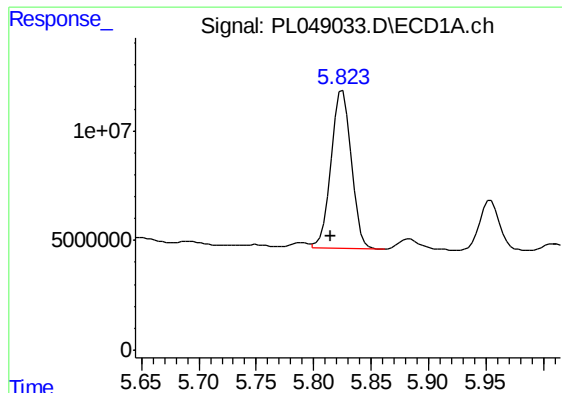

#14 Endrin


R.T.: 5.825 min
Delta R.T.: 0.010 min
Response: 88895706
Conc: 7.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-1-BDL

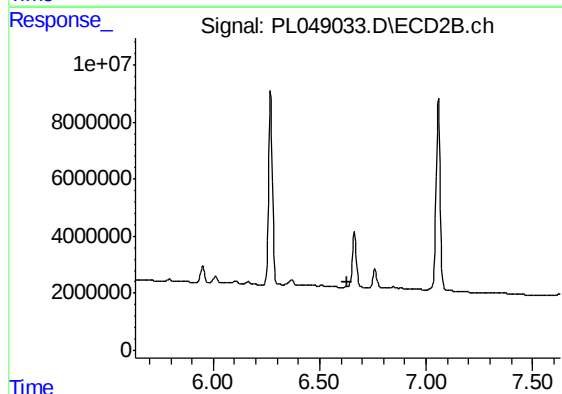


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.632 min
Response: 0
Conc: N.D.

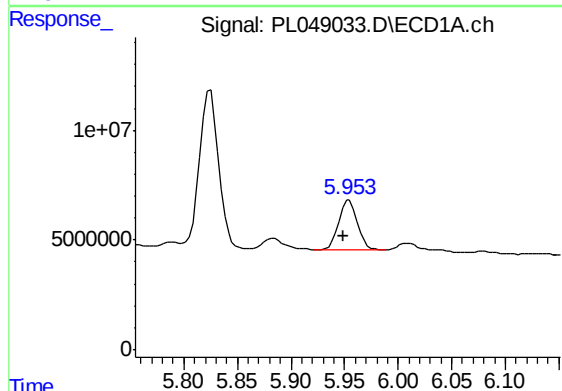


#16 4,4'-DDD

R.T.: 5.954 min
Delta R.T.: 0.005 min
Response: 27094344
Conc: 2.78 ng/ml

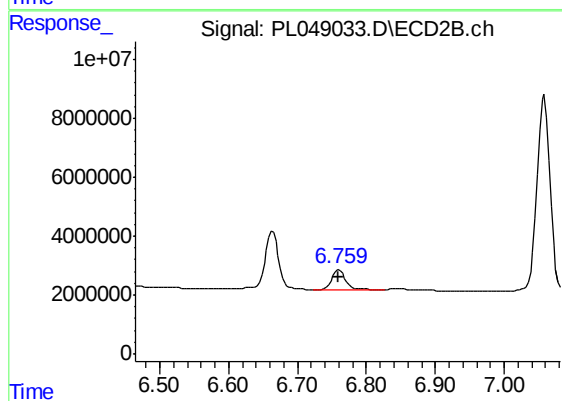

#16 4,4'-DDD


R.T.: 6.760 min
Delta R.T.: 0.000 min
Response: 9106567
Conc: 4.06 ng/ml

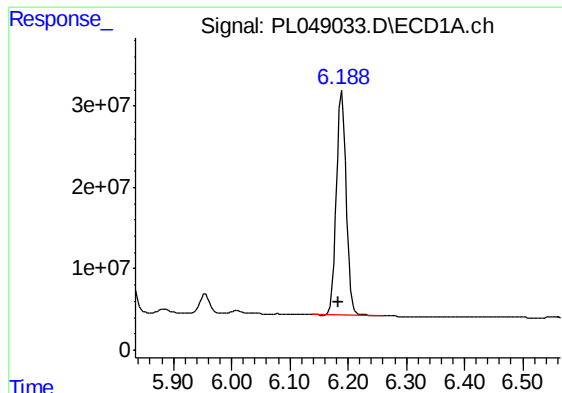

#17 4,4'-DDT


R.T.: 6.189 min
Delta R.T.: 0.006 min
Response: 327737297
Conc: 32.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-1-BDL

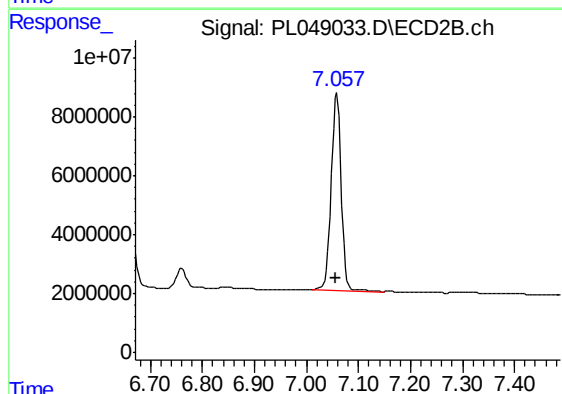


#17 4,4'-DDT

R.T.: 7.058 min
Delta R.T.: 0.002 min
Response: 89326162
Conc: 38.07 ng/ml

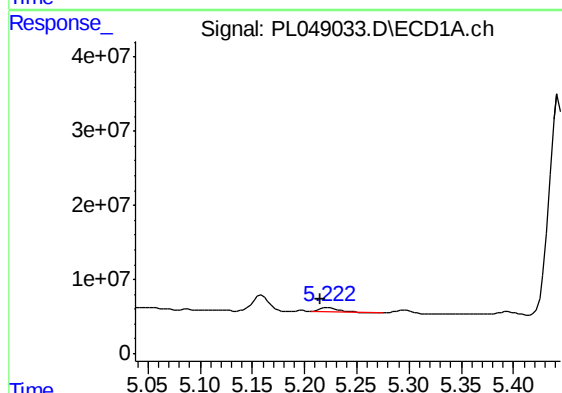


#25 Chlordane-3

R.T.: 5.223 min
Delta R.T.: 0.007 min
Response: 9407342
Conc: 5.97 ng/ml

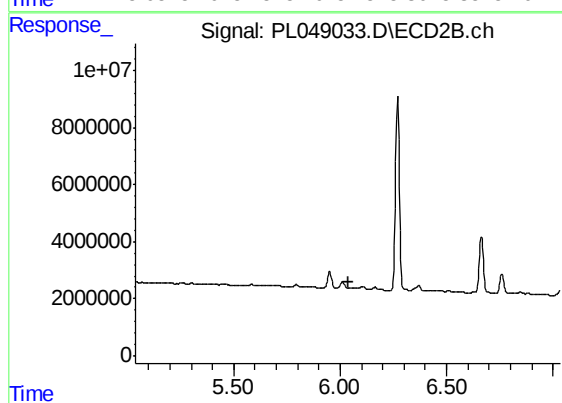

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.038 min
Response: 0
Conc: N.D.

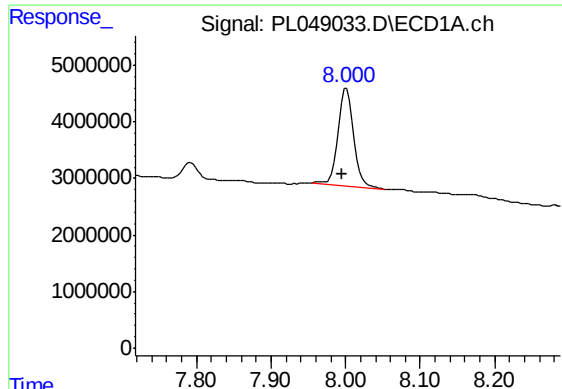

#28 Decachlorobiphenyl

R.T.: 8.001 min
Delta R.T.: 0.006 min
Response: 24065665
Conc: 2.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-1-BDL

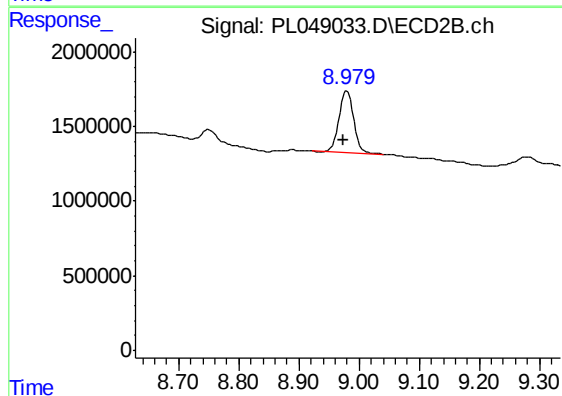

#28 Decachlorobiphenyl

R.T.: 8.980 min
Delta R.T.: 0.005 min
Response: 6988665
Conc: 2.63 ng/ml