

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052820\
 Data File : PL058954.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2020 15:51
 Operator : AJ\MA
 Sample : PB129147BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB129147BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 28 18:16:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
 Quant Title : GC Extractables
 QLast Update : Wed May 20 11:27:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.527	4.076	37306986	53734110	20.346	19.840
28)	SA Decachlor...	8.307	9.187	34600055	47935629	20.479	18.184
Target Compounds							
2)	A alpha-BHC	3.982	0.000	1811947	0	0.666	N.D. #
4)	MA Heptachlor	0.000	5.262	0	428545	N.D.	0.112 #
7)	B delta-BHC	0.000	5.116f	0	1648109	N.D.	0.452 #
8)	B Heptachlo...	0.000	5.955	0	9520558	N.D.	2.887 #
9)	A Endosulfan I	0.000	6.343f	0	210838	N.D.	0.072 #
14)	MA Endrin	6.100	0.000	1470419	0	0.938	N.D. #
15)	B Endosulfa...	0.000	7.009	0	1240929	N.D.	0.443 #
22)	Mirex	0.000	8.303f	0	499210	N.D.	0.228 #
23)	Chlordane-1	4.435f	5.055f	864092	1673769	16.515	17.451
26)	Chlordane-4	0.000	6.305f	0	2906911	N.D.	6.384 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052820\
Data File : PL058954.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2020 15:51
Operator : AJ\MA
Sample : PB129147BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB129147BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 18:16:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
Quant Title : GC Extractables
QLast Update : Wed May 20 11:27:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

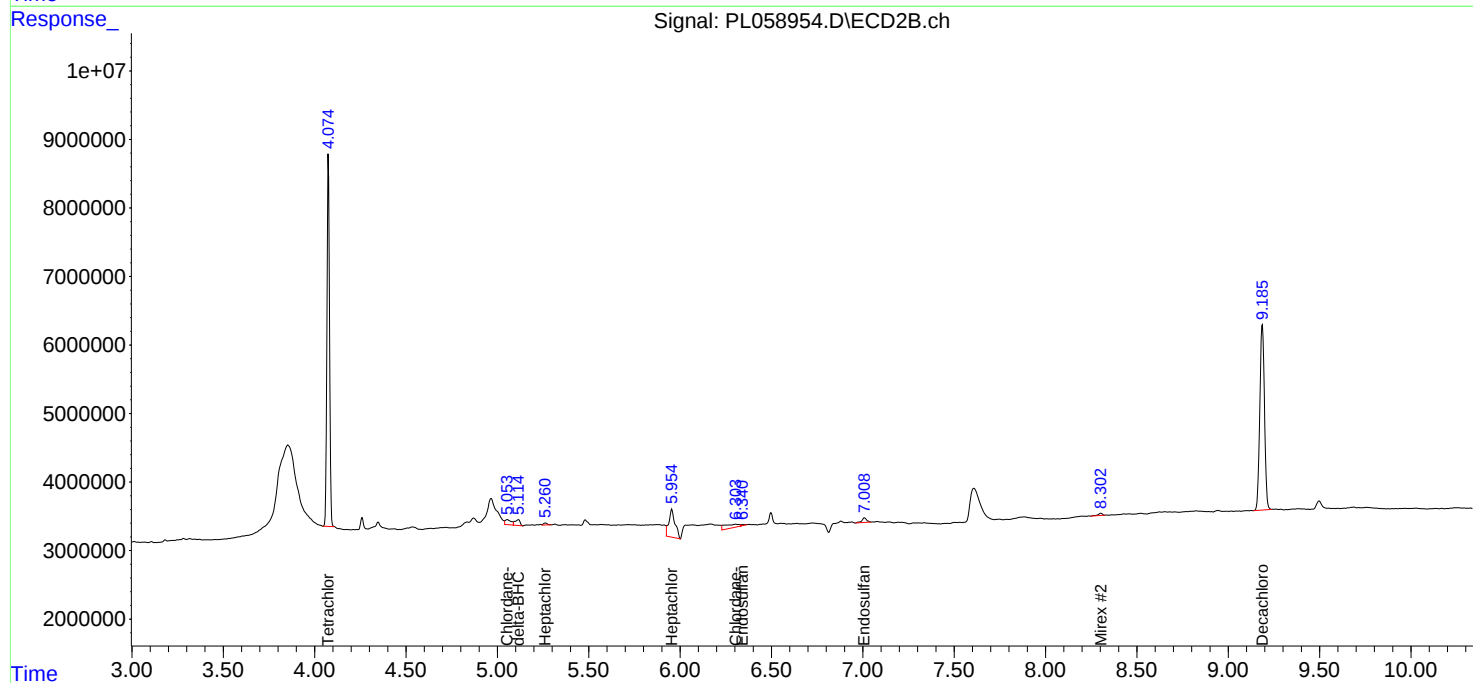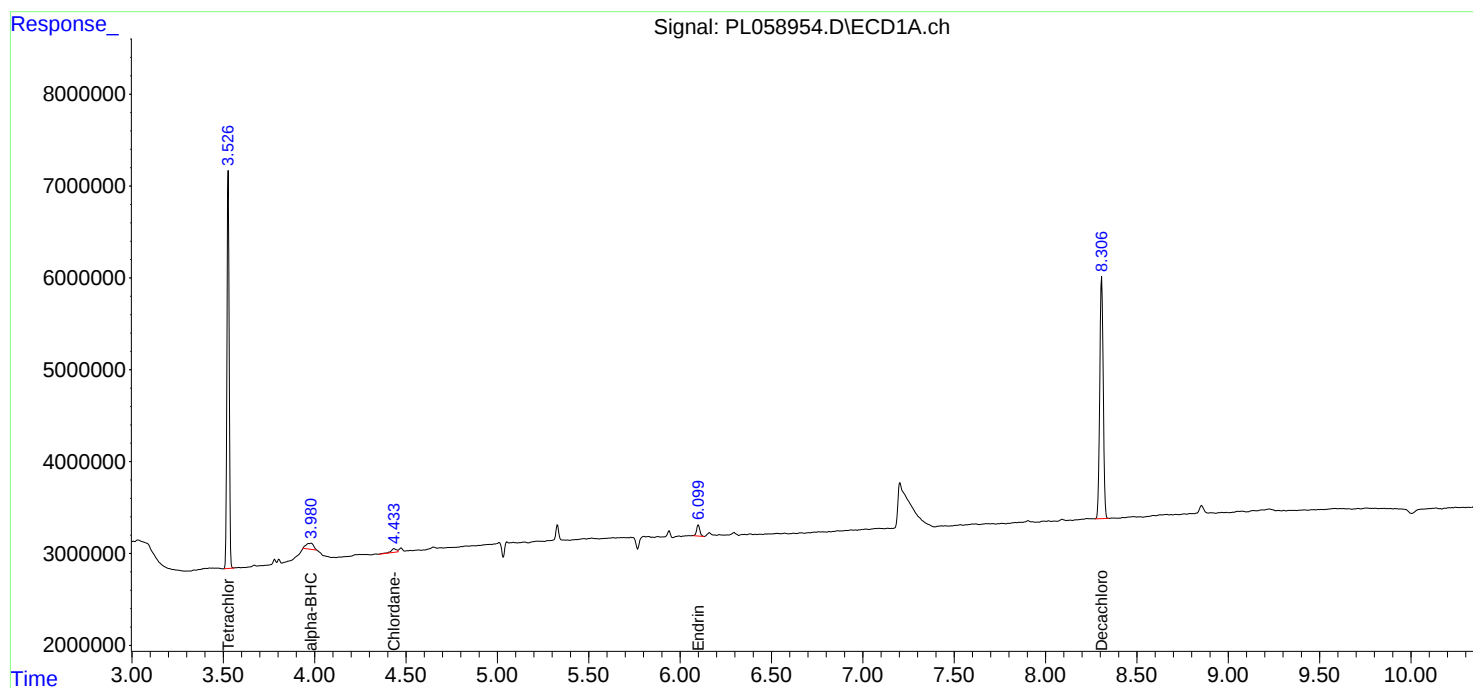


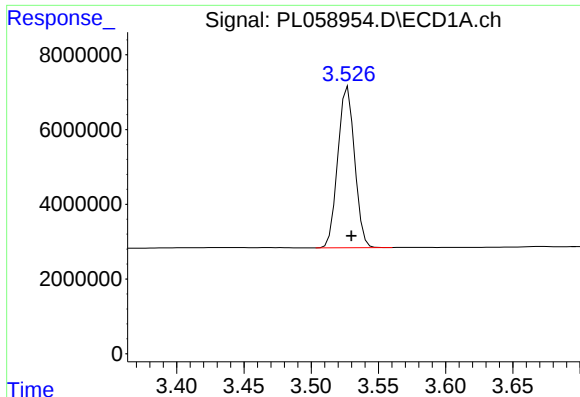

#1 Tetrachloro-m-xylene


R.T.: 3.527 min
Delta R.T.: -0.003 min
Response: 37306986
Conc: 20.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB129147BL

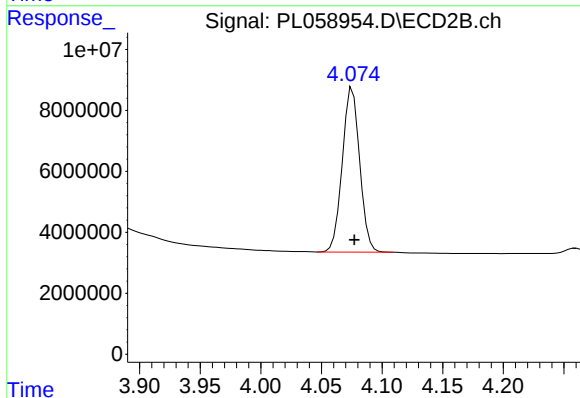


#1 Tetrachloro-m-xylene

R.T.: 4.076 min
Delta R.T.: -0.002 min
Response: 53734110
Conc: 19.84 ng/ml

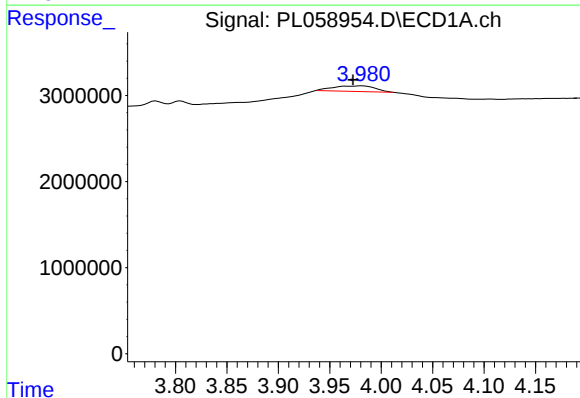


#2 alpha-BHC

R.T.: 3.982 min
Delta R.T.: 0.009 min
Response: 1811947
Conc: 0.67 ng/ml

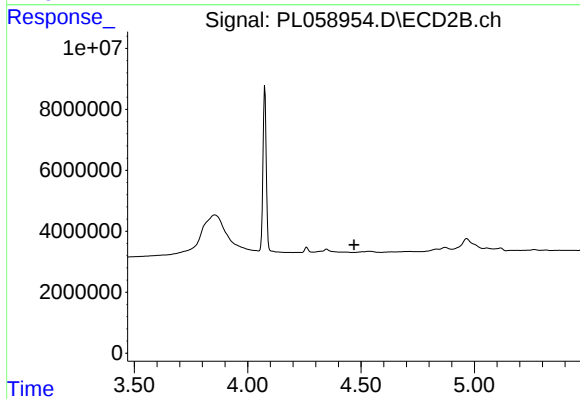

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.469 min
Response: 0
Conc: N.D.

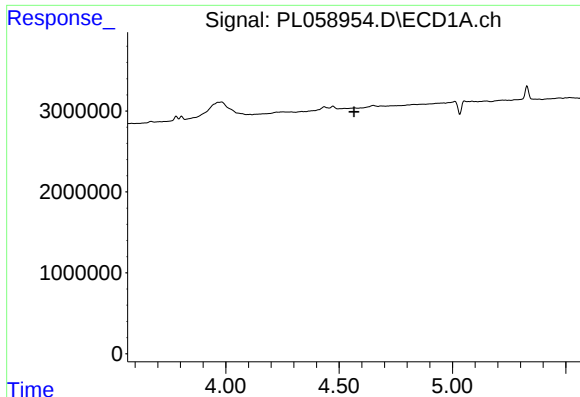

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.566 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB129147BL

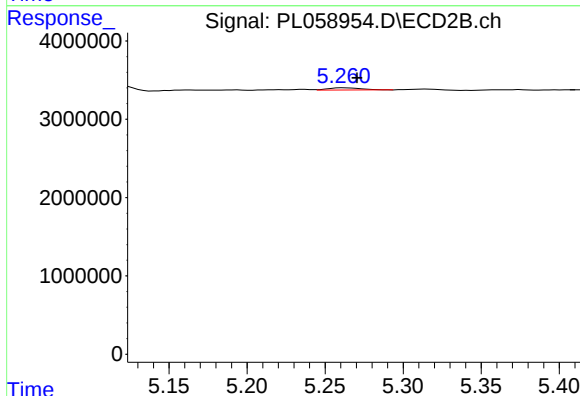


#4 Heptachlor

R.T.: 5.262 min
Delta R.T.: -0.008 min
Response: 428545
Conc: 0.11 ng/ml

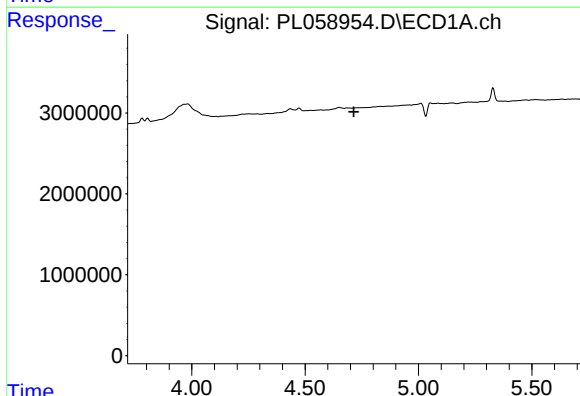


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.715 min
Response: 0
Conc: N.D.

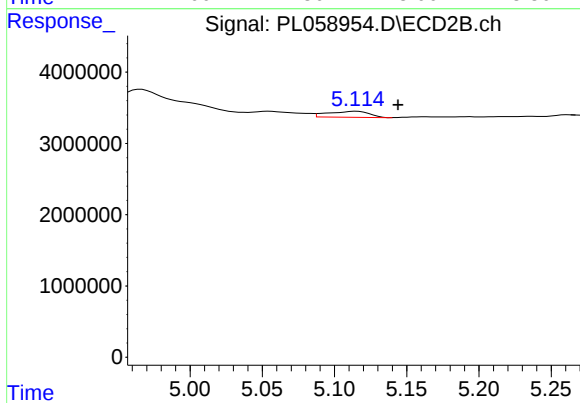

#7 delta-BHC


R.T.: 5.116 min
Delta R.T.: -0.028 min
Response: 1648109
Conc: 0.45 ng/ml

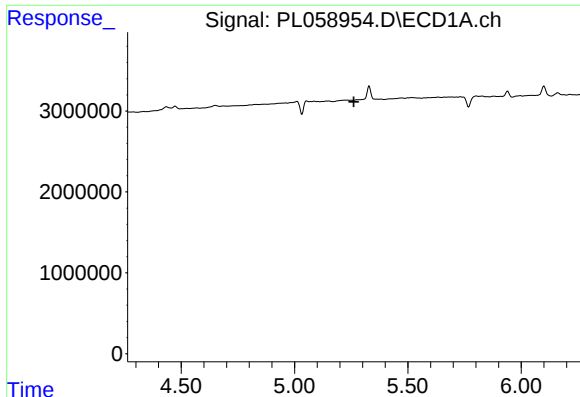

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.261 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB129147BL

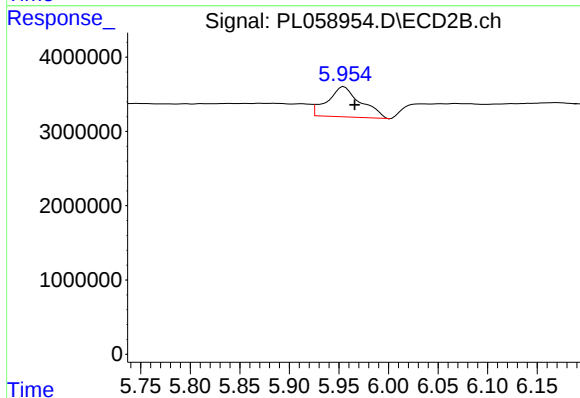


#8 Heptachlor epoxide

R.T.: 5.955 min
Delta R.T.: -0.011 min
Response: 9520558
Conc: 2.89 ng/ml

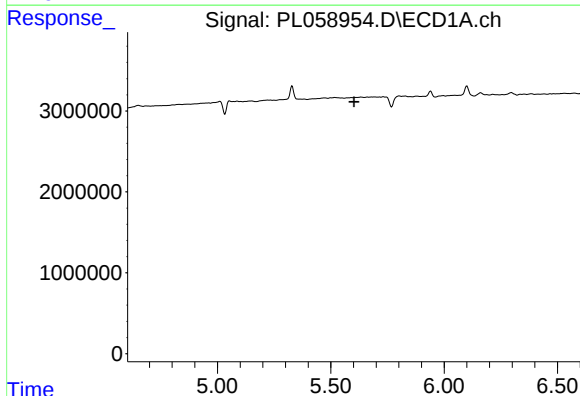


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.603 min
Response: 0
Conc: N.D.

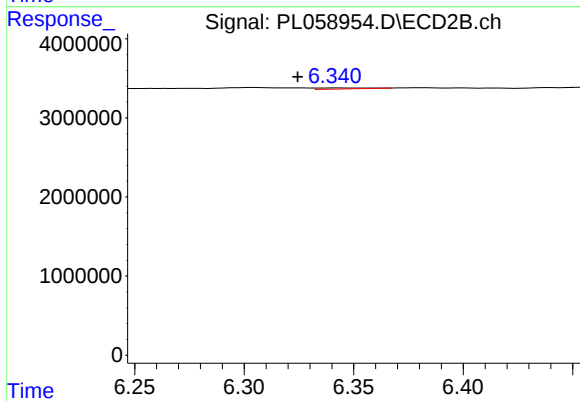

#9 Endosulfan I


R.T.: 6.343 min
Delta R.T.: 0.018 min
Response: 210838
Conc: 0.07 ng/ml

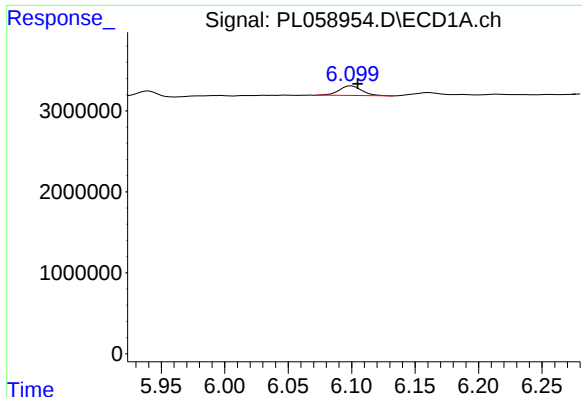

#14 Endrin


R.T.: 6.100 min
Delta R.T.: -0.005 min
Response: 1470419
Conc: 0.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB129147BL

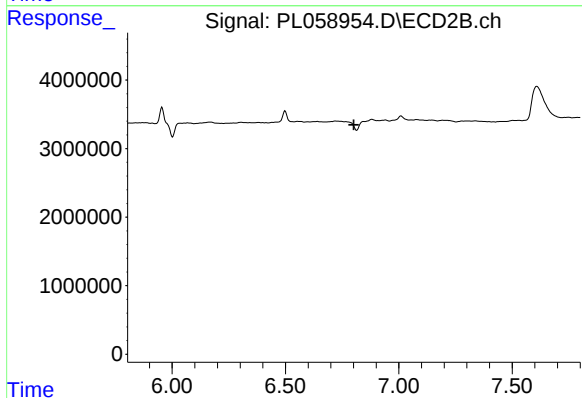


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.802 min
Response: 0
Conc: N.D.

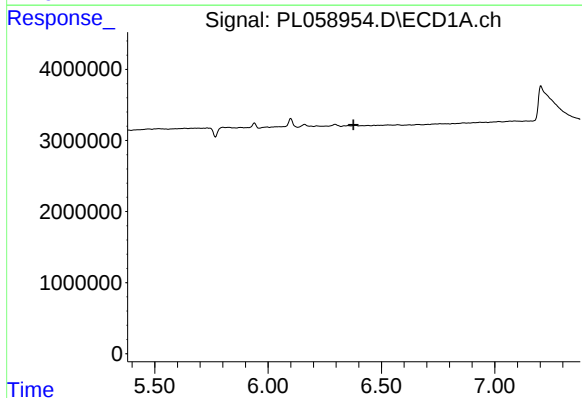


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.377 min
Response: 0
Conc: N.D.

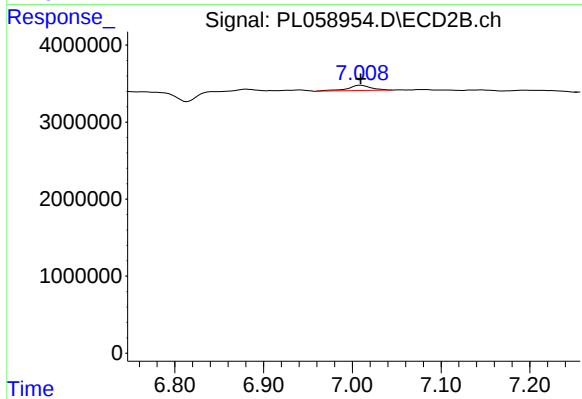

#15 Endosulfan II


R.T.: 7.009 min
Delta R.T.: 0.000 min
Response: 1240929
Conc: 0.44 ng/ml

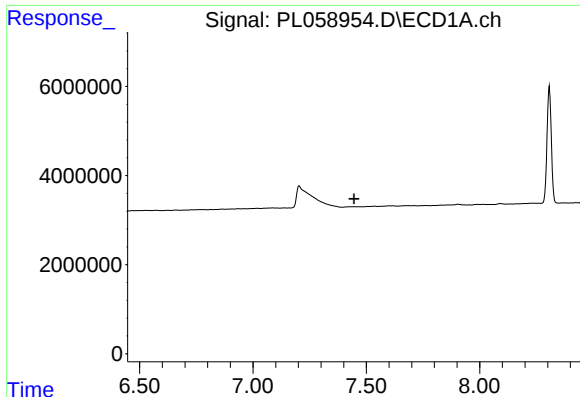

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.446 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB129147BL

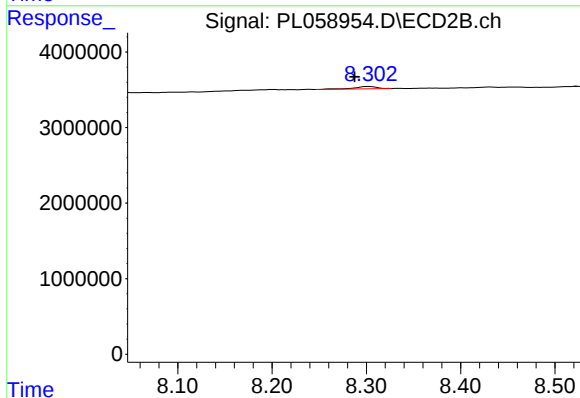


#22 Mirex

R.T.: 8.303 min
Delta R.T.: 0.015 min
Response: 499210
Conc: 0.23 ng/ml

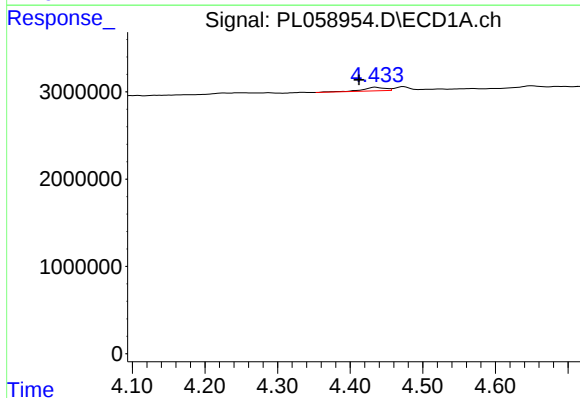


#23 Chlordane-1

R.T.: 4.435 min
Delta R.T.: 0.023 min
Response: 864092
Conc: 16.51 ng/ml

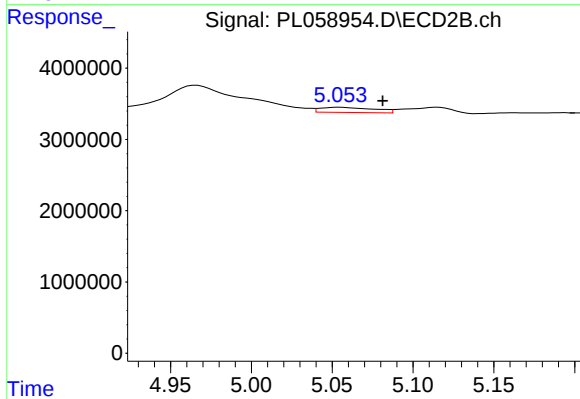

#23 Chlordane-1


R.T.: 5.055 min
Delta R.T.: -0.026 min
Response: 1673769
Conc: 17.45 ng/ml

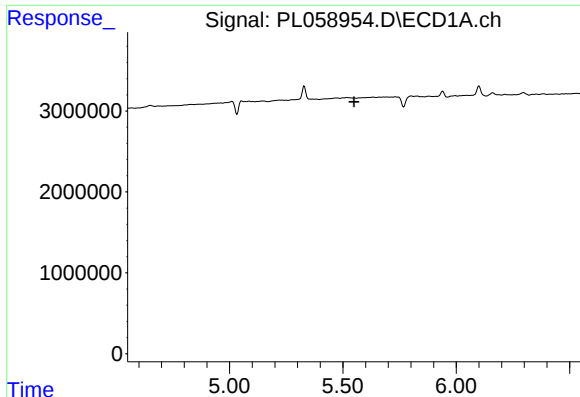

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.549 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB129147BL

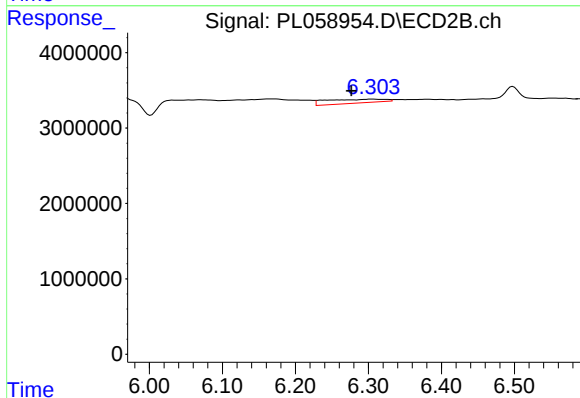


#26 Chlordane-4

R.T.: 6.305 min
Delta R.T.: 0.029 min
Response: 2906911
Conc: 6.38 ng/ml

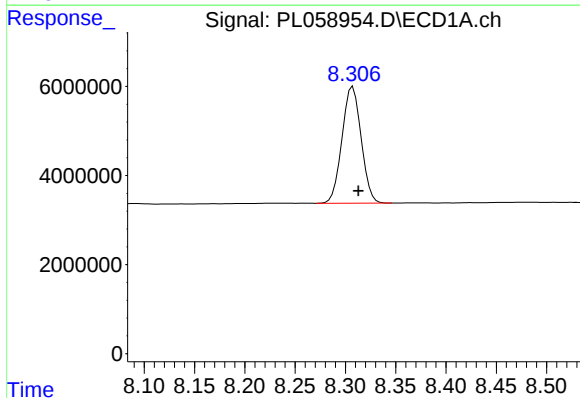

#28 Decachlorobiphenyl

R.T.: 8.307 min
Delta R.T.: -0.006 min
Response: 34600055
Conc: 20.48 ng/ml

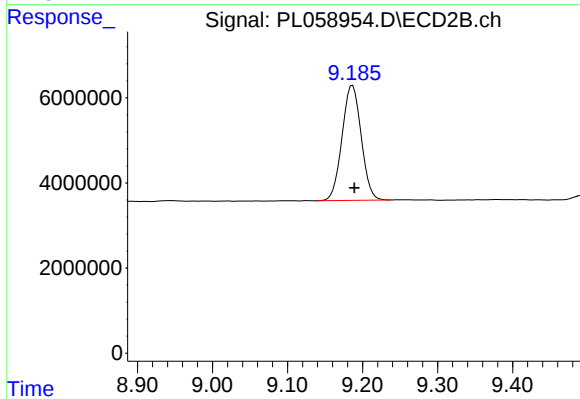

#28 Decachlorobiphenyl

R.T.: 9.187 min
Delta R.T.: -0.002 min
Response: 47935629
Conc: 18.18 ng/ml