

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052820\
 Data File : PL058951.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2020 15:09
 Operator : AJ\MA
 Sample : L2773-14
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NM25-COMP-2020-0-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 29 17:58:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
 Quant Title : GC Extractables
 QLast Update : Wed May 20 11:27:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.528	4.075	23162876	32890212	12.632	12.144
28)	SA Decachlor...	8.307	9.186	18131478	24520694	10.731	9.302
Target Compounds							
11)	B alpha-Chl...	5.545	6.276	2864188	18458852	1.565	5.683 #
12)	B 4,4'-DDE	5.708	6.427	2522459	5557928	1.536	1.947 #
17)	MA 4,4'-DDT	6.465	7.218	4016235	2250720	2.761	0.946 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052820\
Data File : PL058951.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2020 15:09
Operator : AJ\MA
Sample : L2773-14
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
NM25-COMP-2020-0-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 29 17:58:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
Quant Title : GC Extractables
QLast Update : Wed May 20 11:27:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

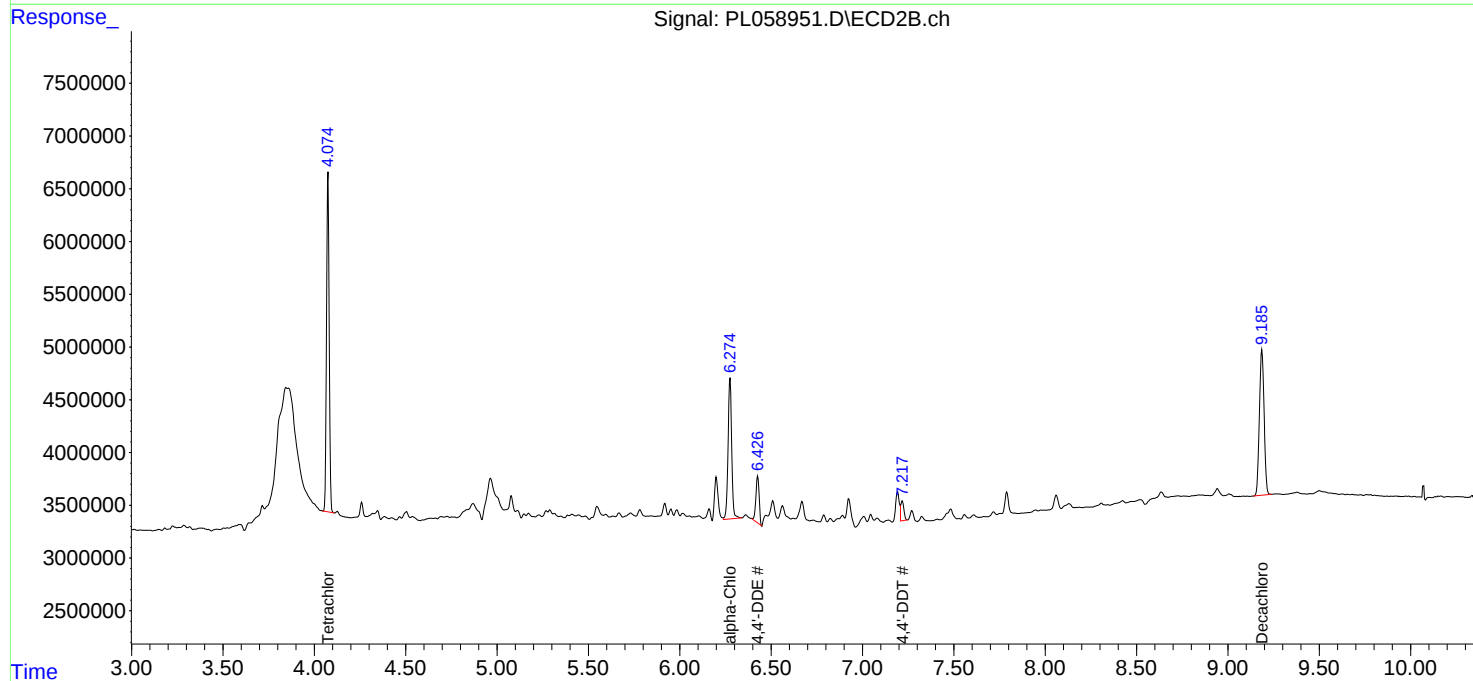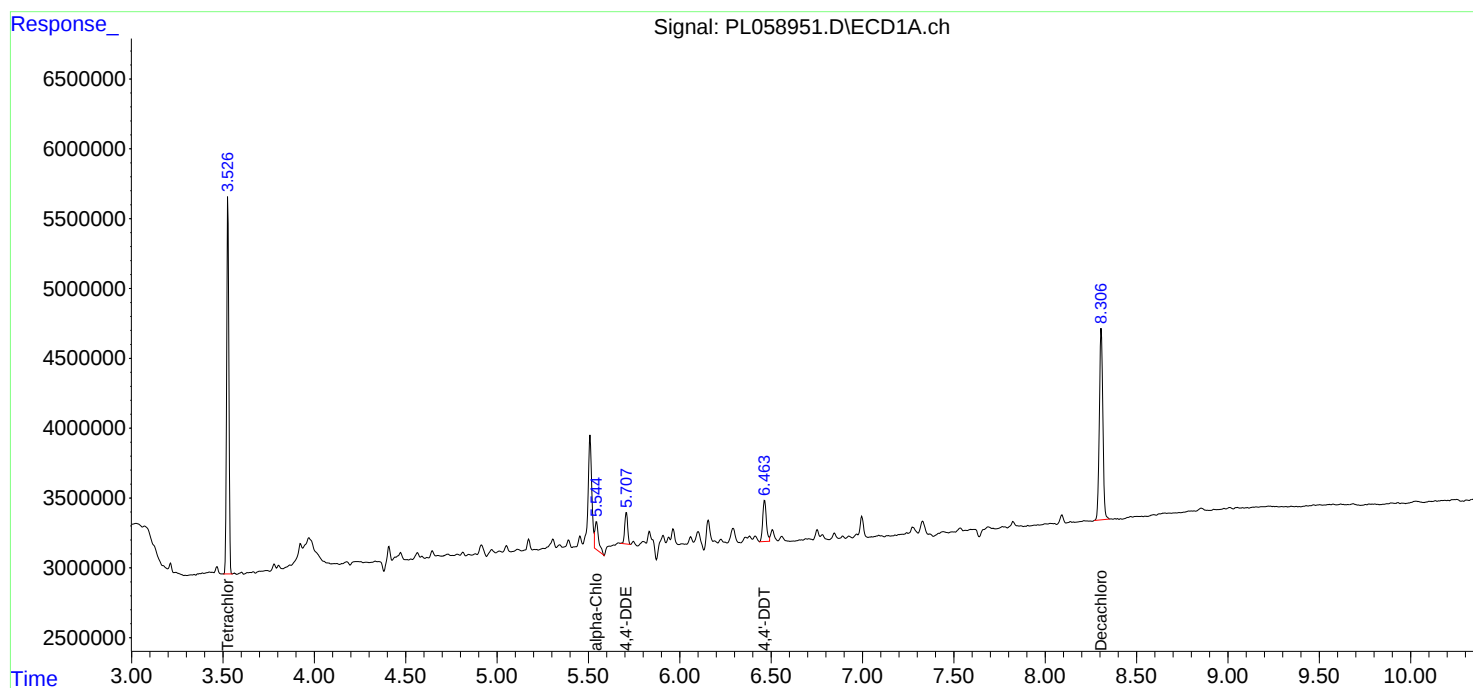


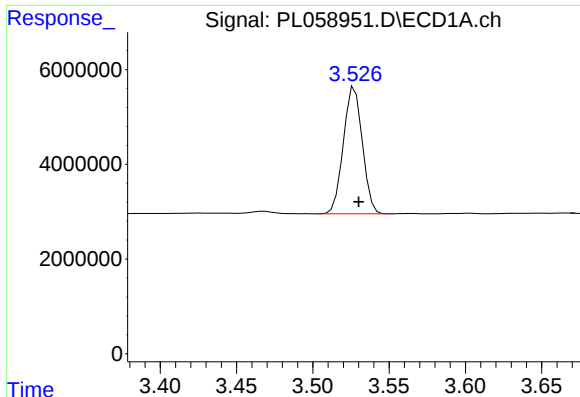

#1 Tetrachloro-m-xylene


R.T.: 3.528 min
Delta R.T.: -0.002 min
Response: 23162876
Conc: 12.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
NM25-COMP-2020-0-6

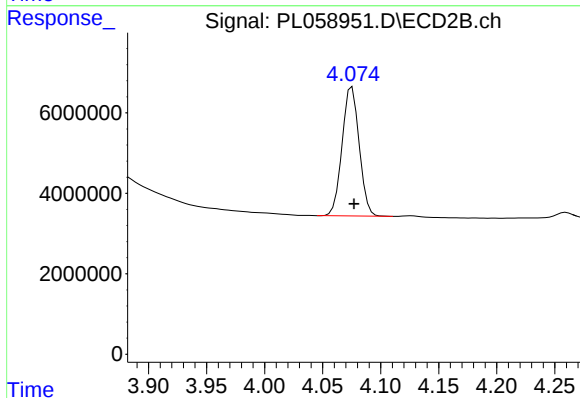


#1 Tetrachloro-m-xylene

R.T.: 4.075 min
Delta R.T.: -0.002 min
Response: 32890212
Conc: 12.14 ng/ml

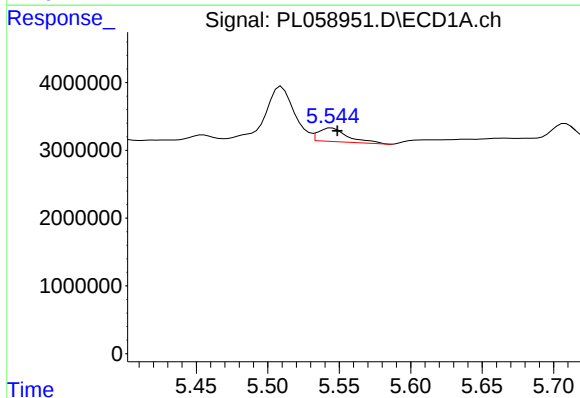


#11 alpha-Chlordane

R.T.: 5.545 min
Delta R.T.: -0.004 min
Response: 2864188
Conc: 1.57 ng/ml

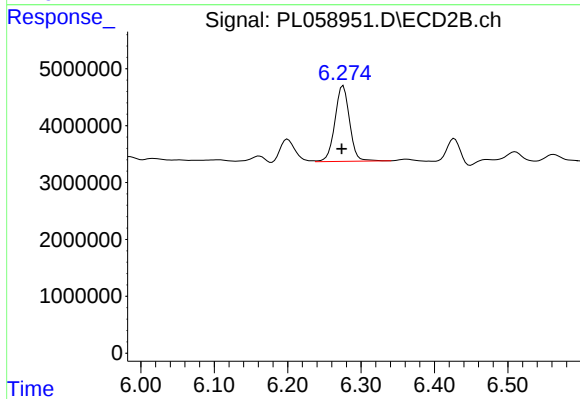

#11 alpha-Chlordane


R.T.: 6.276 min
Delta R.T.: 0.002 min
Response: 18458852
Conc: 5.68 ng/ml

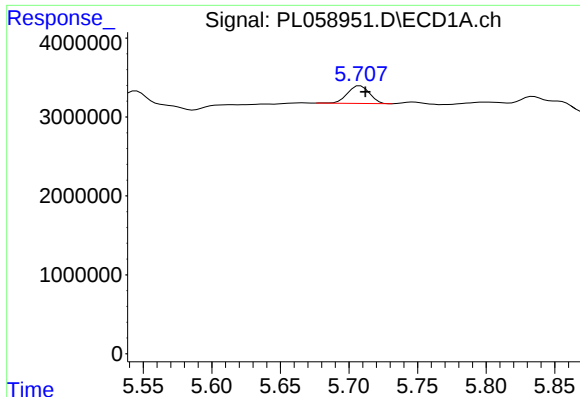

#12 4,4'-DDE


R.T.: 5.708 min
Delta R.T.: -0.004 min
Response: 2522459
Conc: 1.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
NM25-COMP-2020-0-6

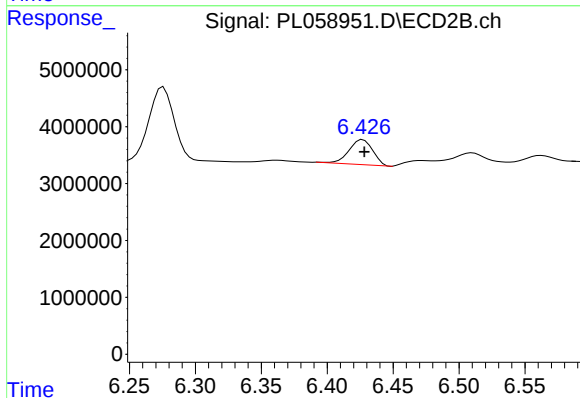


#12 4,4'-DDE

R.T.: 6.427 min
Delta R.T.: 0.000 min
Response: 5557928
Conc: 1.95 ng/ml

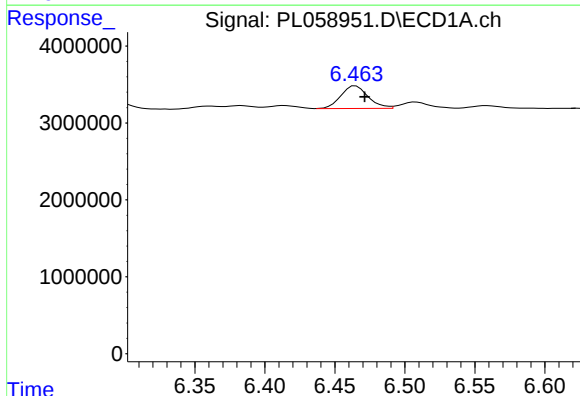


#17 4,4'-DDT

R.T.: 6.465 min
Delta R.T.: -0.006 min
Response: 4016235
Conc: 2.76 ng/ml

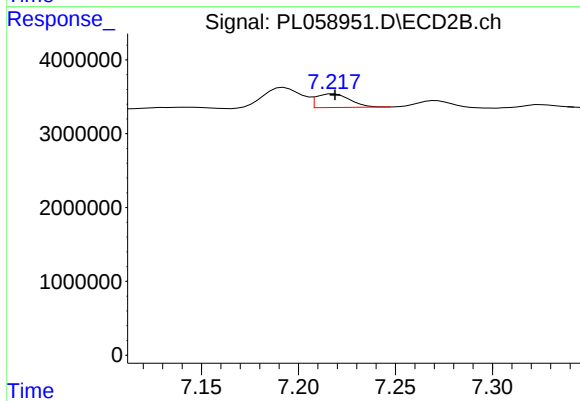

#17 4,4'-DDT


R.T.: 7.218 min
Delta R.T.: 0.000 min
Response: 2250720
Conc: 0.95 ng/ml

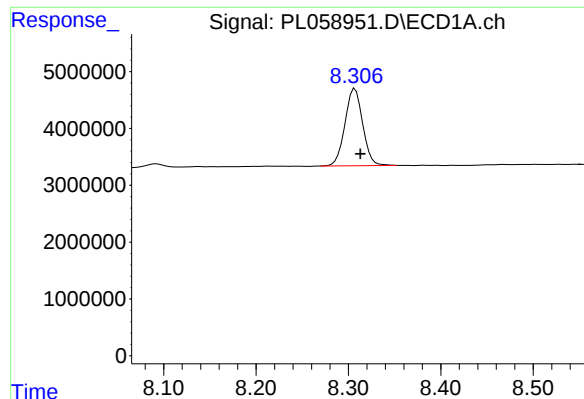

#28 Decachlorobiphenyl

R.T.: 8.307 min
Delta R.T.: -0.006 min
Response: 18131478
Conc: 10.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
NM25-COMP-2020-0-6

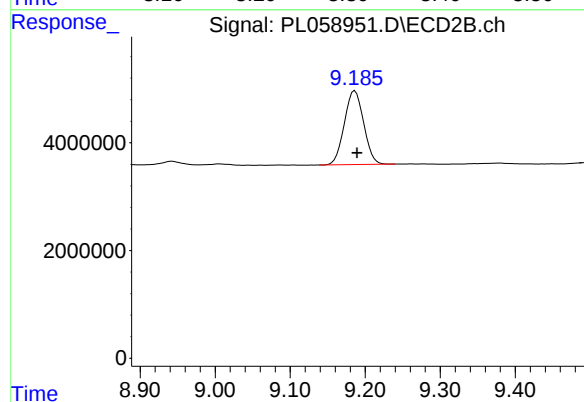

#28 Decachlorobiphenyl

R.T.: 9.186 min
Delta R.T.: -0.003 min
Response: 24520694
Conc: 9.30 ng/ml