

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052820\
 Data File : PL058971.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2020 20:21
 Operator : AJ\MA
 Sample : L2773-19
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NM58-COMP-2020-0-6

Manual Integrations
 APPROVED

mohammad
 6/1/2020 1:26:07 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 29 01:25:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
 Quant Title : GC Extractables
 QLast Update : Wed May 20 11:27:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.528	4.077	20256665	29615951	11.047	10.935
28) SA Decachlor...	8.308	9.188	9350948	13271927	5.535	5.034
Target Compounds						
11) B alpha-Chl...	5.544	6.276	1992957	15516698	1.089m	4.777 #
12) B 4,4'-DDE	5.709	6.428	1099322	3067323	0.669	1.075 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052820\
Data File : PL058971.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2020 20:21
Operator : AJ\MA
Sample : L2773-19
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
NM58-COMP-2020-0-6


Manual Integrations
APPROVED

mohammad
6/1/2020 1:26:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 29 01:25:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052020.M
Quant Title : GC Extractables
QLast Update : Wed May 20 11:27:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

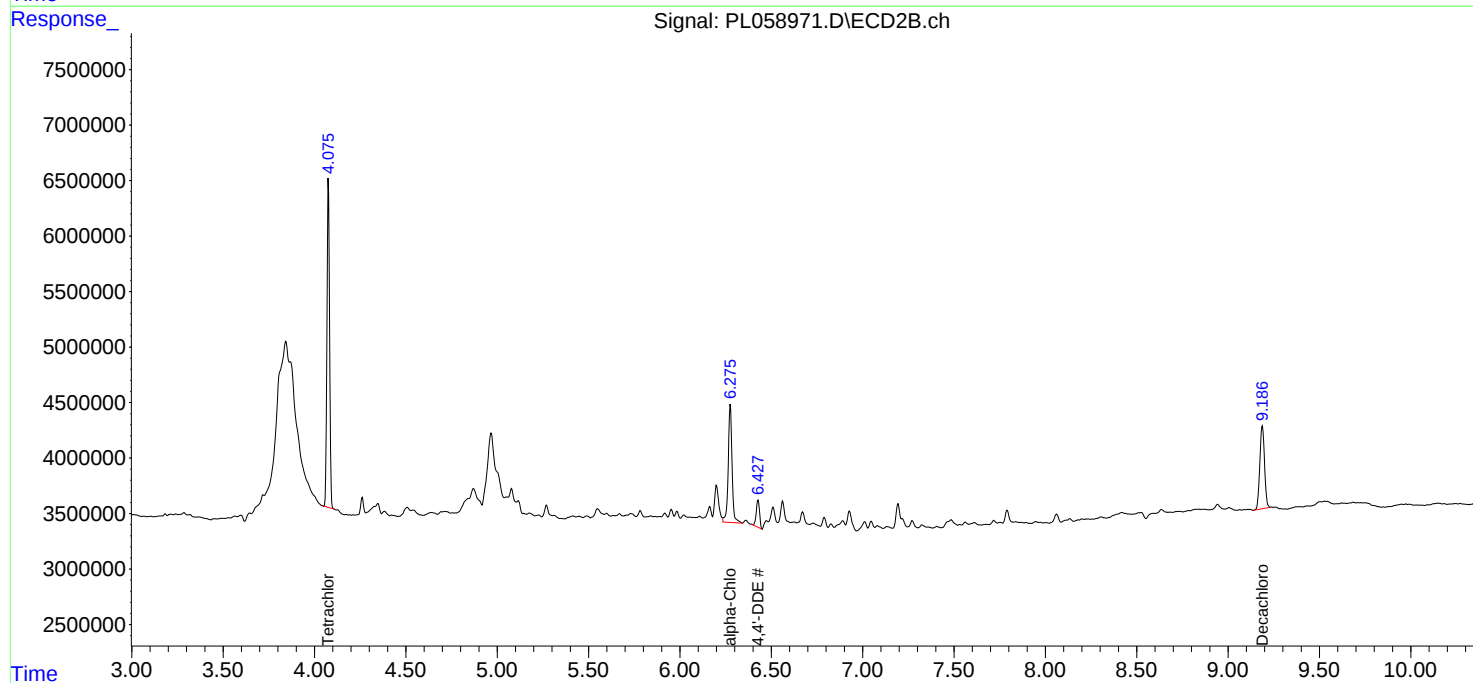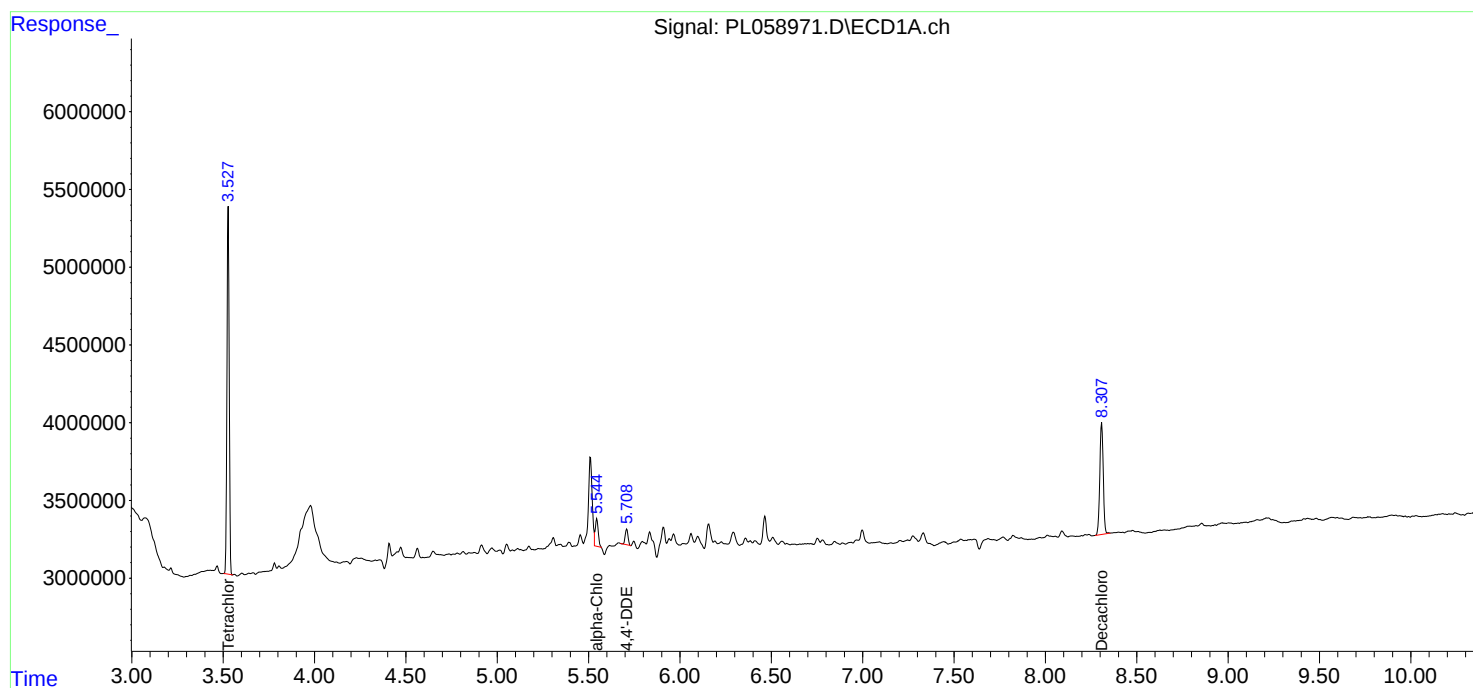

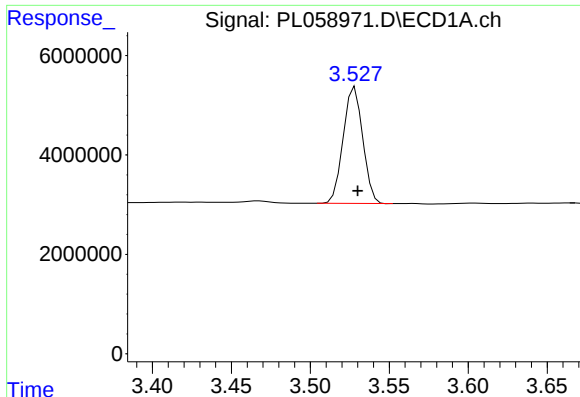


#1 Tetrachloro-m-xylene

R.T.: 3.528 min
Delta R.T.: -0.002 min
Response: 20256665
Conc: 11.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
NM58-COMP-2020-0-6


Manual Integrations
APPROVED

mohammad
6/1/2020 1:26:07 PM

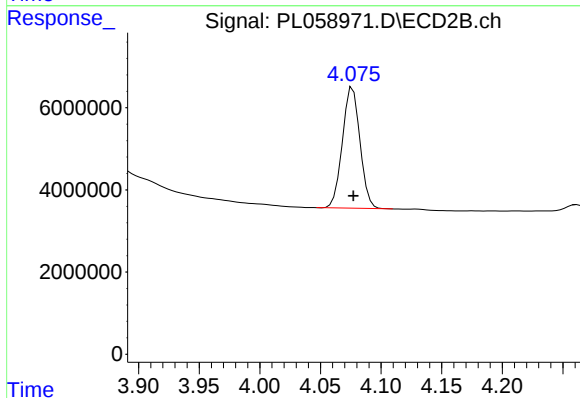


#1 Tetrachloro-m-xylene

R.T.: 4.077 min
Delta R.T.: 0.000 min
Response: 29615951
Conc: 10.93 ng/ml

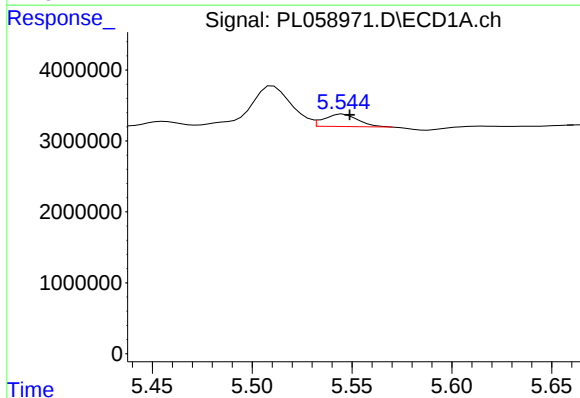


#11 alpha-Chlordane

R.T.: 5.544 min
Delta R.T.: -0.005 min
Response: 1992957
Conc: 1.09 ng/ml m

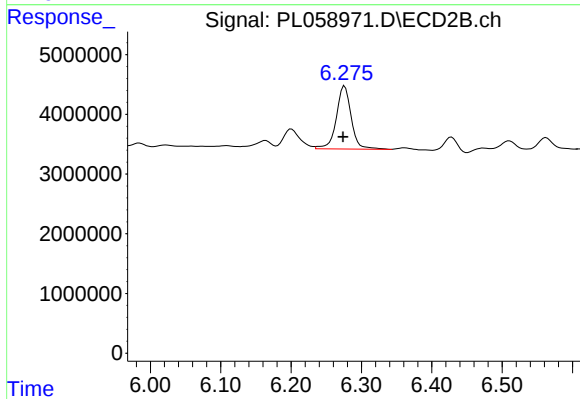

#11 alpha-Chlordane

R.T.: 6.276 min
Delta R.T.: 0.002 min
Response: 15516698
Conc: 4.78 ng/ml

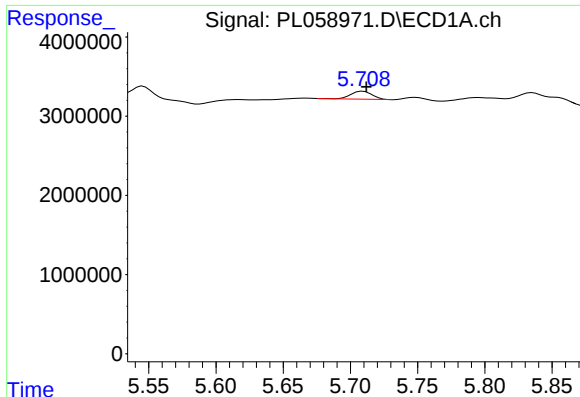


#12 4,4'-DDE

R.T.: 5.709 min
Delta R.T.: -0.003 min
Response: 1099322
Conc: 0.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
NM58-COMP-2020-0-6


Manual Integrations
APPROVED

mohammad
6/1/2020 1:26:07 PM

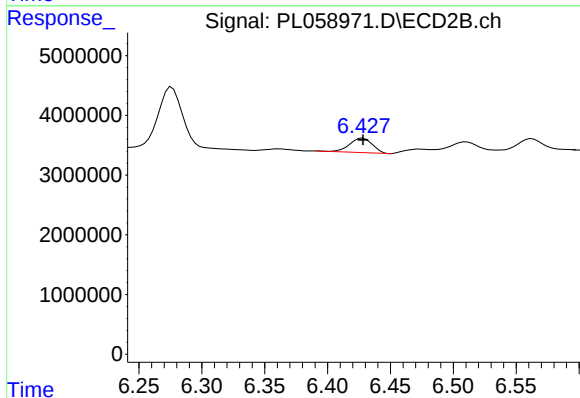


#12 4,4'-DDE

R.T.: 6.428 min
Delta R.T.: 0.000 min
Response: 3067323
Conc: 1.07 ng/ml

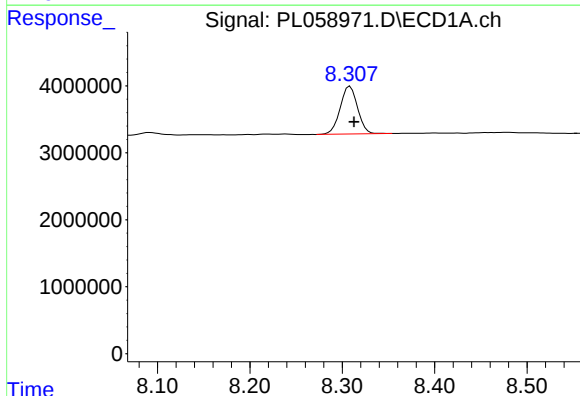

#28 Decachlorobiphenyl

R.T.: 8.308 min
Delta R.T.: -0.004 min
Response: 9350948
Conc: 5.53 ng/ml

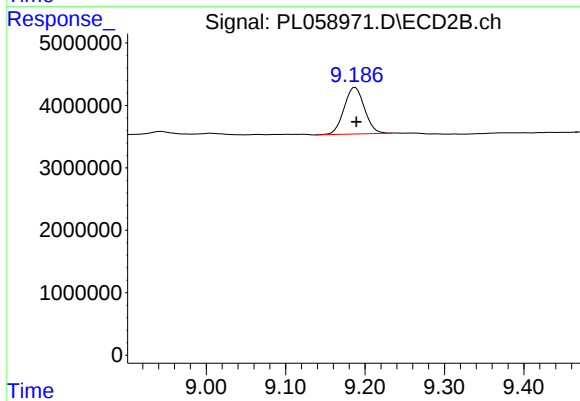

#28 Decachlorobiphenyl

R.T.: 9.188 min
Delta R.T.: -0.001 min
Response: 13271927
Conc: 5.03 ng/ml