

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052821\
 Data File : PL066923.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 May 2021 09:05
 Operator : AR\AJ
 Sample : PIBLK65
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 28 05:33:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052721CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 27 02:30:58 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.484	5.532	10874622	17547166	20.377	19.844
2)	SA Decachlor...	10.229	11.434	26172891	34608976	39.032	37.908
Target Compounds							
13)	MA Dieldrin	7.652f	0.000	783779	0	1.155	N.D. #
15)	B Endosulfa...	8.135f	0.000	3920577	0	6.529	N.D. #
16)	A 4,4'-DDD	0.000	9.033f	0	5095026	N.D.	6.876


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052821\
Data File : PL066923.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 May 2021 09:05
Operator : AR\AJ
Sample : PIBLK65
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 05:33:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052721CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 27 02:30:58 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

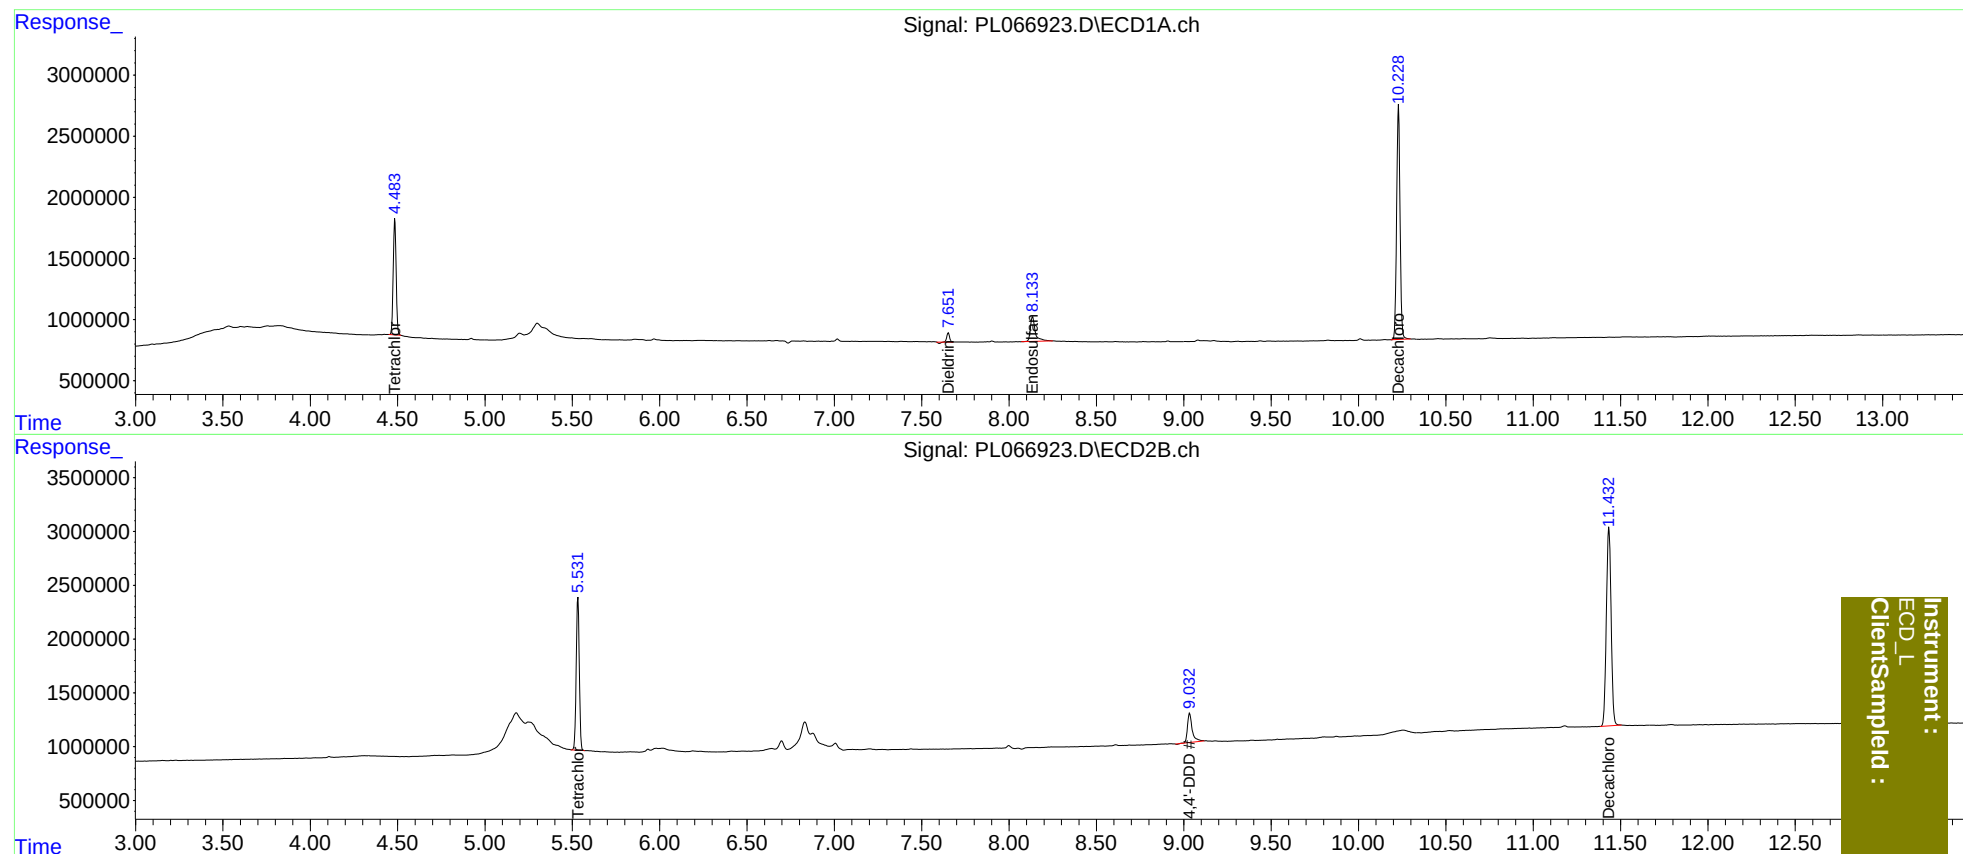


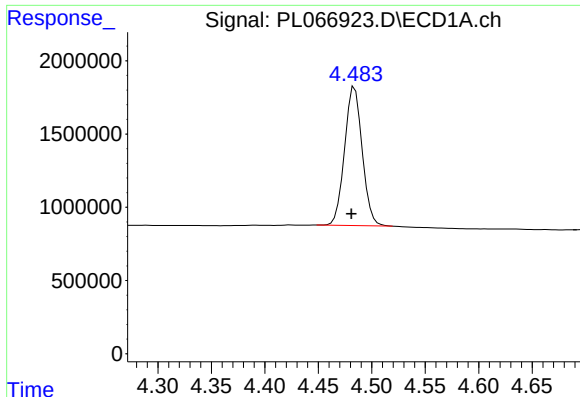

#1 Tetrachloro-m-xylene


R.T.: 4.484 min
Delta R.T.: 0.003 min
Response: 10874622
Conc: 20.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

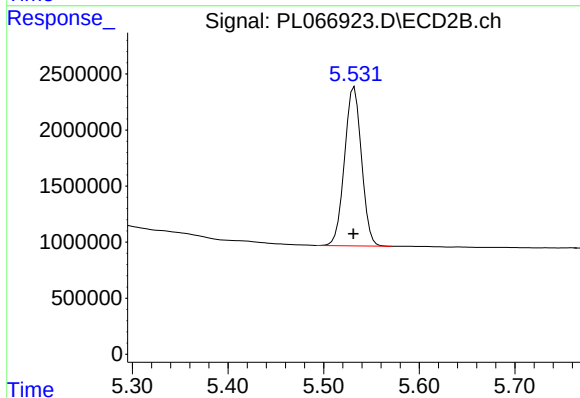


#1 Tetrachloro-m-xylene

R.T.: 5.532 min
Delta R.T.: 0.001 min
Response: 17547166
Conc: 19.84 ng/ml

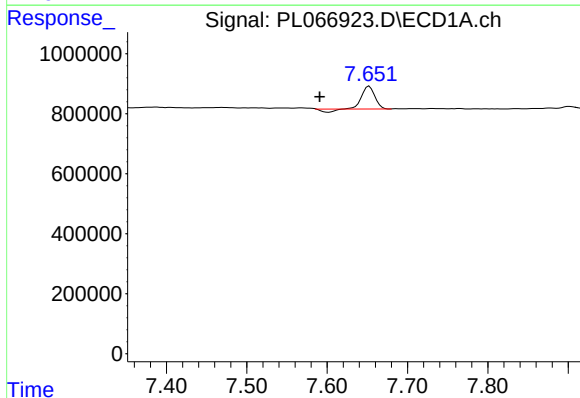


#13 Dieldrin

R.T.: 7.652 min
Delta R.T.: 0.061 min
Response: 783779
Conc: 1.15 ng/ml

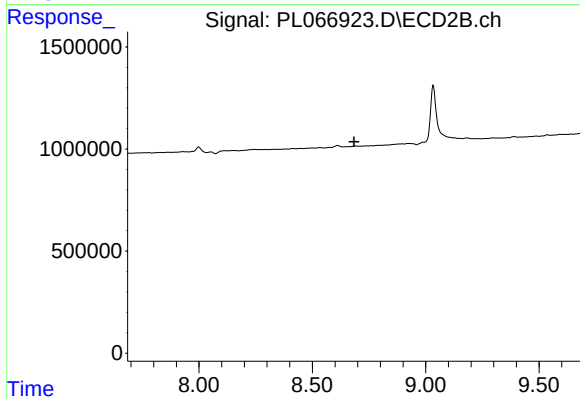

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 8.685 min
Response: 0
Conc: N.D.

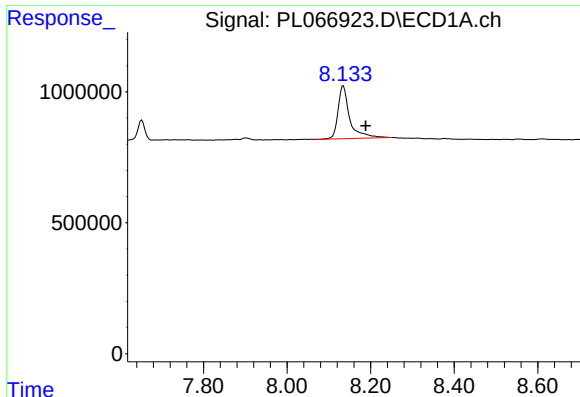

#15 Endosulfan II


R.T.: 8.135 min
Delta R.T.: -0.054 min
Response: 3920577
Conc: 6.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

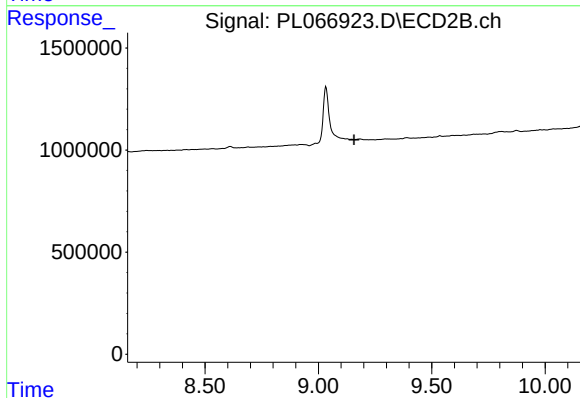


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 9.158 min
Response: 0
Conc: N.D.

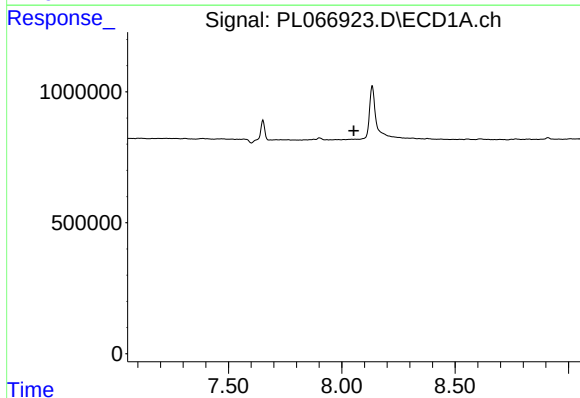


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.053 min
Response: 0
Conc: N.D.

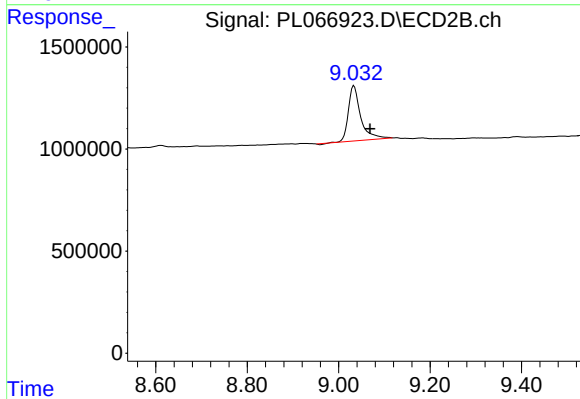

#16 4,4'-DDD


R.T.: 9.033 min
Delta R.T.: -0.035 min
Response: 5095026
Conc: 6.88 ng/ml

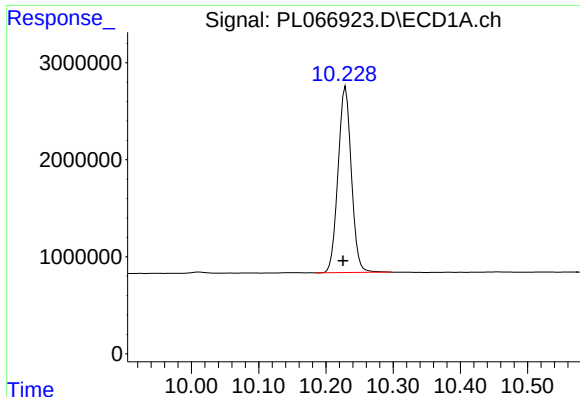

#27 Decachlorobiphenyl

R.T.: 10.229 min
Delta R.T.: 0.004 min
Response: 26172891
Conc: 39.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

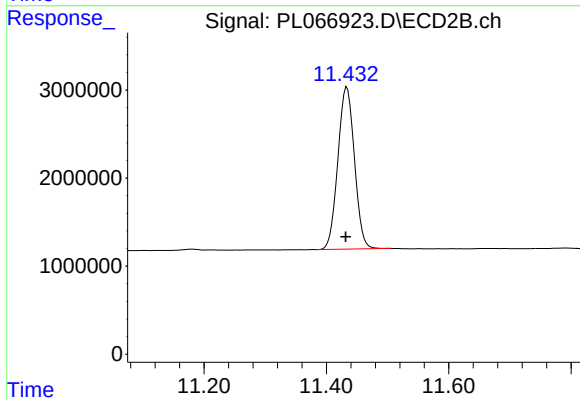

#27 Decachlorobiphenyl

R.T.: 11.434 min
Delta R.T.: 0.002 min
Response: 34608976
Conc: 37.91 ng/ml