

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052821\
 Data File : PL066926.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 May 2021 10:03
 Operator : AR\AJ
 Sample : PB136278BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 28 05:34:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052721CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 27 02:30:58 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.481	5.531	10019584	16818693	18.775	19.020
2)	SA Decachlor...	10.226	11.432	25294201	34511524	37.722	37.801
Target Compounds							
15)	B Endosulfa...	8.131f	0.000	5439822	0	9.059	N.D. #
16)	A 4,4'-DDD	0.000	9.032f	0	7162429	N.D.	9.666

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052821\
Data File : PL066926.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 May 2021 10:03
Operator : AR\AJ
Sample : PB136278BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 05:34:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052721CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 27 02:30:58 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

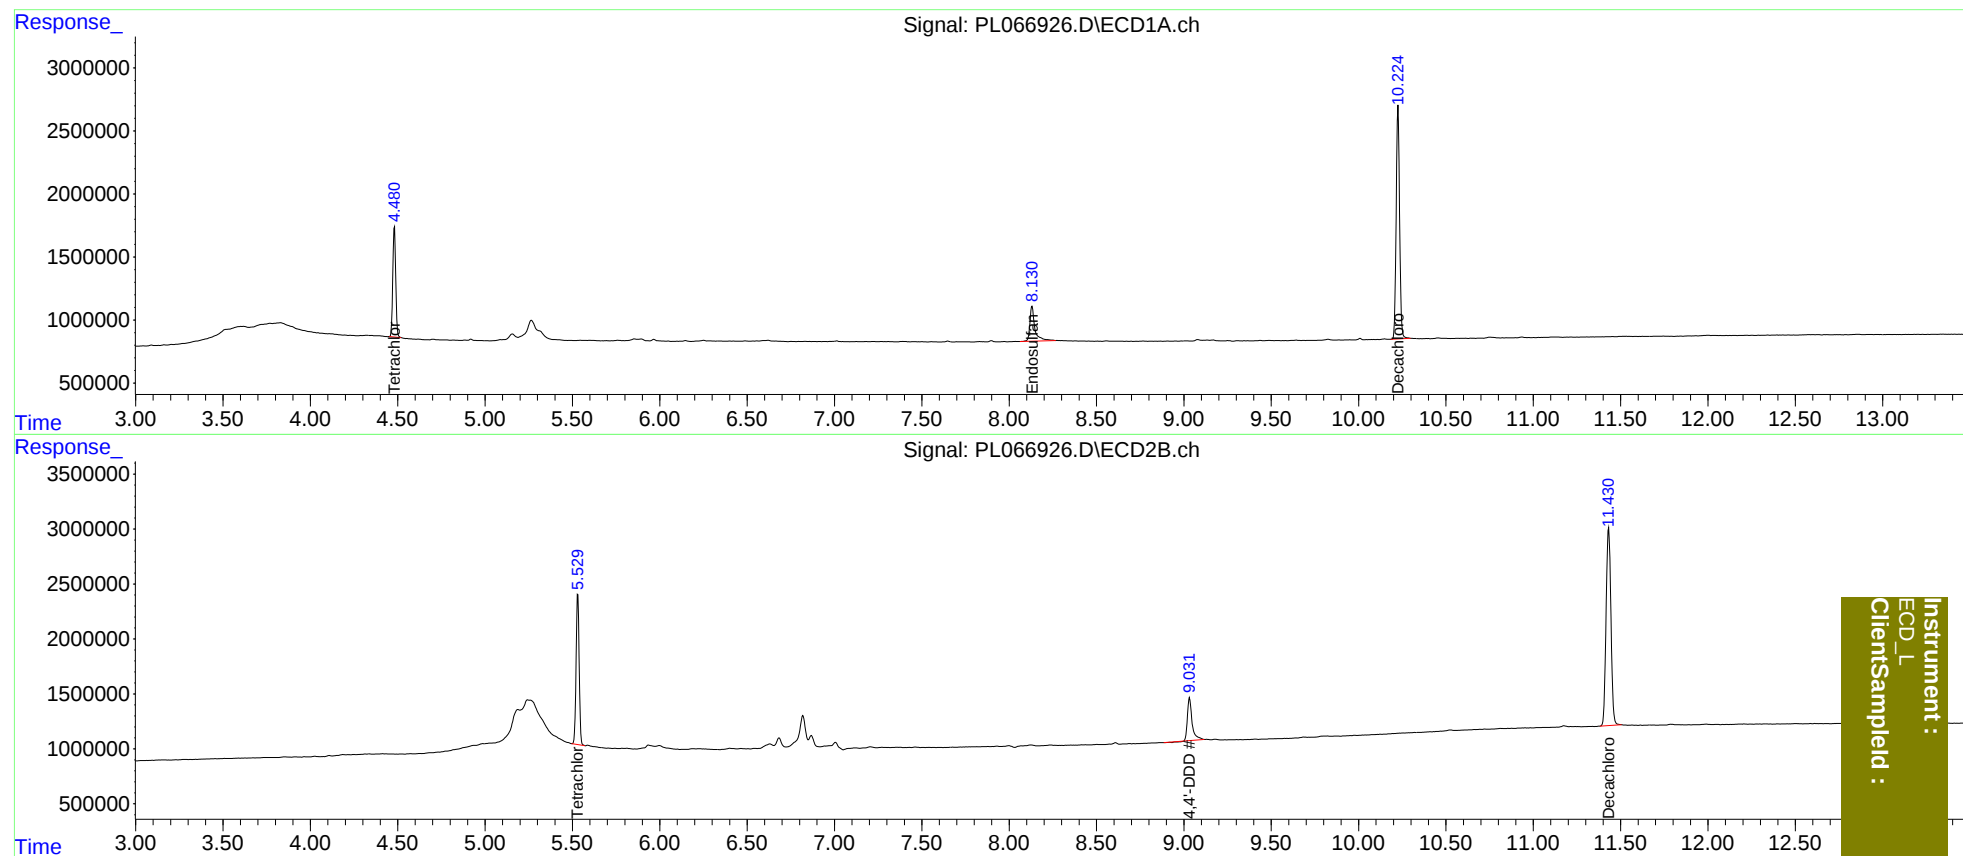


Instrument :
ECD_L
ClientSampled :

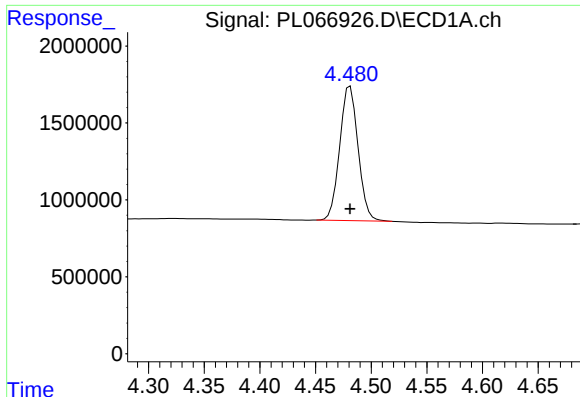

#1 Tetrachloro-m-xylene


R.T.: 4.481 min
Delta R.T.: 0.000 min
Response: 10019584
Conc: 18.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

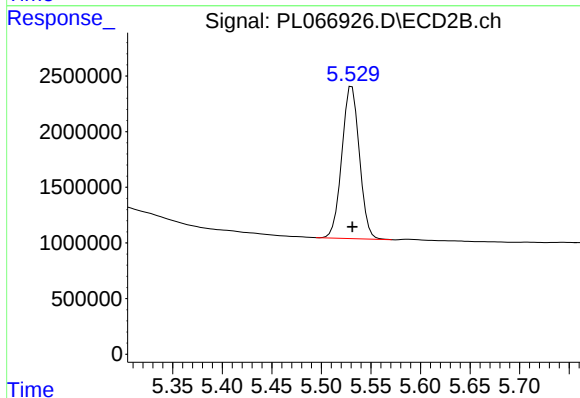


#1 Tetrachloro-m-xylene

R.T.: 5.531 min
Delta R.T.: 0.000 min
Response: 16818693
Conc: 19.02 ng/ml

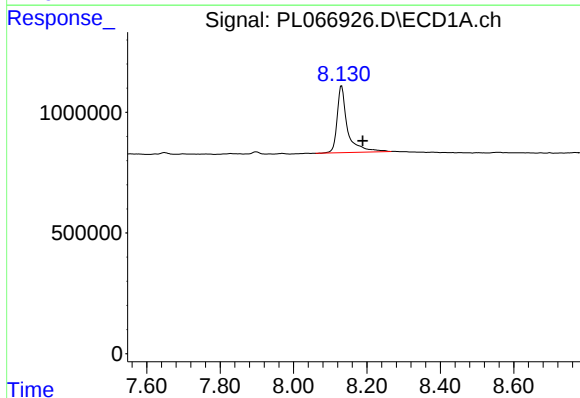


#15 Endosulfan II

R.T.: 8.131 min
Delta R.T.: -0.058 min
Response: 5439822
Conc: 9.06 ng/ml

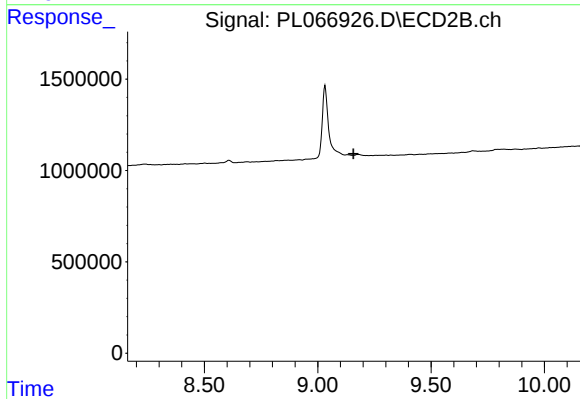

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 9.158 min
Response: 0
Conc: N.D.

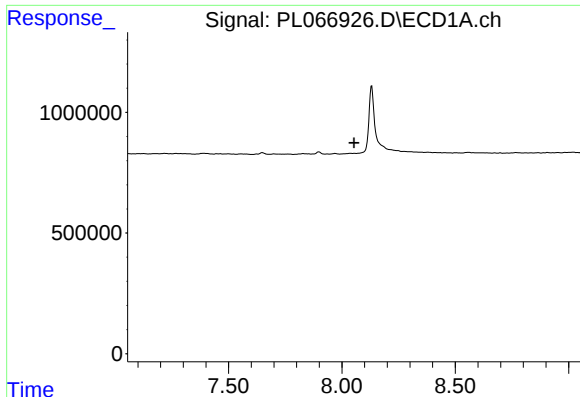

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.053 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

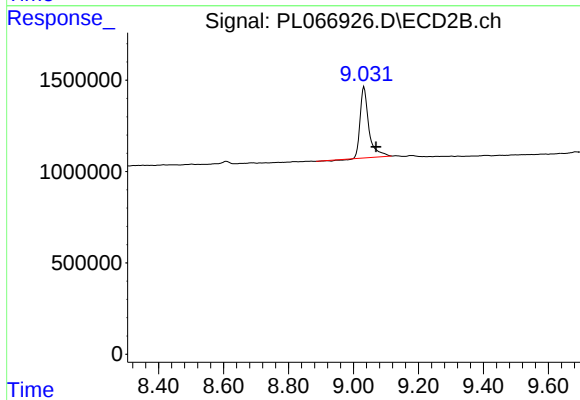


#16 4,4'-DDD

R.T.: 9.032 min
Delta R.T.: -0.037 min
Response: 7162429
Conc: 9.67 ng/ml

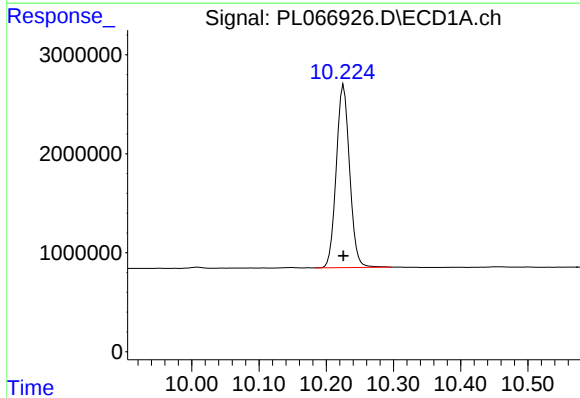

#27 Decachlorobiphenyl

R.T.: 10.226 min
Delta R.T.: 0.000 min
Response: 25294201
Conc: 37.72 ng/ml

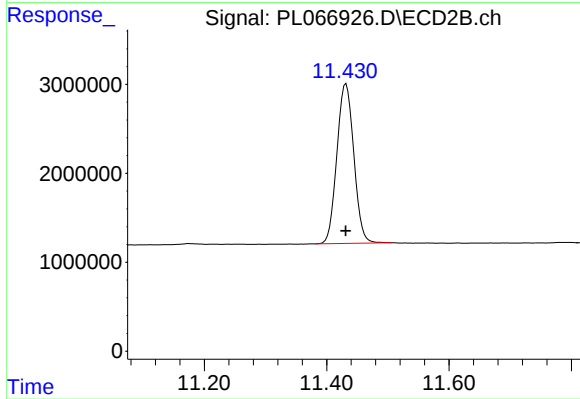

#27 Decachlorobiphenyl

R.T.: 11.432 min
Delta R.T.: 0.000 min
Response: 34511524
Conc: 37.80 ng/ml