

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052821\
 Data File : PL066928.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 May 2021 10:43
 Operator : AR\AJ
 Sample : M2250-01
 Misc : TOX MDL 100 PPB
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-WATER-QT3-2021-05

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 28 06:32:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052721CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 27 02:30:58 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.481	5.530	10260445	17125551	19.226	19.367
27)	SA Decachlor...	10.225	11.431	25725972	35277520	38.366	38.640
Target Compounds							
22)	Toxaphene-1	7.562	8.577	306969	512300	108.865	97.921
23)	Toxaphene-2	7.731	8.895	405863	471781	106.448	85.744
24)	Toxaphene-3	8.226	9.333	980554	566392	88.639	86.527
25)	Toxaphene-4	8.492	9.418	992213	1188904	85.817	90.746
26)	Toxaphene-5	9.008	9.948	1226250	944863	94.309	89.618

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052821\
Data File : PL066928.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 May 2021 10:43
Operator : AR\AJ
Sample : M2250-01
Misc : TOX MDL 100 PPB
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 06:32:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052721CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 27 02:30:58 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

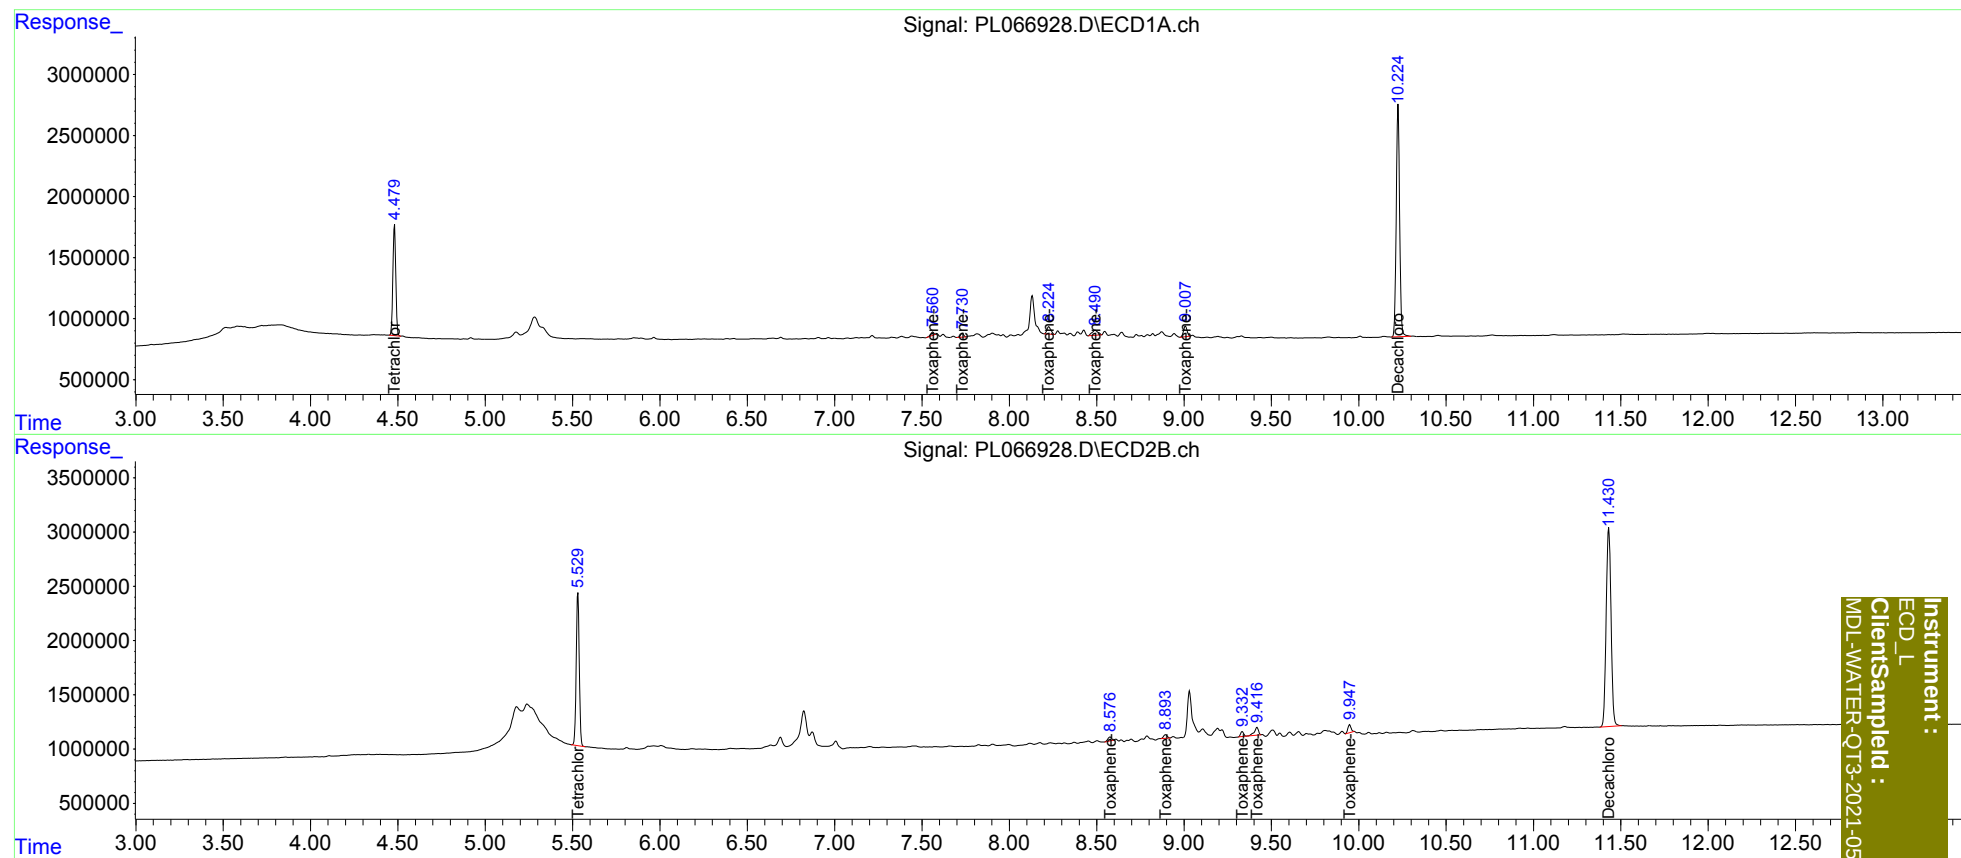

Instrument :
ECD_L
Client Sample :
MDL-WATER-QT3-2021-05