

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052822\
 Data File : PL075164.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2022 10:34
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 02:55:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Tue May 31 02:52:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.644	4.644	13217107	36412373	22.488	22.986
28)	SA Decachlor...	11.642	10.393	12131120	28199590	22.625	20.550
Target Compounds							
7)	B delta-BHC	0.000	6.406	0	435589	N.D.	0.203 #
8)	B Heptachlo...	8.127	0.000	509934	0	0.747	N.D. #
13)	MA Dieldrin	0.000	7.761	0	1056844	N.D.	0.609 #
14)	MA Endrin	0.000	8.074f	0	2799794	N.D.	1.799 #
17)	MA 4,4'-DDT	9.529	8.468	258613	344018	0.444	0.241 #
18)	B Endrin al...	9.431	0.000	326609	0	0.743	N.D. #
19)	B Endosulfa...	0.000	8.779	0	332178	N.D.	0.222 #
20)	A Methoxychlor	0.000	9.042f	0	213380	N.D.	0.263 #
21)	B Endrin ke...	10.188f	0.000	99120	0	0.161	N.D. #
27)	Chlordane-5	0.000	8.132	0	147422	N.D.	2.862 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052822\
Data File : PL075164.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2022 10:34
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 02:55:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Tue May 31 02:52:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

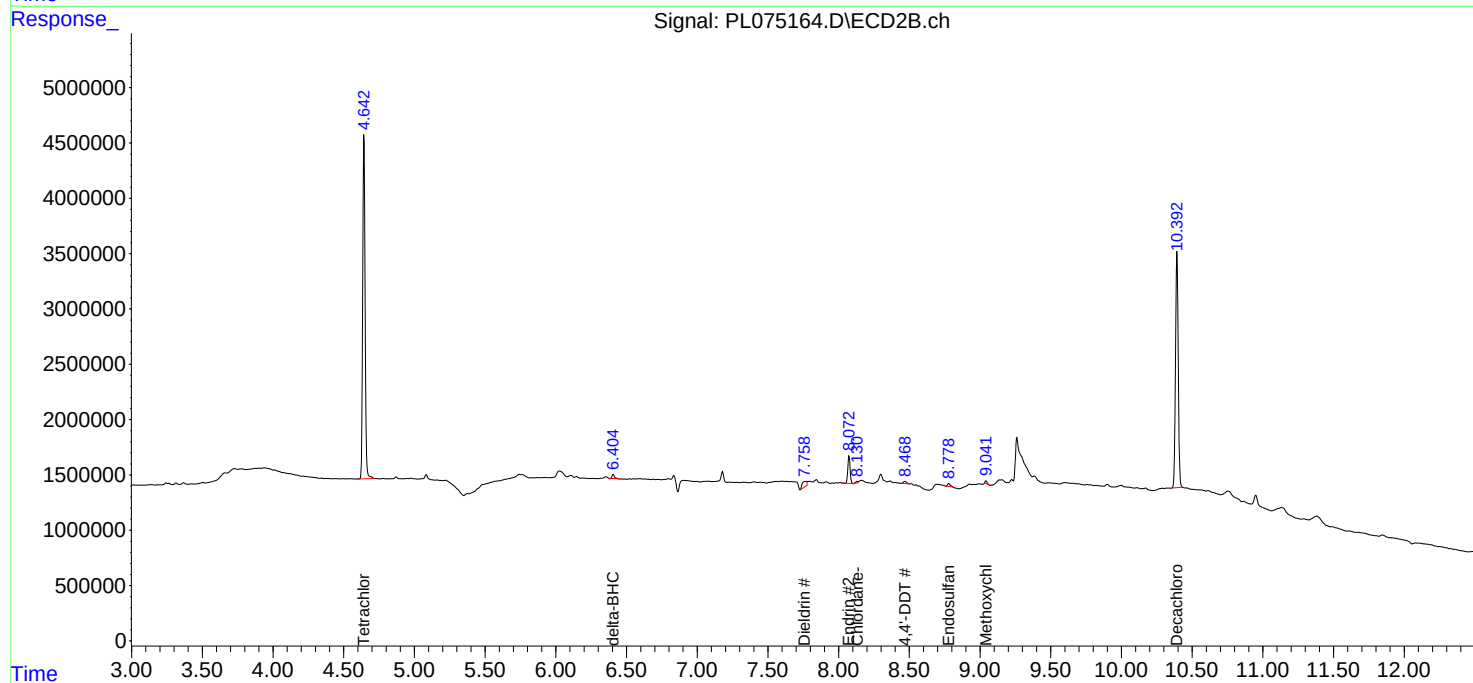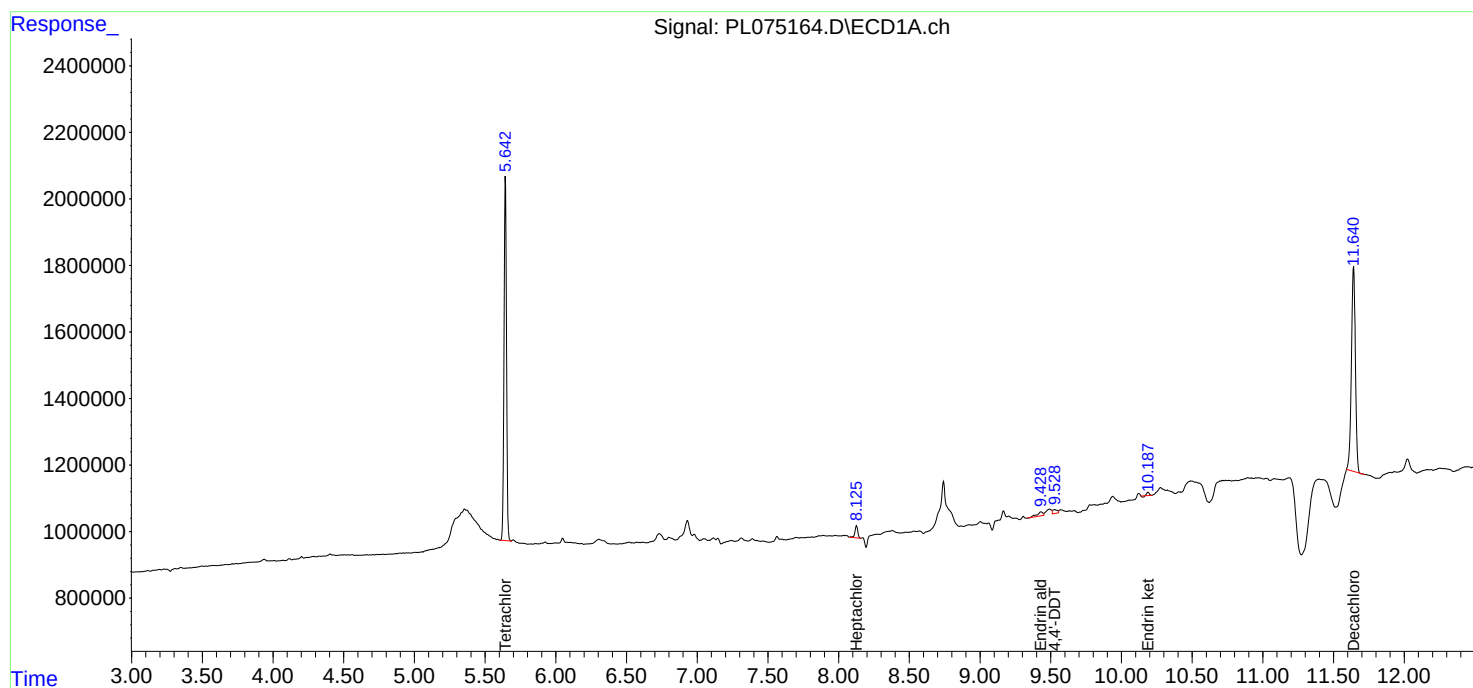


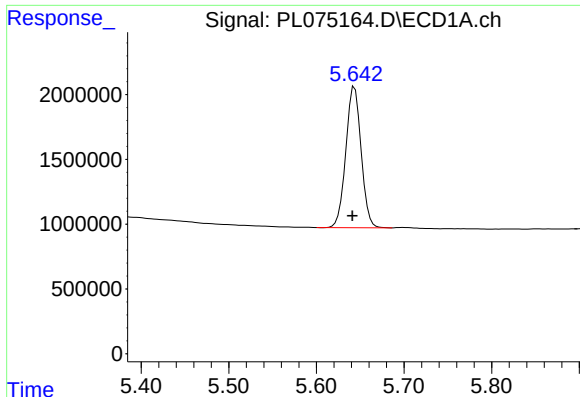

#1 Tetrachloro-m-xylene


R.T.: 5.644 min
Delta R.T.: 0.003 min
Response: 13217107
Conc: 22.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

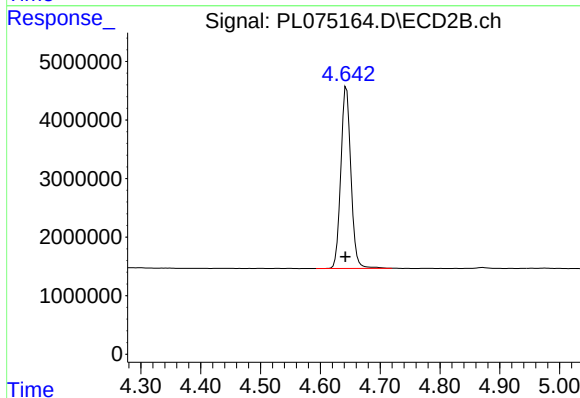


#1 Tetrachloro-m-xylene

R.T.: 4.644 min
Delta R.T.: 0.002 min
Response: 36412373
Conc: 22.99 ng/ml

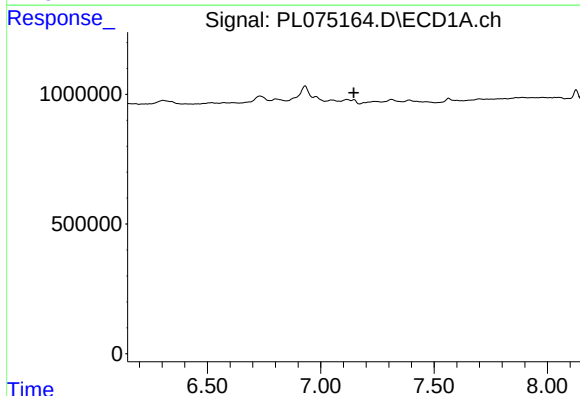


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

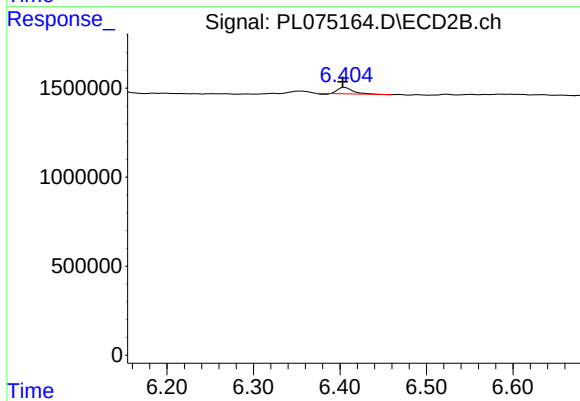

#7 delta-BHC


R.T.: 6.406 min
Delta R.T.: 0.002 min
Response: 435589
Conc: 0.20 ng/ml

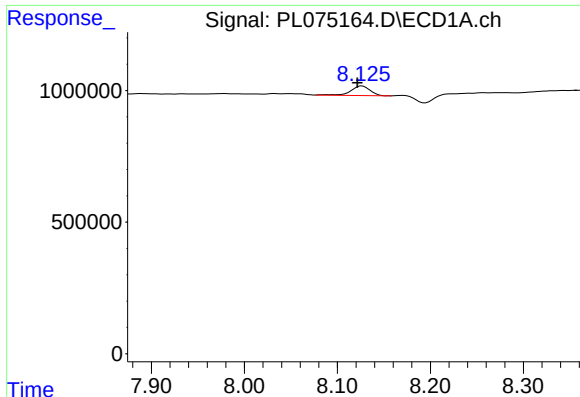

#8 Heptachlor epoxide


R.T.: 8.127 min
Delta R.T.: 0.005 min
Response: 509934
Conc: 0.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

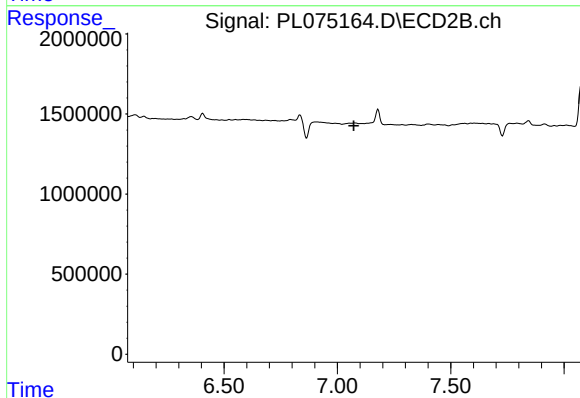


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.072 min
Response: 0
Conc: N.D.

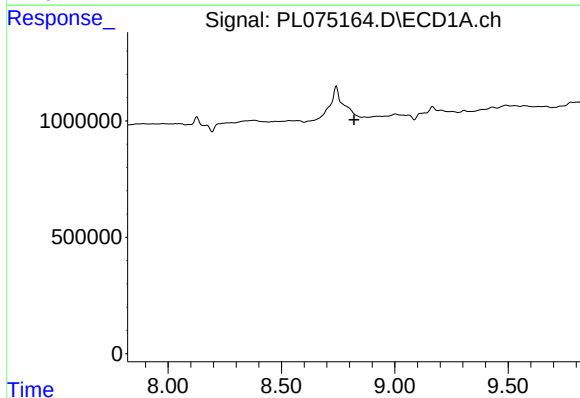


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.821 min
Response: 0
Conc: N.D.

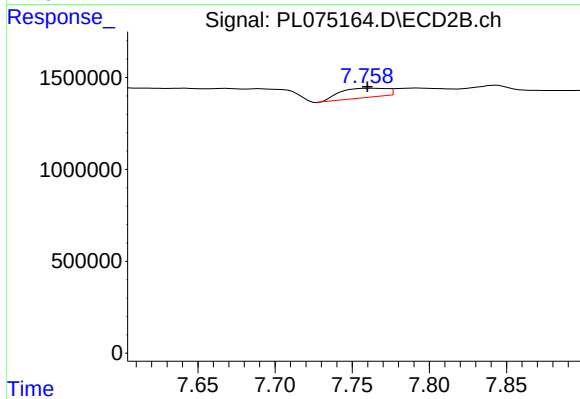

#13 Dieldrin


R.T.: 7.761 min
Delta R.T.: 0.001 min
Response: 1056844
Conc: 0.61 ng/ml

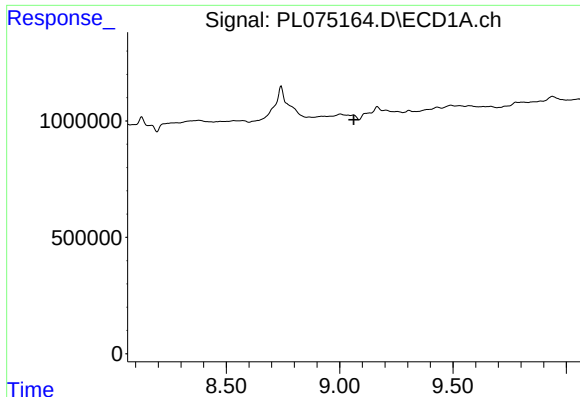

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

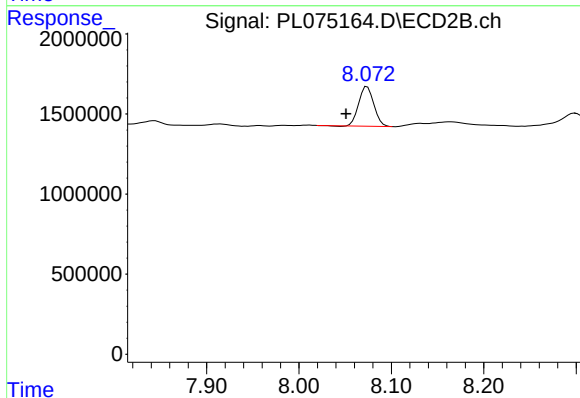


#14 Endrin

R.T.: 8.074 min
Delta R.T.: 0.023 min
Response: 2799794
Conc: 1.80 ng/ml

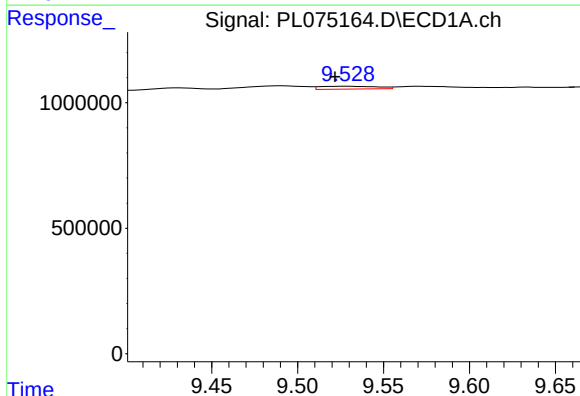


#17 4,4'-DDT

R.T.: 9.529 min
Delta R.T.: 0.007 min
Response: 258613
Conc: 0.44 ng/ml

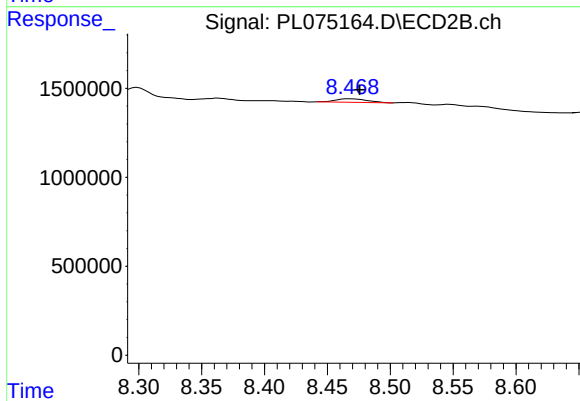

#17 4,4'-DDT


R.T.: 8.468 min
Delta R.T.: -0.008 min
Response: 344018
Conc: 0.24 ng/ml

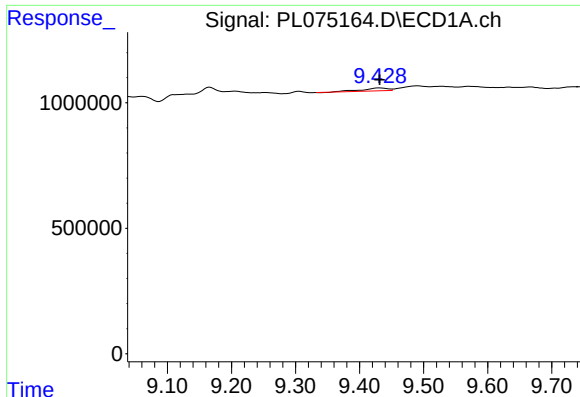

#18 Endrin aldehyde


R.T.: 9.431 min
Delta R.T.: 0.000 min
Response: 326609
Conc: 0.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

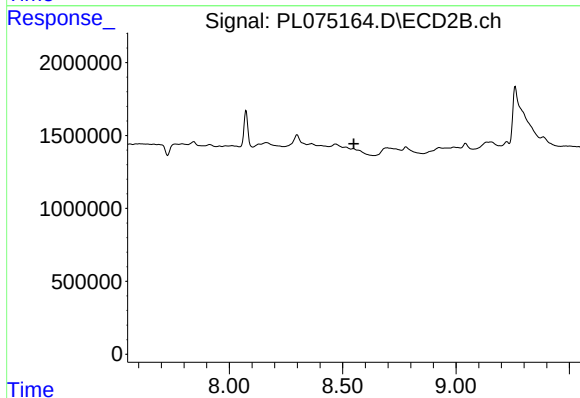


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 8.549 min
Response: 0
Conc: N.D.

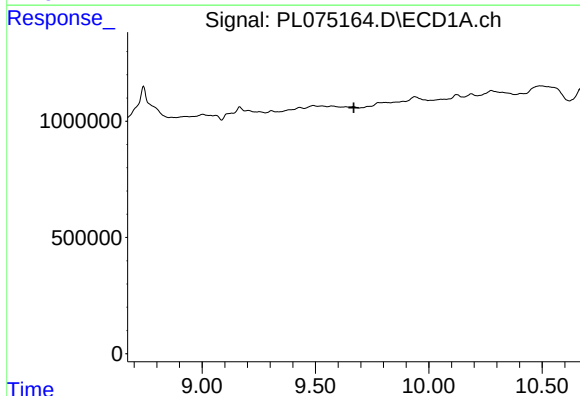


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 9.669 min
Response: 0
Conc: N.D.

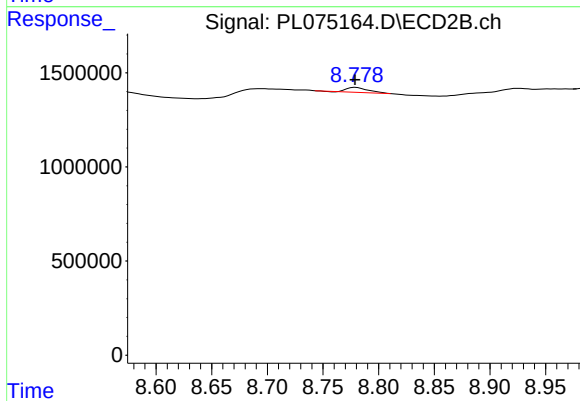

#19 Endosulfan Sulfate


R.T.: 8.779 min
Delta R.T.: 0.000 min
Response: 332178
Conc: 0.22 ng/ml

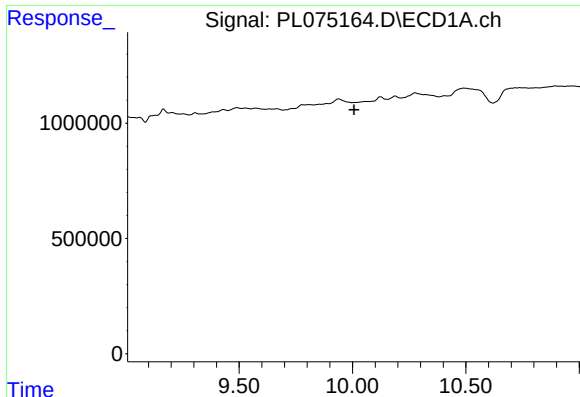

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 10.008 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

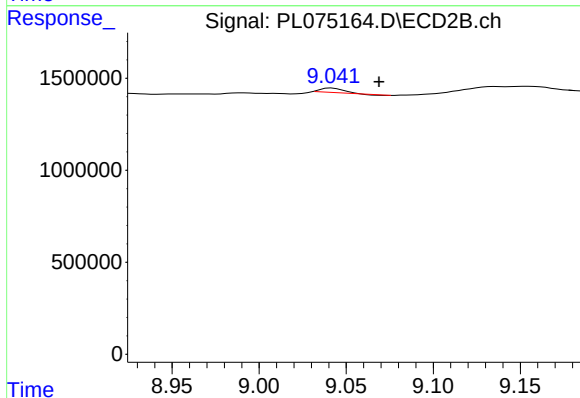


#20 Methoxychlor

R.T.: 9.042 min
Delta R.T.: -0.027 min
Response: 213380
Conc: 0.26 ng/ml

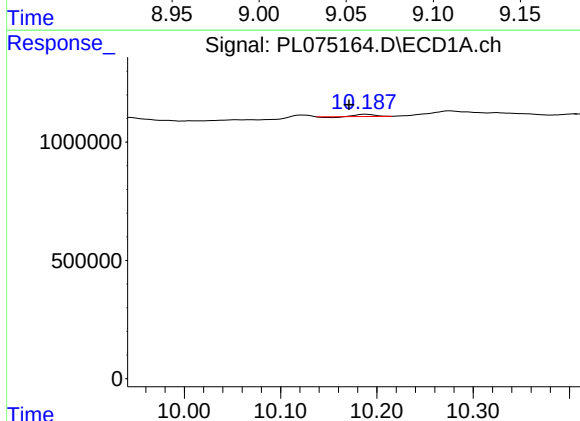


#21 Endrin ketone

R.T.: 10.188 min
Delta R.T.: 0.017 min
Response: 99120
Conc: 0.16 ng/ml

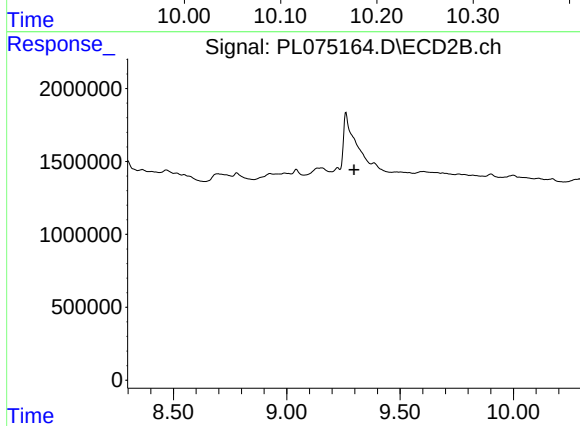

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.298 min
Response: 0
Conc: N.D.

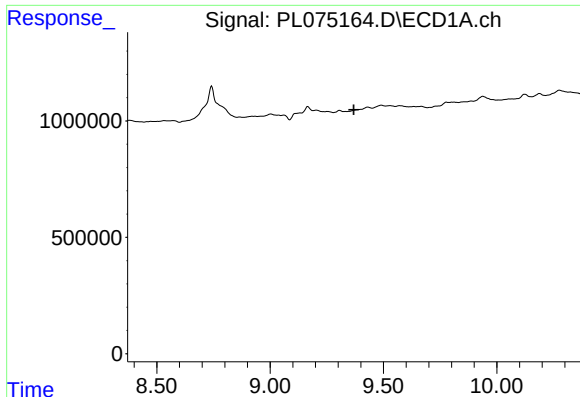

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 9.369 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

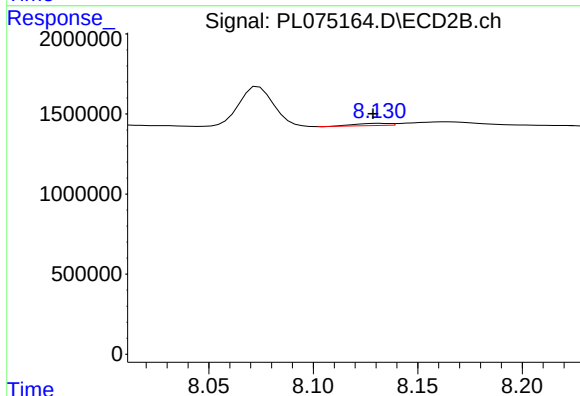


#27 Chlordane-5

R.T.: 8.132 min
Delta R.T.: 0.003 min
Response: 147422
Conc: 2.86 ng/ml

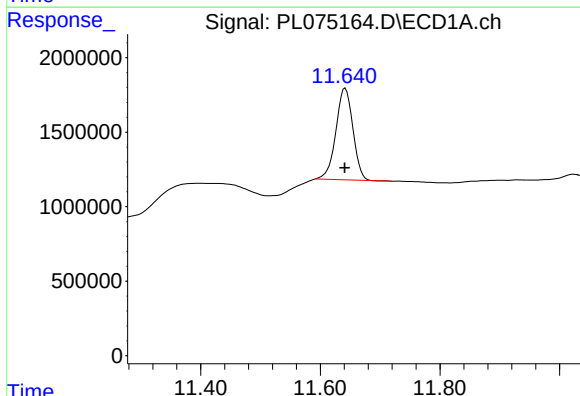

#28 Decachlorobiphenyl

R.T.: 11.642 min
Delta R.T.: 0.000 min
Response: 12131120
Conc: 22.62 ng/ml

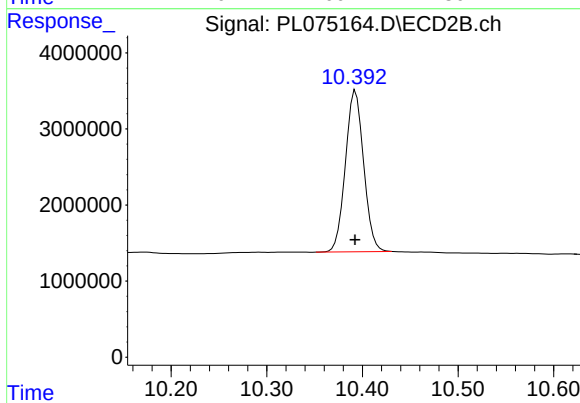

#28 Decachlorobiphenyl

R.T.: 10.393 min
Delta R.T.: 0.000 min
Response: 28199590
Conc: 20.55 ng/ml