

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052822\
 Data File : PL075189.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2022 21:50
 Operator : AR\AJ
 Sample : N3026-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 02:58:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Tue May 31 02:52:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.641	4.641	11442560	29795322	19.469	18.808
28)	SA Decachlor...	11.641	10.391	7210150	18050953	13.447	13.154
Target Compounds							
5)	MB Aldrin	0.000	6.488	0	287576	N.D.	0.149 #
11)	B alpha-Chl...	0.000	7.425	0	234657	N.D.	0.128 #
13)	MA Dieldrin	8.820	7.760	209372	239021	0.330	0.138 #
14)	MA Endrin	0.000	8.075f	0	474124	N.D.	0.305 #
15)	B Endosulfa...	9.306	8.331f	226129	2551250	0.401	1.621 #
17)	MA 4,4'-DDT	9.494f	0.000	126722	0	0.218	N.D. #
18)	B Endrin al...	0.000	8.577f	0	117868	N.D.	0.098 #
21)	B Endrin ke...	10.189f	0.000	227981	0	0.371	N.D. #
26)	Chlordane-4	0.000	7.425	0	234657	N.D.	1.211 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052822\
Data File : PL075189.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2022 21:50
Operator : AR\AJ
Sample : N3026-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 02:58:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Tue May 31 02:52:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

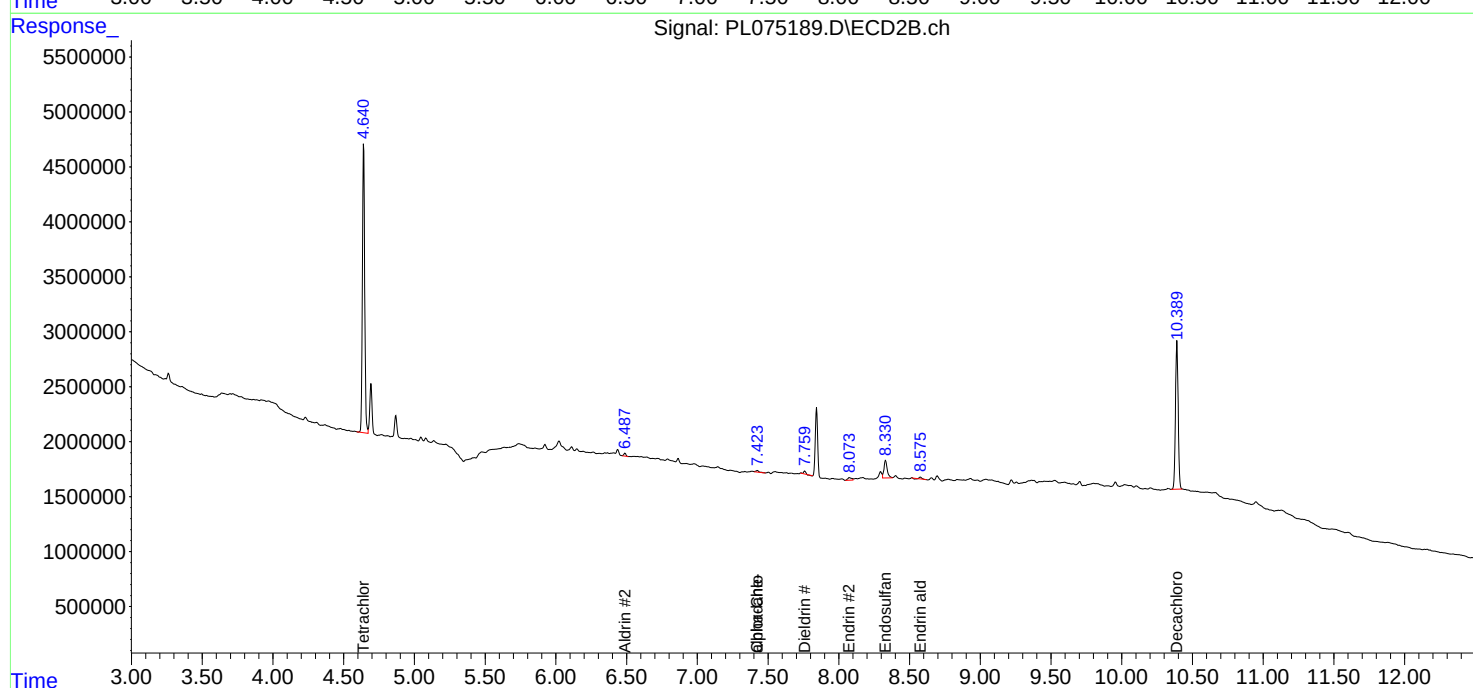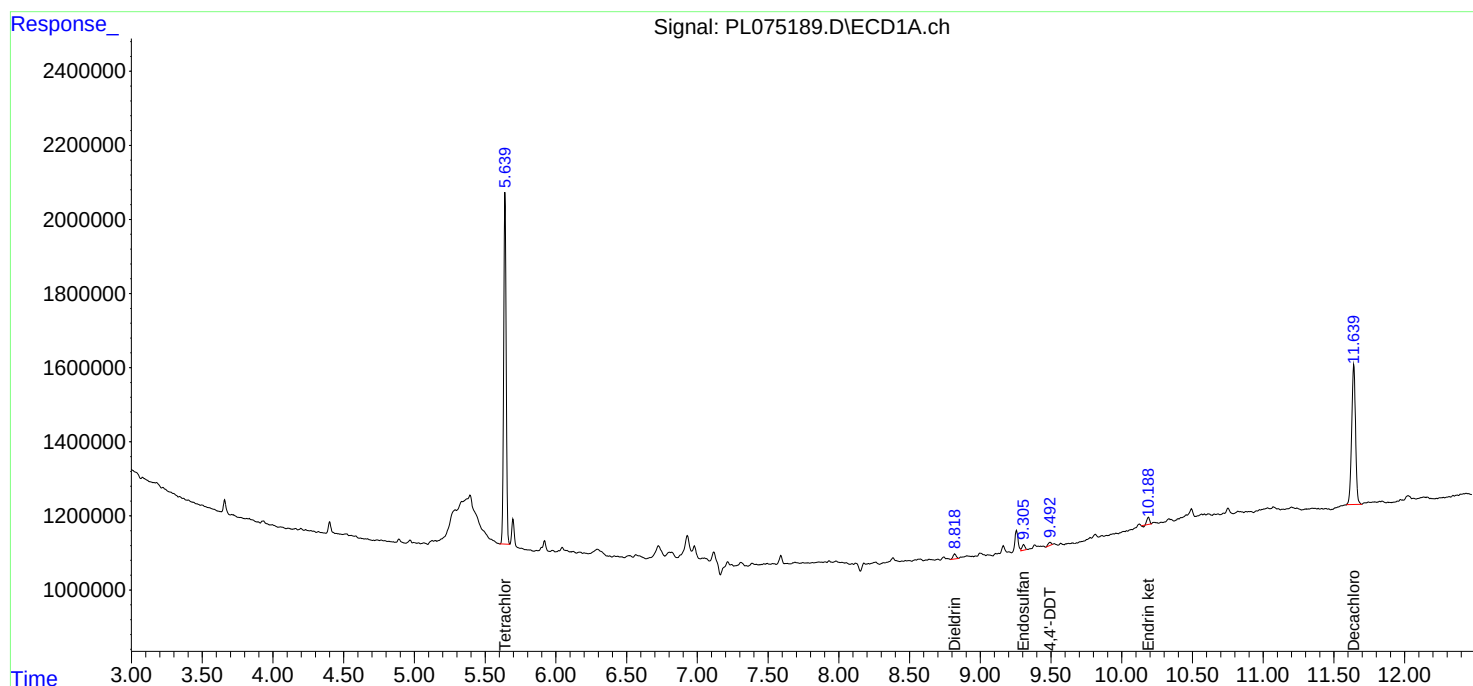


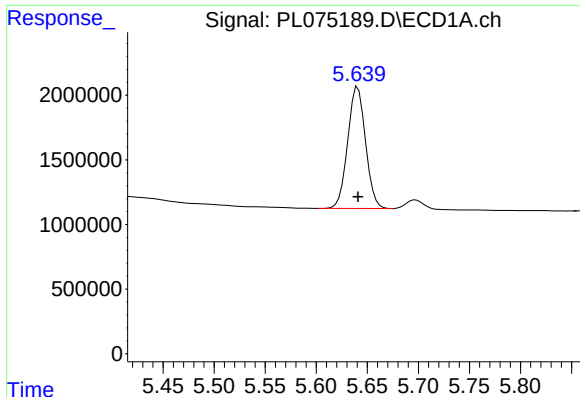

#1 Tetrachloro-m-xylene


R.T.: 5.641 min
Delta R.T.: 0.000 min
Response: 11442560
Conc: 19.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

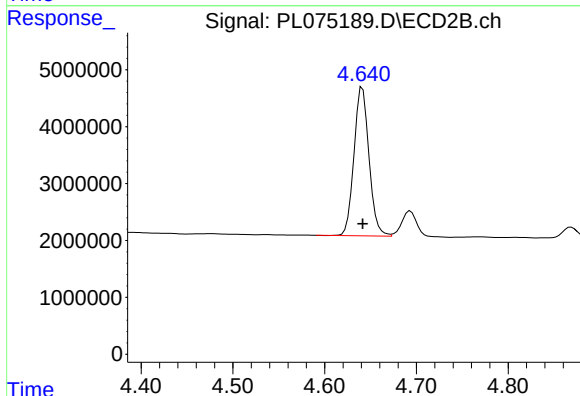


#1 Tetrachloro-m-xylene

R.T.: 4.641 min
Delta R.T.: 0.000 min
Response: 29795322
Conc: 18.81 ng/ml

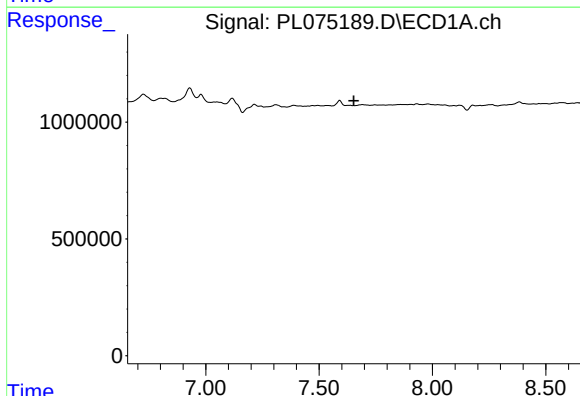


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 7.654 min
Response: 0
Conc: N.D.

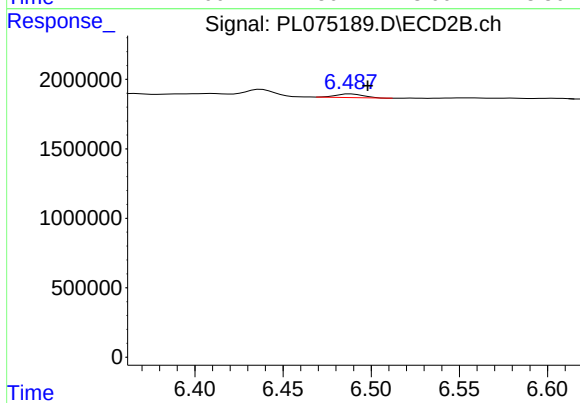

#5 Aldrin


R.T.: 6.488 min
Delta R.T.: -0.010 min
Response: 287576
Conc: 0.15 ng/ml

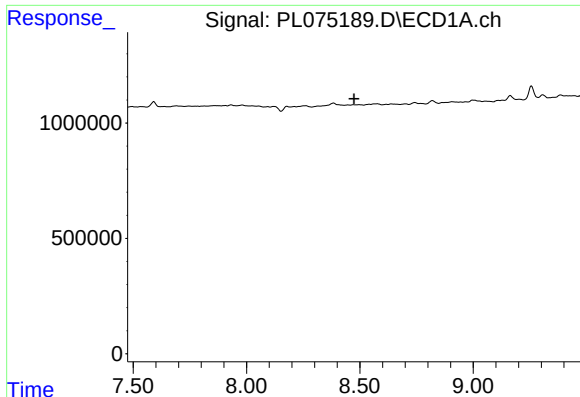

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.474 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

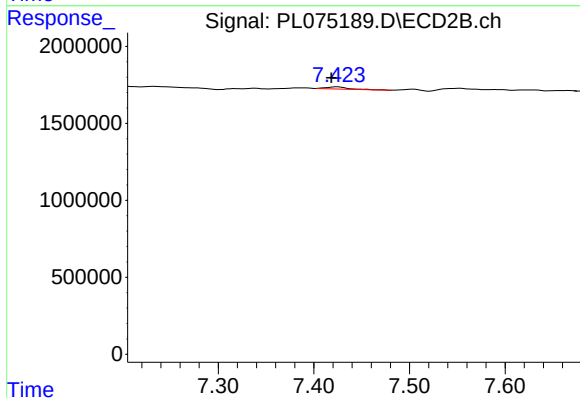


#11 alpha-Chlordane

R.T.: 7.425 min
Delta R.T.: 0.006 min
Response: 234657
Conc: 0.13 ng/ml

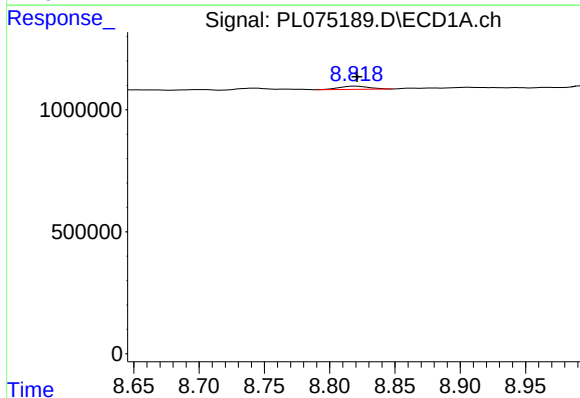


#13 Dieldrin

R.T.: 8.820 min
Delta R.T.: -0.001 min
Response: 209372
Conc: 0.33 ng/ml

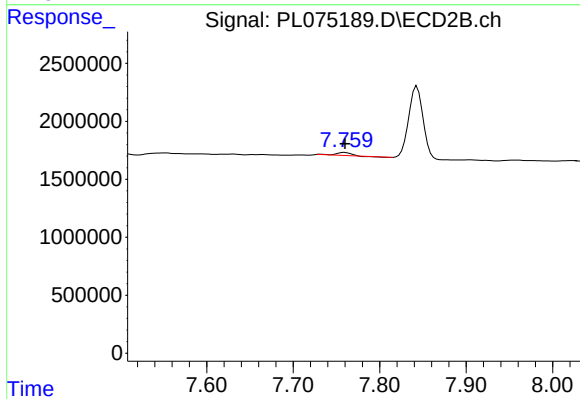

#13 Dieldrin


R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 239021
Conc: 0.14 ng/ml

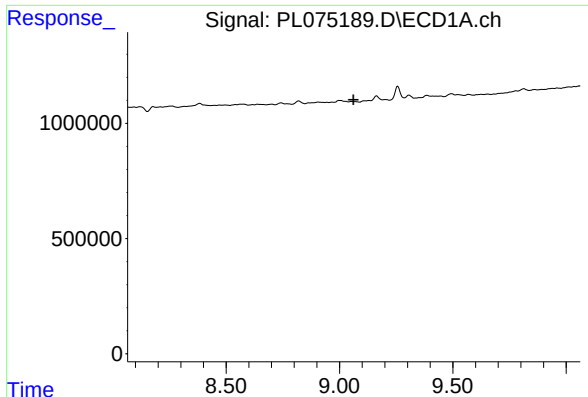

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

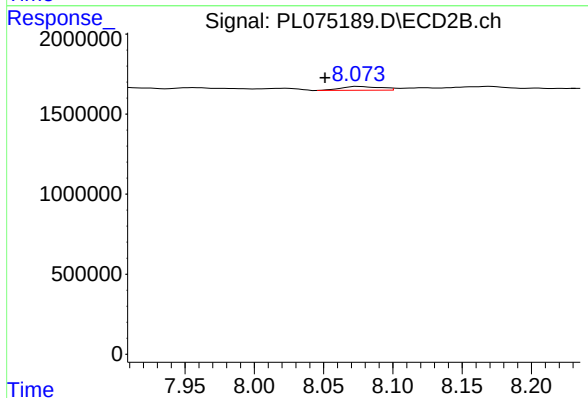


#14 Endrin

R.T.: 8.075 min
Delta R.T.: 0.024 min
Response: 474124
Conc: 0.30 ng/ml

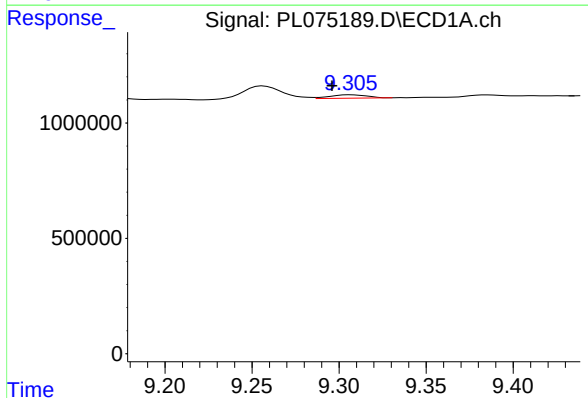


#15 Endosulfan II

R.T.: 9.306 min
Delta R.T.: 0.011 min
Response: 226129
Conc: 0.40 ng/ml

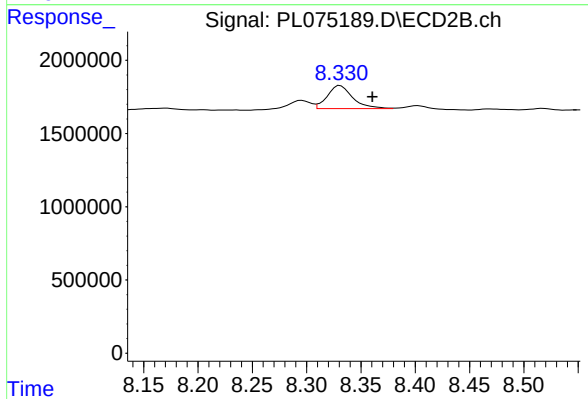

#15 Endosulfan II


R.T.: 8.331 min
Delta R.T.: -0.030 min
Response: 2551250
Conc: 1.62 ng/ml

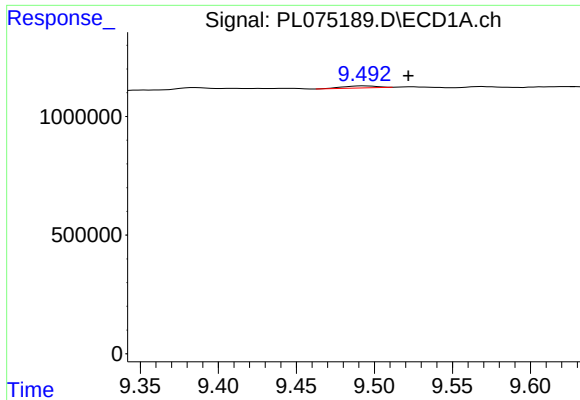

#17 4,4'-DDT


R.T.: 9.494 min
Delta R.T.: -0.028 min
Response: 126722
Conc: 0.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

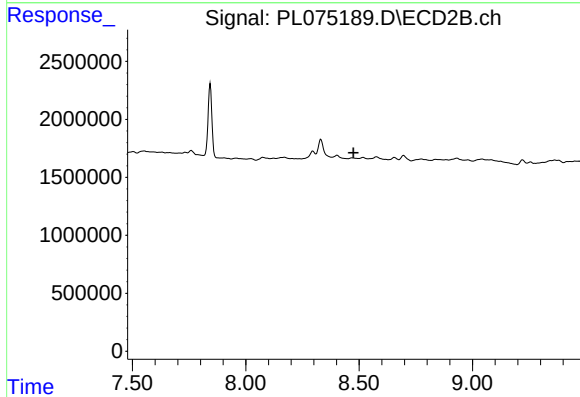


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 8.476 min
Response: 0
Conc: N.D.

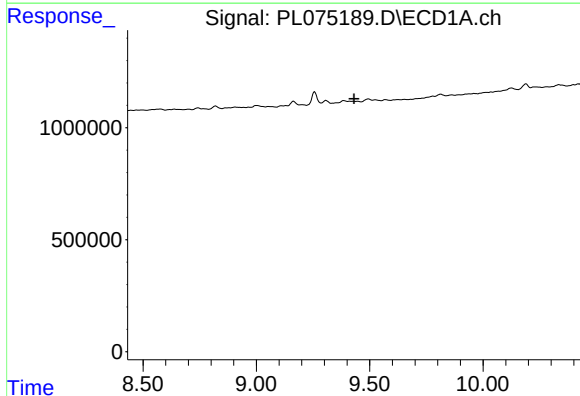


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 9.431 min
Response: 0
Conc: N.D.

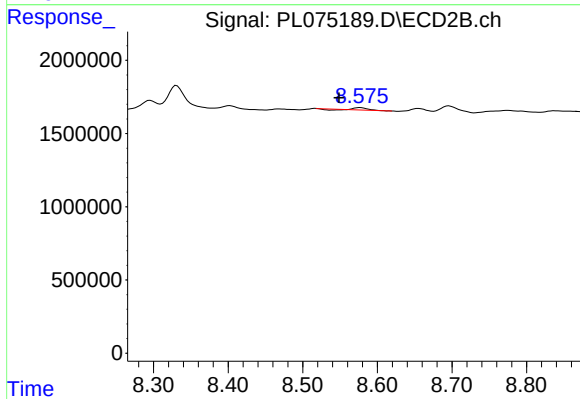

#18 Endrin aldehyde


R.T.: 8.577 min
Delta R.T.: 0.028 min
Response: 117868
Conc: 0.10 ng/ml

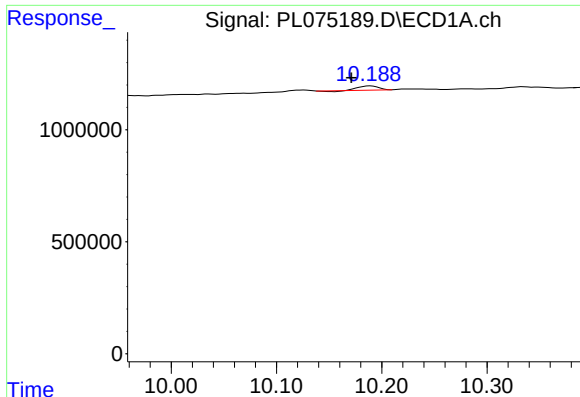

#21 Endrin ketone


R.T.: 10.189 min
Delta R.T.: 0.018 min
Response: 227981
Conc: 0.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

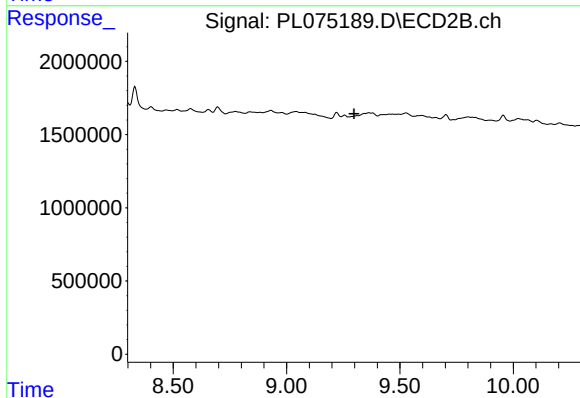


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.298 min
Response: 0
Conc: N.D.

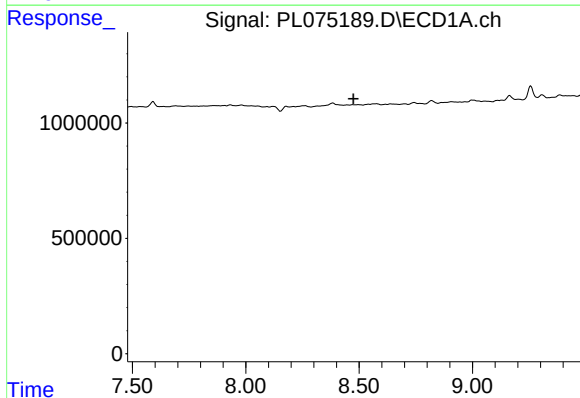


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.476 min
Response: 0
Conc: N.D.

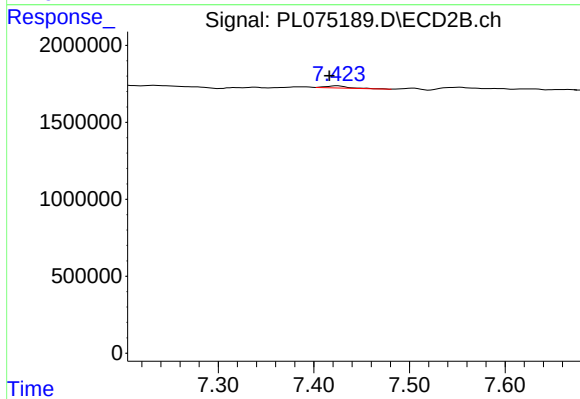

#26 Chlordane-4


R.T.: 7.425 min
Delta R.T.: 0.009 min
Response: 234657
Conc: 1.21 ng/ml

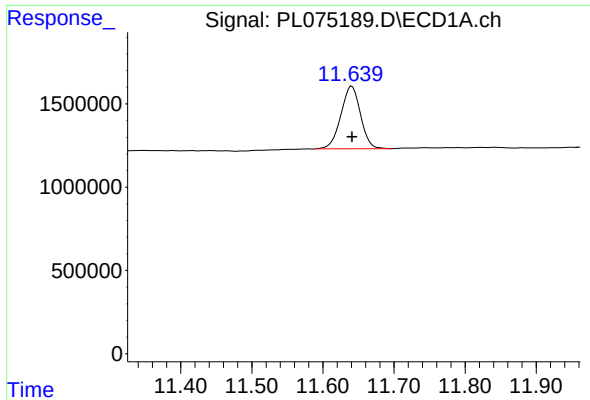

#28 Decachlorobiphenyl

R.T.: 11.641 min
Delta R.T.: 0.000 min
Response: 7210150
Conc: 13.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

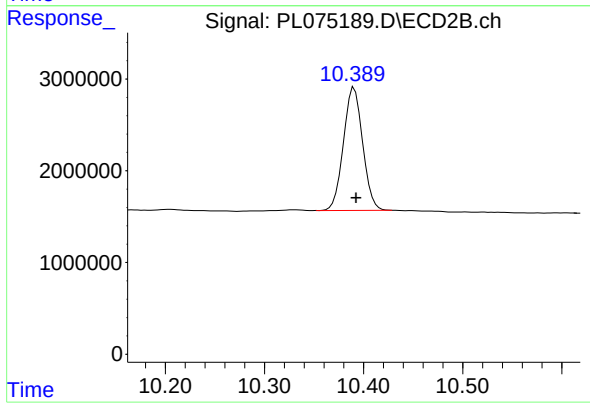

#28 Decachlorobiphenyl

R.T.: 10.391 min
Delta R.T.: -0.002 min
Response: 18050953
Conc: 13.15 ng/ml