

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052822\
 Data File : PL075199.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 May 2022 01:10
 Operator : AR\AJ
 Sample : N3026-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 03:01:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Tue May 31 02:52:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.641	4.641	11700762	30561940	19.908	19.292
28)	SA Decachlor...	11.641	10.391	7026464	16219388	13.105	11.819
Target Compounds							
5)	MB Aldrin	0.000	6.489	0	323430	N.D.	0.168 #
11)	B alpha-Chl...	0.000	7.426	0	226750	N.D.	0.124 #
13)	MA Dieldrin	8.821	7.760	197659	524705	0.312	0.302
14)	MA Endrin	0.000	8.074f	0	161985	N.D.	0.104 #
15)	B Endosulfa...	9.305	8.331f	213051	1619460	0.377	1.029 #
17)	MA 4,4'-DDT	9.496f	0.000	119038	0	0.204	N.D. #
21)	B Endrin ke...	10.188f	0.000	276432	0	0.450	N.D. #
26)	Chlordane-4	0.000	7.426	0	226750	N.D.	1.170 #
27)	Chlordane-5	9.388f	0.000	94342	0	4.328	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052822\
Data File : PL075199.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 May 2022 01:10
Operator : AR\AJ
Sample : N3026-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 03:01:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Tue May 31 02:52:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

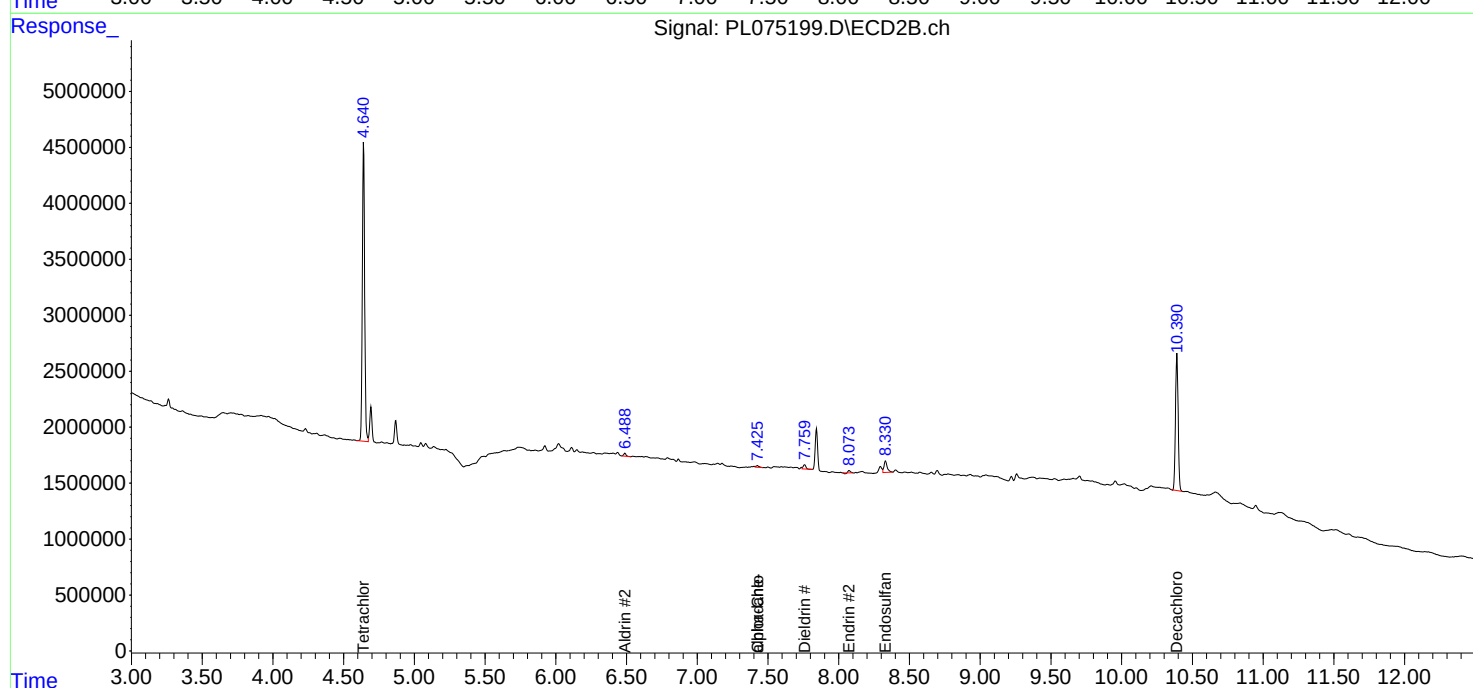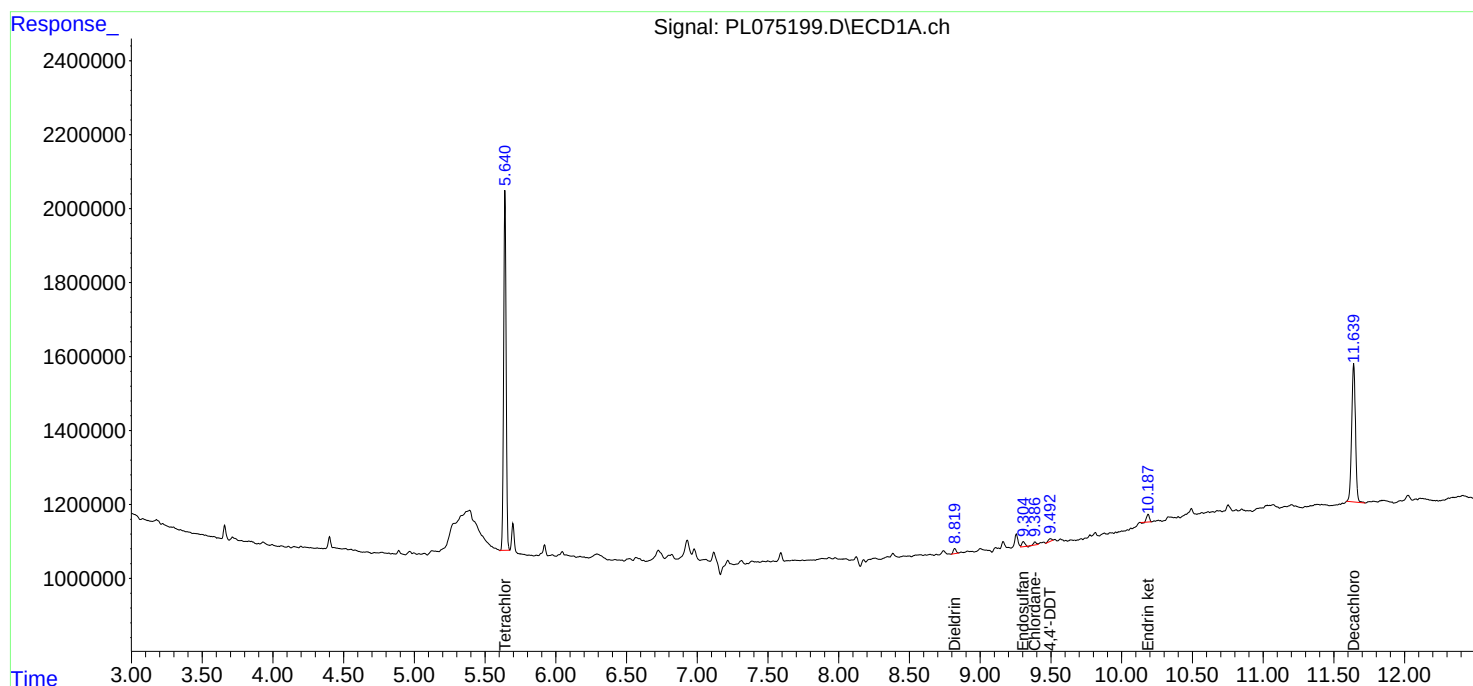


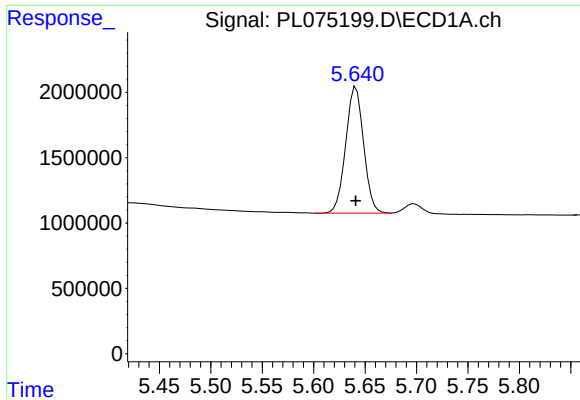

#1 Tetrachloro-m-xylene


R.T.: 5.641 min
Delta R.T.: 0.000 min
Response: 11700762
Conc: 19.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

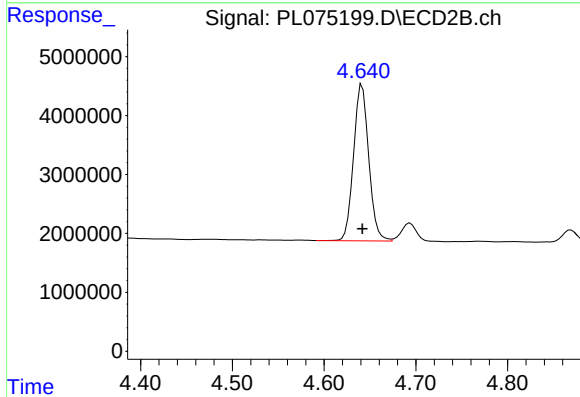


#1 Tetrachloro-m-xylene

R.T.: 4.641 min
Delta R.T.: 0.000 min
Response: 30561940
Conc: 19.29 ng/ml

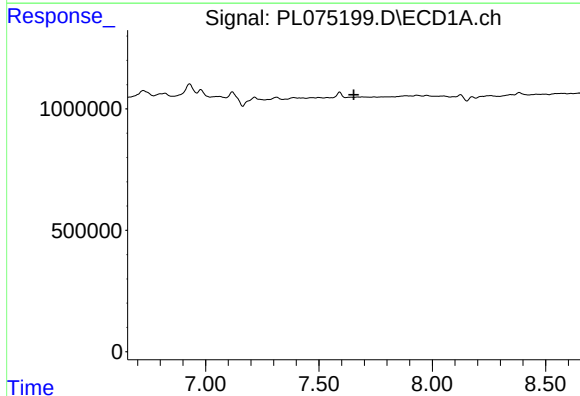


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 7.654 min
Response: 0
Conc: N.D.

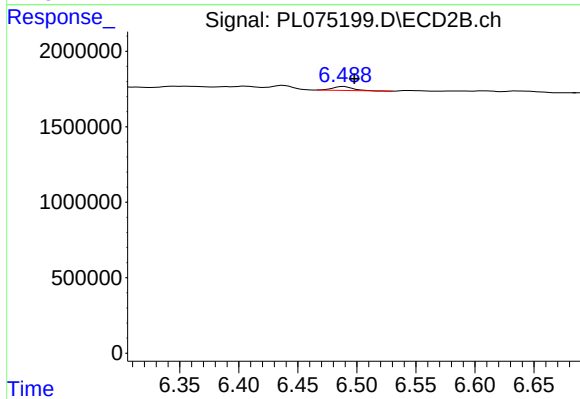

#5 Aldrin


R.T.: 6.489 min
Delta R.T.: -0.009 min
Response: 323430
Conc: 0.17 ng/ml

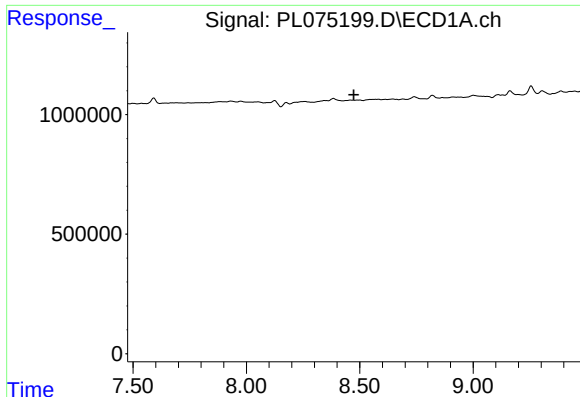

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.474 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

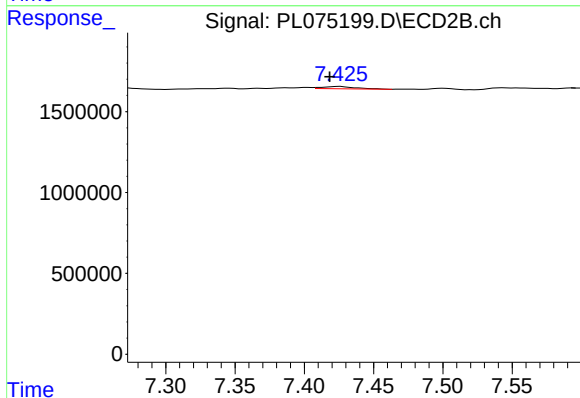


#11 alpha-Chlordane

R.T.: 7.426 min
Delta R.T.: 0.008 min
Response: 226750
Conc: 0.12 ng/ml

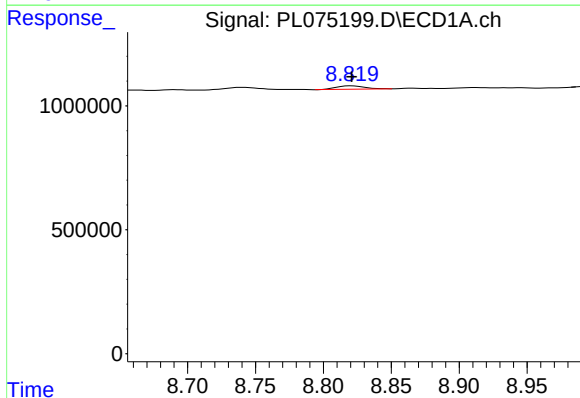


#13 Dieldrin

R.T.: 8.821 min
Delta R.T.: 0.000 min
Response: 197659
Conc: 0.31 ng/ml

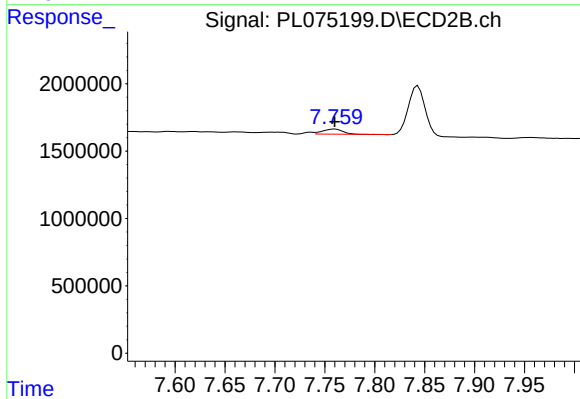

#13 Dieldrin


R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 524705
Conc: 0.30 ng/ml

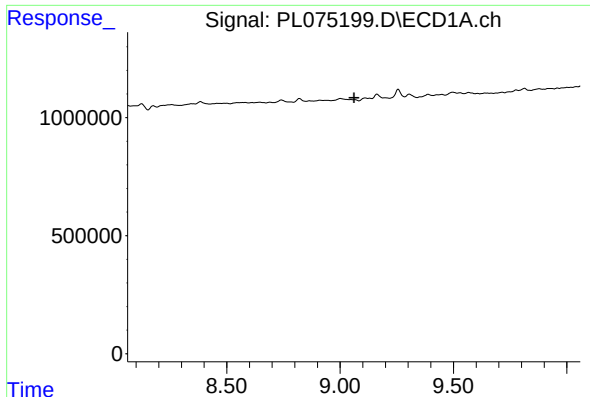

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

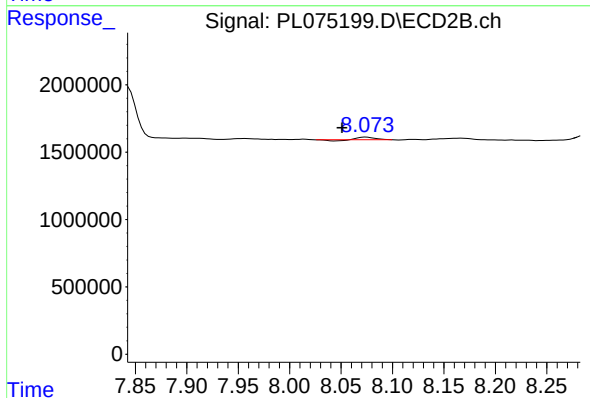


#14 Endrin

R.T.: 8.074 min
Delta R.T.: 0.023 min
Response: 161985
Conc: 0.10 ng/ml

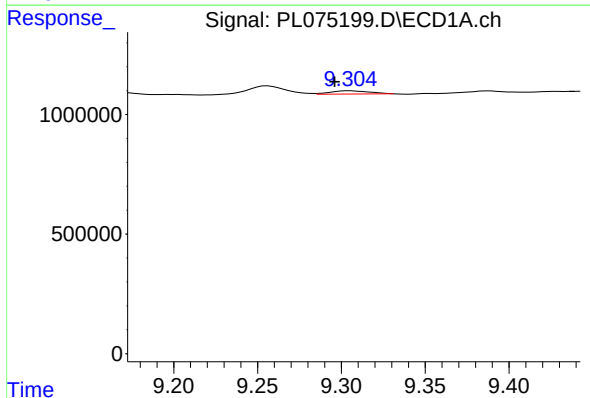


#15 Endosulfan II

R.T.: 9.305 min
Delta R.T.: 0.009 min
Response: 213051
Conc: 0.38 ng/ml

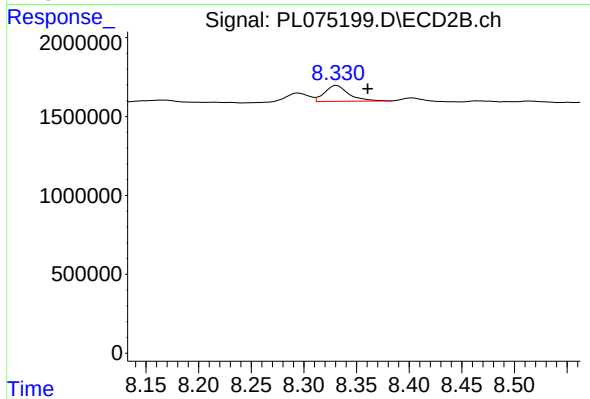

#15 Endosulfan II


R.T.: 8.331 min
Delta R.T.: -0.029 min
Response: 1619460
Conc: 1.03 ng/ml

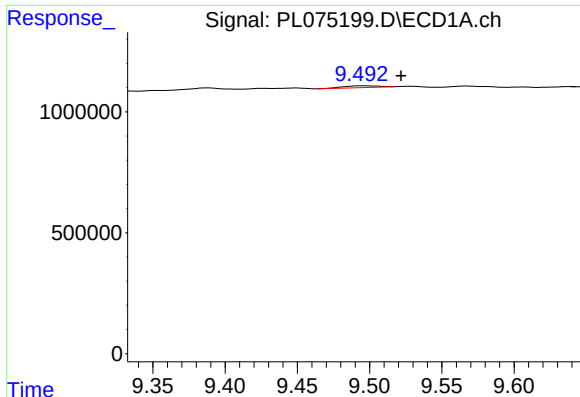

#17 4,4'-DDT


R.T.: 9.496 min
Delta R.T.: -0.026 min
Response: 119038
Conc: 0.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

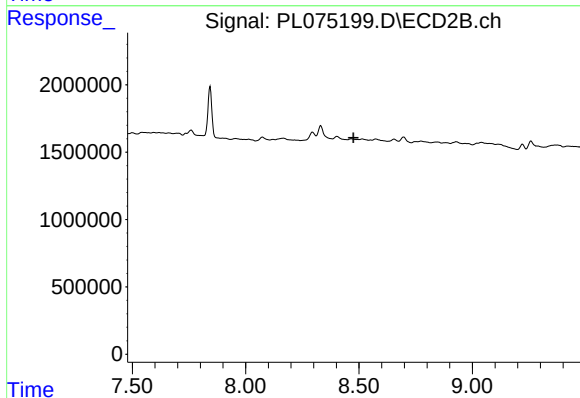


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 8.476 min
Response: 0
Conc: N.D.

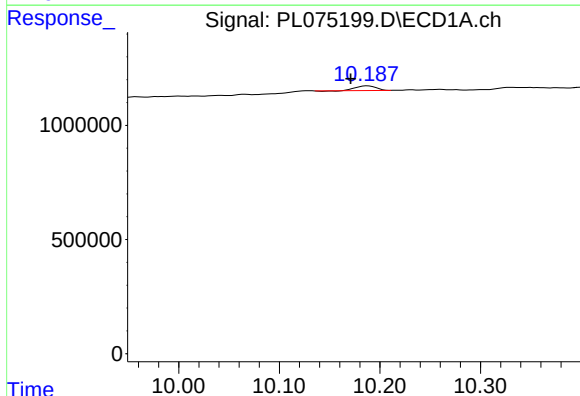


#21 Endrin ketone

R.T.: 10.188 min
Delta R.T.: 0.017 min
Response: 276432
Conc: 0.45 ng/ml

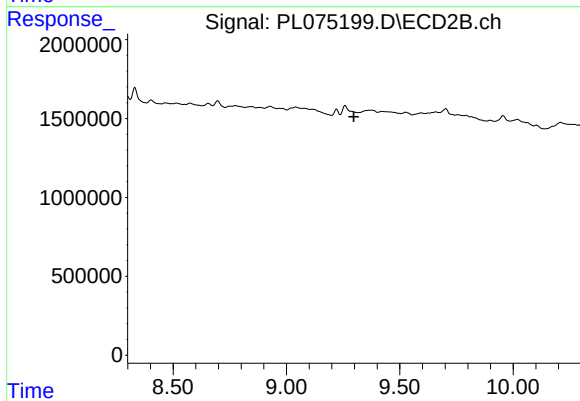

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 9.298 min
Response: 0
Conc: N.D.

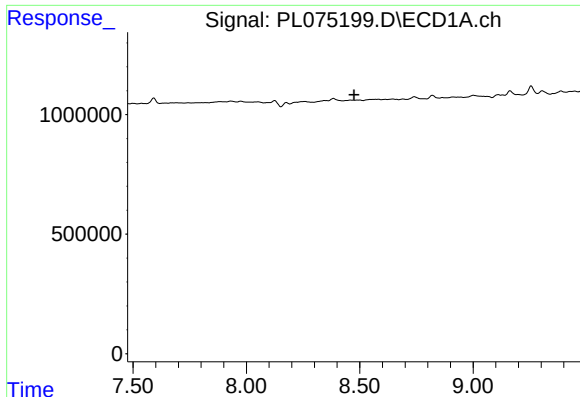

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 8.476 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

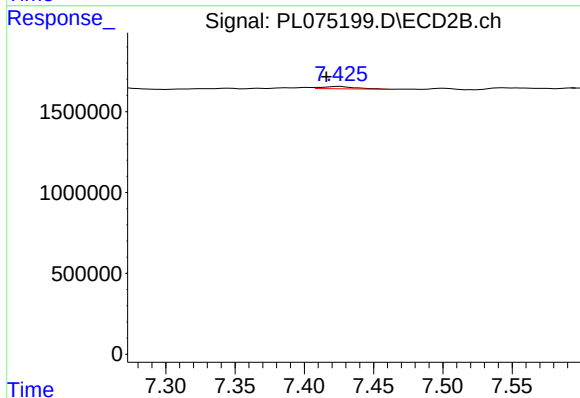


#26 Chlordane-4

R.T.: 7.426 min
Delta R.T.: 0.010 min
Response: 226750
Conc: 1.17 ng/ml

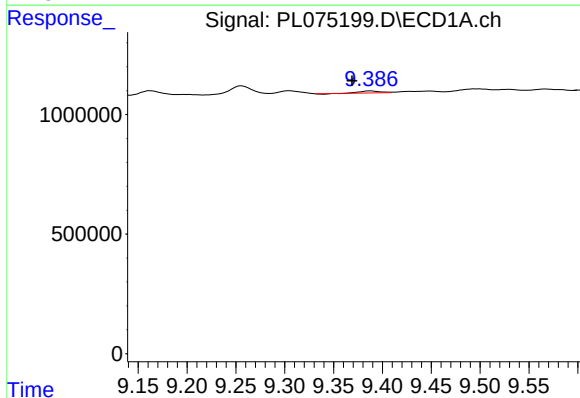


#27 Chlordane-5

R.T.: 9.388 min
Delta R.T.: 0.019 min
Response: 94342
Conc: 4.33 ng/ml

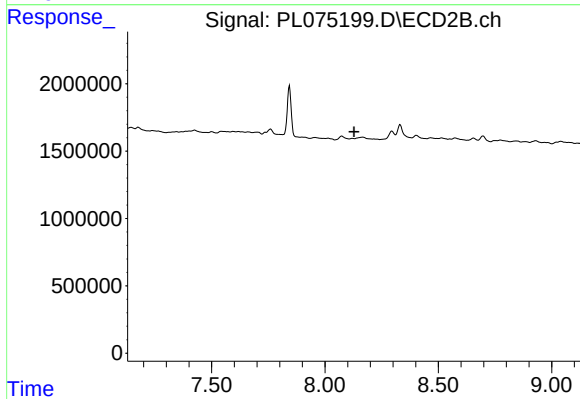

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 8.129 min
Response: 0
Conc: N.D.

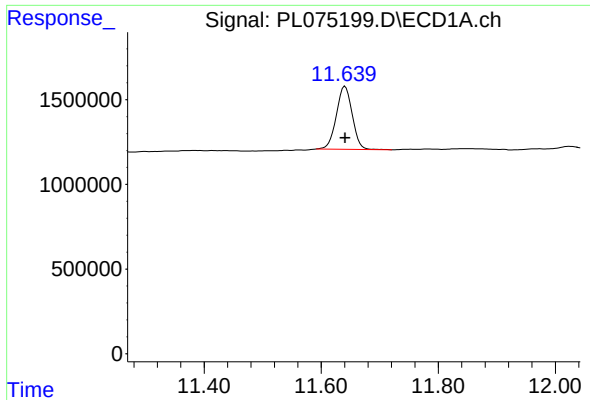

#28 Decachlorobiphenyl

R.T.: 11.641 min
Delta R.T.: 0.000 min
Response: 7026464
Conc: 13.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

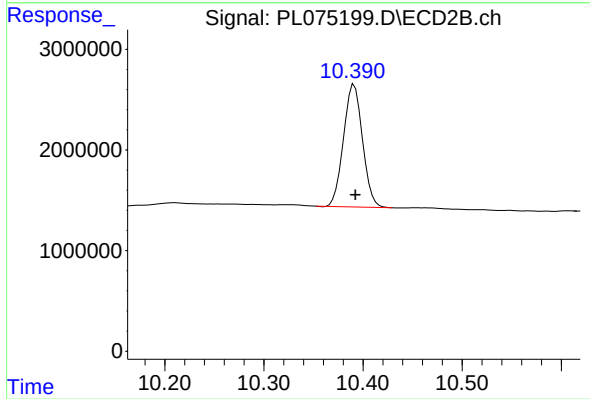

#28 Decachlorobiphenyl

R.T.: 10.391 min
Delta R.T.: -0.001 min
Response: 16219388
Conc: 11.82 ng/ml