

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052822\
 Data File : PL075204.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 May 2022 02:33
 Operator : AR\AJ
 Sample : N2921-02
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 03:02:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Tue May 31 02:52:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.641	4.642	4613895	13157311	7.850	8.306
28)	SA Decachlor...	11.639	10.391	7704207	17277857	14.369	12.591
Target Compounds							
7)	B delta-BHC	0.000	6.406	0	167886	N.D.	0.078 #
8)	B Heptachlo...	8.124	0.000	6233644	0	9.131	N.D. #
10)	B gamma-Chl...	8.364f	7.331f	552738	2681456	0.820	1.458 #
12)	B 4,4'-DDE	8.680f	0.000	920161	0	1.582	N.D. #
13)	MA Dieldrin	8.813	7.744f	5463428	1460902	8.621	0.842 #
14)	MA Endrin	9.056	8.068f	2458659	16054710	4.630	10.313 #
15)	B Endosulfa...	9.272f	8.359	5386379	5497578	9.543	3.492 #
16)	A 4,4'-DDD	9.203	0.000	19234903	0	38.892	N.D. #
17)	MA 4,4'-DDT	0.000	8.468	0	44811650	N.D.	31.334 #
19)	B Endosulfa...	0.000	8.779	0	38529368	N.D.	25.742 #
22)	Mirex	10.658	0.000	711341	0	1.467	N.D. #
25)	Chlordane-3	8.364f	7.331f	552738	2681456	5.631	14.703 #
27)	Chlordane-5	0.000	8.130	0	44520409	N.D.	864.176 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052822\
Data File : PL075204.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 May 2022 02:33
Operator : AR\AJ
Sample : N2921-02
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 03:02:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Tue May 31 02:52:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

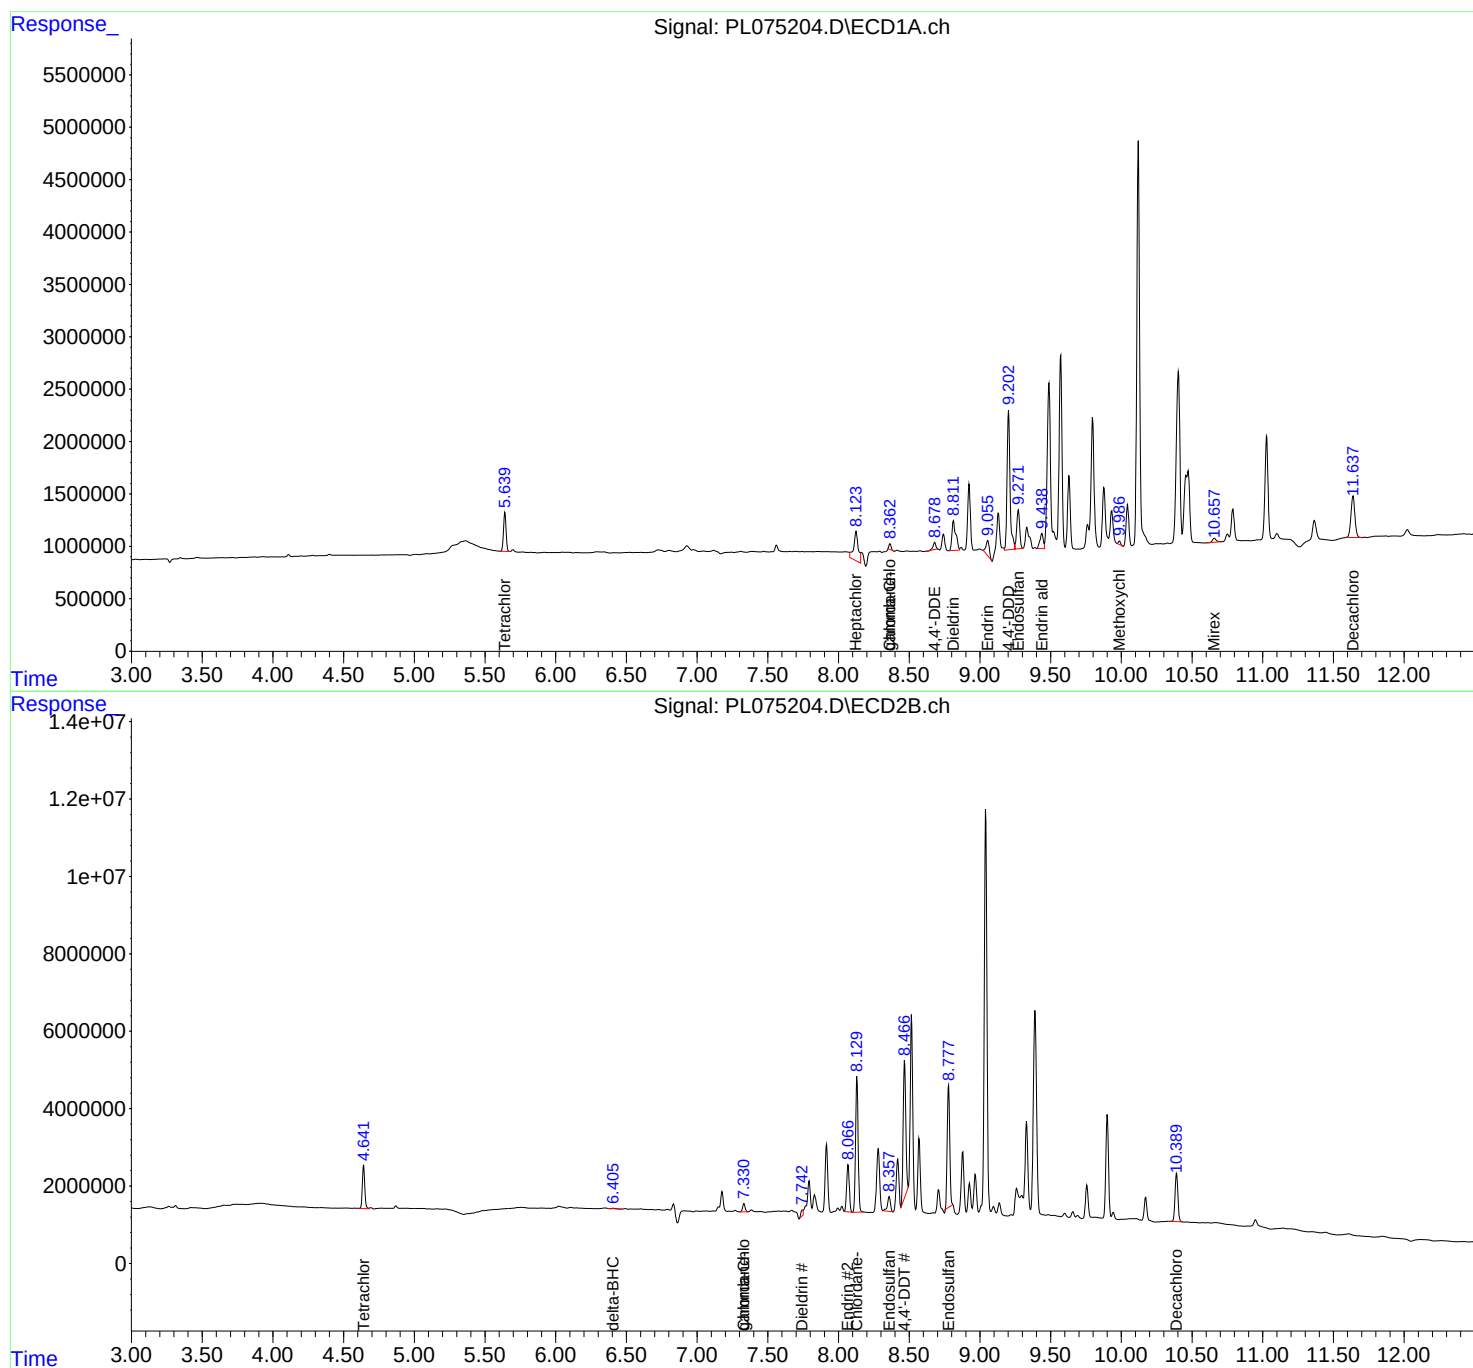


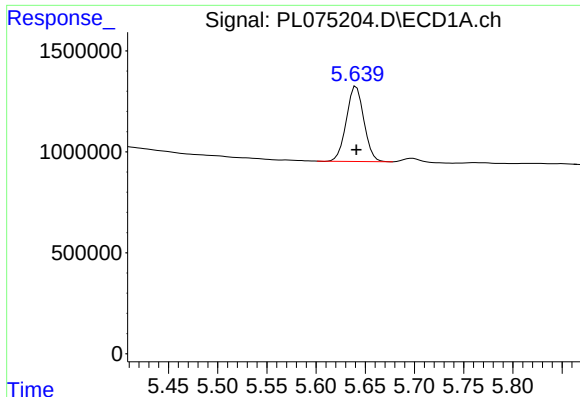

#1 Tetrachloro-m-xylene


R.T.: 5.641 min
Delta R.T.: 0.000 min
Response: 4613895
Conc: 7.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

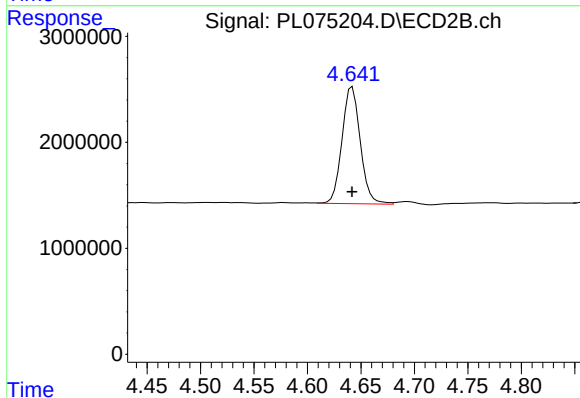


#1 Tetrachloro-m-xylene

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 13157311
Conc: 8.31 ng/ml

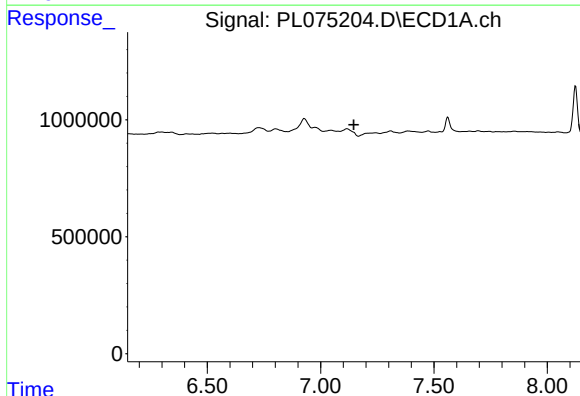


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

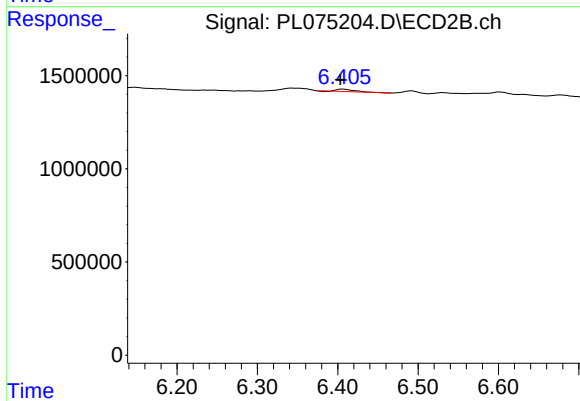

#7 delta-BHC


R.T.: 6.406 min
Delta R.T.: 0.003 min
Response: 167886
Conc: 0.08 ng/ml

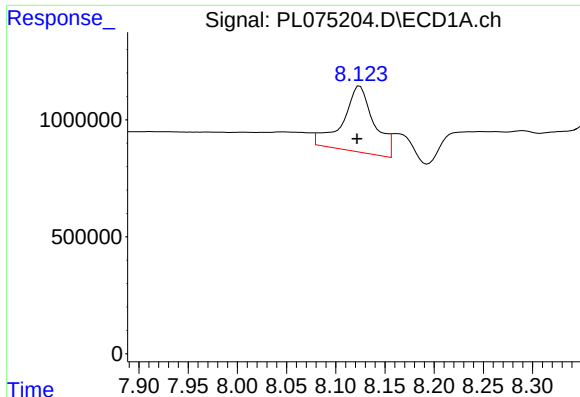

#8 Heptachlor epoxide


R.T.: 8.124 min
Delta R.T.: 0.003 min
Response: 6233644
Conc: 9.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

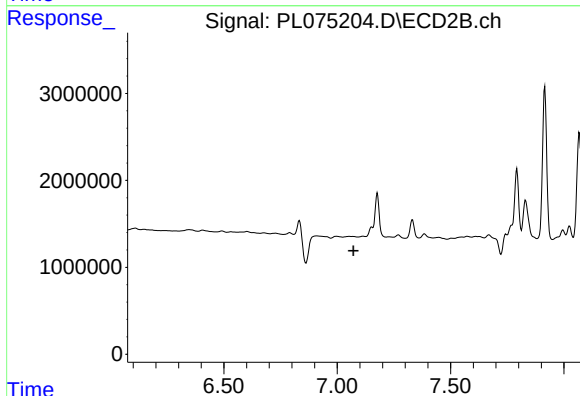


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.072 min
Response: 0
Conc: N.D.

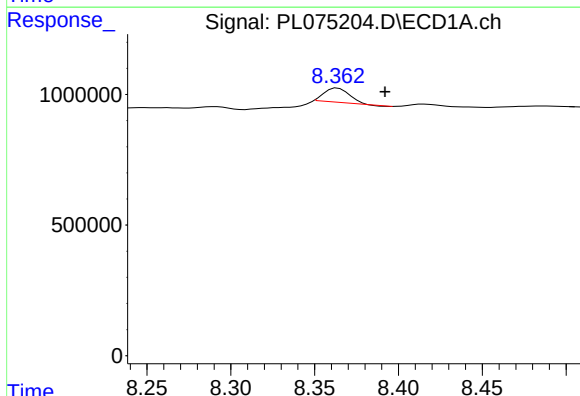


#10 gamma-Chlordane

R.T.: 8.364 min
Delta R.T.: -0.028 min
Response: 552738
Conc: 0.82 ng/ml

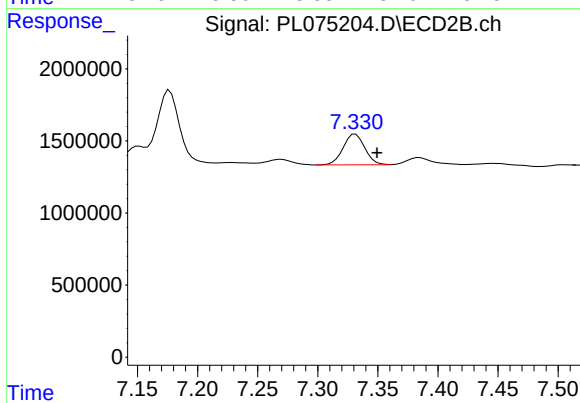

#10 gamma-Chlordane


R.T.: 7.331 min
Delta R.T.: -0.018 min
Response: 2681456
Conc: 1.46 ng/ml

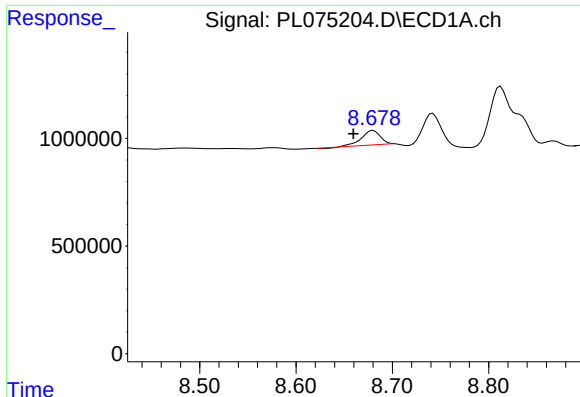

#12 4,4'-DDE


R.T.: 8.680 min
Delta R.T.: 0.020 min
Response: 920161
Conc: 1.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

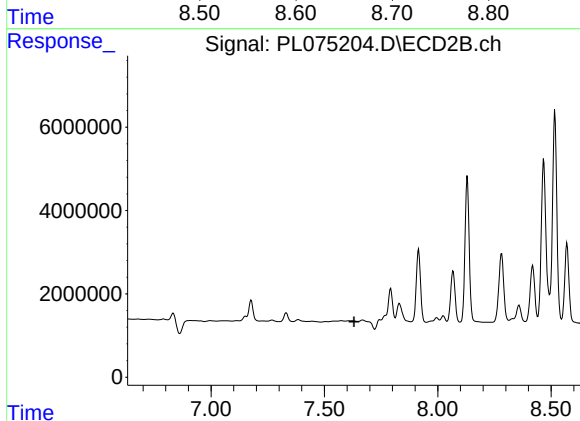


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 7.630 min
Response: 0
Conc: N.D.

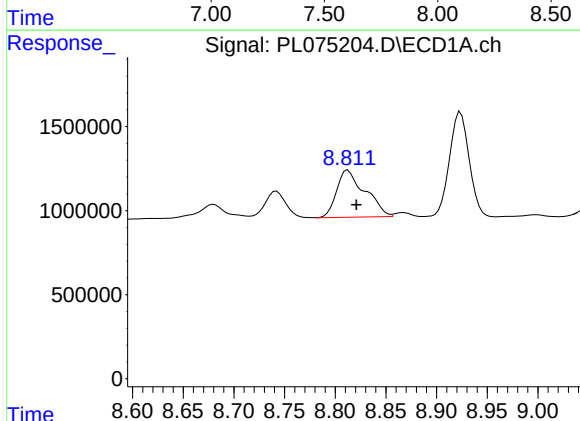


#13 Dieldrin

R.T.: 8.813 min
Delta R.T.: -0.008 min
Response: 5463428
Conc: 8.62 ng/ml

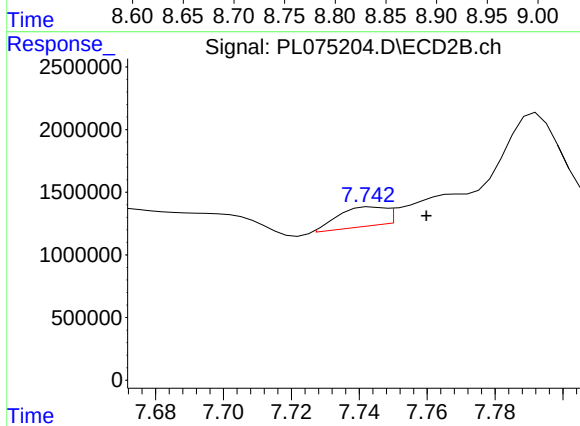

#13 Dieldrin


R.T.: 7.744 min
Delta R.T.: -0.016 min
Response: 1460902
Conc: 0.84 ng/ml

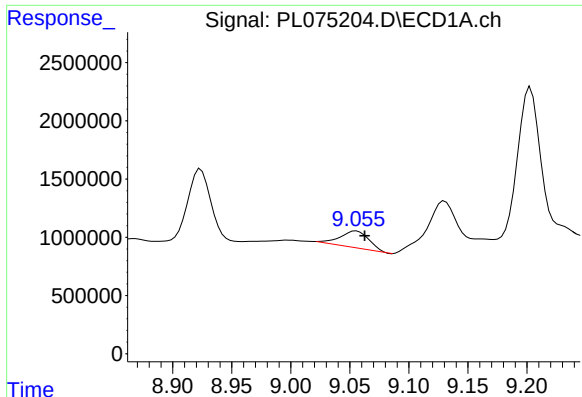

#14 Endrin


R.T.: 9.056 min
Delta R.T.: -0.007 min
Response: 2458659
Conc: 4.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

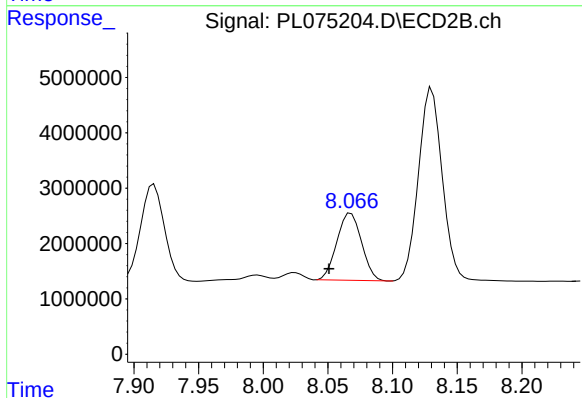


#14 Endrin

R.T.: 8.068 min
Delta R.T.: 0.017 min
Response: 16054710
Conc: 10.31 ng/ml

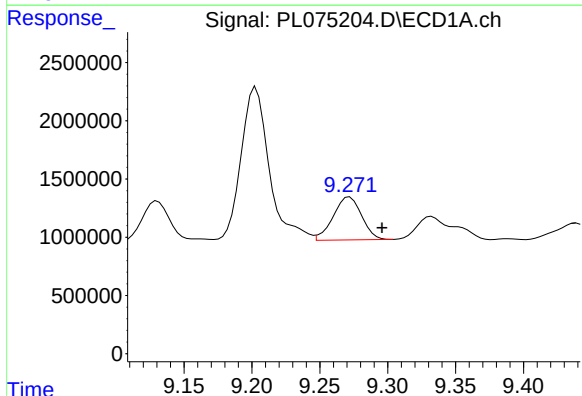


#15 Endosulfan II

R.T.: 9.272 min
Delta R.T.: -0.024 min
Response: 5386379
Conc: 9.54 ng/ml

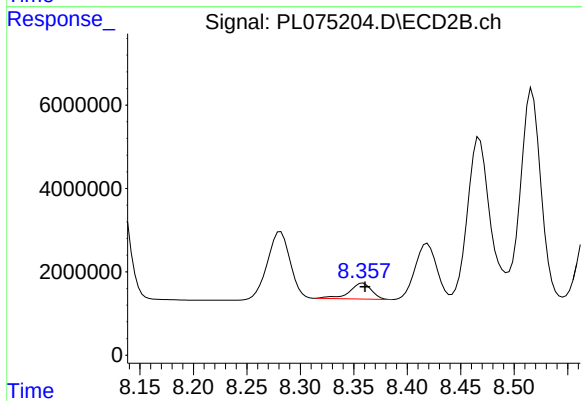

#15 Endosulfan II


R.T.: 8.359 min
Delta R.T.: -0.002 min
Response: 5497578
Conc: 3.49 ng/ml

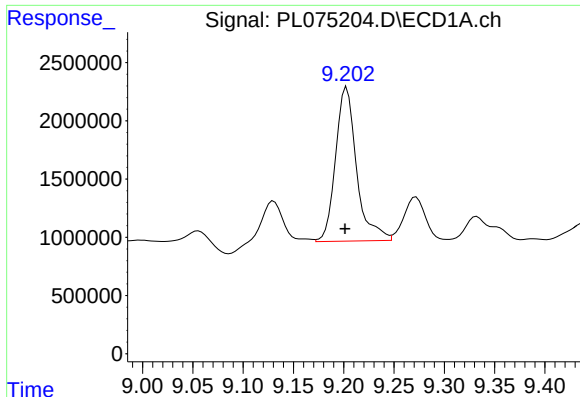

#16 4,4'-DDD


R.T.: 9.203 min
Delta R.T.: 0.002 min
Response: 19234903
Conc: 38.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

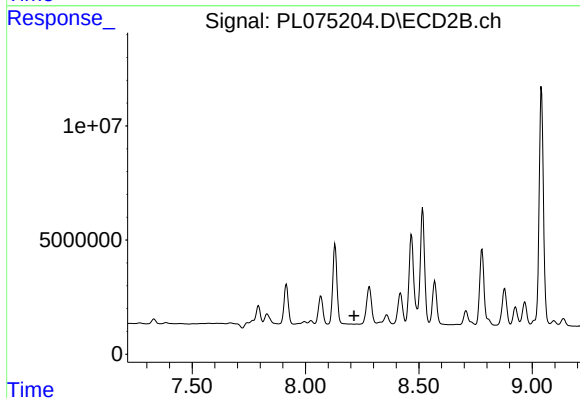


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.215 min
Response: 0
Conc: N.D.

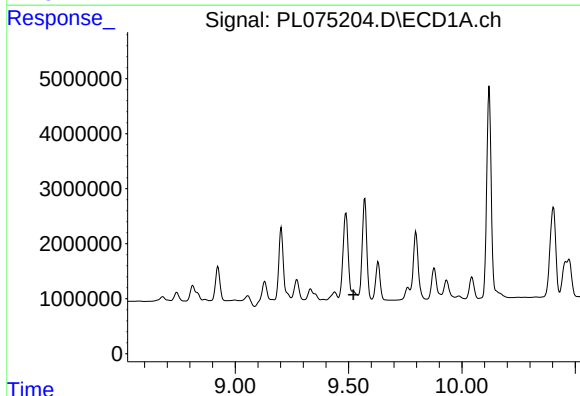


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.522 min
Response: 0
Conc: N.D.

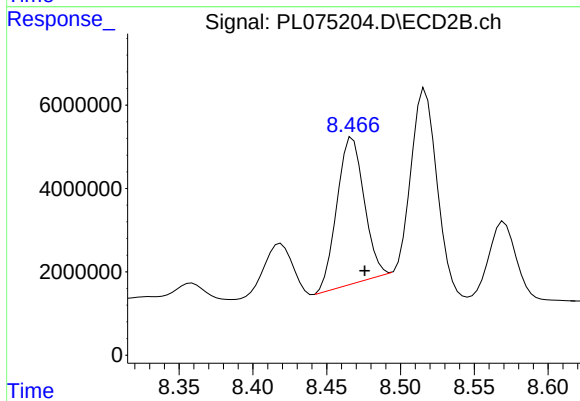

#17 4,4'-DDT


R.T.: 8.468 min
Delta R.T.: -0.008 min
Response: 44811650
Conc: 31.33 ng/ml

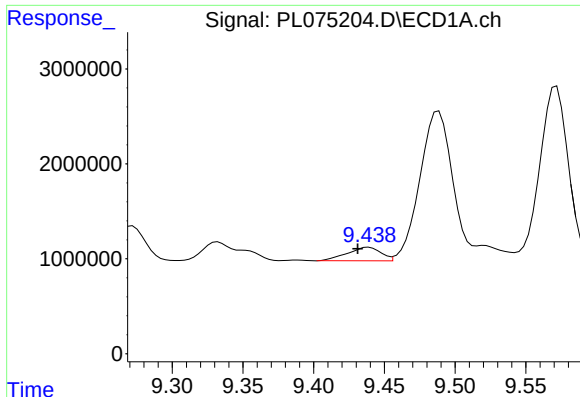

#18 Endrin aldehyde


R.T.: 9.439 min
Delta R.T.: 0.008 min
Response: 2357607
Conc: 5.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

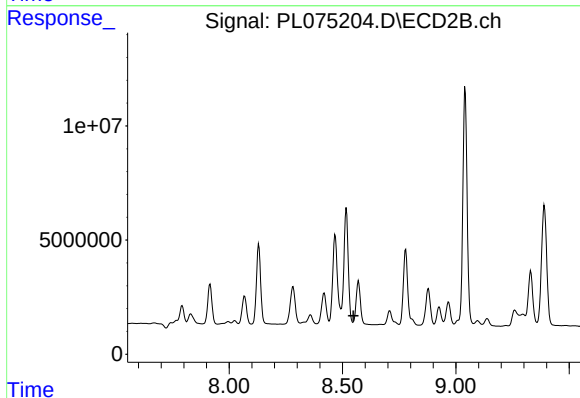


#18 Endrin aldehyde

R.T.: 8.570 min
Delta R.T.: 0.022 min
Response: -33769565
Conc: N.D.

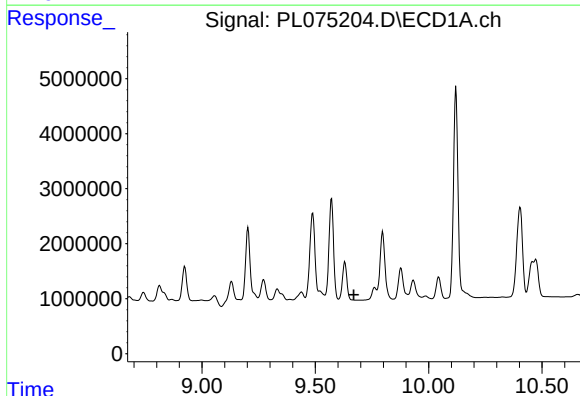


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 9.669 min
Response: 0
Conc: N.D.

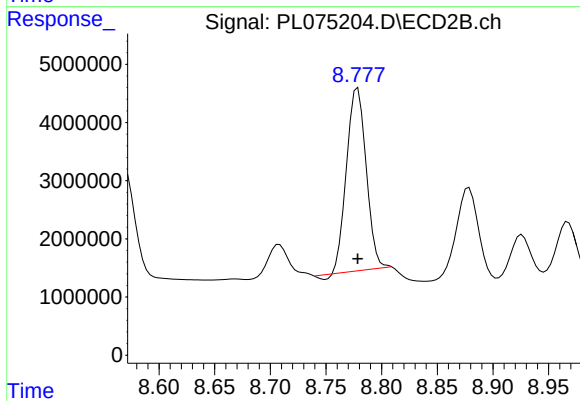

#19 Endosulfan Sulfate


R.T.: 8.779 min
Delta R.T.: 0.000 min
Response: 38529368
Conc: 25.74 ng/ml

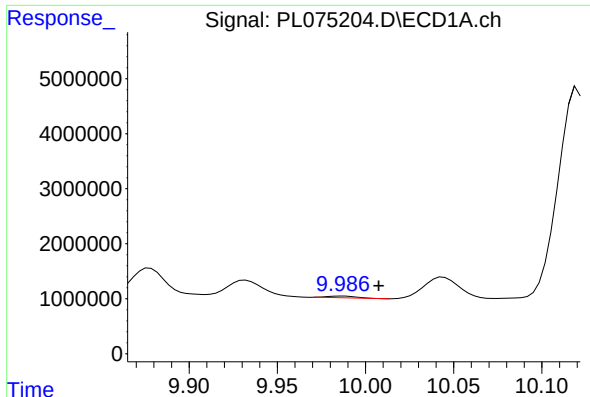

#20 Methoxychlor


R.T.: 9.987 min
Delta R.T.: -0.020 min
Response: 357369
Conc: 1.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

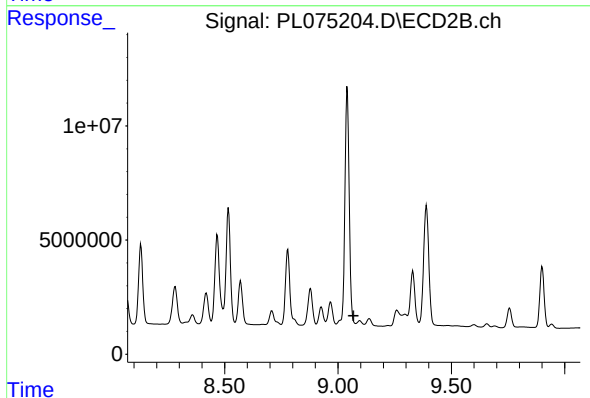


#20 Methoxychlor

R.T.: 9.096 min
Delta R.T.: 0.027 min
Response: -4816917
Conc: N.D.

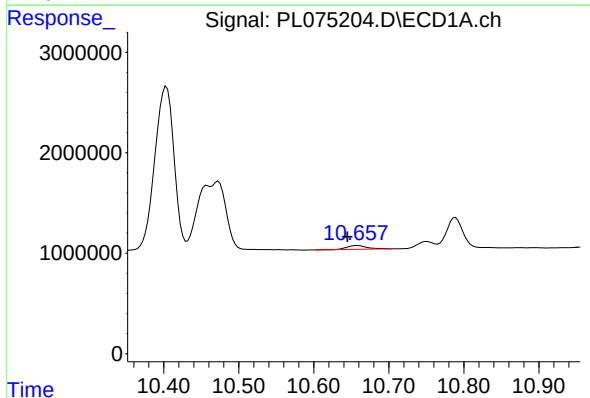


#22 Mirex

R.T.: 10.658 min
Delta R.T.: 0.013 min
Response: 711341
Conc: 1.47 ng/ml

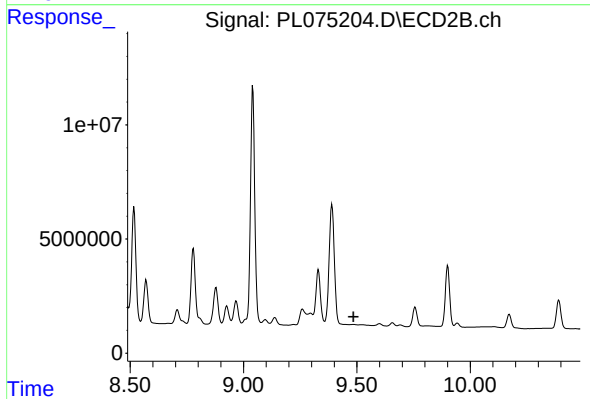

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 9.485 min
Response: 0
Conc: N.D.

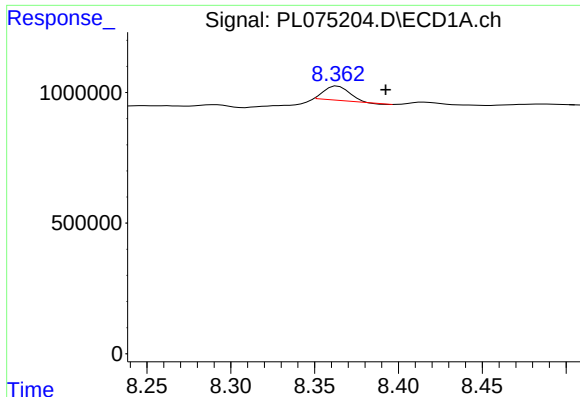

#25 Chlordane-3


R.T.: 8.364 min
Delta R.T.: -0.029 min
Response: 552738
Conc: 5.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

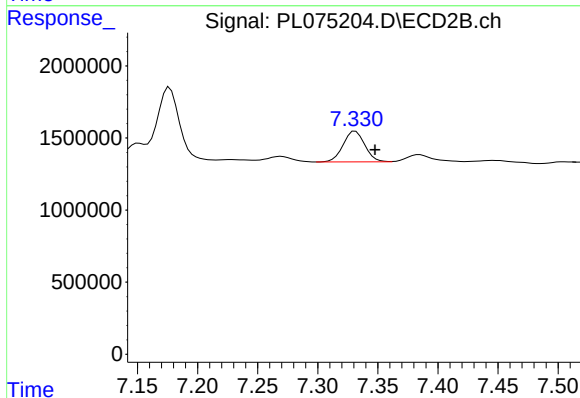


#25 Chlordane-3

R.T.: 7.331 min
Delta R.T.: -0.016 min
Response: 2681456
Conc: 14.70 ng/ml

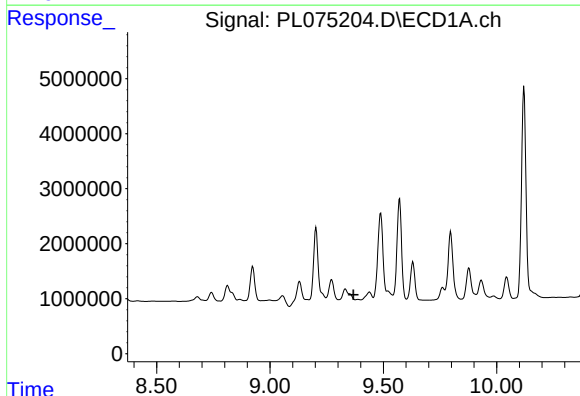


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.369 min
Response: 0
Conc: N.D.

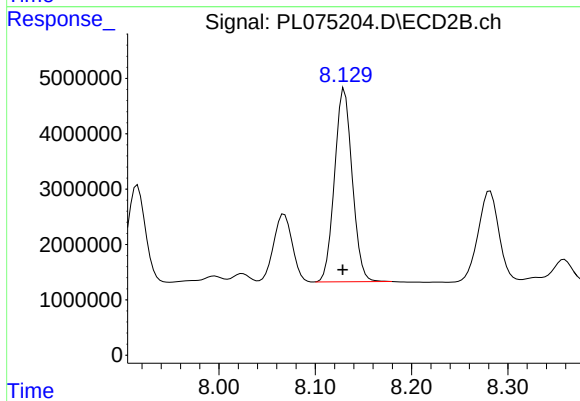

#27 Chlordane-5


R.T.: 8.130 min
Delta R.T.: 0.002 min
Response: 44520409
Conc: 864.18 ng/ml

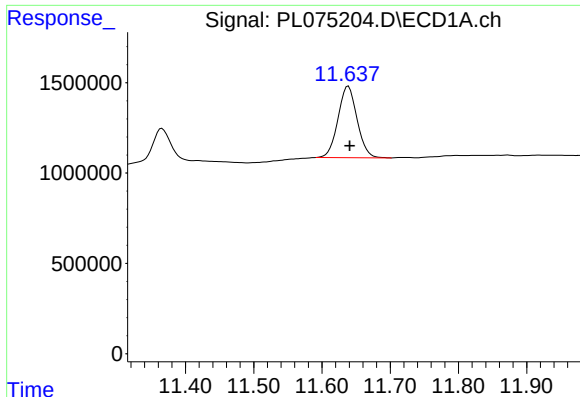

#28 Decachlorobiphenyl

R.T.: 11.639 min
Delta R.T.: -0.002 min
Response: 7704207
Conc: 14.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

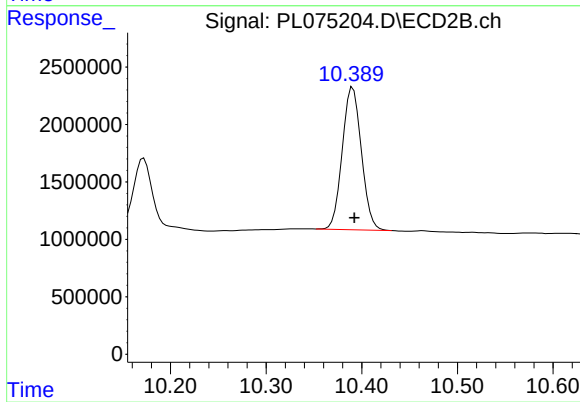

#28 Decachlorobiphenyl

R.T.: 10.391 min
Delta R.T.: -0.002 min
Response: 17277857
Conc: 12.59 ng/ml