

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL052822\  
 Data File : PL075216.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 29 May 2022 05:51  
 Operator : AR\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 31 03:07:17 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL052822.M  
 Quant Title : GC Extractables  
 QLast Update : Tue May 31 02:52:42 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

|                             | Compound        | RT#1    | RT#2   | Resp#1   | Resp#2   | ng/ml  | ng/ml   |
|-----------------------------|-----------------|---------|--------|----------|----------|--------|---------|
| -----                       |                 |         |        |          |          |        |         |
| System Monitoring Compounds |                 |         |        |          |          |        |         |
| 1)                          | SA Tetrachlo... | 5.641   | 4.642  | 12207560 | 31554787 | 20.770 | 19.919  |
| 28)                         | SA Decachlor... | 11.642  | 10.392 | 10973075 | 24445226 | 20.465 | 17.814  |
| Target Compounds            |                 |         |        |          |          |        |         |
| 8)                          | B Heptachlo...  | 8.126   | 0.000  | 1980623  | 0        | 2.901  | N.D. #  |
| 13)                         | MA Dieldrin     | 0.000   | 7.766  | 0        | 1456489  | N.D.   | 0.839 # |
| 14)                         | MA Endrin       | 0.000   | 8.073f | 0        | 818098   | N.D.   | 0.526 # |
| 15)                         | B Endosulfa...  | 9.305   | 0.000  | 70830    | 0        | 0.125  | N.D. #  |
| 21)                         | B Endrin ke...  | 10.188f | 0.000  | 273324   | 0        | 0.445  | N.D. #  |
| 27)                         | Chlordane-5     | 0.000   | 8.132  | 0        | 87168    | N.D.   | 1.692 # |
| -----                       |                 |         |        |          |          |        |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL052822\  
Data File : PL075216.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 29 May 2022 05:51  
Operator : AR\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: May 31 03:07:17 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL052822.M  
Quant Title : GC Extractables  
QLast Update : Tue May 31 02:52:42 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

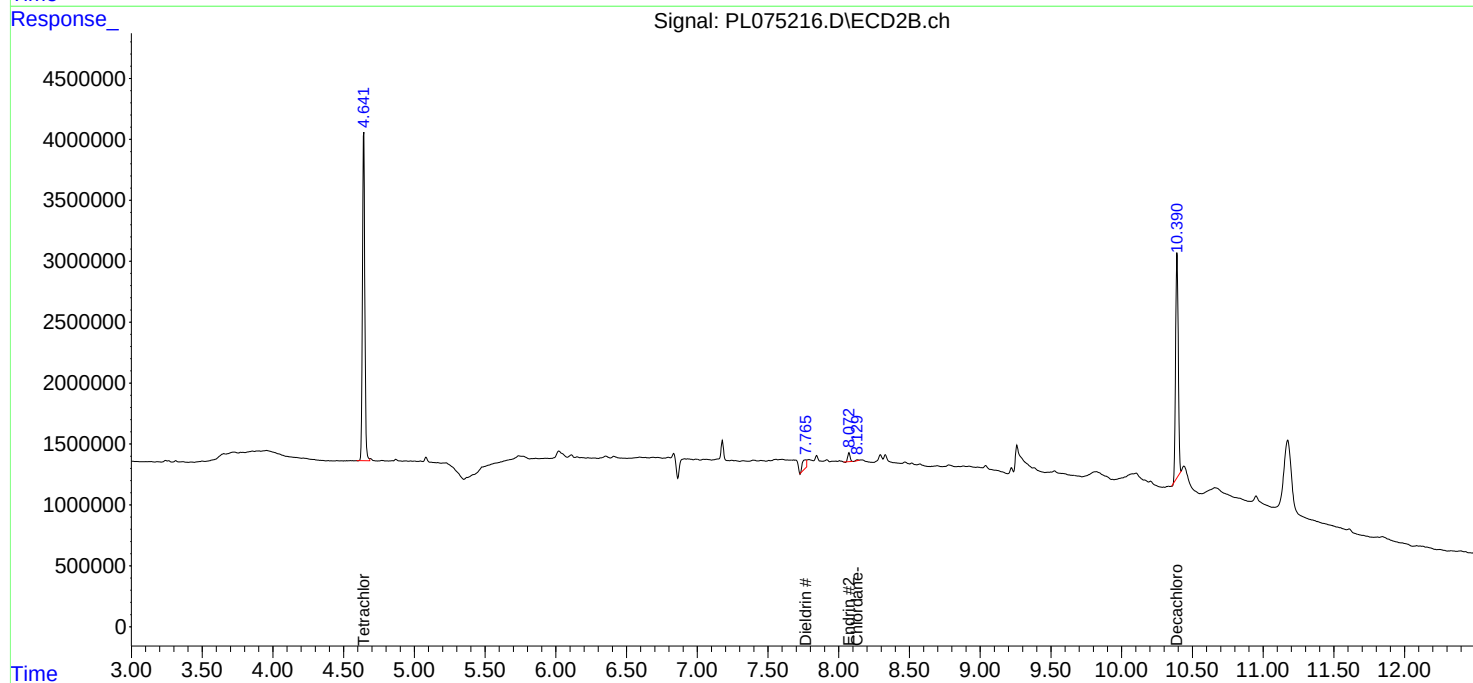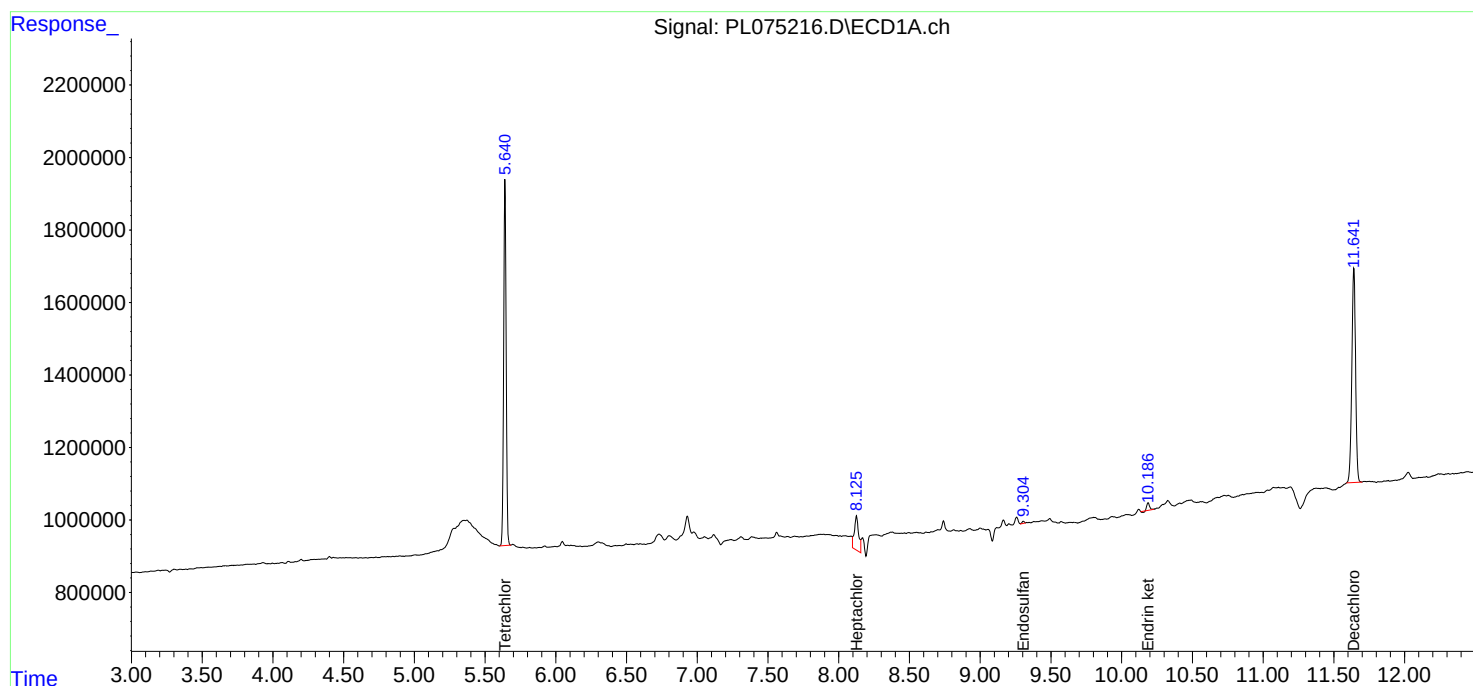


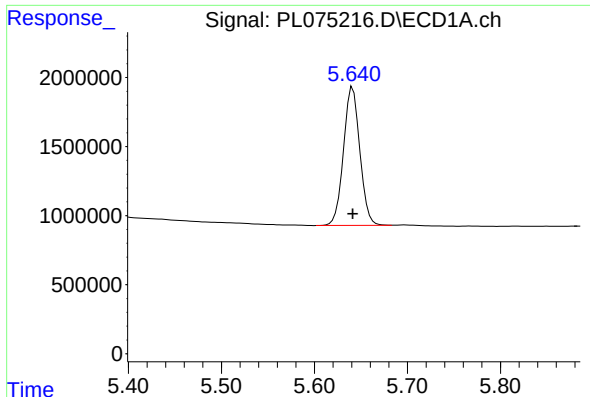

#1 Tetrachloro-m-xylene


R.T.: 5.641 min  
Delta R.T.: 0.000 min  
Response: 12207560  
Conc: 20.77 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

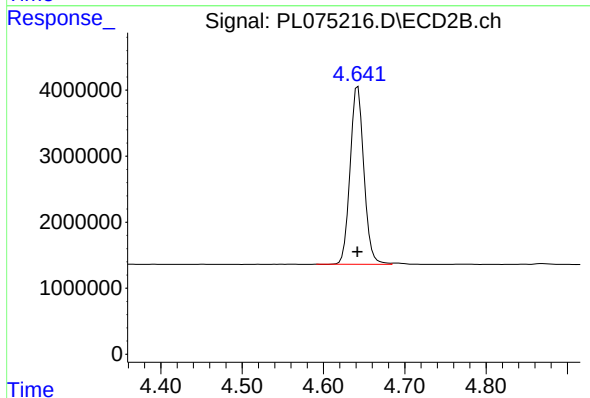


#1 Tetrachloro-m-xylene

R.T.: 4.642 min  
Delta R.T.: 0.000 min  
Response: 31554787  
Conc: 19.92 ng/ml

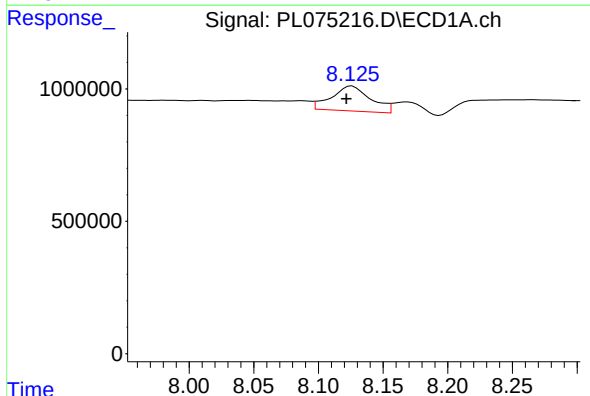


#8 Heptachlor epoxide

R.T.: 8.126 min  
Delta R.T.: 0.004 min  
Response: 1980623  
Conc: 2.90 ng/ml

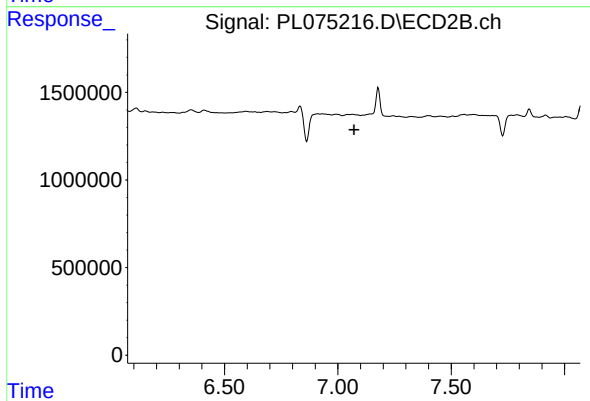

#8 Heptachlor epoxide


R.T.: 0.000 min  
Exp R.T.: 7.072 min  
Response: 0  
Conc: N.D.

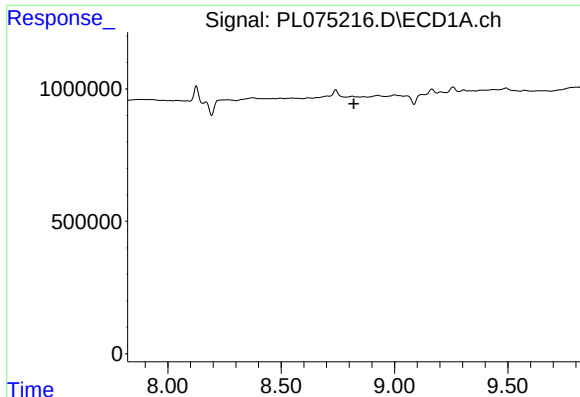

#13 Dieldrin


R.T.: 0.000 min  
Exp R.T.: 8.821 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :

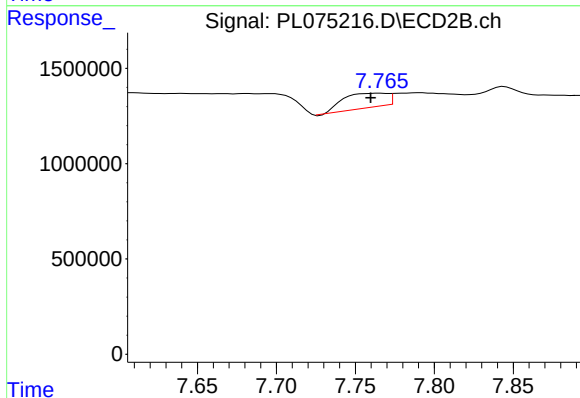


#13 Dieldrin

R.T.: 7.766 min  
Delta R.T.: 0.006 min  
Response: 1456489  
Conc: 0.84 ng/ml

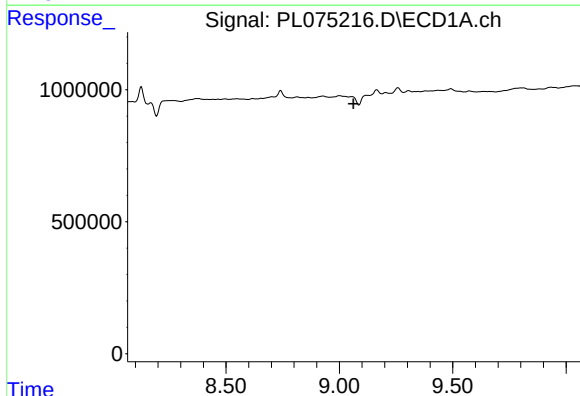


#14 Endrin

R.T.: 0.000 min  
Exp R.T.: 9.062 min  
Response: 0  
Conc: N.D.

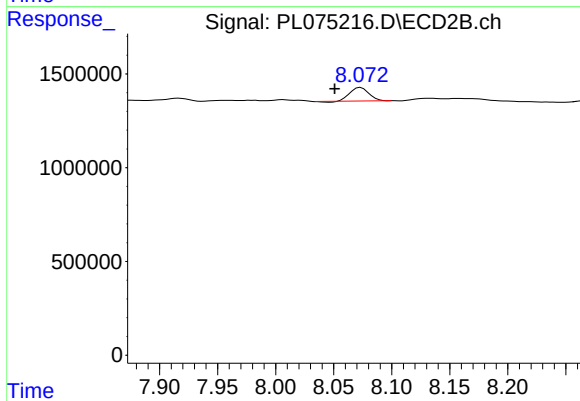

#14 Endrin


R.T.: 8.073 min  
Delta R.T.: 0.022 min  
Response: 818098  
Conc: 0.53 ng/ml

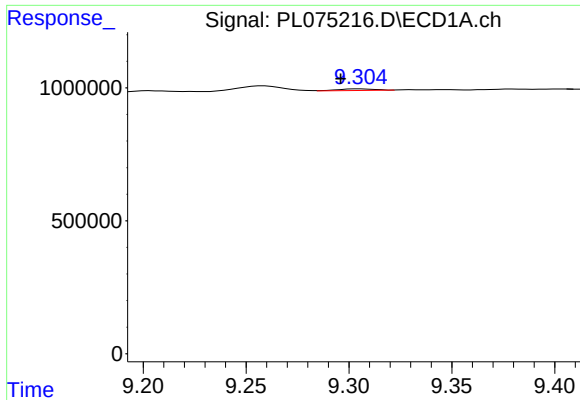

#15 Endosulfan II


R.T.: 9.305 min  
Delta R.T.: 0.009 min  
Response: 70830  
Conc: 0.13 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

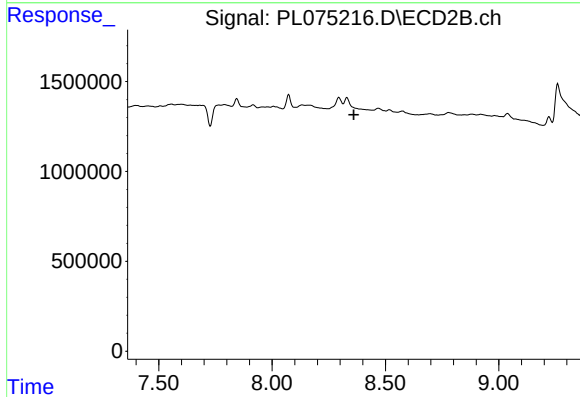


#15 Endosulfan II

R.T.: 0.000 min  
Exp R.T. : 8.361 min  
Response: 0  
Conc: N.D.

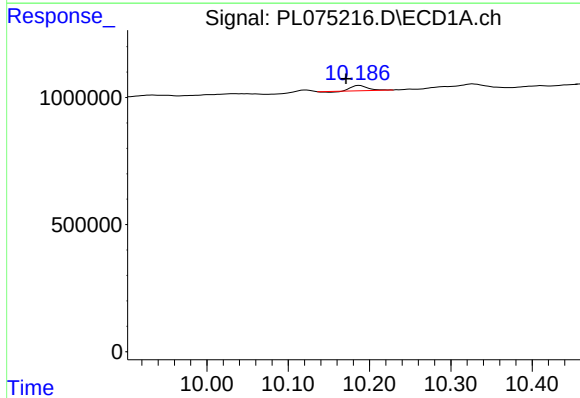


#21 Endrin ketone

R.T.: 10.188 min  
Delta R.T.: 0.016 min  
Response: 273324  
Conc: 0.45 ng/ml

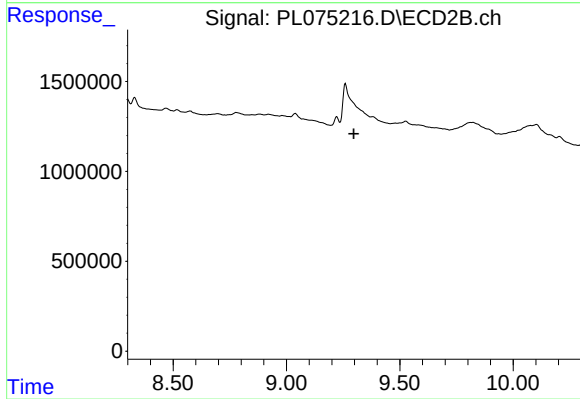

#21 Endrin ketone


R.T.: 0.000 min  
Exp R.T. : 9.298 min  
Response: 0  
Conc: N.D.

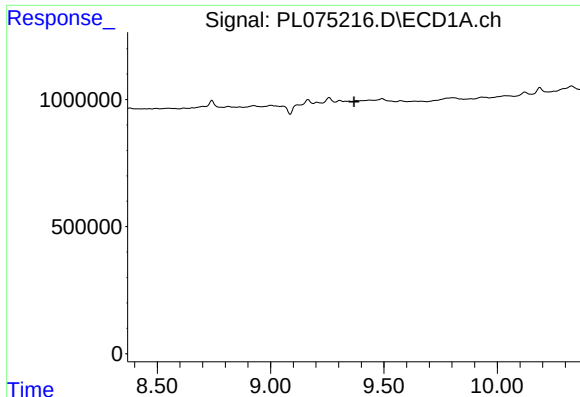

#27 Chlorine-5


R.T.: 0.000 min  
Exp R.T.: 9.369 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :

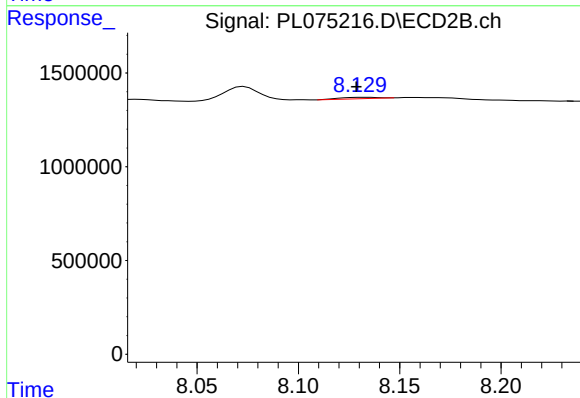


#27 Chlorine-5

R.T.: 8.132 min  
Delta R.T.: 0.004 min  
Response: 87168  
Conc: 1.69 ng/ml

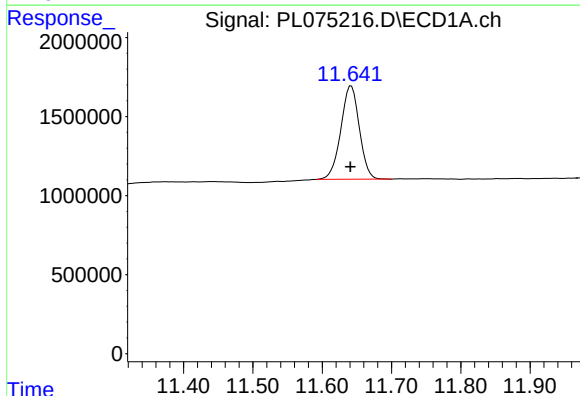

#28 Decachlorobiphenyl

R.T.: 11.642 min  
Delta R.T.: 0.000 min  
Response: 10973075  
Conc: 20.47 ng/ml

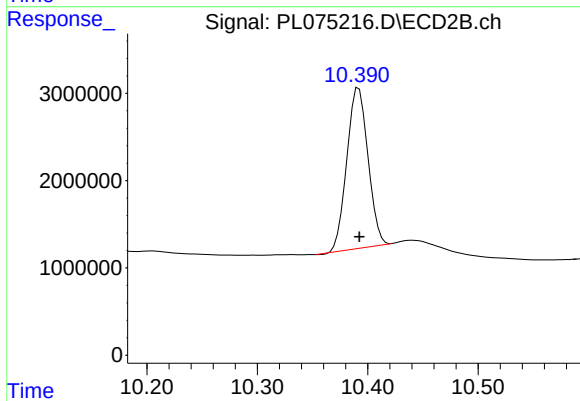

#28 Decachlorobiphenyl

R.T.: 10.392 min  
Delta R.T.: 0.000 min  
Response: 24445226  
Conc: 17.81 ng/ml