

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053022\
 Data File : PL075222.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 May 2022 02:39
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 03:13:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Tue May 31 02:52:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.644	4.642	13105732	33287104	22.299	21.013
28)	SA Decachlor...	11.640	10.392	10658944	24703626	19.879	18.002
Target Compounds							
5)	MB Aldrin	7.638f	0.000	599058	0	0.822	N.D. #
7)	B delta-BHC	0.000	6.407	0	85854	N.D.	0.040 #
8)	B Heptachlo...	8.127	0.000	1476560	0	2.163	N.D. #
13)	MA Dieldrin	0.000	7.781f	0	2823536	N.D.	1.627 #
14)	MA Endrin	0.000	8.074f	0	1285598	N.D.	0.826 #
15)	B Endosulfa...	9.306	0.000	122411	0	0.217	N.D. #
21)	B Endrin ke...	10.187f	0.000	333078	0	0.543	N.D. #
22)	Mirex	10.674f	0.000	455323	0	0.939	N.D. #
24)	Chlordane-2	7.638	0.000	599058	0	20.459	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053022\
Data File : PL075222.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 May 2022 02:39
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 03:13:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Tue May 31 02:52:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

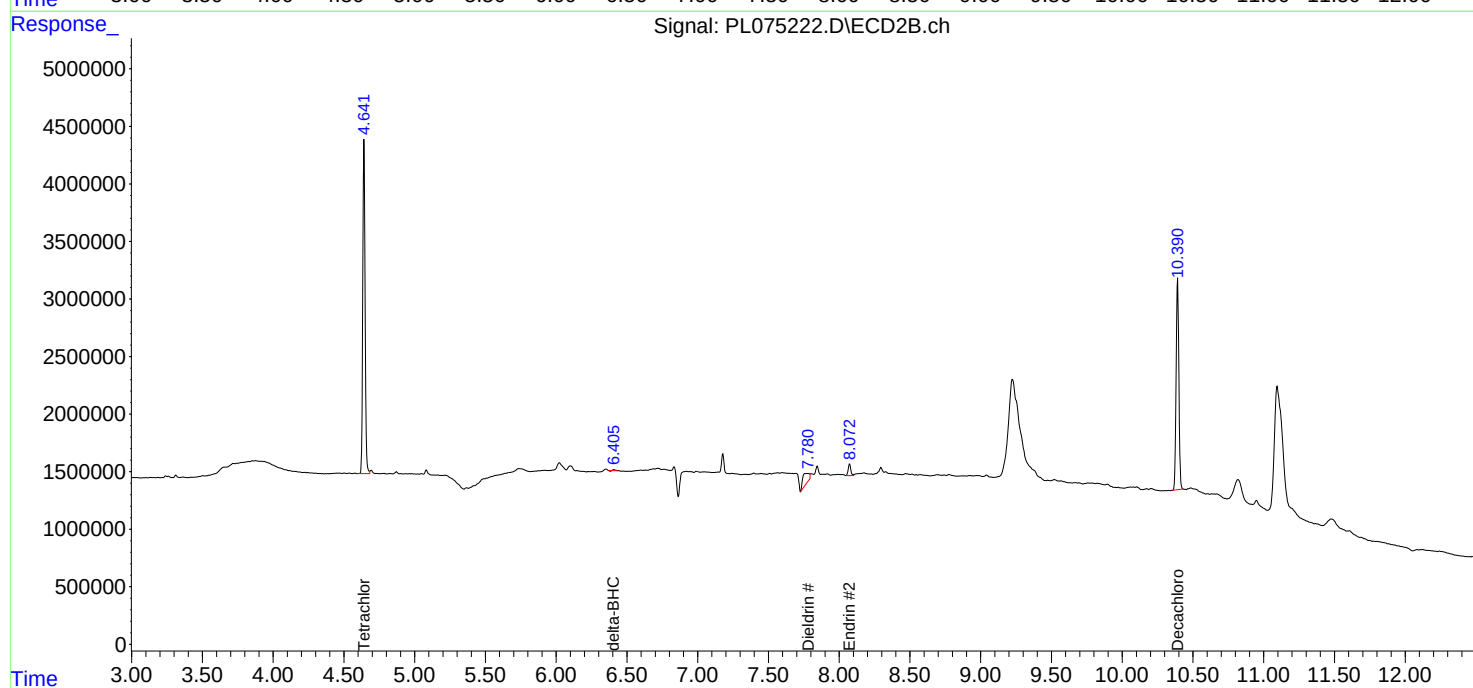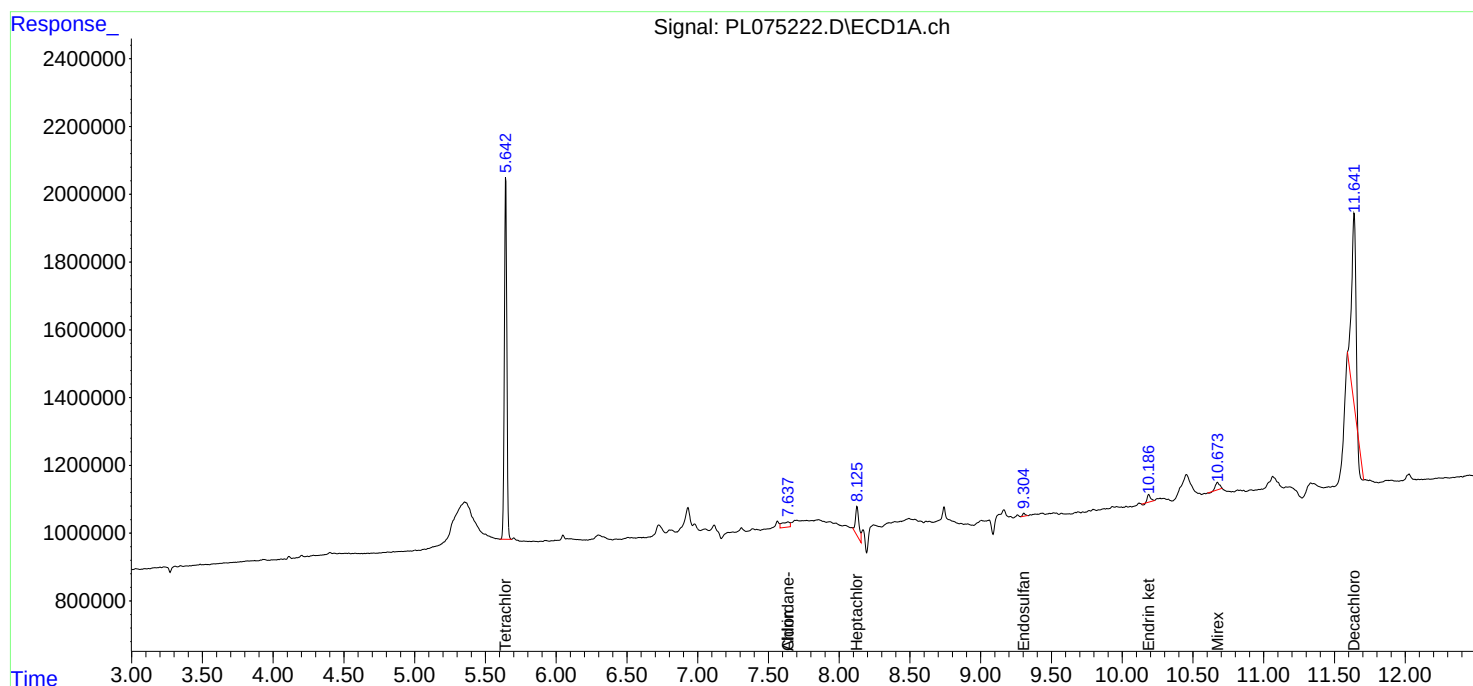


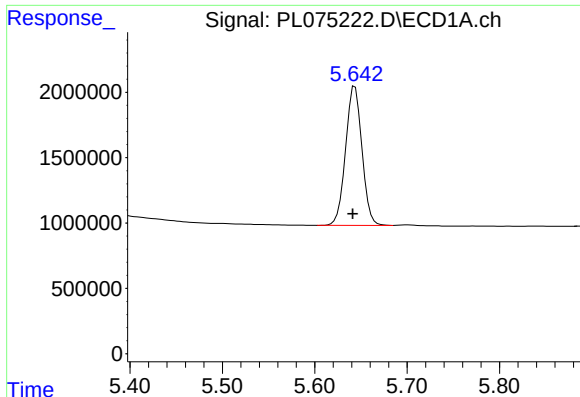

#1 Tetrachloro-m-xylene


R.T.: 5.644 min
Delta R.T.: 0.003 min
Response: 13105732
Conc: 22.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

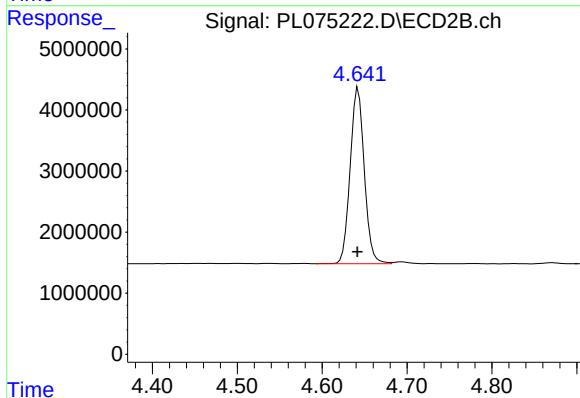


#1 Tetrachloro-m-xylene

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 33287104
Conc: 21.01 ng/ml

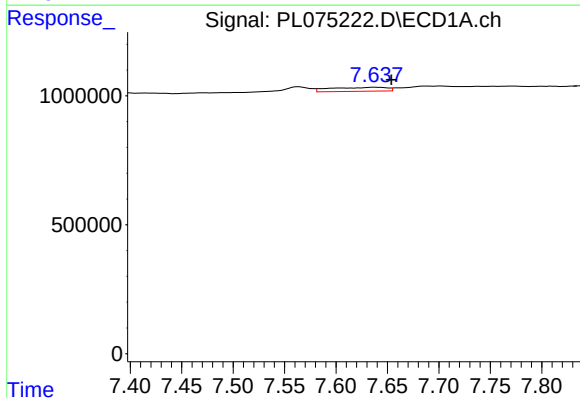


#5 Aldrin

R.T.: 7.638 min
Delta R.T.: -0.015 min
Response: 599058
Conc: 0.82 ng/ml

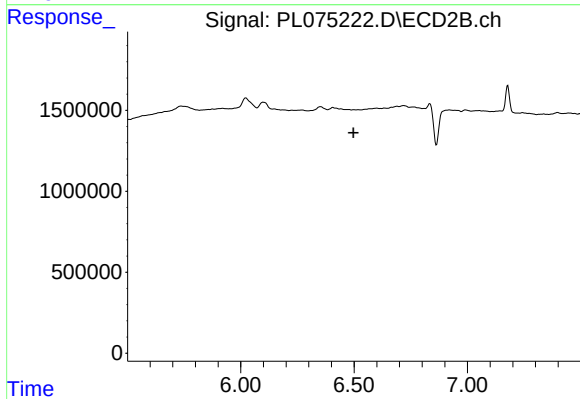

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 6.498 min
Response: 0
Conc: N.D.

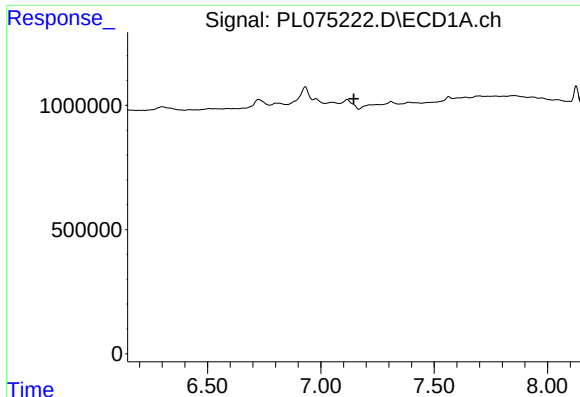

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 7.146 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

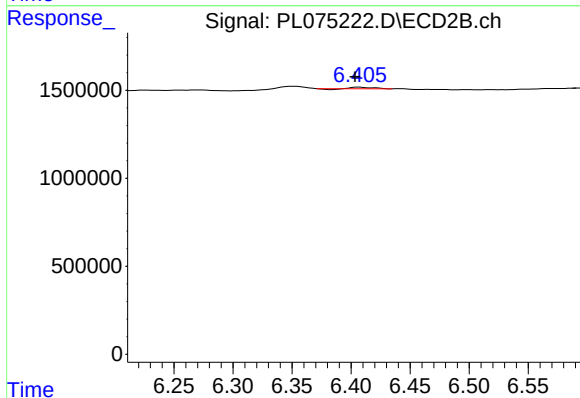


#7 delta-BHC

R.T.: 6.407 min
Delta R.T.: 0.003 min
Response: 85854
Conc: 0.04 ng/ml

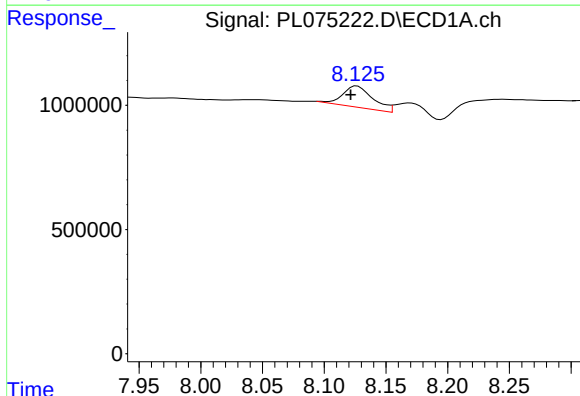


#8 Heptachlor epoxide

R.T.: 8.127 min
Delta R.T.: 0.005 min
Response: 1476560
Conc: 2.16 ng/ml

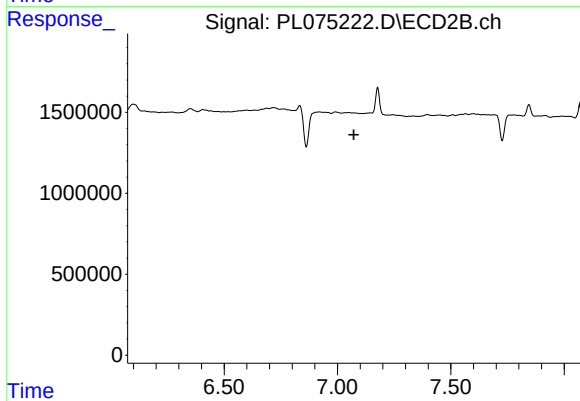

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 7.072 min
Response: 0
Conc: N.D.

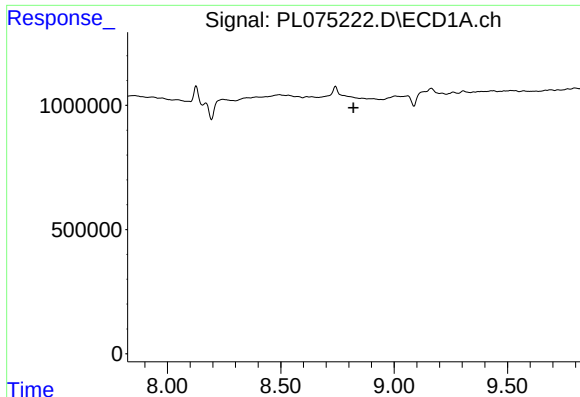

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.821 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

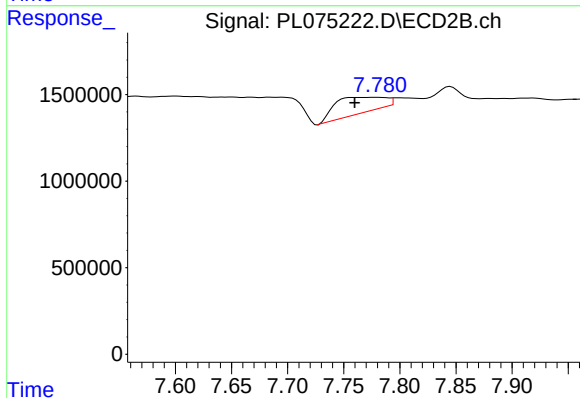


#13 Dieldrin

R.T.: 7.781 min
Delta R.T.: 0.021 min
Response: 2823536
Conc: 1.63 ng/ml

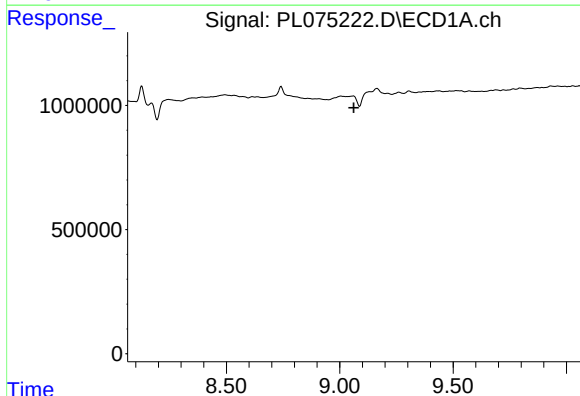


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

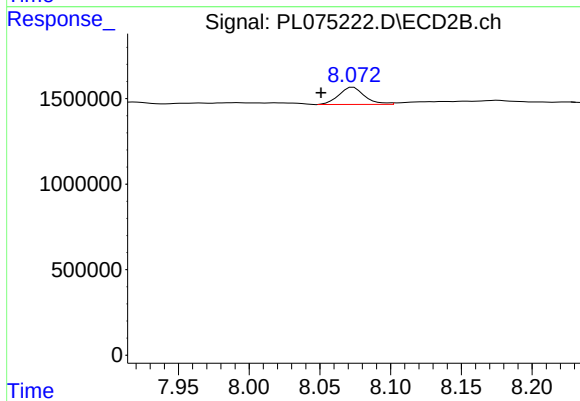

#14 Endrin


R.T.: 8.074 min
Delta R.T.: 0.023 min
Response: 1285598
Conc: 0.83 ng/ml

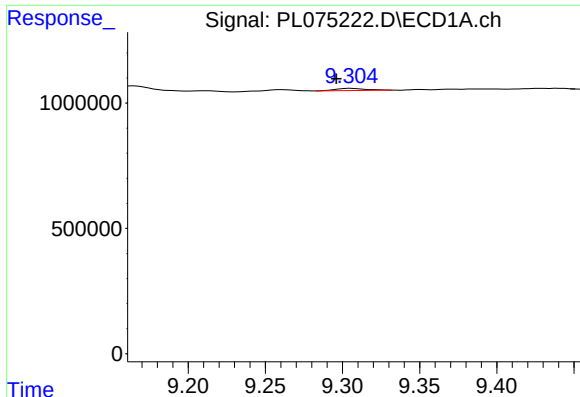

#15 Endosulfan II


R.T.: 9.306 min
Delta R.T.: 0.010 min
Response: 122411
Conc: 0.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

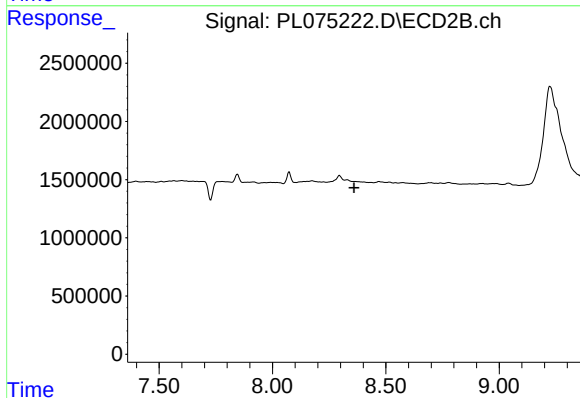


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.361 min
Response: 0
Conc: N.D.

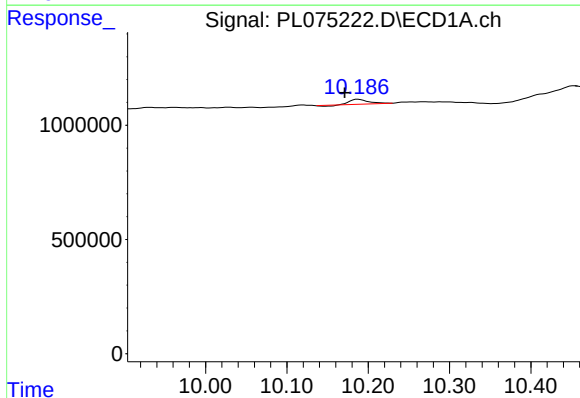


#21 Endrin ketone

R.T.: 10.187 min
Delta R.T.: 0.016 min
Response: 333078
Conc: 0.54 ng/ml

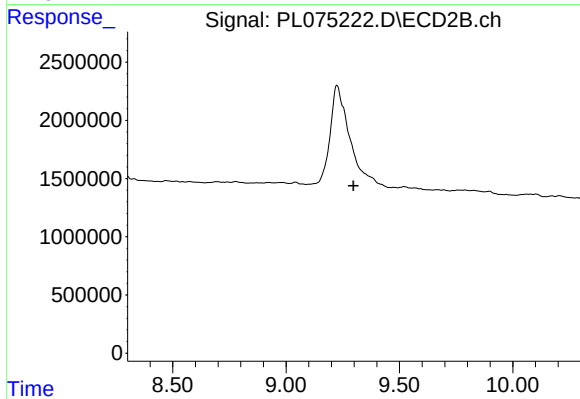

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 9.298 min
Response: 0
Conc: N.D.

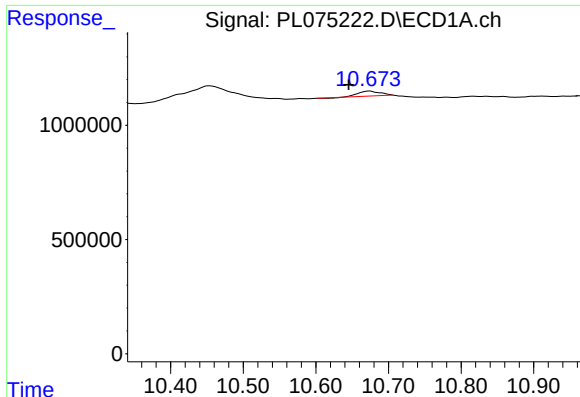

#22 Mirex


R.T.: 10.674 min
Delta R.T.: 0.029 min
Response: 455323
Conc: 0.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

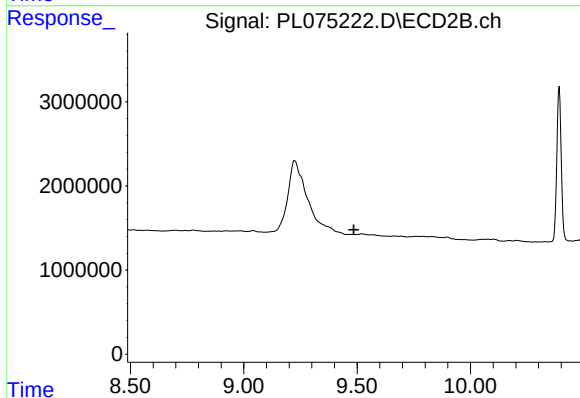


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 9.485 min
Response: 0
Conc: N.D.

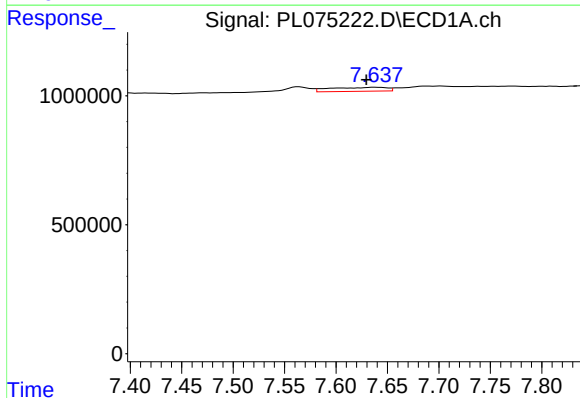


#24 Chlordane-2

R.T.: 7.638 min
Delta R.T.: 0.009 min
Response: 599058
Conc: 20.46 ng/ml

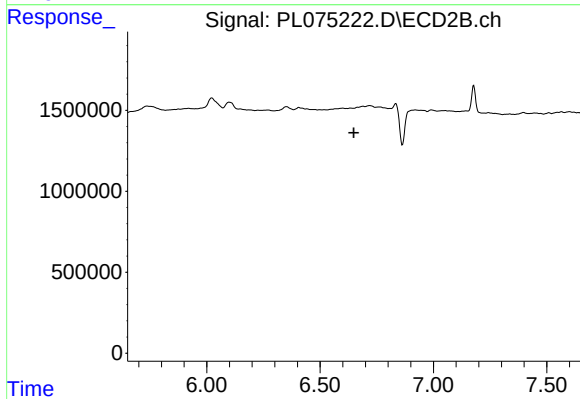

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 6.649 min
Response: 0
Conc: N.D.

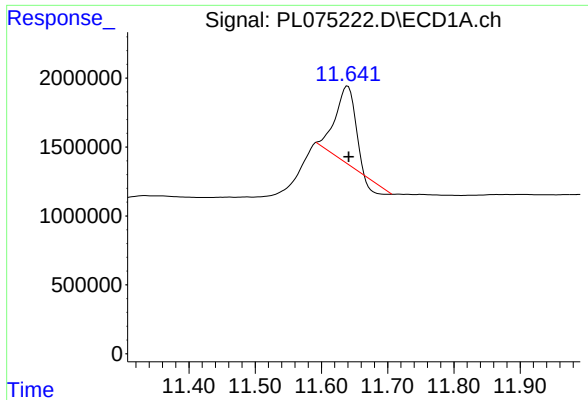

#28 Decachlorobiphenyl

R.T.: 11.640 min
Delta R.T.: -0.001 min
Response: 10658944
Conc: 19.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

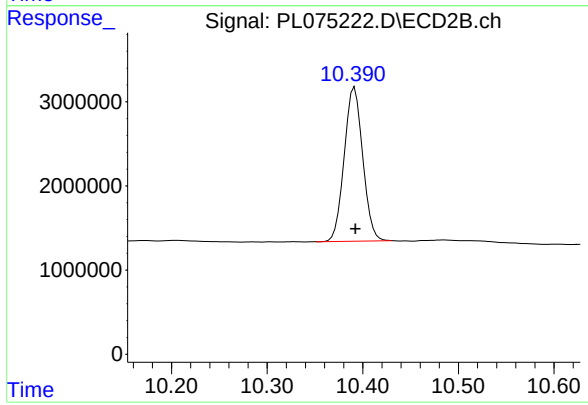

#28 Decachlorobiphenyl

R.T.: 10.392 min
Delta R.T.: 0.000 min
Response: 24703626
Conc: 18.00 ng/ml