

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053022\
 Data File : PL075247.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 May 2022 11:52
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 03:20:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
 Quant Title : GC Extractables
 QLast Update : Tue May 31 02:52:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.641	4.641	13394117	34072222	22.789	21.508
28)	SA Decachlor...	11.638	10.390	12456085	28890688	23.231	21.053
Target Compounds							
7)	B delta-BHC	0.000	6.407	0	305548	N.D.	0.142 #
8)	B Heptachlo...	8.125	0.000	3220883	0	4.718	N.D. #
13)	MA Dieldrin	0.000	7.761	0	2850843	N.D.	1.643 #
14)	MA Endrin	0.000	8.072f	0	860213	N.D.	0.553 #
16)	A 4,4'-DDD	9.203	0.000	145447	0	0.294	N.D. #
17)	MA 4,4'-DDT	0.000	8.467	0	402637	N.D.	0.282 #
19)	B Endosulfa...	9.673	8.777	171598	384044	0.308	0.257
21)	B Endrin ke...	10.184	0.000	456844	0	0.744	N.D. #
27)	Chlordane-5	0.000	8.131	0	279224	N.D.	5.420 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL053022\
Data File : PL075247.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 May 2022 11:52
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 03:20:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052822.M
Quant Title : GC Extractables
QLast Update : Tue May 31 02:52:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

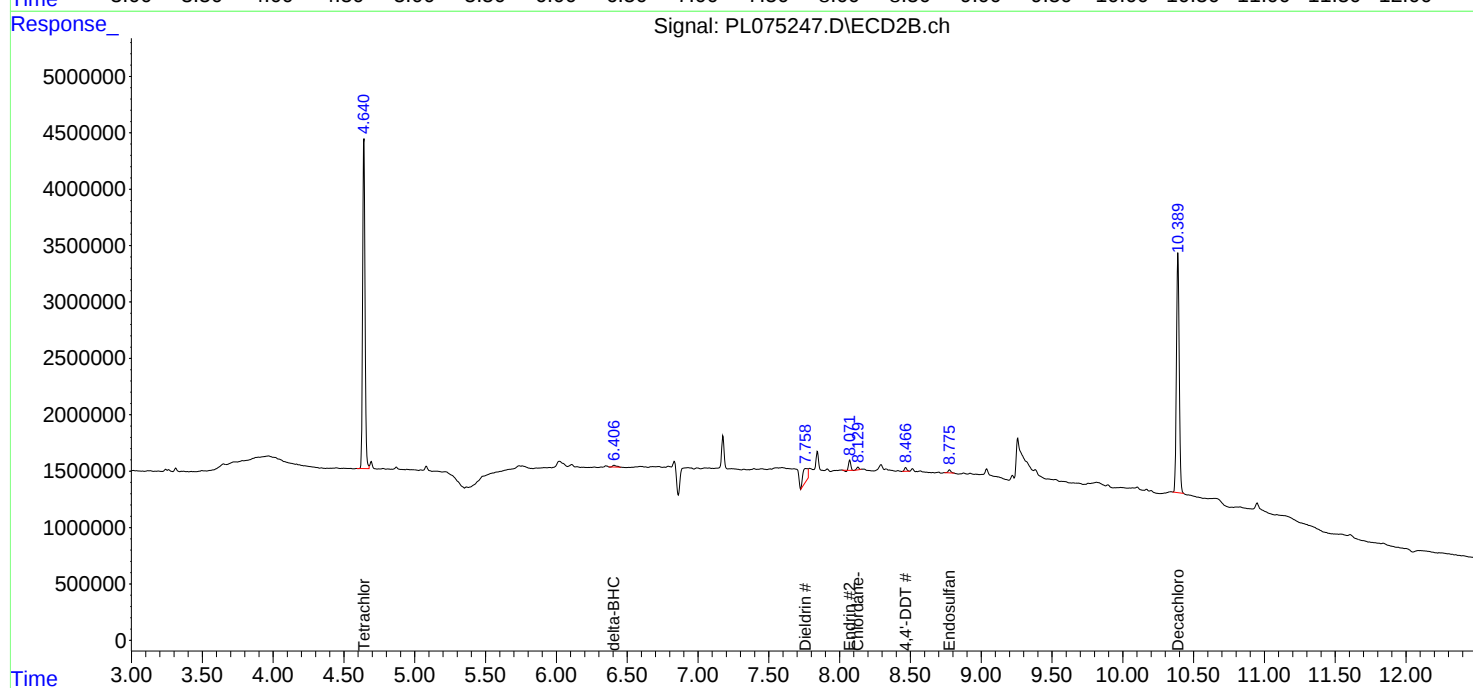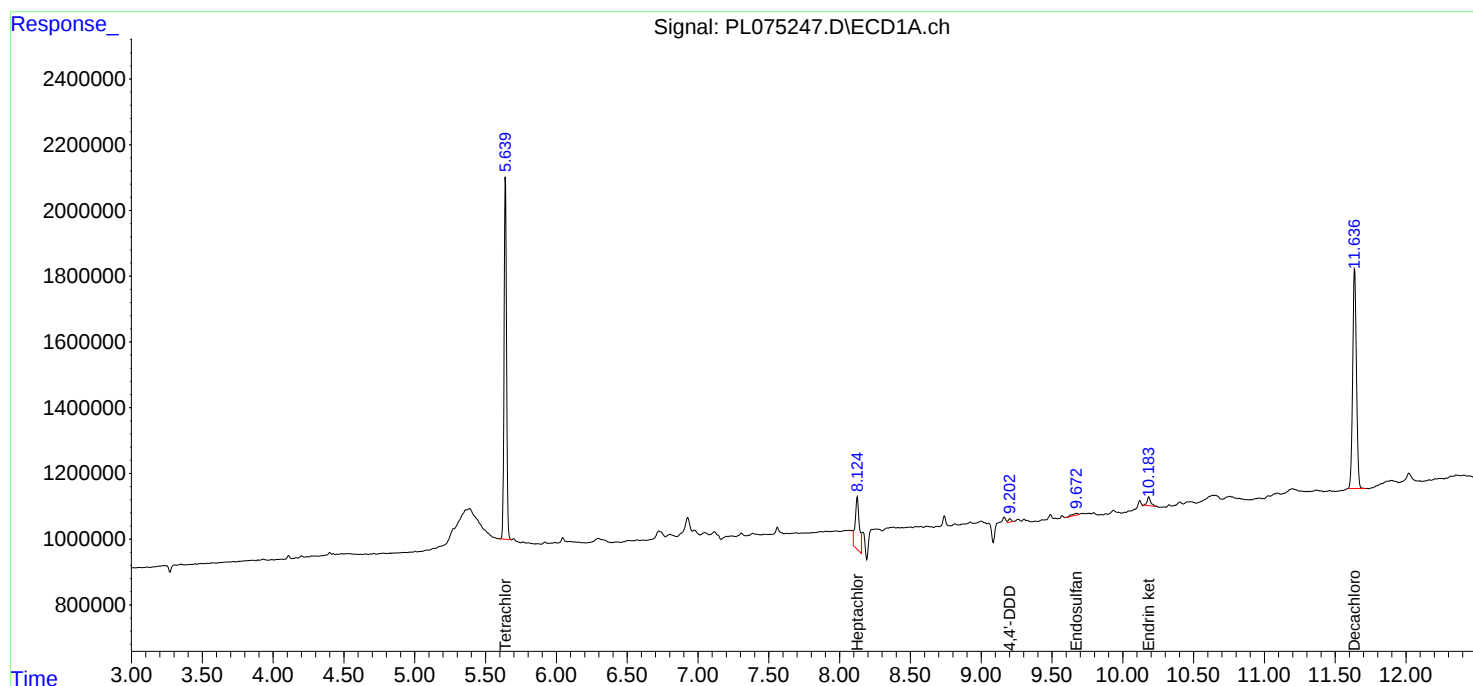


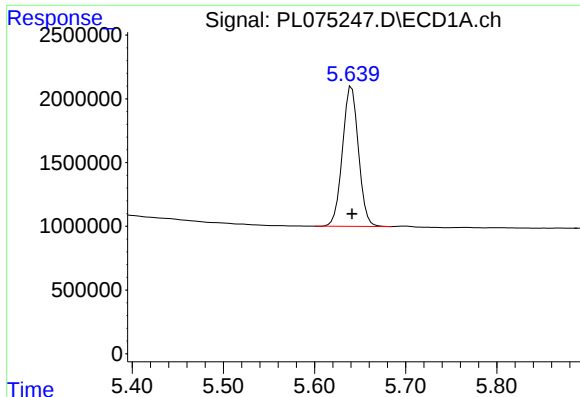

#1 Tetrachloro-m-xylene


R.T.: 5.641 min
Delta R.T.: 0.000 min
Response: 13394117
Conc: 22.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

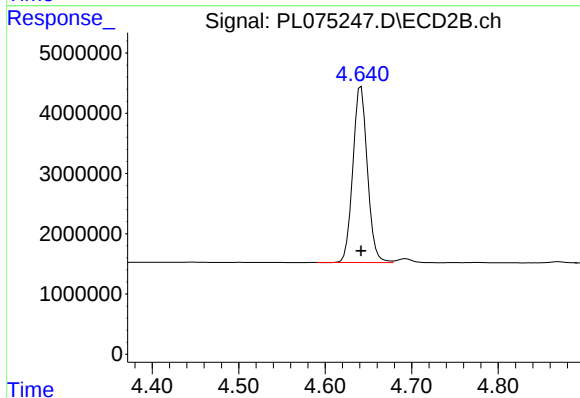


#1 Tetrachloro-m-xylene

R.T.: 4.641 min
Delta R.T.: 0.000 min
Response: 34072222
Conc: 21.51 ng/ml

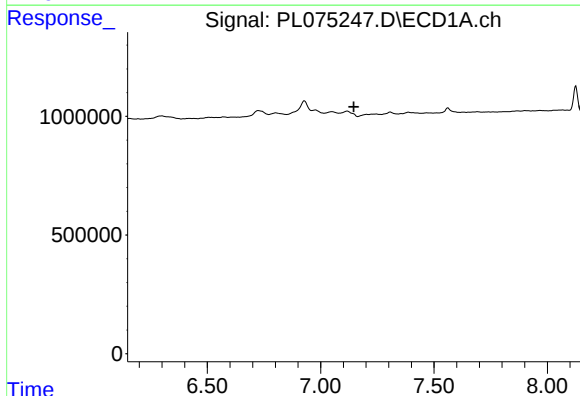


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

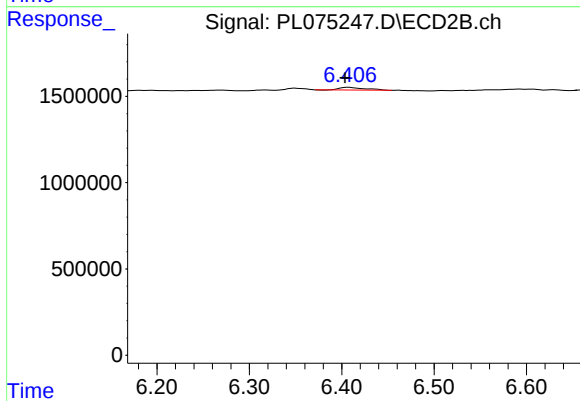

#7 delta-BHC


R.T.: 6.407 min
Delta R.T.: 0.004 min
Response: 305548
Conc: 0.14 ng/ml

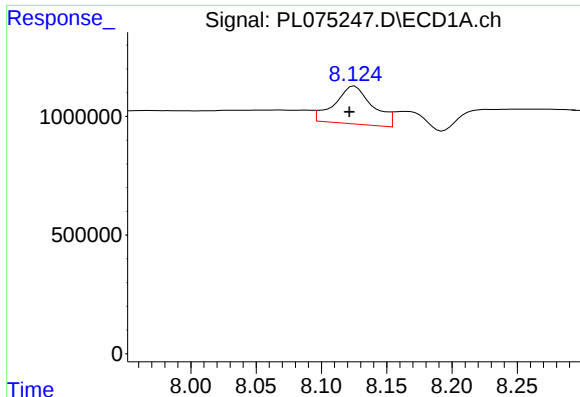

#8 Heptachlor epoxide


R.T.: 8.125 min
Delta R.T.: 0.004 min
Response: 3220883
Conc: 4.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

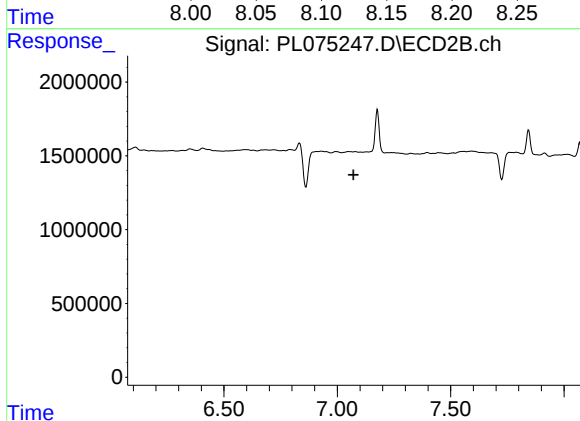


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.072 min
Response: 0
Conc: N.D.

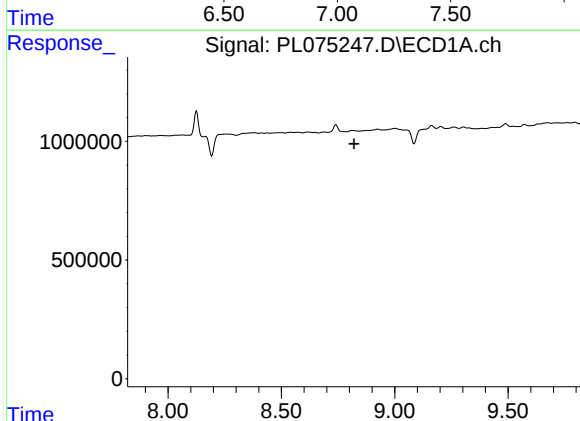


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.821 min
Response: 0
Conc: N.D.

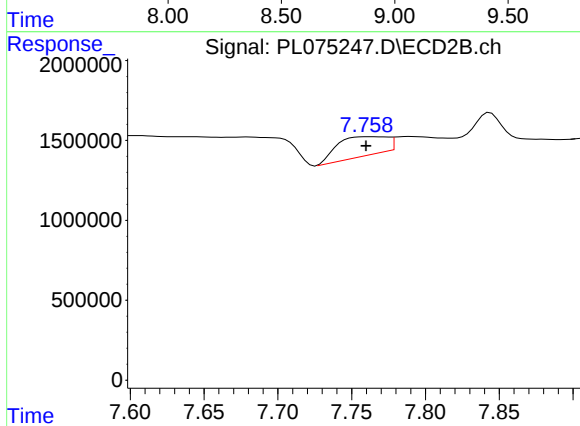

#13 Dieldrin


R.T.: 7.761 min
Delta R.T.: 0.000 min
Response: 2850843
Conc: 1.64 ng/ml

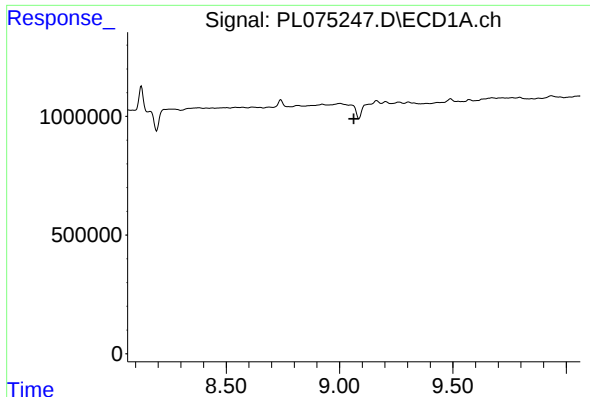

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.062 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

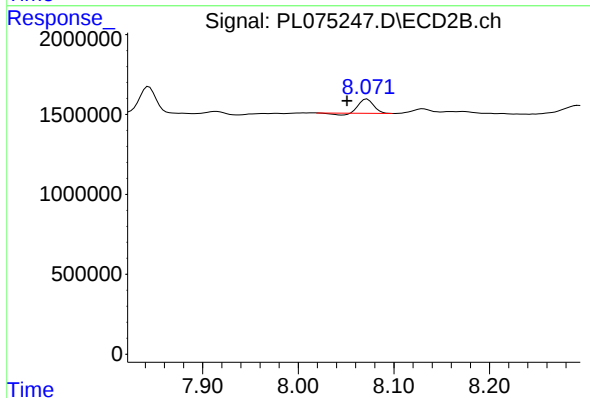


#14 Endrin

R.T.: 8.072 min
Delta R.T.: 0.021 min
Response: 860213
Conc: 0.55 ng/ml

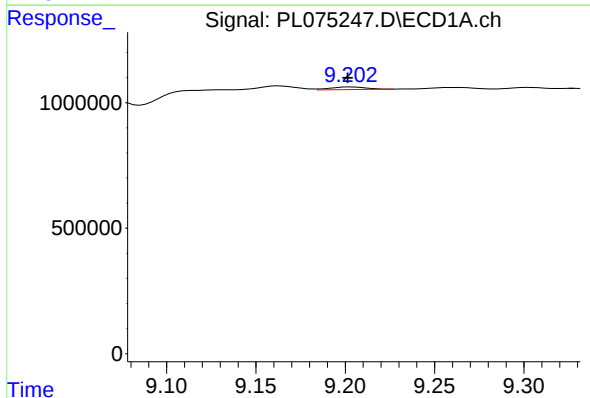


#16 4,4'-DDD

R.T.: 9.203 min
Delta R.T.: 0.002 min
Response: 145447
Conc: 0.29 ng/ml

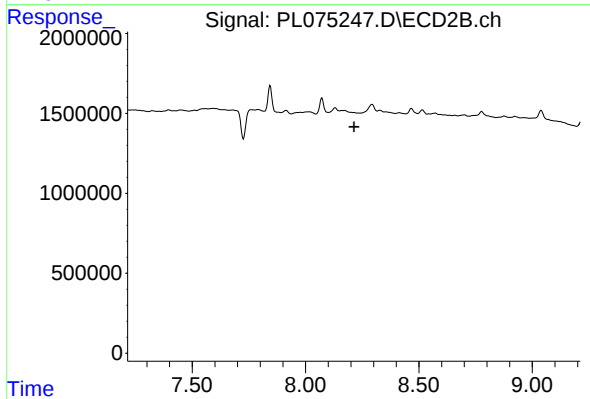

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.215 min
Response: 0
Conc: N.D.

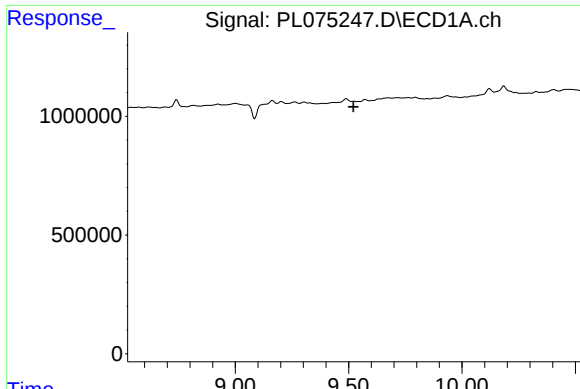

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 9.522 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

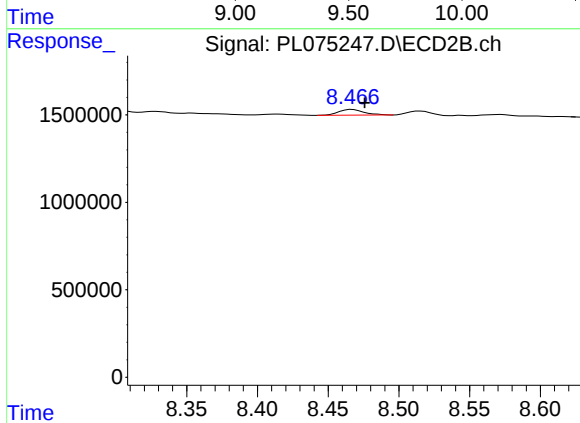


#17 4,4'-DDT

R.T.: 8.467 min
Delta R.T.: -0.009 min
Response: 402637
Conc: 0.28 ng/ml

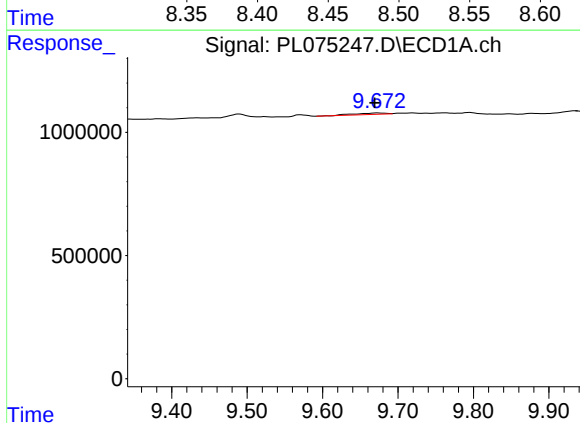


#19 Endosulfan Sulfate

R.T.: 9.673 min
Delta R.T.: 0.004 min
Response: 171598
Conc: 0.31 ng/ml

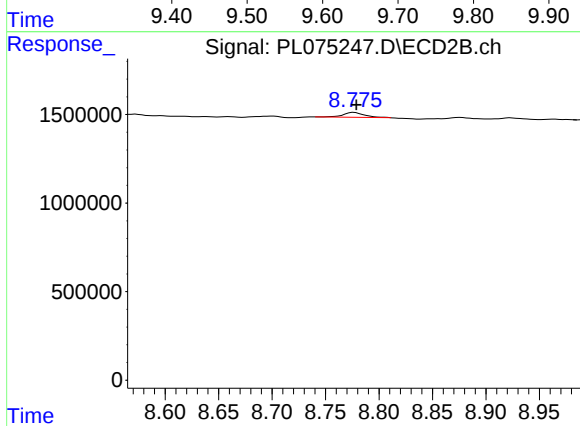

#19 Endosulfan Sulfate


R.T.: 8.777 min
Delta R.T.: -0.002 min
Response: 384044
Conc: 0.26 ng/ml

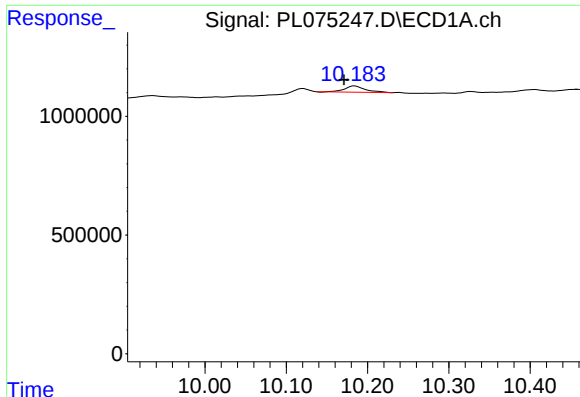

#21 Endrin ketone


R.T.: 10.184 min
Delta R.T.: 0.013 min
Response: 456844
Conc: 0.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

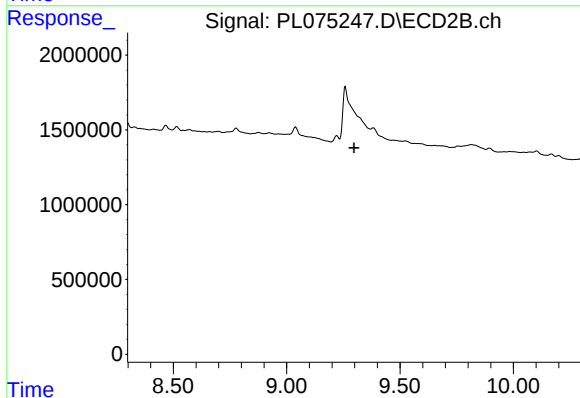


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.298 min
Response: 0
Conc: N.D.

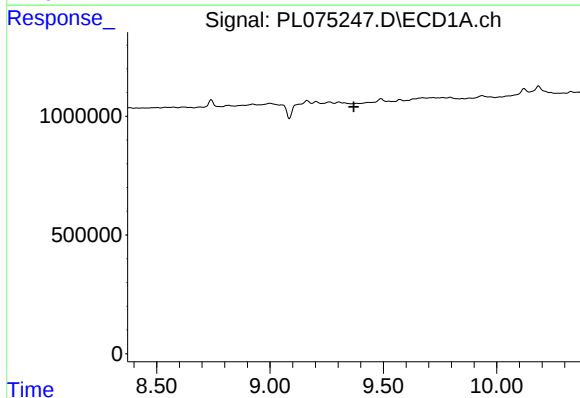


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.369 min
Response: 0
Conc: N.D.

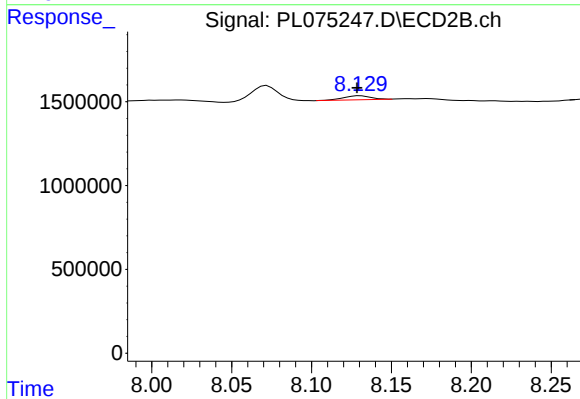

#27 Chlordane-5


R.T.: 8.131 min
Delta R.T.: 0.002 min
Response: 279224
Conc: 5.42 ng/ml

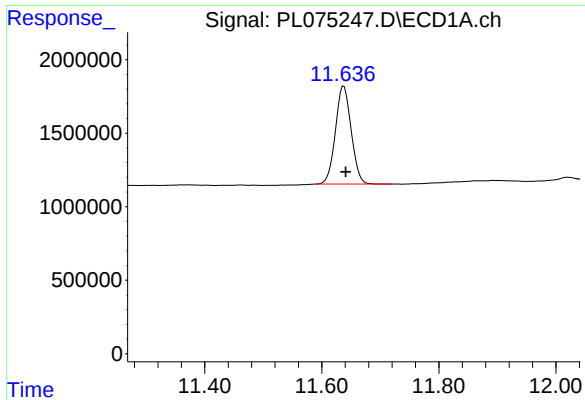

#28 Decachlorobiphenyl

R.T.: 11.638 min
Delta R.T.: -0.003 min
Response: 12456085
Conc: 23.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

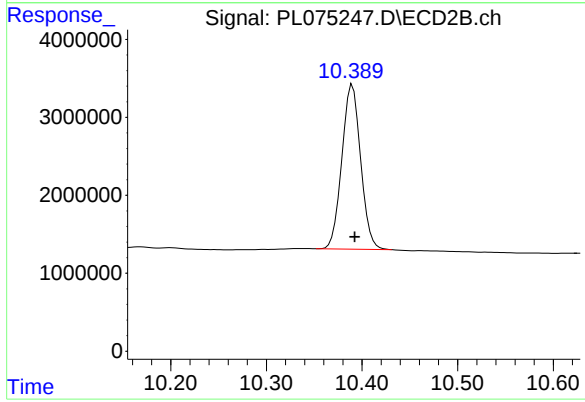

#28 Decachlorobiphenyl

R.T.: 10.390 min
Delta R.T.: -0.002 min
Response: 28890688
Conc: 21.05 ng/ml